



a Standard per-pair evaluation hides collapse

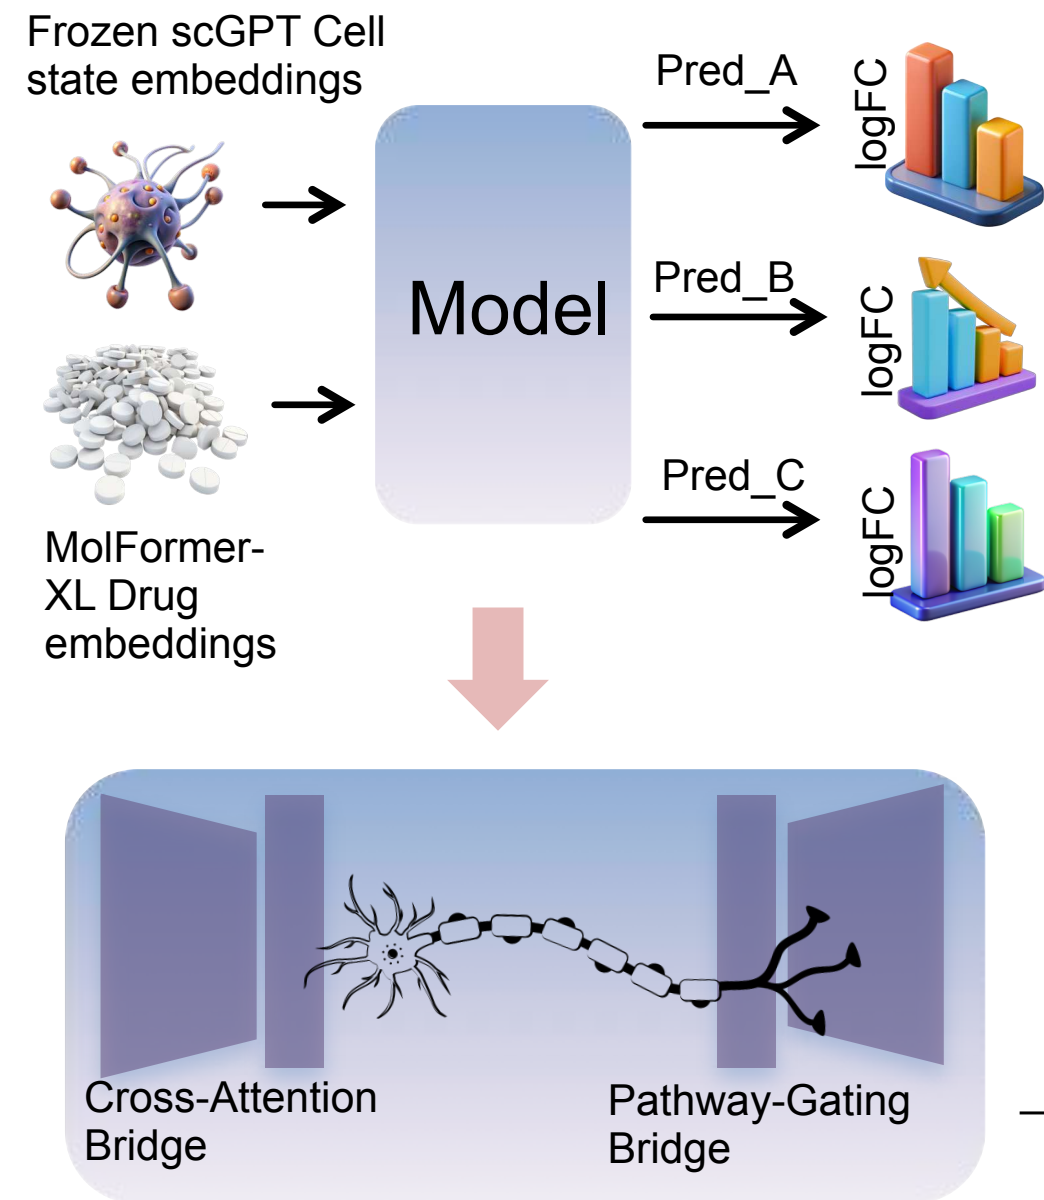

b Off-diagonal drug-discrimination control exposes collapse

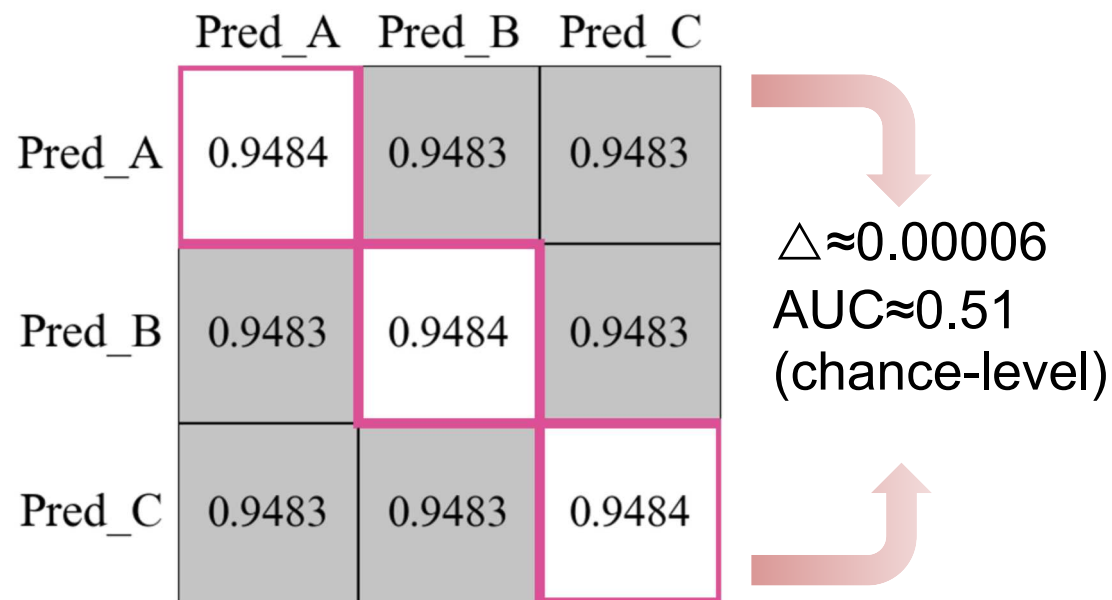

Calibration ladder

