




CST Cerner Help > Interactive View and I&O (IView)>Pacemaker Documentation (Nurse)

Pacemaker Documentation (Nurse)

This help topic is aimed at the Nurses who are responsible for documenting Pacemaker or other Cardiac Rhythm Devices documentation in **Interactive View and I&O (IView)**.

1. Select **Interactive View and I&O (IView)** in the Menu.
2. Select the applicable band that has **Pacemaker/Cardiac Rhythm Devices** section (e.g. Cathlab Quick View band).
3. Select **Pacemaker/Cardiac Rhythm Devices** section.
4. Click the **Dynamic Group**  icon.

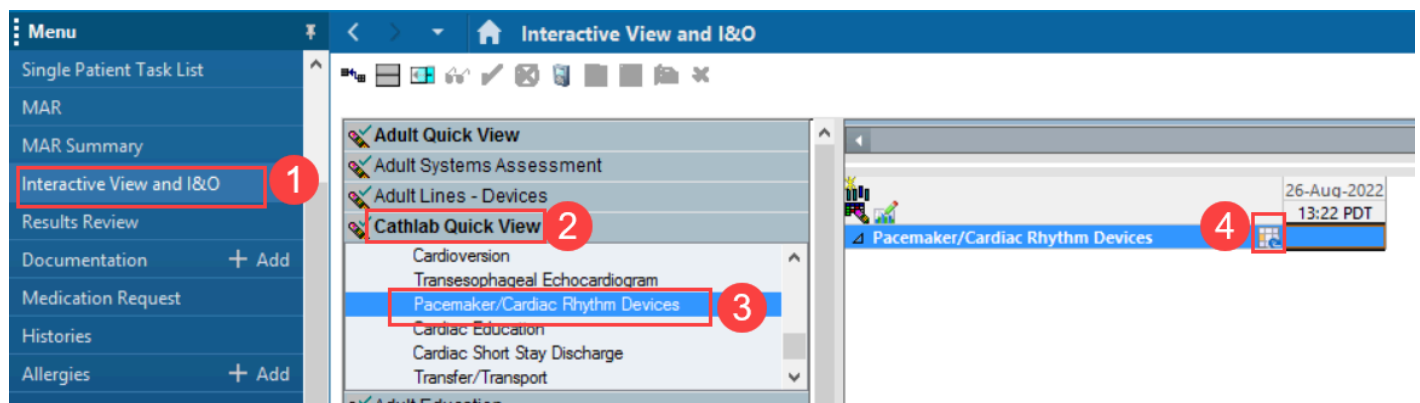

NOTE: The **Pacemaker/Cardiac Rhythm Devices** section can be found in the following iView bands:

- Adult Systems Assessment
- Adult Critical Care Systems Assessment
- Cathlab Quick View
- Adult Procedures
- ED Adult Interventions

- ED Adult Systems Assessment
- ED Pediatric Interventions
- ED Pediatric Systems Assessment
- NICU Special Assessment
- OB Systems Assessment
- Pediatric Procedures
- Pediatric Systems Assessment

5. Select a **Cardiac Rhythm Device Type** in the **Dynamic Group** window and click **OK**.

The screenshot shows a window titled "Dynamic Group - LEARN, KANKOK - 740016080". Inside the window, there is a "Label:" field with the text "Temporary Epicardial". Below this is a "Cardiac Rhythm Device Type:" dropdown menu. The dropdown menu is open, showing a list of options: "Temporary Epicardial", "Temporary Transvenous", "Temporary Transcutaneous", "Permanent External", and "Permanent Internal". The "Temporary Epicardial" option is highlighted in blue. A red circle with the number "5" is placed next to the dropdown menu. At the bottom of the window, there are "OK" and "Cancel" buttons. The "OK" button is highlighted with a red rectangle.

The label of the cardiac rhythm device (e.g. Temporary Epicardial) displays.


6. Document relevant information about the pacemaker or other cardiac rhythm device in the appropriate documentation fields.

NOTES:

- If documenting Independent Double Check (IDC) is required when you take care of patients with temporary pacemakers (e.g. Temporary Epicardial Pacemaker), select **Temporary Epicardial Pacemaker Assessment and Settings IDC** response in the **Device Safety Checklist** field, followed by selecting **Yes** in the **Temporary Epicardial IDC Completed** field.

- After selecting **Yes** in the **Temporary Epicardial IDC Completed** field and signing the iView documentation, you will be prompted to add the witness' name and the witness will add the credentials in the **Authorizing Signature** window.

- Click the **green checkmark** ✓ to sign the documentation.

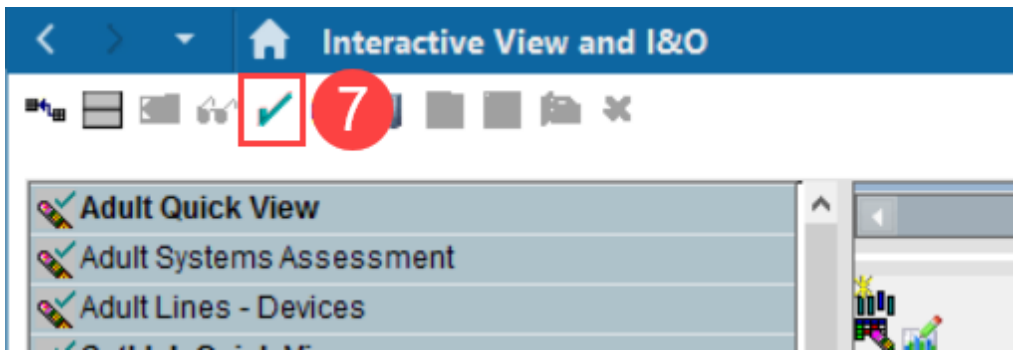

NOTE: Add another Dynamic Group if the patient has more than one Cardiac Rhythm Device Type.

Related Topics

- [Dynamic Group Documentation](#)

Related Positions

- Cardiology Nurse
- Inpatient Nurse
- Critical Care Nurse
- Emergency Nurse
- NICU Nurse
- Pediatric Nurse

Key Words

- Cardiac Device
- Cardiac Rhythm Device
- Implanted defibrillator
- Pacemaker

Last Updated: September 27, 2022

A joint initiative of:

