



MSForest Manual

Raw File Triage, Visualization, and Conversion

Introduction

MSForest is a desktop tool for rapid triage of raw files in proteomics. It helps you inspect directories of raw mass spectrometry files before committing to downstream analysis. The goal is to identify errors before database searching and statistical analysis, so you can fix problems or re-run samples before concluding an experiment.

At each stage, MSForest is designed to help you see the forest through the trees. Instead of opening one spectrum at a time, MSForest first shows the batch: which files were written correctly, which injections produced a chromatographic signal, which runs look unlike their neighbors, and which files need closer inspection. When the batch view raises a question, the individual raw file visualizer is designed to show you the complete structure first, rather than the acquired spectra first. It gives you tools to drill into the file with TIC views, targeted XICs, acquisition structure, ion injection time summaries, and method metadata.

MSForest is built on MSRawJava, a lightweight Java library and command-line interface for supported Thermo, Bruker timsTOF, EncyclopeDIA `.dia`, and `mzML` workflows. Most users interact with MSForest, but the MSRawJava CLI and library are covered later for scripted conversion and developer integration. This manual is written for MSForest/MSRawJava version `v26.5.28`. Project versions are date-based and are updated from the build date, so a later release may have a different version number while keeping the same general workflow.

The guide is organized around questions an analyst can ask immediately after or during acquisition. The most important habit is to start broad and only then drill down:

- **Did every file finish writing correctly?** A missing or failed sparkline can flag truncation, save errors, unsupported files, or files that cannot be parsed.
- **Did material actually enter the instrument?** An empty or extremely low TIC trace can indicate no sample in the vial, a depleted sample, injection failure, or a blocked flow path.
- **Does one sample look unlike its neighbors?** Related injections should show similar rough TIC shapes. A single outlier can flag sample handling, matrix, or preparation problems that deserve follow-up.
- **Did the spray stay stable across the gradient?** Use the raw file visualizer's TIC or Global view to localize dropouts, flat regions, LC interruptions, or acquisition pauses.
- **Are contaminants present?** Use targeted XICs in the single-file visualizer to test PEGs, polysiloxanes, detergents, and contaminant peptides from proteins like keratins or trypsin.
- **Did the method match the intended design?** The Structure, Global, Range Statistics, and Settings views help answer whether isolation windows, AGC/IIT settings, and Thermo instrument methods are what you expected.

The feature descriptions below follow that workflow: install MSForest, screen a directory, investigate suspicious files, convert files after triage, and use MSRawJava directly only when you need scripted conversion or developer access.

Supported input types:

- Thermo `.raw`
- Bruker timsTOF `.d` directories
- EncyclopeDIA `.dia`
- `mzML`

Supported output types:

- EncyclopeDIA `.dia`
- Mascot Generic Format `.mgf`
- `mzML`

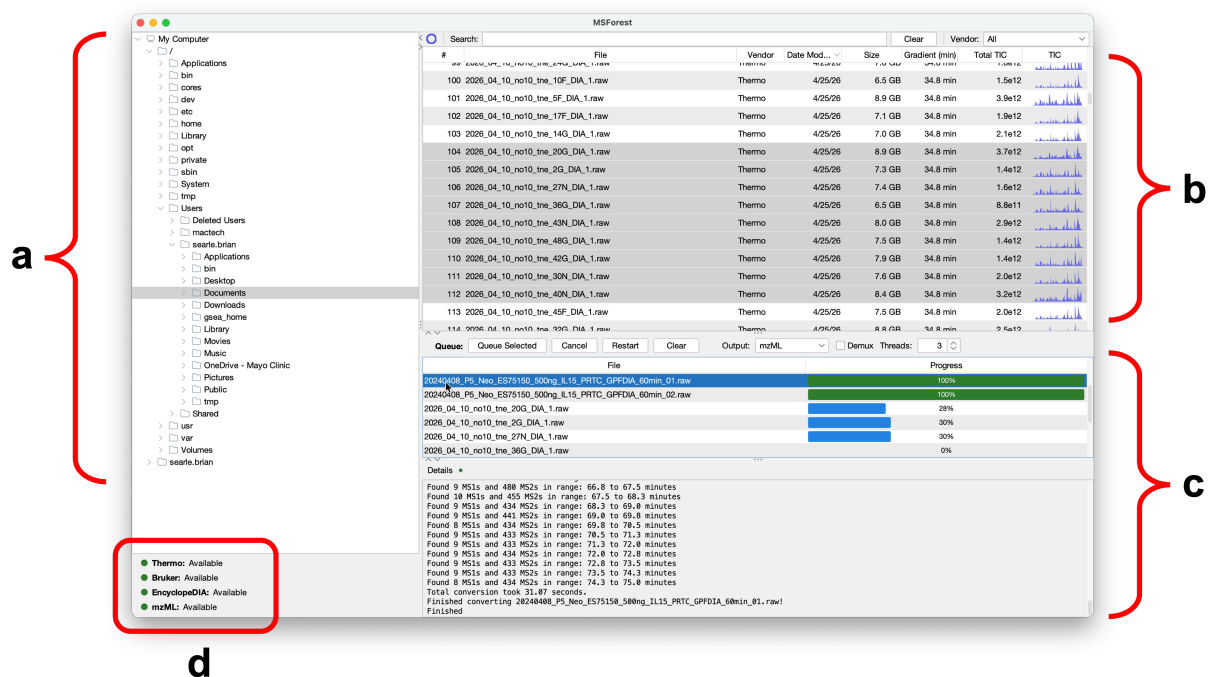


Figure 1. MSForest main browser layout. The main browser is organized for directory-level triage before conversion. The left panel (a) is the directory browser, the upper table (b) lists raw files detected in the selected directory, the lower panel (c) contains conversion settings, queued tasks, and job details, and the reader status panel (d) reports whether the bundled readers are available.

Installation

Most users should install MSForest from the platform-specific installer. The installers include the application runtime and bundled native components used by the Thermo and Bruker readers, so normal desktop users do not need to install Java, .NET, Rust, Maven, or vendor SDKs separately.

Build-from-source instructions are intentionally kept out of this installation chapter. Developers who want to build or embed MSRawJava should read [MSRawJava Library and Building from Source](#).

macOS

The macOS package is distributed as a `.dmg` .

1. Download the MSForest macOS `.dmg` .
2. Open the `.dmg` .
3. Drag `MSForest` into `Applications` , or follow the installer prompts if the release package uses an installer window.
4. Launch `MSForest` from `Applications` .

If macOS blocks the app because it is unsigned or not notarized:

1. Try opening `MSForest` once from Finder so macOS records the blocked launch.
2. Open **System Settings > Privacy & Security**.
3. Find the message about `MSForest` being blocked.
4. Click **Open Anyway**.
5. Confirm the prompt and launch the application.

An alternate Gatekeeper workflow is:

1. Control-click or right-click `MSForest` .
2. Choose **Open**.
3. Confirm that you want to open the application.

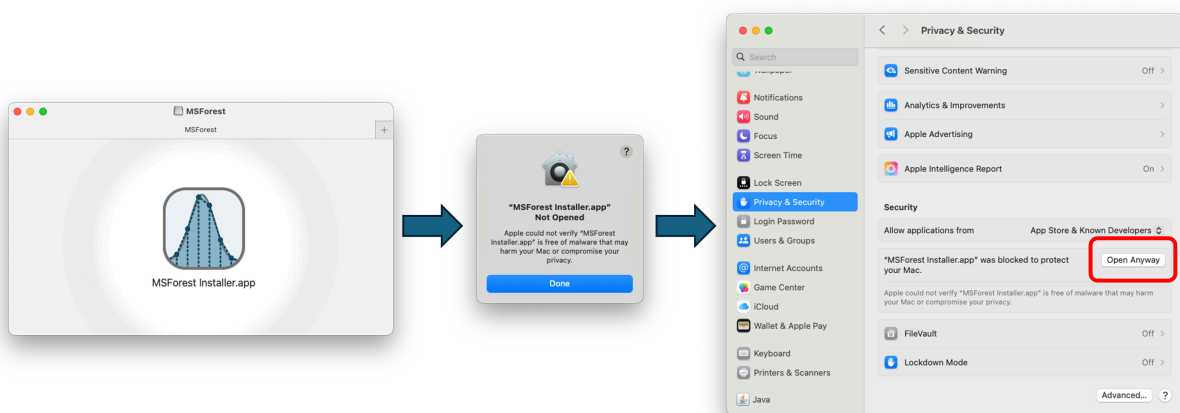


Figure 2. Opening an unsigned MSForest package on macOS. After mounting the `.dmg` and attempting to open MSForest, macOS may block the app because it is unsigned or not notarized. Open **System Settings > Privacy & Security**, find the blocked application message, and use **Open Anyway** to allow the launch.

Windows

The Windows package is distributed as a 64-bit `.exe` installer.

1. Download the MSForest Windows x64 installer.
2. Double-click the `.exe`.
3. Follow the installer prompts.
4. Launch `MSForest` from the Start menu or the installed application shortcut.

If Windows SmartScreen blocks the installer because it is unsigned:

1. In the SmartScreen warning, click **More info**.
2. Confirm that the publisher/file name is the MSForest installer you downloaded.
3. Click **Run anyway**.
4. Continue through the installer.

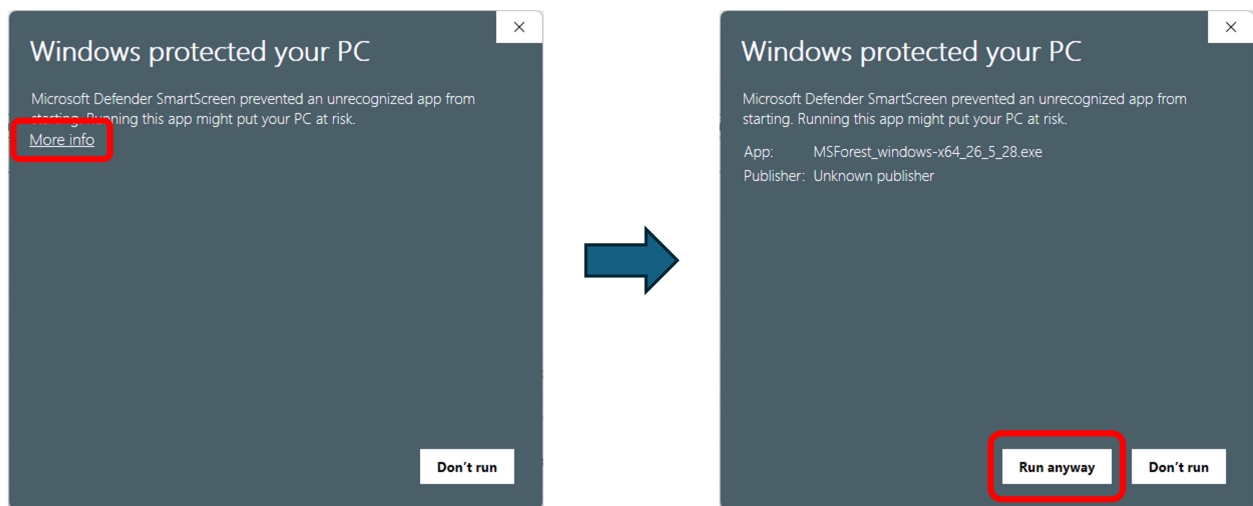


Figure 3. Opening an unsigned MSForest installer on Windows. Windows SmartScreen may initially hide the launch option for an unsigned installer. Click **More info**, confirm that the file is the MSForest installer you intended to run, and then click **Run anyway**.

Linux and Ubuntu

The Linux package is distributed as an install4j Unix installer. These instructions target Ubuntu, but the same general workflow applies to other desktop Linux distributions with a compatible runtime environment.

1. Download the MSForest Unix/Linux installer.
2. Make the installer executable if needed:

```
chmod +x MSForest_unix_*.sh
```

3. Run the installer:

```
./MSForest_unix_*.sh
```

4. Follow the prompts and choose an installation directory.
5. Launch `MSForest` from the installed launcher, desktop entry, or application directory.

If the desktop environment does not show the launcher immediately, open the installation directory and run the `MSForest` executable directly.

No Linux-specific installer screenshot is included in this manual yet. The Ubuntu workflow uses the same install4j Unix installer flow described above, launched from a terminal after marking the installer executable.

First Launch

On first launch, MSForest asks whether the current computer is an instrument computer. Choose **Yes (min processing)** on acquisition computers where conversion should not consume significant CPU resources. Choose **No (max processing)** on analysis workstations where MSForest can use more processing capacity. This can be changed later in **File > Preferences**.

Main Browser

The main browser is the triage view. Use it before opening individual files. The goal is to decide whether a directory of acquisitions looks sane enough to convert, which files deserve closer inspection, and whether a problem is isolated to one injection or shared across a batch.

The browser is designed to answer questions like:

- **Did the files write correctly?** Rows with missing metrics or no sparkline may be truncated, still writing, inaccessible, or unparsable.
- **Are any runs empty or failed?** Very low total TIC and flat sparklines can flag empty vials, depleted samples, failed injections, failed sample prep, or blocked flow paths.
- **Are related samples coherent?** Replicate injections and related sample classes should have broadly similar TIC shapes. A single odd trace is often the first clue that one injection needs follow-up.
- **Does one sample look biologically or chemically unusual?** A urine sample with blood contamination or a plasma extracellular-vesicle preparation with platelet contamination may stand out before you know the cause.
- **Are late or unusual TIC features worth inspecting?** Browser sparklines can flag features for follow-up, but targeted XICs in the visualizer are needed before naming a contaminant.
- **Which files should be visualized or queued for conversion?** Use the summary table to select suspicious files for inspection and acceptable files for conversion.

The window has three main areas, shown in Figure 1:

- The directory tree on the left.
- The directory summary table in the upper right.
- The conversion queue and job details panel in the lower right.

Opening a Directory

Use the directory tree to browse to a folder containing raw files. Selecting a directory scans it for supported files and updates the summary table. The scanner recognizes Thermo `.raw` files, Bruker `.d` directories, EncyclopeDIA `.dia` files, and `mzML` files.

You can also use **File > Open** to choose a raw file or directory. MSForest selects the enclosing folder in the browser and highlights the chosen file when possible.

Directory scans run in the background. Large folders and network drives may take longer, especially while MSForest reads slower metrics such as gradient length, total TIC, and TIC traces.

Directory Summary Table

The summary table gives one row per discovered raw file. The columns are:

- `#` : table row number.
- `File` : raw file or directory name.
- `Vendor` : detected vendor or file format.
- `Modified` : last modified date from the file system.
- `Size` : total size on disk.
- `Gradient` : run length in minutes.
- `Total TIC` : sum of MS1 total ion current values.
- `TIC` : compact total ion current sparkline across retention time.

The table appears quickly with file names and basic file-system information, then fills in slower metrics as readers finish. The spinner near the search bar shows whether background metric extraction is still running.

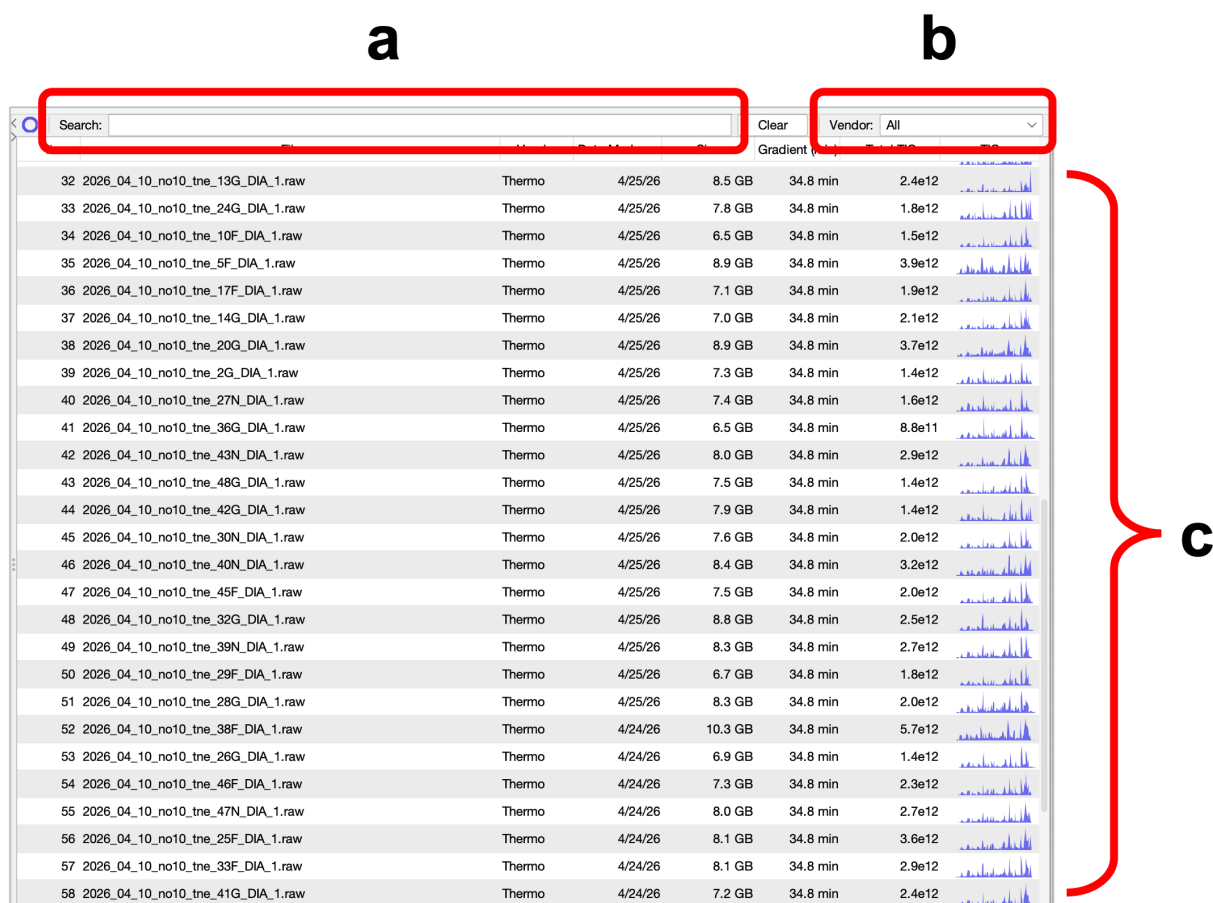


Figure 4. Directory-level consistency checking. The search box (a) filters files by name, the vendor selector (b) narrows the table to a specific raw-file type, and the file list (c) shows run summaries and TIC sparklines. Similar replicate injections should have similar rough sparkline shapes; missing, flat, or unusual traces are the first files to inspect in detail.

What the Directory Browser Can and Cannot Tell You

The directory browser screens files. It does not replace single-file inspection.

The browser can:

- Flag empty or failed injections.
- Flag gross outliers among related samples.
- Flag missing metrics or failed parsing.
- Flag late or unusual TIC features for follow-up.

The browser cannot:

- Identify chemical contaminants by itself.
- Definitively diagnose spray stability by itself.

- Prove sample identity or biological cause by itself.

Reading the Spark Charts

The TIC sparkline is intentionally small. It is not meant to replace the visualizer; it is meant to let you scan dozens or hundreds of injections quickly. The useful comparison is usually relative: compare neighboring files from the same sample type, method, or replicate set.

Common questions and signals:

- **Did the run fail to parse or save correctly?** A row with no sparkline, missing gradient, or missing total TIC should be treated as suspicious. It may be a truncated file, a file still being copied, a permission problem, or a reader error. Open it in the visualizer or check the Logging Console before trusting it.
- **Was the vial empty, depleted, or not injected correctly?** A very low total TIC and nearly flat sparkline suggest an empty injection, failed autosampler draw, depleted vial, failed sample prep, blocked flow path, or little analyte material. If blanks are expected, compare against actual blanks rather than against sample injections.
- **Do replicates agree?** Replicates rarely match perfectly, but their rough shapes should agree: similar gradient envelope, similar high-intensity regions, and similar late features. A single replicate with a different envelope is worth opening before conversion.
- **Does one sample look unlike its neighbors?** A biological or preparation outlier can show up as a different TIC envelope. Examples include blood contamination in urine or platelet contamination in plasma extracellular-vesicle preparations. The browser can flag the outlier; use the visualizer to test what changed.
- **Is there a late or unusual TIC feature?** A strong late hump or spike can be worth investigating, especially if it appears in blanks, washes, or only one sample class. Use targeted XICs in the visualizer before calling it PEG, polysiloxane, detergent, plasticizer, carryover, or another contaminant.

Do not over-interpret small sparkline differences. The browser is for prioritization. Use the visualizer when a sparkline asks a concrete follow-up question.

Searching, Filtering, and Sorting

Use **Search** to filter rows by file name. Press Escape while the search field is focused, or click **Clear**, to reset the search.

Use **Vendor** to filter by supported vendor or file format. This is useful in mixed directories containing raw files, `.dia` files, and `mzML` files.

Click column headers to sort. MSForest remembers table sort order, column order, and column widths between sessions.

Selecting Files

The summary table supports multiple selection. Select one or more files to queue them for conversion. Double-click a row to open that file in the raw file visualizer.

Right-click a row for context actions:

- **Visualize** opens the selected file in the raw file visualizer.
- **Show Enclosing Folder** selects the file's folder in the directory tree.
- **Select All** selects all visible rows in the current table.

In a typical triage pass, sort or group the directory so related injections are adjacent, scan the sparklines for outliers, open the suspicious runs, and only then queue the files that pass inspection.

Menus

The main menu provides access to the browser, visualizer, preferences, windows, and diagnostic tools.

File

- **Open** selects a raw file or directory.
- **Preferences** opens application preferences.
- **Quit** closes MSForest.

View

- **Visualize Raw File** opens a raw file directly in the visualizer.

Window

- Brings the main browser to the front.
- Switches between open visualization windows.
- Moves to the previous or next window.

Help

- **How to Cite** shows citation information.
- **Educational Demos** opens the built-in loading-panel demos.
- **Logging Console** shows captured standard output and error messages.

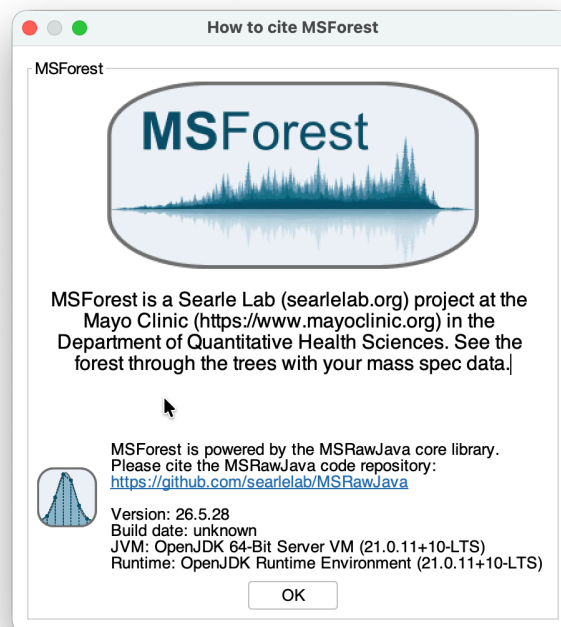


Figure 5. Citation information. The **How to Cite** dialog provides citation guidance for MSForest/MSRawJava. Use it when preparing publications, methods sections, or internal documentation that needs to identify the software version and project.

Logging Console

Open **Help > Logging Console** when a conversion or reader problem needs more context than the job details panel shows. The console captures standard output and error messages from the GUI session, including reader startup messages and exceptions that may not fit in a table cell or progress message.

Installed MSForest builds also write install4j launcher logs next to the application launcher. `error.log` captures standard error and is appended across launches, so older startup failures may still be present. `output.log` captures standard output and is rewritten each time MSForest launches. Check both files when MSForest fails before the Logging Console opens.

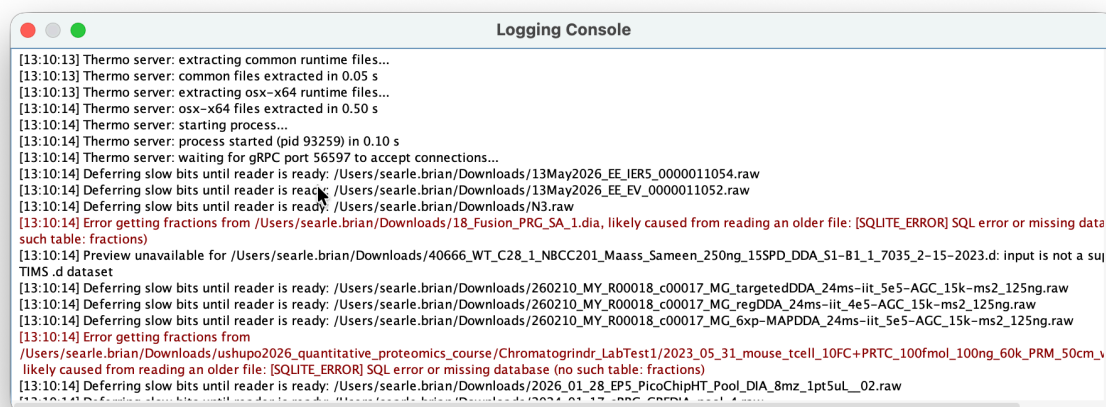


Figure 6. Logging Console. The Logging Console captures diagnostic output from the GUI session. It is most useful when a file has missing metrics, a reader fails to initialize, or a conversion job fails before the job details panel contains enough context.

Preferences

Open preferences with **File > Preferences**.

The **Processing** tab controls processing thread limits and verbose core logging. Thread changes require a restart because the reader and conversion thread pools are created when the application starts.

The **Conversion** tab controls defaults used by queued GUI conversions:

- Demux tolerance in ppm.
- Minimum MS1 intensity.
- Minimum MS2 intensity.

The **GUI** tab controls the last directory, look and feel, and saved layout resets. You can reset window positions, split pane dimensions, or table parameters if the interface layout becomes inconvenient.

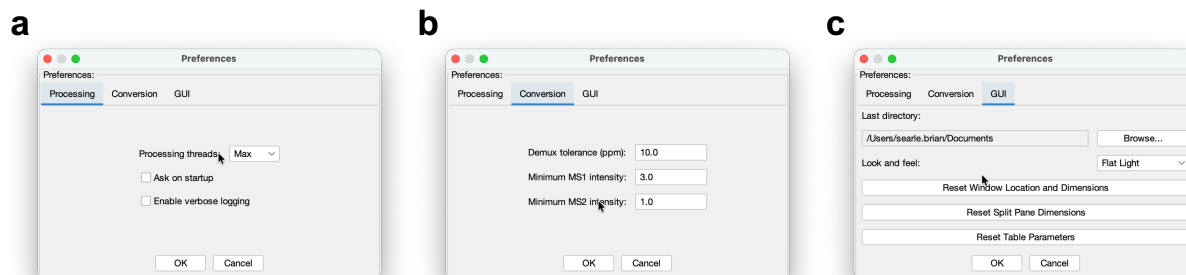


Figure 7. MSForest preferences. Preferences are split into processing controls (a), conversion defaults (b), and GUI layout/appearance settings (c). Processing settings are especially important on instrument computers, where limiting background work can prevent raw-file inspection or conversion from competing with acquisition software.

File Conversion in the GUI

The conversion panel is attached to the bottom of the main browser. Use it after the browser and visualizer have answered the basic triage questions. Conversion is deliberately downstream of inspection: the point is to decide which files are ready for downstream analysis, which files need recollection, and which files should be kept only for troubleshooting or documentation.

The conversion panel answers operational questions:

- **Which inspected files are ready for downstream analysis?** Select only the files you want to convert.
- **Which output format does the next tool need?** Choose `.dia`, `.mgf`, or `mzML`.
- **Does this dataset need demultiplexing?** Enable demux only for supported staggered-window workflows.
- **Can this computer handle parallel conversion right now?** Adjust GUI thread count based on whether this is an instrument computer or an analysis workstation.

The conversion controls are shown in the lower main-browser region in Figure 1c.

Conversion Controls

The conversion toolbar includes:

- **Queue Selected:** adds selected files from the directory summary table.
- **Cancel:** cancels queued and running jobs.
- **Restart:** requeues failed or canceled jobs and resumes processing.
- **Clear:** removes jobs that have not started or were canceled.

The parameter controls include:

- **Output:** output format, using the available `OutputType` values.
- **Demux:** enables staggered-window demultiplexing when supported.
- **Threads:** number of files that can be converted in parallel by the GUI queue.

Select a job in the queue to view details and per-job log messages in the details console.

Output Formats

MSForest can write:

- EncyclopeDIA `.dia`
- `.mgf`
- `mzML`

Output files are written to the same directory as the input file unless the workflow explicitly provides another output directory. The GUI conversion queue uses the input file's parent directory.

Demultiplexing

The **Demux** checkbox enables staggered-window demultiplexing for supported inputs. It is intended for Thermo, EncyclopeDIA `.dia`, and `mzML` sources where the acquisition structure supports staggered-window demultiplexing.

Bruker `.d` files do not support staggered demultiplexing in MSForest. When Bruker files are selected, the GUI disables the checkbox and conversion proceeds without demultiplexing.

Demux tolerance is set in **File > Preferences > Conversion**.

Output Naming

For normal conversions, the output file uses the input base name with the selected output extension.

Demultiplexed outputs include a `.demux` suffix before the output extension. For example:

- `sample.raw` to demultiplexed `mzML` : `sample.demux.mzML`
- `sample.raw` to demultiplexed `.dia` : `sample.demux.dia`
- `sample.raw` to demultiplexed `.mgf` : `sample.demux.mgf`

When converting `.dia` to `.dia` in the same directory, MSForest avoids overwriting the input by writing a `.2.dia` file. When converting `mzML` to `mzML` in the same directory, it writes `.2.mzML`.

Job States and Logs

The progress column shows conversion progress. Completed jobs are shown as successful or failed. Canceled jobs remain visible until cleared.

Select a queue row to inspect:

- Source vendor or format.
- Output type.
- Input path.
- Conversion messages.

Use **Help > Logging Console** when the application needs broader diagnostic context beyond a single job.

Raw File Visualizer

Open the visualizer when the directory view raises a question. The raw file visualizer is the detailed inspection window for confirming signal, localizing acquisition problems, extracting targeted chromatograms, and checking whether the method matches the experiment. Open it by double-clicking a file in the directory summary table, right-clicking a file and choosing **Visualize**, or choosing **View > Visualize Raw File**.

The visualizer is not just a spectrum viewer. It is a fast way to test hypotheses from triage:

- **The file looked empty:** use Scans and the TIC trace to confirm whether there is real MS1 or MS2 signal.
- **The signal seemed to drop out:** use the Global view or TIC trace to localize flat regions, unstable spray, LC interruptions, or acquisition pauses.
- **The file looked chemically odd:** use targeted XICs for PEGs, polysiloxanes, detergents, plasticizers, carryover ions, or lab-specific background ions.
- **The sample looked unlike neighbors:** compare TIC, XICs, spectra, and method structure against a normal file from the same batch.
- **The method looked wrong:** use Structure, Global, and Settings to check isolation windows, scheduling, acquisition type, and Thermo instrument method text.
- **The fill behavior looked odd:** use Range Statistics to compare ion injection time distributions across adjacent isolation windows and retention-time bins.

The visualizer opens in a separate window. Multiple visualizer windows can be open at the same time, and the **Window** menu can switch between them.



Figure 8. Raw file visualizer layout. The visualizer starts from a scan table (a), scan type selector (b), and search field (c), then uses tabs (d) to switch the main visualization region (e) between scans, range statistics, acquisition structure, global summaries, and settings. This layout supports moving from "is there signal?" to "what kind of signal?" without leaving the file.

Scans Tab

The **Scans** tab is the default visualizer view. It combines:

- A scan table.
- A scan type filter.
- A text search field.
- A top chromatogram plot.
- A spectrum plot for the selected scan or merged selection.
- A histogram and per-scan properties panel.
- An ion mobility plot when ion mobility data is available.

The scan table columns are:

- **#** : table row number.
- **Name** : vendor-provided scan or spectrum name.
- **RT** : scan start time in minutes.
- **Precursor** : precursor m/z, blank for MS1.
- **TIC** : total ion current for the scan.

Use the scan type filter to view all spectra, MS1 scans, or MS2 scans for a specific isolation window. Use the search field to filter the scan table by text.

Selecting a scan updates the spectrum plot. Selecting multiple scans merges them for display using a mass tolerance, which is useful when inspecting a local region of a chromatogram.

Use this tab first when you are trying to answer whether there is real signal in the file. Select an MS1 scan near the expected elution range and inspect whether peptide-like isotope envelopes are present. Then select MS2 scans in the relevant isolation window to check whether fragment spectra contain meaningful peaks rather than only chemical background. If a browser sparkline looked empty, the Scans tab usually confirms quickly whether the file is truly empty or whether the signal is present but unusual.

Chromatogram Navigation

The top plot shows the active chromatogram. In normal mode it shows total ion current over retention time. When XIC extraction is active, it shows extracted chromatogram traces.

Clicking the chromatogram selects the nearest visible scan row. Keyboard and chart navigation can move through scans without leaving the visualizer.

Spectrum, Ion Mobility, Histogram, and Properties

The lower panel shows the current spectrum as intensity versus m/z. For timsTOF data with ion mobility values, the visualizer also shows an ion mobility versus m/z view.

The **Histogram** tab shows the log10 fragment intensity distribution for the selected spectrum. The **Properties** tab shows per-scan vendor metadata when available.

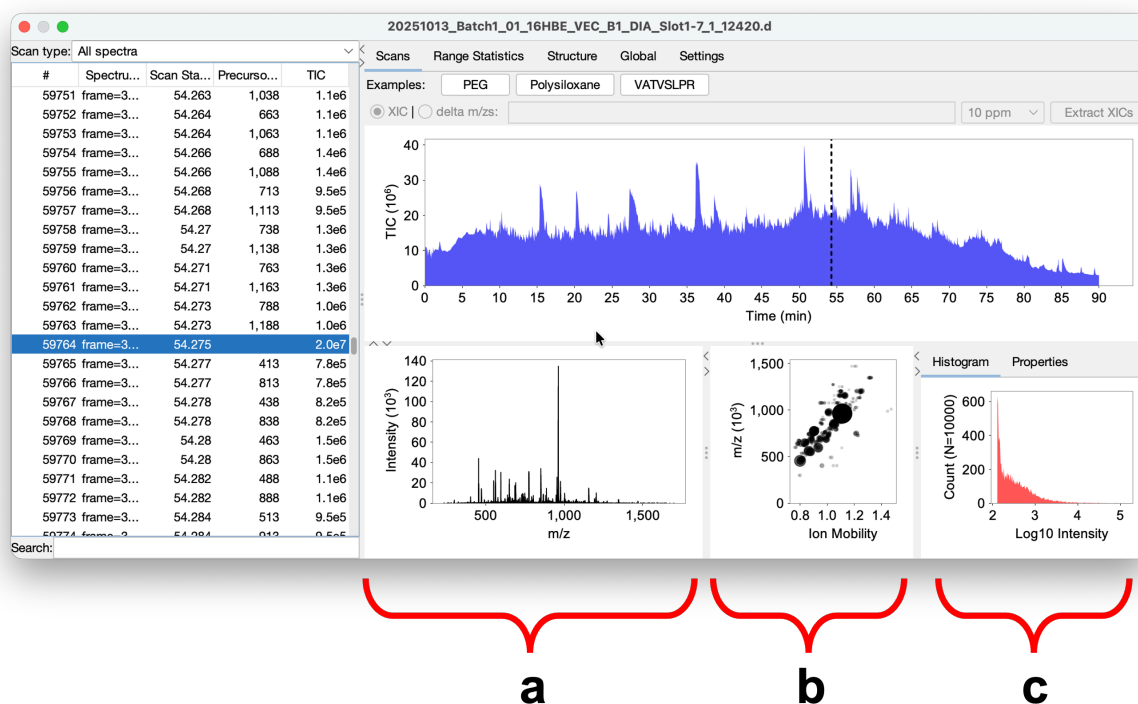


Figure 9. timsTOF spectrum and ion mobility inspection. Selecting a scan from the TIC trace (a) updates the spectrum view and the two-dimensional ion mobility/m/z plot (b). The intensity histogram (c) shows the broad distribution of peak intensities, which helps separate meaningful signal from abundant low-intensity points in mobility-resolved data.

Extracted Ion Chromatograms

The XIC controls are above the top chromatogram. MSForest accepts multiple targets separated by commas or whitespace.

Targets may be:

- Numeric m/z values, such as 371.228 .
- Chemical formulas, such as [C2H6SiO]5 .
- Peptide sequences with charge notation, such as VATVSLPR++ .

Use the tolerance selector to set extraction tolerance. Choose **XIC** mode to plot extracted intensity, or **delta m/zs** mode to plot mass error for extracted signal. Click **Extract XICs** to run the extraction.

The example buttons populate common demonstration targets:

- PEG
- Polysiloxane
- VATVSLPR

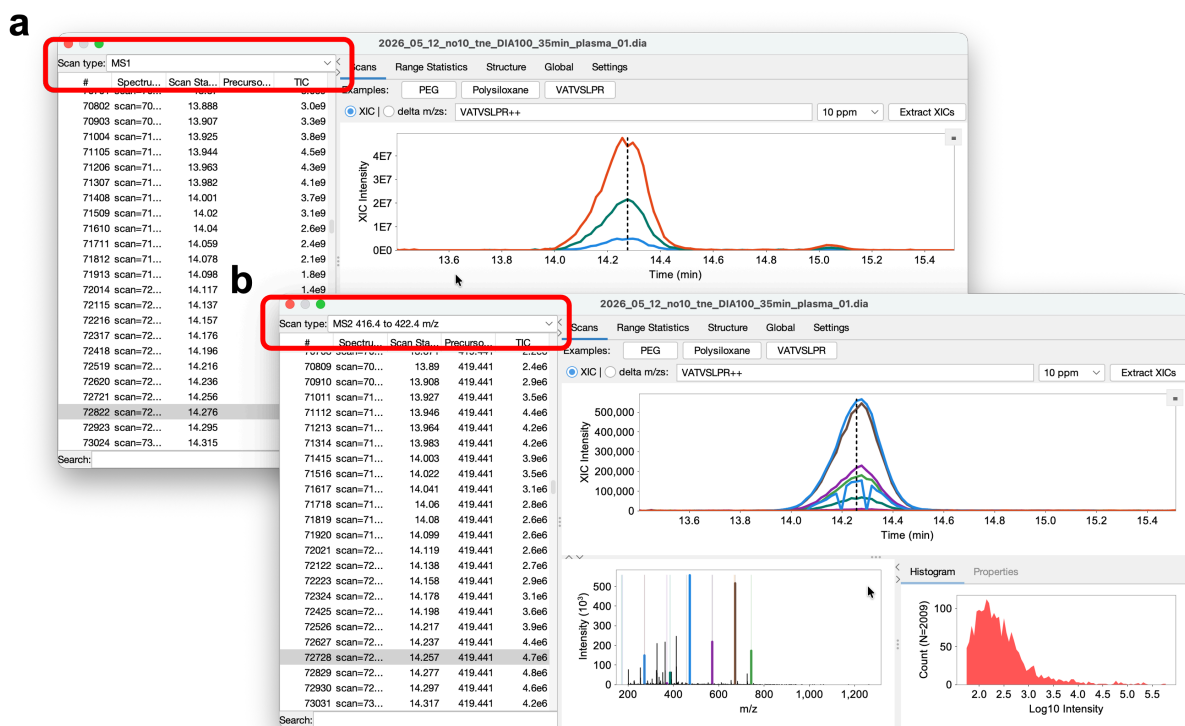


Figure 10. Peptide XICs for fast signal checks. The peptide VATVSLPR is extracted at the MS1 level (a) and MS2 level (b). Comparing precursor and fragment traces helps confirm that peptide signal is present, estimate chromatographic peak width and points across the peak, and test tailing, scheduling, or isolation hypotheses.

Use XIC extraction to turn a suspicion into a specific answer:

- **PEGs and polysiloxanes:** Extract a short series of expected contaminant masses. A repeating pattern with coherent peaks, especially late in the gradient or in blanks, supports a contaminant diagnosis.
- **Other contaminants:** For PGG-like plasticizers, detergents, or lab-specific background ions, enter the known m/z values or formulas and compare traces across the run.
- **Expected peptides:** Enter peptide sequences or precursor m/z values to confirm that peptide signal exists and elutes where expected.
- **Peak width and sampling:** Use precursor and MS2 traces to estimate whether the chromatographic peak has enough points across it for downstream quantification. If peaks are too narrow for the duty cycle, the method may need adjustment.
- **MS1 versus MS2 behavior:** Change the scan type filter before extraction to compare precursor traces with fragment or DIA-window traces. A precursor peak without corresponding MS2 signal may indicate isolation, scheduling, or sensitivity problems.

The XIC view is intentionally lightweight. It is for fast forensic confirmation, not full targeted quantification.

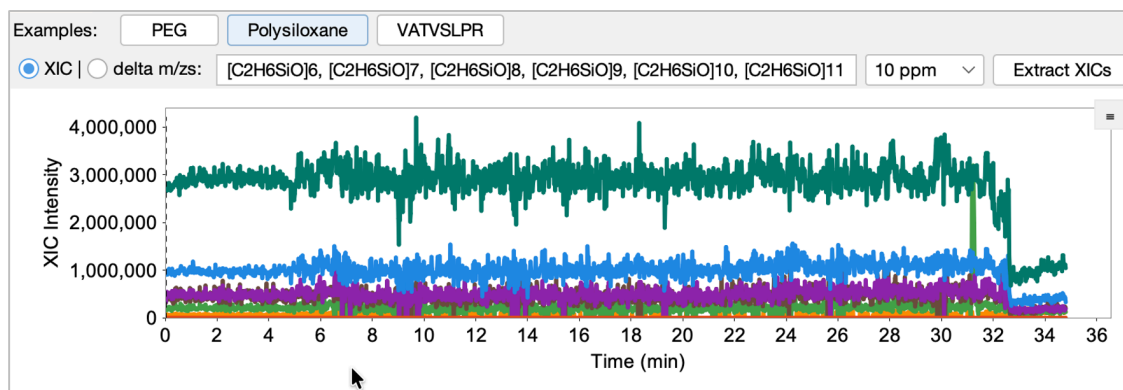
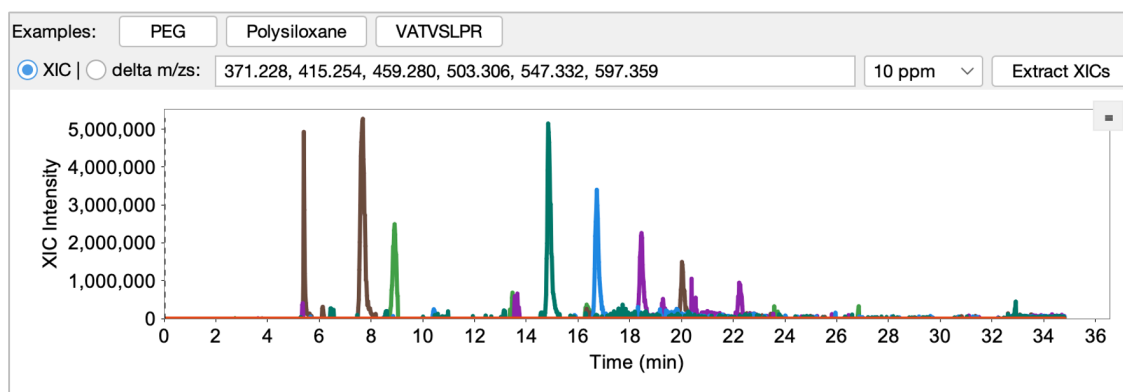
a**b**

Figure 11. Contaminant XICs. Polysiloxane traces (a) show broad atmospheric/background contamination across the run, while PEG traces (b) show a common polymer contaminant series with related masses and elution patterns. These XICs are useful when late-gradient sparkline features or blank injections flag a chemical-background question for follow-up.

Range Statistics Tab

The **Range Statistics** tab summarizes ion injection time distributions. It shows boxplots grouped by precursor isolation window and by retention-time bin.

Use this tab to ask whether the method is filling the instrument the way you expected. High ion injection times usually mean the instrument needed longer to accumulate ions, which can indicate low ion flux, weak signal, or a max-injection-time-limited region. Very low ion injection times usually mean the AGC target was reached quickly, which can reflect abundant analyte, high chemical background, or method settings that differ from neighboring windows. Retention-time bins with unusual behavior can point to gradient regions where the method or chromatography is not balanced.

For DIA and PRM methods, compare ranges that should behave similarly. One window that looks very different from adjacent windows is often more informative than the absolute value alone. Treat Range Statistics as a comparison view, not as a universal good-or-bad threshold for ion injection time.

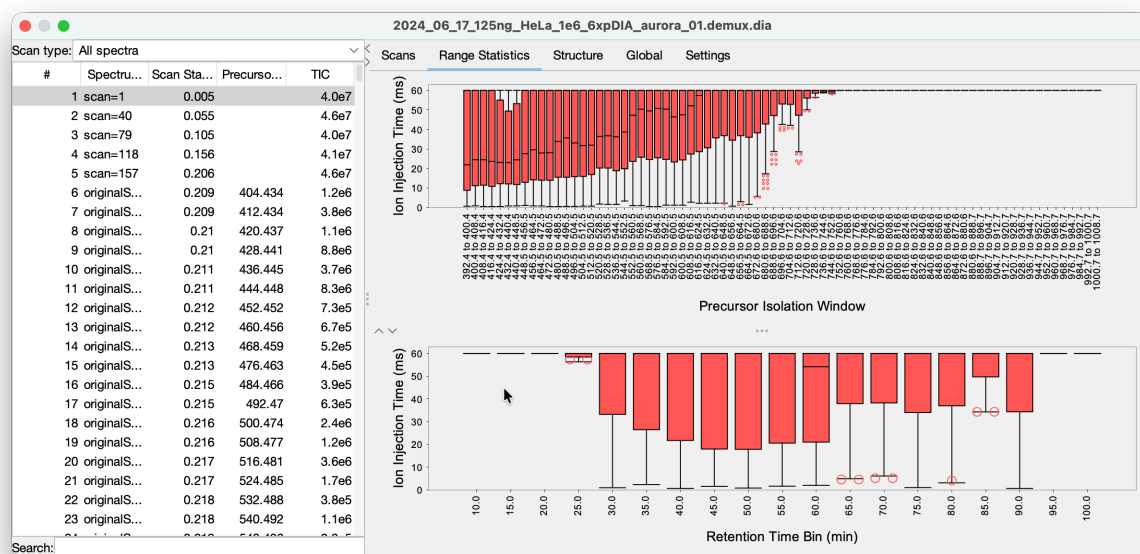


Figure 12. Ion injection time by isolation window and retention time. Range Statistics summarizes ion injection time distributions for an Orbitrap DIA run. The boxplots show median values and spread for each m/z window and retention-time range, making it easier to identify windows that are consistently high, consistently low, max-injection-time-limited, or behaving differently from neighboring windows.

Structure Tab

The **Structure** tab shows the acquisition structure across the run. For DIA and PRM-style acquisitions, this is the fastest way to confirm that the intended isolation-window layout was actually acquired.

Use this tab to identify wrong method files, missing windows, unexpected inclusion lists, or acquisition schemes that do not match the expected experiment. The important question is not "what does one scan look like?" but "did the instrument execute the scan plan I thought I loaded?"

Look for:

- Missing expected DIA or PRM windows.
- Windows that jump unexpectedly in m/z or retention time.
- Sections where the acquisition design changes when it should be constant.
- Inclusion-list or scheduled-method regions that start or stop at the wrong time.
- Methods that appear to be DDA, PRM, or DIA when you expected a different acquisition style.

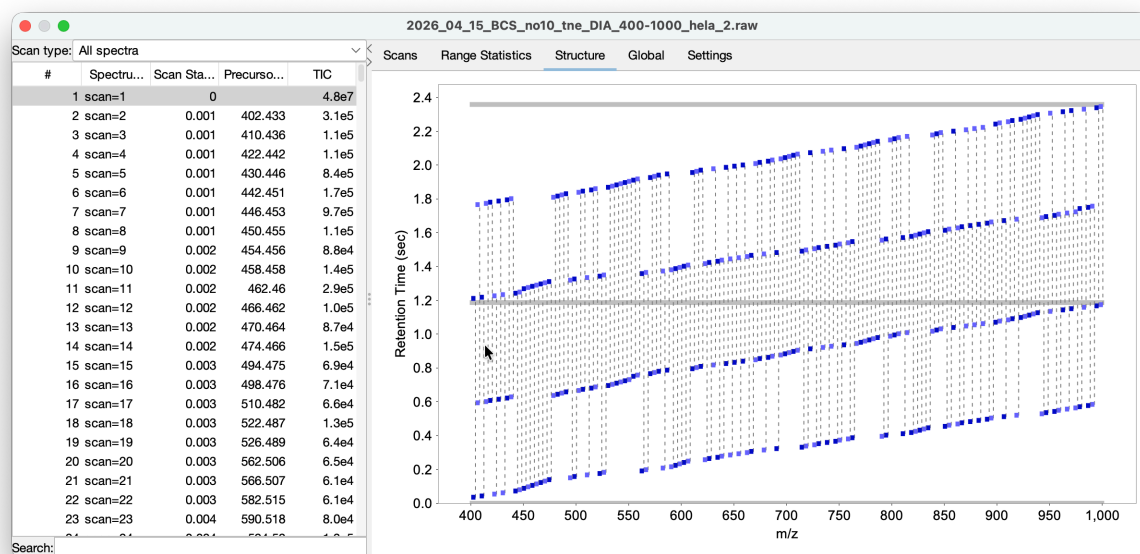


Figure 13. Acquisition structure over two cycles. The Structure view shows the first 2.4 seconds of retention time, covering two full acquisition cycles. MS1 scans are shown in gray and MS2 scans in purple, making the cycle order and isolation-window layout visible at a glance.

Global Tab

The **Global** tab shows run-level signal and acquisition trends. It is intended for quick inspection of whole-run behavior rather than individual spectra.

Use this tab to localize spray instability, signal dropouts, gradient problems, and other run-level anomalies. If the browser sparkline flagged a missing or unusual section, the Global tab is where you test when it happened and whether it affected the whole run or only certain scan types.

Questions to ask:

- Does TIC rise and fall with the expected chromatographic envelope?
- Is there an abrupt loss of signal that suggests spray dropout?
- Are there late-gradient features that should be followed up with targeted XICs?
- Do MS1 and MS2 trends diverge in a way that suggests method timing or isolation problems?
- Are acquisition summaries stable across the full method duration?

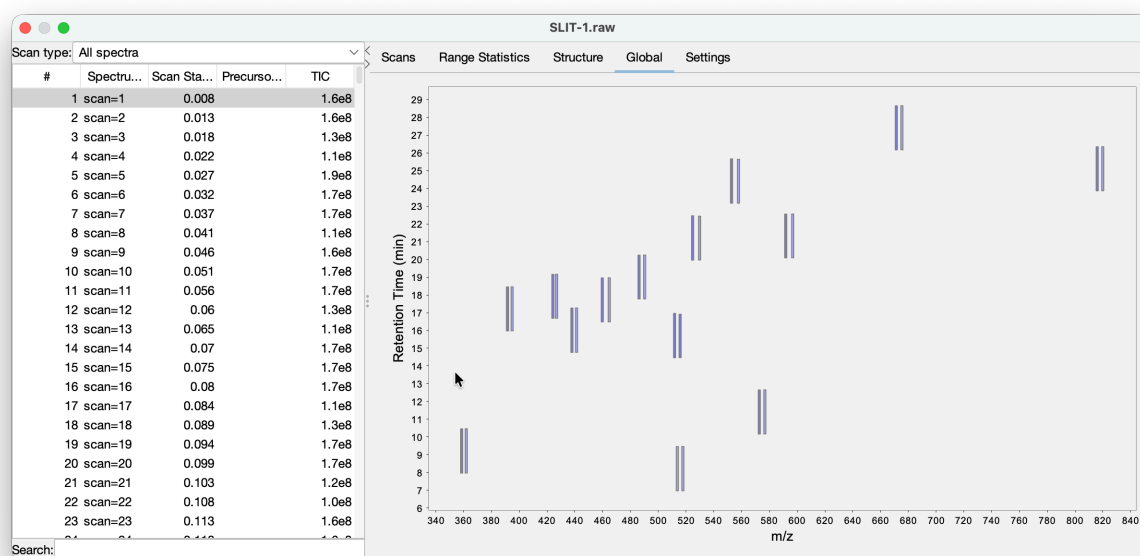


Figure 14. Global acquisition structure for scheduled PRM. This global structure view shows a heavy/light PRM method with retention-time scheduling. It is useful for confirming that scheduled windows appear at the intended retention times and that method regions are not missing, shifted, or unexpectedly jumping.

Settings Tab

The **Settings** tab shows file-level metadata in a sortable table. For Thermo files, MSForest can also display extracted instrument method text in method tabs.

This is useful for confirming that the expected method was loaded, checking instrument metadata, and diagnosing acquisition problems that are easier to see in settings than in spectra.

For Thermo files, use the instrument method text to confirm:

- Correct method duration.
- Expected scan type, polarity, resolution, and mass range.
- Expected DIA, PRM, or DDA settings.
- AGC target and maximum ion injection time settings.
- Expected source and tune-related settings.
- Whether an old method, wrong inclusion list, or wrong scheduled acquisition was loaded.

When the Structure or Global tabs reveal a method-design problem, the Settings tab is often where you find the cause.


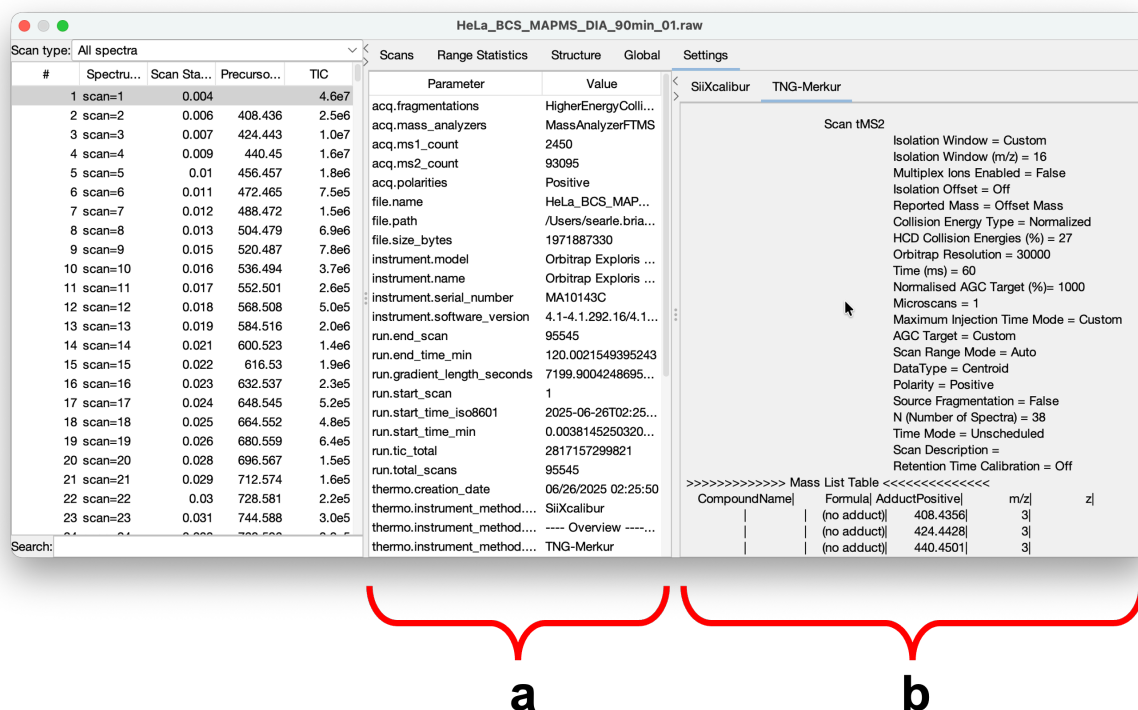


Figure 15. Raw file settings and Thermo method text. The Settings tab separates general raw-file parameters available across file types (a) from Thermo-specific method details (b), including LC and MS settings. Use this view to confirm method duration, scan settings, AGC/IIT limits, source settings, and whether the intended instrument method was loaded.

Older DIA Schema Prompt

When opening an older EncyclopeDIA .dia file, MSForest may ask whether to upgrade the file schema. Accepting the prompt updates the file so missing schema fields are available to the visualizer. If you need to preserve the original file byte-for-byte, make a copy before opening and upgrading it.

MSRawJava CLI Interface

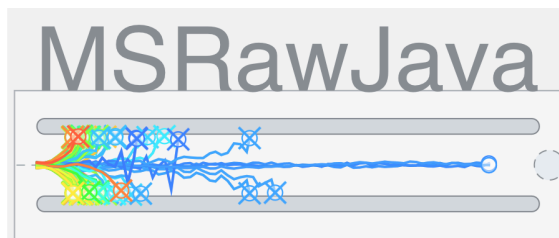

The MSRawJava CLI is intended for conversion workflows, scripted processing, and batch jobs. Use the GUI when you are still asking whether the data look trustworthy. Use the CLI when the decision has already been made and you need repeatable conversion.

The CLI answers a different set of questions:

- **Can I convert this directory reproducibly from a script?**
- **Can I run the same conversion on a workstation, server, or workflow engine?**
- **Can I convert only after GUI triage has identified the files worth processing?**
- **Can I log conversion output for later review?**
- **Can I control demultiplexing and thread count without opening the GUI?**

It accepts one or more files or directories, discovers supported input files, and writes the selected output format.

General form:

```
java -jar MSRawJava.jar [options] PATHS...
```

The exact jar name may include a version number in release packages.

For version `v26.5.28`, release artifacts commonly include `26.5.28` in the file name. Substitute the actual downloaded jar name in the examples below.

Basic Examples

Convert every supported Thermo `.raw` and Bruker `.d` file under a directory to the default EncyclopeDIA `.dia` output:

```
java -jar MSRawJava.jar /path/to/raws/
```

Write MGF files:

```
java -jar MSRawJava.jar -f mgf /path/to/raws/
```

Write mzML files:

```
java -jar MSRawJava.jar -f mzml /path/to/raws/
```

Write outputs to a separate directory:

```
java -jar MSRawJava.jar -f mzml -o /path/to/output /path/to/raws/
```

Enable staggered-window demultiplexing:

```
java -jar MSRawJava.jar -f mzml --demux --demux-ppm 10.0 /path/to/raws/
```

Write a log file:

```
java -jar MSRawJava.jar -f dia --log-file run.log /path/to/raws/
```

Process with a fixed thread count:

```
java -jar MSRawJava.jar --threads 4 -f mzml /path/to/raws/
```

Input Discovery

The CLI always discovers Thermo `.raw` files and Bruker `.d` directories. By default, directory discovery does not include `.dia` or `mzML` files unless explicitly enabled.

Use these flags when you want to convert or demultiplex existing intermediate files:

```
java -jar MSRawJava.jar --discoverDIAFiles -f mzml /path/to/dia-files/  
java -jar MSRawJava.jar --discoverMzMLFiles -f dia /path/to/mzml-files/
```

If no supported files are found, the CLI prints an error listing supported vendor/file types.

Output Format

Use `-f` or `--format` :

```
-f dia  
-f mgf  
-f mzml
```

The default is `dia` .

Output Directory

Use `-o` or `--output` to write all outputs to a directory:

```
java -jar MSRawJava.jar -o /data/converted /data/raw
```

Without `--output` , each output is written next to its input.

The CLI avoids overwriting same-format `.dia` and `mzML` inputs in the same directory by adding `.2` to the output name. Demultiplexed outputs use `.demux` in the output name.

Intensity Thresholds

The timsTOF path uses minimum intensity thresholds:

```
--min-ms1 3.0
--min-ms2 1.0
```

Raise these values to reduce low-intensity peaks in Bruker-derived output. The defaults are appropriate for typical use unless you have a specific downstream reason to change them.

Demultiplexing Options

Enable demultiplexing:

```
--demux
```

Configure demultiplexing:

```
--demux-k 7
--demux-interp cubic
--demux-interp logquadratic
--demux-exclude-edges
--demux-ppm 10.0
```

`--demux-k` sets the local approximation size. Valid values are 7 through 9. `--demux-interp` selects the interpolation method. `--demux-exclude-edges` omits edge sub-windows with single coverage. `--demux-ppm` sets the ion-matching mass tolerance.

Demultiplexing is not available for Bruker `.d` files. If requested for Bruker input, MSRawJava reports that it will process without demultiplexing.

Logging and Console Behavior

Use `--log-file` to write logs to a file. The log file is overwritten on each run.

Use `--batch` for batch environments where progress bars and status updates are not useful.

Use `--no-ansi` to disable ANSI terminal output even when the CLI detects a terminal.

Use `--silent` to suppress non-error output.

Examples:

```
java -jar MSRawJava.jar --batch --log-file convert.log /data/raw
java -jar MSRawJava.jar --silent -f mzml /data/raw
java -jar MSRawJava.jar --no-ansi -f dia /data/raw
```

Full Option Reference

<code>-f, --format [fmt]</code>	Output format: dia mgf mzml
<code>-o, --output [path]</code>	Output directory
<code>--log-file [path]</code>	Write log output to a file
<code>--min-ms1 [#]</code>	Minimum MS1 intensity threshold for timsTOF
<code>--min-ms2 [#]</code>	Minimum MS2 intensity threshold for timsTOF
<code>--demux</code>	Enable staggered-window demultiplexing
<code>--demux-k [#]</code>	Local approximation size for demux, 7-9
<code>--demux-interp [method]</code>	Interpolation method: cubic logquadratic
<code>--demux-exclude-edges</code>	Exclude edge sub-windows from demux output
<code>--demux-ppm [#]</code>	Mass tolerance in ppm for demux ion matching
<code>--discoverDIAFiles</code>	Include EncyclopeDIA .dia files during directory discovery
<code>--discoverMzMLFiles</code>	Include mzML files during directory discovery
<code>--threads [#]</code>	Processing worker threads
<code>--batch</code>	Disable status bar and progress updates
<code>--silent</code>	Suppress non-error output
<code>--no-ansi</code>	Disable ANSI output

MSRawJava Library and Building from Source

This chapter is for developers. It is intentionally brief because the main user workflow is MSForest-first triage followed by GUI or CLI conversion. Use the library when you need to ask the same questions programmatically: discover raw files, read metadata and scan summaries, extract spectra, inspect TIC traces, or convert files inside another Java application.

Library Concepts

MSRawJava normalizes supported vendor files into shared Java interfaces and model classes.

Important classes and interfaces:

- `StripeFileInterface` : common reader interface for metadata, ranges, TIC traces, scan summaries, MS1 scans, MS2 scans, and on-demand spectra.
- `ThermoRawFile` : reader for Thermo `.raw` files through the bundled local server.
- `BrukerTIMSFile` : reader for Bruker timsTOF `.d` directories through the bundled native bridge.
- `EncyclopeDIAFile` : reader/writer for `.dia` files.
- `MzmlFile` : reader for `mzML` files.
- `VendorFileFinder` : directory discovery for supported input types.
- `ConversionParameters` : shared conversion settings.
- `RawFileConverters` : conversion entry points.
- `AcquiredSpectrum` , `PrecursorScan` , `FragmentScan` , `Range` , and `WindowData` : core spectrum and acquisition-window model classes.

Minimal Reader Example

```
Path input = Path.of("/data/sample.raw");
ThermoRawFile raw = new ThermoRawFile();
try {
    raw.openFile(input);
    float gradientSeconds = raw.getGradientLength();
    var ranges = raw.getRanges();
    var summaries = raw.getScanSummaries(0f, Float.MAX_VALUE);
    var ms1 = raw.getPrecursors(0f, Float.MAX_VALUE);
    var ms2 = raw.getStripes(new Range(0f, Float.MAX_VALUE), 0f, Float.MAX_VALUE, false);
} finally {
    raw.close();
}
```

For Bruker data, use `BrukerTIMSFile` and open the `.d` directory path.

Minimal Conversion Example

```
Path input = Path.of("/data/sample.raw");
Path outputDir = Path.of("/data/converted");

ProcessingThreadPool pool = ProcessingThreadPool.createWithThreadLimit(null);
ThermoRawFile raw = new ThermoRawFile();
```



```
try {
    raw.openFile(input);
    ConversionParameters params = ConversionParameters.builder()
        .outType(OutputType.mzML)
        .build();
    RawFileConverters.writeStandard(pool, raw, outputDir, params,
        new LoggingProgressIndicator(LoggingProgressIndicator.Mode.BATCH, false));
} finally {
    raw.close();
    pool.close();
}
```

Use `RawFileConverters.writeDemux(...)` instead of `writeStandard(...)` when converting supported staggered-window DIA data with demultiplexing.

Building from Source

MSRawJava is a Maven multi-module project with `core` and `gui` modules. The project targets Java 11 for compilation. Full packaging can also build the native Thermo server and Bruker JNI bridge.

For a Java-only build:

```
mvn -DskipTests -Dskip.build.natives=true package
```

For a full build, install:

- JDK 11 or newer, with Java 17 recommended for local development.
- Maven 3.9 or newer.
- .NET SDK 8.0.x.
- Rust toolchain.
- Zig 0.12 or newer.
- `cargo-zigbuild` .

Then run:

```
mvn -DskipTests package
```

If Maven struggles with the native build, prebuild native components explicitly:

```
scripts/build-all-net.sh
scripts/build-all-rust.sh
mvn -DskipTests package
```

Run `scripts/build-all-net.sh` before `scripts/build-all-rust.sh` , because the .NET build script cleans the target space used by the packaged native resources.

For detailed platform setup, including macOS Homebrew and Windows WSL 2/Ubuntu dependency installation, see `QUICKSTART.md` .

Developer Verification Commands

Fast compile without native rebuild:

```
mvn -pl core,gui -am -Dskip.build.natives=true -Dmaven.test.skip=true compile
```

Full Java tests without native rebuild:

```
mvn -pl core,gui -am -Dskip.build.natives=true test
```

Focused tests:

```
mvn -pl core -am -Dskip.build.natives=true -Dtest=MainCliArgumentsTest test  
mvn -pl gui -am -Dskip.build.natives=true -Dtest=SomeGuiTest test
```

Scope and Alternatives

MSForest and MSRawJava are intentionally focused. They support a practical set of Thermo, Bruker timsTOF, EncyclopeDIA `.dia`, and `mzML` workflows rather than trying to cover every vendor format and conversion option.

Use MSForest when you need quick visual triage, acquisition-structure inspection, XIC extraction, or a native desktop workflow across macOS, Windows, and Linux. Use the MSRawJava CLI when you need focused, scriptable conversion for supported formats. Use ProteoWizard when you need unsupported vendor formats, non-vendor peak picking, conversion options outside MSRawJava's scope, or the broadest possible file-format compatibility.

Troubleshooting

Troubleshooting is easiest if you keep the same question-first workflow. Start with the browser to see whether the problem is visible across a directory, then use the visualizer to isolate the failure mode, then check logs or conversion output.

Common symptom-to-view mapping:

- **No sparkline or missing metrics:** start with file accessibility, truncation, unsupported format, or reader errors; check the Logging Console.
- **Flat or tiny TIC:** inspect the Scans tab and XICs for whether sample material is present; consider empty vial, failed injection, or depleted sample.
- **Sparkline gap or sudden drop:** use the Global tab to test whether there was spray dropout or acquisition interruption.
- **One replicate looks different:** open the outlier and a normal replicate side by side, then compare Global, Structure, and XIC traces.
- **Late high-intensity features:** use XIC extraction for PEGs, polysiloxanes, detergents, and other suspected contaminants.
- **Unexpected isolation behavior:** use Structure for method design and Range Statistics for AGC/IIT behavior.
- **Thermo method uncertainty:** use Settings to inspect metadata and instrument method text.

No Files Found

Confirm that the selected path contains supported files:

- Thermo `.raw`
- Bruker `.d`
- EncyclopeDIA `.dia`
- `mzML`

The CLI discovers `.raw` and `.d` by default. Use `--discoverDIAFiles` or `--discoverMzMLFiles` for directory discovery of `.dia` or `mzML`.

In the GUI, select the parent directory of the files. For Bruker data, select or browse to the directory containing the `.d` bundle.

Unsupported File Type

MSForest and MSRawJava support a focused set of raw and intermediate file types. Use the scope guidance above when a file type or conversion option is outside that supported set.

macOS Blocks the App

This usually means the package is unsigned or not notarized. Use the **Open Anyway** workflow in **System Settings > Privacy & Security**, or right-click the app and choose **Open**.

Windows SmartScreen Blocks the Installer

Click **More info**, confirm the installer is the expected MSForest download, then click **Run anyway**.

Linux Installer Does Not Run

Make sure the installer is executable:

```
chmod +x MSForest_unix_*.sh
```

Then run it from a terminal so any error message is visible:

```
./MSForest_unix_*.sh
```

Thermo Reader Startup Issues

MSForest starts the Thermo reader server automatically. If Thermo files fail to open:

- Open **Help > Logging Console** and look for server startup or port messages.
- If the GUI did not start cleanly, check the install4j `error.log` and `output.log` files next to the application launcher.
- Restart MSForest to clear a stale server process.
- Try a local file path instead of a network-mounted path.
- Confirm that security software is not blocking the bundled local server executable.

Slow Directory Scans

Directory scanning is fastest on local disks. Network drives, large Bruker `.d` directories, and directories with many files can take longer because MSForest reads gradient length, TIC, and sparkline data in the background.

If MSForest is running on an instrument computer, limit processing threads in **File > Preferences > Processing**.

Conversion Is Slower Than Expected

Check:

- Thread count in the GUI conversion panel.
- Processing thread limit in preferences.
- Whether the input is on a slow or network file system.
- Whether demultiplexing is enabled.

Demultiplexing does more computation than standard conversion and should be expected to take longer.

Demux Is Disabled

Demultiplexing is disabled for Bruker `.d` files. It is available for supported Thermo, EncyclopeDIA `.dia`, and `mzML` workflows.

Older DIA Schema Upgrade

When opening an old `.dia` file, MSForest may offer to upgrade the schema. If preserving the original file is important, make a copy before accepting the upgrade.

Licenses

MSForest and MSRawJava are distributed under the Apache License 2.0. This section lists bundled or used third-party components by license family. It is not a copy of the license terms.

Apache License 2.0

adler2, alloc-no-stdlib, alloc-stdlib, anyhow, Apache Arrow crates, atoi, base64, bitflags, brotli, cfg-if, chrono, commons-math3, core-foundation-sys, crc32fast, crossbeam-* crates, displaydoc, either, ejml-all, ejml-cdense, ejml-core, ejml-ddense, ejml-dsparse, ejml-fdense, ejml-fsparse, ejml-simple, ejml-zdense, error_prone_annotations, failureaccess, flatbuffers, flatlaf, flatlaf-extras, flate2, getrandom, Grpc.*, Grpc.AspNetCore, Grpc.AspNetCore.Server.Reflection, grpc-api, grpc-context, grpc-core, grpc-netty-shaded, grpc-protobuf, grpc-protobuf-lite, grpc-stub, grpc-util, guava, hashbrown, hashlink, iana-time-zone, integer-encoding, itoa, j2objc-annotations, libc, libm, listenablefuture, lock_api, lz4_flex, miniz_oxide, num-traits, once_cell, parquet, parking_lot, parking_lot_core, paste, perfmark-api, picocli, proto-google-common-protos, rayon, rayon-core, scopeguard, serde, serde_core, serde_derive, serde_json, seq-macro, smallvec, sqlite-jdbc, static_assertions, thrift, timsrust, twox-hash, zerocopy, zstd, zstd-safe, and zstd-sys.

MIT License

animal-sniffer-annotations, byteorder, bytes, checker-qual, CommandLineParser, combine, fallible-iterator, fallible-streaming-iterator, jsvg, libsqlite3-sys, linreg, memchr, Microsoft.AspNetCore.* packages, Microsoft.Extensions.* packages, Microsoft .NET runtime components, Newtonsoft.Json, Newtonsoft.Json.Bson, OpenMcdf.Extensions, ordered-float, rusqlite, System.* packages, .NETCore.App Runtime 8.0.25, and.AspNetCore.App Runtime 8.0.25.

BSD-Style Licenses

Google.Protobuf, protobuf-java, ryu, and snap.

Mozilla Public License 2.0

OpenMcdf and openpdf.

GNU Lesser General Public License 2.1

jcommon, jfreechart, and trove4j.

CDDL 1.1

javax.annotation-api.

Thermo Fisher Scientific Proprietary Licenses

CommonCore BackgroundSubtraction, CommonCore Data, CommonCore MassPrecisionEstimator, CommonCore RandomAccessReaderPlugin, CommonCore RawfileReader, and RawFileReader.