



The only corrected MR direction did not pass instrument-level orientation checks

a 224-direction MR status

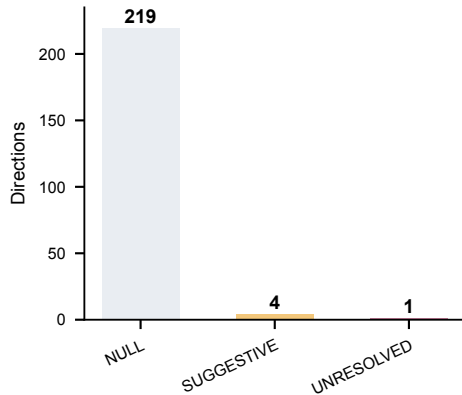

b CRAE-CKD instrument audit



c Directionality audit

Wald $P = 2.60 \times 10^{-6}$
 $F = 40.83$

Steiger = FALSE
 $P = 6.62 \times 10^{-7}$; no replication

Directional support not established