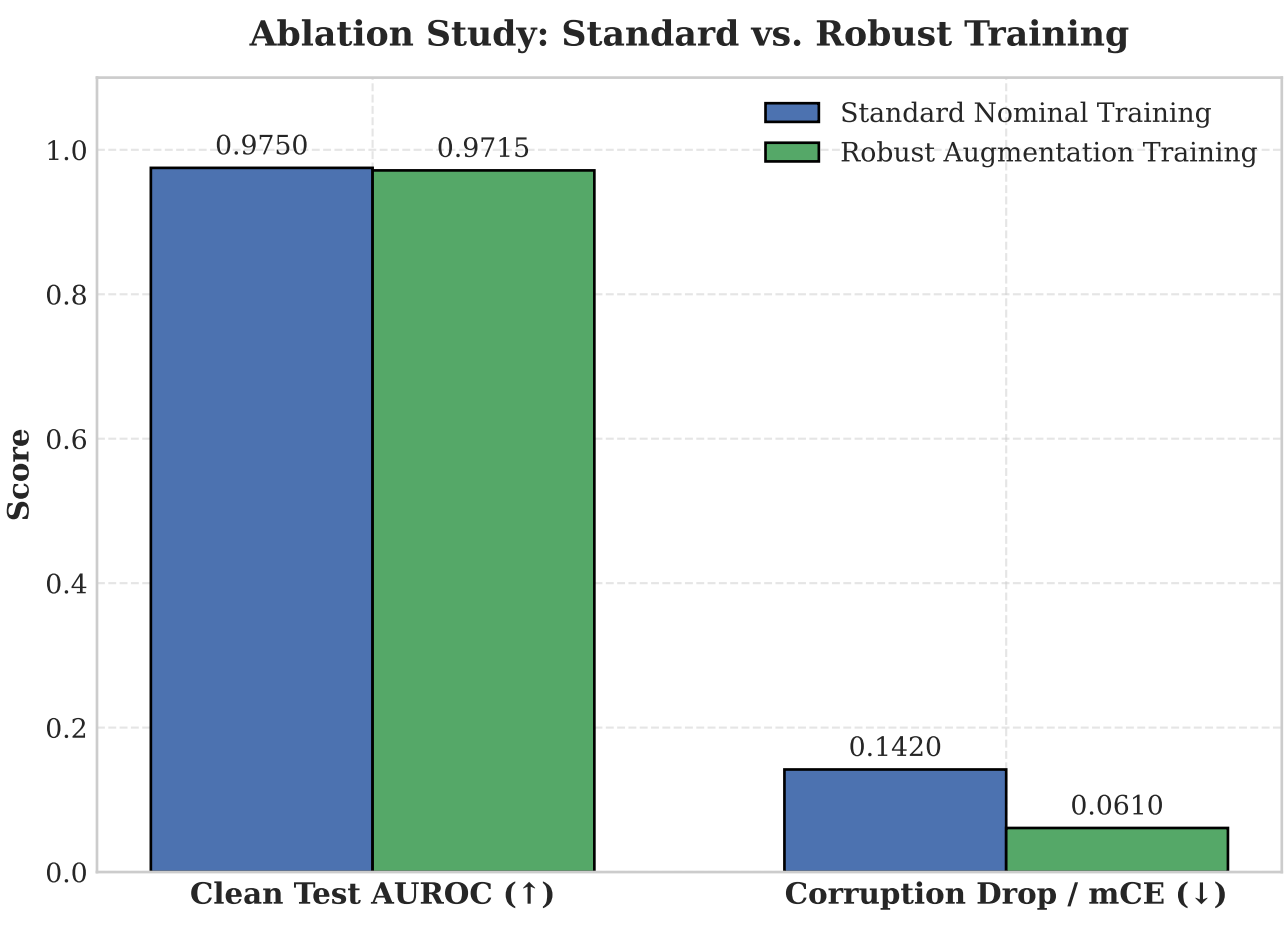
Ablation Study: Standard vs. Robust Training
Standard Nominal Training
Robust Augmentation Training
Score
1.0
0.8
0.6
0.4
0.2
0.0
0.9750
0.9715
0.1420
0.0610
Clean Test AUROC (↑)
Corruption Drop / mCE (↓)