**HARTMANN**

Easy Care Hub · Clinical visualisation platform

REV. 1.4 · 2026-04 · PR-ECH-0001 · 2026-04

# User Manual

## HARTMANN Easy Care Hub

| AUDIENCE | APPLIES TO | LANGUAGE |
| --- | --- | --- |
| **Authorised care-facility staff** | **Easy Care Hub v1.4.x** | **English (EN)** |

**Important — not an emergency alarm system**

The Easy Care Hub platform is not a medical device under EU MDR 2017/745. It is intended solely for the visualisation of data generated by connected devices. In case of acute, life-threatening symptoms, contact emergency services immediately.

DISTRIBUTOR

**PAUL HARTMANN AG**

Paul-Hartmann-Straße 12 · 89522 Heidenheim · Germany · info@hartmann.info

ON THIS DOCUMENT

# Table of contents


| | | |
|---|---|---|
| 1 | General | 3 |
| 2 | Platform overview | 6 |
| 3 | Residents overview | 10 |
| 4 | Resident detail page | 12 |
| 5 | Notifications | 16 |
| 6 | Devices | 19 |
| 7 | Administration | 20 |
| 8 | My account | 23 |
| 9 | About & legal | 24 |


© 2026 PAUL HARTMANN AG

SECTION

# 1 General

This User Manual describes the functionality of the HARTMANN Easy Care Hub platform and provides guidance on its use. The platform is intended for authorised staff in care facilities to visualise and organise resident-related data produced by connected monitoring devices. It covers navigation, user roles, notification configuration, administration and day-to-day clinical workflows.

## 1.1 Scope and intended audience

Easy Care Hub is intended for authorised care-facility personnel — System Owners, Administrators, Head Nurses and Nurses — to visualise heart rate, breathing rate and bed-presence data alongside configured notifications. It is not intended for life-critical alarming, diagnostic decision-making or continuous emergency monitoring.

## 1.2 Important safety and usage information

- The Easy Care Hub platform itself is not a medical device under EU MDR 2017/745. It is intended solely for the visualisation and presentation of data generated by connected devices.
- Values shown are for informational purposes only. They are not intended for diagnostic or therapeutic use and must not be used as the sole basis for medical decisions, treatment or clinical interventions.
- Clinical decisions remain the sole responsibility of qualified healthcare professionals based on a comprehensive assessment of the resident using appropriate medical judgement and established clinical procedures.
- The accuracy, completeness and availability of the displayed data depend on correct functioning, configuration and data transmission of the connected medical devices.
- The Easy Care Hub does not guarantee real-time monitoring. Displayed values may be subject to processing or transmission delays.
- Always verify critical information using appropriate clinical methods. Do not rely exclusively on the platform.
- Connected devices remain regulated medical devices subject to their own Instructions for Use.

© 2026 PAUL HARTMANN AG

**WARNING**

**Not an emergency alarm**

The Easy Care Hub is not intended to be used as an alarm system for life-threatening situations in which immediate medical intervention is necessary. Real-time delivery of alerts cannot be guaranteed. In case of acute, life-threatening symptoms, contact emergency services immediately.

## 1.3 Roles and permissions

Three roles are supported: System Owner, Administrator and User. The permission model uses CRUDS — Create, Read, Update, Delete, Share. The table below summarises per-capability permissions.

| Capability | System Owner | Administrator | User |
|---|---|---|---|
| **Vital signs** | R | R | R |
| **Devices** | RUS | RUS | — |
| **Locations** | CRUS | RUS | R |
| **Residents** | CRUS | CRUS | RS |
| **Users** | CRUS | CRUS | — |
| **Individual thresholds** | CRUS | CRUS | R |
| **Baseline thresholds** | CRUS | CRUS | R |
| **Reports** | R / Download | R / Download | R / Download |
| **Notifications** | R / Reviewed | R / Reviewed | R / Reviewed |

*C = Create · R = Read · U = Update · D = Delete · S = Share · — = no access*

## 1.4 Abbreviations and glossary

**HR**
Heart Rate — number of heartbeats per minute.

**BrR**
Breathing Rate — number of breaths taken per minute.

**Global settings**
Notification configurations that apply system-wide to all residents.

**Individual settings**
Per-resident overrides for global settings, e.g. out-of-bed duration.

**Baseline**
A personalised threshold derived from the resident's recent data history.

**MDR**
Medical Device Regulation (EU) 2017/745.

**Audit log**
Per-resident archive of notifications already reviewed by a caregiver.

© 2026 PAUL HARTMANN AG

SECTION

# 2 Platform overview

## 2.1 Login

Only authorised users can access the Easy Care Hub interface. After your account is created and a password set, sign in with your registered email address and password. The login also supports Single Sign-On when configured at facility level.

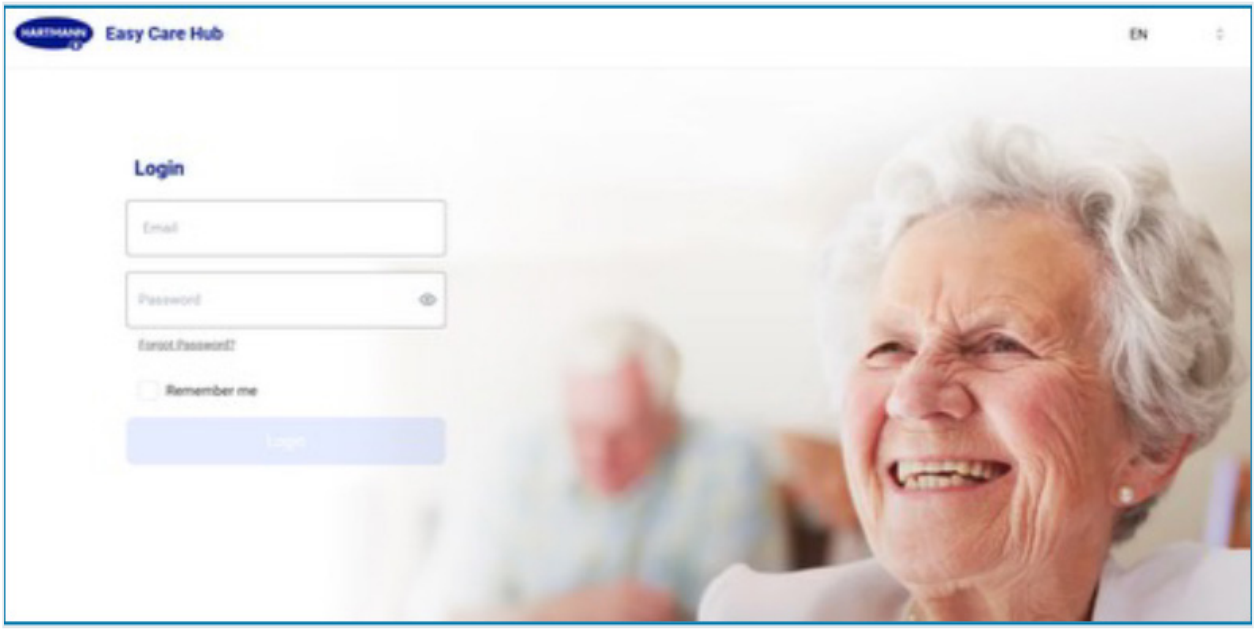


*Fig. 2.1 — The Easy Care Hub login screen.*

1. Enter your user email in the email field.
2. Enter your password in the password field.
3. Click Login. The platform authenticates your credentials and displays the Dashboard with resident tiles.
4. If you tick Remember me, your email will be remembered on the device.
5. Use Forgot password? to request a reset link. A confirmation message and a Return home button are shown.

## 2.2 Menu

On login, the Vitals Dashboard opens by default. The left-hand menu can be expanded or collapsed via the arrow at the bottom. The following sections are visible according to your role:

- Vitals
- Residents
- Notifications
- Devices
- Administration

## 2.3 Navigation bar

The top navigation bar is always visible. From left to right it contains:

- The HARTMANN / Easy Care Hub logo — returns to the Dashboard.
- The Support icon — opens the Legal/About and FAQ tabs.
- The user icon — opens My Account, About Us and Log out.

## 2.4 Dashboard

The Dashboard is the default landing view after login. It displays all devices assigned to the facility, grouped by zone. Resident tiles are colour-coded by current status. Clicking a tile opens the Resident Detail Page on the Trends tab.

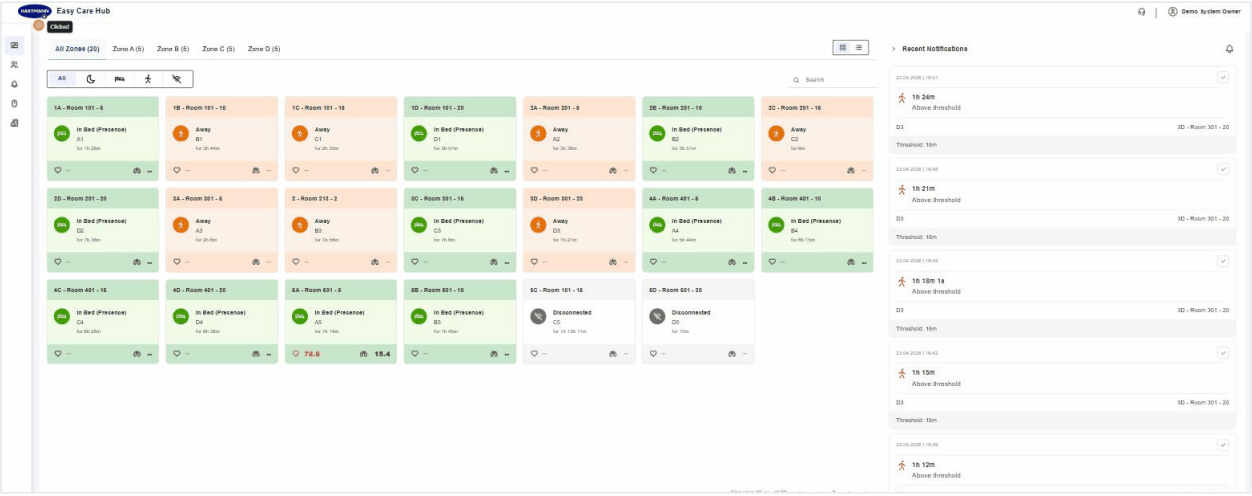


*Fig. 2.2 — The Vitals Dashboard with zone tabs, status-filter icons, resident tiles and the notification sidebar.*

### ZONES

Tabs across the top group residents by facility zone — e.g. All Zones, Zone A, Zone B, Zone C, Zone D — with the resident count shown beside each label. Selecting a tab filters every tile on the

Dashboard to that zone only.

All Zones is selected by default. Click another zone tab to filter the view to devices assigned to that zone.

### VIEW TOGGLE

Switch between tile view and table view using the toggle at the top right. The table view shows the same resident data in columns — Resident ID, Status, Duration, BrR (brpm), HR (bpm), Location, Zone, Device ID, Last updated — for quick scanning of large facilities.

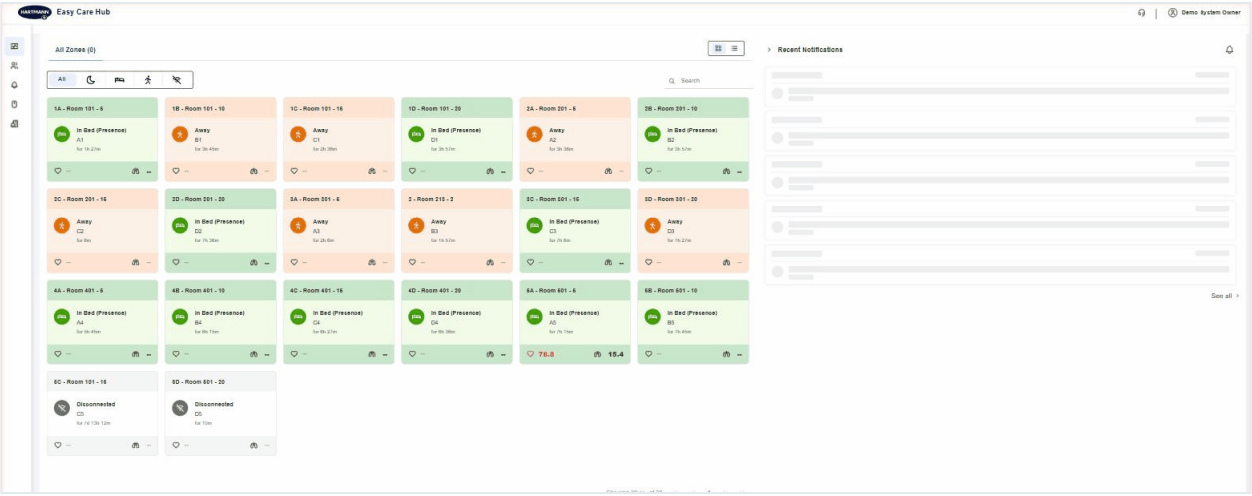


*Fig. 2.3 — Dashboard in table view: the same residents as columns for scanning a full floor at once.*

### VISUAL STATUS FILTER

Use the visual status filter to narrow the dashboard by resident status: All, Asleep, Away, In Bed or Disconnected.

### SEARCH

Use the search field to find a specific device number or resident identifier.

### NOTIFICATION SIDEBAR

The sidebar lists active notifications for HR, BrR and Out-of-Bed in order of triggering. Click the check icon to mark a notification as reviewed — it is removed from the sidebar and archived to the resident's Audit Log. Click See all to open the full Notifications page. The bell icon at the top right collapses or expands the sidebar.

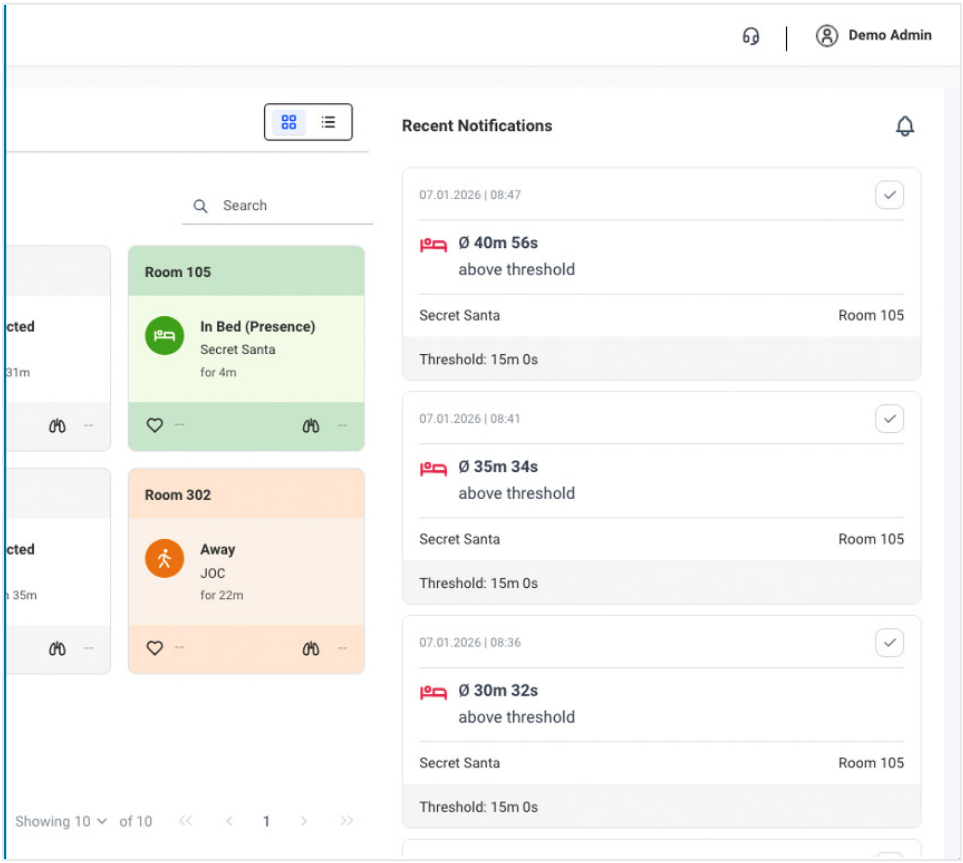


*Fig. 2.4 — The notification sidebar showing recent out-of-bed alerts and resident status tiles.*

**TIP**

### Keyboard shortcuts

Press 1–9 to switch between the first nine zones. Press / to focus the search field. Press ? to open the keyboard shortcut reference.

SECTION

# 3 Residents overview

Selecting Residents in the left menu opens the Residents overview — a single table of every resident in the facility with their linked device and location. Columns shown:

- Resident ID
- Device ID
- Zone
- Location
- Resident status (Active / Discharged)

## 3.1 Finding a resident

Use the search field at the top of the table to filter by Resident ID, device or location. Matches are ranked by recency.

## 3.2 Creating a new resident

Click + Create Resident in the top-right corner. A sidebar opens on the right with the following fields:

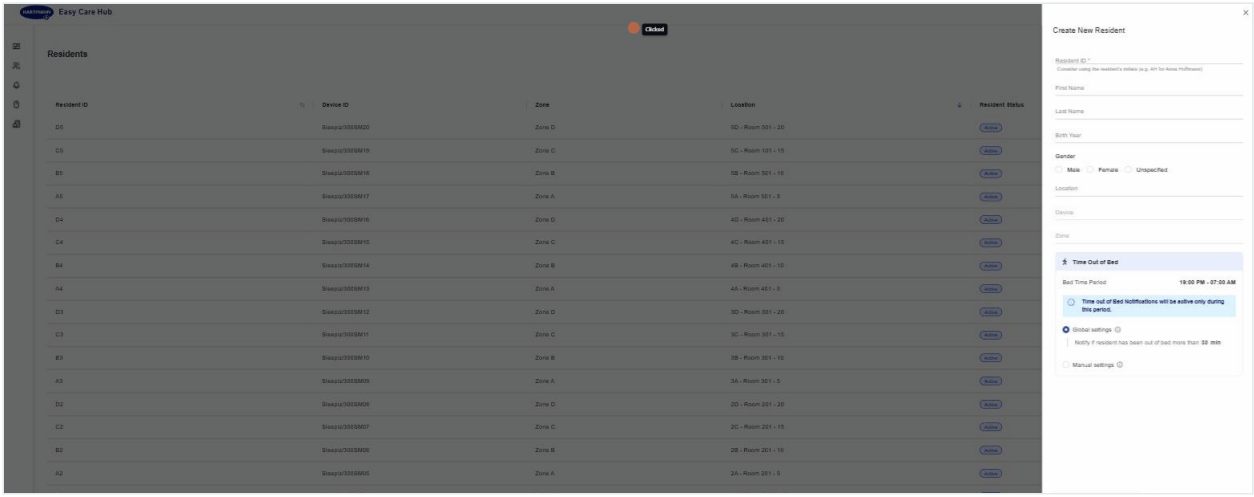


*Fig. 3.1 — Create New Resident sidebar with ID, name, location and time-out-of-bed settings.*

1. Resident ID (required).

2. First name, last name, date of birth (optional).
3. Gender (optional).
4. Location (dropdown). Once selected, Device and Zone fields become active; Zone is filled automatically based on location.
5. Time-out-of-bed notification — defaults to the global setting. Choose Manual settings to override.

> **NOTE**
>
> **Location already assigned**
>
> If the chosen location is already assigned to another resident, a confirmation popup appears. Click Yes to reassign the location, or No to leave the field blank.

Manual settings offer three options: notify if the resident has been out of bed more than N minutes; notify if the resident is out of bed N% longer than usual; disable. When all mandatory fields are filled, the Create button becomes active; the sidebar closes and a confirmation message appears.

SECTION

# 4 Resident detail page

The Resident Detail Page can be reached from several entry points: the Residents list (Overview tab), a Dashboard tile (Trends tab), or a notification (Notifications tab). The header always shows Resident ID, HR (bpm), BrR (brpm) and bed presence.

## 4.1 Overview tab

Displays general information about the resident, split into Details and Individual Notifications.

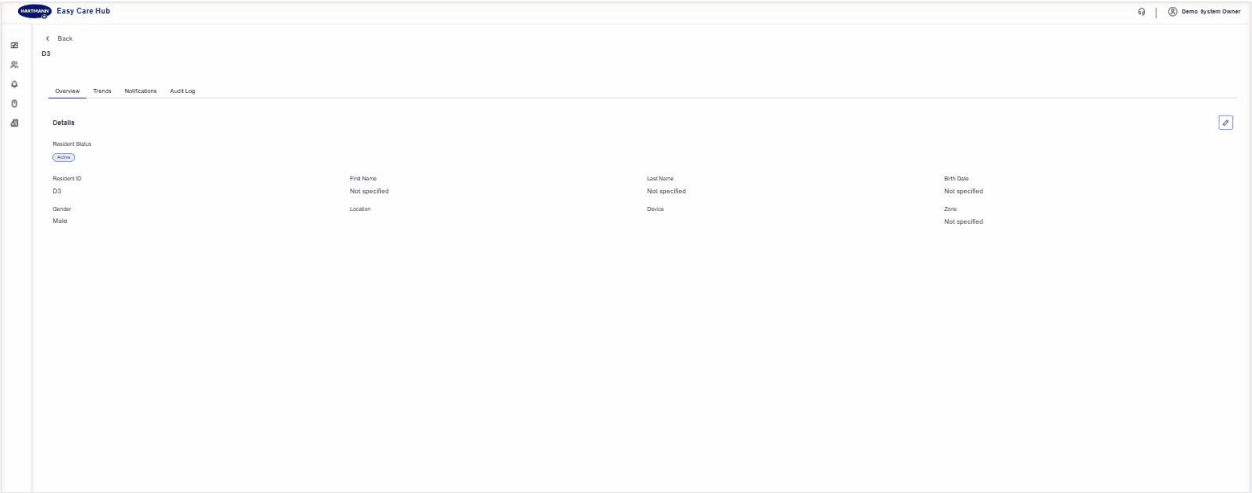


*Fig. 4.1 — Resident Detail · Overview tab. Status, ID, name, birth date, gender and assignment to location / device / zone.*

### DETAILS

- Status (Active / Discharged)
- Resident ID
- First & last name, date of birth
- Gender
- Location, Device, Zone

### INDIVIDUAL NOTIFICATIONS

- Time-out-of-bed rule — inherits the global rule by default, or can be overridden.
- Bedtime period is editable only from the Administration section, not here.

- Manual settings expose the same three options as during resident creation.

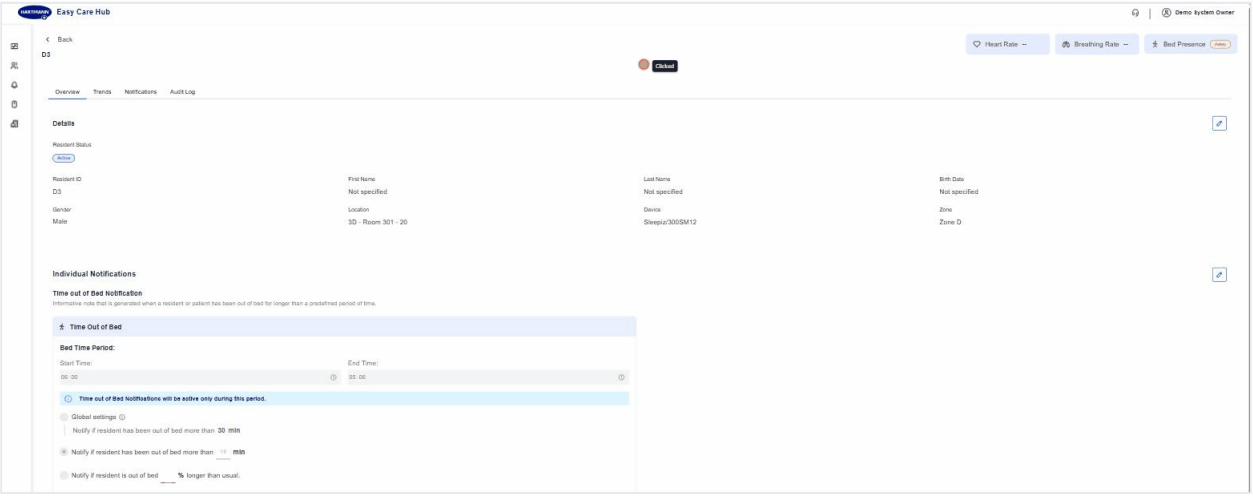


*Fig. 4.2 — The Individual Notifications section of the Overview tab. Per-resident Time-out-of-Bed rules override the facility-wide default.*

## 4.2 Trends tab

Shows the resident's HR and BrR over time alongside the last night's sleep report. Filter by date or timeframe. Y-axis ranges: HR 40–120 bpm, BrR 5–40 brpm. Yellow and purple markers indicate the configured global thresholds and baseline values.

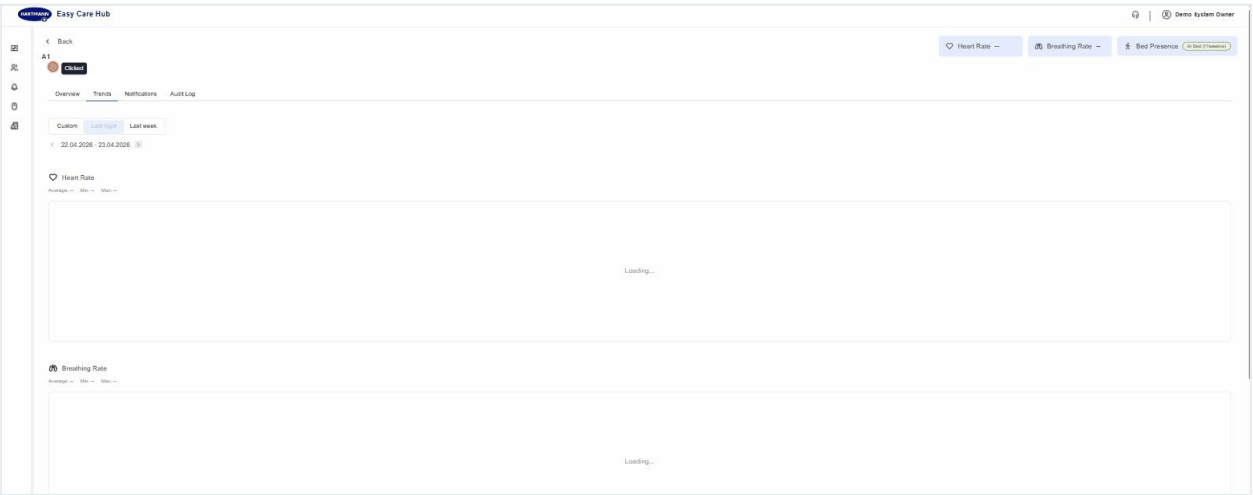


*Fig. 4.3 — Trends tab with Custom / Last night / Last week presets and Heart Rate + Breathing Rate line charts.*

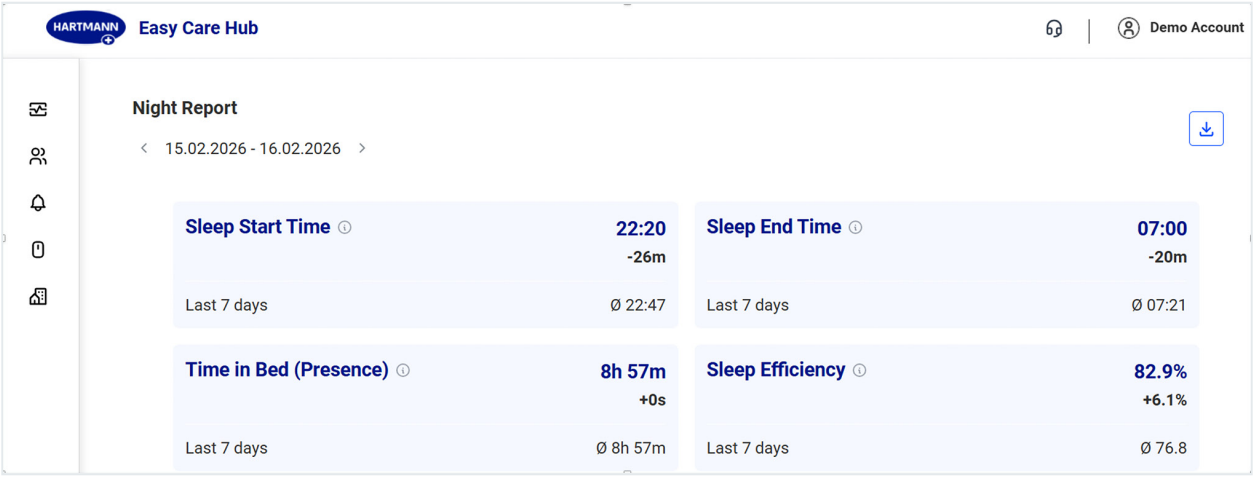


*Fig. 4.4 — Night report on the Trends tab, with sleep start / end, time in bed, and sleep efficiency against the 7-day average.*

**TIP**

**Why is data missing?**

Night-report data are typically delivered about 30 minutes after the facility's defined night period. If values are still missing, data quality may have been insufficient — for example, the resident was not in bed, or fewer than four hours of data were recorded. If this occurs repeatedly while the resident was in bed, contact customer service.

## 4.3 Notifications tab

Lists every notification for this resident with Type, Resident ID, Device ID, Time, Details and Actions. Three preset ranges are available above the table:

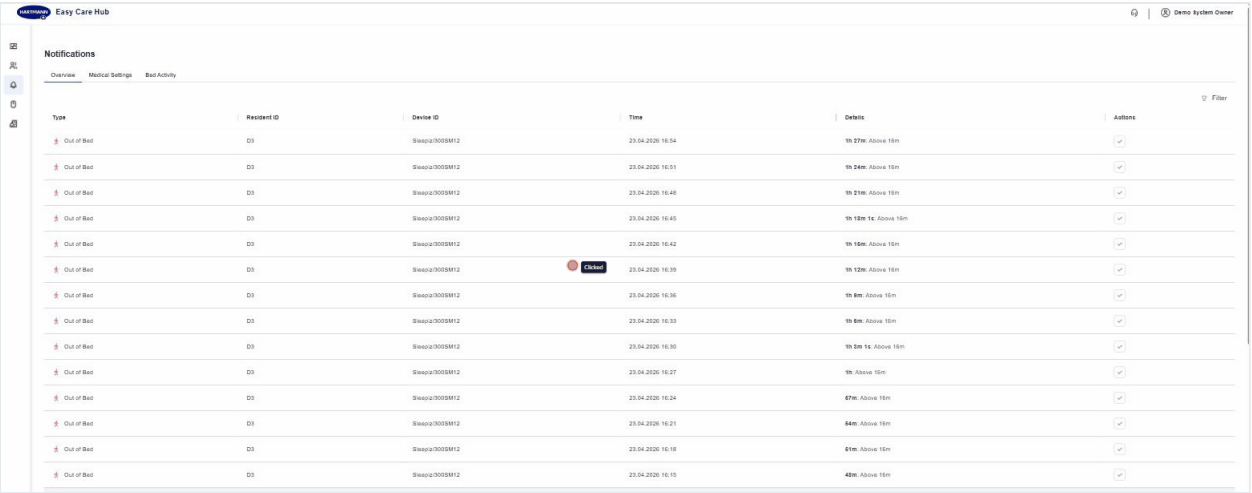


*Fig. 4.5 — Notifications tab on the Resident Detail Page, with preset date ranges, filter and per-row acknowledge.*

- Custom — pick a calendar date range.

- Last Night.
- Last Week.

Mark a notification as reviewed using the check icon in the Actions column. Once reviewed, it is removed from this tab and moved to the Audit Log. Click Filter to narrow by type (HR, BrR, Out of Bed); active filters show as chips above the table.

## 4.4 Audit Log tab

A chronological archive of every reviewed notification. Columns: Type, Device ID, Time, Details, Actions. Since these entries have been reviewed, the check icon is not interactive. Audit Logs can be exported as CSV or PDF from the toolbar.

© 2026 PAUL HARTMANN AG

SECTION

# 5 Notifications

The Notifications page aggregates alerts across the entire facility. Reach it from the left menu or via See all in the Dashboard sidebar. Three tabs are available:

- Overview
- Medical settings
- Bed activity

## 5.1 Overview tab

All active notifications across all residents, listed chronologically with Type, Resident ID, Device ID, Time/Details and Actions. Mark-as-reviewed and advanced filtering are supported. Filter criteria: Type, Resident ID, Device ID, Period and Status (New / Reviewed).

## 5.2 Medical settings tab

Global notification settings for clinical values. Configured rules apply to all residents and cannot be overridden at resident level. Two notification models are available:

**Threshold-based**
Alerts trigger when HR or BrR crosses configured static thresholds.

**Baseline-based**
Alerts trigger when values deviate significantly from the resident's own recent history.

By default the platform pre-fills these values using ranges derived from medical studies and established clinical guidelines. Click the edit icon on the right to modify; the other tabs become unavailable while a bottom bar with Cancel and Save is shown.

NOTE

**Typical default thresholds**

Heart Rate alert range: 72–78 bpm. Breathing Rate alert range: 12–27 brpm. These are starting points only — each facility should validate ranges with its clinical lead before going live.

## 5.3 Bed activity tab

Configures the Out-of-Bed notification applied to all residents by default. Override per resident from the Resident Detail page. Three rules can be applied:

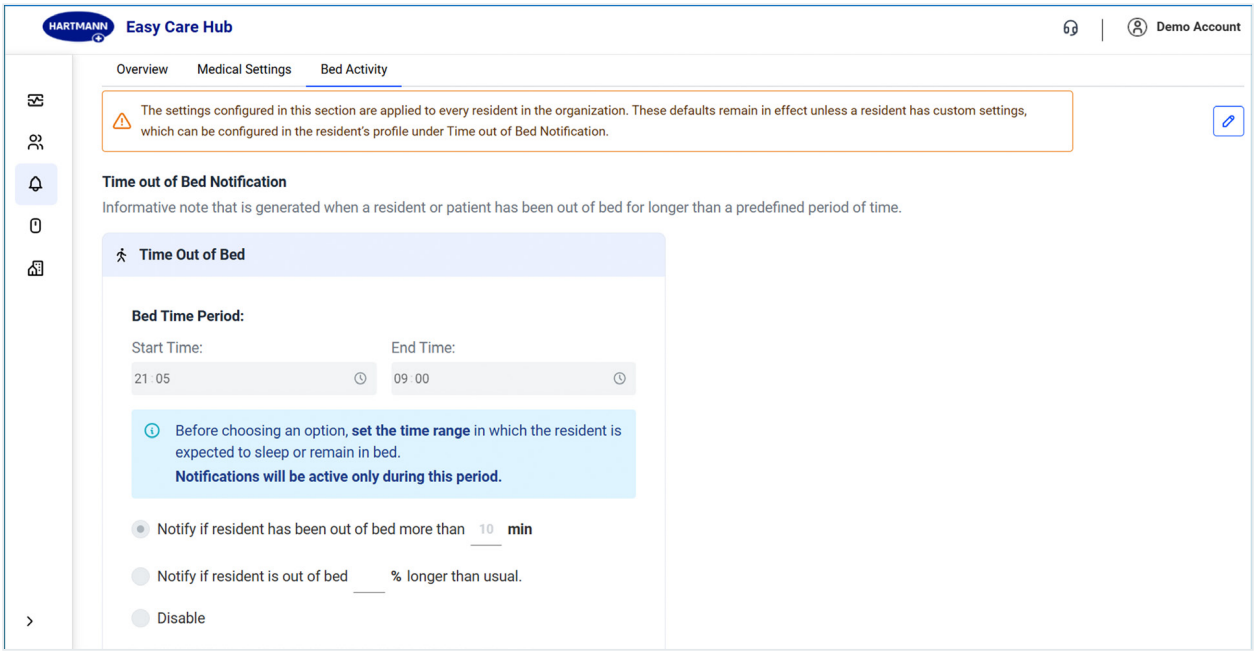


*Fig. 5.1 — Bed Activity tab: facility-wide out-of-bed rules and bedtime period.*

1. Notify if the resident has been out of bed more than N minutes.
2. Notify if the resident is out of bed N% longer than usual.
3. Disable.

Set the Bedtime Period by clicking the time fields. Notifications remain enabled during these hours — when residents are expected to be sleeping.

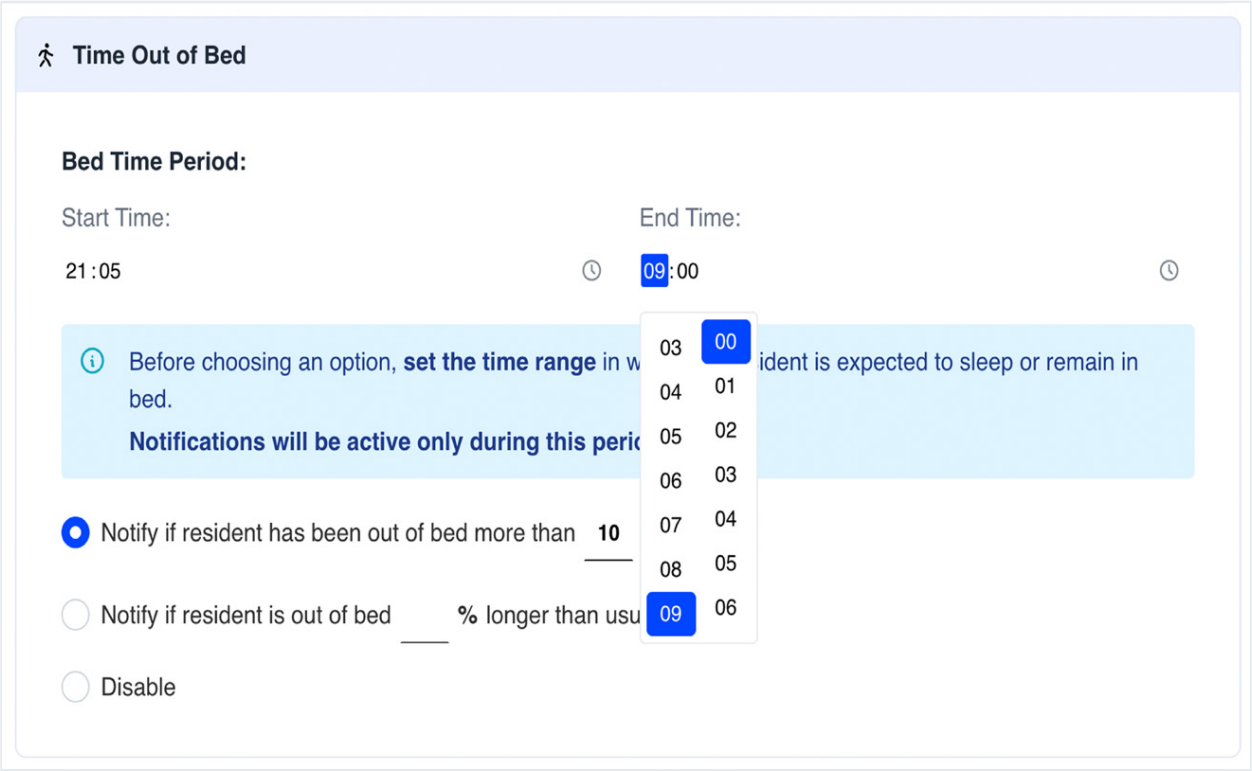


*Fig. 5.2 — Bedtime Period picker.*

SECTION

# 6 Devices

NOTE

**Role restriction**

The Devices page is visible only to System Owner and Administrator roles. Head Nurse or Nurse users will not see this section.

The Devices page lists every device in the facility:

- Device ID
- Zone
- Location
- Resident ID
- Device status (Active / Disconnected)

Clicking a device opens its detail page. Zone, Location and assigned Resident can be edited from there; you may also create a new Location inline via + Create new location. Cancel prompts a confirmation popup if unsaved changes exist; Save persists the change and shows a confirmation toast.

© 2026 PAUL HARTMANN AG

SECTION

# 7 Administration

**NOTE**

**Role restriction**

Administration is visible only to System Owner and Administrator roles. Only System Owners can delete zones, locations or users.

Administration gathers Zones, Locations and Users. Create-action buttons and a Back link are always visible at the top.

## 7.1 Zones

Table of every zone with Name, Description, Total / Active / Disconnected device counts and Actions (Delete — System Owner only). Create a zone via + Create Zone; Name is required, Description optional.

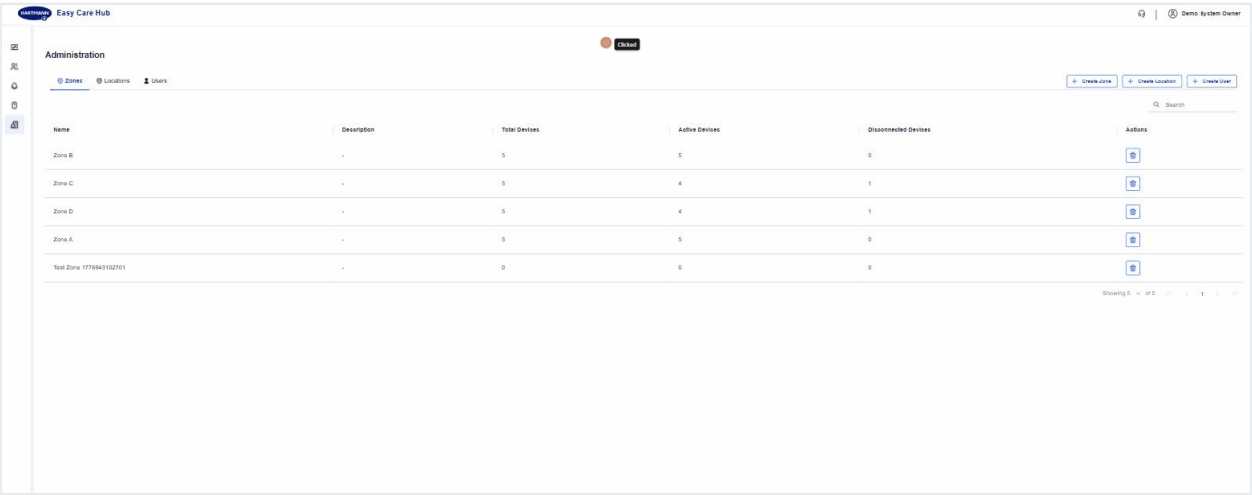


*Fig. 7.1 — Administration · Zones, showing device counts per zone (total, active, disconnected) and the Create Zone / Location / User actions top-right.*

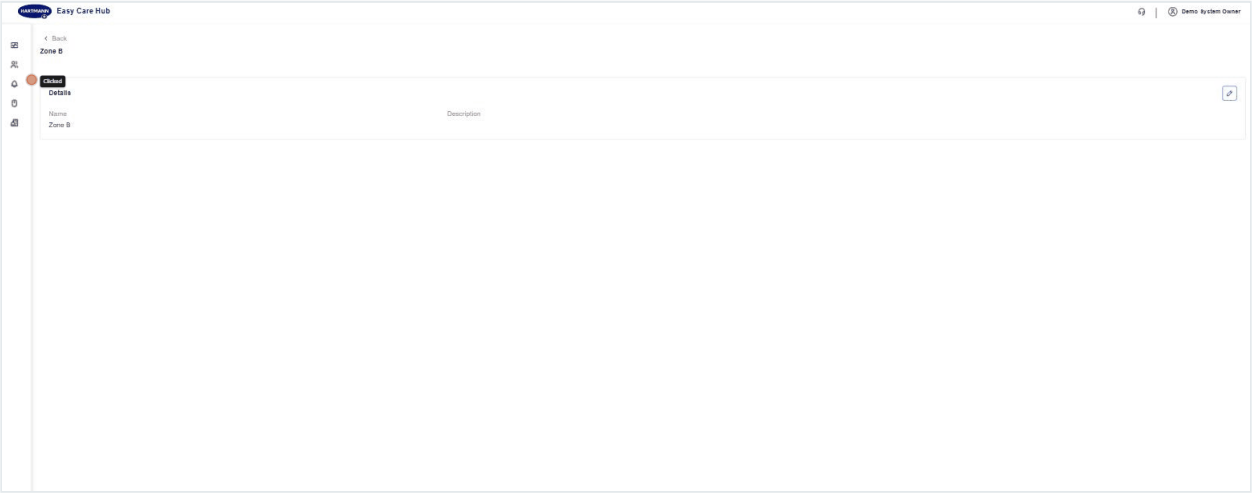


*Fig. 7.2 — Zone detail: editable Name and Description, with an edit icon top-right.*

## 7.2 Locations

Table of every location with Name, Zone, Device ID, Resident ID and Actions. Create a location via + Create Location; Floor, Room and Bed populate a live Preview. Saving enables the Create button once at least one field is filled.

## 7.3 Users

Lists every user with Name, Access Level, Email, Status and Last Updated. Create new users via + Create User with First Name, Last Name, Email, Role and Access Level — the level's capabilities are shown below the field for clarity.

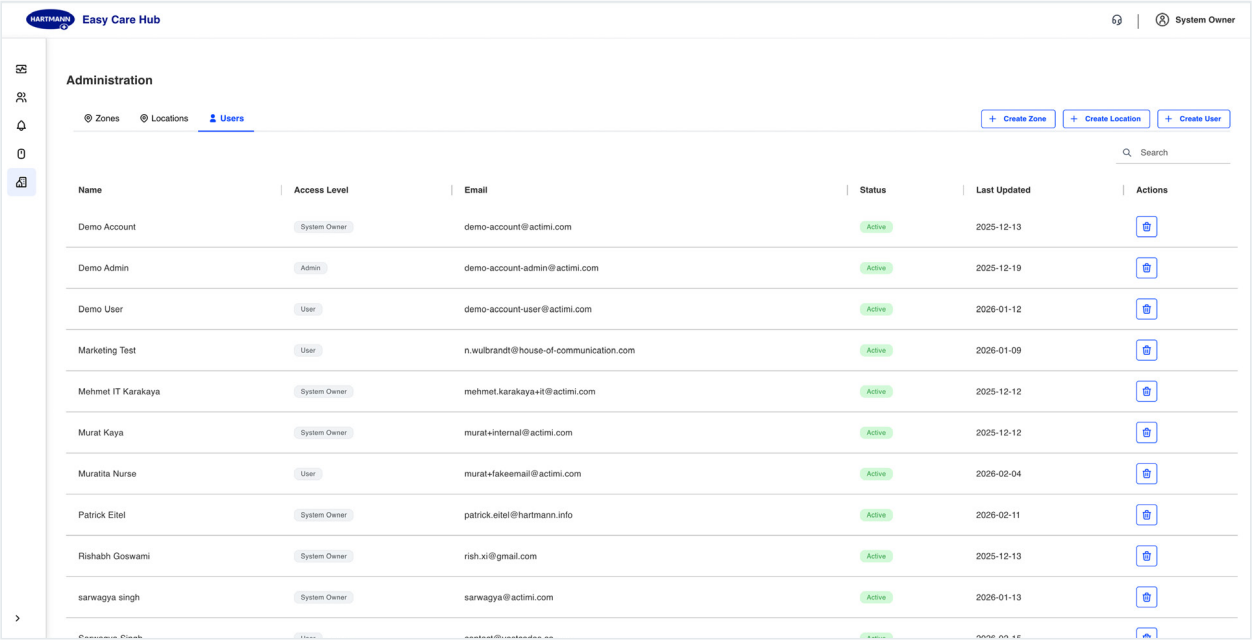


*Fig. 7.3 — Administration · Users. Each row shows role badge, email, status and last-updated timestamp.*

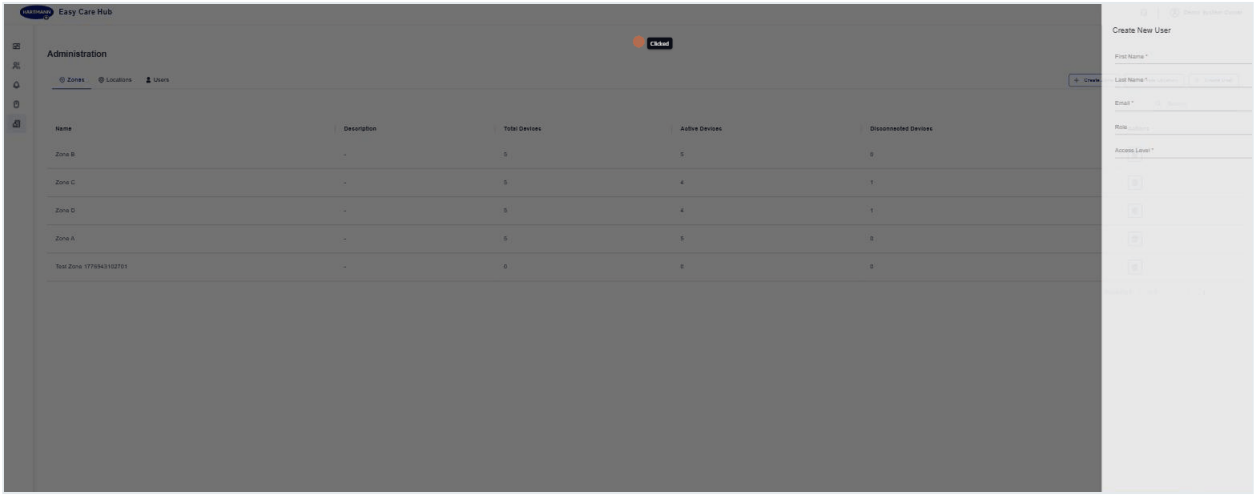


*Fig. 7.4 — Create New User sidebar: First / Last Name, Email, Role and Access Level. Access-level capabilities appear below the selection.*

SECTION

# 8 My account

Click the user avatar in the upper-right corner and select My Account to view and edit your profile. The editable fields are:

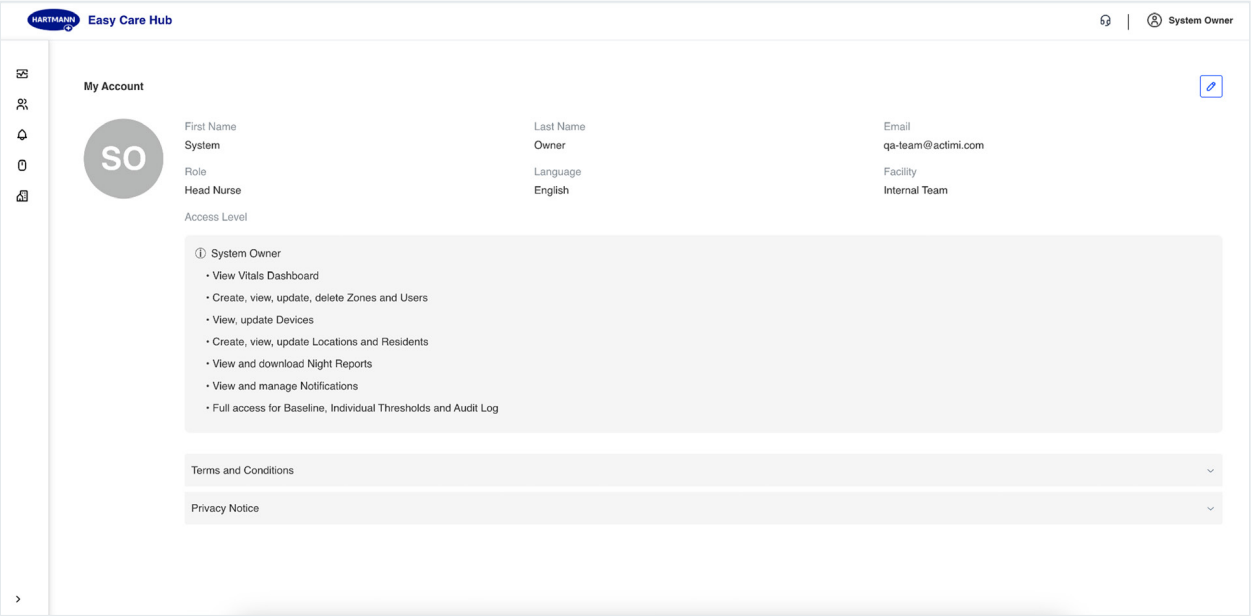


*Fig. 8.1 — My Account page showing role-level capabilities.*

- First name (editable)
- Last name (editable)
- Email (editable)
- Role
- Language — English or Deutsch
- Facility
- Access Level
- Terms & Conditions, Privacy Notice

Click the edit icon to change editable fields. If you press Cancel with unsaved changes, a confirmation popup asks whether to discard them.

SECTION

# 9 About & legal

The About & Legal screen consolidates platform information into four sections.

## 9.1 Software version

Platform version, build date and release type.

## 9.2 Distributor

PAUL HARTMANN AG, Paul-Hartmann-Straße 12, 89522 Heidenheim, Germany. info@hartmann.info · +49 7321 360. A Need more help? button redirects to the FAQ tab.

## 9.3 Manufacturer — Sleepiz

Sleepiz AG, Hornbachstrasse 23, 8008 Zurich, Switzerland. info@sleepiz.com · +41 44 586 08 88. Responsible for the hardware unit (accessory to a medical device under Article 2(2) of EU MDR 2017/745, class IIa) using radar technology to allow contactless monitoring of breathing patterns, respiration rate and heart rate. The hardware unit is intended to be used with the Sleepiz One+ Cloud Software analysing signals. The software is considered a Class IIa medical device.

## 9.4 Manufacturer — ACTIMI

ACTIMI GmbH, Albert-Schäffle Str. 119, 70186 Stuttgart, Germany. support@actimi.com · +49 711 20944000.

**Actimi Dashboard (Frontend)**
Non-medical device. Intended solely for the visualisation of health data and notifications. Does not perform medical calculations, diagnoses or risk assessments.

**Actimi Signals (Backend)**
Medical Device Class IIa (MDR). UDI-DI: 42700031203-API-XG. Generation of notifications of vital parameters based on professional societies or patient-specific adjustments.

© 2026 PAUL HARTMANN AG

**WARNING**

**Safety reminder**

Actimi Signals and the Actimi Dashboard are not intended for monitoring in emergency situations. Real-time delivery of alerts cannot be guaranteed. In case of acute, life-threatening symptoms, emergency services must be contacted immediately.

© 2026 PAUL HARTMANN AG