

Titration report

LabX

Method

Method ID	CDC_GranTED	Release state	Released
Name	EQP	Modified by	PredefinedUser
Modified on	2/3/2026 2:15:08 PM		

Summary

Samples


Sample ID	Name	Result	State
1	0.1 M TRIS - 5 mL in 60 mL H2O	Sample size	5 mL
		Consumption R1	5.158 mL
		Concentration R2	0.103 mol/L
			OK
			OK

Main Results

Sample ID1	Sample ID2	Result Title	Name	Result	State
0.1 M TRIS - 5 mL in 60 mL H2O		Consumption	R1	5.158 mL	OK
0.1 M TRIS - 5 mL in 60 mL H2O		Concentration	R2	0.103 mol/L	OK

Titration (EQP) [1] Scope 1/1, Sample 1/1

E - V & dE/dV - V Curve Scope 1/1, Sample 1/1

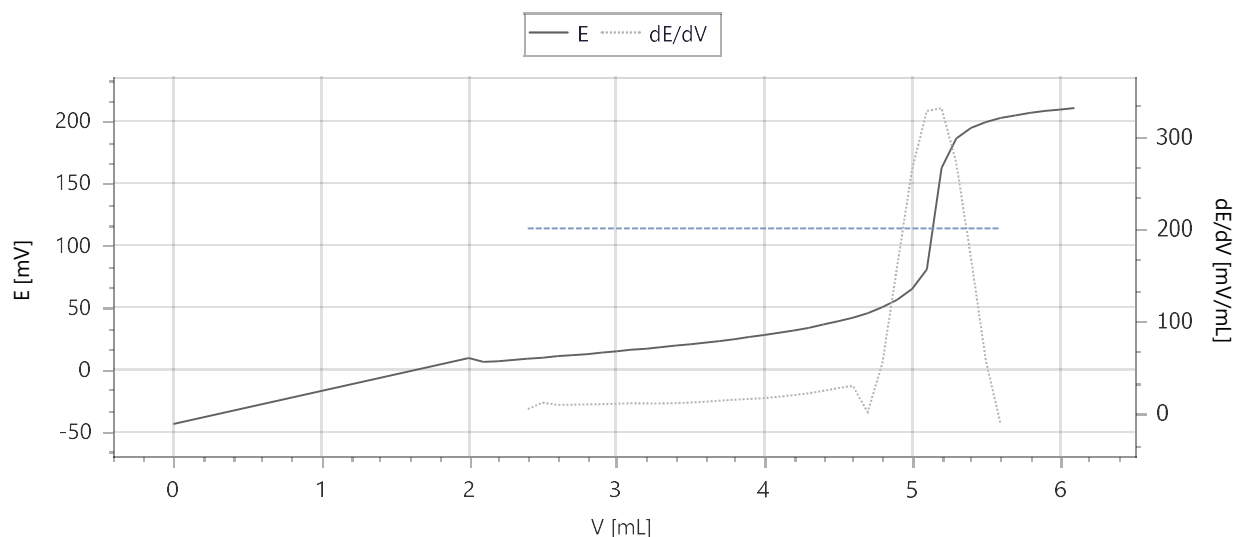

Measured Values Scope 1/1, Sample 1/1

Time [s]	V [mL]	Meas. value [mV]	dV [mL]	Temp. [°C]	dE [mV]	dE/dV [mV/mL]	EQP
0	0.0000	-43.8		25.0			
7	2.0000	9.5	2.0000	25.0	53.3		
40	2.1000	6.2	0.1000	25.0	-3.3		
44	2.2000	6.9	0.1000	25.0	0.7		

Titration report

LabX

47	2.3000	7.9	0.1000	25.0	1.0	
51	2.4000	8.8	0.1000	25.0	0.9	5.26
55	2.5000	9.7	0.1000	25.0	0.9	12.06
58	2.6000	10.9	0.1000	25.0	1.2	9.70
61	2.7000	11.7	0.1000	25.0	0.8	9.98
64	2.8000	12.6	0.1000	25.0	0.9	10.31
67	2.9000	13.8	0.1000	25.0	1.2	10.43
71	3.0000	14.8	0.1000	25.0	1.0	11.01
74	3.1000	16.1	0.1000	25.0	1.3	11.47
77	3.2000	17.0	0.1000	25.0	0.9	11.37
80	3.3000	18.2	0.1000	25.0	1.2	11.34
84	3.4000	19.6	0.1000	25.0	1.4	11.66
88	3.5000	20.5	0.1000	25.0	0.9	12.30
91	3.6000	21.8	0.1000	25.0	1.3	13.25
94	3.7000	23.2	0.1000	25.0	1.4	14.34
97	3.8000	24.7	0.1000	25.0	1.5	15.38
100	3.9000	26.4	0.1000	25.0	1.7	16.22
104	4.0000	28.0	0.1000	25.0	1.6	17.01
107	4.1000	29.9	0.1000	25.0	1.9	18.60
111	4.2000	31.5	0.1000	25.0	1.6	20.29
114	4.3000	33.7	0.1000	25.0	2.2	22.16
118	4.4000	36.4	0.1000	25.0	2.7	24.86
123	4.5000	39.1	0.1000	25.0	2.7	27.78
127	4.6000	41.9	0.1000	25.0	2.8	30.24
131	4.7000	45.6	0.1000	25.0	3.7	1.91
136	4.8000	50.4	0.1000	25.0	4.8	55.10
140	4.9000	56.3	0.1000	25.0	5.9	159.43
143	5.0000	65.1	0.1000	25.0	8.8	263.06
152	5.1000	80.9	0.1000	25.0	15.8	326.75
	5.158116	128.4				331.77
164	5.2000	162.6	0.1000	25.0	81.7	329.76
169	5.3000	186.4	0.1000	25.0	23.8	270.61
172	5.4000	194.9	0.1000	25.0	8.5	167.68
176	5.5000	199.7	0.1000	25.0	4.8	57.41
179	5.6000	202.8	0.1000	25.0	3.1	-10.94
182	5.7000	205.1	0.1000	25.0	2.3	
185	5.8000	207.1	0.1000	25.0	2.0	
188	5.9000	208.5	0.1000	25.0	1.4	
191	6.0000	209.7	0.1000	25.0	1.2	
194	6.1000	210.8	0.1000	25.0	1.1	

EQP

Sample Series

Name	Internal ID
Label 1	Label 2
Label 3	Label 4
Label 5	Label 6

Comment

Sample

Titration report

LabX

Sample ID 1

Sample ID 2

Sample ID 3

Sample Parameters

Type	Name	Qualified name	Value
------	------	----------------	-------

Used Instruments

Name	T9_MSG_SA_002	Serial number	B551866924
------	---------------	---------------	------------

Responsible User

Time	Login name	Full name
03.02.2026 14:16:46	PredefinedUser	Administrator