

Titration report

LabX

Method

Method ID	CDC_GranTED-DYN	Release state	Released
Name	Titr TRIS with HCl - Gran Verification	Modified by	PredefinedUser
Modified on	2/5/2026 7:31:59 AM		

Summary

Samples


Sample ID	Name	Result	State
1	0.1 M TRIS - 5 mL in 60 mL H2O	Sample size	5 mL
		Consumption R1	5.013993 mL
		Concentration R2	0.10028 mol/L

Main Results

Sample ID1	Sample ID2	Result Title	Name	Result	State
0.1 M TRIS - 5 mL in 60 mL H2O		Consumption	R1	5.013993 mL	OK
0.1 M TRIS - 5 mL in 60 mL H2O		Concentration	R2	0.10028 mol/L	OK

Titration (EQP) [1] Scope 1/1, Sample 1/1

E - V & dE/dV - V Curve Scope 1/1, Sample 1/1

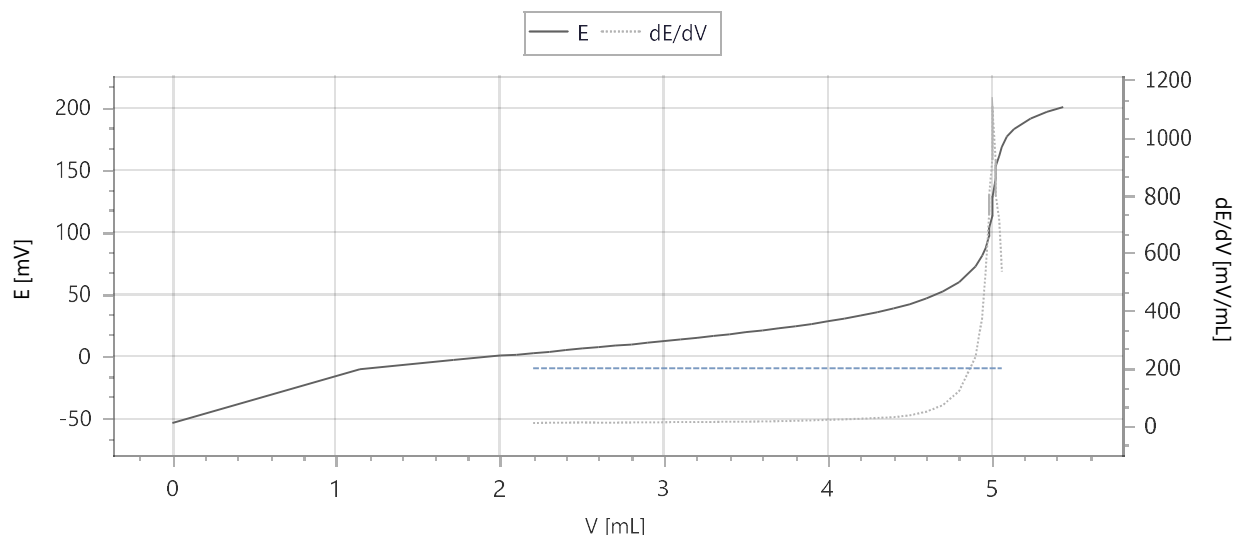

Measured Values Scope 1/1, Sample 1/1

Time [s]	V [mL]	Meas. value [mV]	dV [mL]	Temp. [°C]	dE [mV]	dE/dV [mV/mL]	EQP
0	0.0000	-53.9		25.0			
11	1.1430	-10.8	1.1430	25.0	43.1		
17	1.7145	-3.2	0.5715	25.0	7.6		

Titration report

LabX

22	2.0000	0.3	0.2855	25.0	3.5	
56	2.1000	0.9	0.1000	25.0	0.6	
59	2.2000	2.1	0.1000	25.0	1.2	10.39
63	2.3000	3.3	0.1000	25.0	1.2	11.31
66	2.4000	4.6	0.1000	25.0	1.3	11.73
69	2.5000	5.9	0.1000	25.0	1.3	12.24
73	2.6000	7.0	0.1000	25.0	1.1	11.80
76	2.7000	8.2	0.1000	25.0	1.2	11.81
80	2.8000	9.1	0.1000	25.0	0.9	12.14
84	2.9000	10.7	0.1000	25.0	1.6	12.60
86	3.0000	11.9	0.1000	25.0	1.2	13.07
90	3.1000	13.2	0.1000	25.0	1.3	13.57
94	3.2000	14.6	0.1000	25.0	1.4	13.86
97	3.3000	15.9	0.1000	25.0	1.3	14.01
101	3.4000	17.4	0.1000	25.0	1.5	14.82
104	3.5000	19.0	0.1000	25.0	1.6	15.05
108	3.6000	20.4	0.1000	25.0	1.4	15.70
112	3.7000	22.1	0.1000	25.0	1.7	16.67
116	3.8000	23.8	0.1000	25.0	1.7	17.99
120	3.9000	25.5	0.1000	25.0	1.7	19.65
123	4.0000	27.8	0.1000	25.0	2.3	21.46
127	4.1000	30.0	0.1000	25.0	2.2	22.96
132	4.2000	32.5	0.1000	25.0	2.5	25.18
136	4.3000	35.1	0.1000	25.0	2.6	27.90
141	4.4000	38.1	0.1000	25.0	3.0	30.50
144	4.5000	41.6	0.1000	25.0	3.5	37.11
149	4.6000	46.2	0.1000	25.0	4.6	49.57
155	4.7000	51.7	0.1000	25.0	5.5	72.04
160	4.8000	59.2	0.1000	25.0	7.5	121.17
167	4.9000	71.8	0.1000	25.0	12.6	239.23
177	4.9405	80.5	0.0405	25.0	8.7	375.57
182	4.9620	86.7	0.0215	25.0	6.2	537.44
192	4.9830	96.9	0.0210	25.0	10.2	735.01
197	4.9930	103.1	0.0100	25.0	6.2	797.15
201	5.0030	112.8	0.0100	25.0	9.7	926.16
214	5.0130	127.4	0.0100	25.0	14.6	1104.32
	5.013993	128.9				1104.73
						EQP
222	5.0230	142.3	0.0100	25.0	14.9	918.69
225	5.0330	152.4	0.0100	25.0	10.1	801.61
228	5.0445	160.5	0.0115	25.0	8.1	714.33
232	5.0610	167.7	0.0165	25.0	7.2	534.88
235	5.0910	176.1	0.0300	25.0	8.4	
242	5.1350	182.1	0.0440	25.0	6.0	
250	5.2350	190.5	0.1000	25.0	8.4	
255	5.3350	196.1	0.1000	25.0	5.6	
259	5.4350	199.8	0.1000	25.0	3.7	

Sample Series

Name	Internal ID
Label 1	Label 2
Label 3	Label 4

Titration report

LabX

Label 5

Label 6

Comment

Sample

Sample ID 1

Sample ID 2

Sample ID 3

Sample Parameters

Type	Name	Qualified name	Value
------	------	----------------	-------

Used Instruments

Name	T9_MSG_SA_002	Serial number	B551866924
------	---------------	---------------	------------

Responsible User

Time	Login name	Full name
05.02.2026 07:32:29	PredefinedUser	Administrator