


26  
MISS. ASHWANI BORKAR  
21 Years/F


Date: 25-Jul-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL


Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:41:40  
Page:2/28  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

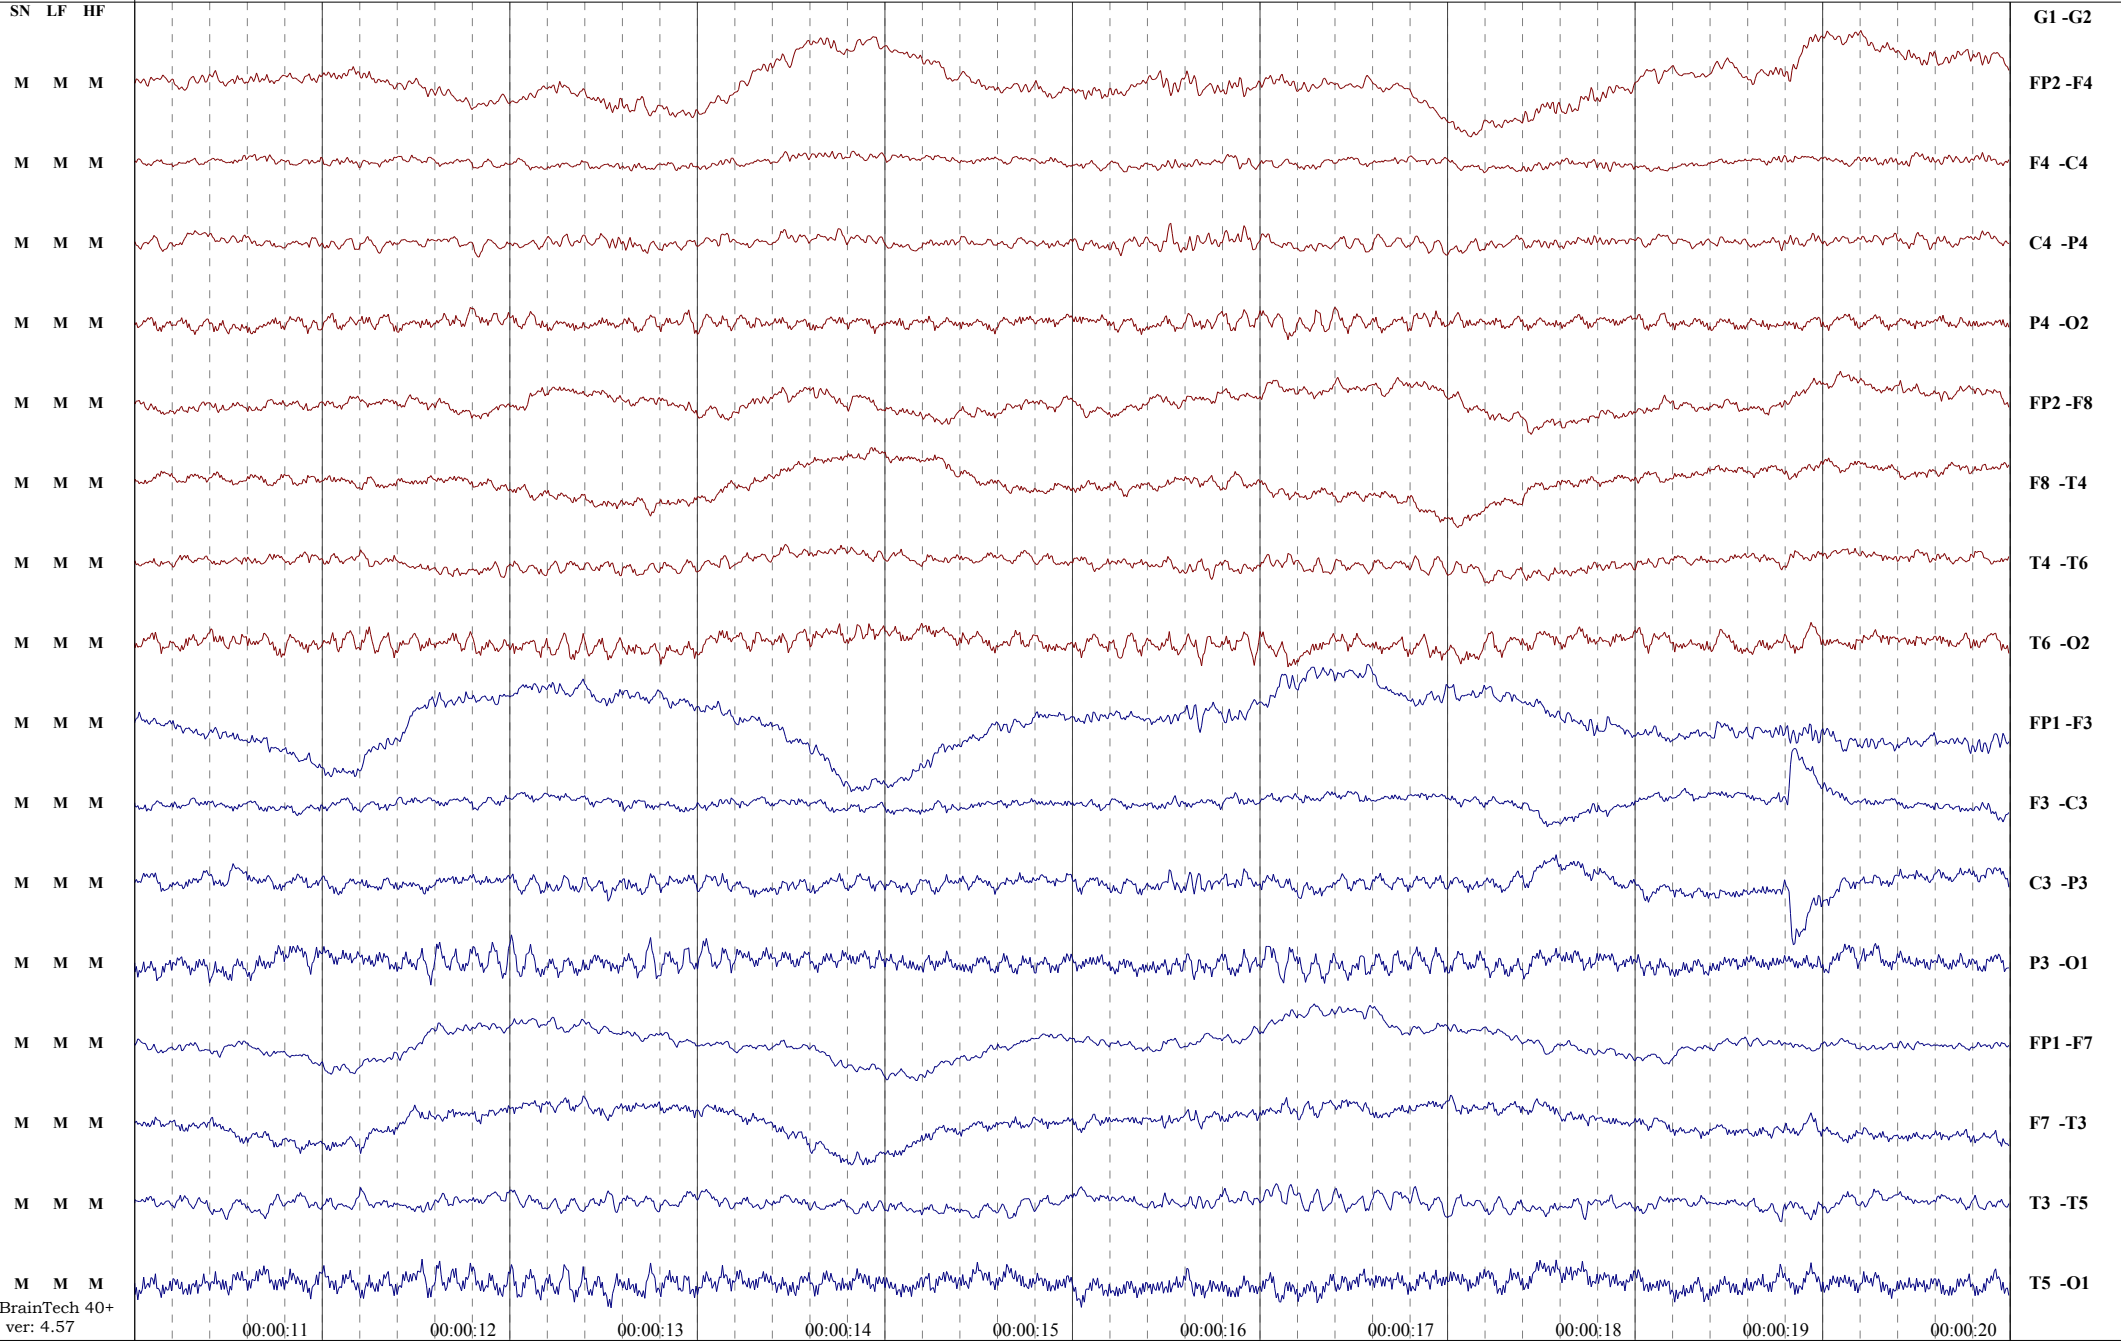

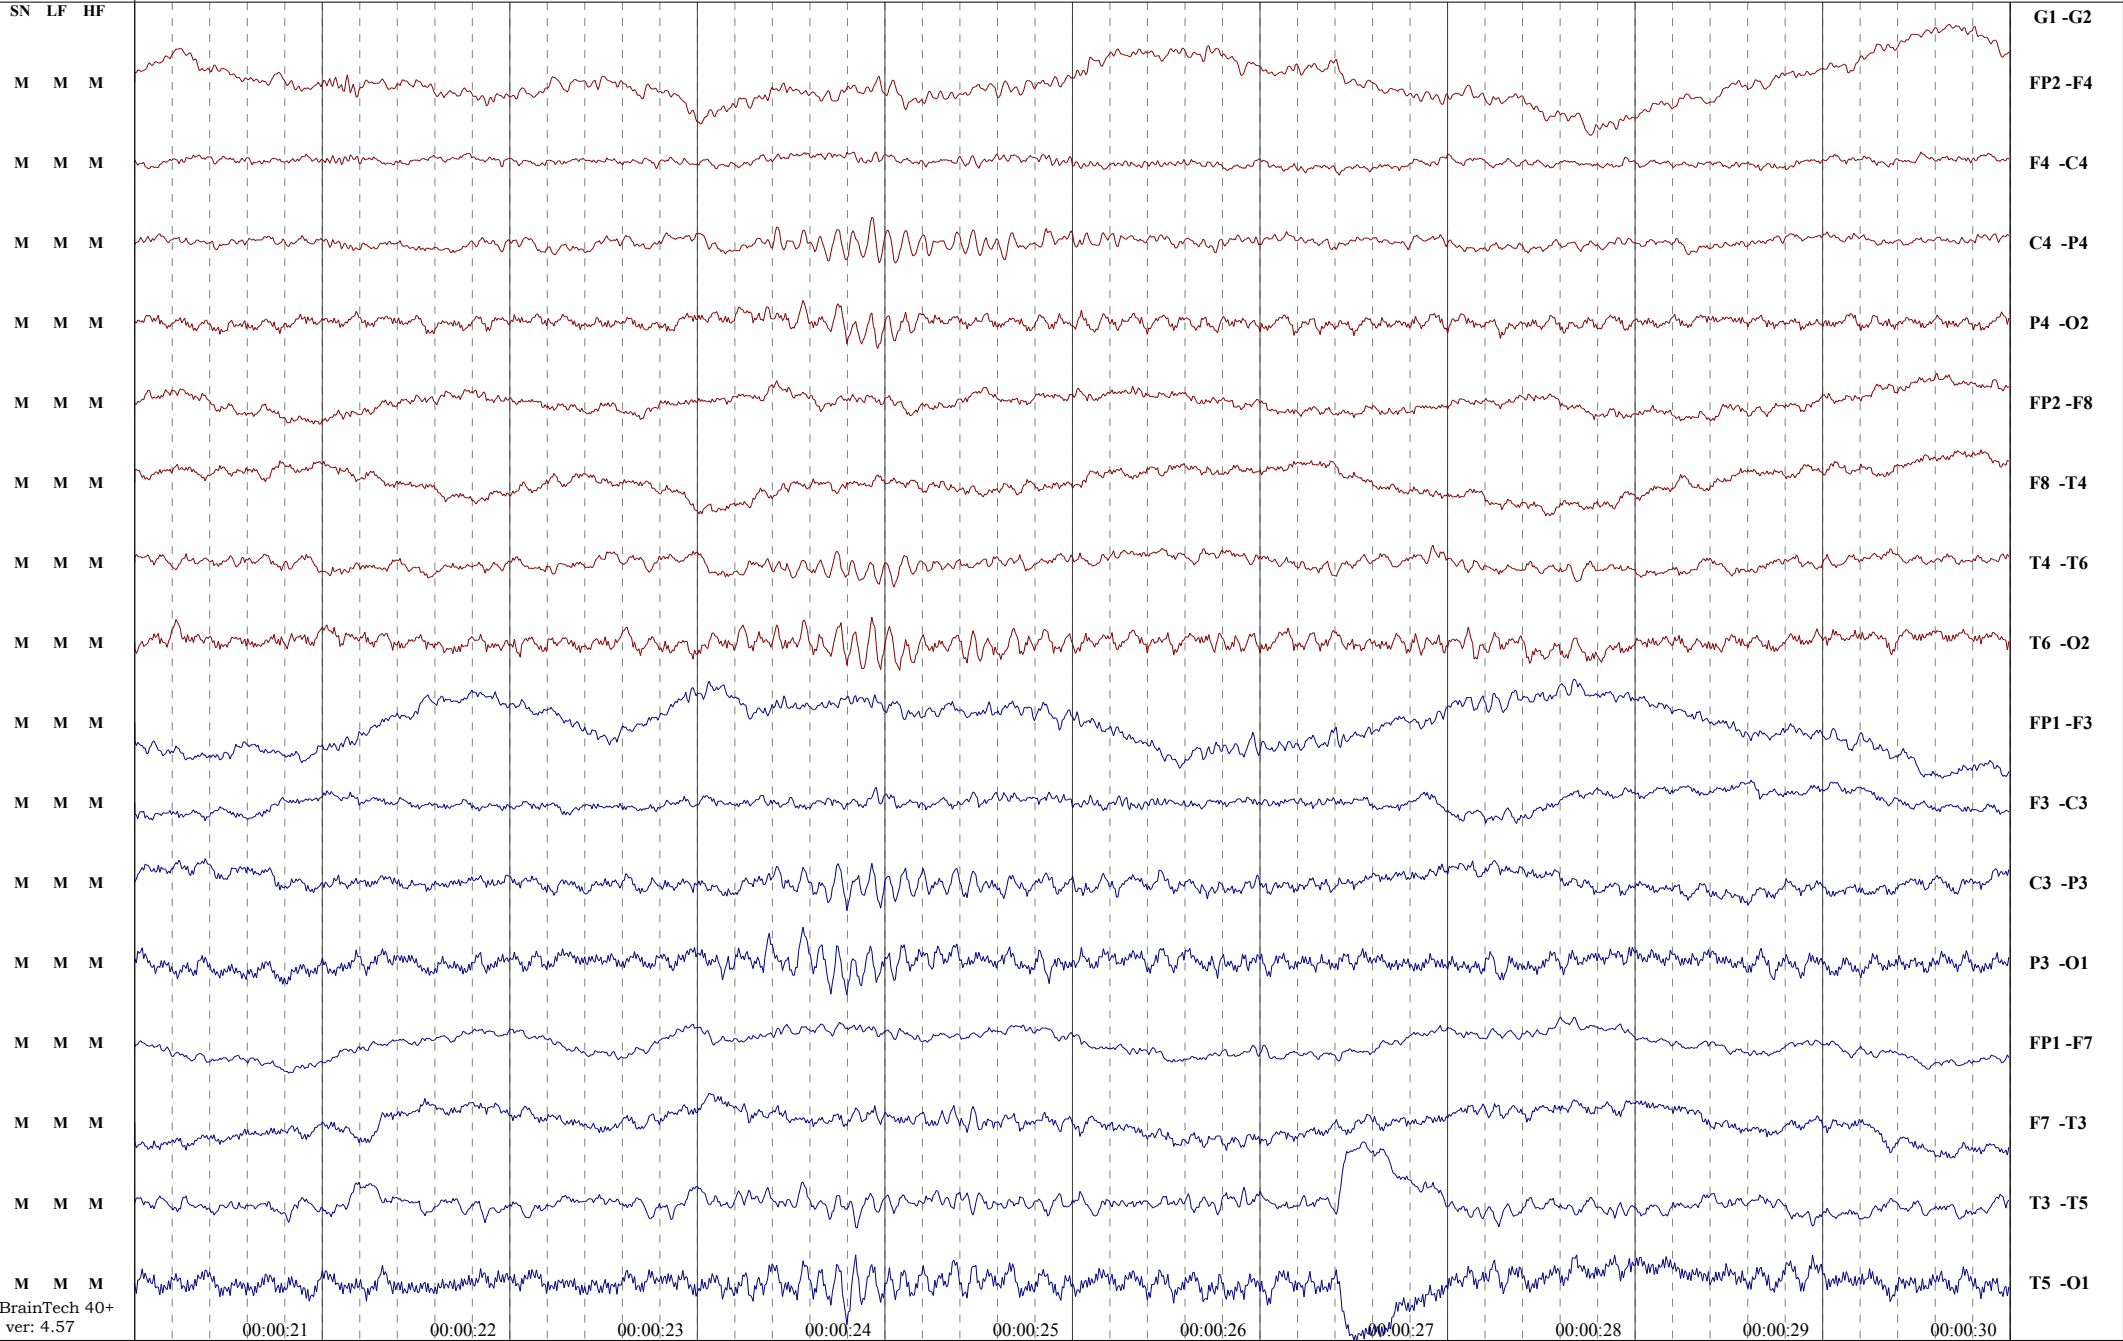

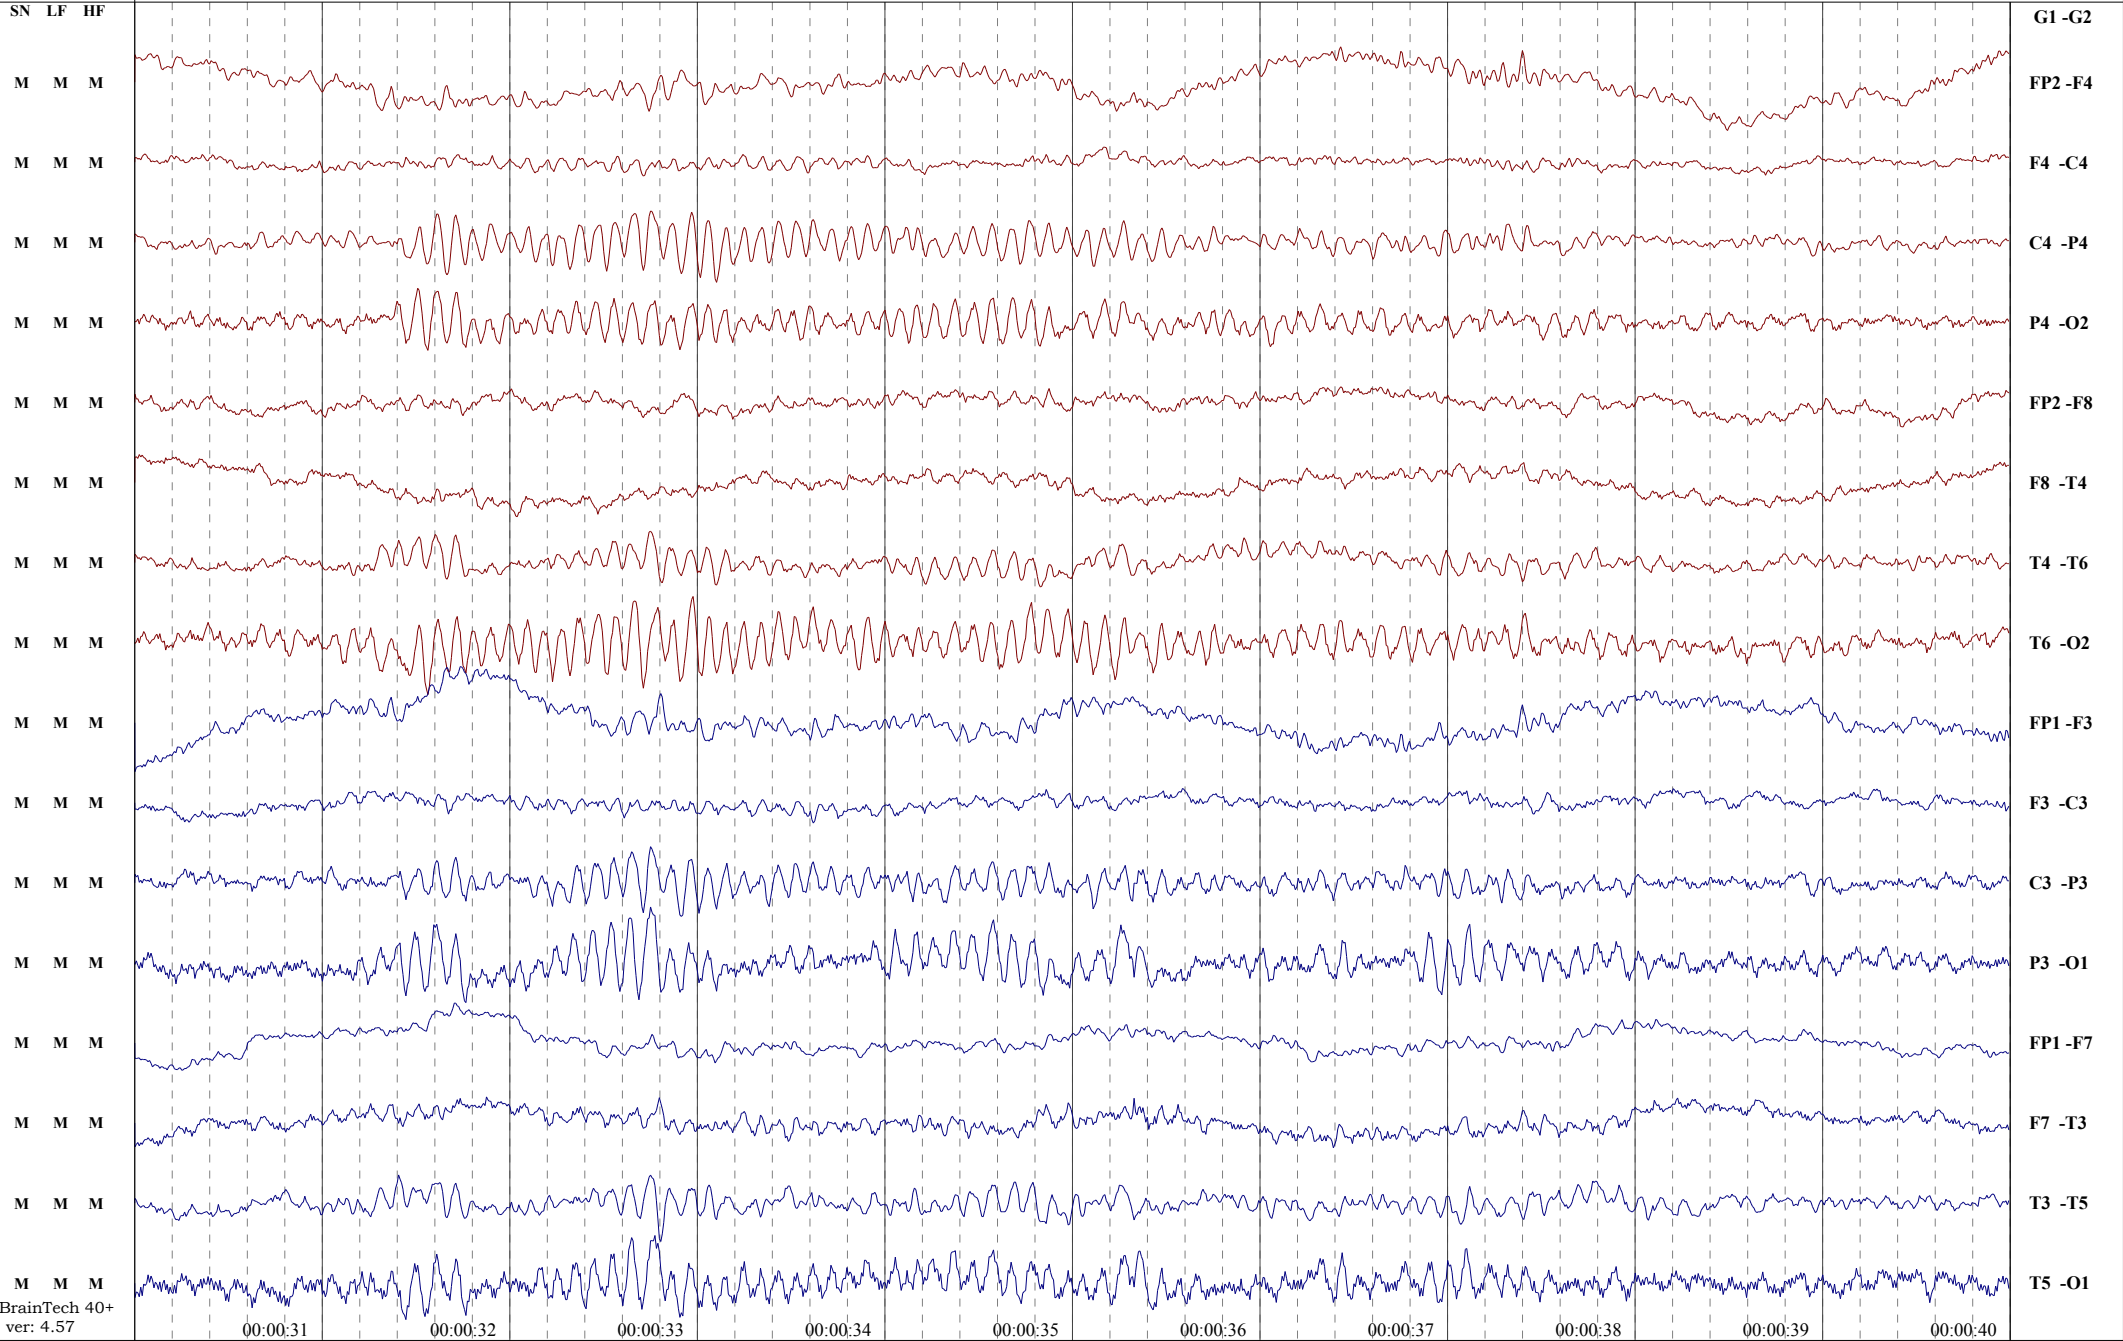






26  
MISS. ASHWANI BORKAR  
21 Years/F

Date: 25-Jul-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:42:20  
Page:6/28  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

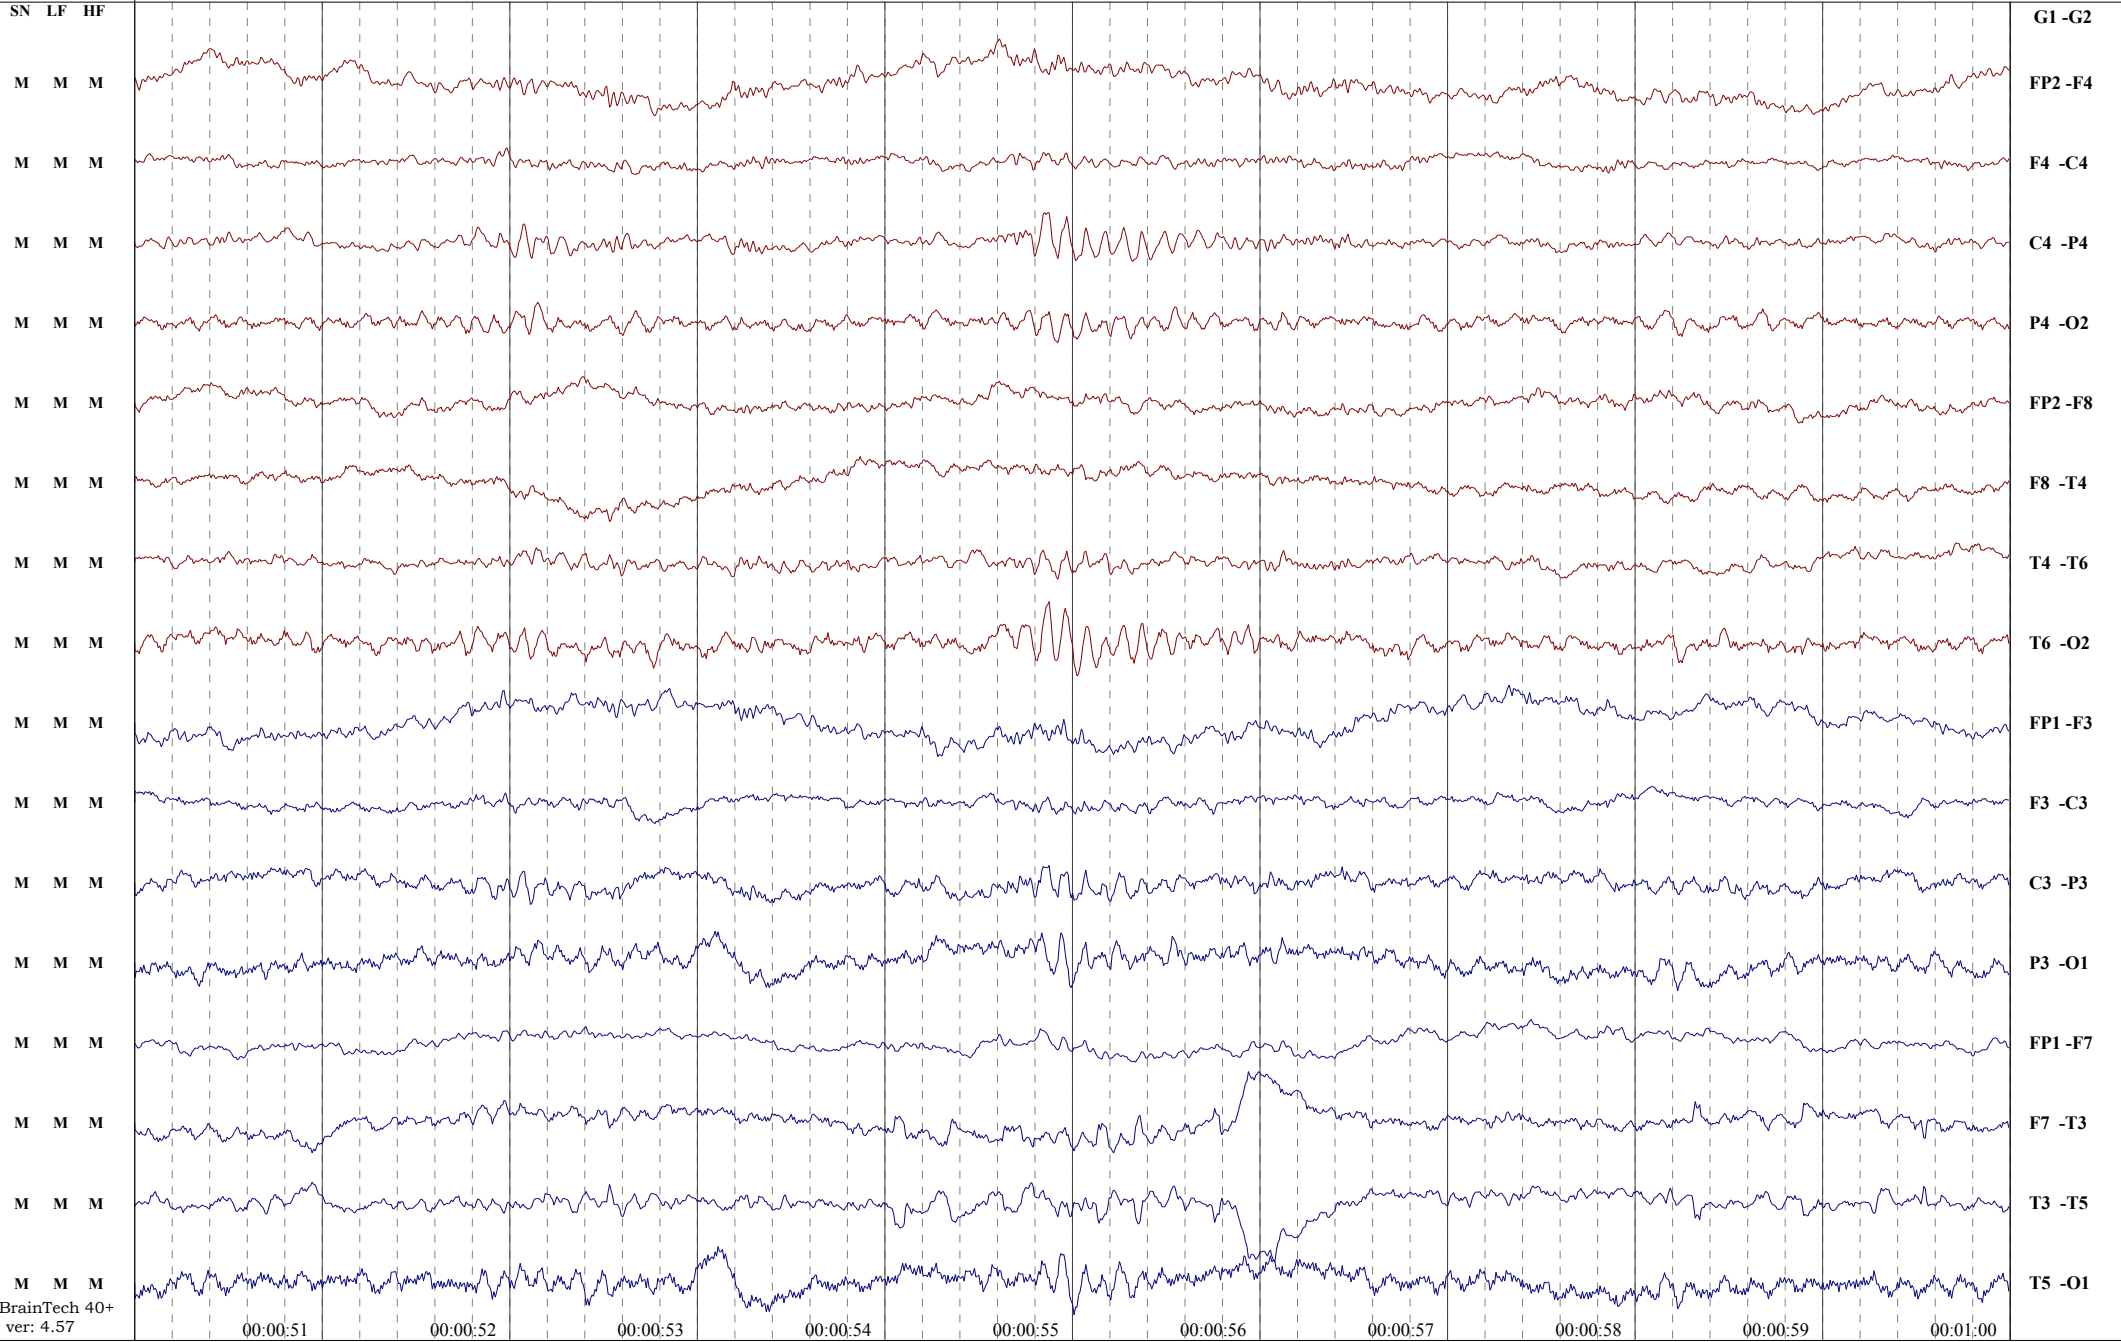


26  
MISS. ASHWANI BORKAR  
21 Years/F

Date: 25-Jul-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:42:30  
Page:7/28  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

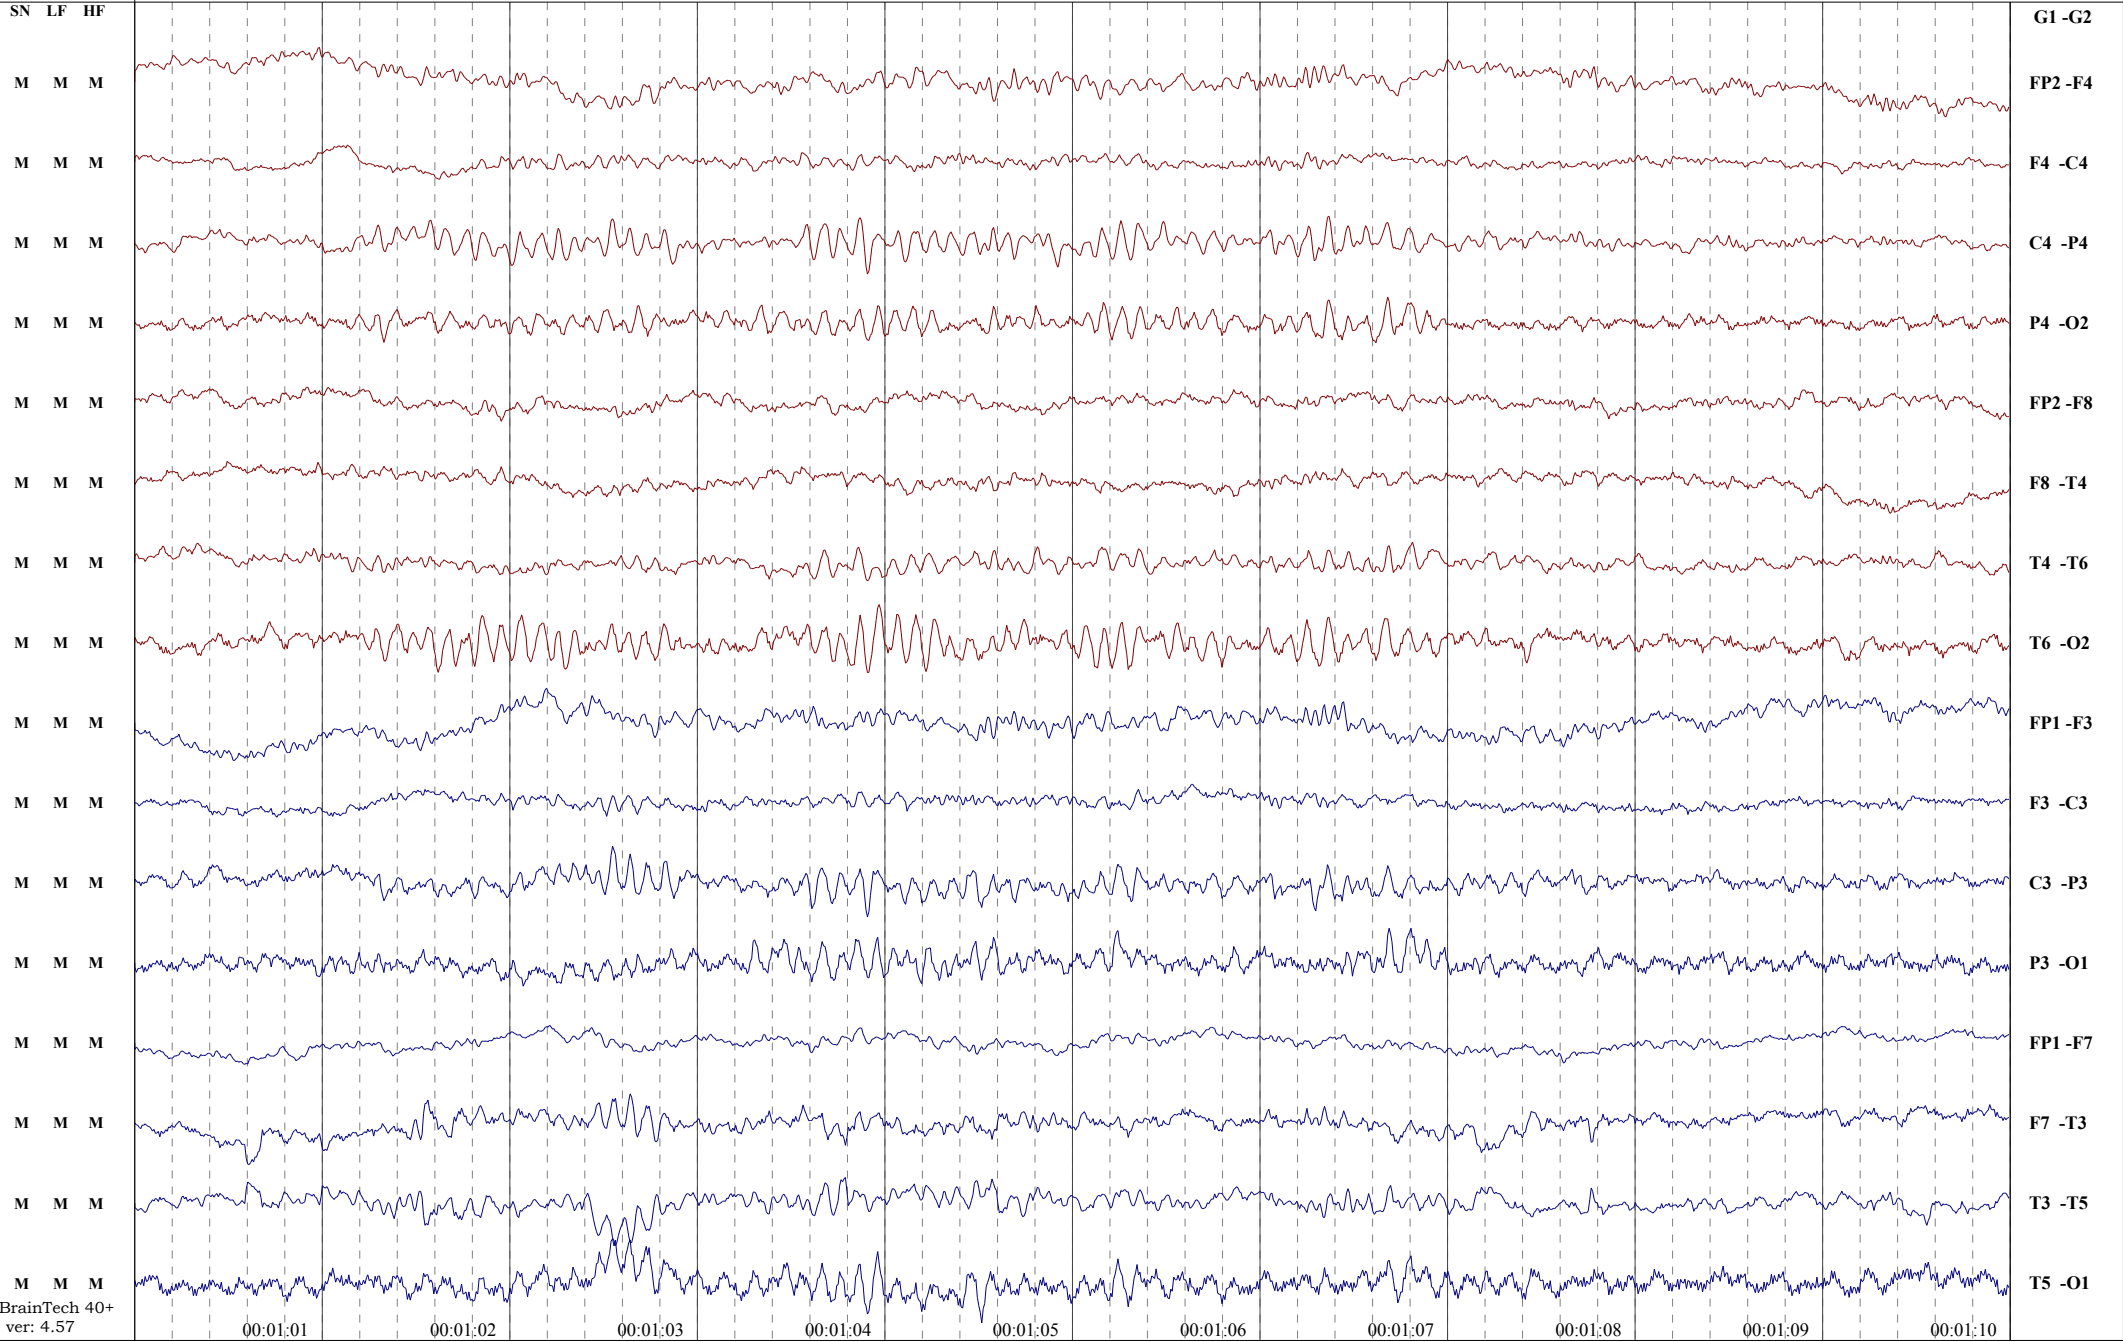


26  
MISS. ASHWANI BORKAR  
21 Years/F

Date: 25-Jul-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:42:40  
Page:8/28  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

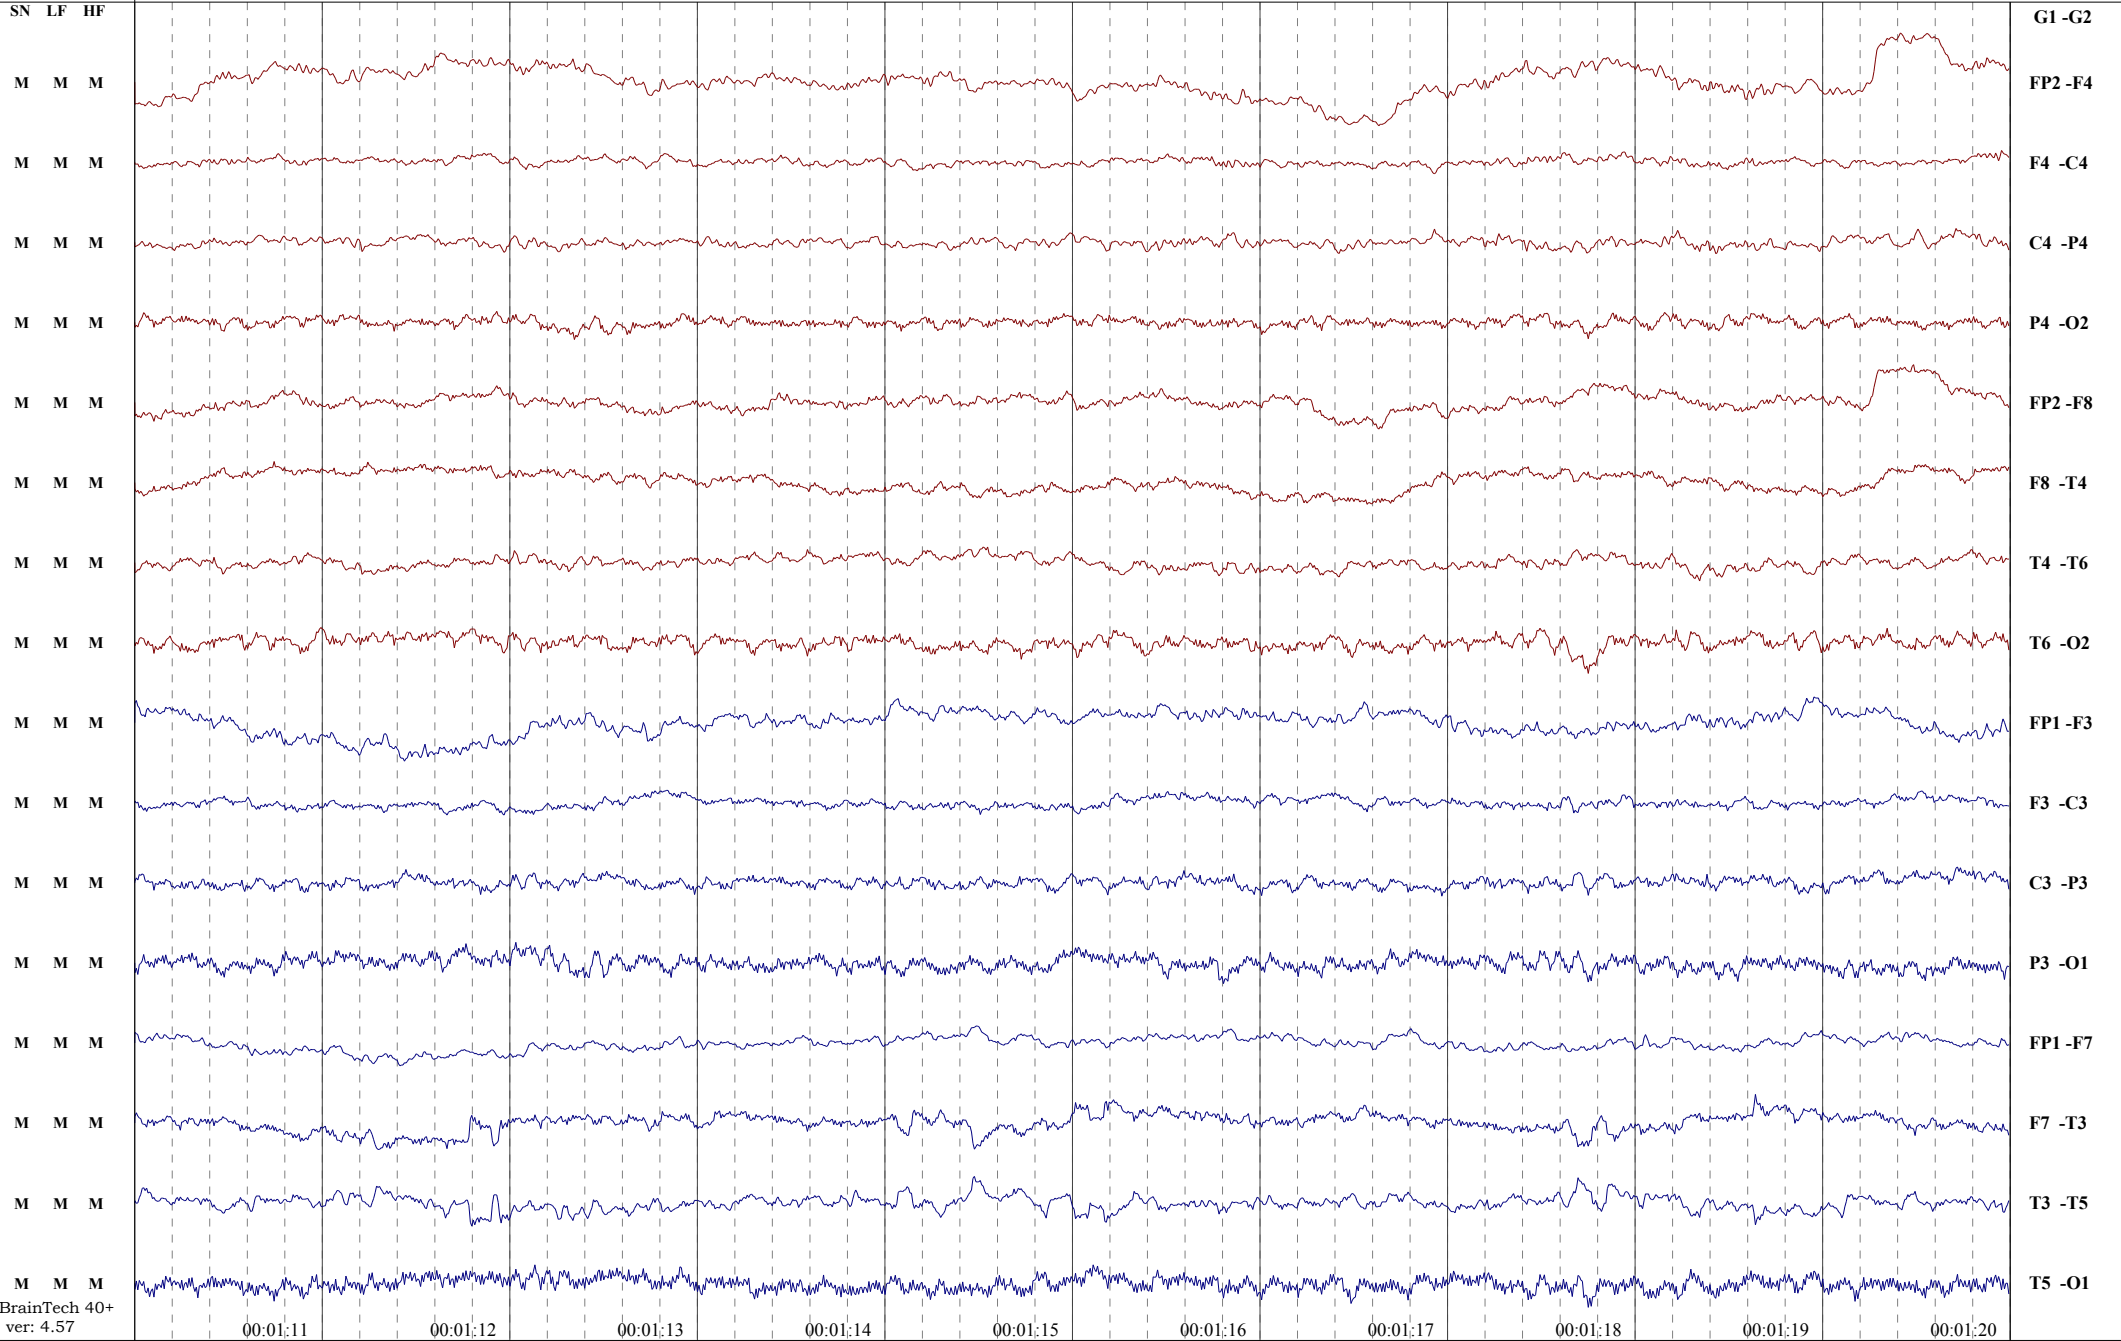




26  
MISS. ASHWANI BORKAR  
21 Years/F

Date: 25-Jul-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:42:50  
Page:9/28  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

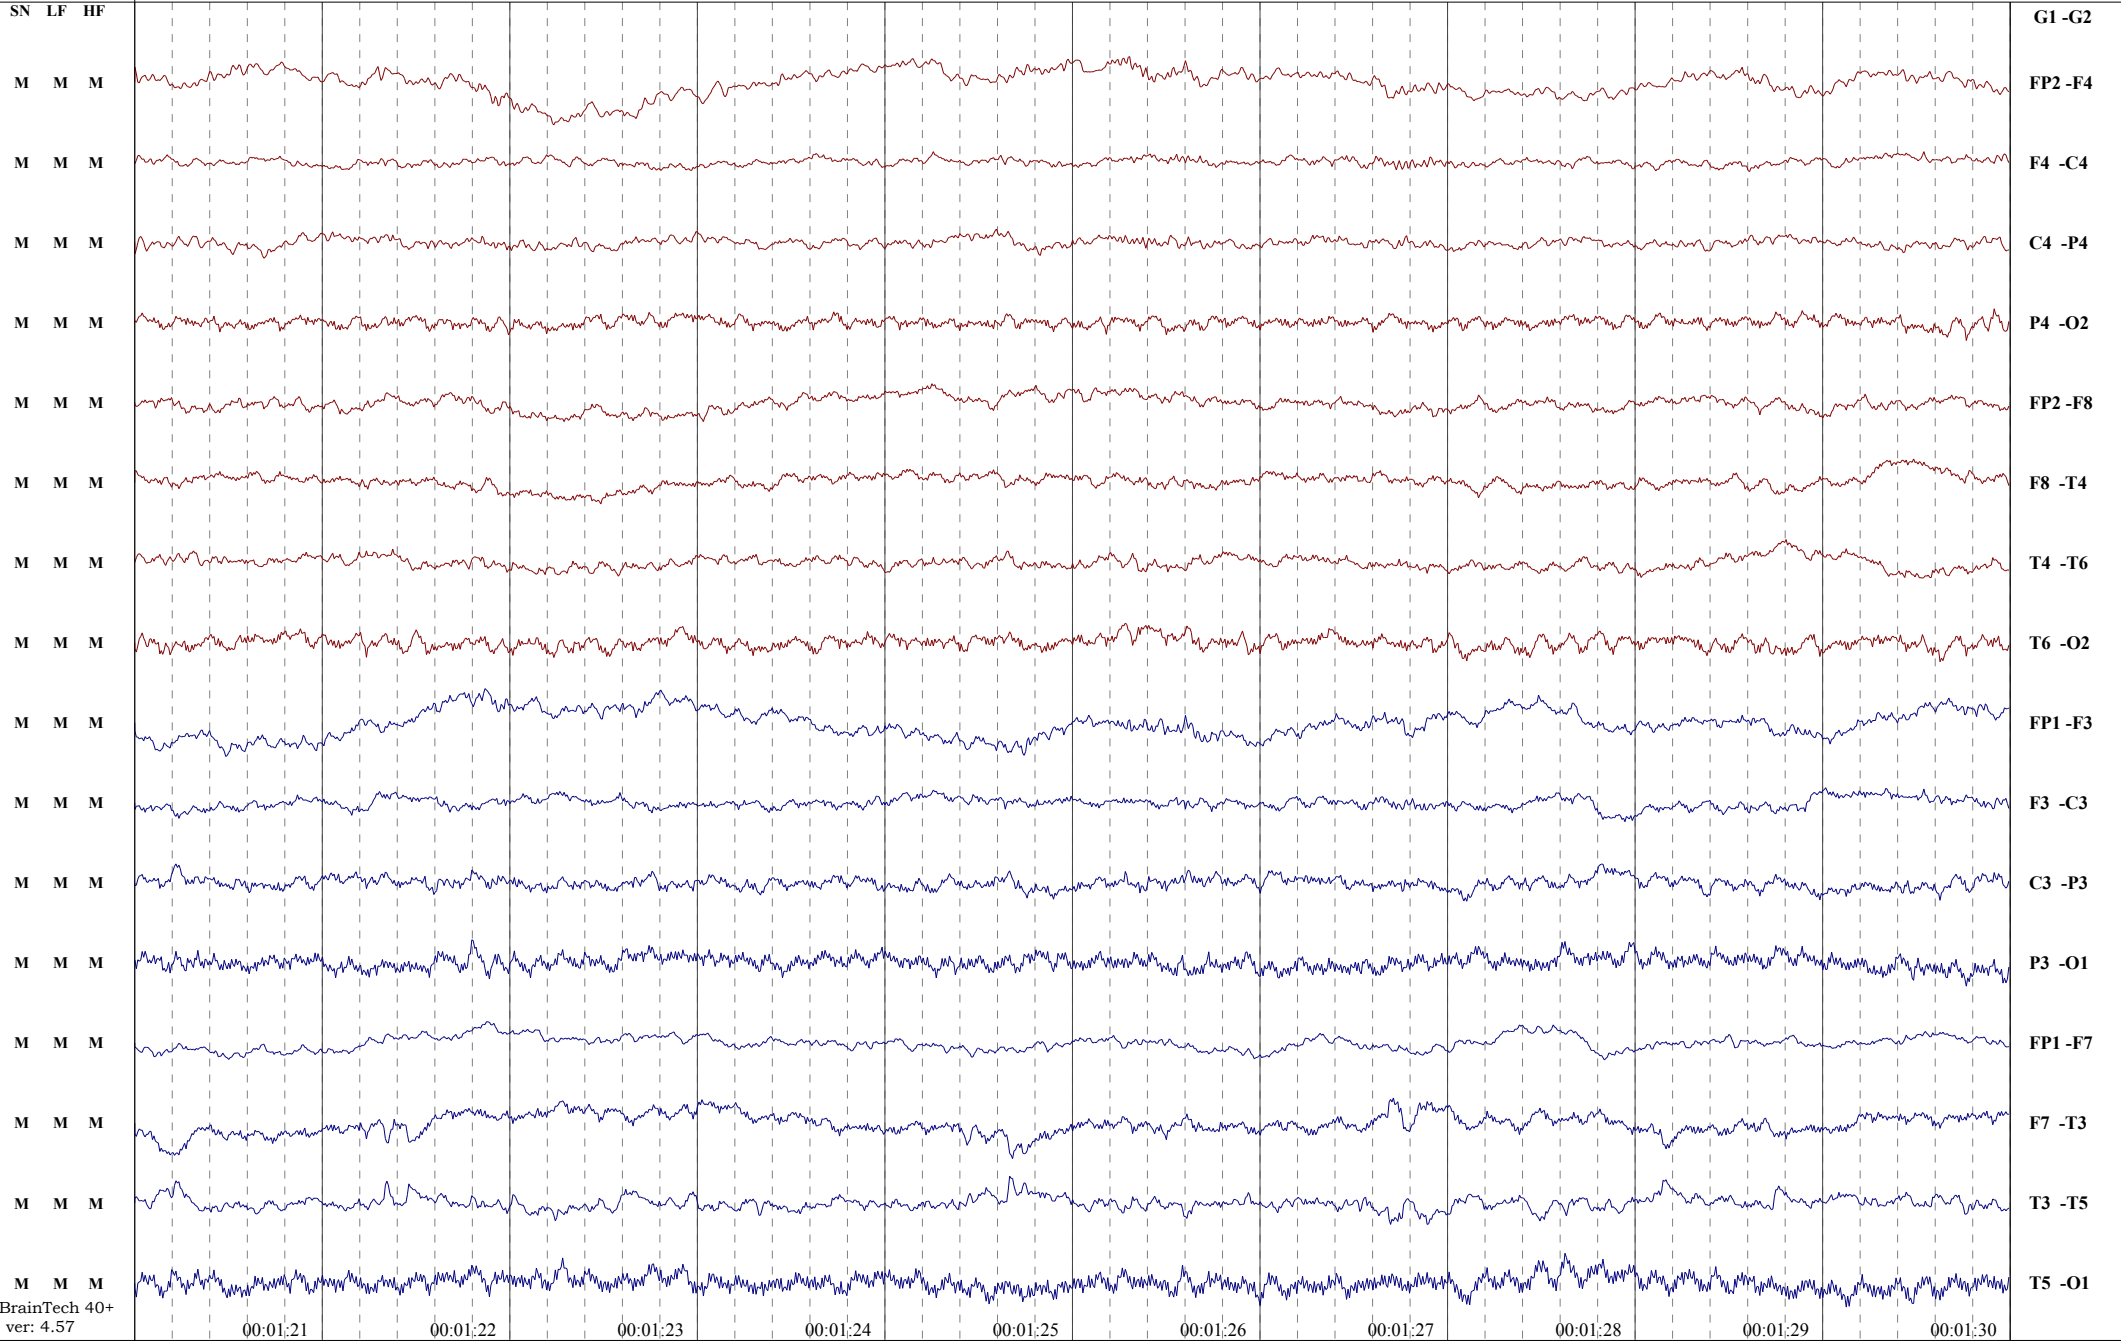




26  
MISS. ASHWANI BORKAR  
21 Years/F

Date: 25-Jul-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:43:10  
Page:11/28  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

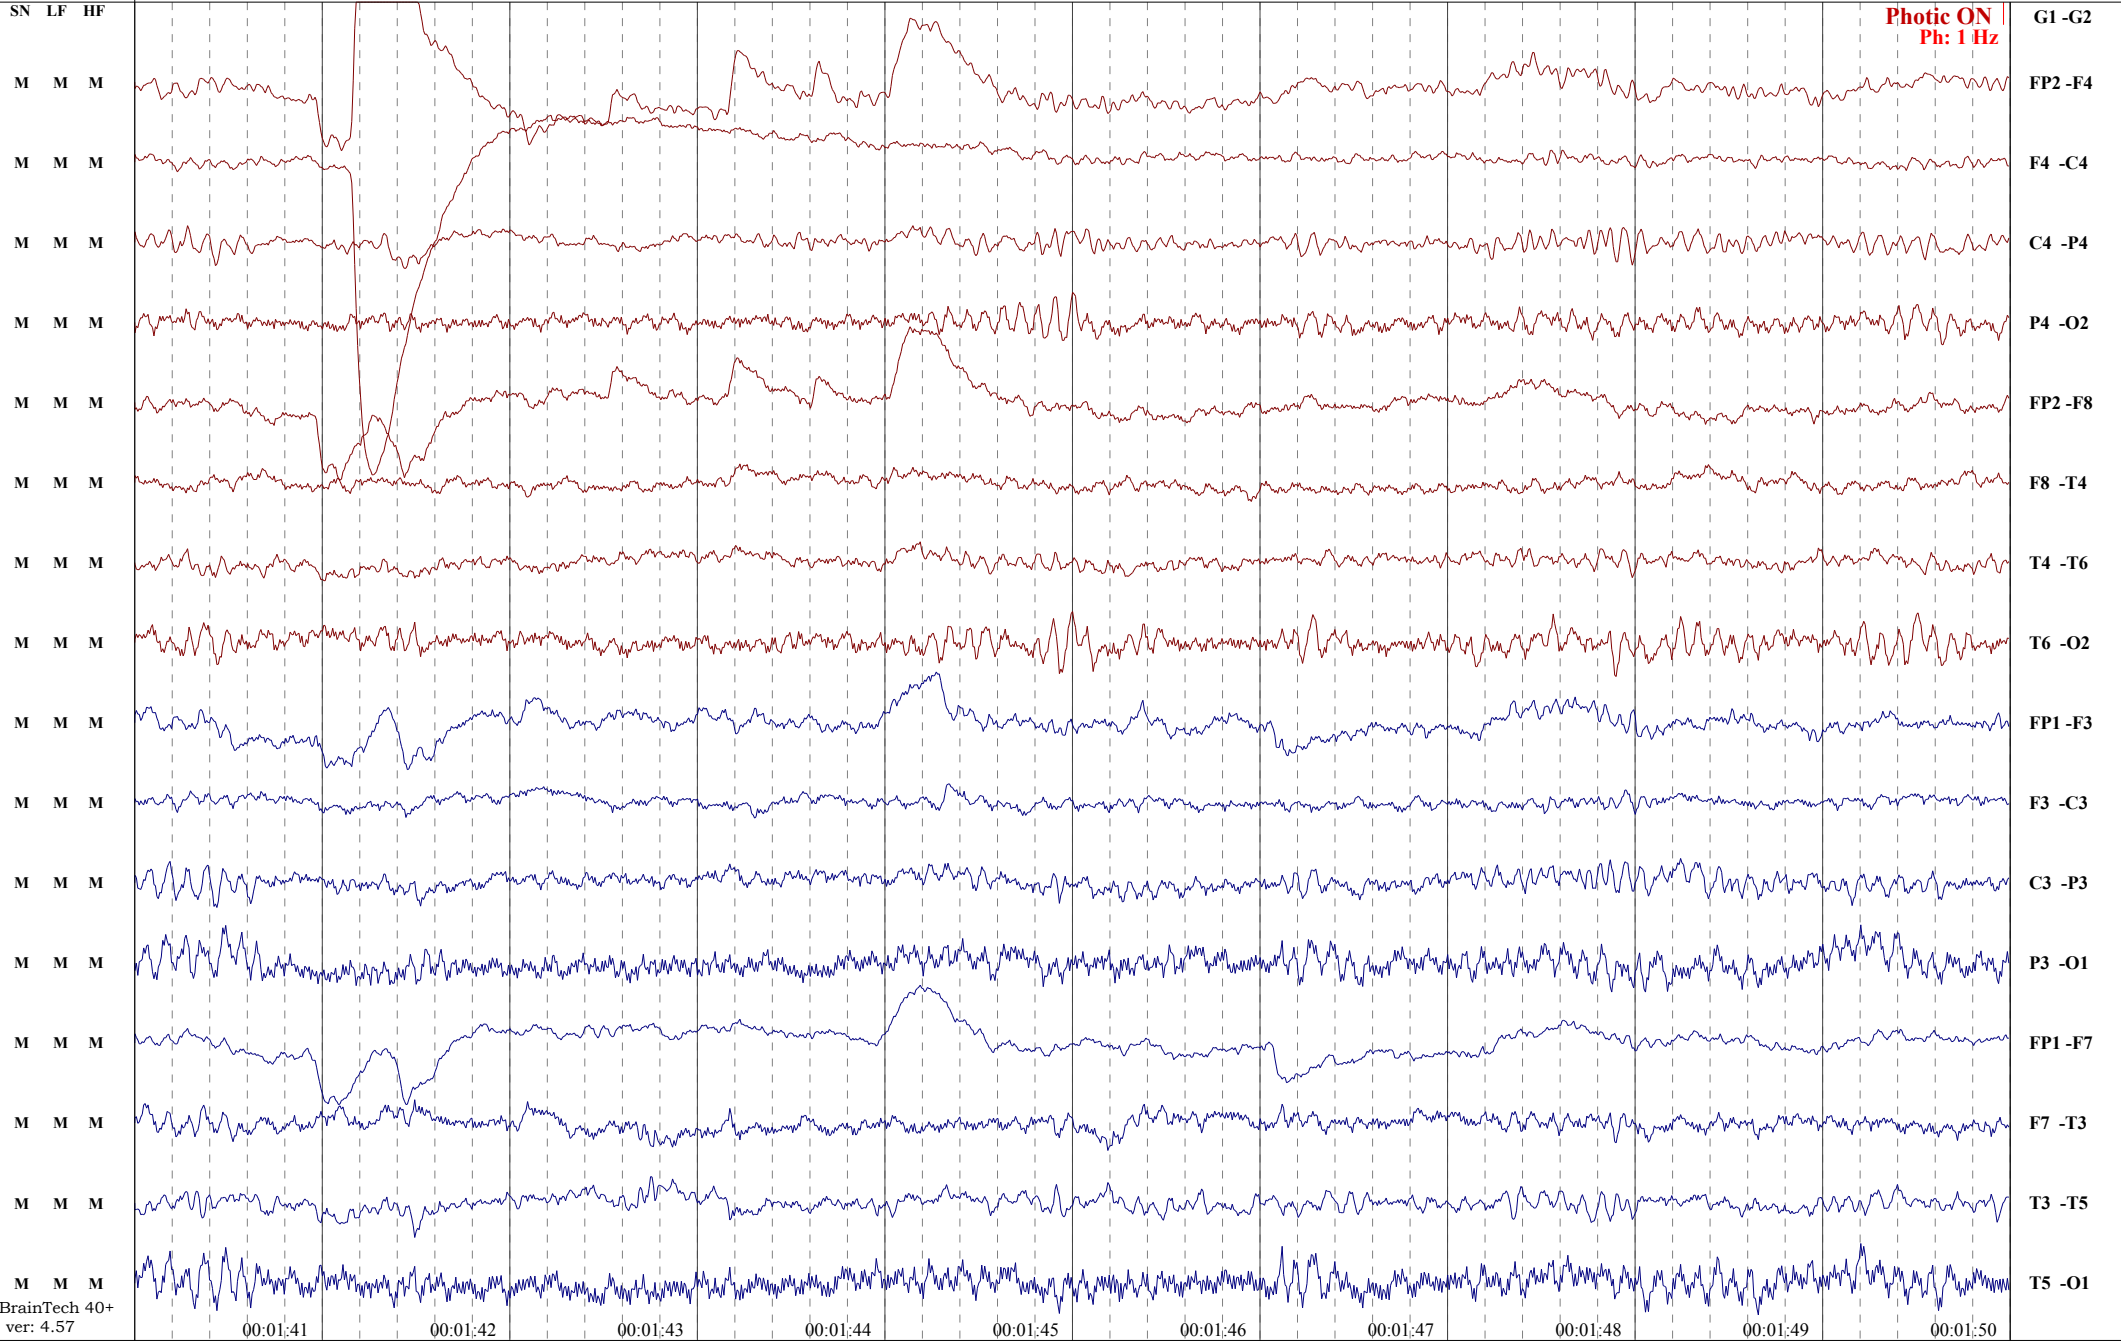


26  
MISS. ASHWANI BORKAR  
21 Years/F

Date: 25-Jul-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:43:20  
Page:12/28  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

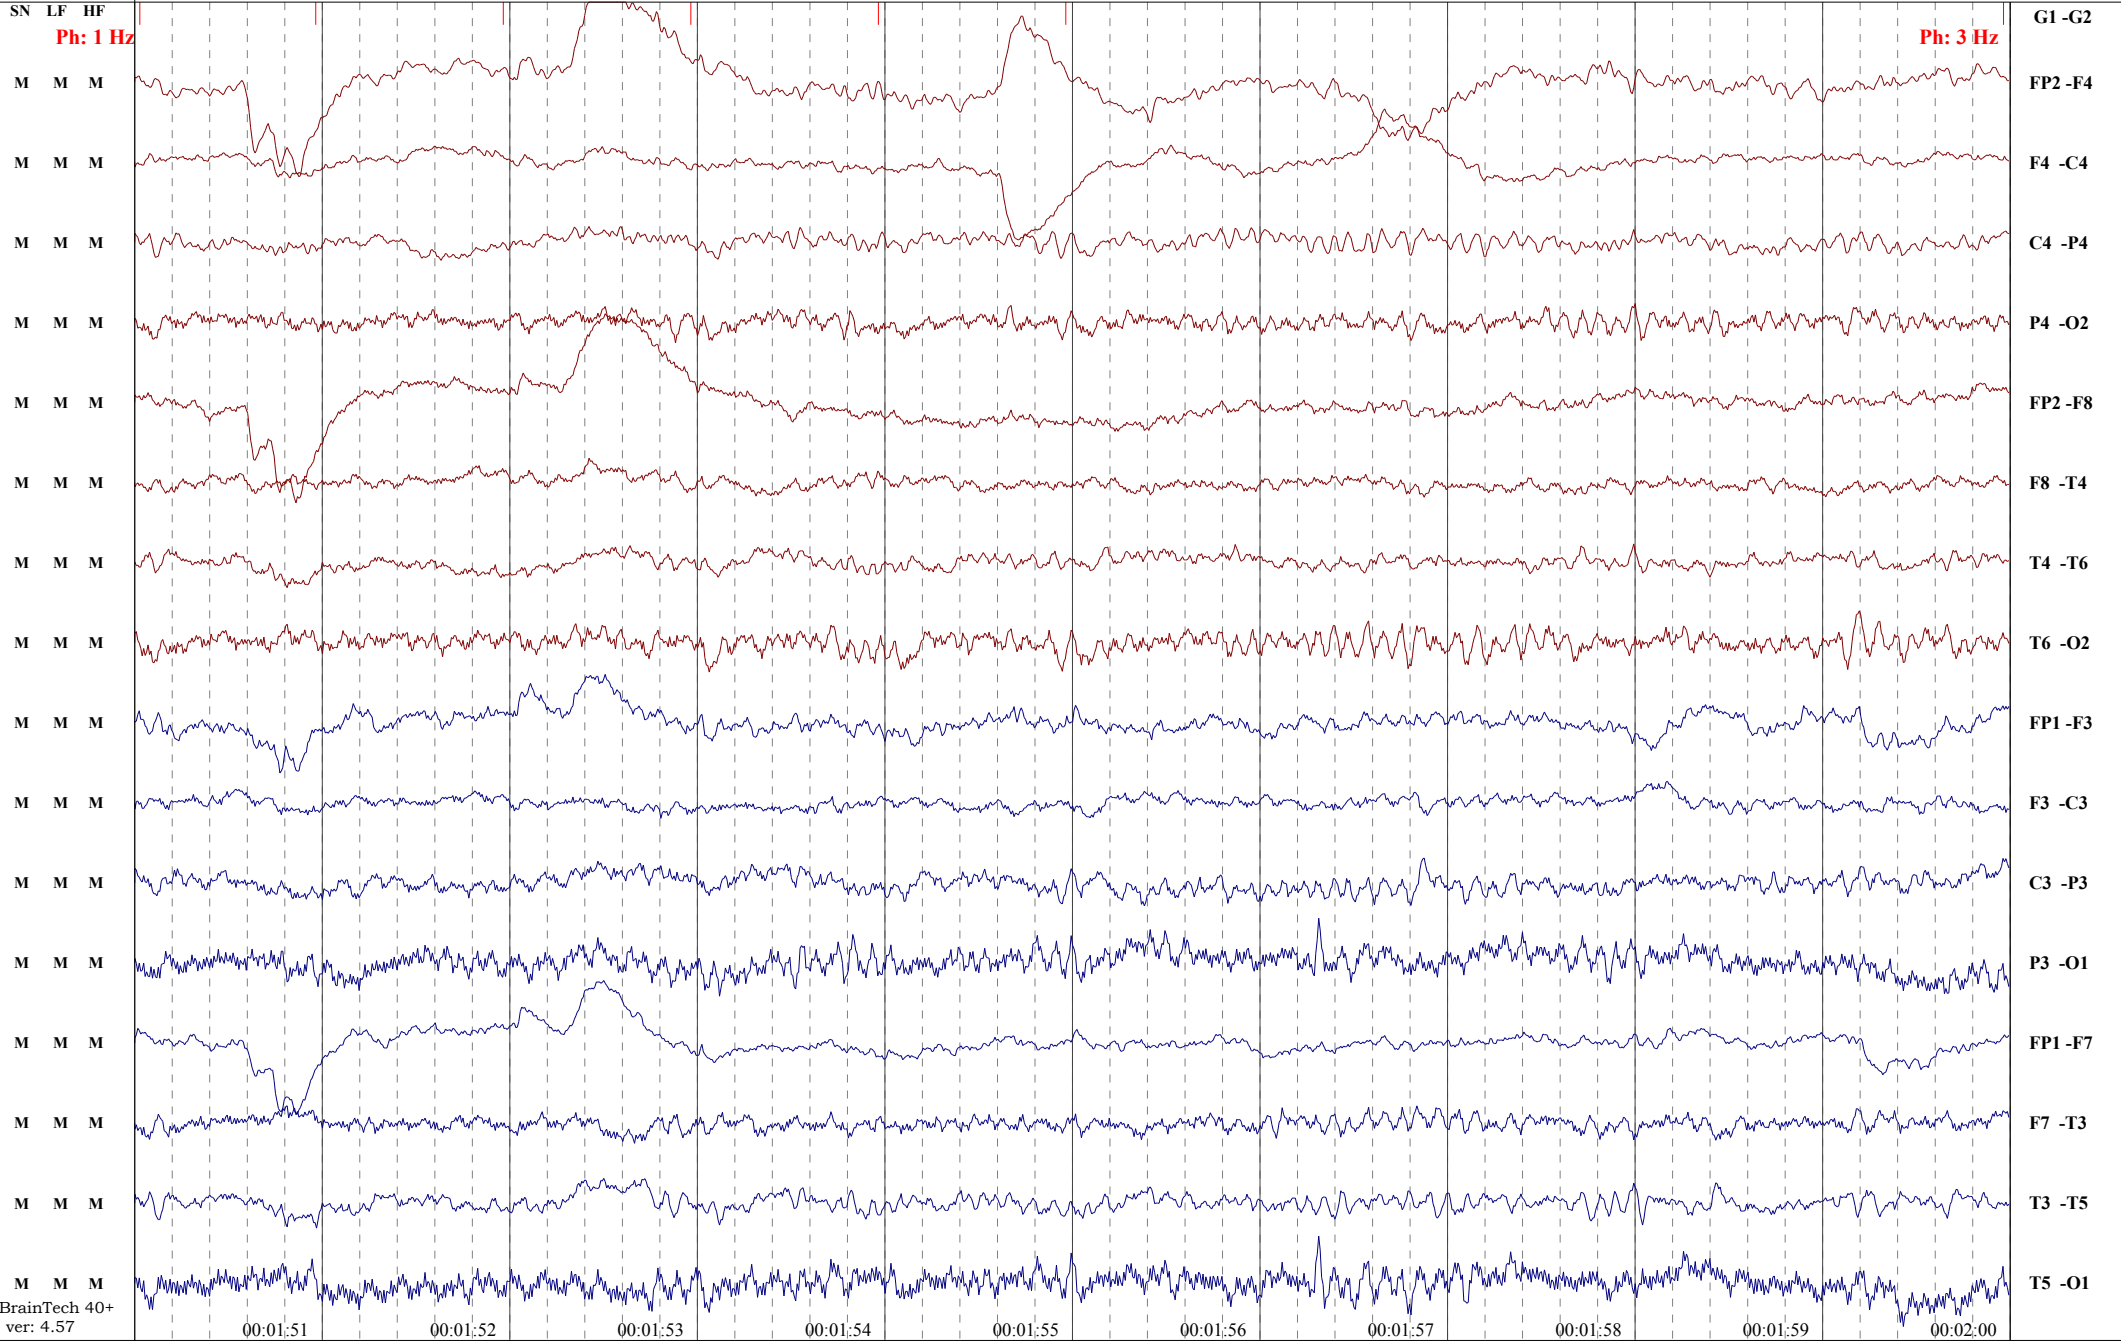


26  
MISS. ASHWANI BORKAR  
21 Years/F

Date: 25-Jul-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:43:30  
Page:13/28  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

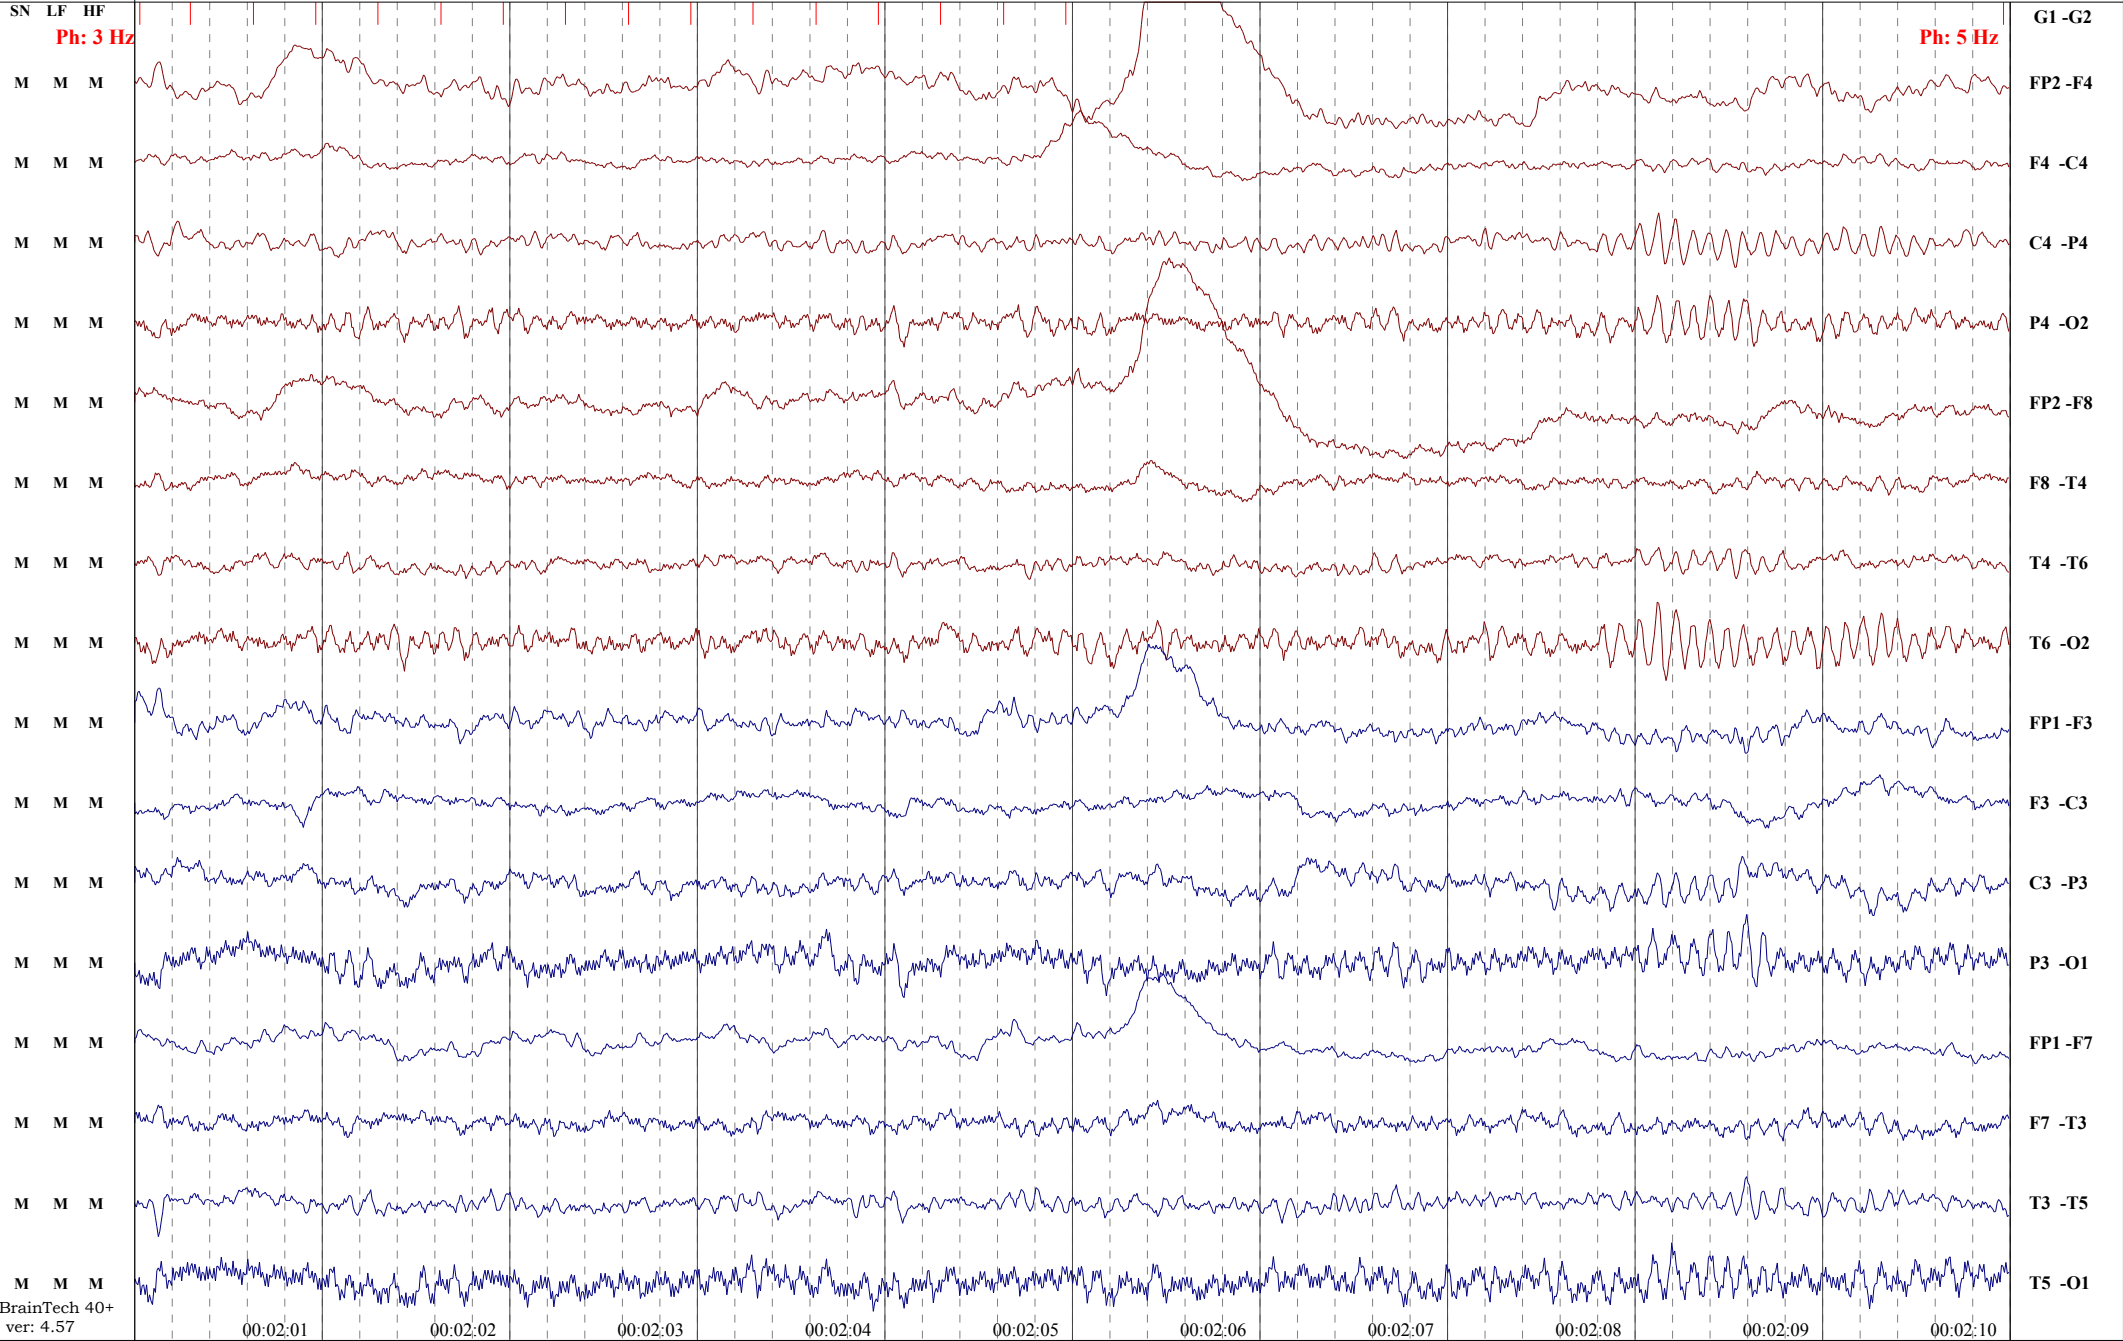




26  
MISS. ASHWANI BORKAR  
21 Years/F

Date: 25-Jul-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL


Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz


Time: 13:43:40  
Page:14/28  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

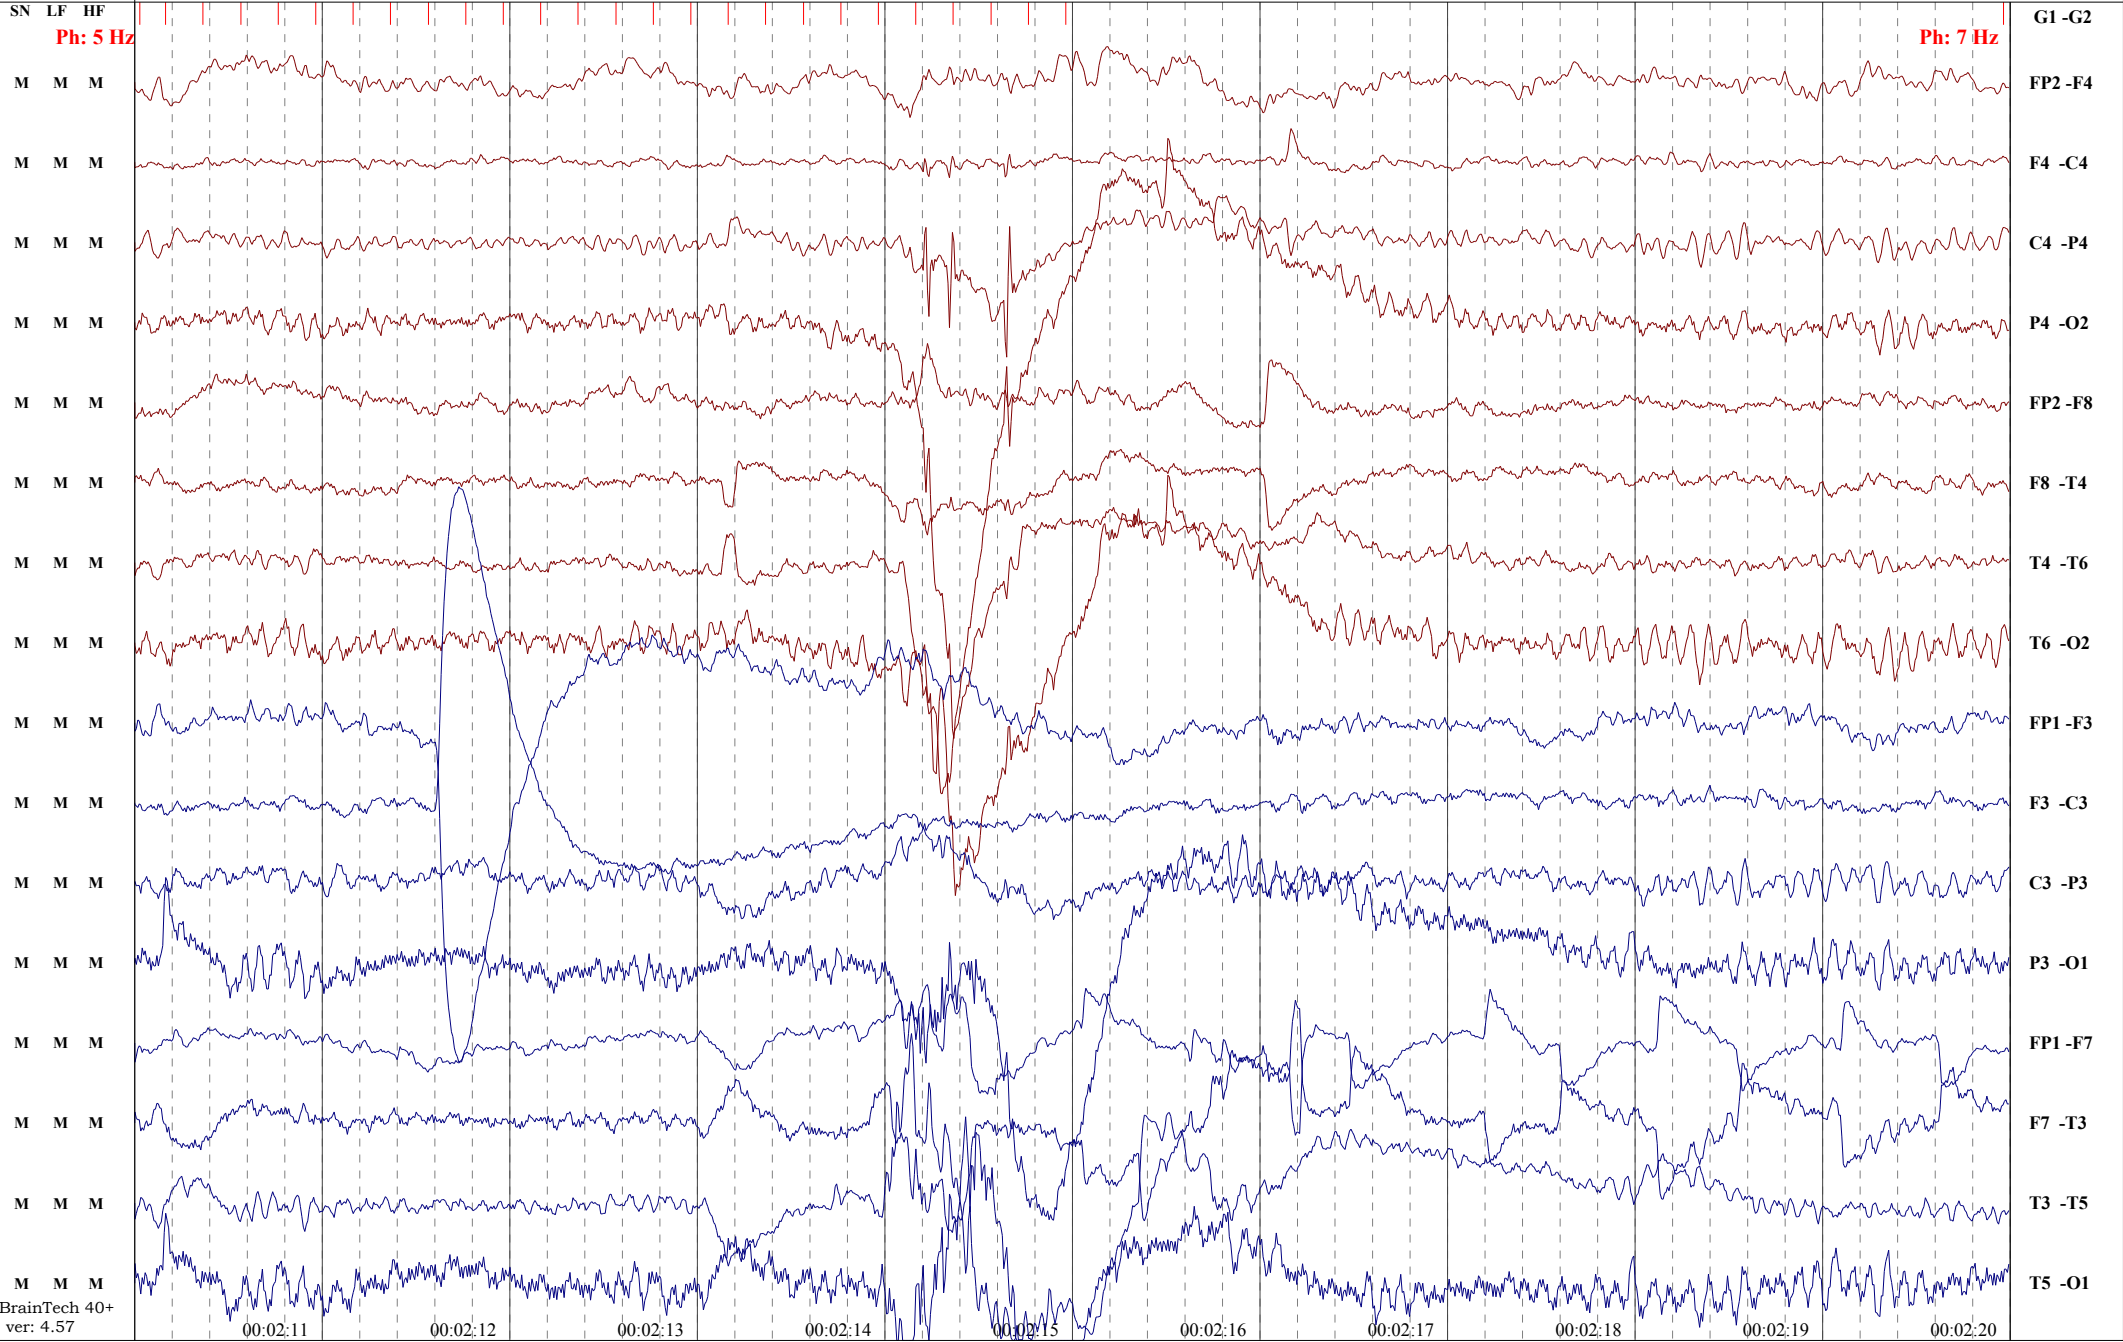



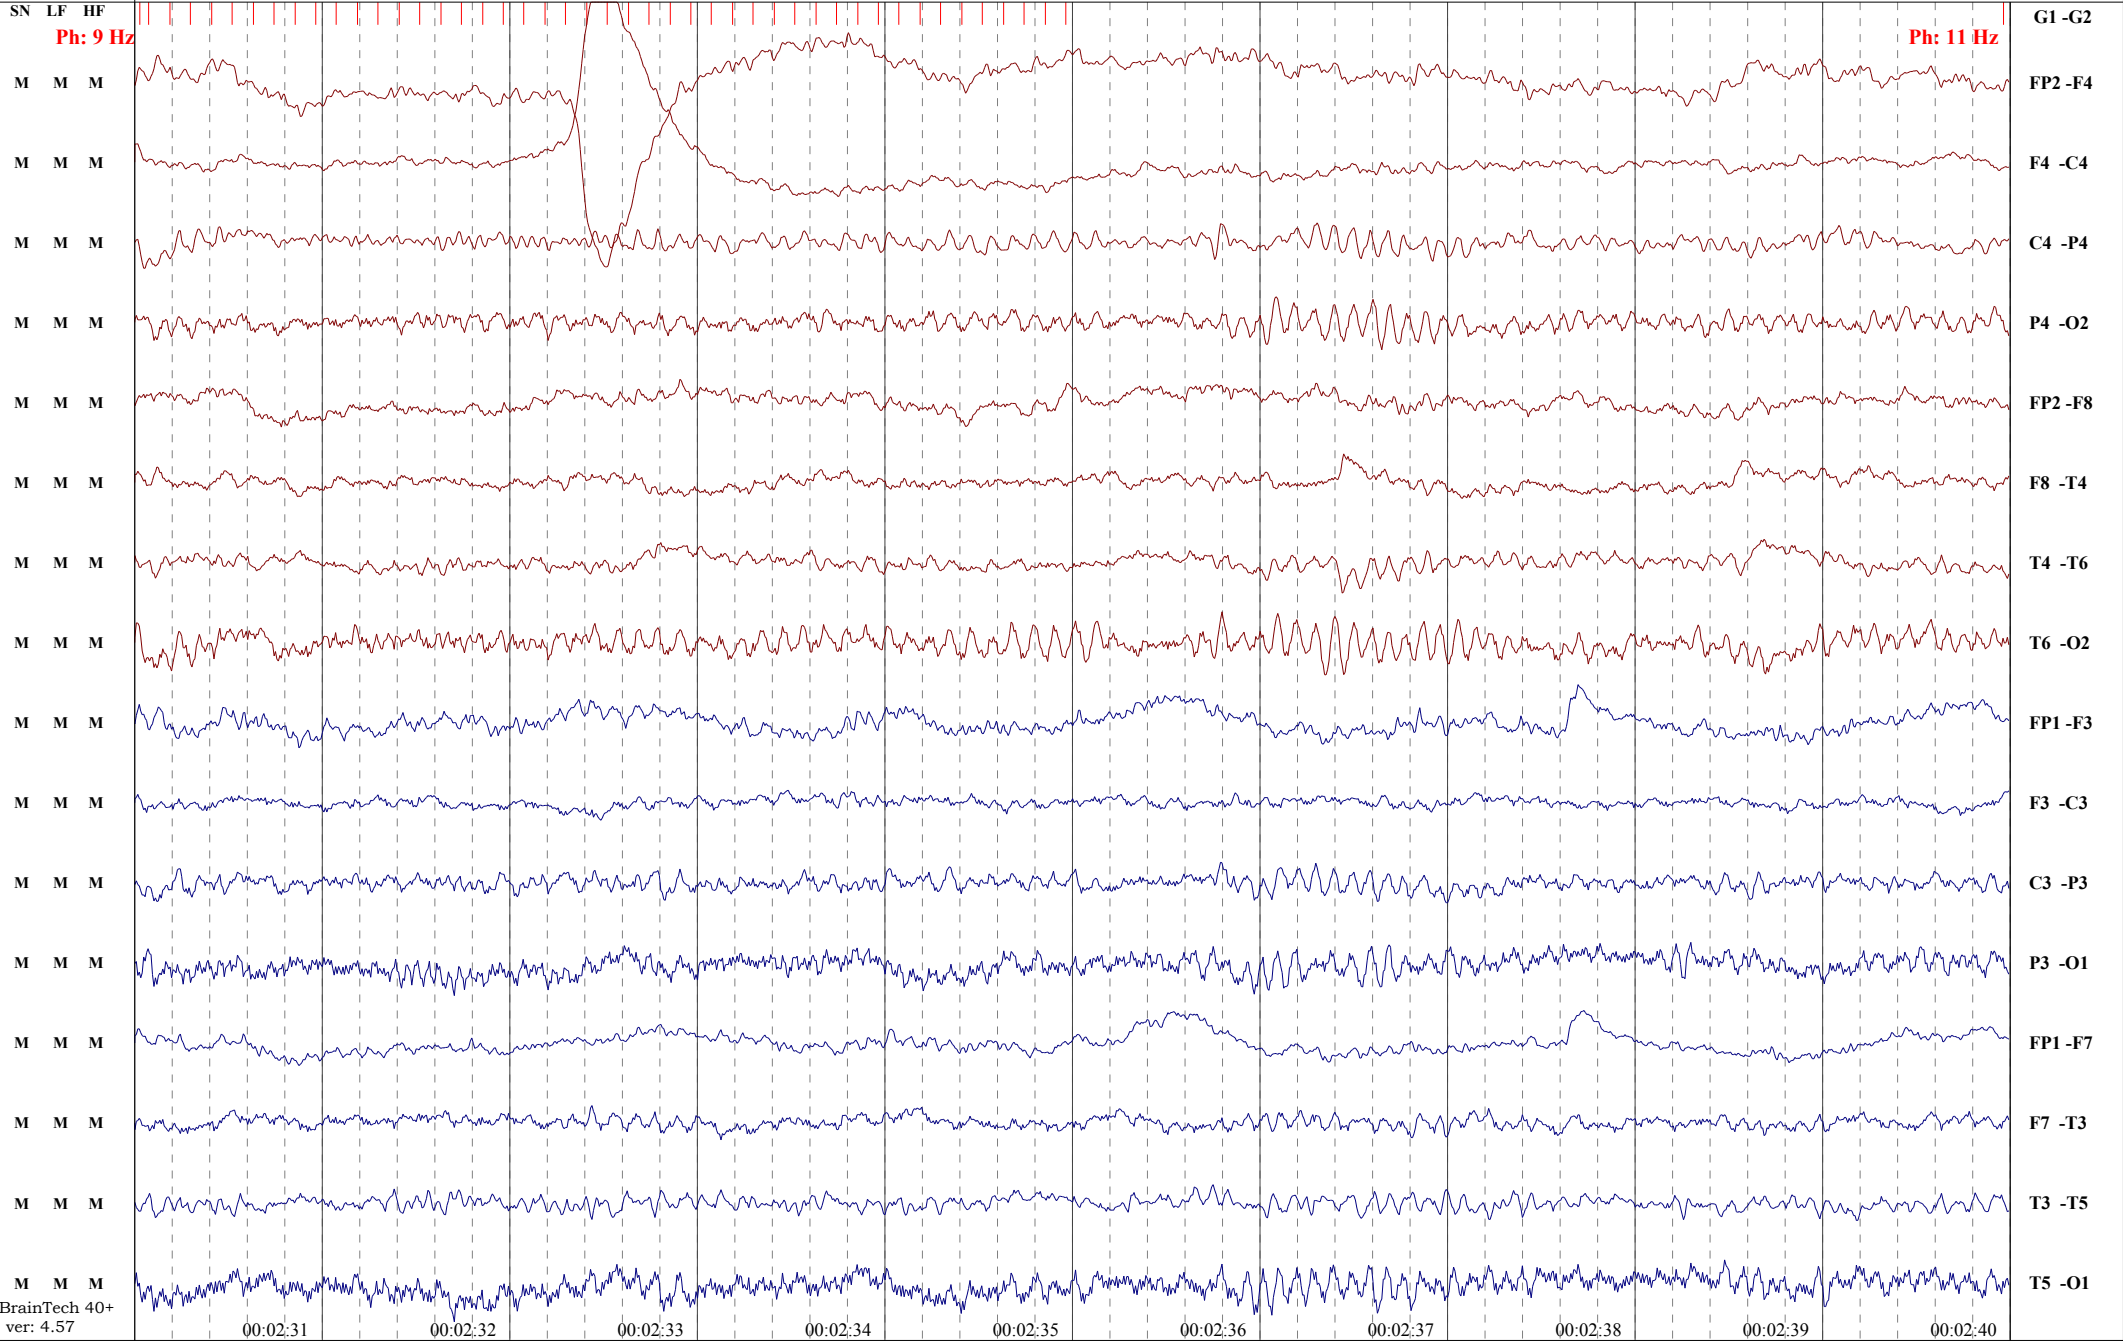

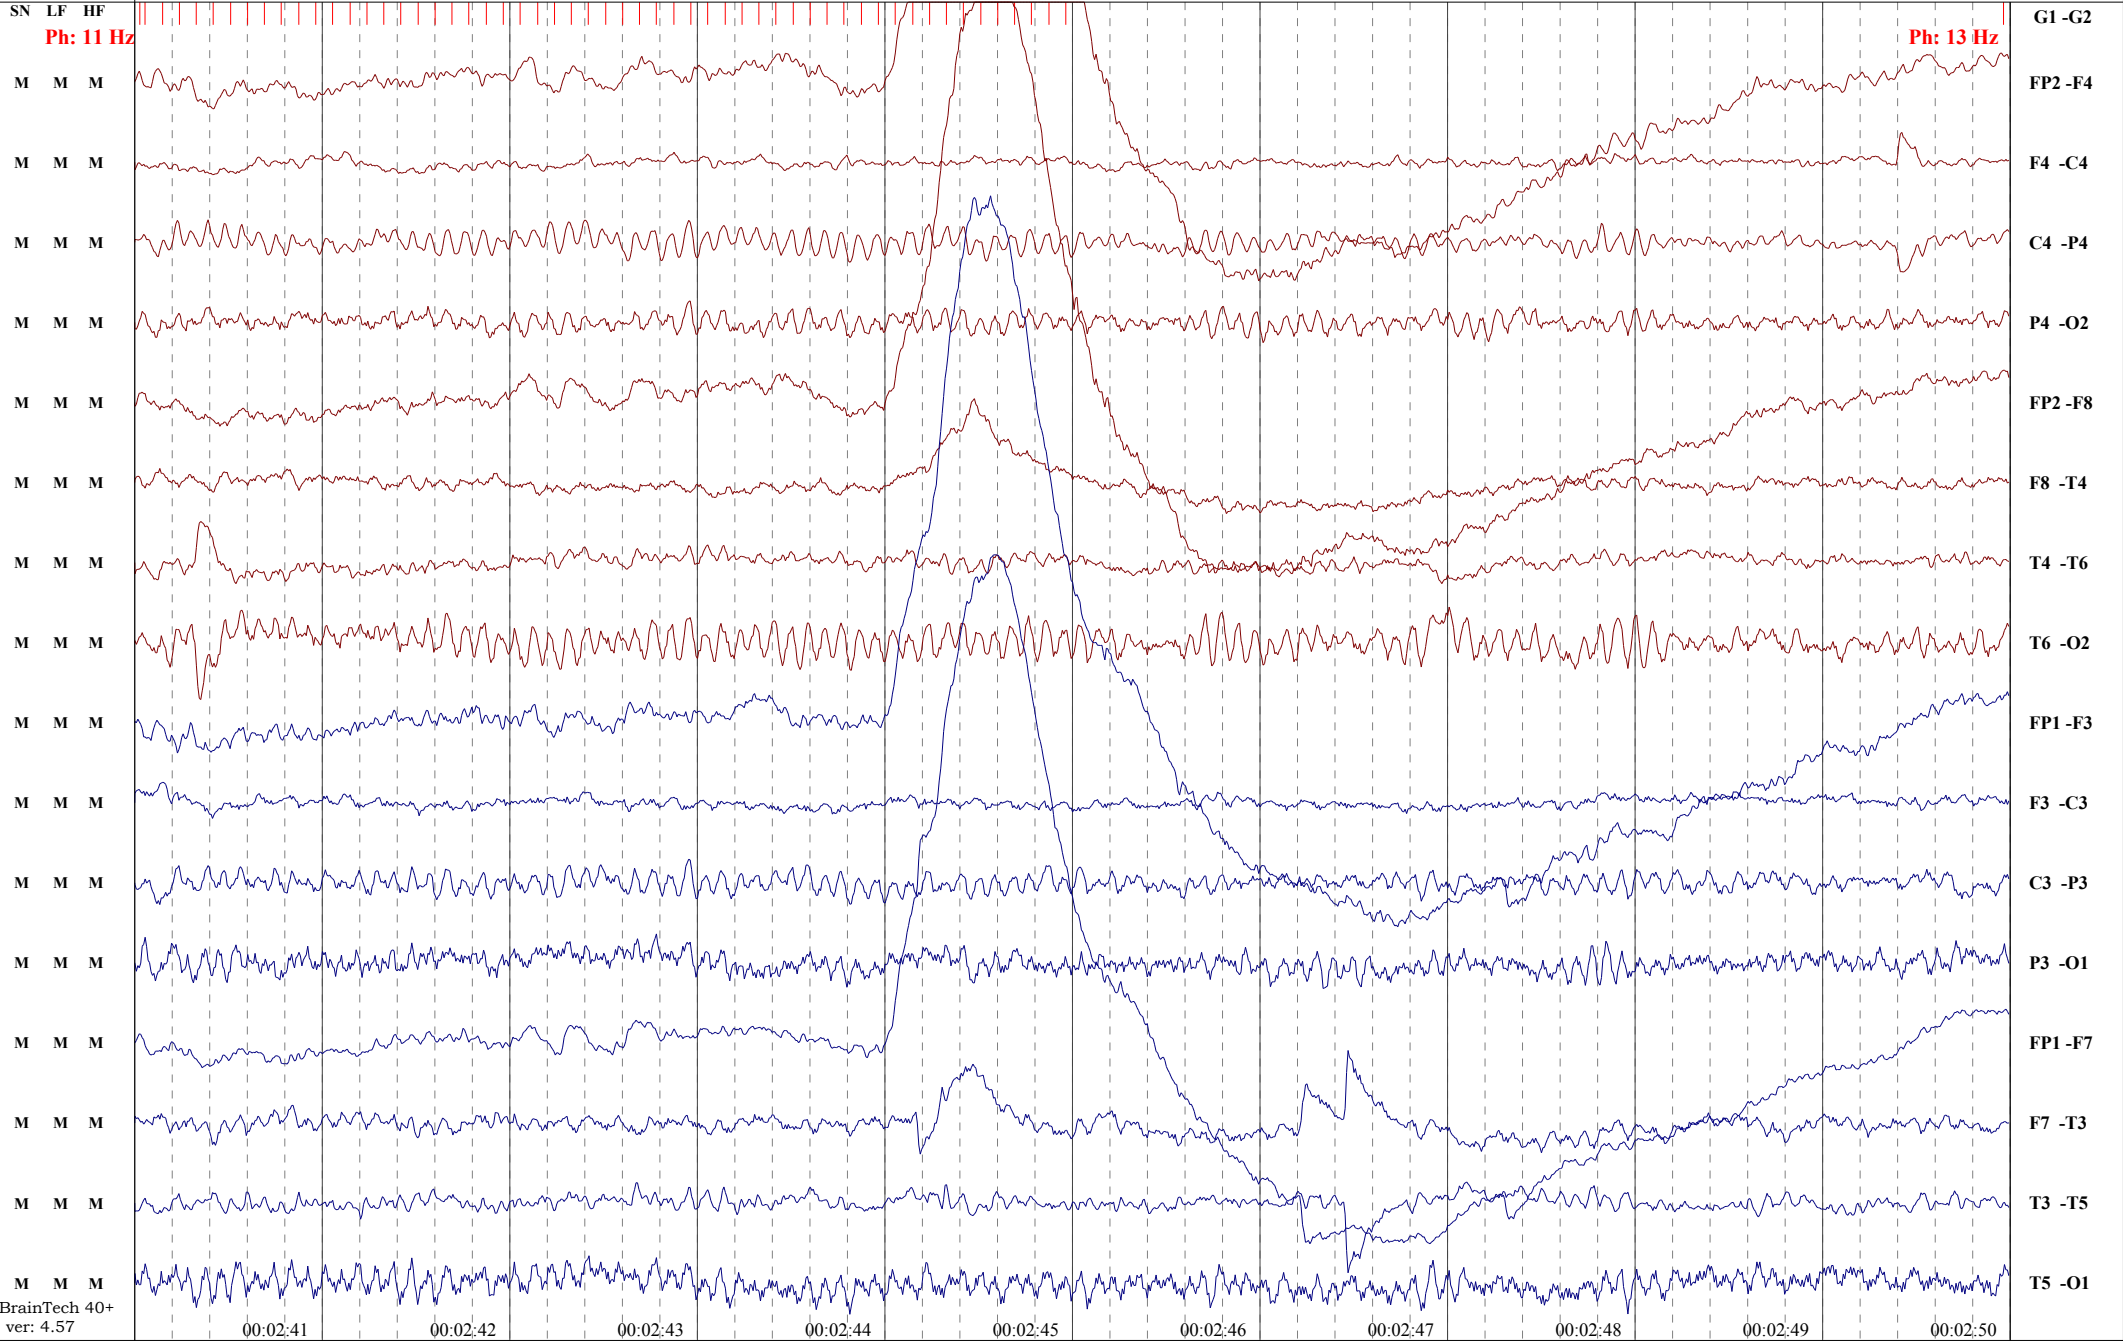


26  
MISS. ASHWANI BORKAR  
21 Years/F

Date: 25-Jul-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:44:11  
Page:17/28  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

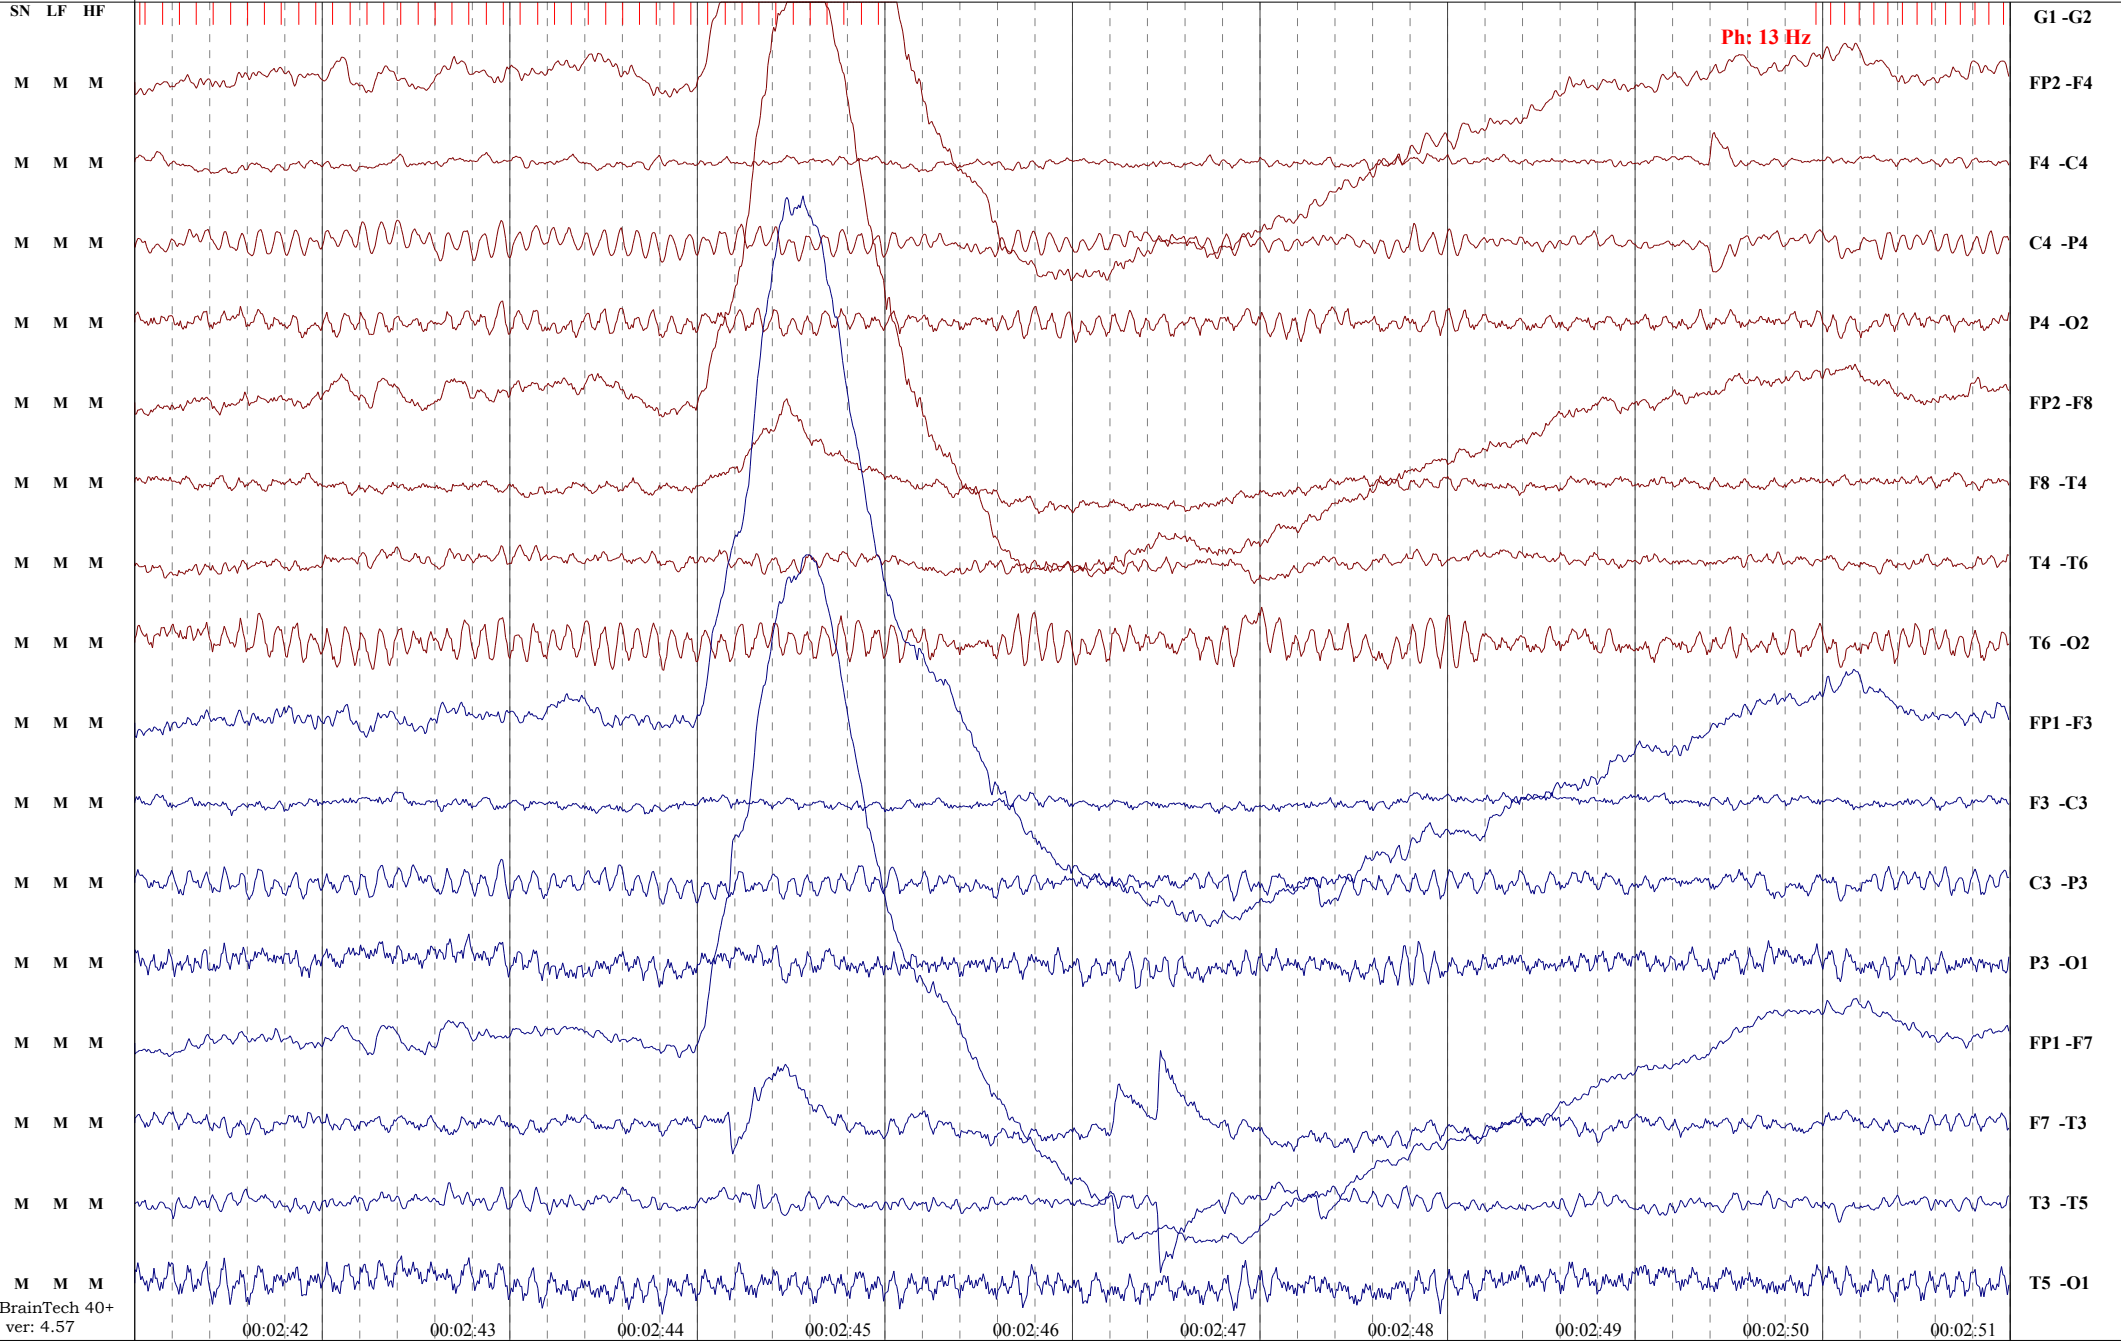




26  
MISS. ASHWANI BORKAR  
21 Years/F


Date: 25-Jul-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:44:21  
Page:18/28  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

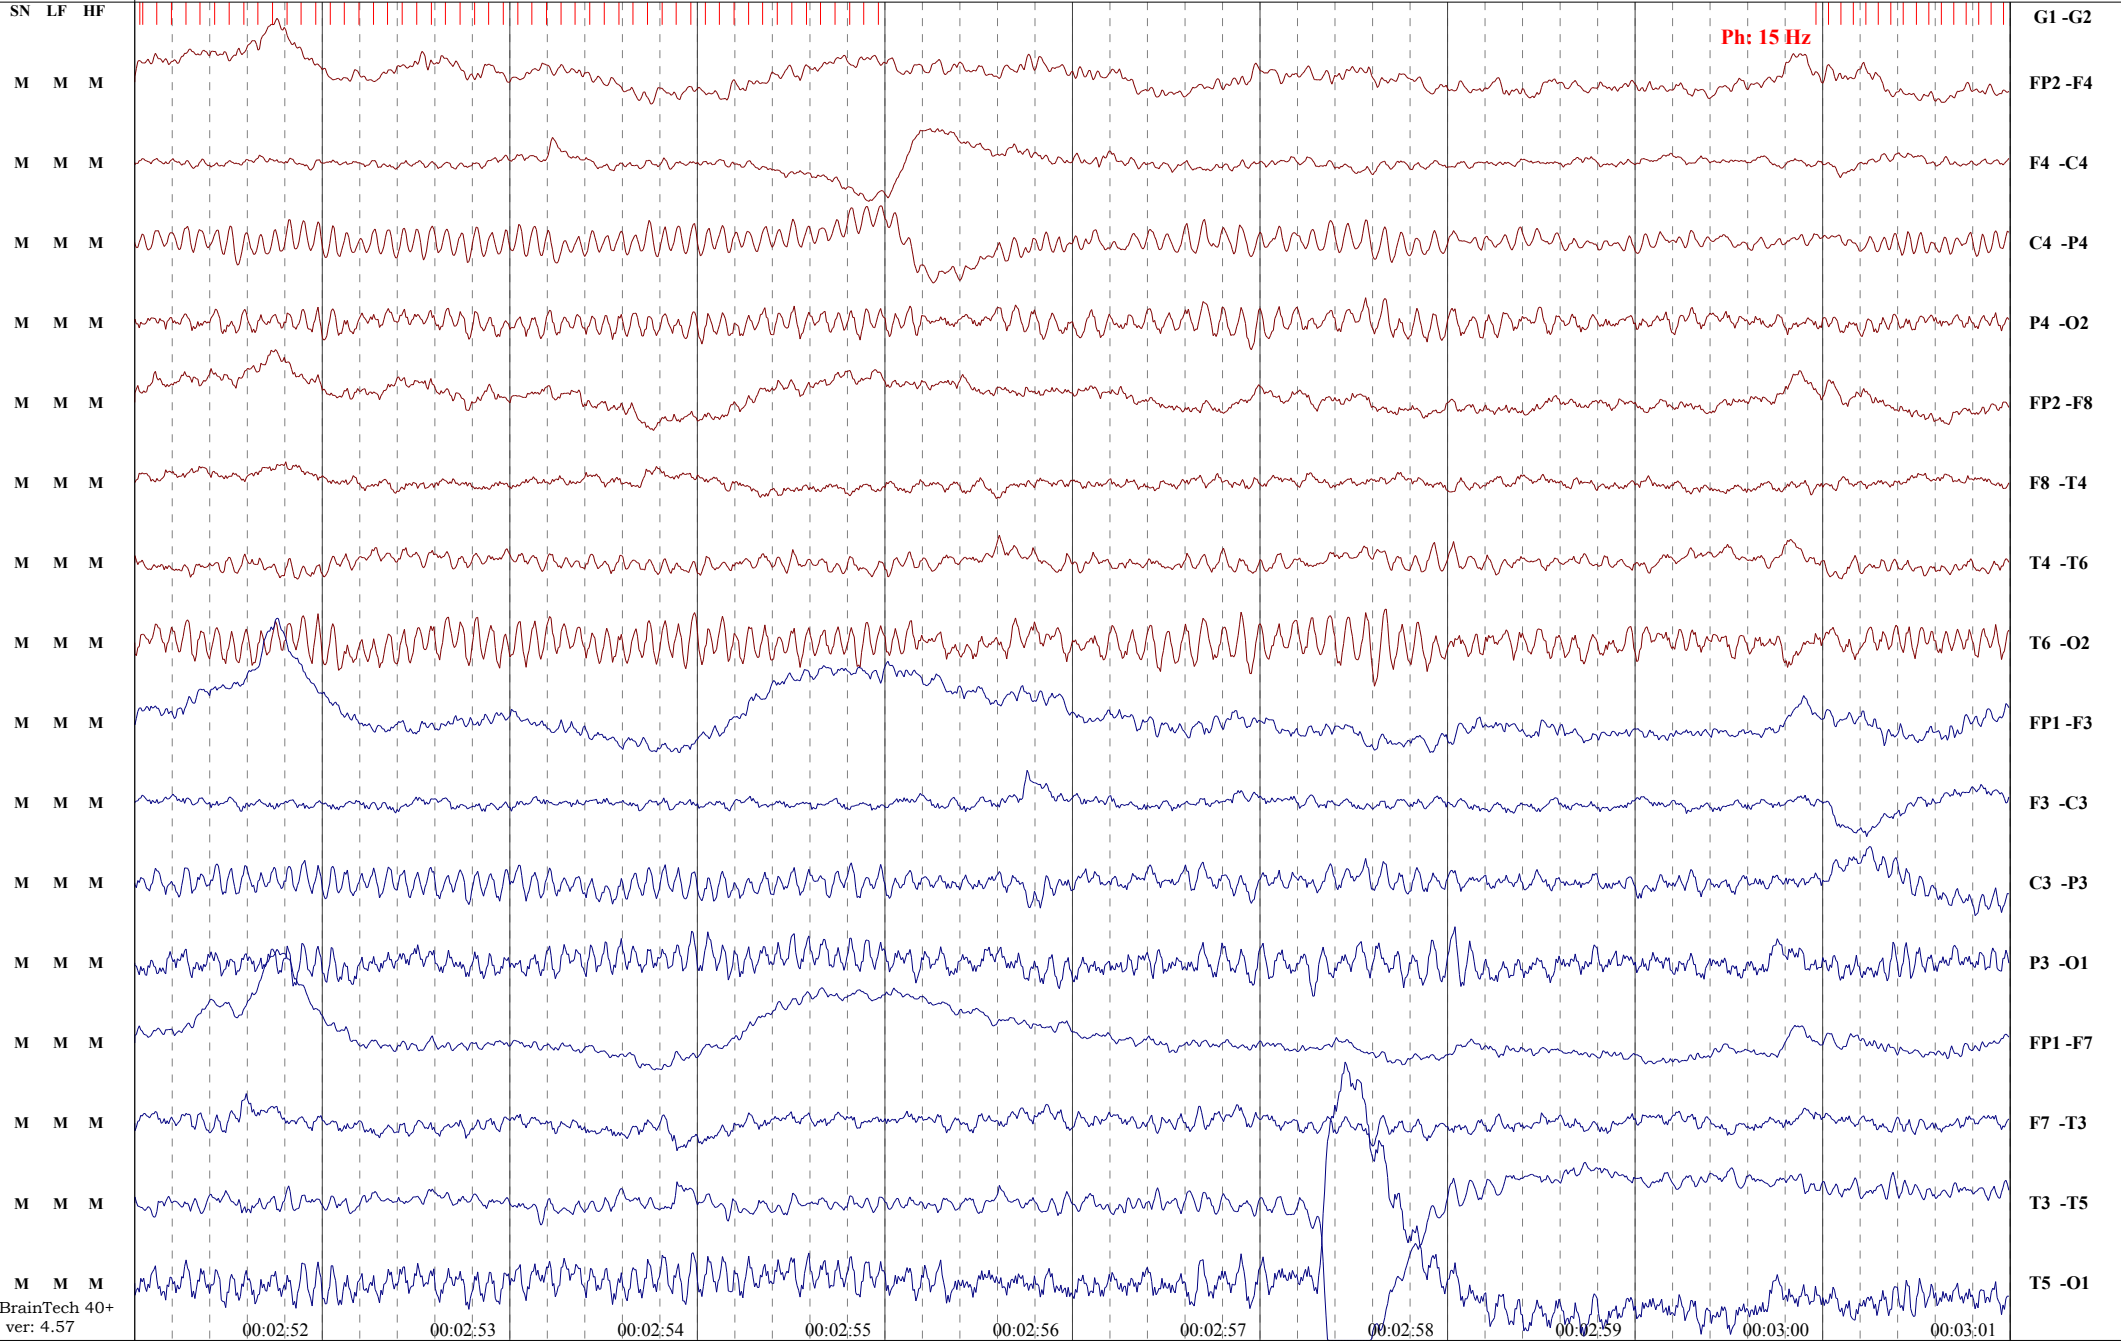

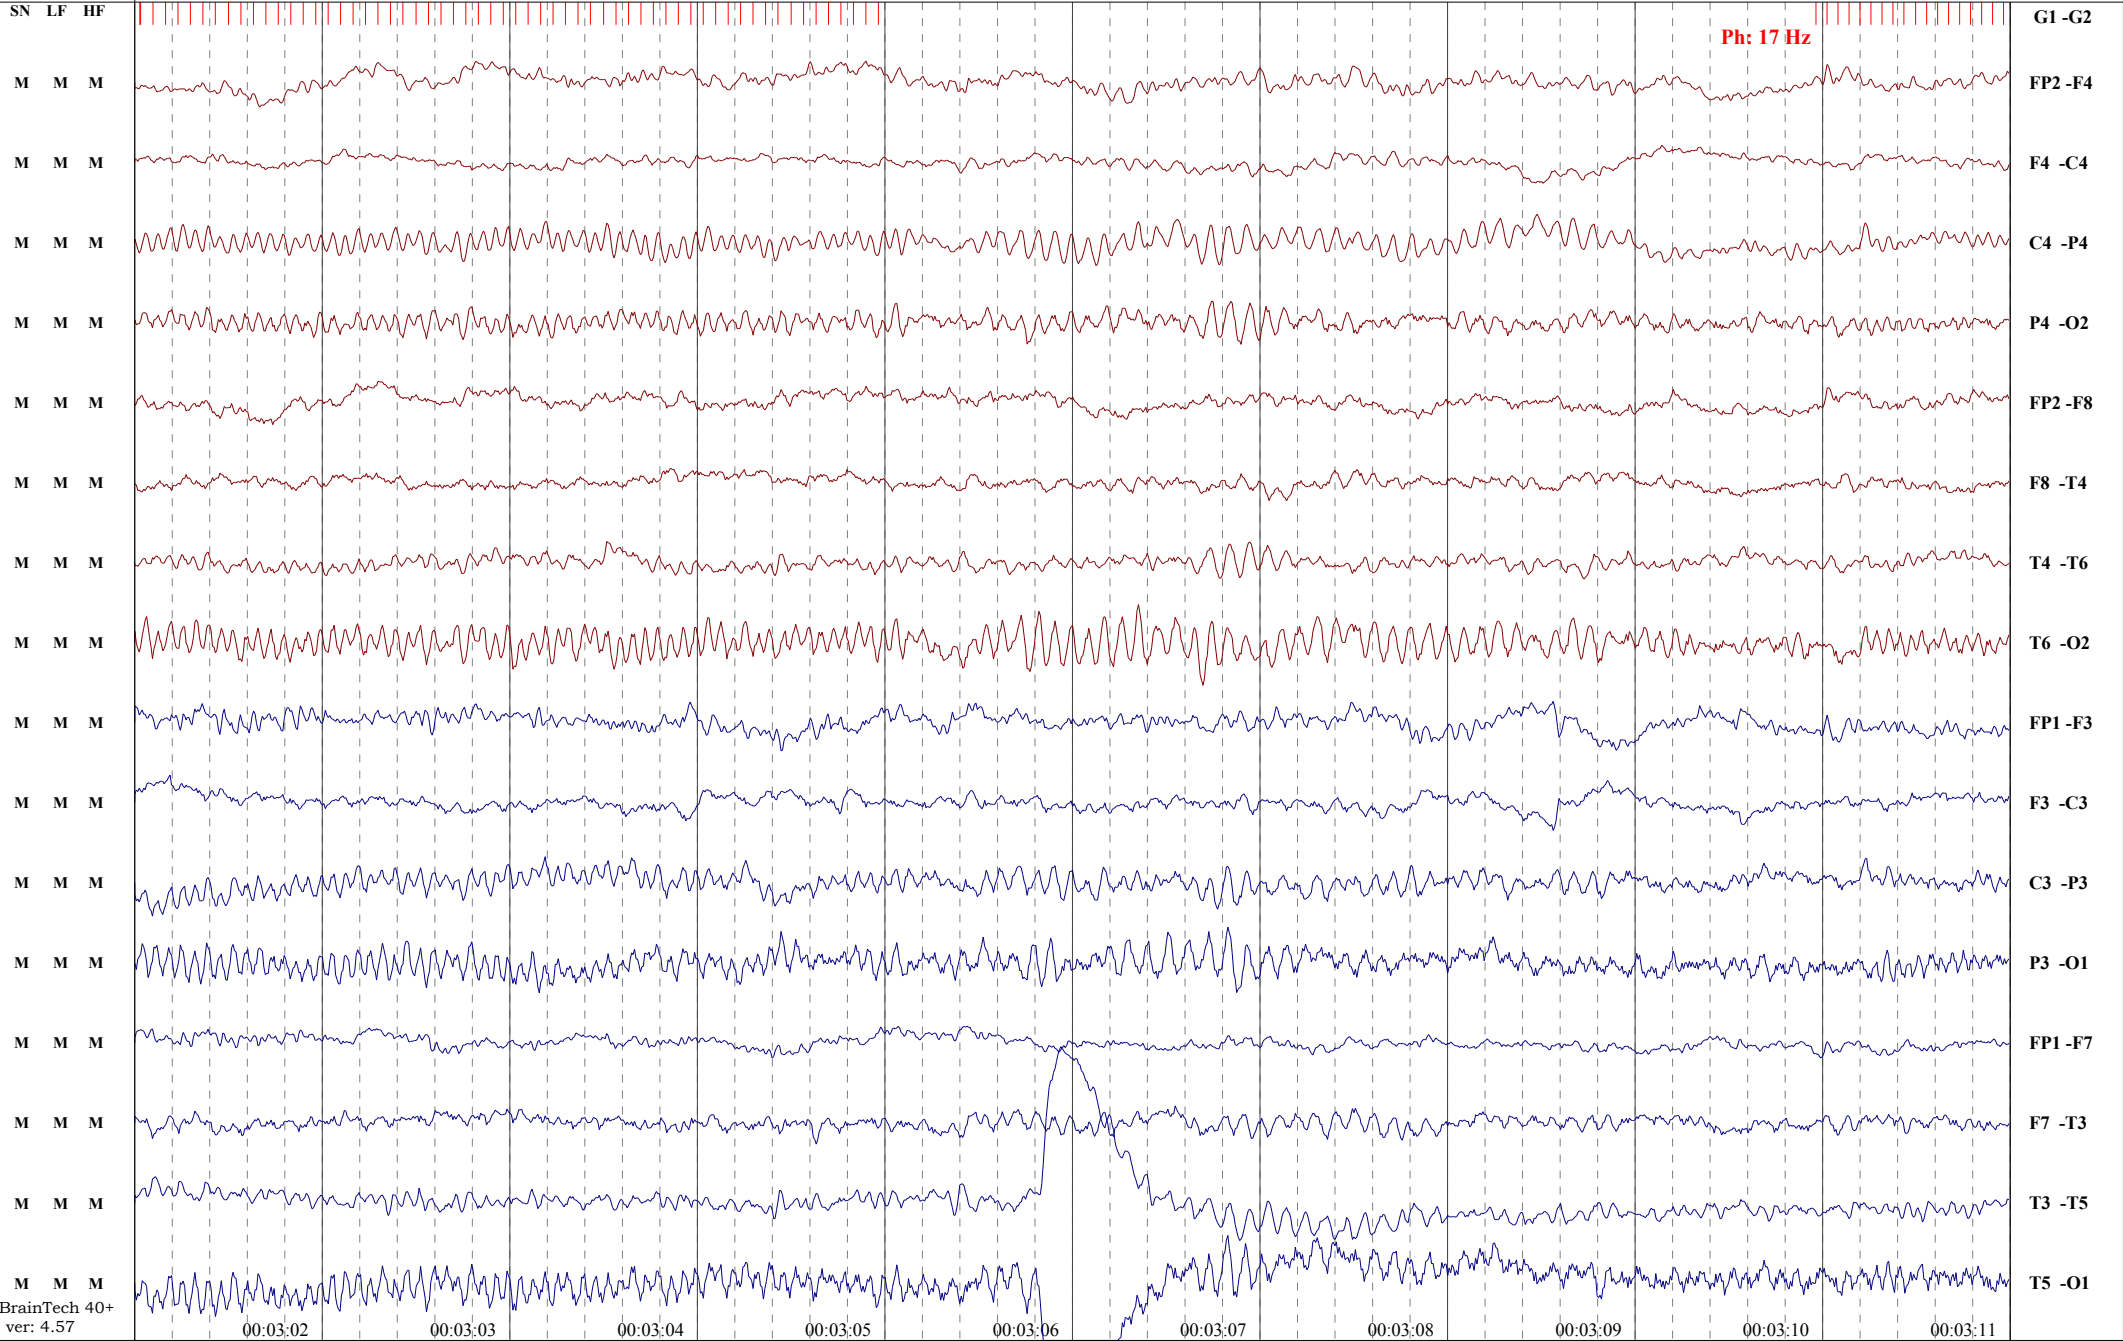

**PRATHAM HOSPITAL**


**26**  
**MISS. ASHWANI BORKAR**  
**21 Years/F**


**Date:** 25-Jul-2023  
**Type:** ANALYSIS  
**BIPOLAR LONGITUDNAL**

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:44:41  
Page:20/28  
Notch: ON

**Ref:DR. RAJNISH PANDEY**  
**Dr. : DR. VIJENDRA PAINKARA**  
**Tech:**

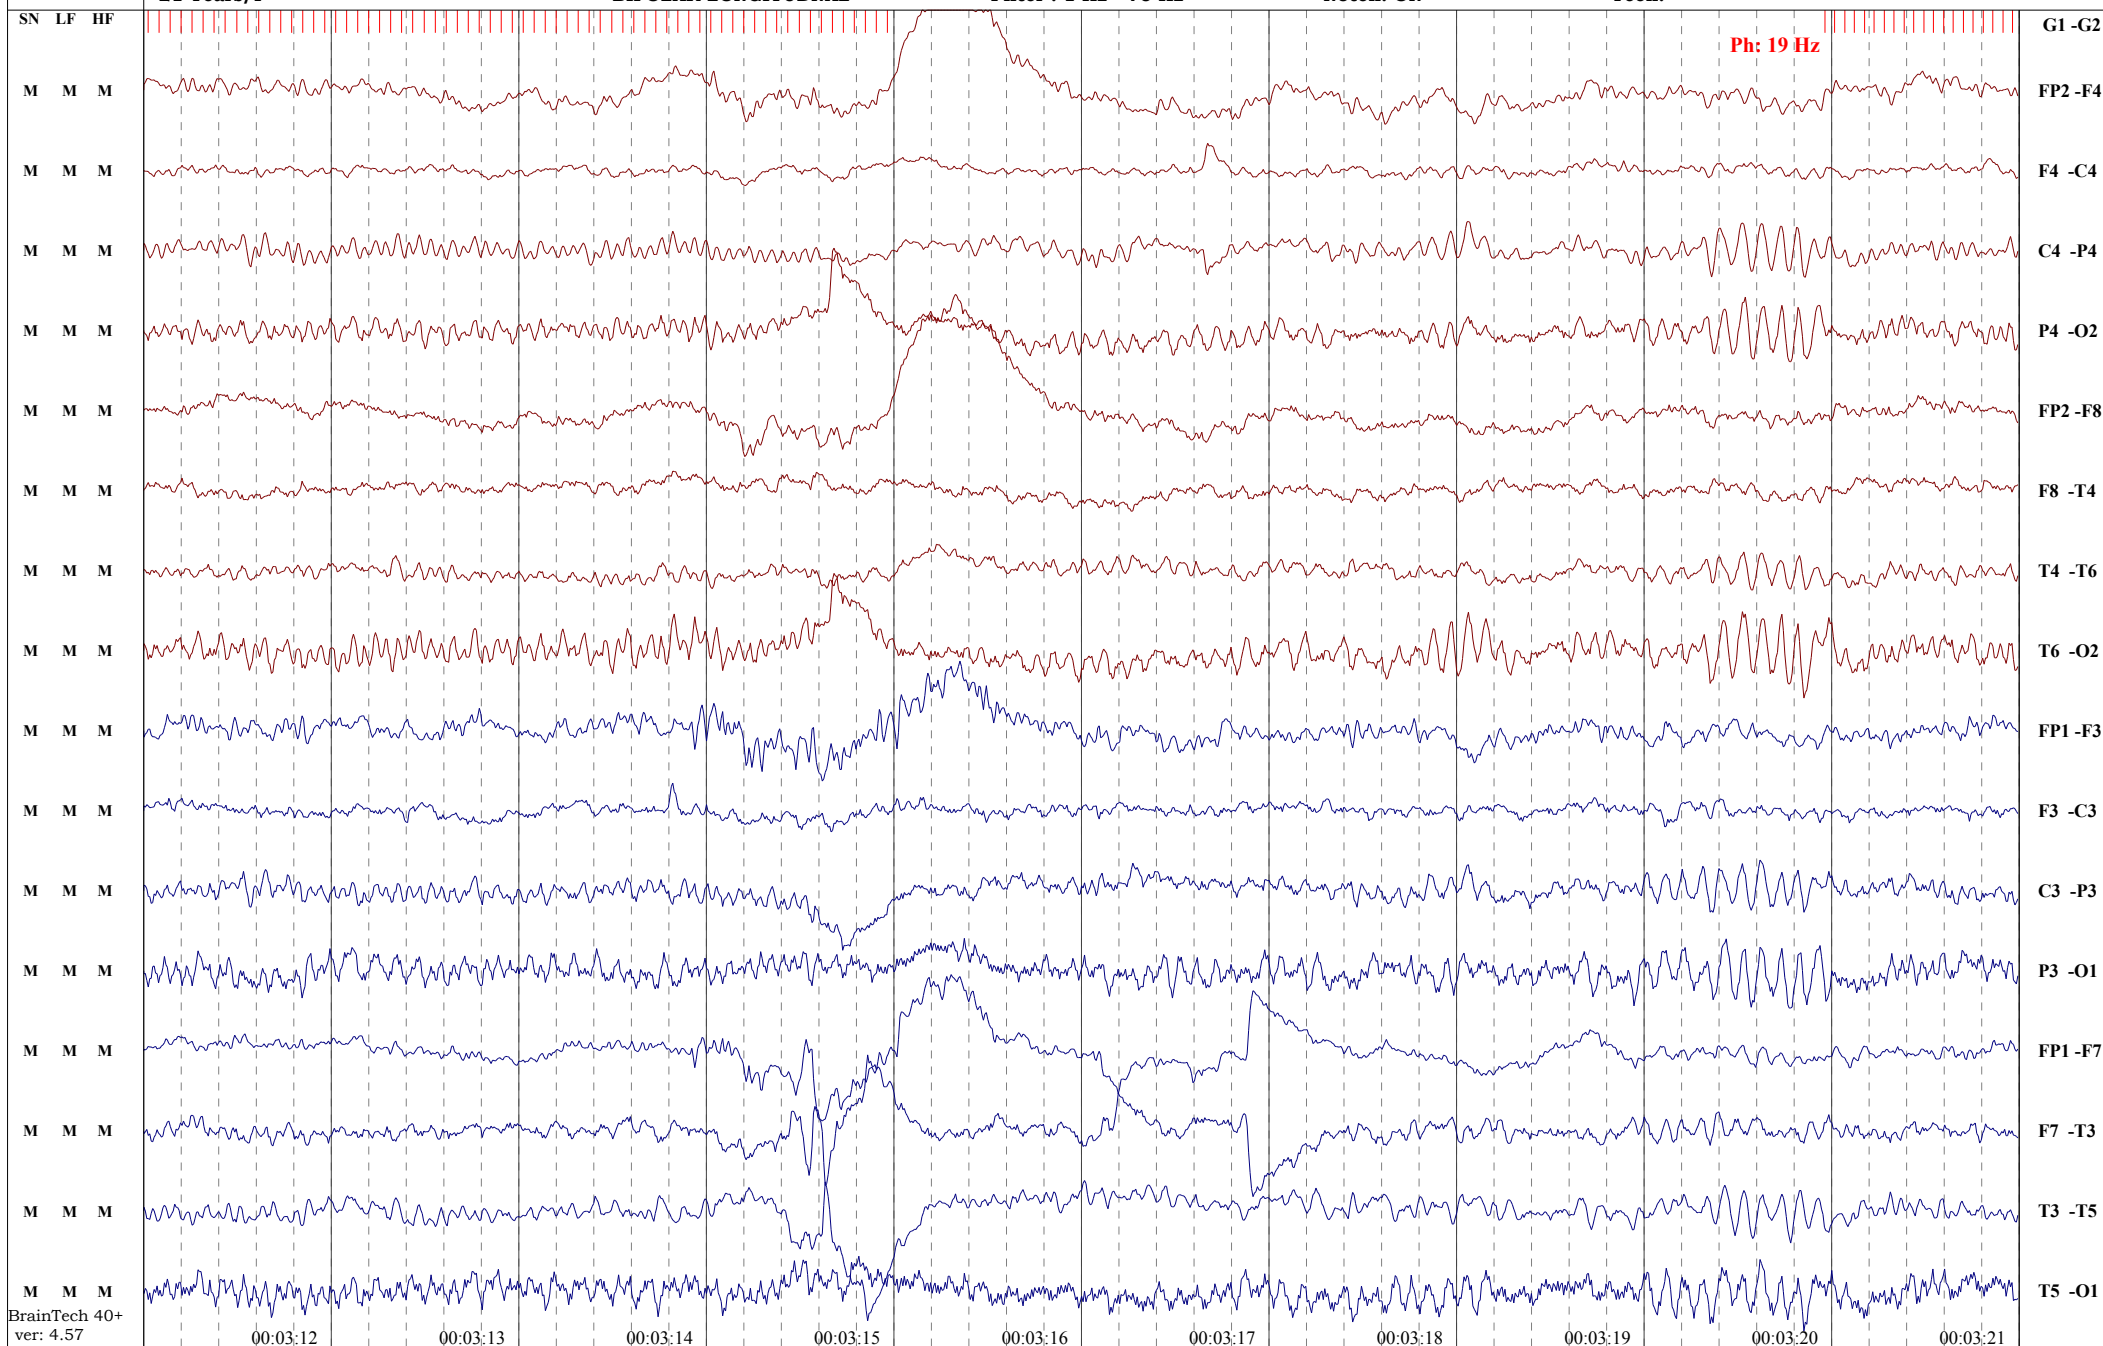

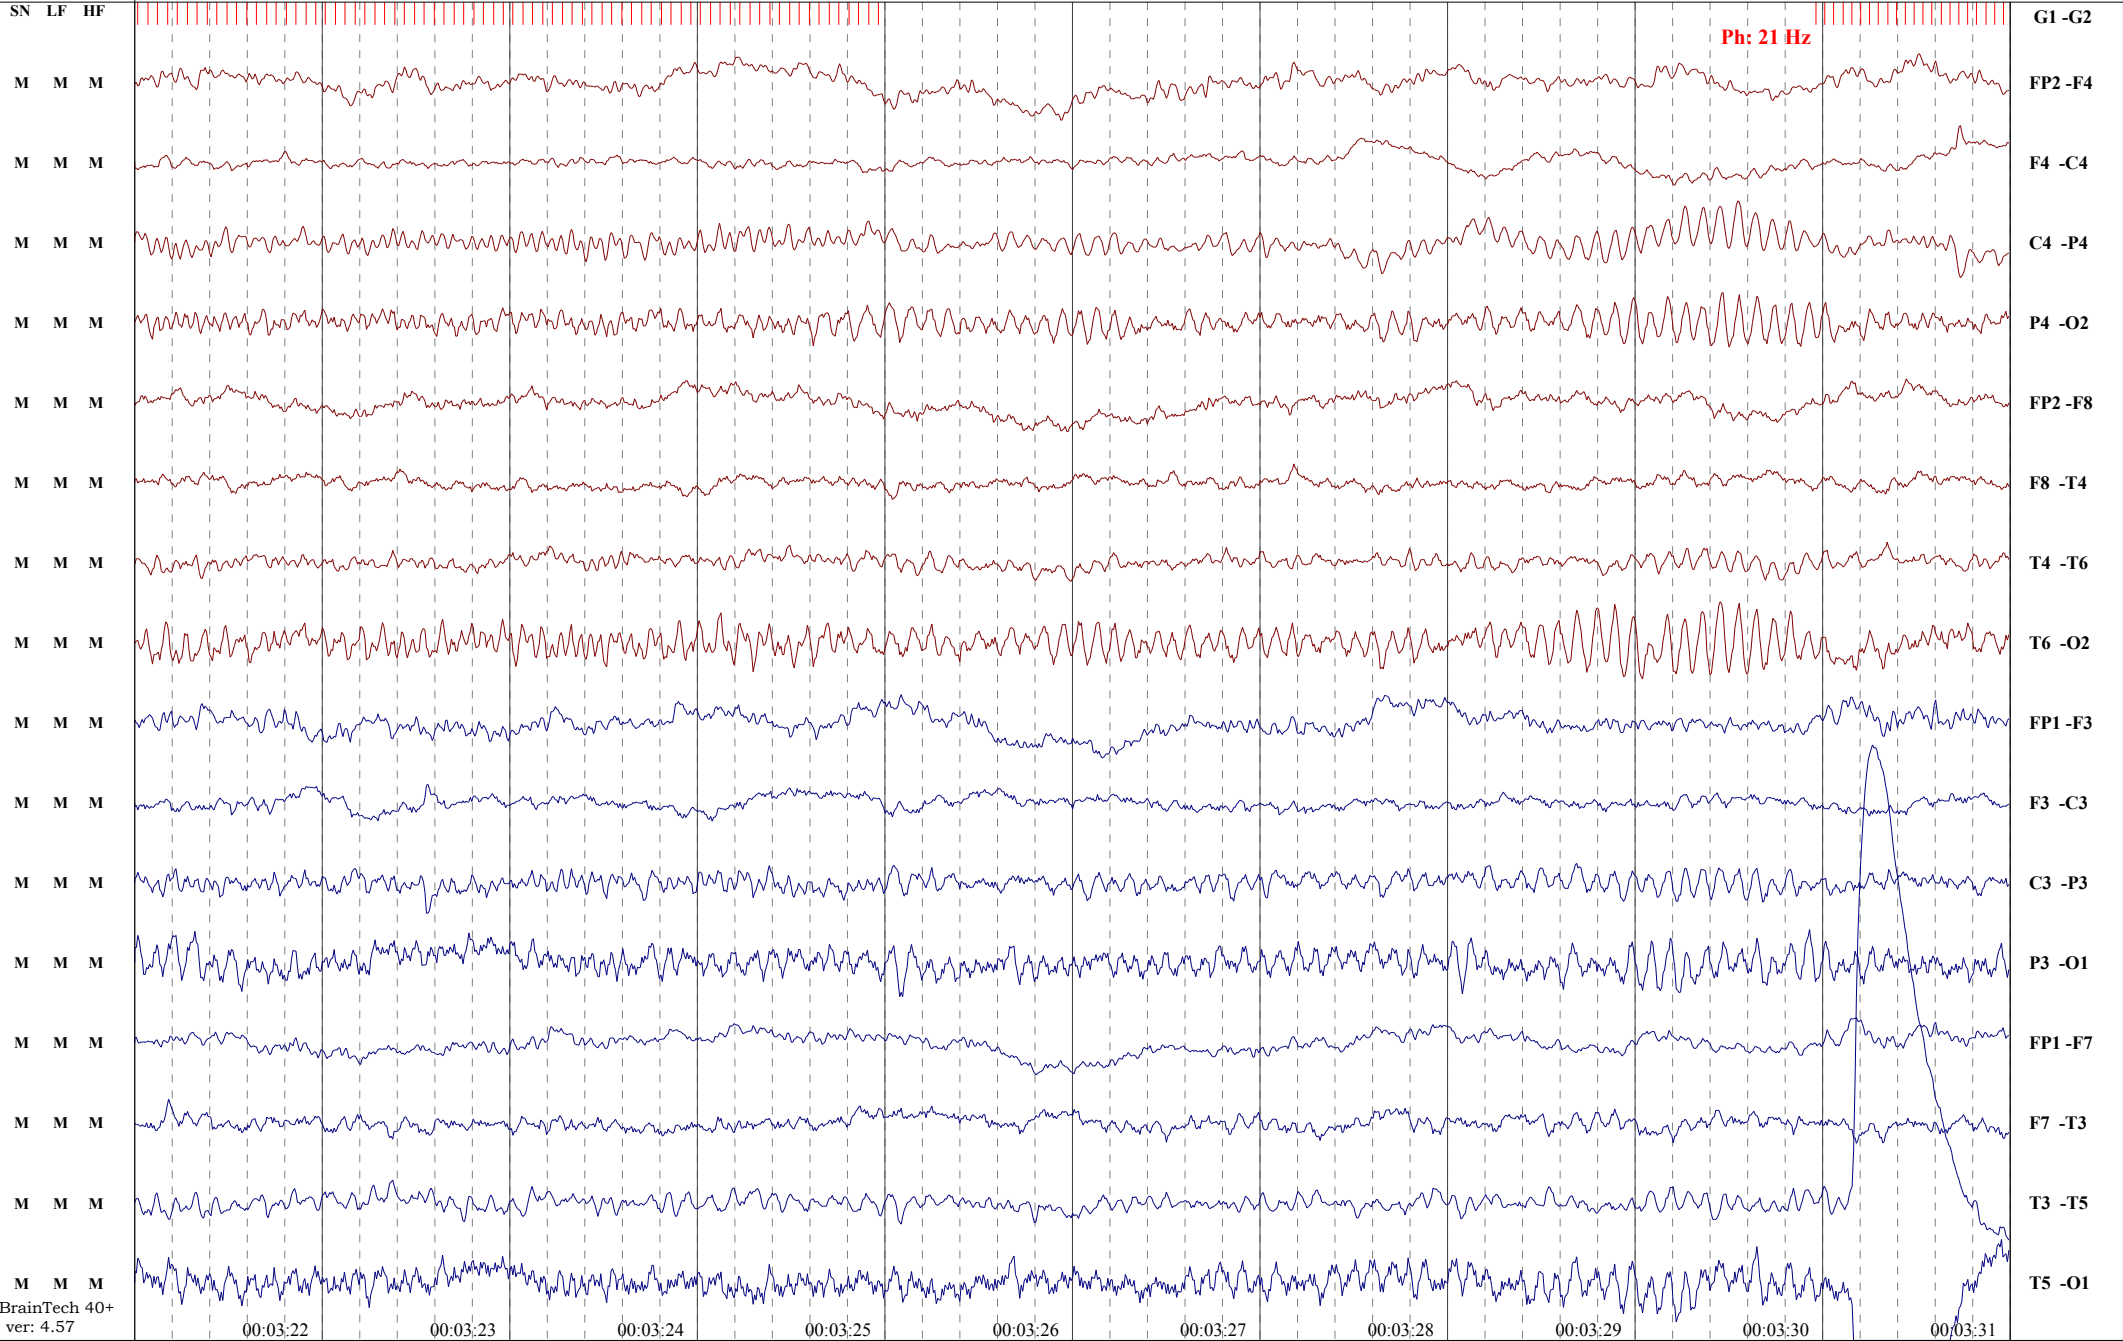




26  
MISS. ASHWANI BORKAR  
21 Years/F

Date: 25-Jul-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL


Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:45:01  
Page:22/28  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

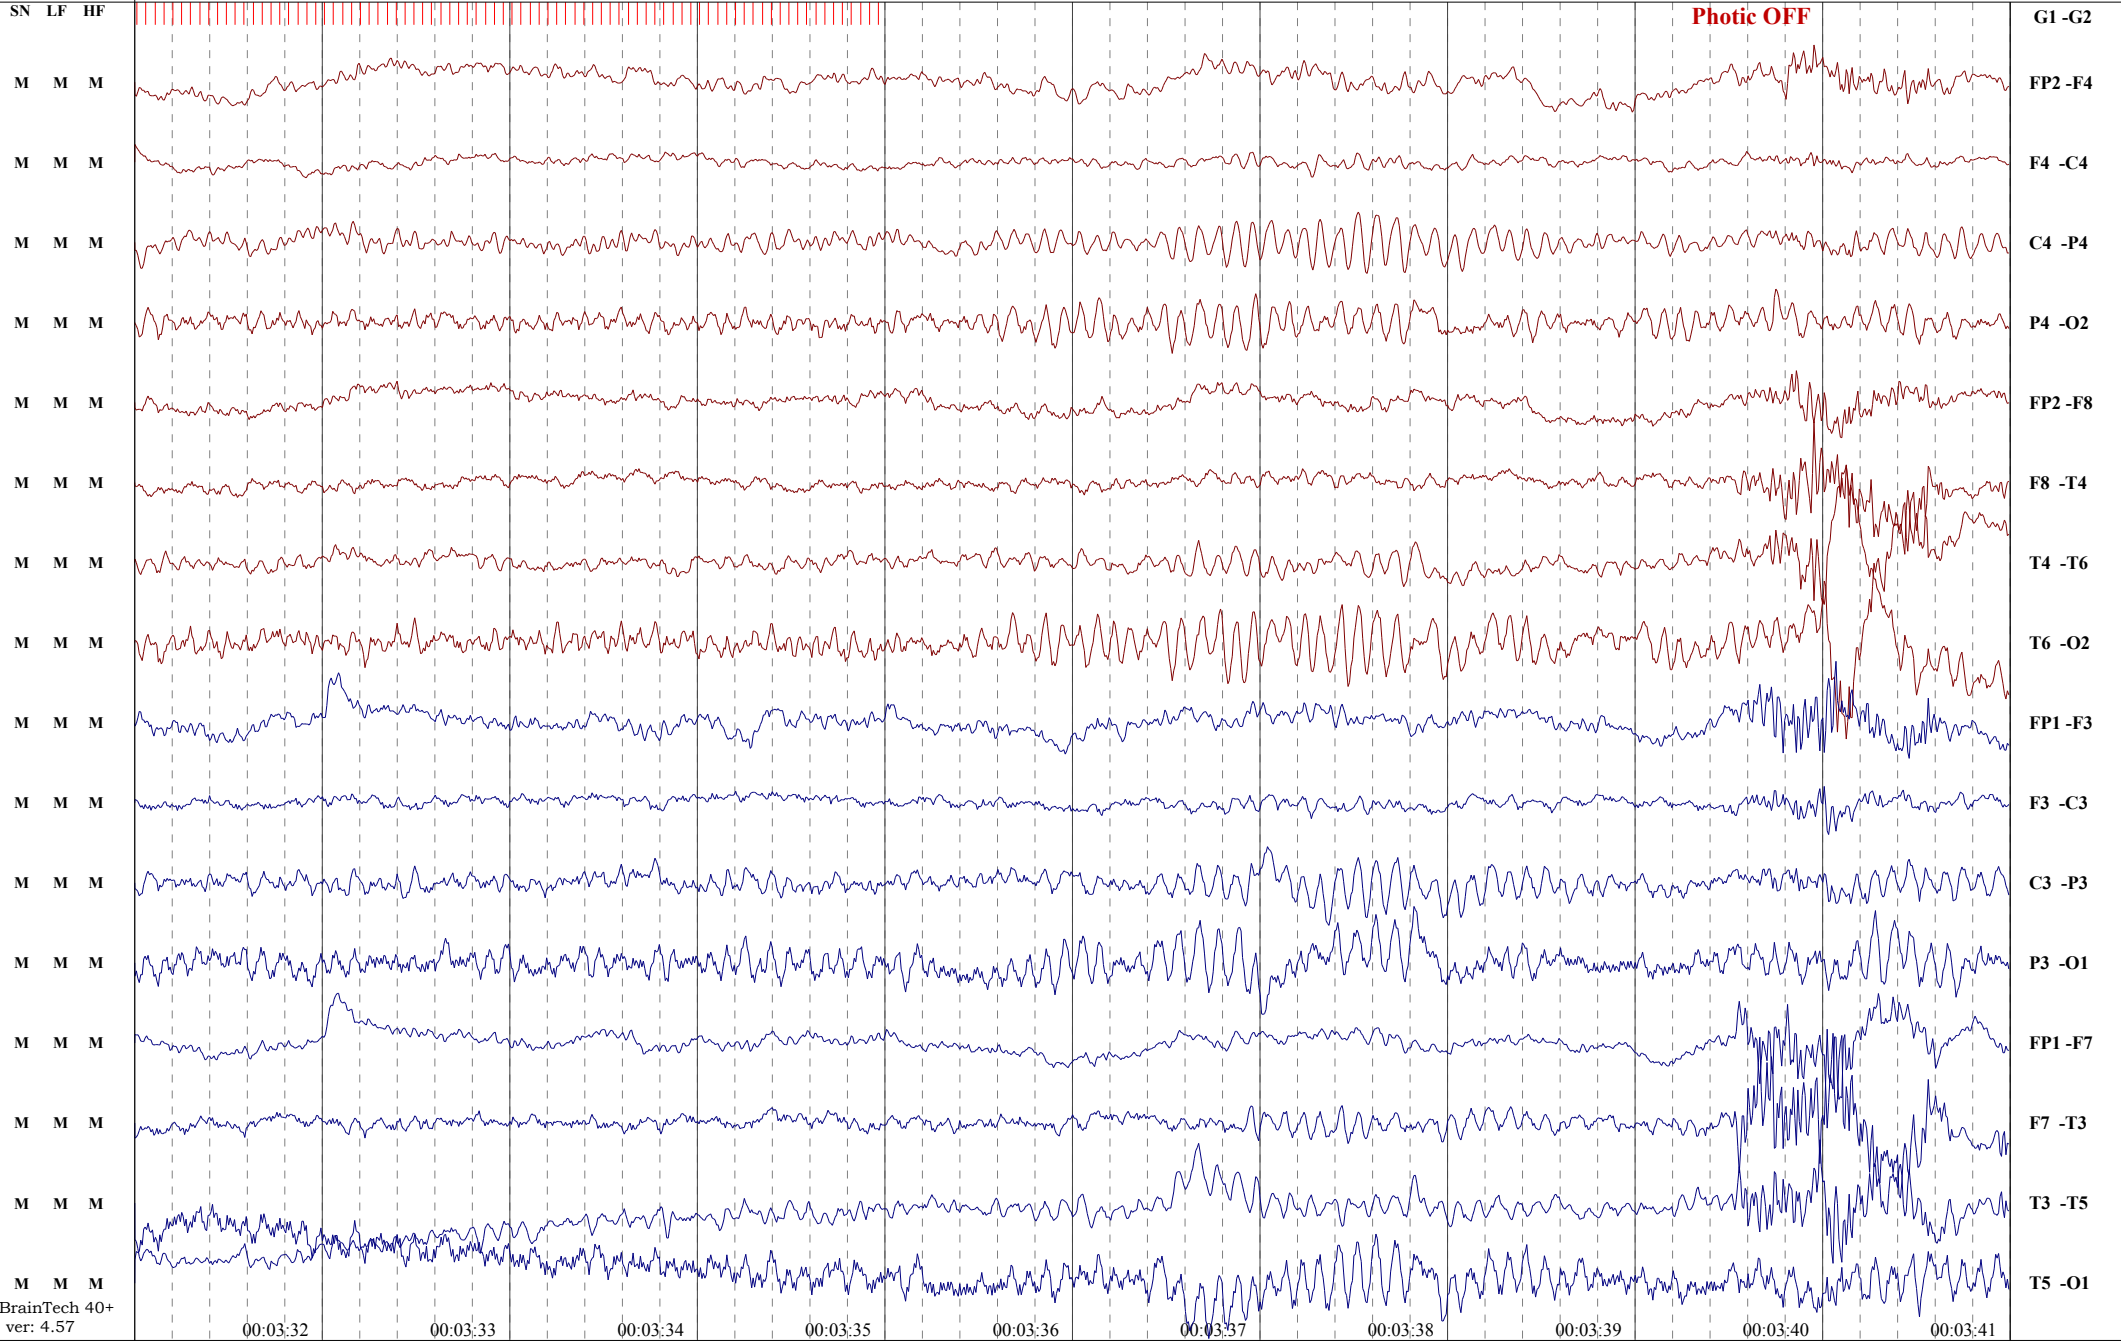



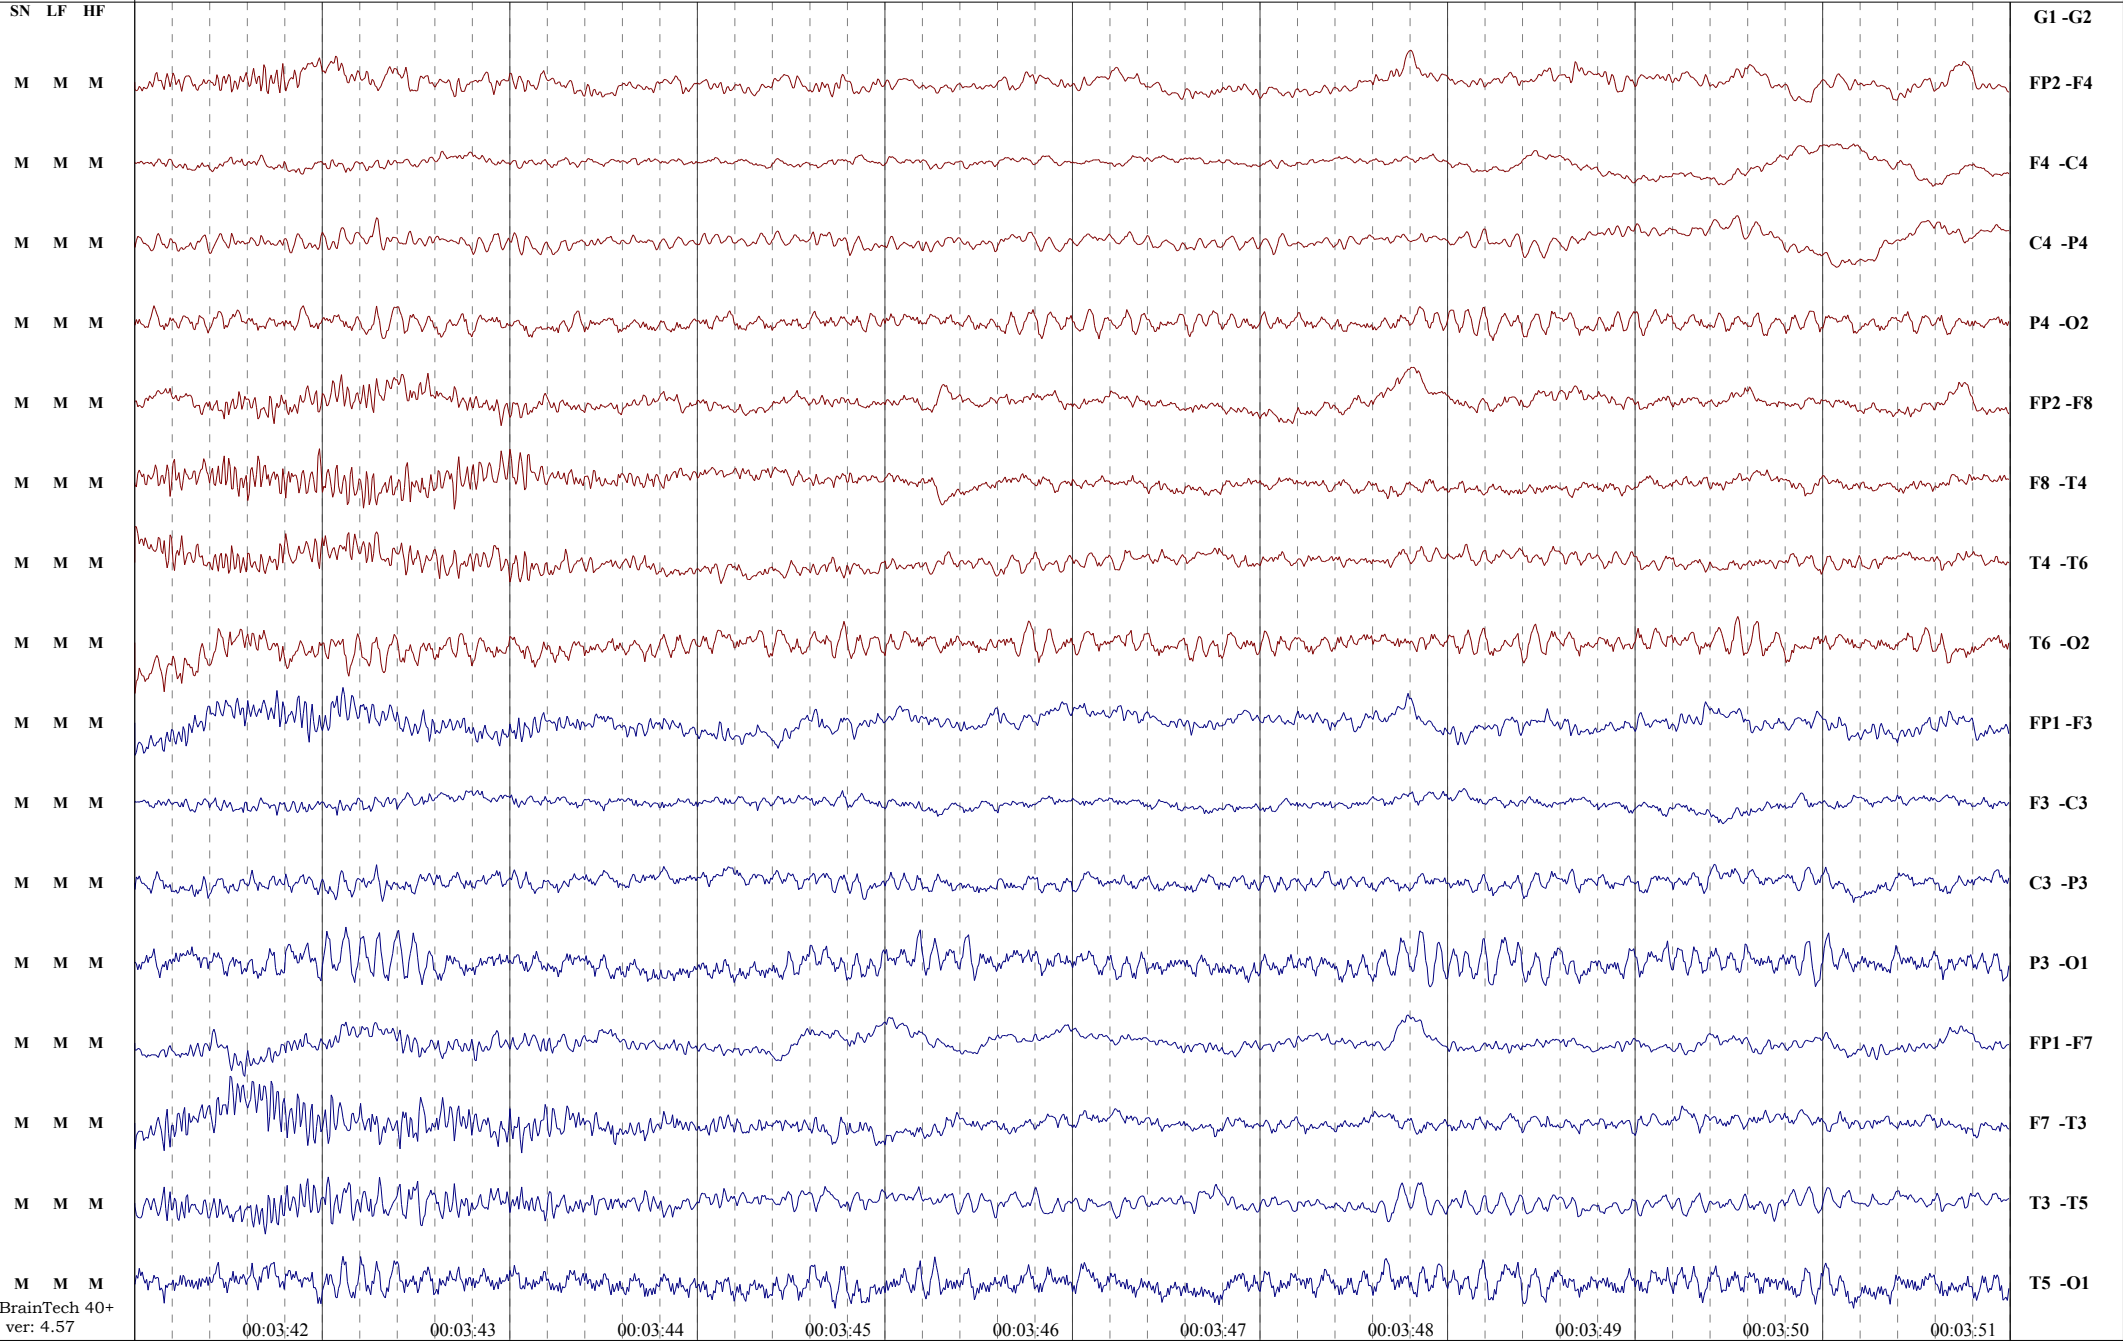


26  
MISS. ASHWANI BORKAR  
21 Years/F

Date: 25-Jul-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:45:21  
Page:24/28  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

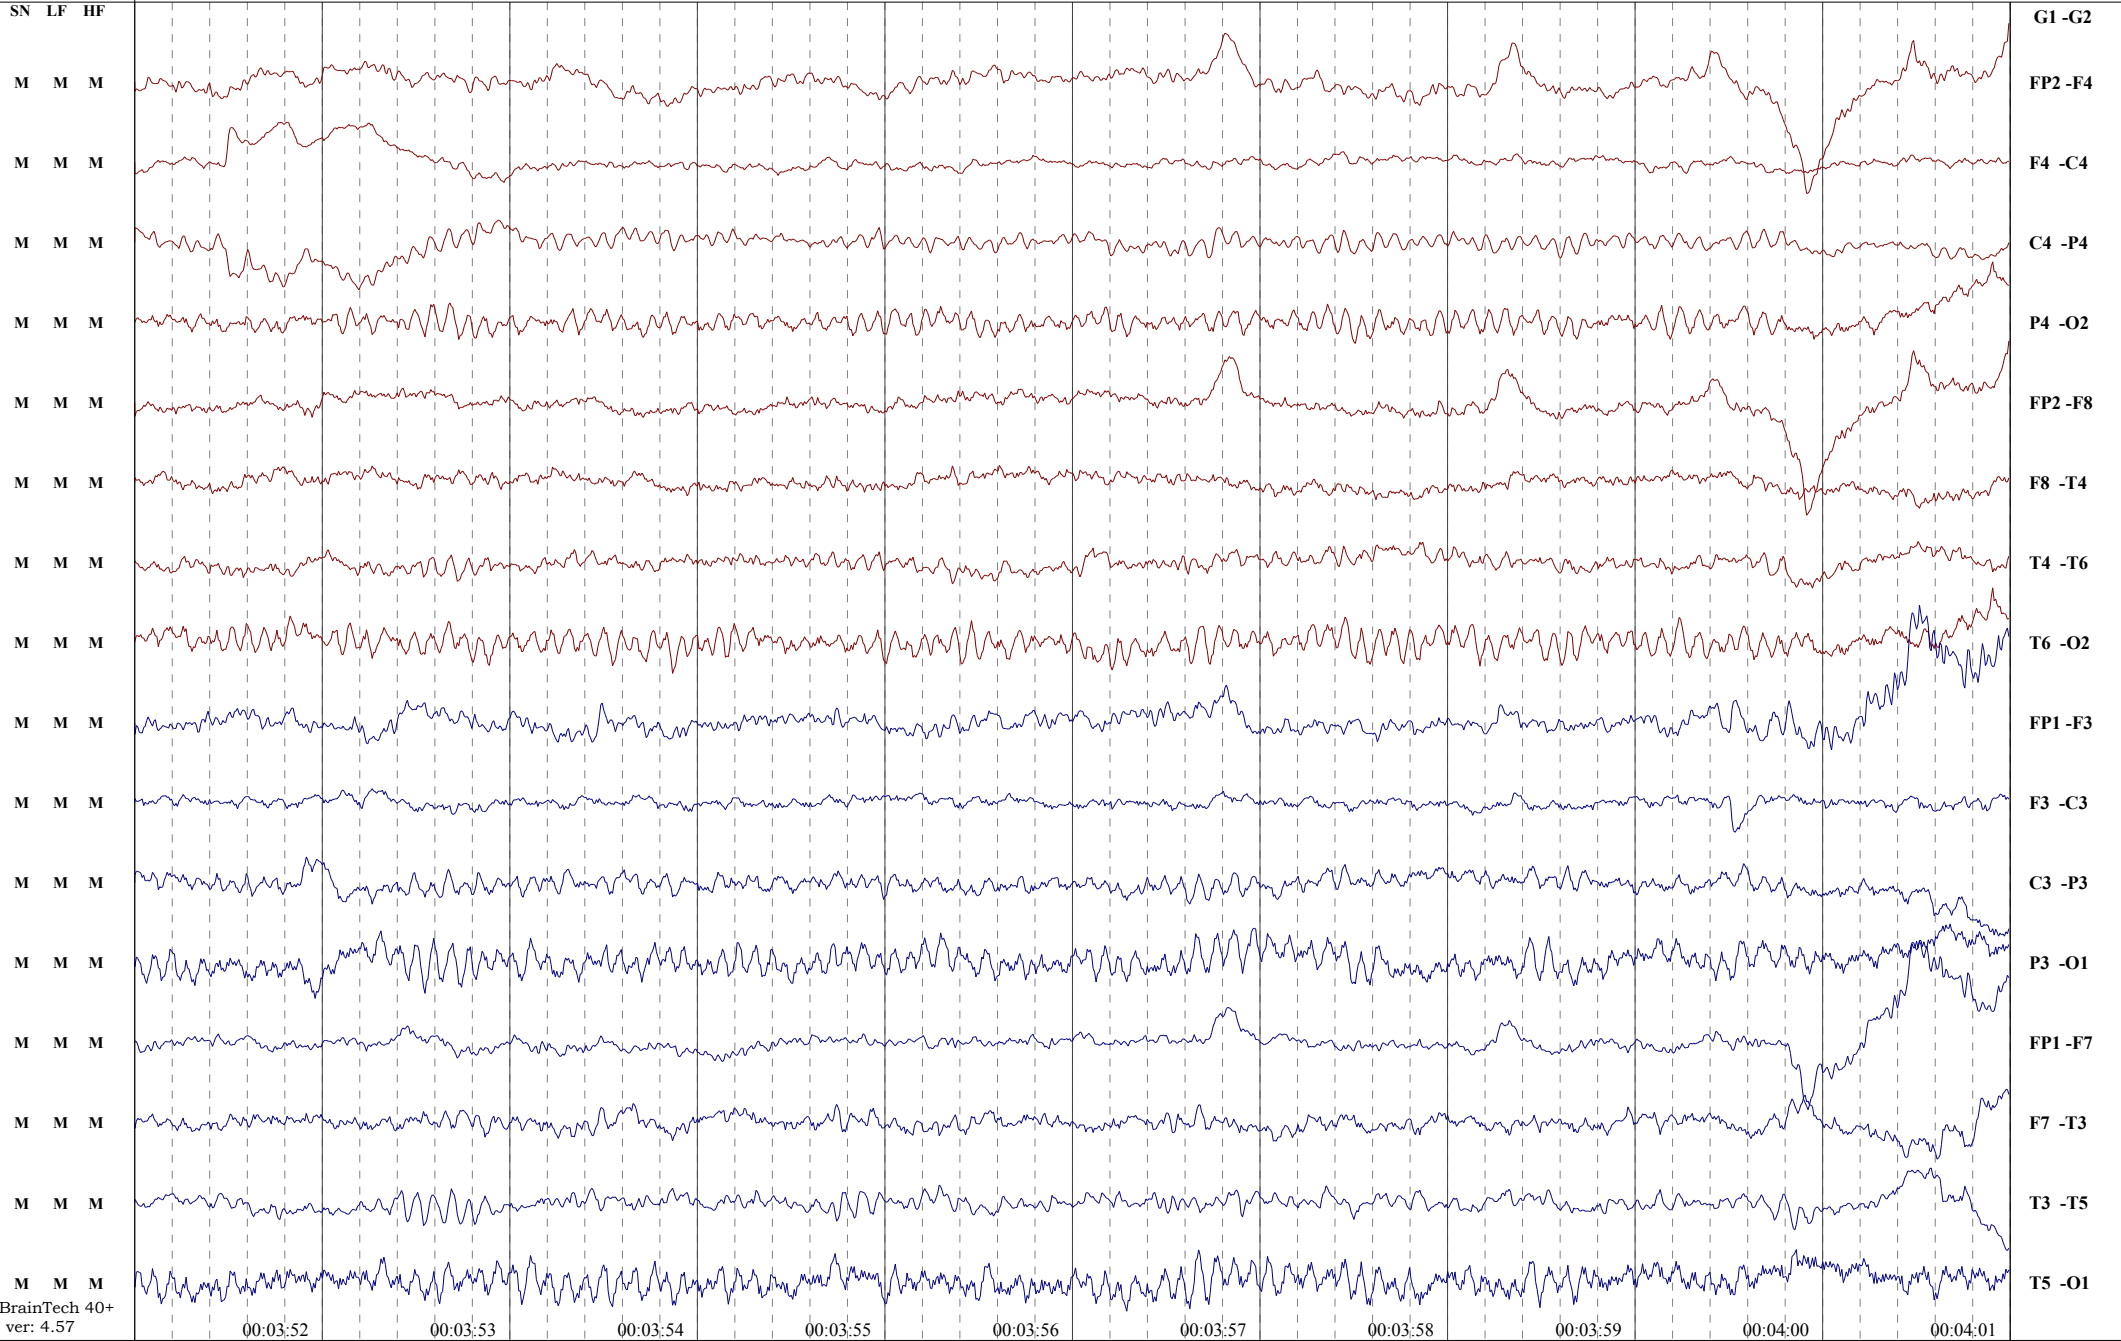


26  
MISS. ASHWANI BORKAR  
21 Years/F

Date: 25-Jul-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:45:31  
Page:25/28  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

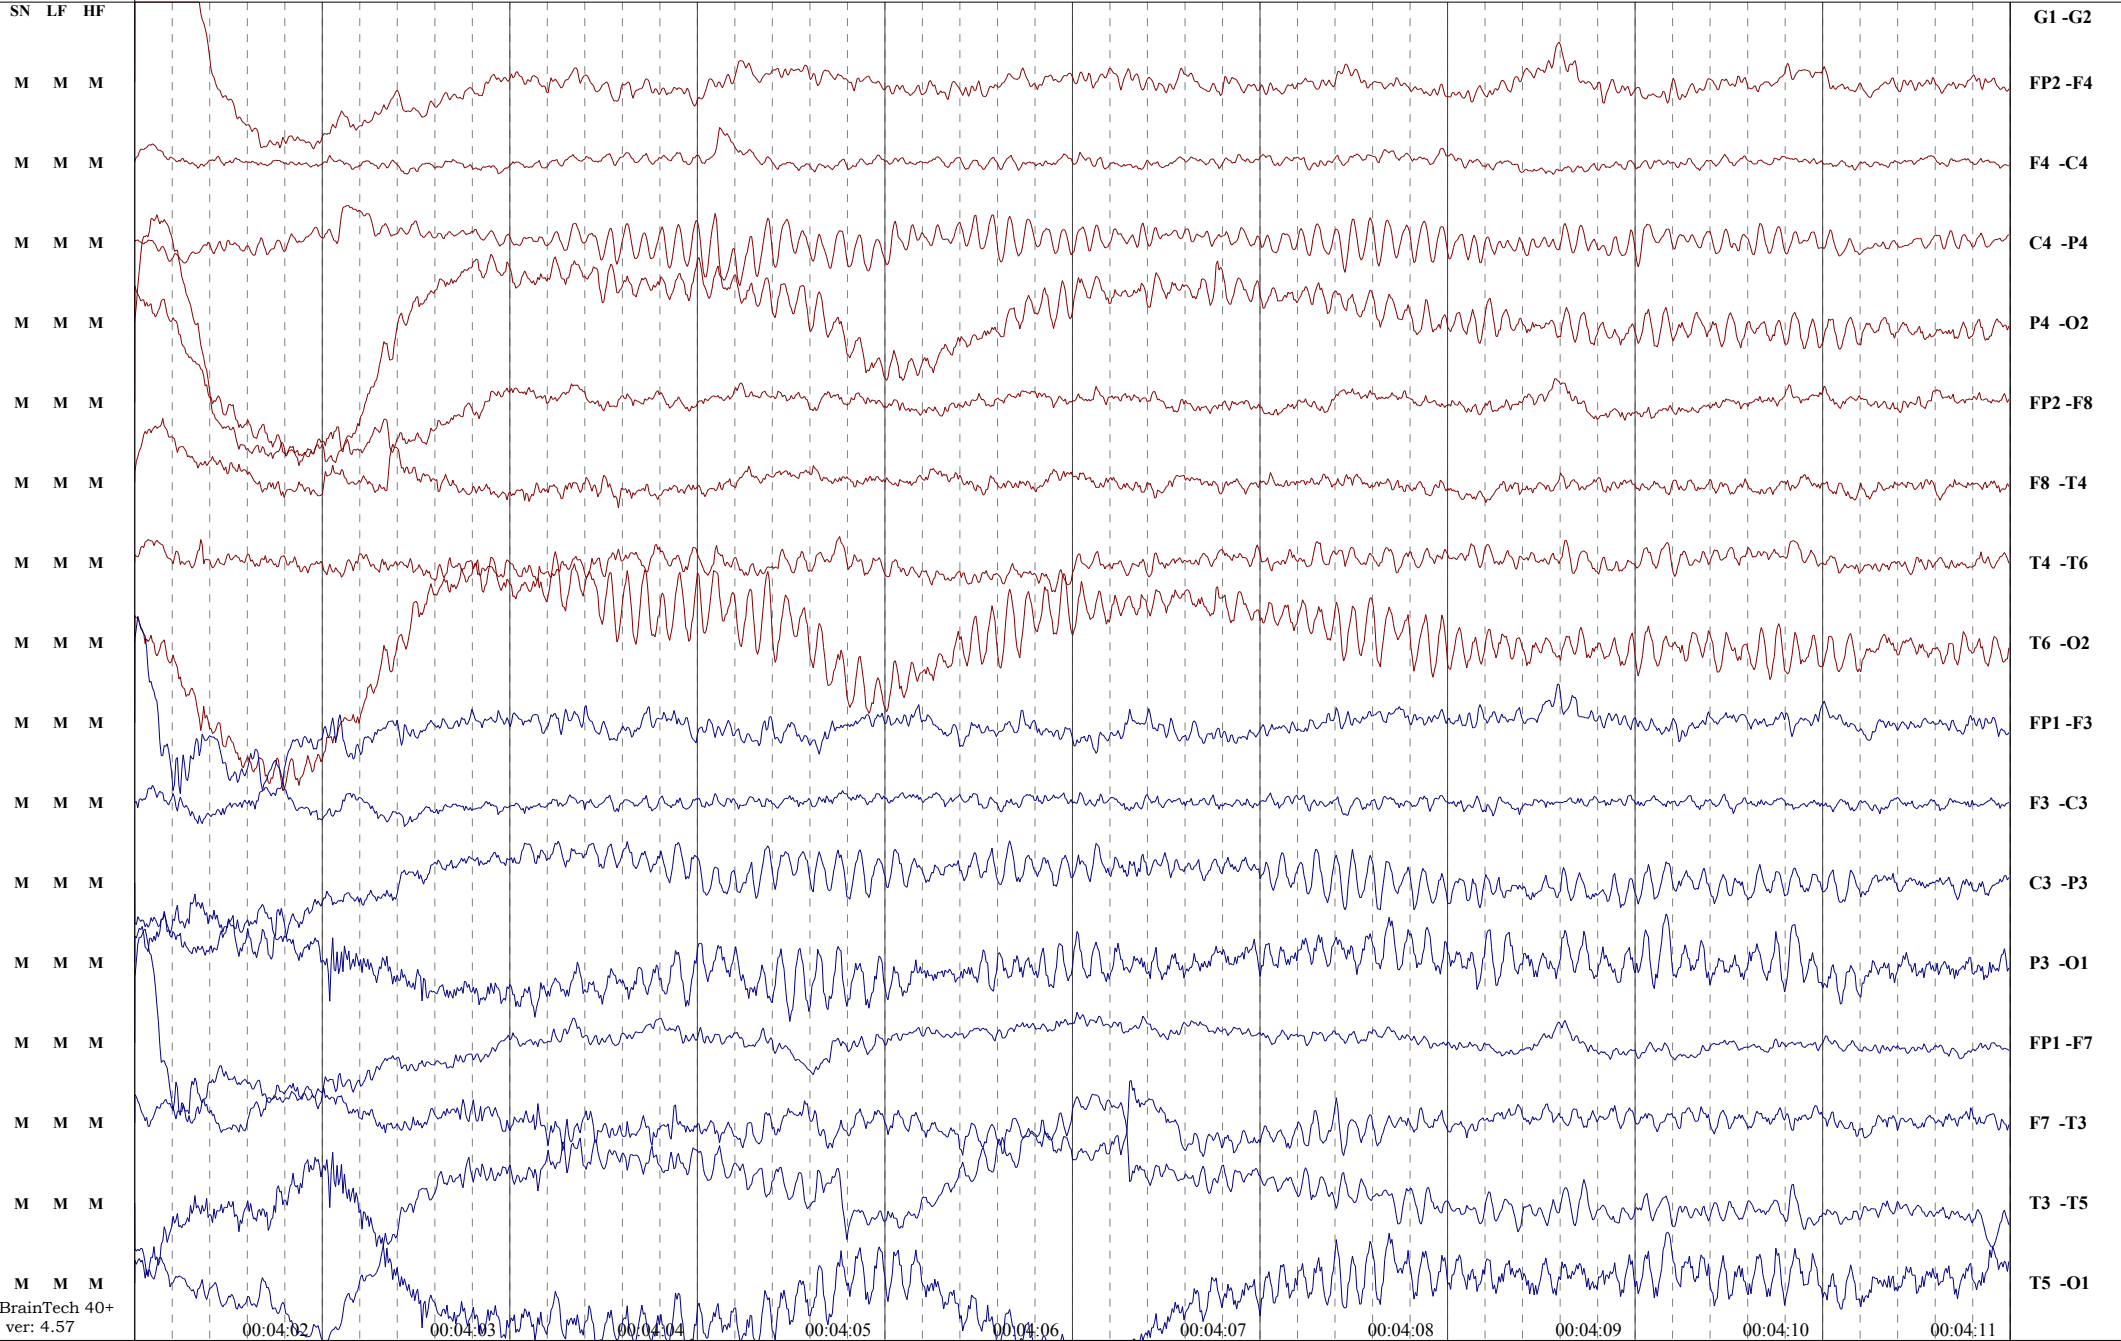


26  
MISS. ASHWANI BORKAR  
21 Years/F

Date: 25-Jul-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:45:41  
Page:26/28  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

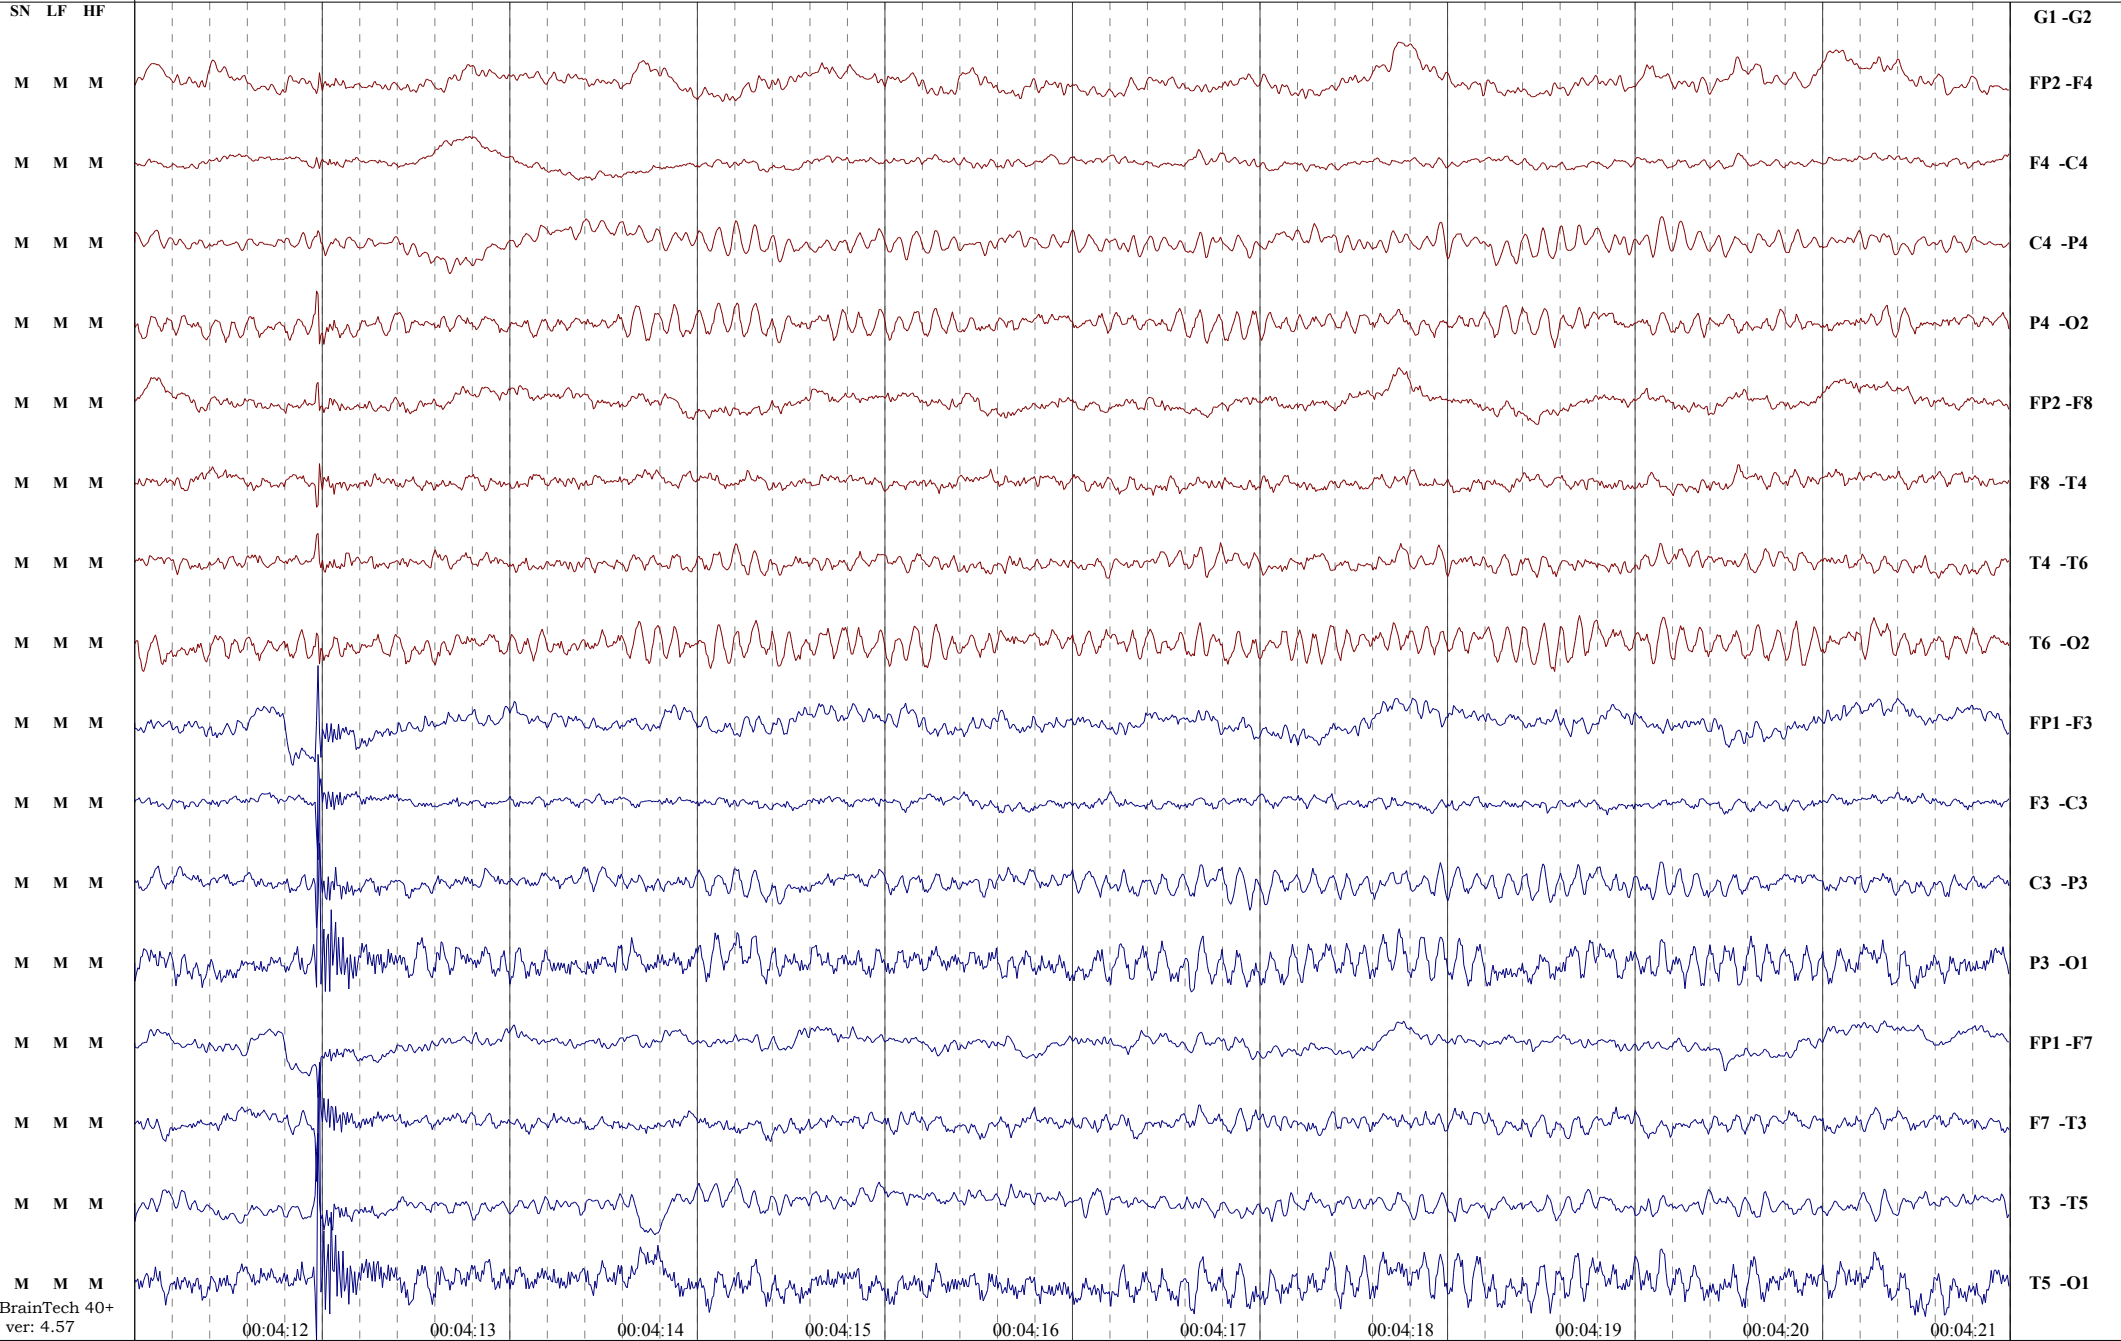



26  
MISS. ASHWANI BORKAR  
21 Years/F

Date: 25-Jul-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:45:51  
Page:27/28  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

