


139
MAST. YAMAN PATEL
12 Years/M

Date: 13-Sep-2023
Type: ANALYSIS
BIPOLAR LONGITUDNAL

Speed : 30 mm/S
Sen : 7.5 uV/mm
Filter : 1 Hz - 70 Hz

Time: 16:40:45
Page:1/25
Notch: ON

Ref:DR. RAJNISH PANDEY
Dr. : DR. VIJENDRA PAINKARA
Tech:

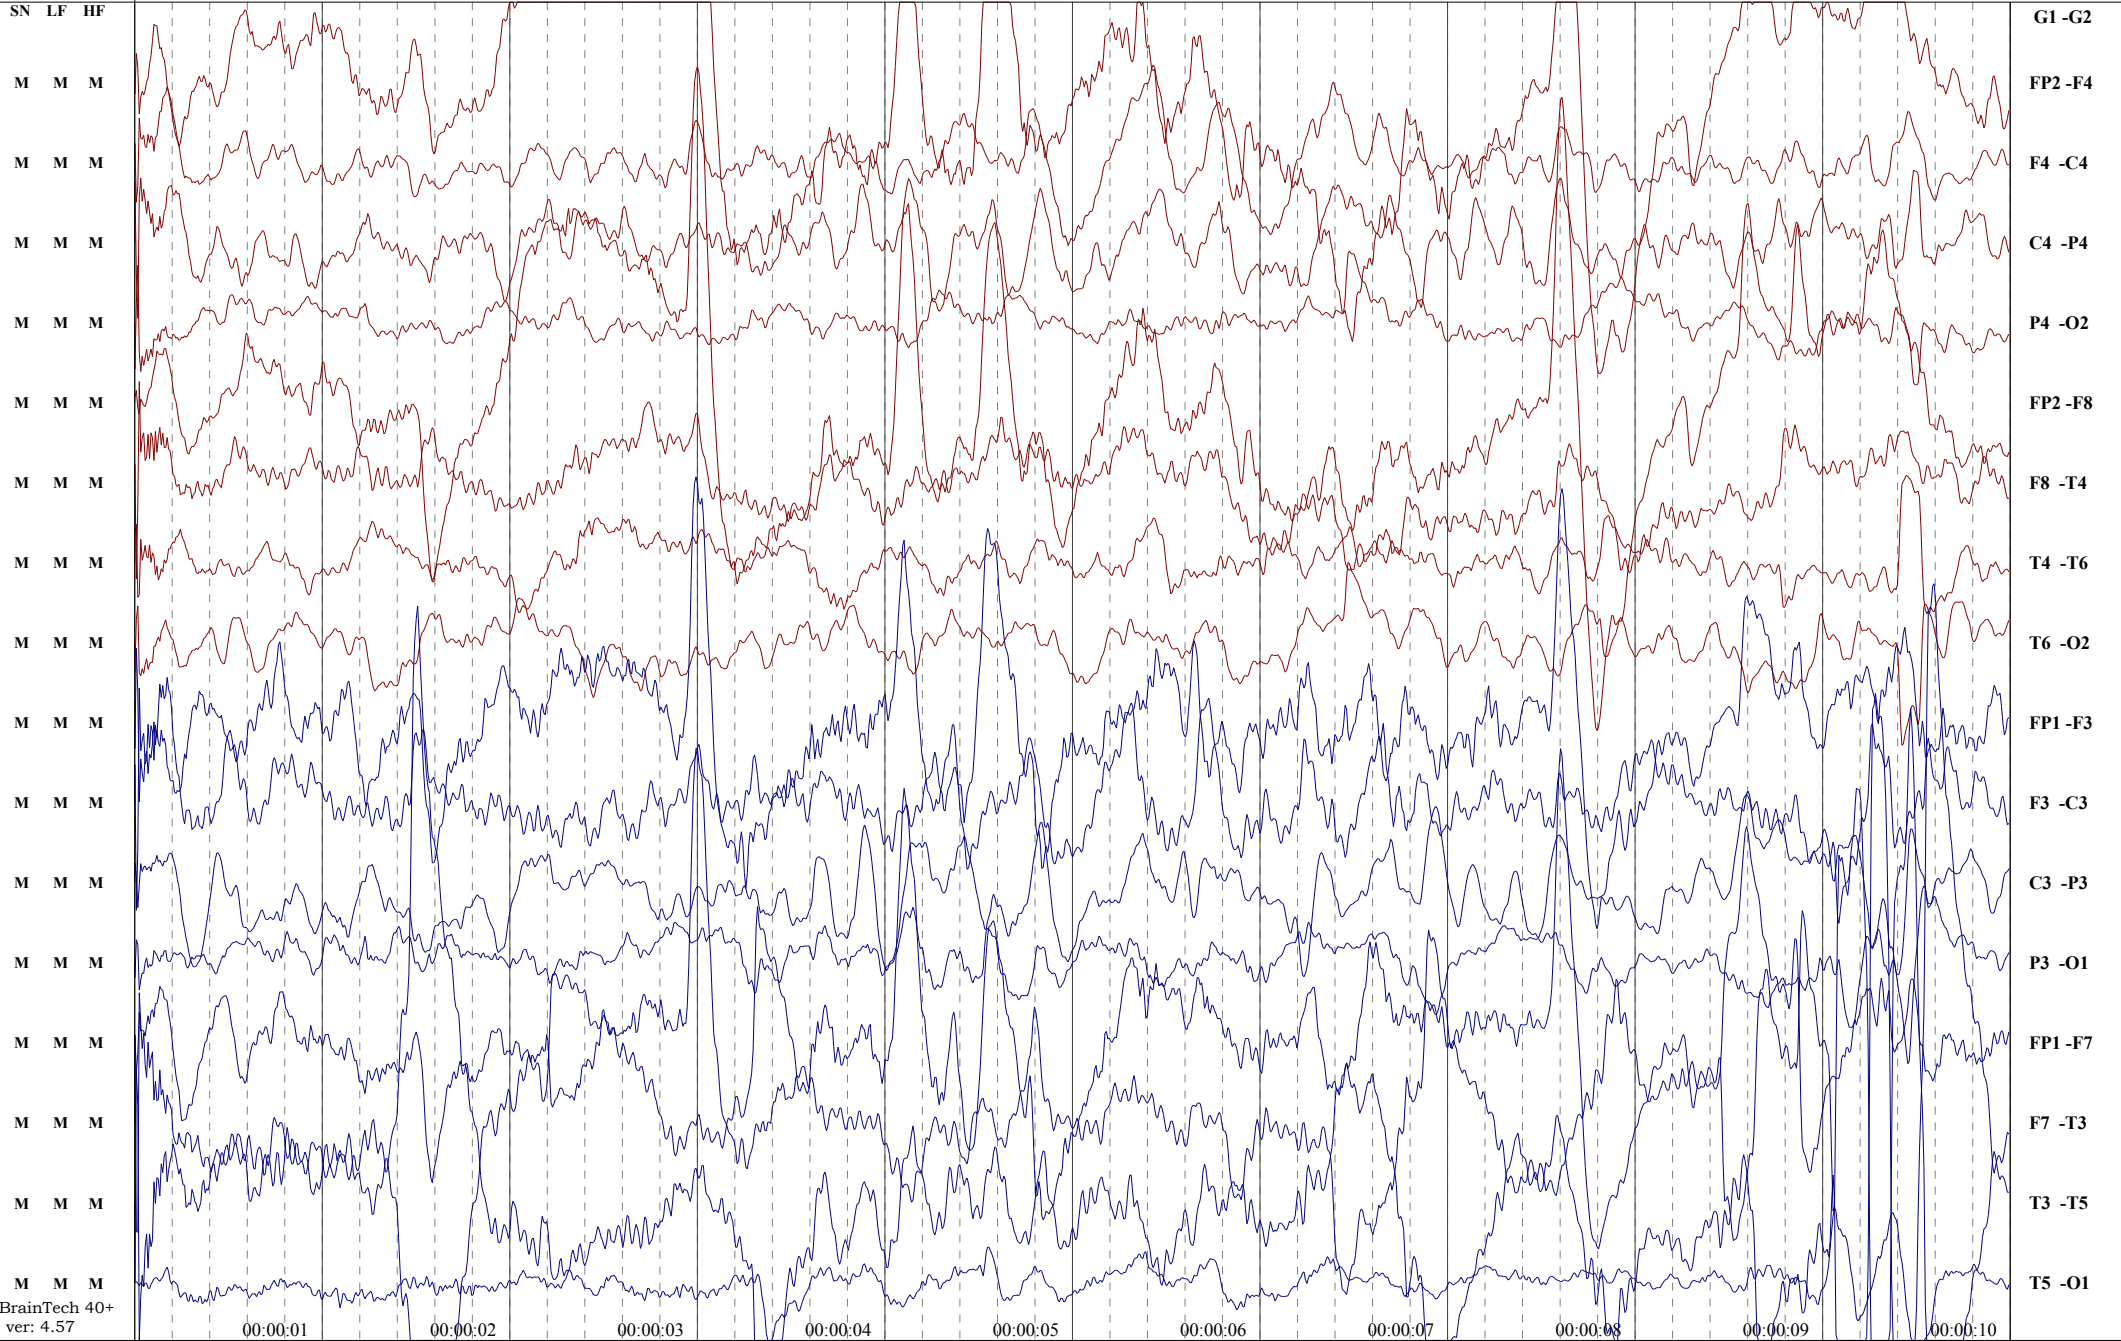


139
MAST. YAMAN PATEL
12 Years/M

Date: 13-Sep-2023
Type: ANALYSIS
BIPOLAR LONGITUDNAL

Speed : 30 mm/S
Sen : 7.5 uV/mm
Filter : 1 Hz - 70 Hz

Time: 16:40:55
Page:2/25
Notch: ON

Ref:DR. RAJNISH PANDEY
Dr. : DR. VIJENDRA PAINKARA
Tech:

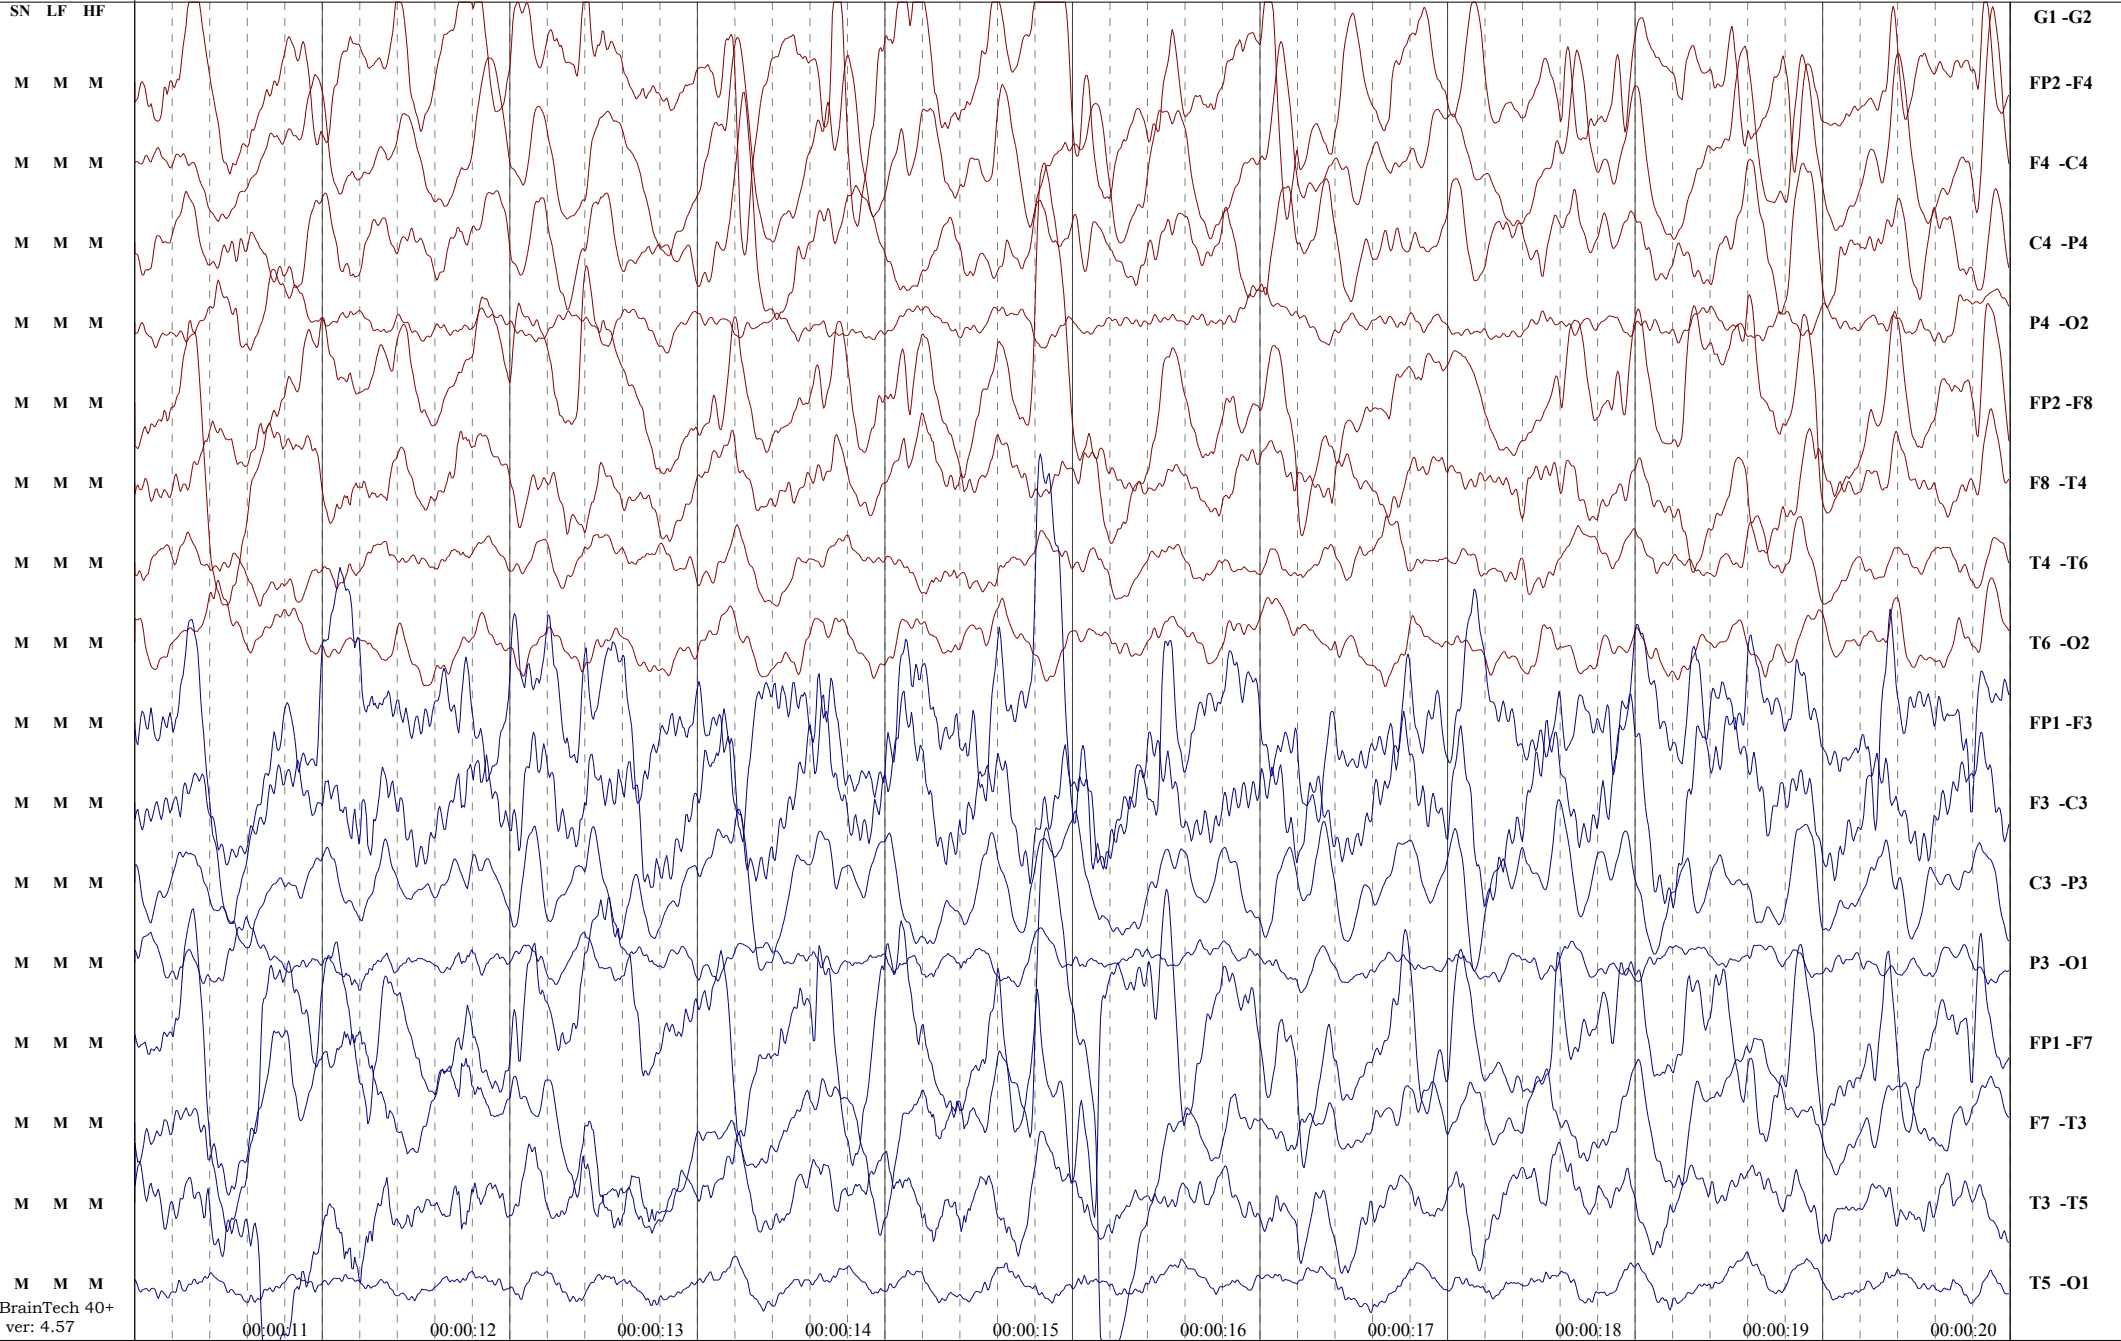


139
MAST. YAMAN PATEL
12 Years/M

Date: 13-Sep-2023
Type: ANALYSIS
BIPOLAR LONGITUDNAL

Speed : 30 mm/S
Sen : 7.5 uV/mm
Filter : 1 Hz - 70 Hz

Time: 16:41:05
Page:3/25
Notch: ON

Ref:DR. RAJNISH PANDEY
Dr. : DR. VIJENDRA PAINKARA
Tech:

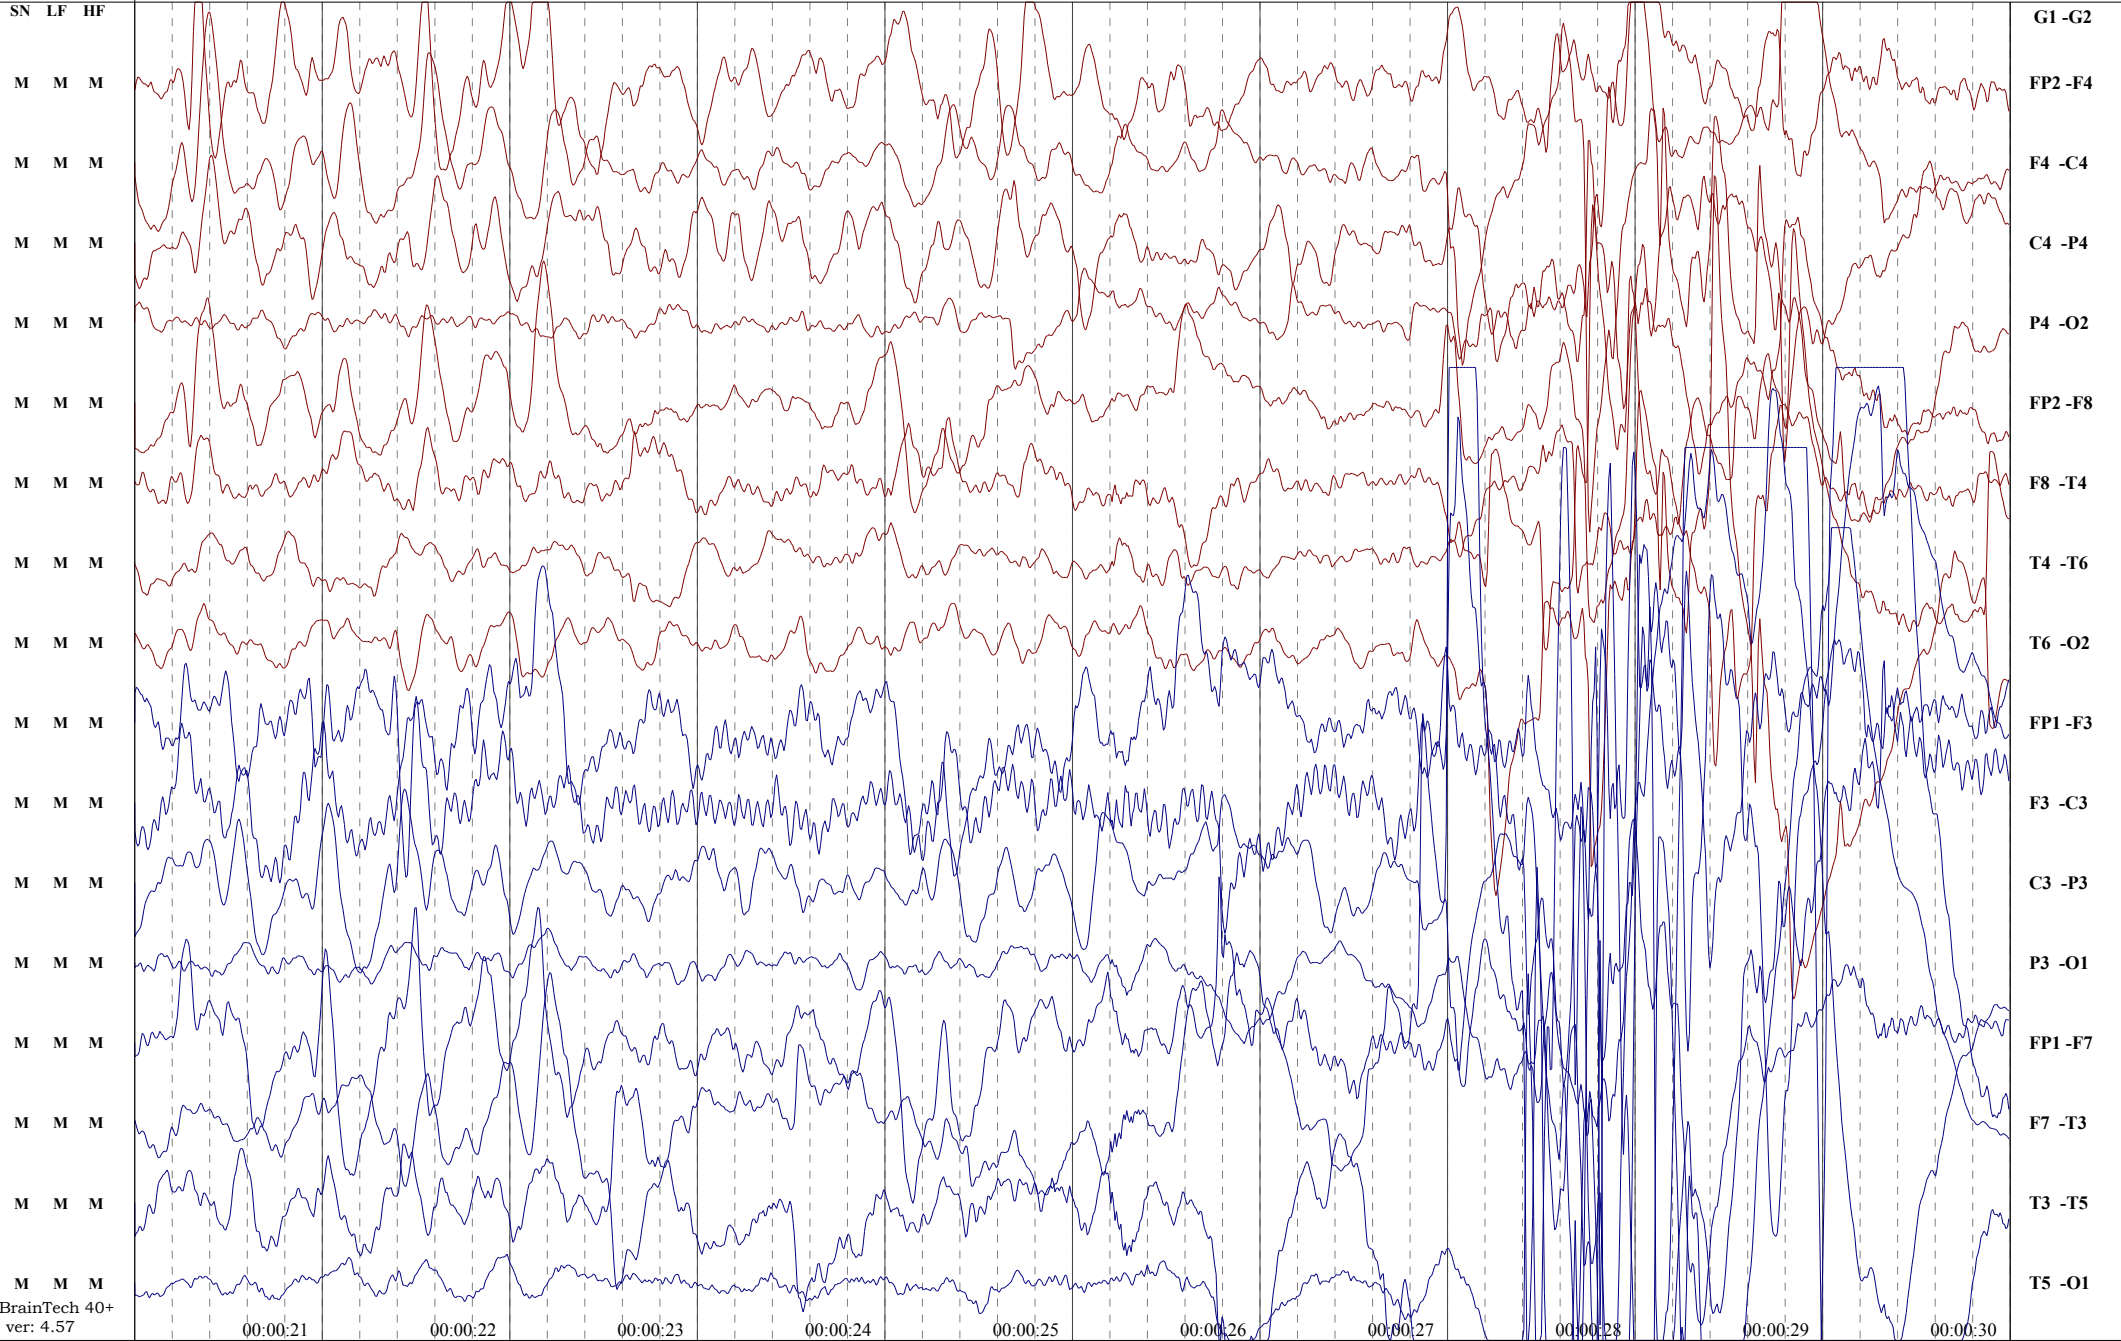


139
MAST. YAMAN PATEL
12 Years/M

Date: 13-Sep-2023
Type: ANALYSIS
BIPOLAR LONGITUDNAL

Speed : 30 mm/S
Sen : 7.5 uV/mm
Filter : 1 Hz - 70 Hz

Time: 16:41:15
Page:4/25
Notch: ON

Ref:DR. RAJNISH PANDEY
Dr. : DR. VIJENDRA PAINKARA
Tech:

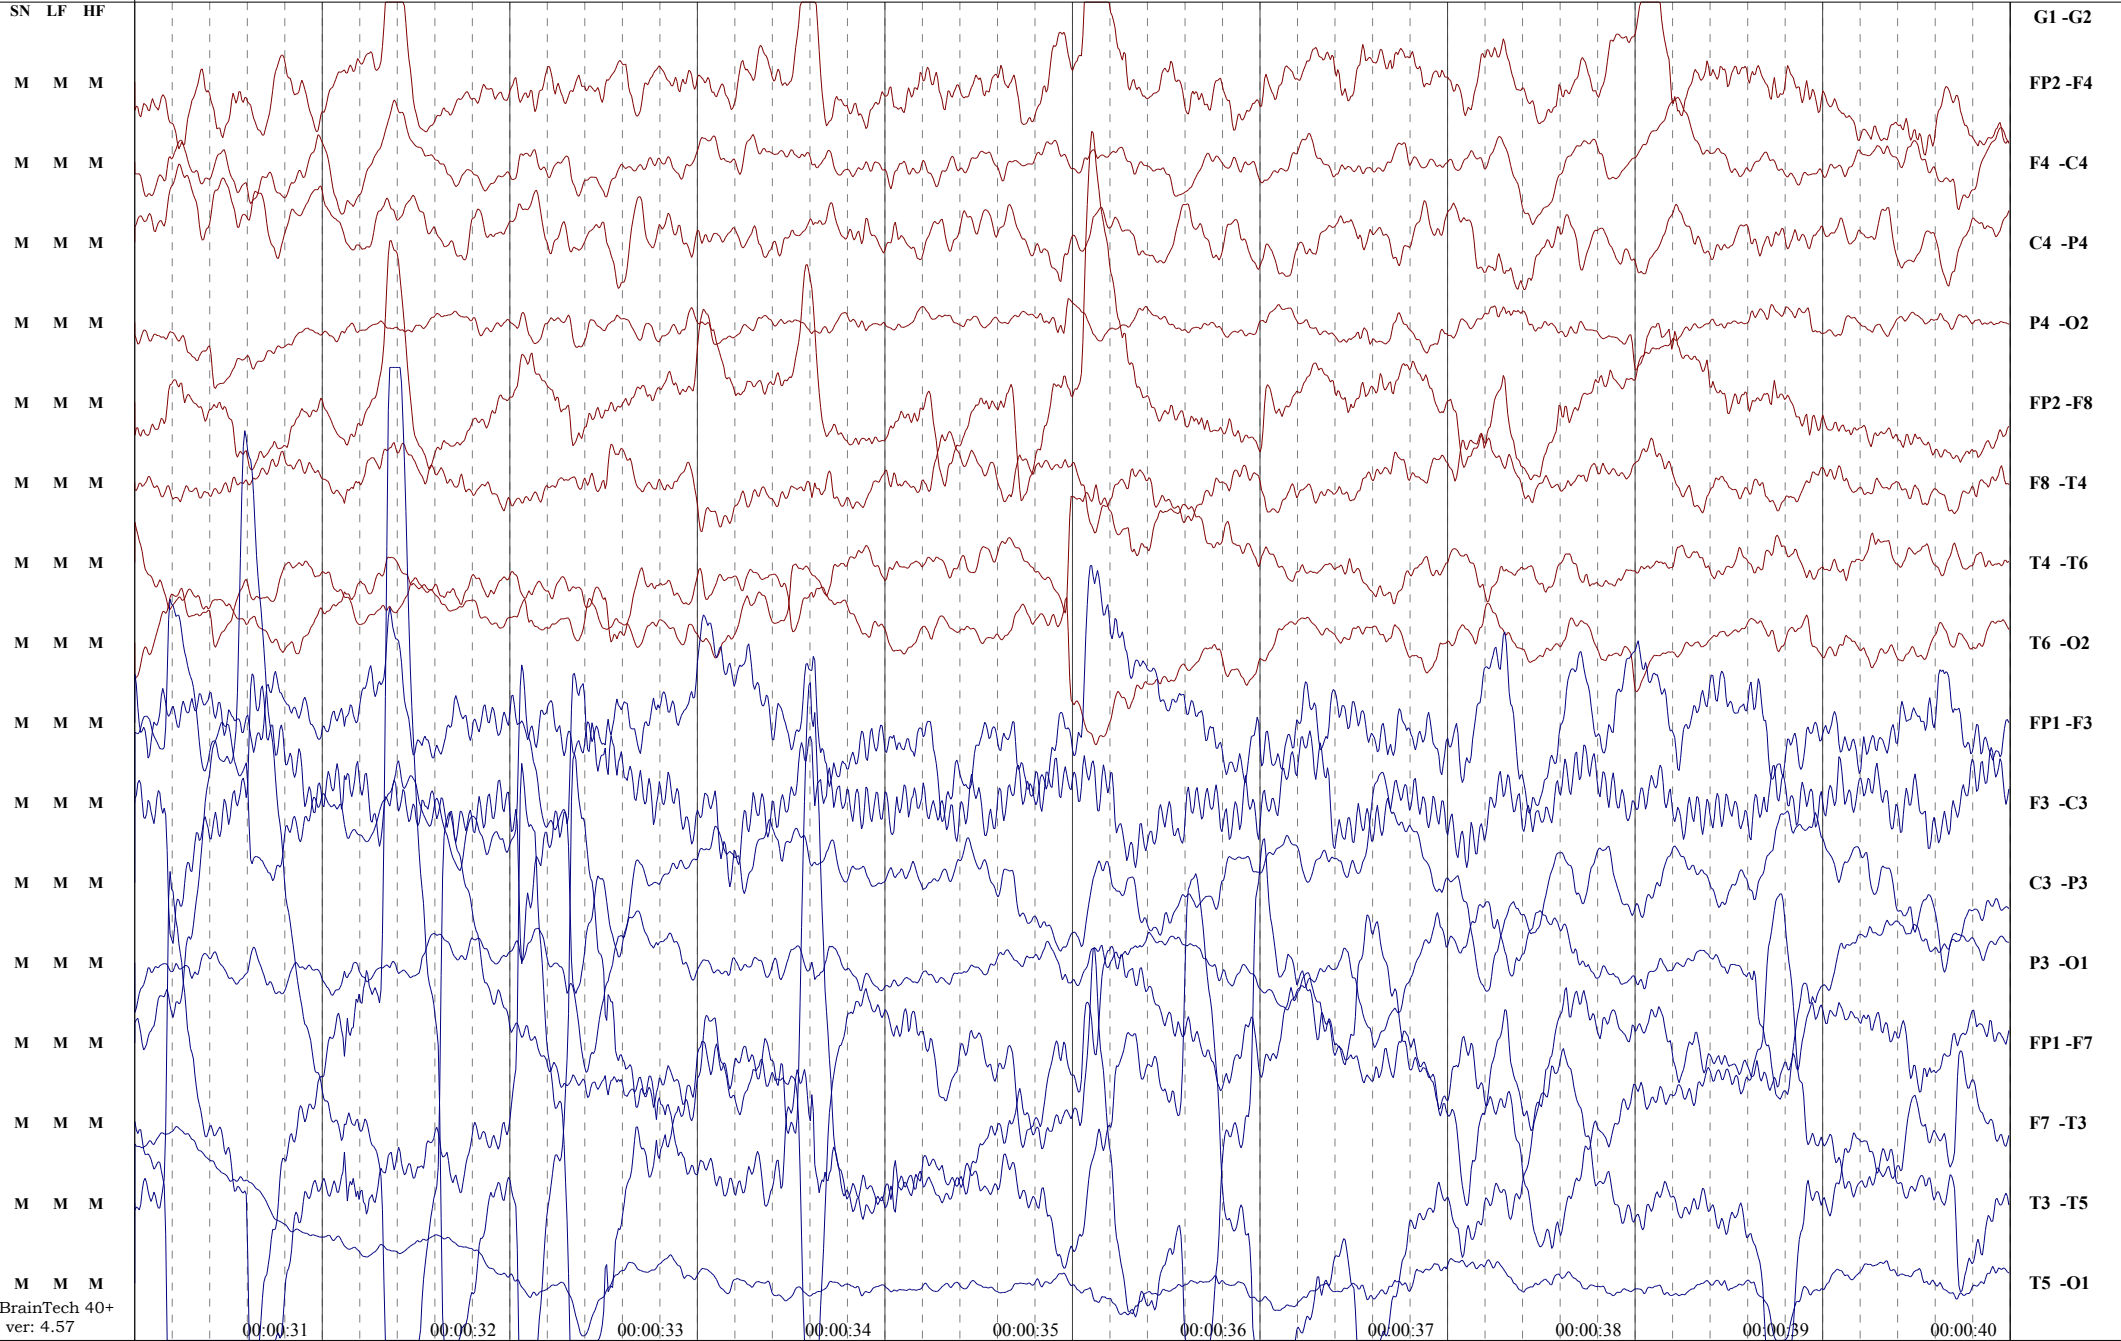


139
MAST. YAMAN PATEL
12 Years/M


Date: 13-Sep-2023
Type: ANALYSIS
BIPOLAR LONGITUDNAL


Speed : 30 mm/S
Sen : 7.5 uV/mm
Filter : 1 Hz - 70 Hz

Time: 16:41:25
Page:5/25
Notch: ON

Ref:DR. RAJNISH PANDEY
Dr. : DR. VIJENDRA PAINKARA
Tech:

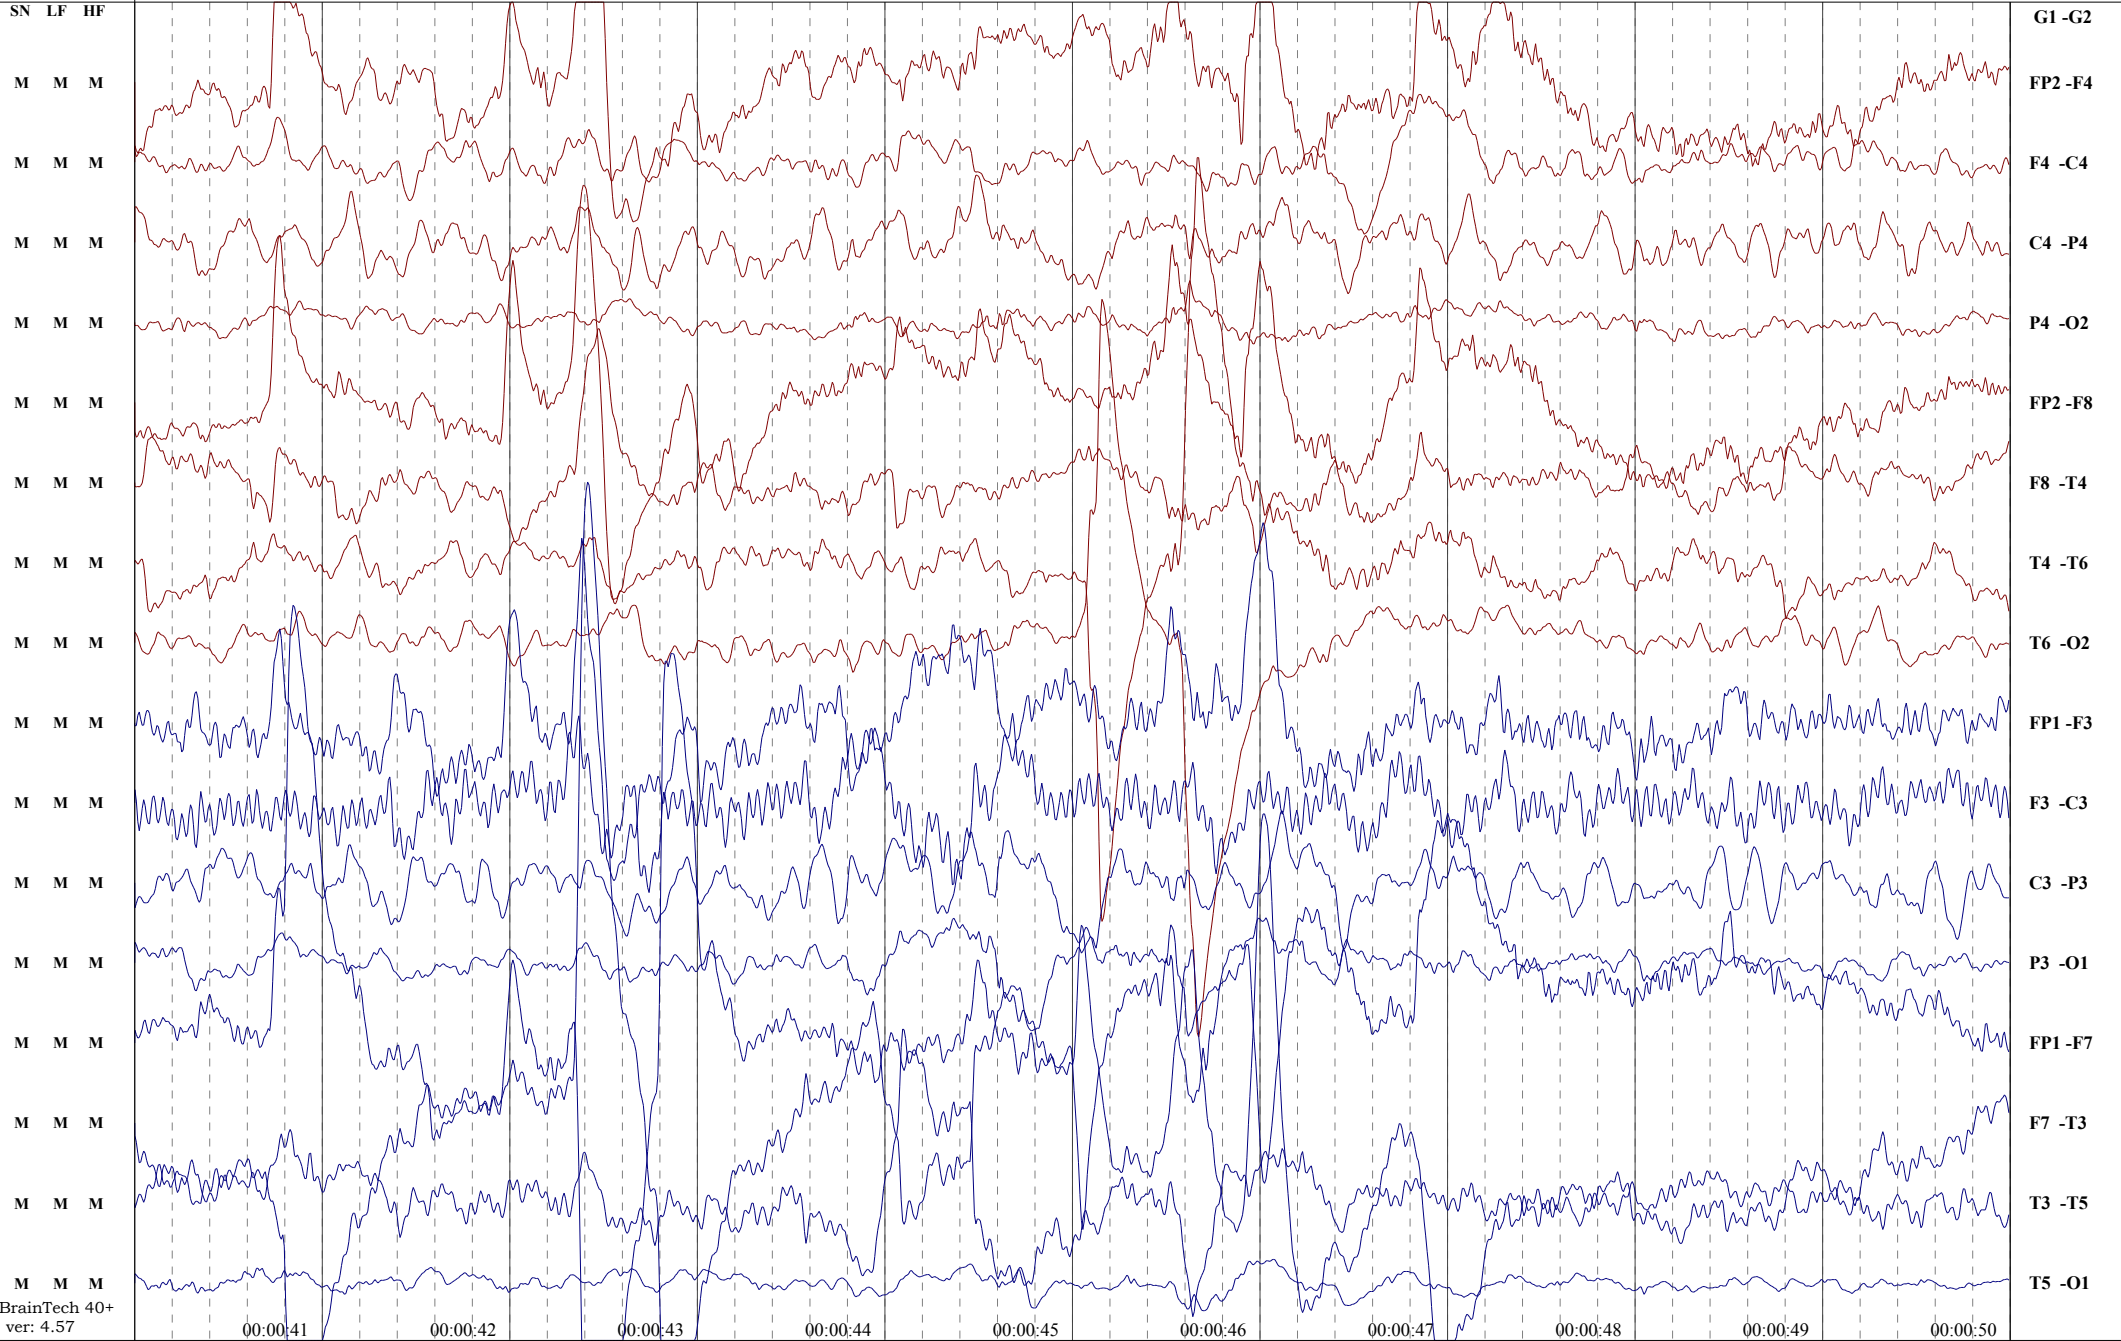

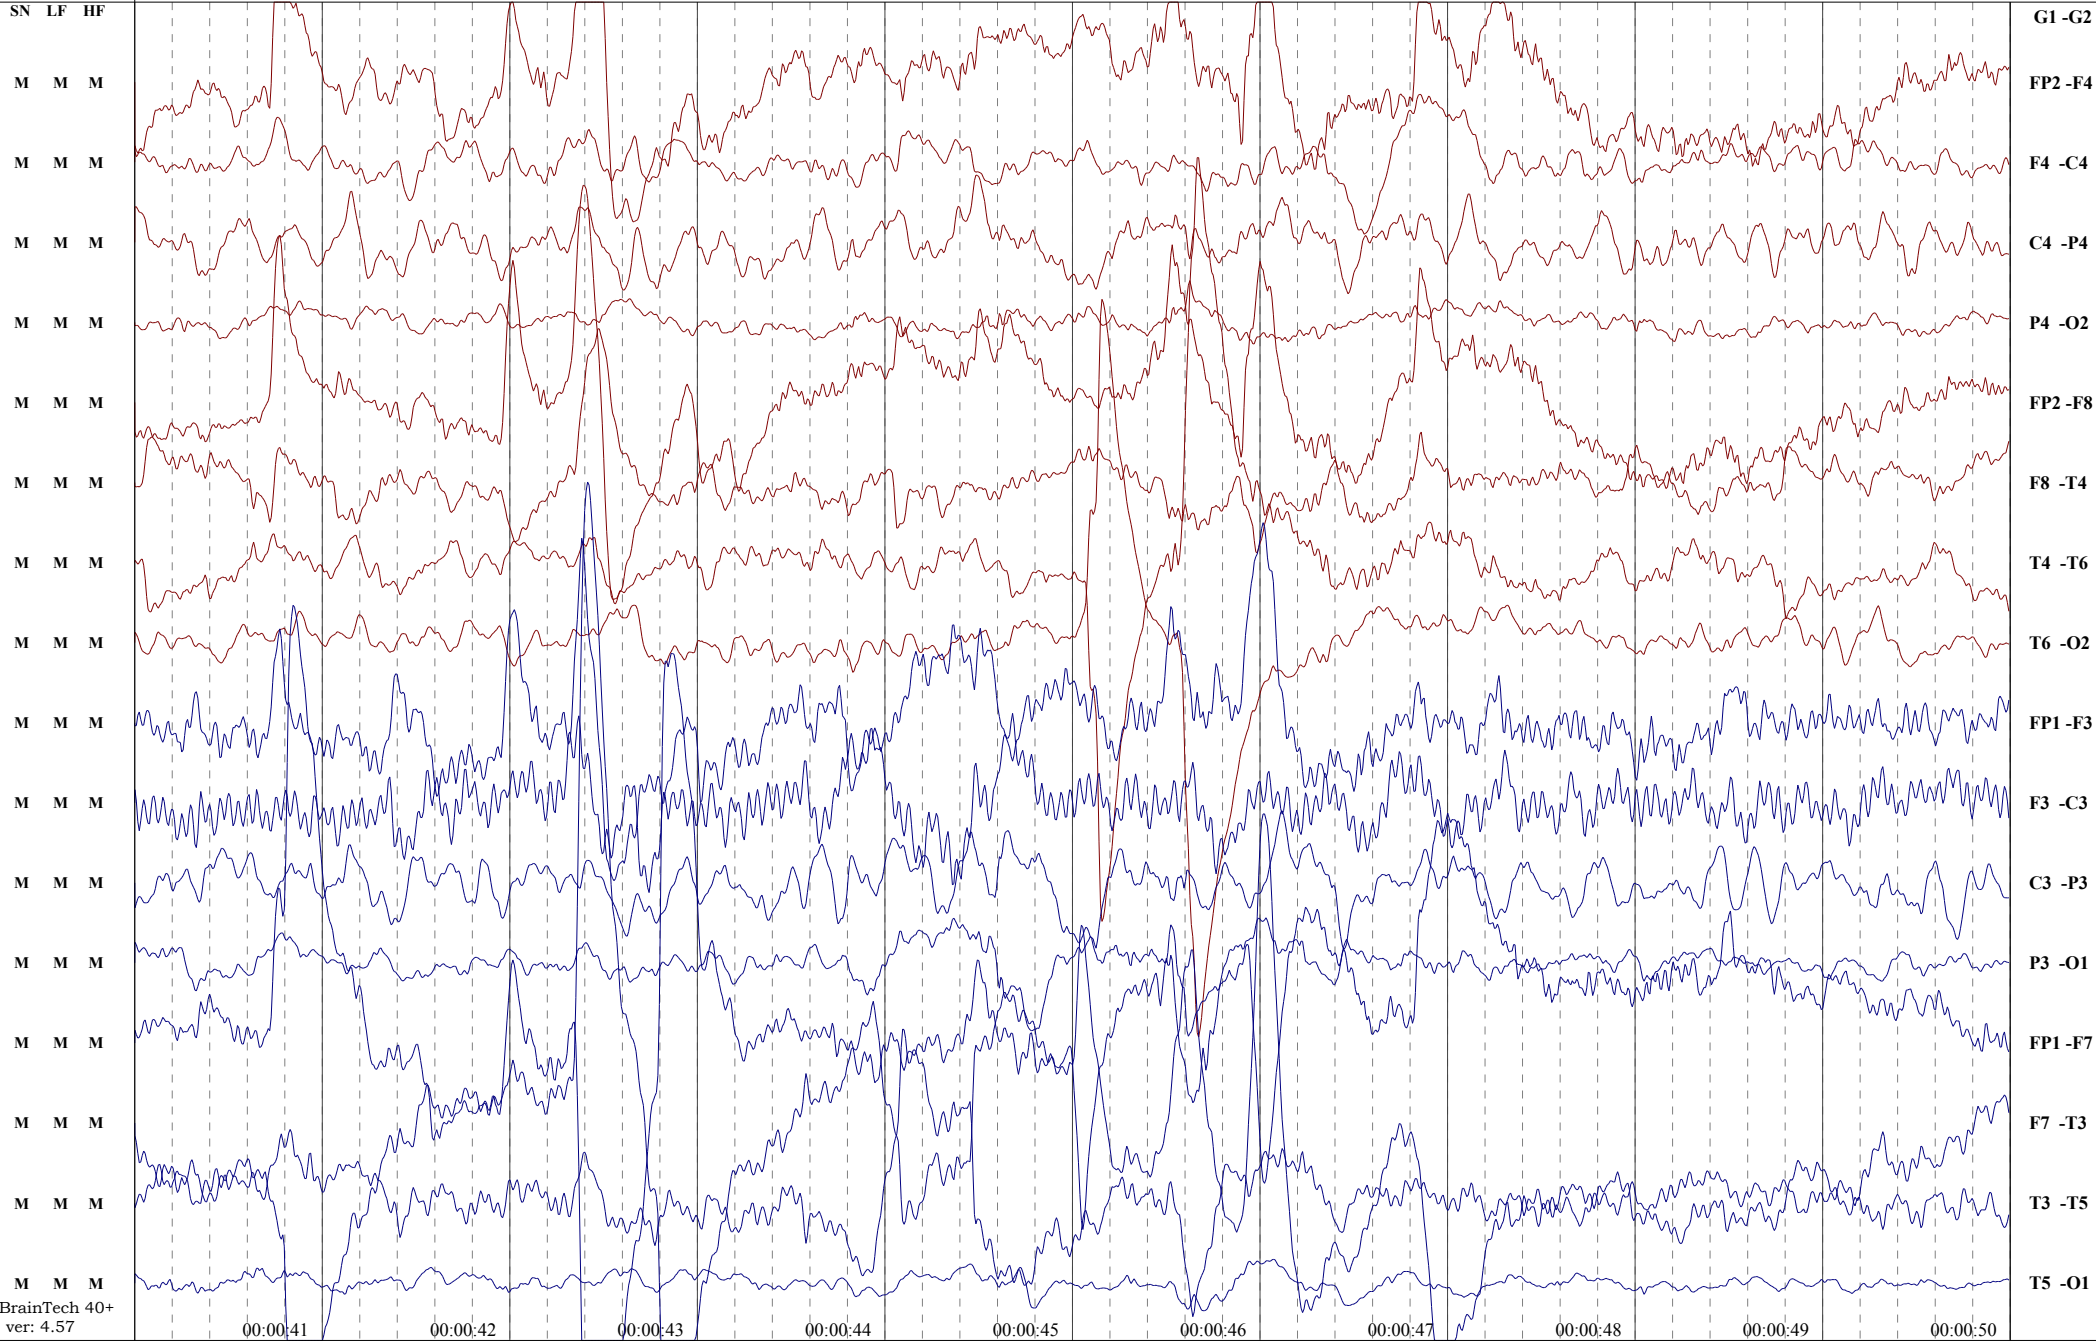

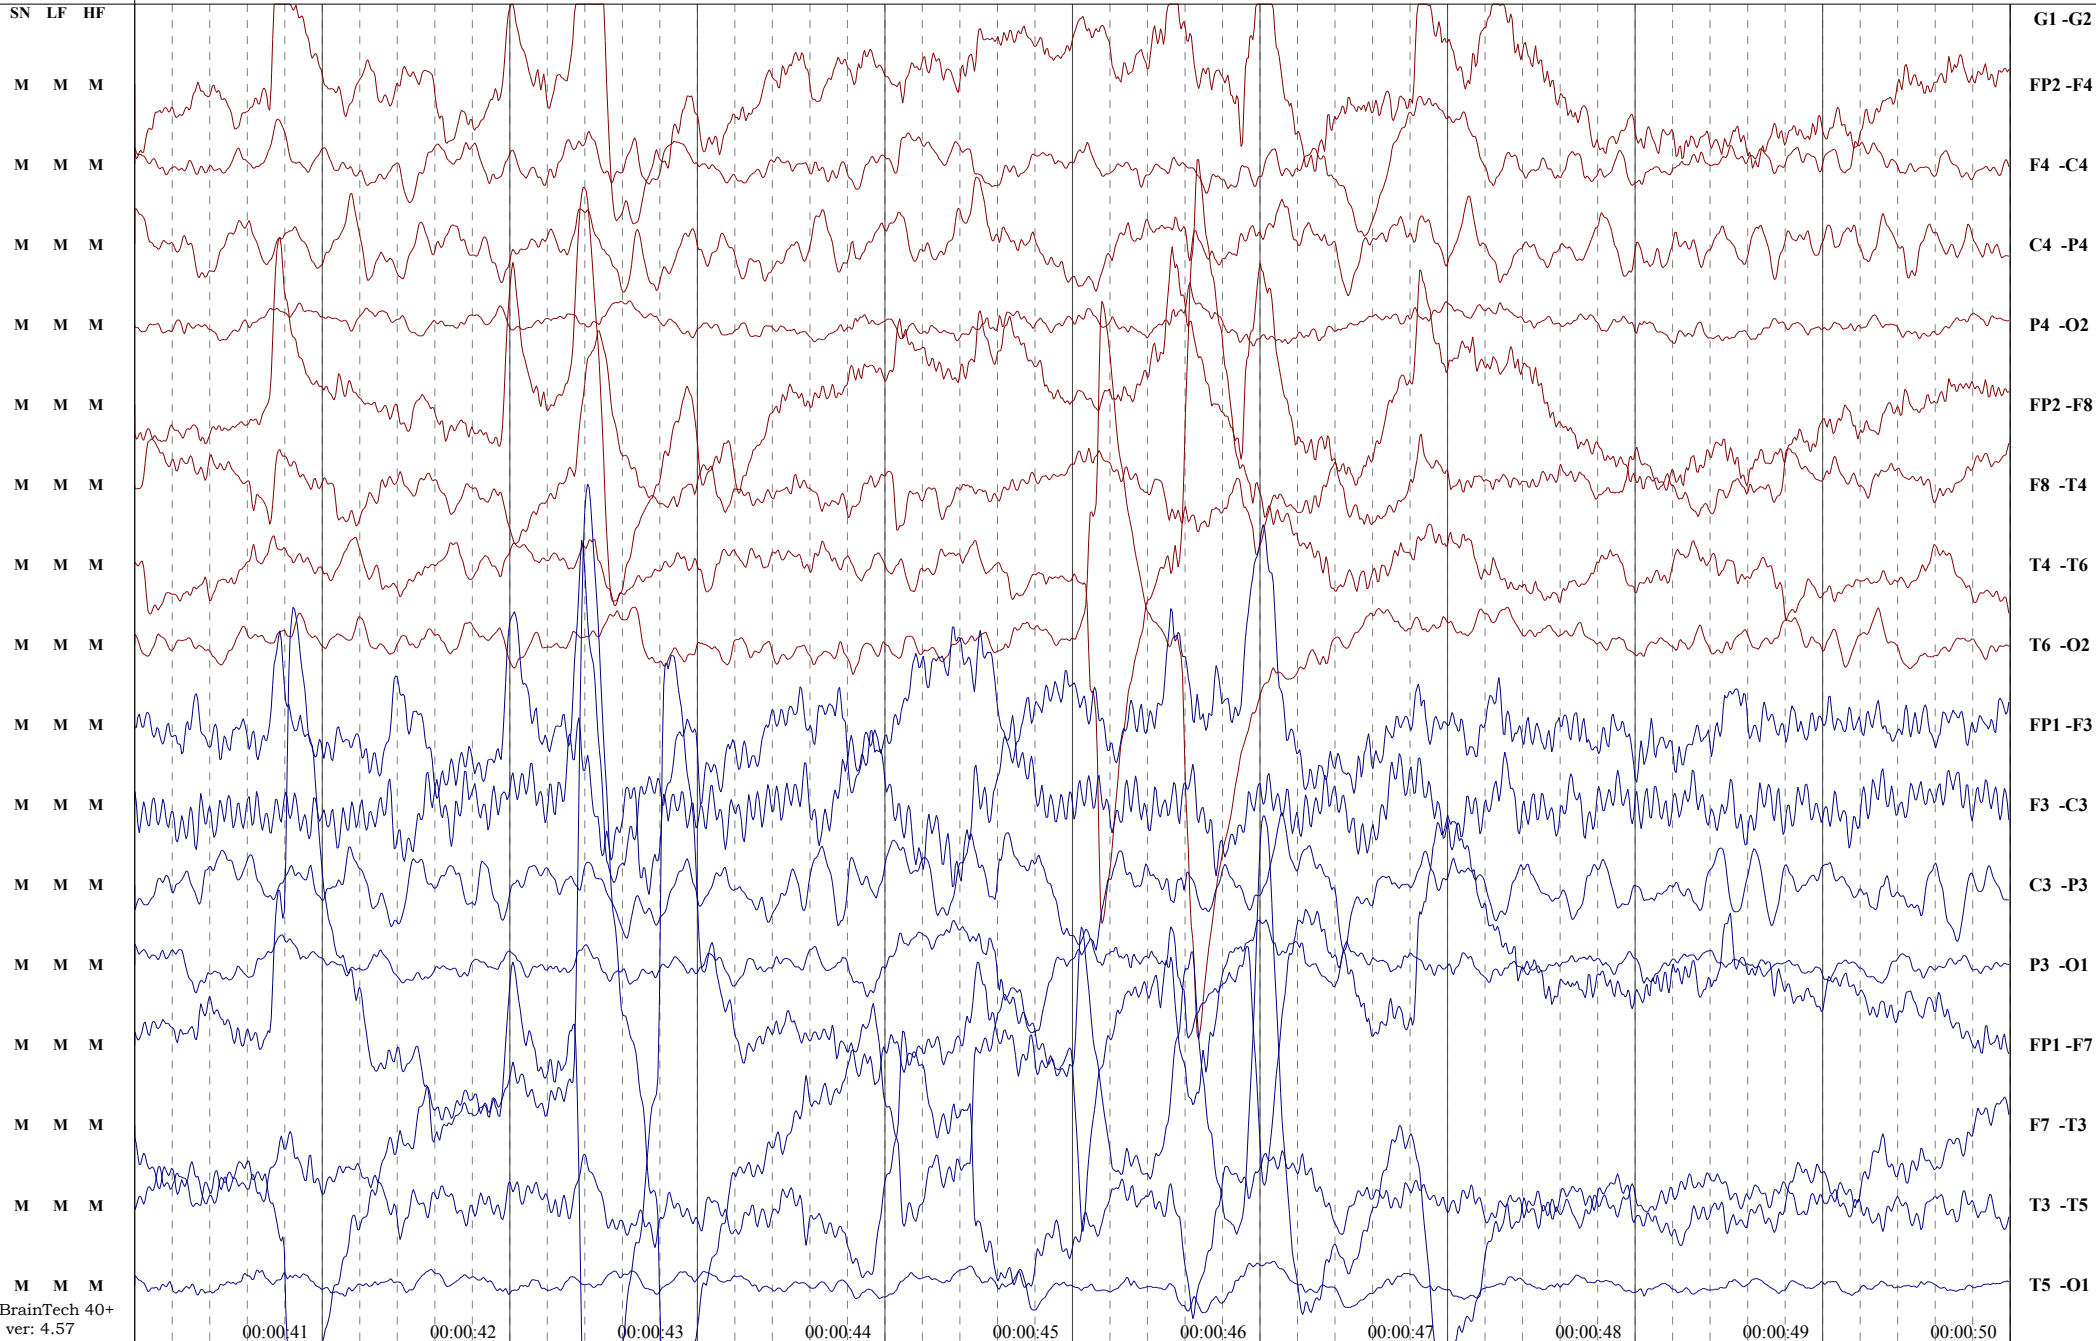


139
MAST. YAMAN PATEL
12 Years/M

Date: 13-Sep-2023
Type: ANALYSIS
BIPOLAR LONGITUDNAL

Speed : 30 mm/S
Sen : 7.5 uV/mm
Filter : 1 Hz - 70 Hz

Time: 16:41:35
Page:6/25
Notch: ON

Ref:DR. RAJNISH PANDEY
Dr. : DR. VIJENDRA PAINKARA
Tech:

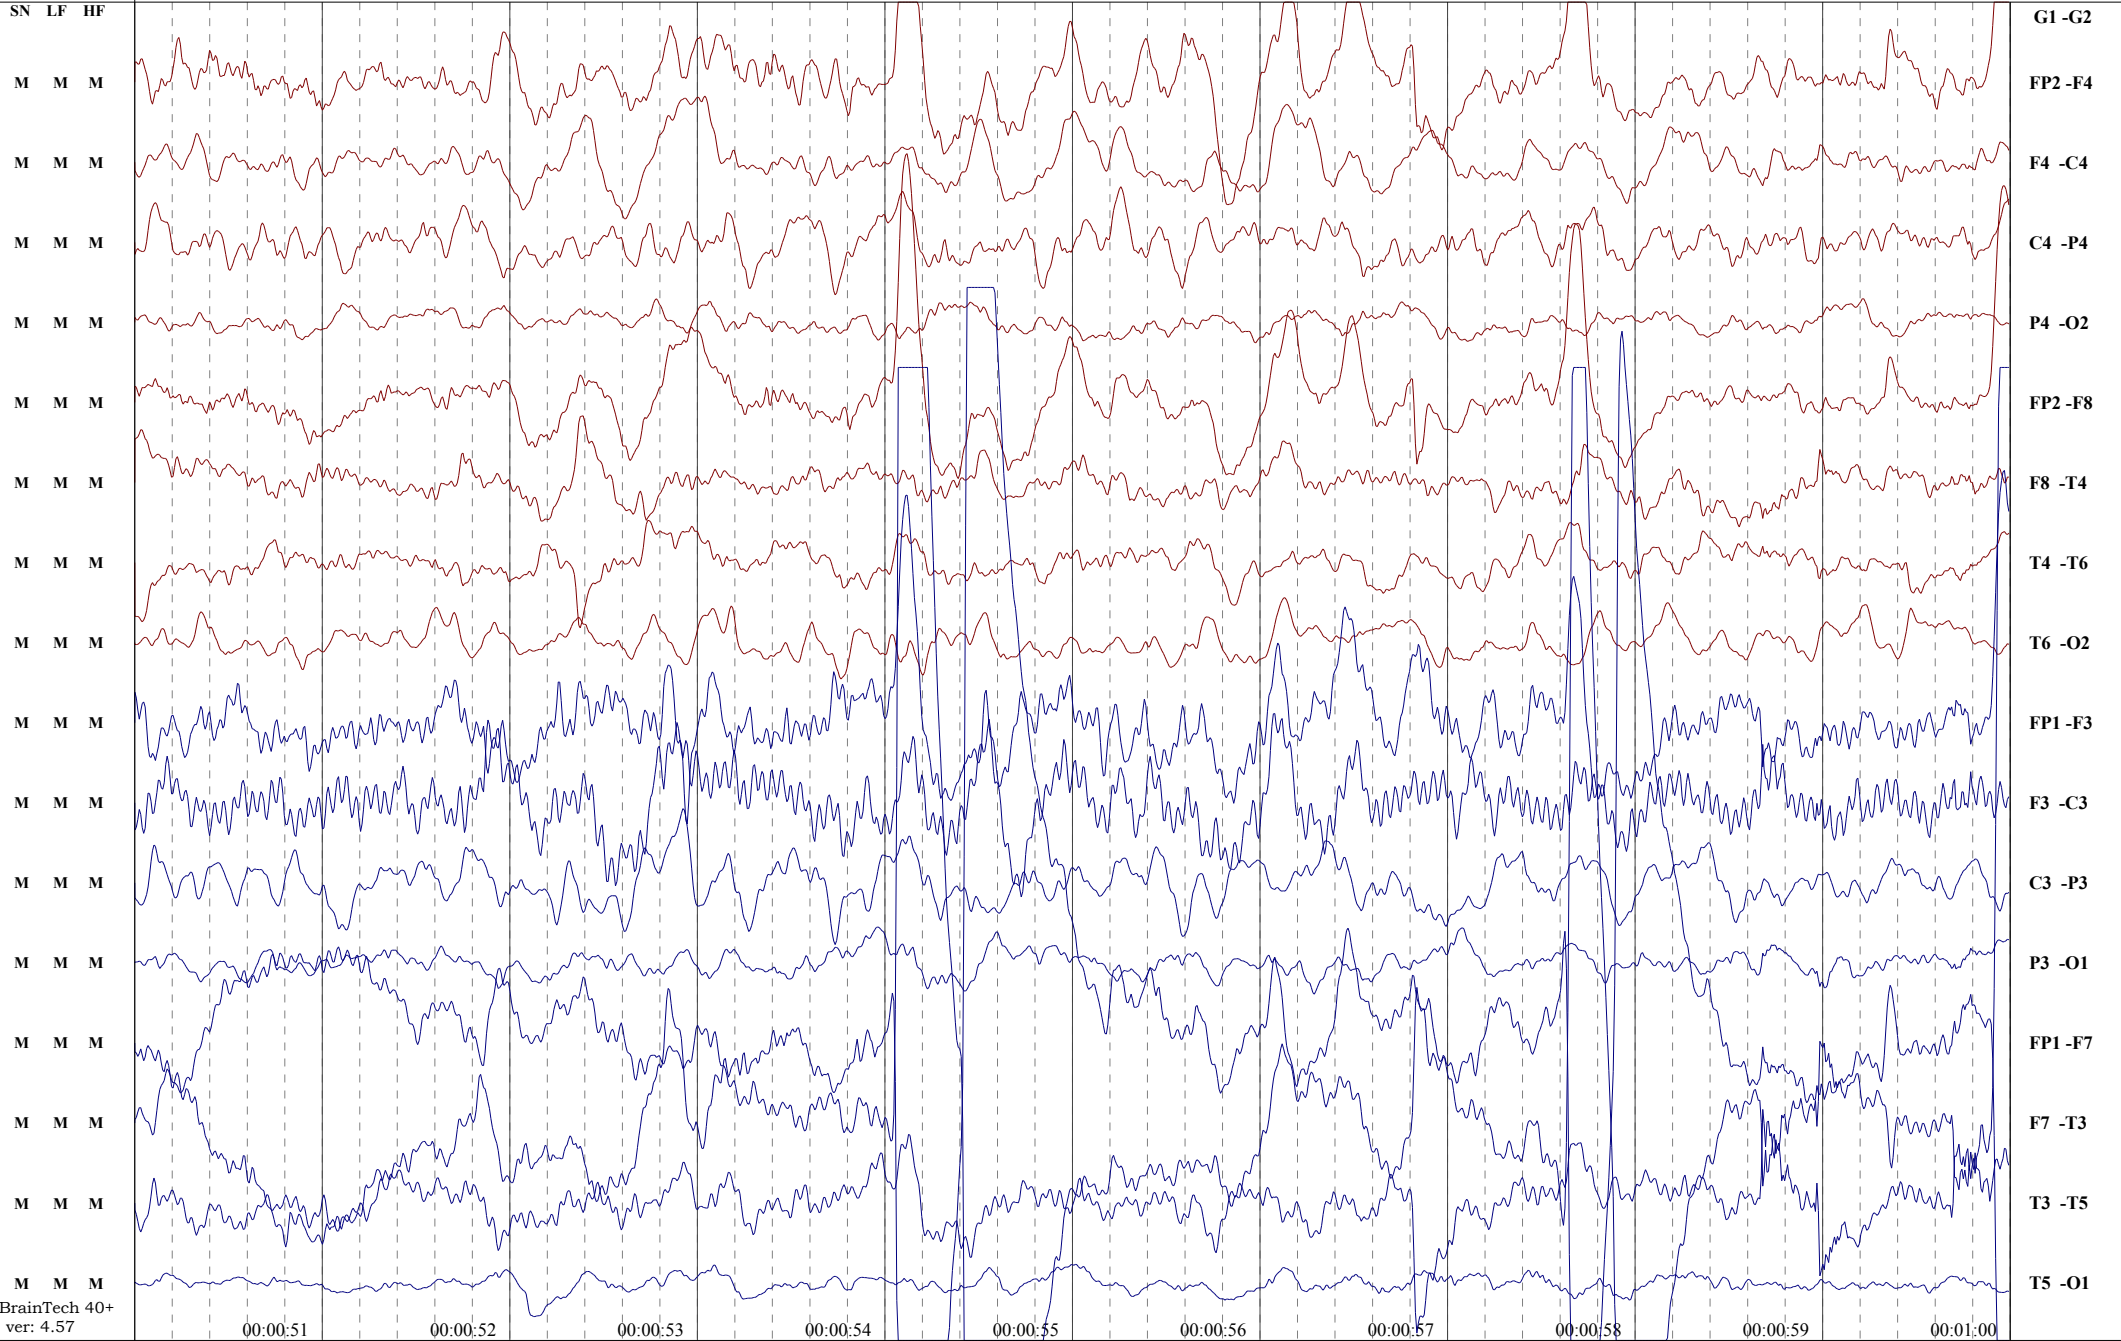


139
MAST. YAMAN PATEL
12 Years/M

Date: 13-Sep-2023
Type: ANALYSIS
BIPOLAR LONGITUDNAL

Speed : 30 mm/S
Sen : 7.5 uV/mm
Filter : 1 Hz - 70 Hz

Time: 16:41:45
Page:7/25
Notch: ON

Ref:DR. RAJNISH PANDEY
Dr. : DR. VIJENDRA PAINKARA
Tech:

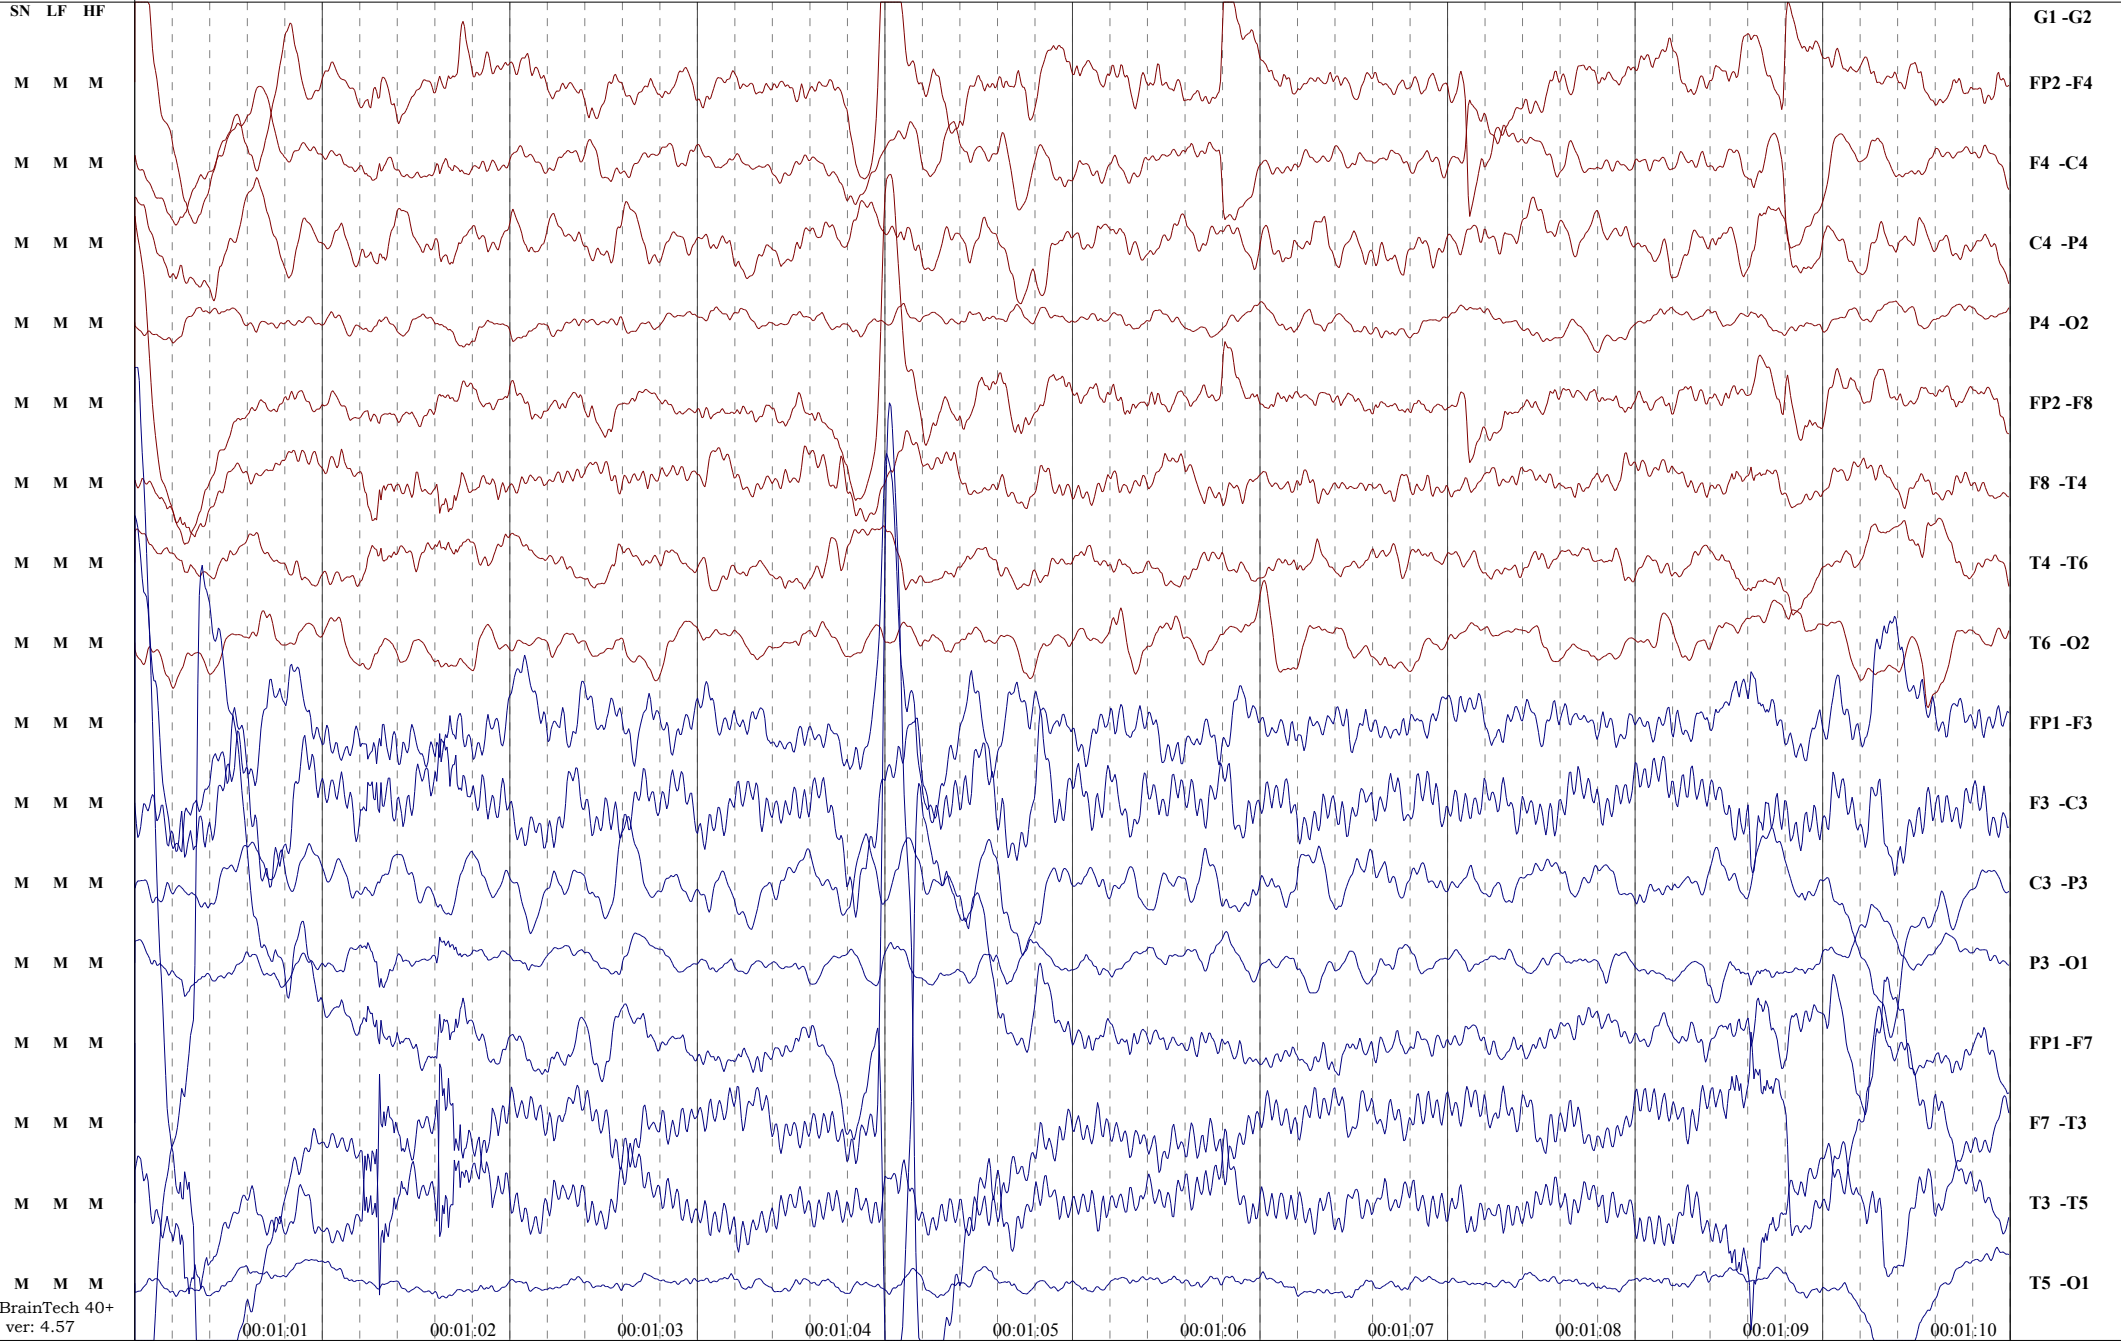


139
MAST. YAMAN PATEL
12 Years/M

Date: 13-Sep-2023
Type: ANALYSIS
BIPOLAR LONGITUDNAL

Speed : 30 mm/S
Sen : 7.5 uV/mm
Filter : 1 Hz - 70 Hz

Time: 16:41:45
Page:7/25
Notch: ON

Ref:DR. RAJNISH PANDEY
Dr. : DR. VIJENDRA PAINKARA
Tech:

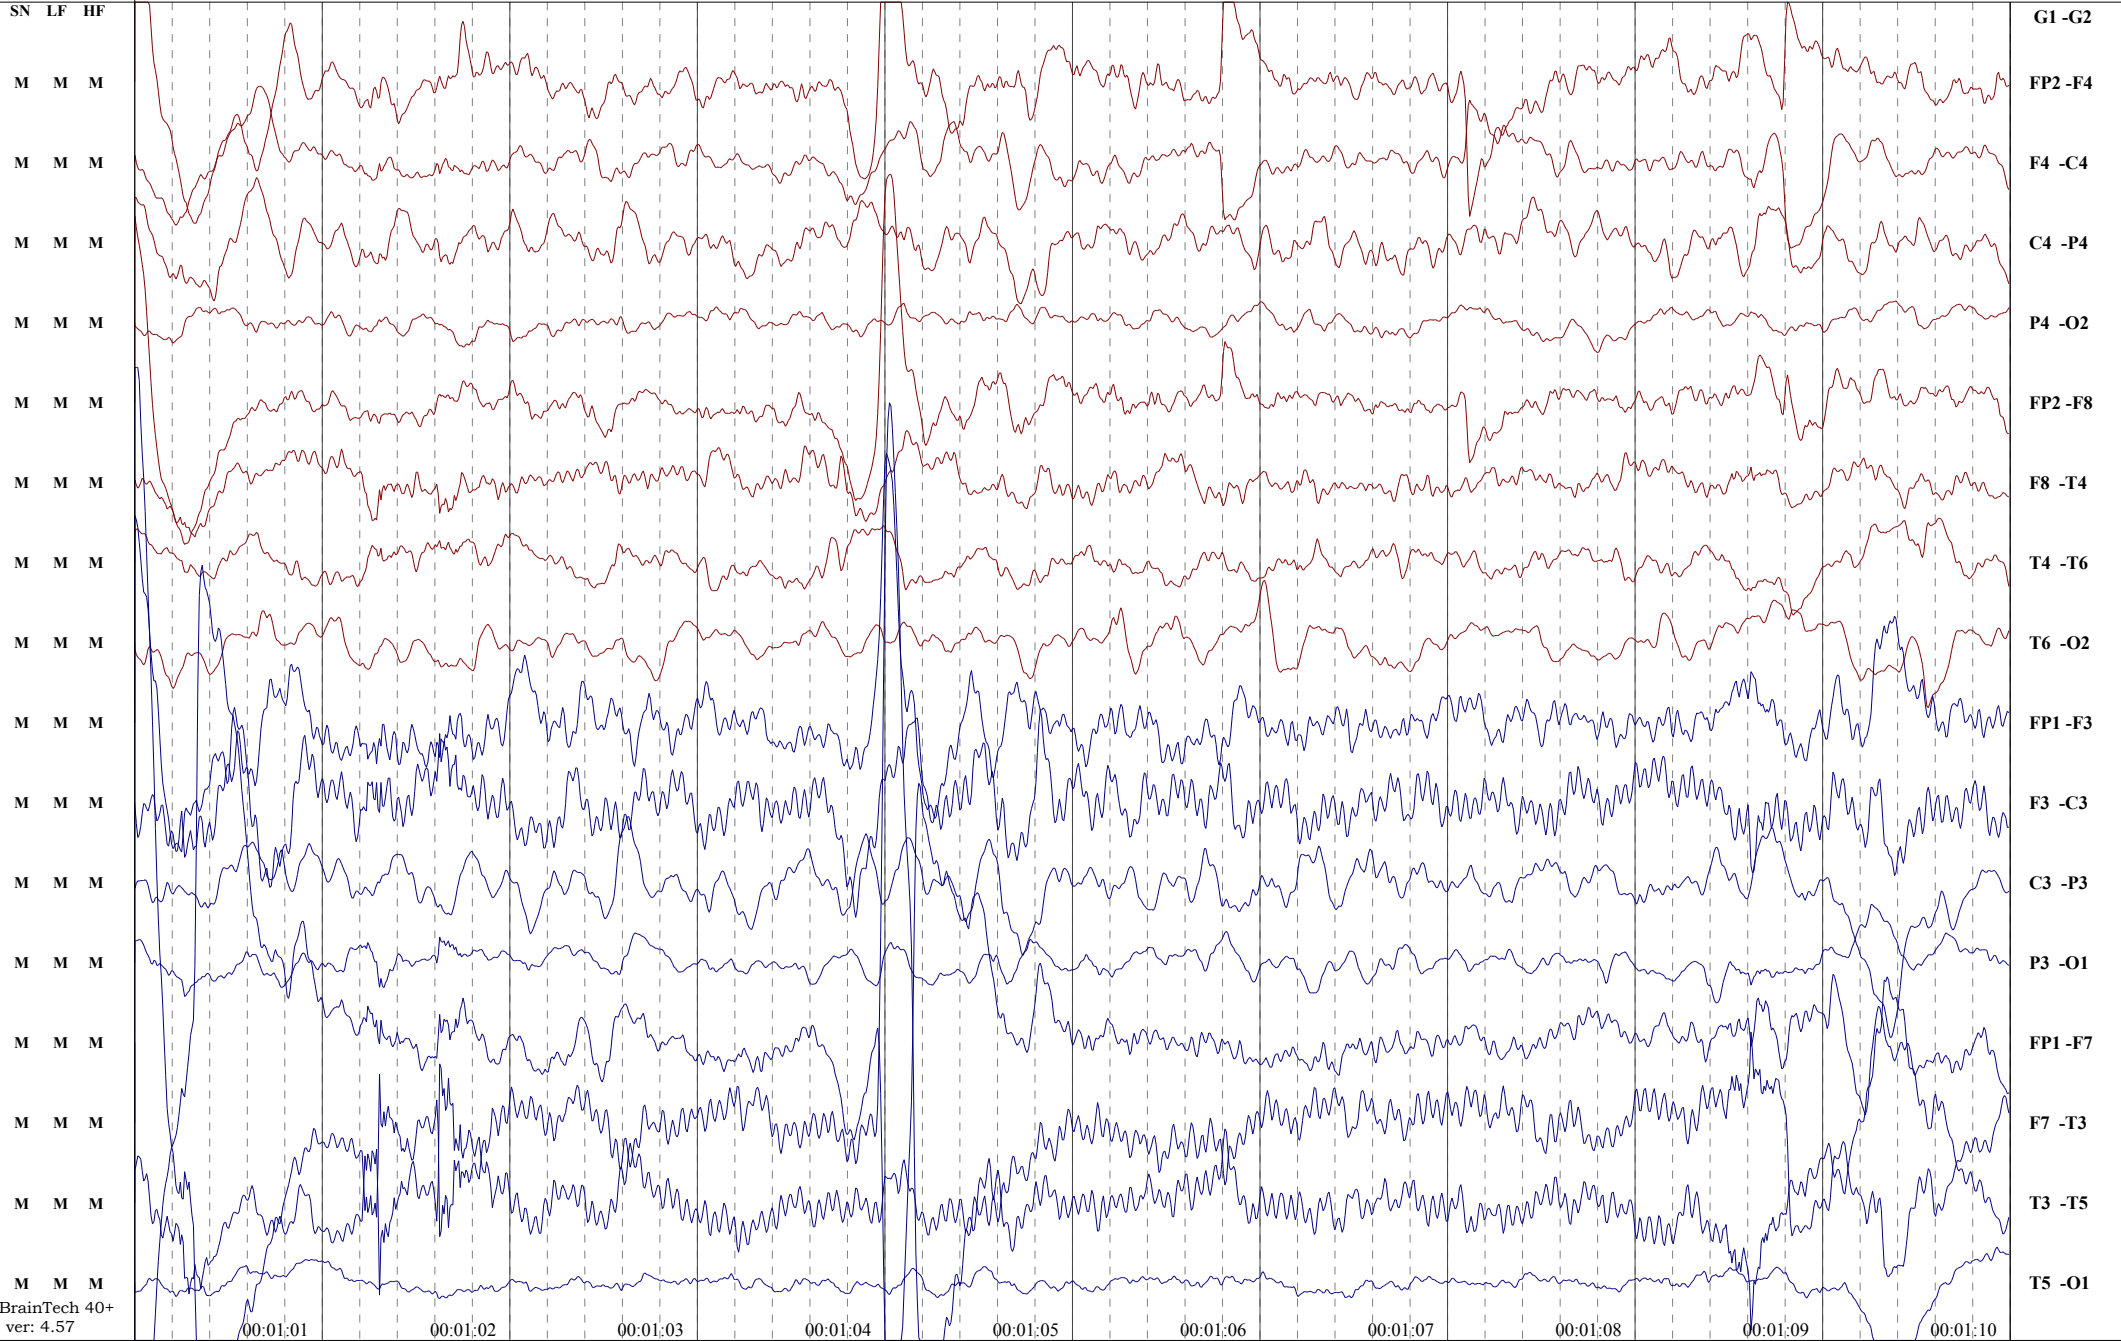


139
MAST. YAMAN PATEL
12 Years/M


Date: 13-Sep-2023
Type: ANALYSIS
BIPOLAR LONGITUDNAL


Speed : 30 mm/S
Sen : 7.5 uV/mm
Filter : 1 Hz - 70 Hz


Time: 16:41:55
Page:8/25
Notch: ON


Ref:DR. RAJNISH PANDEY
Dr. : DR. VIJENDRA PAINKARA
Tech:

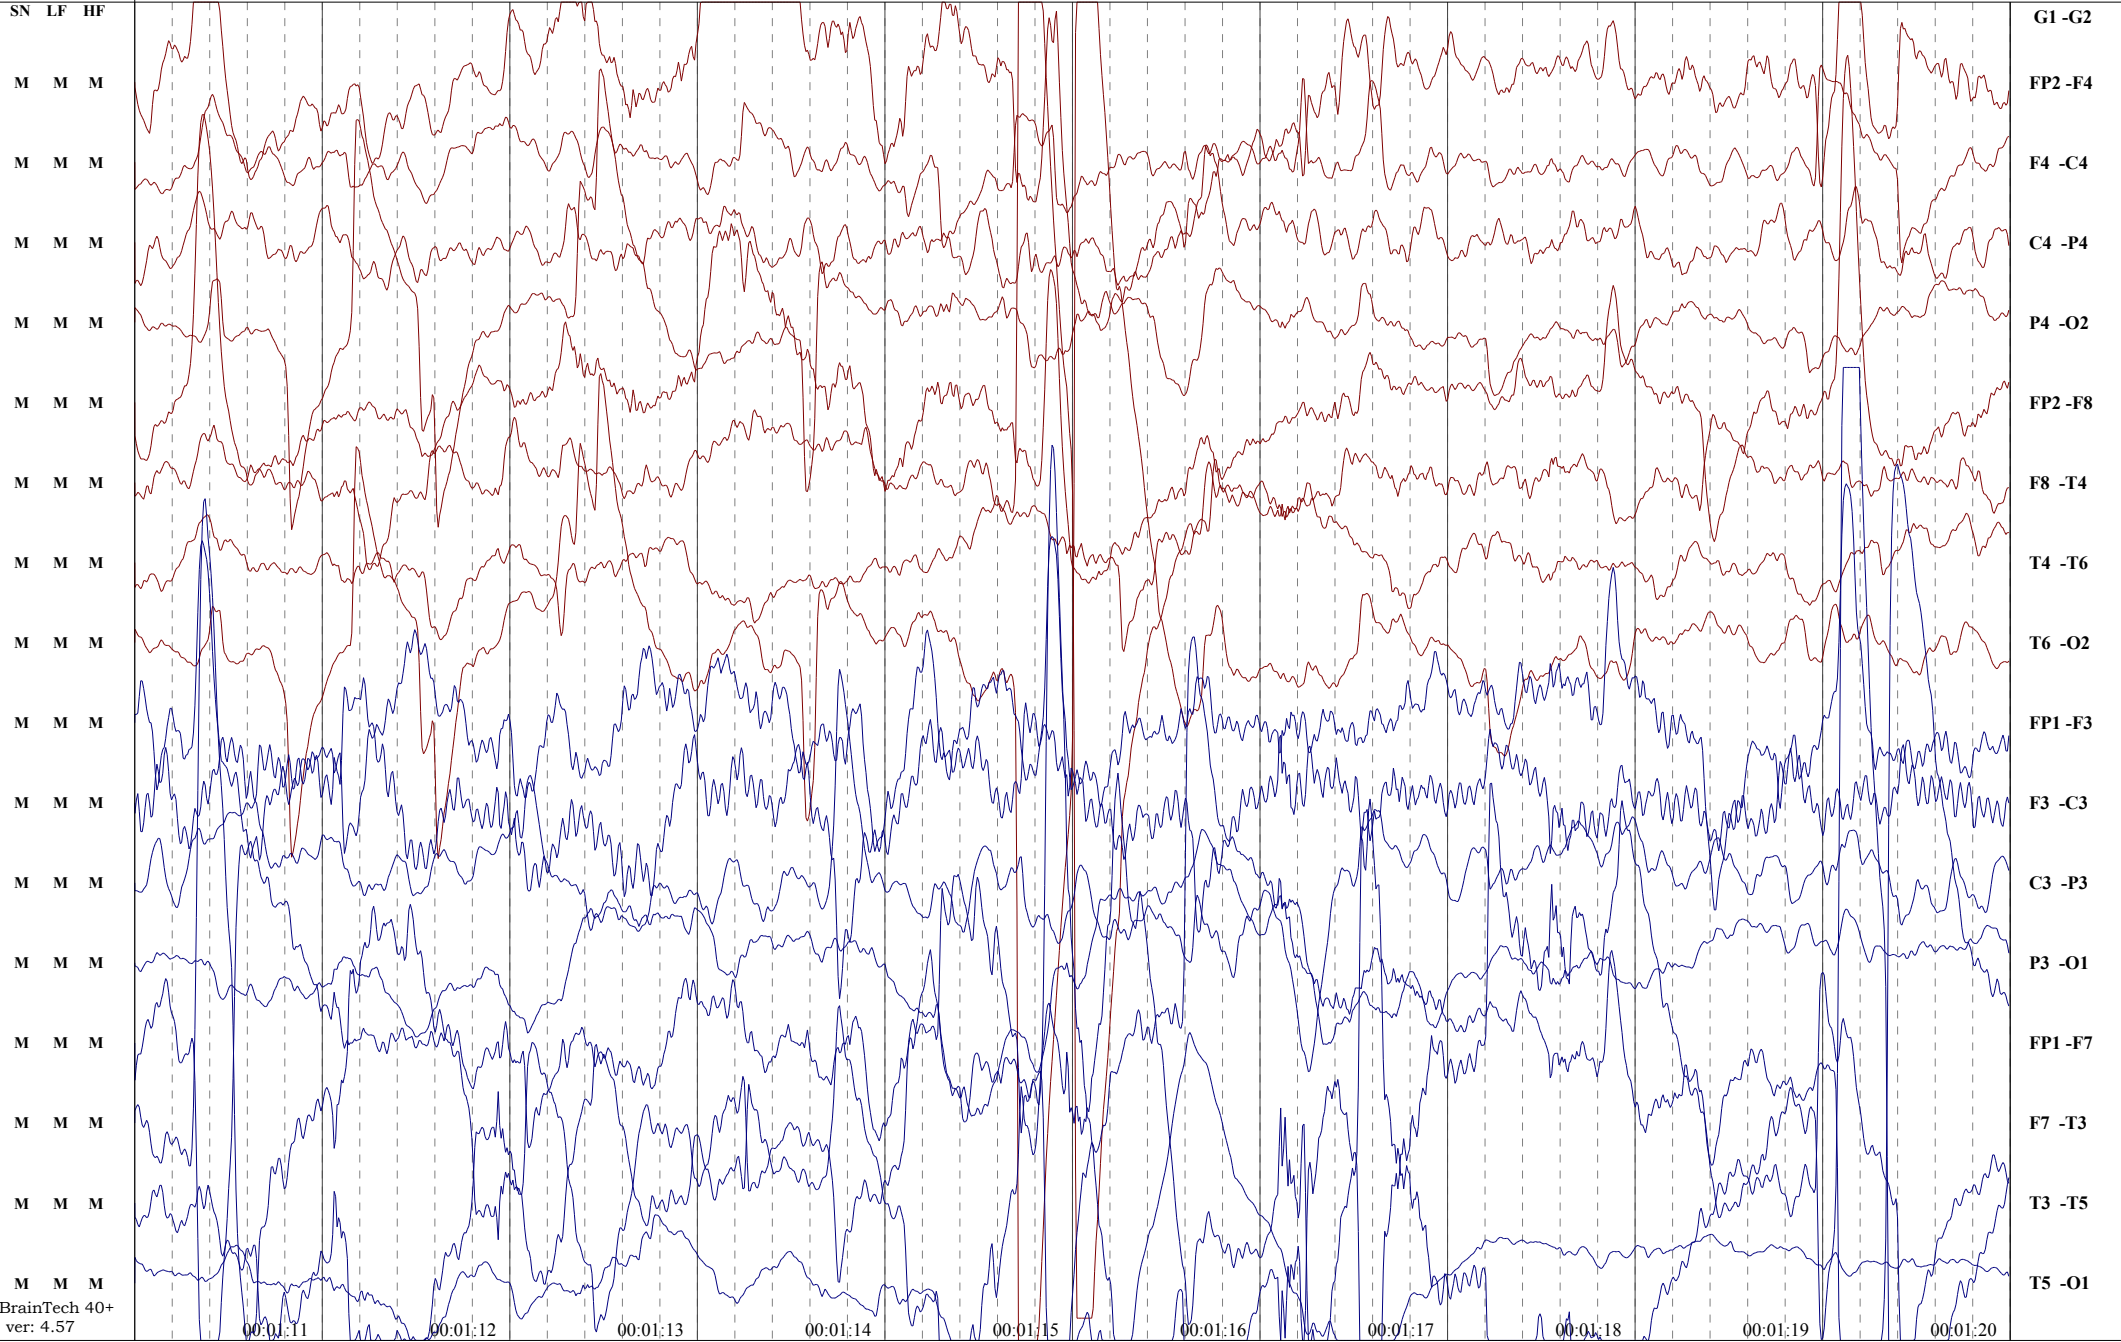


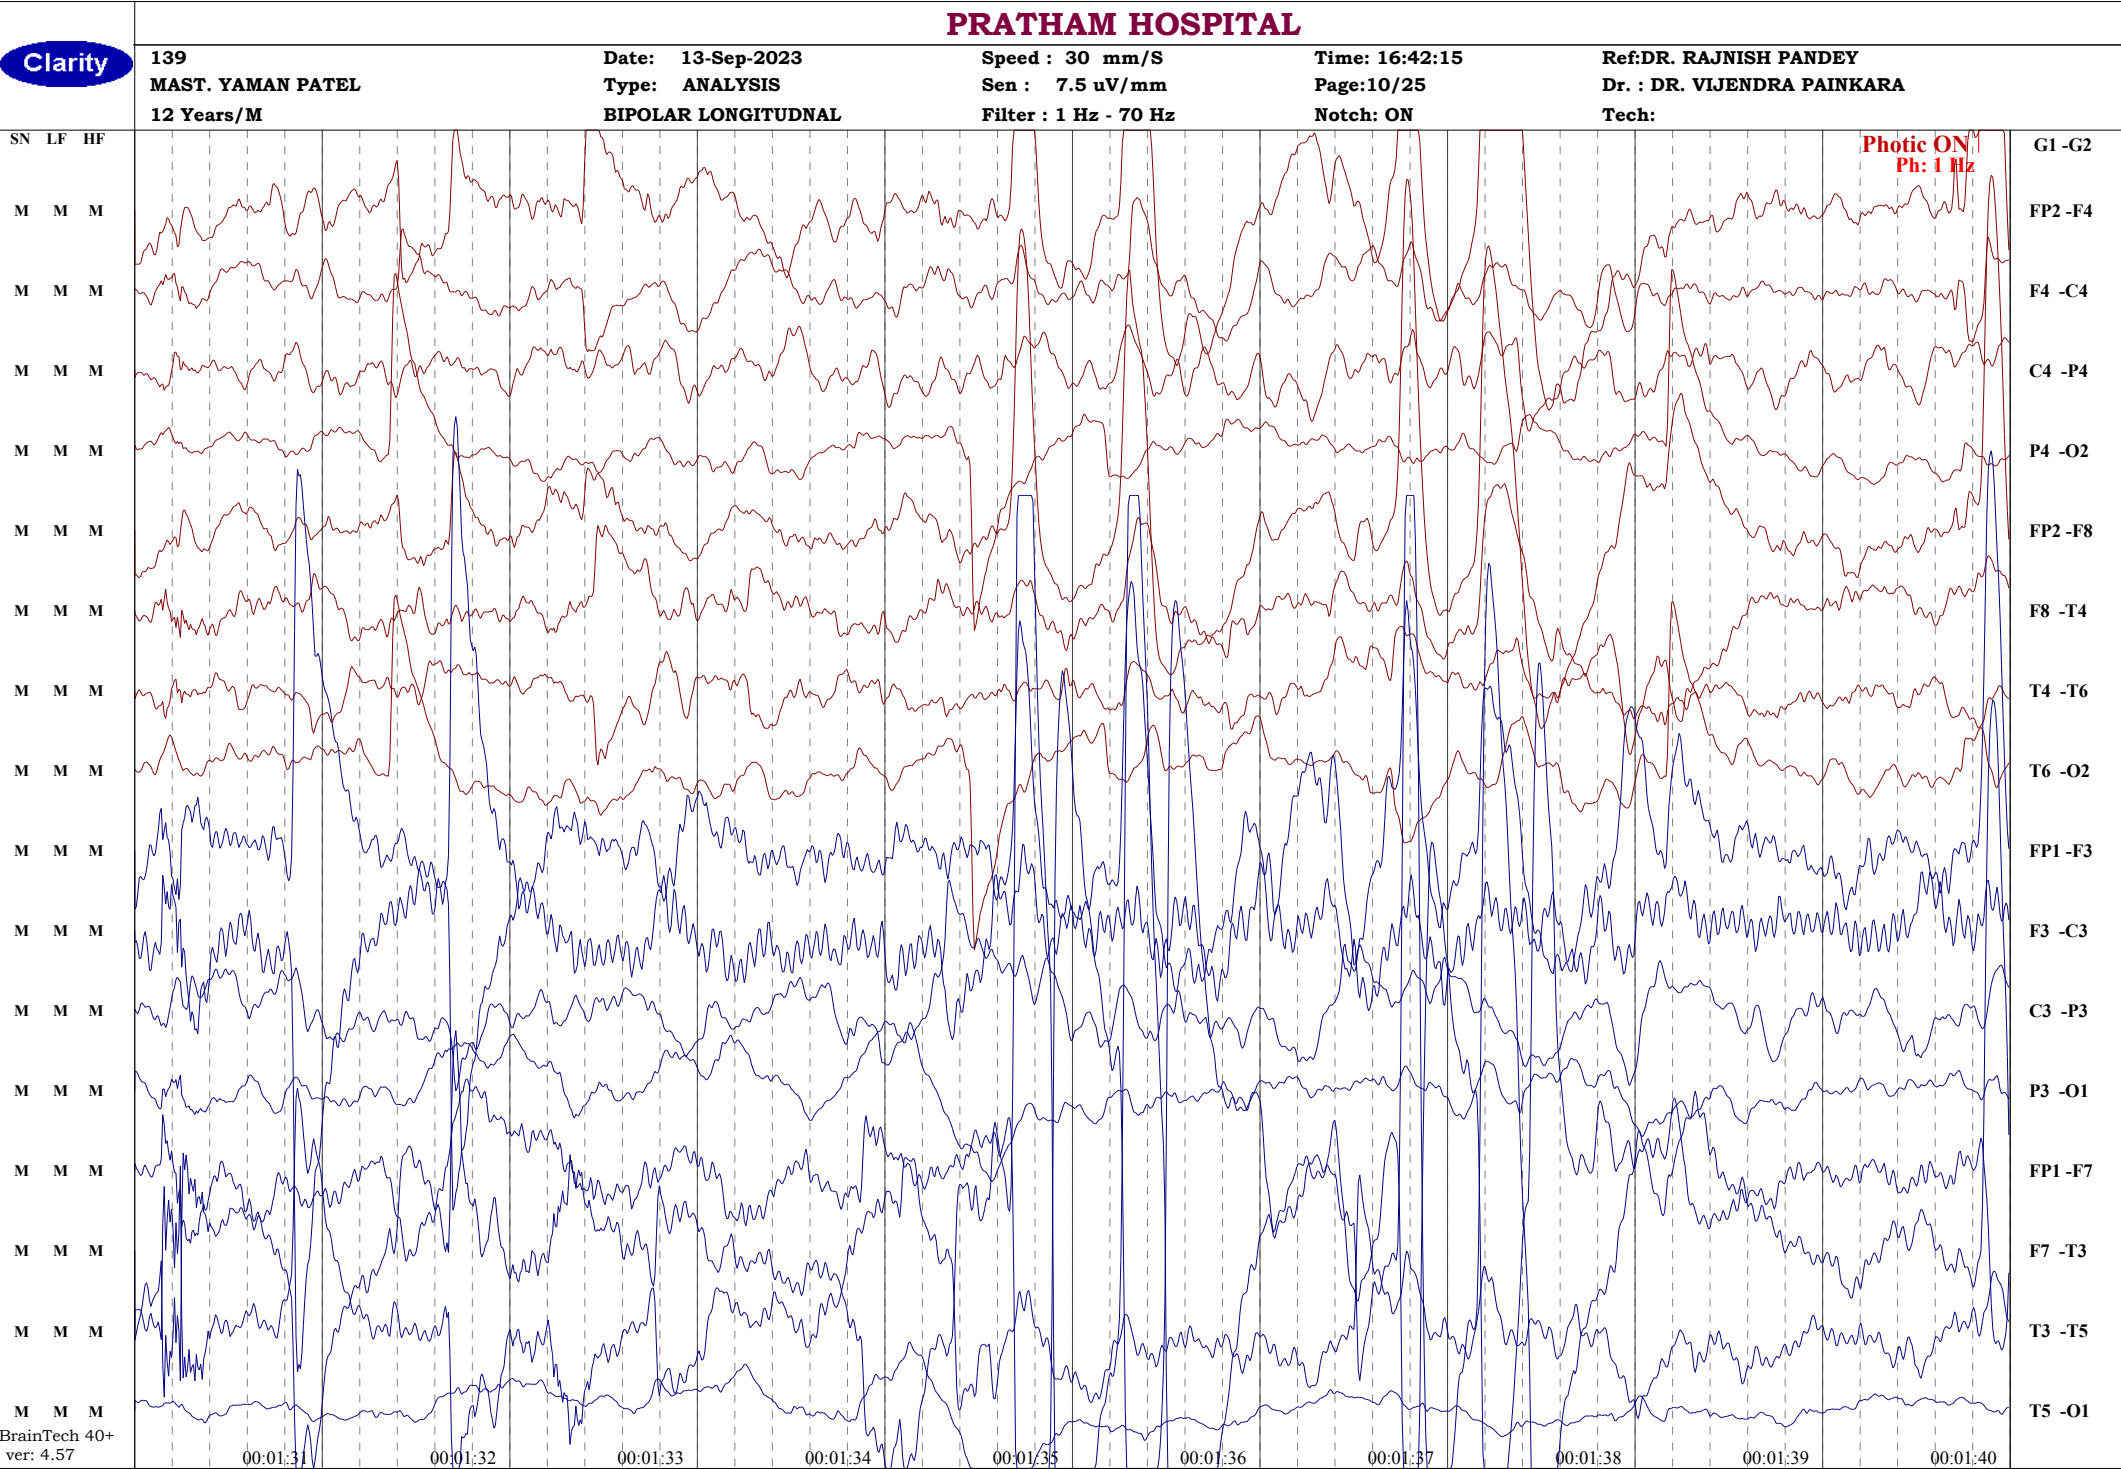


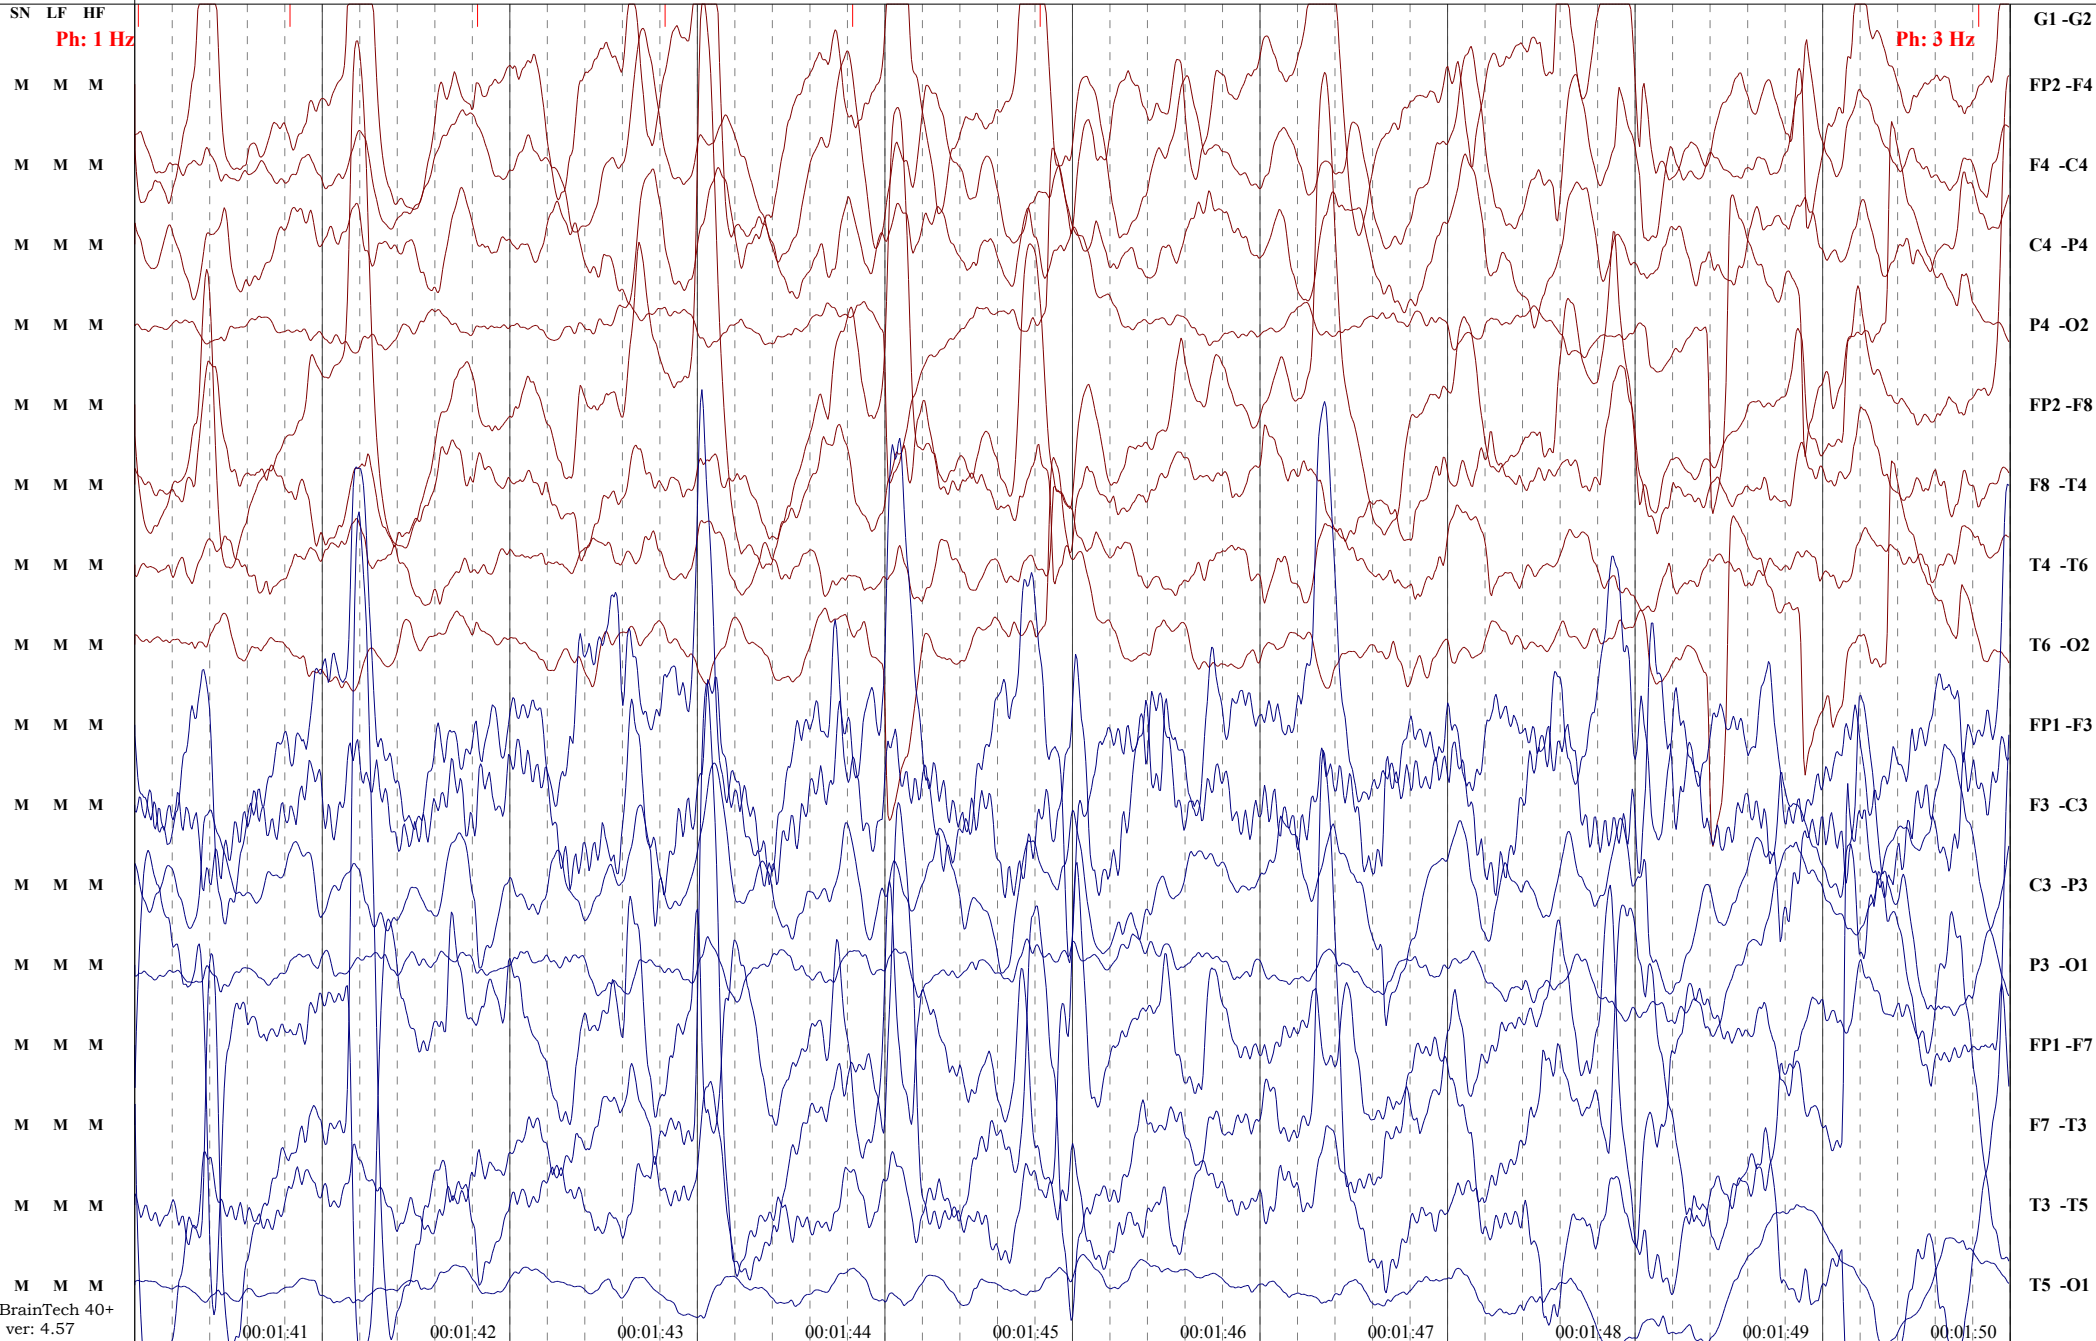


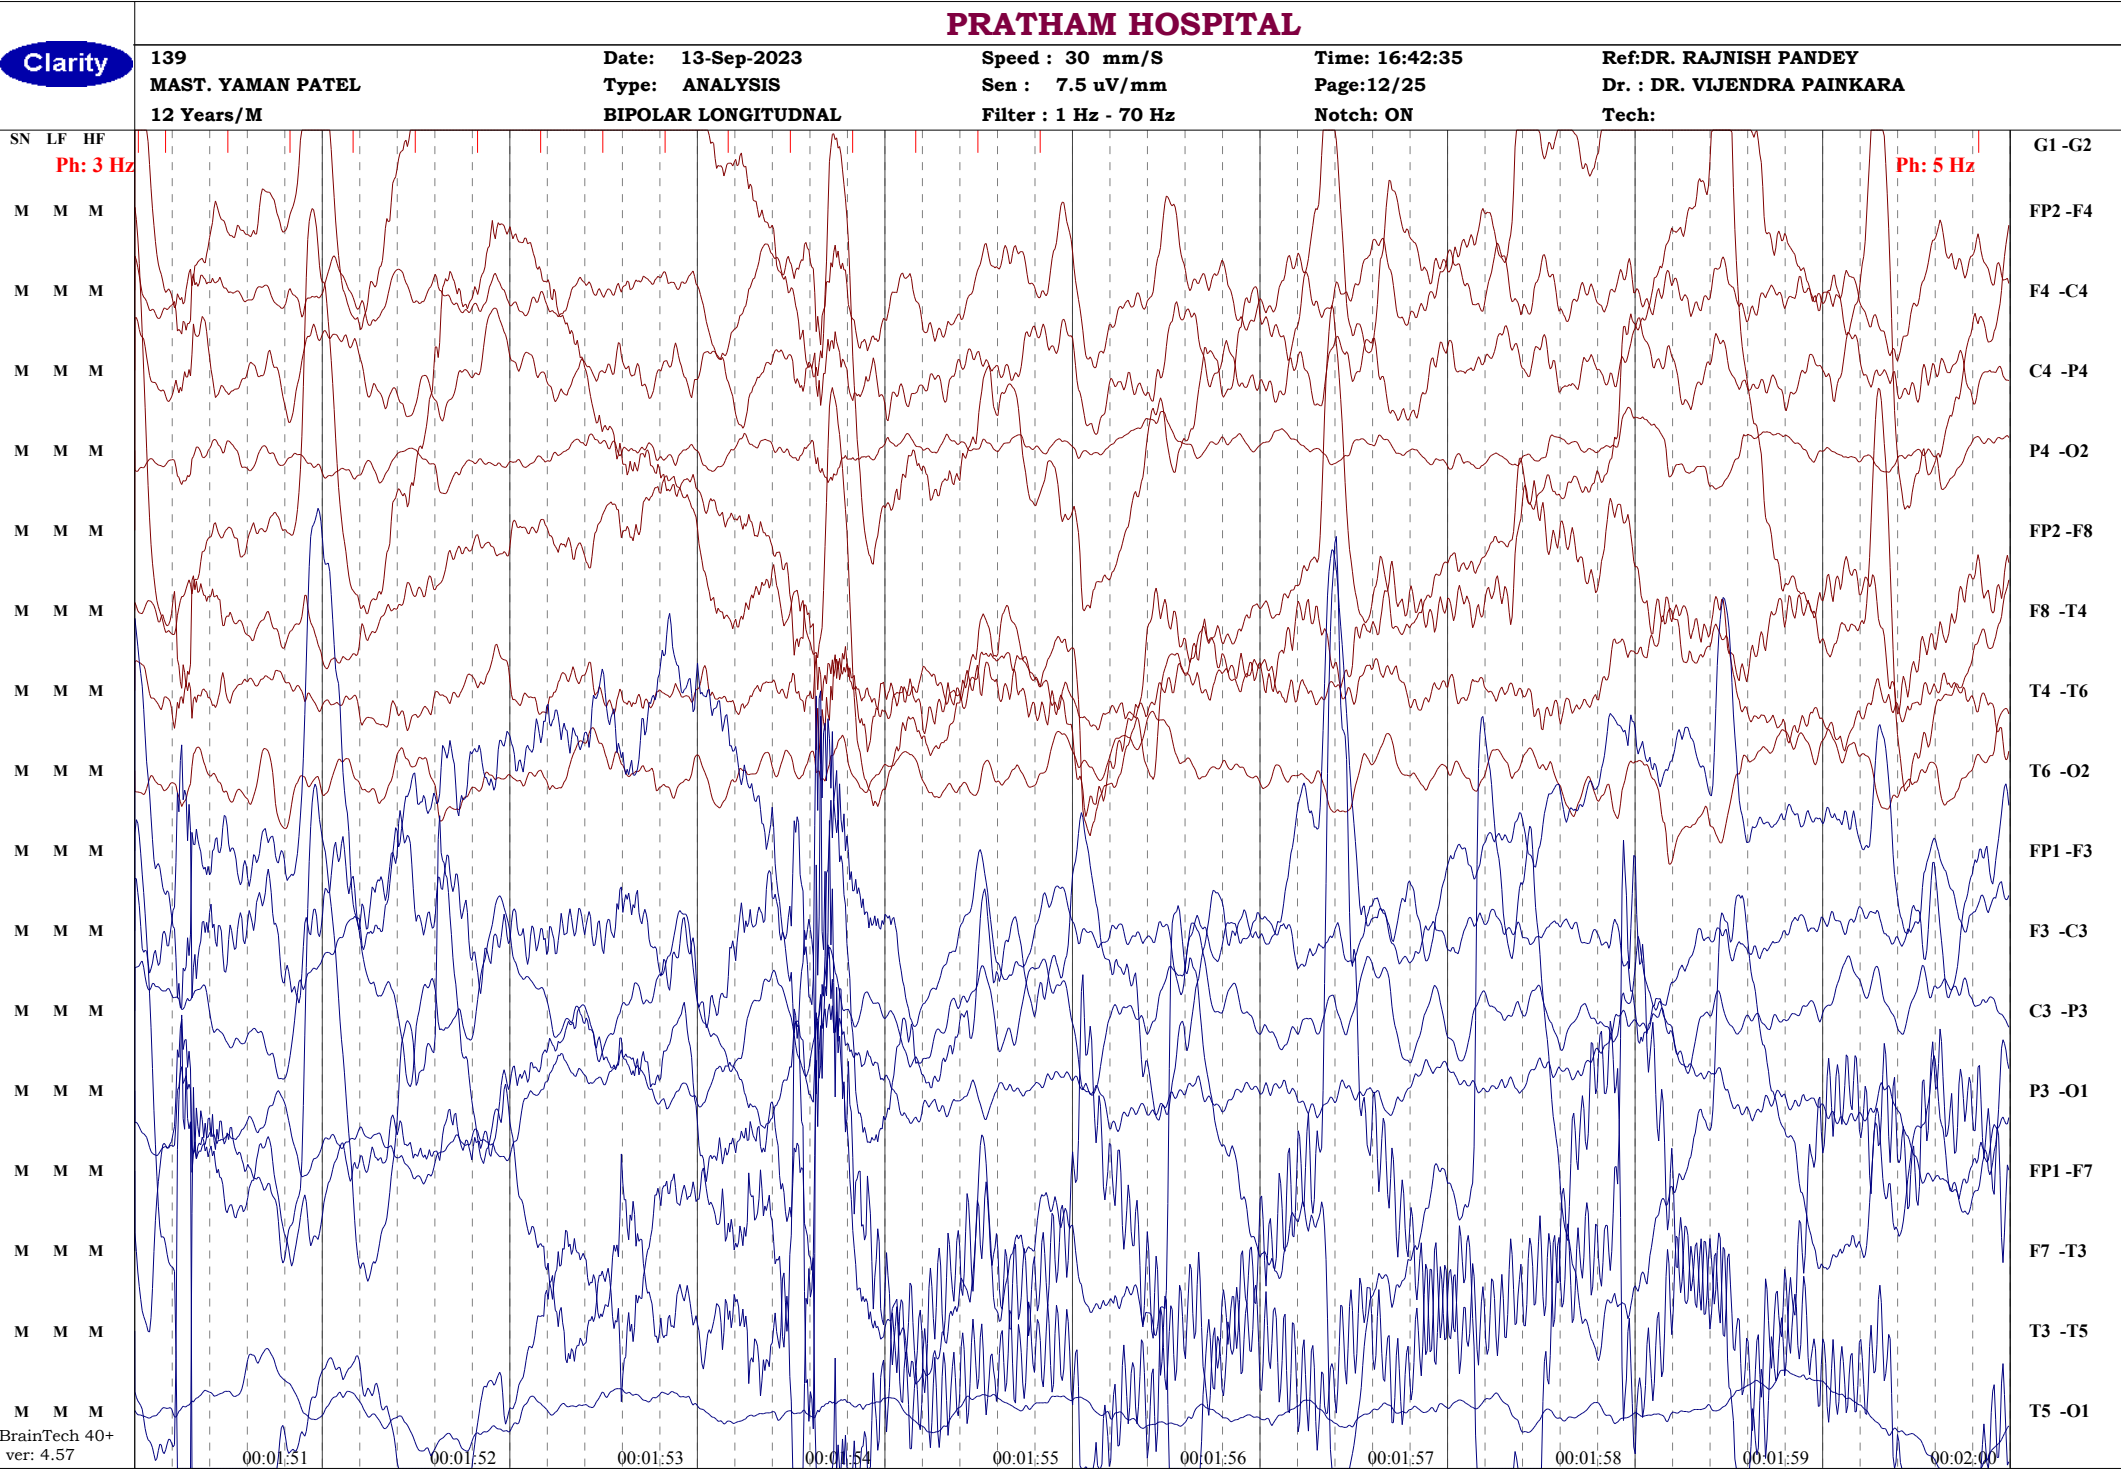


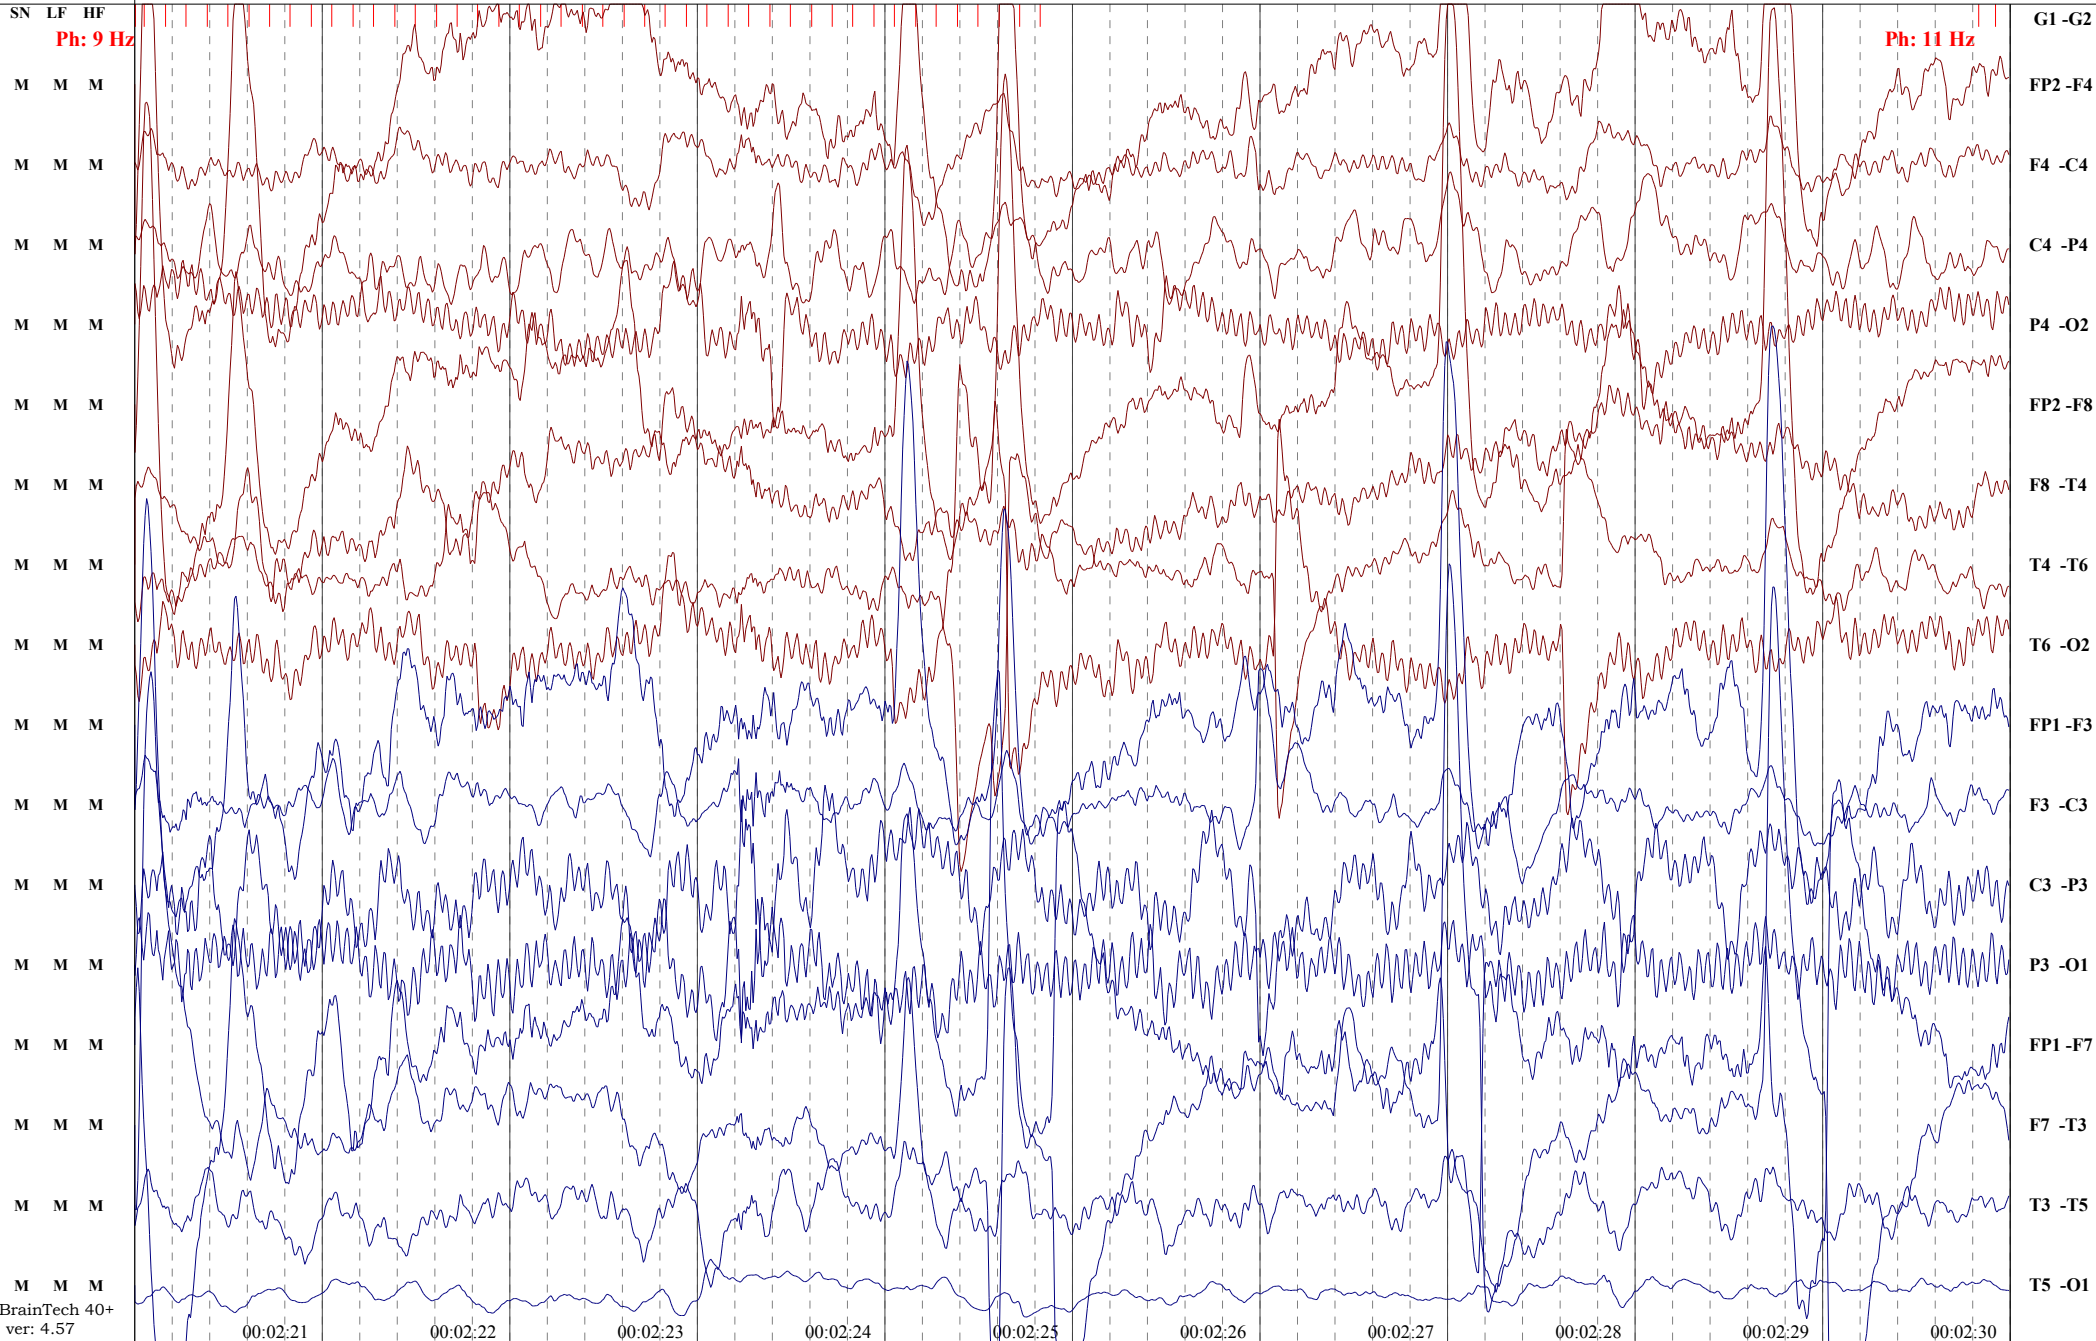


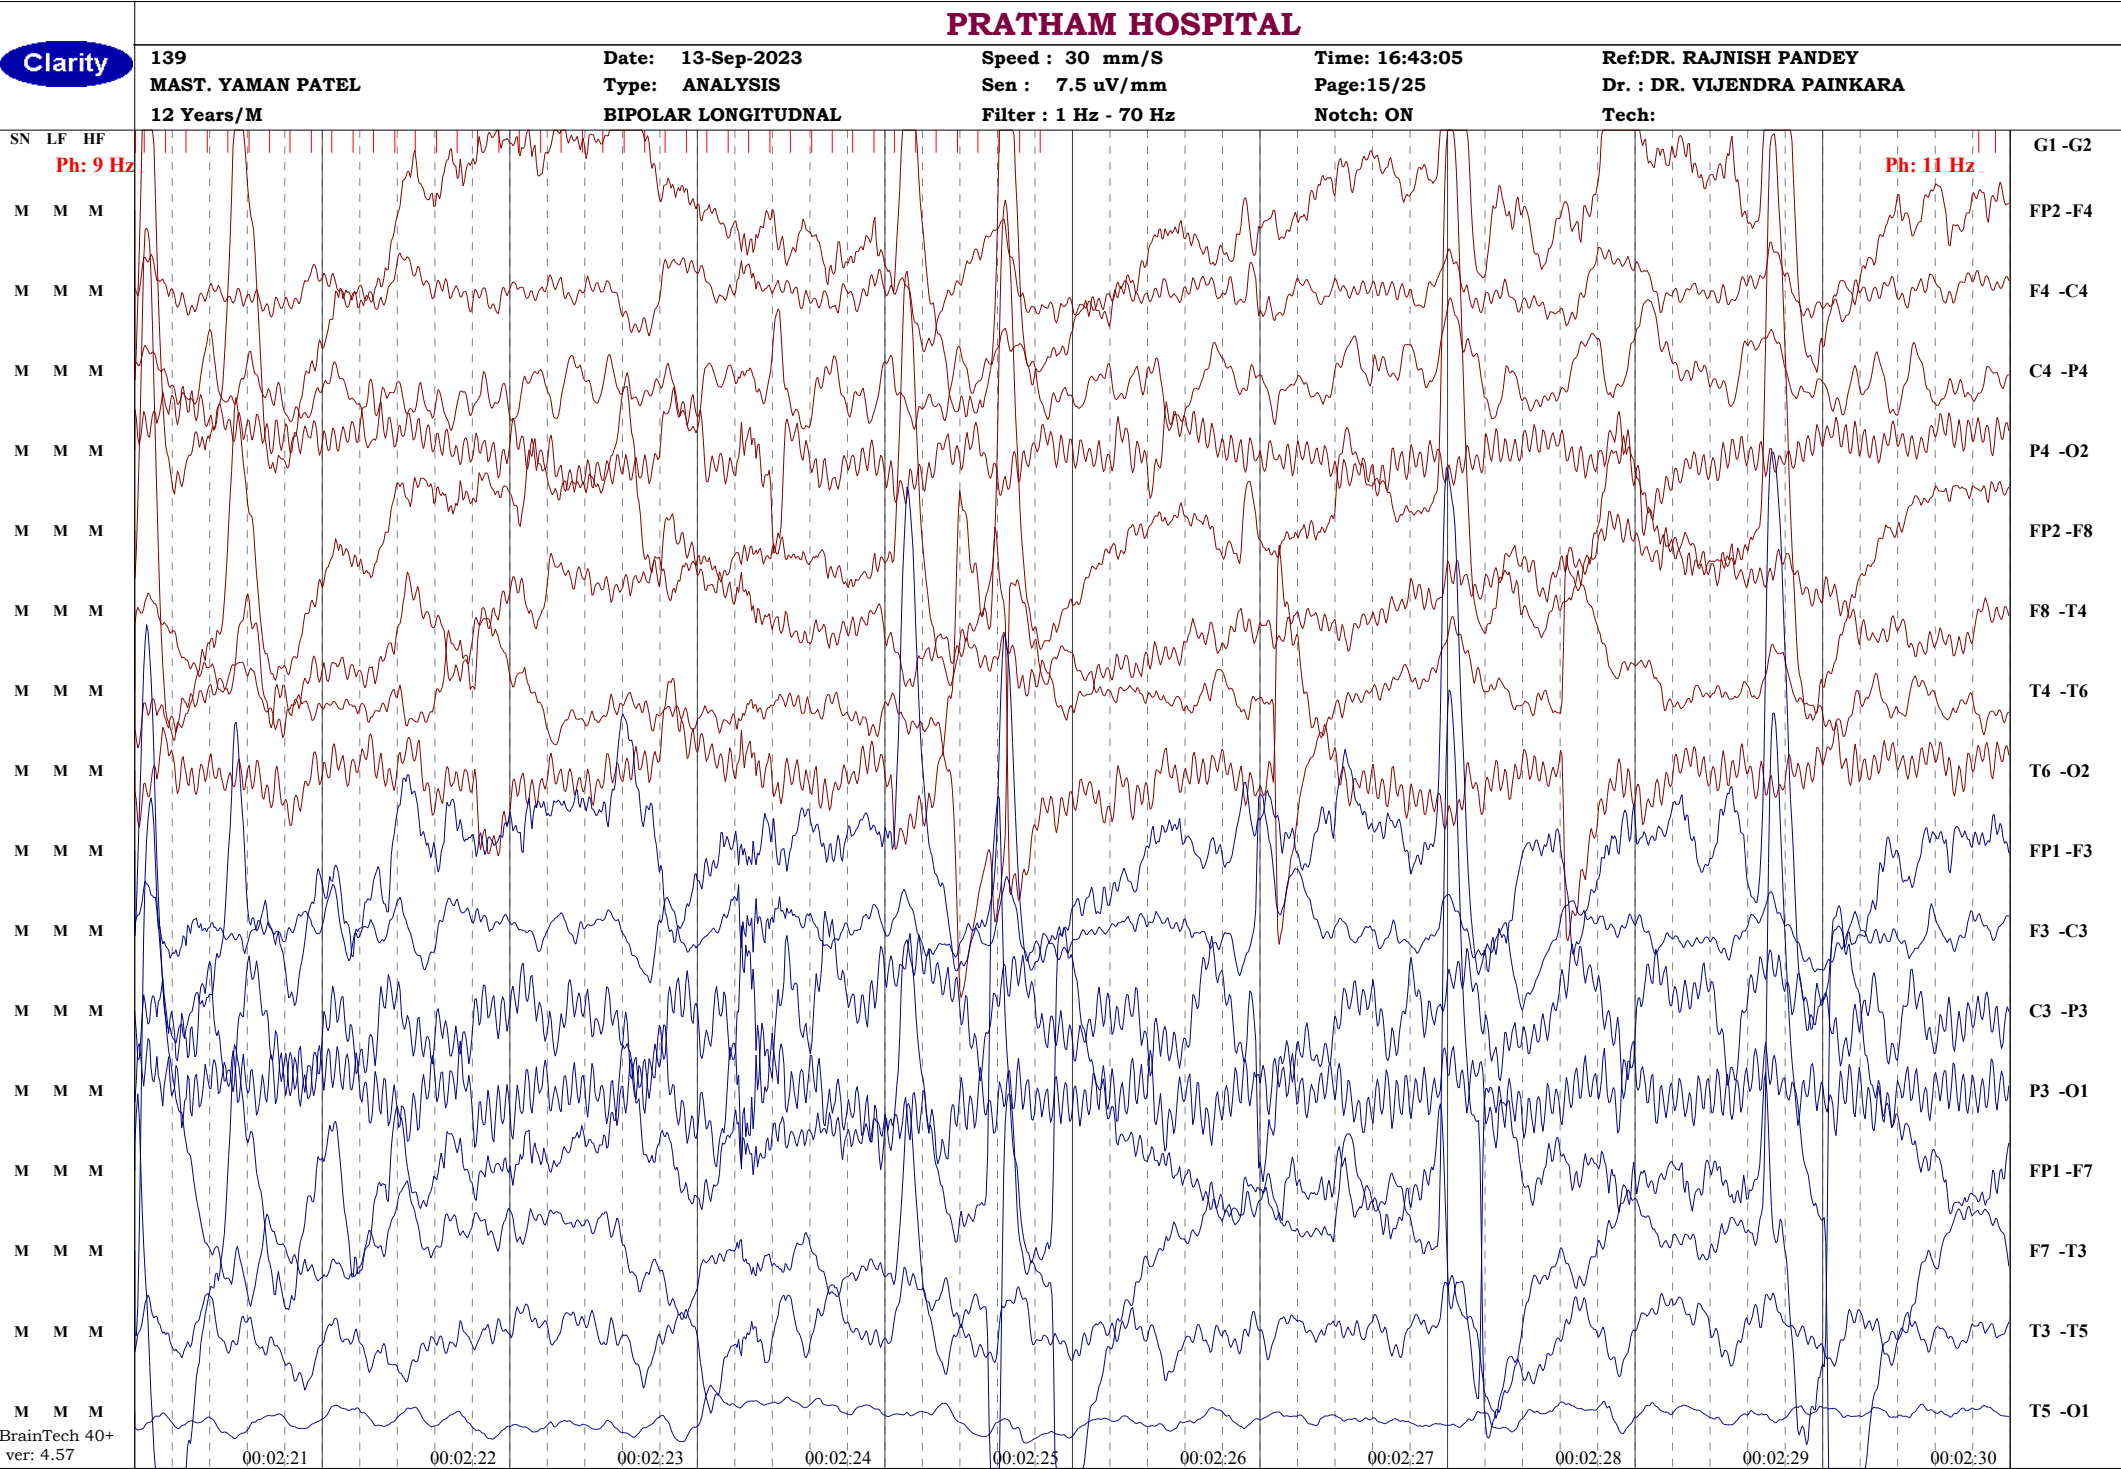


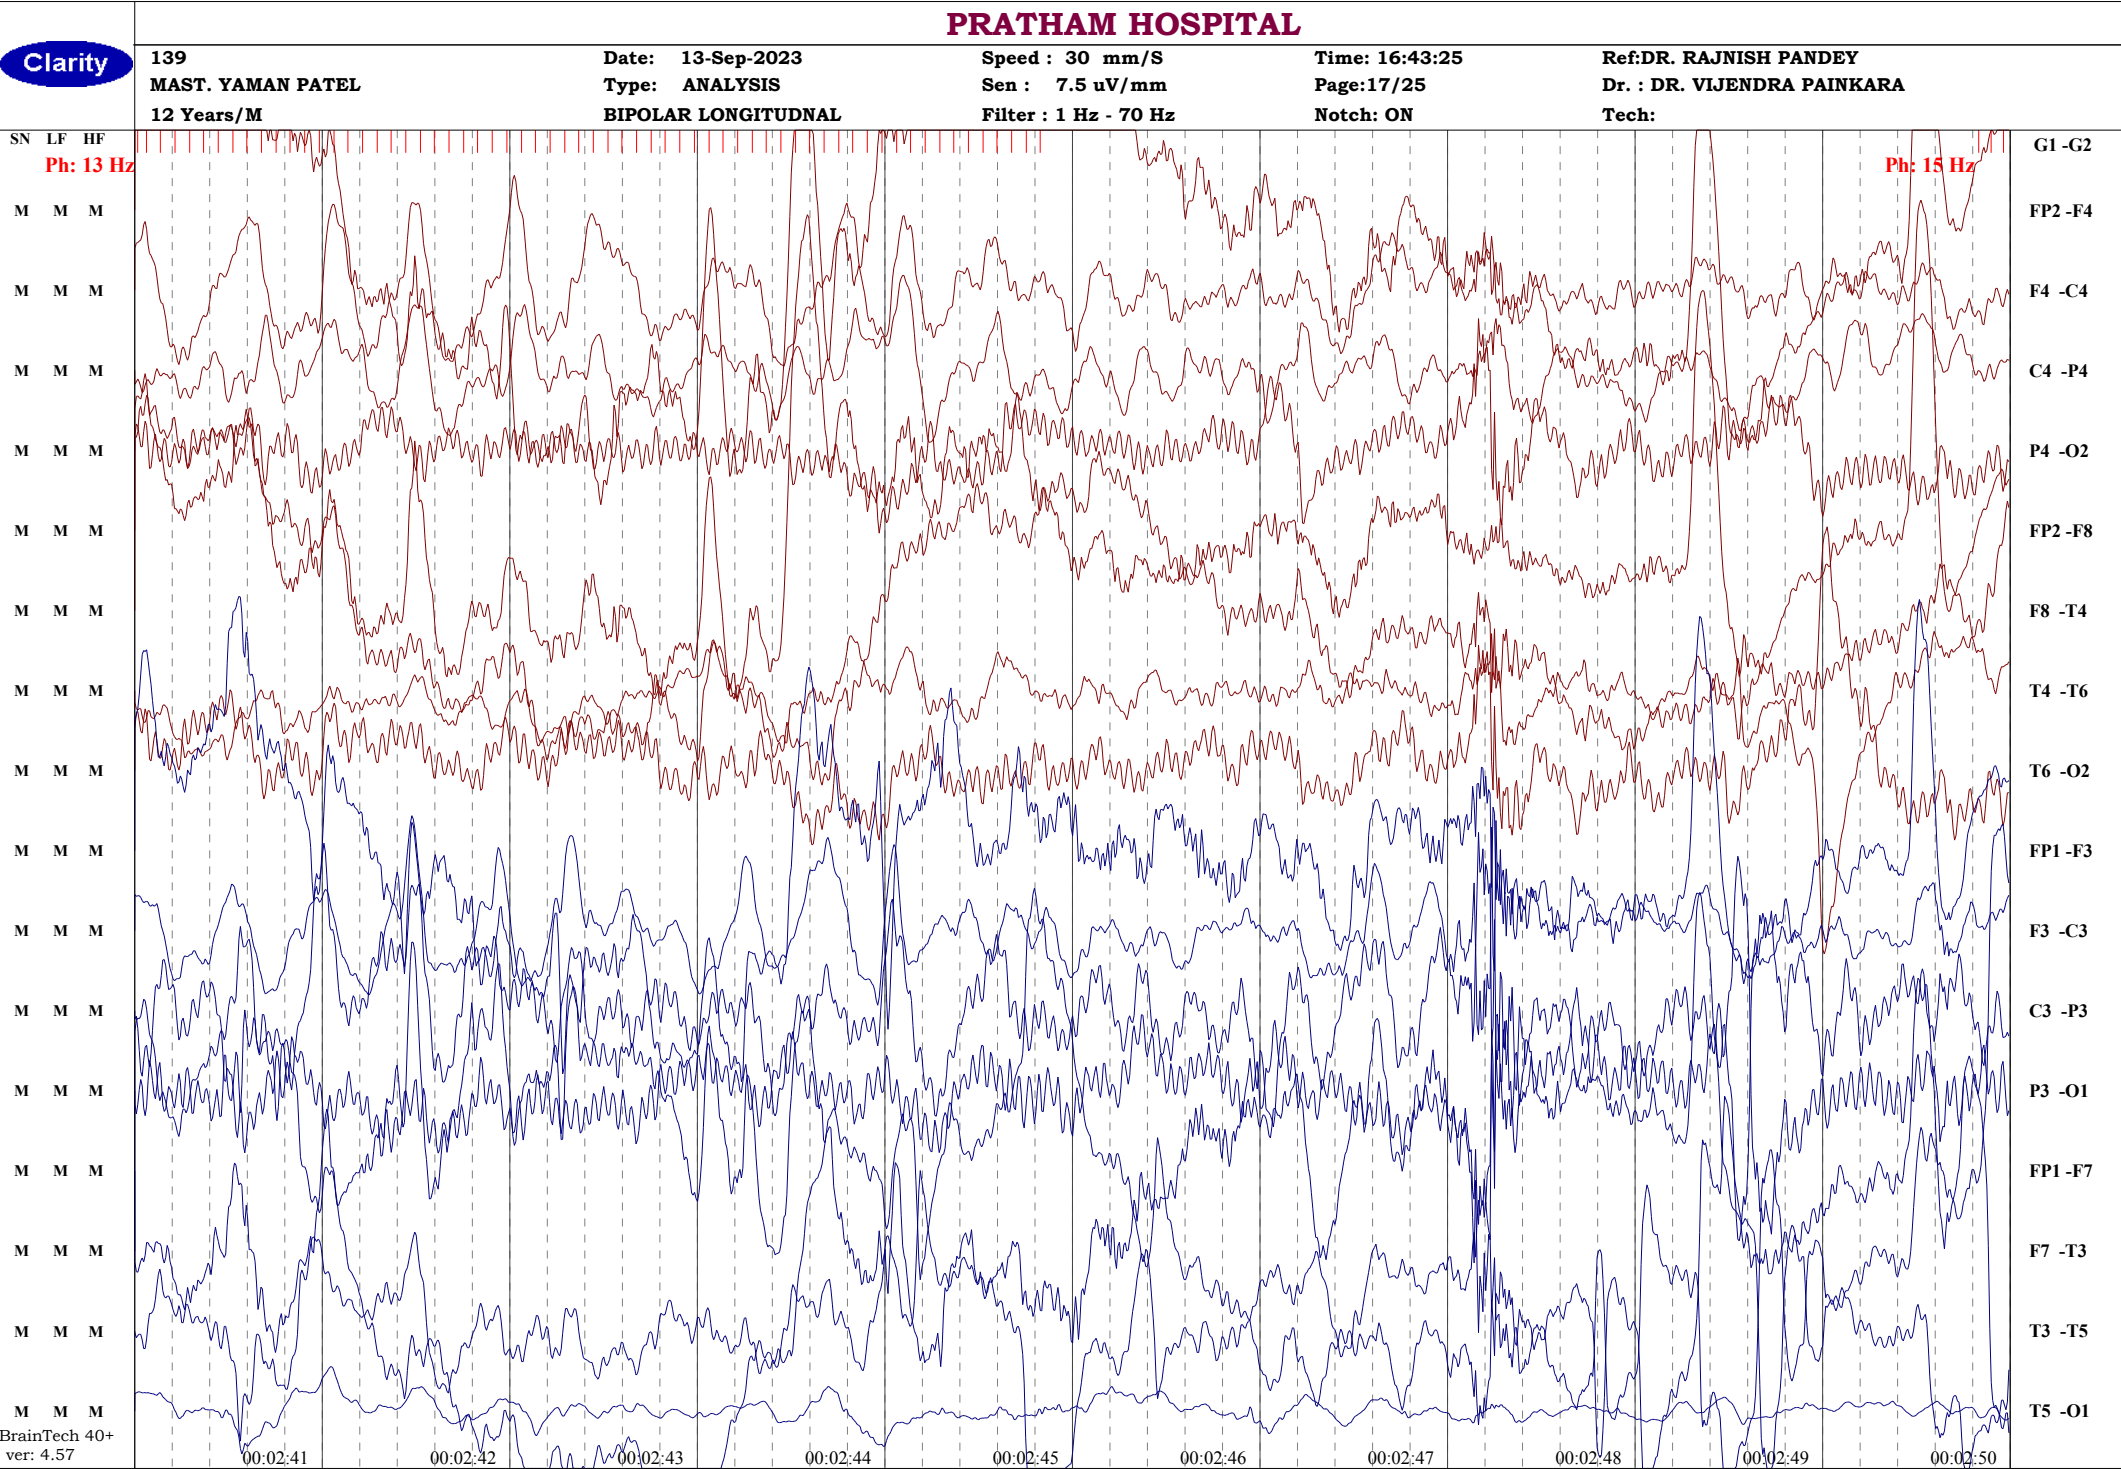

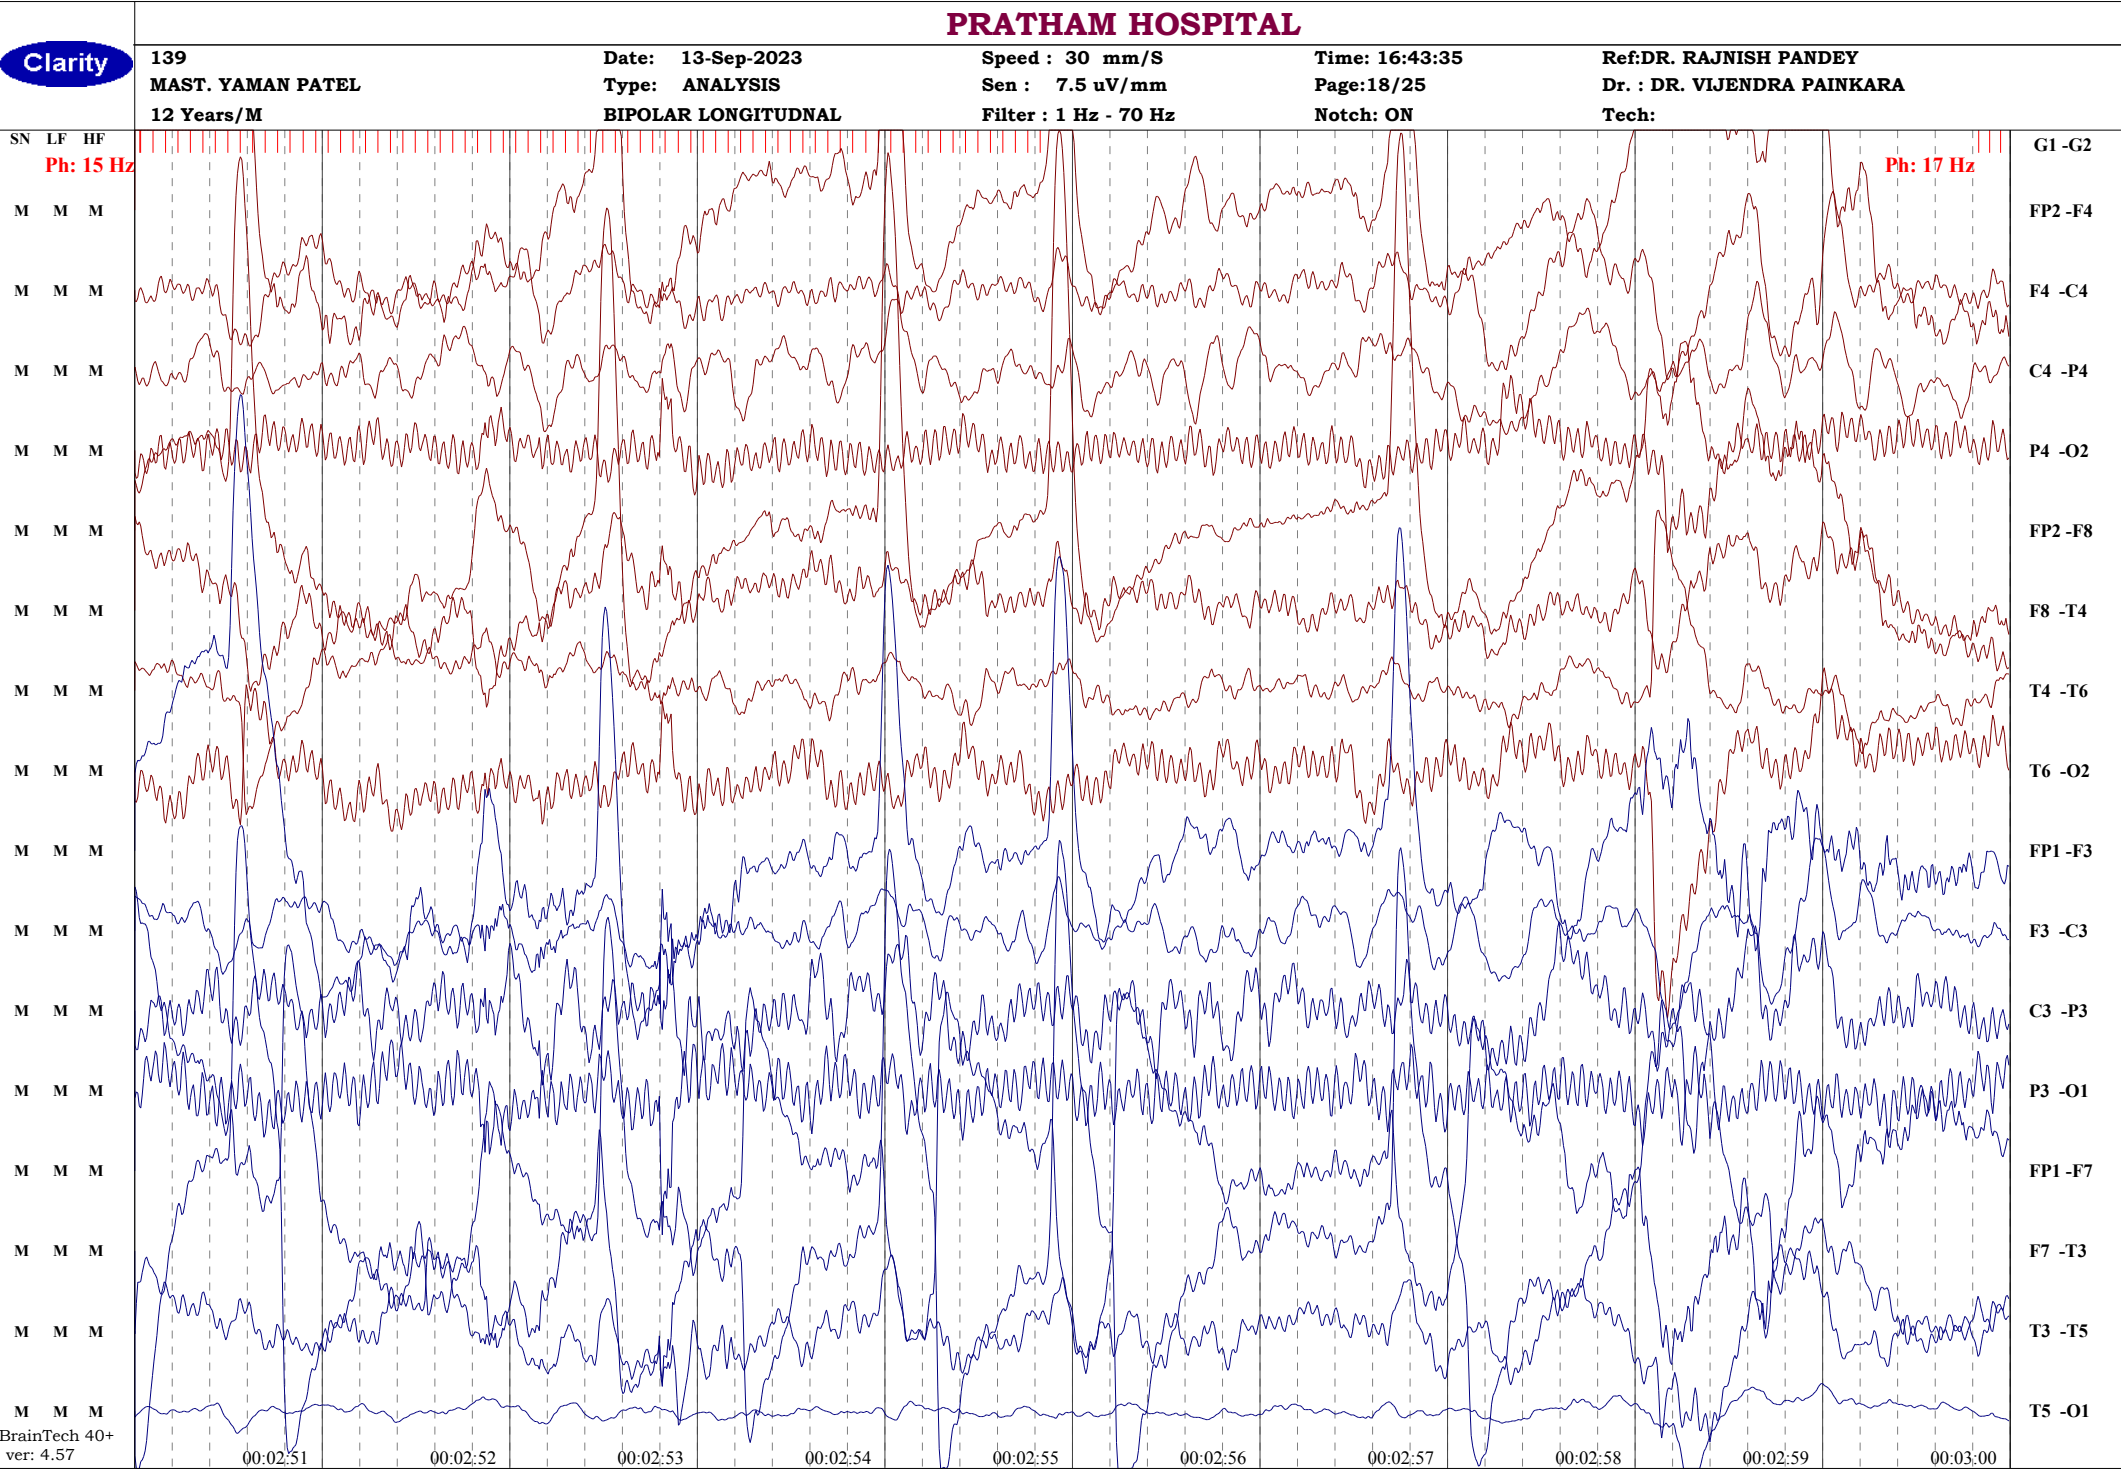

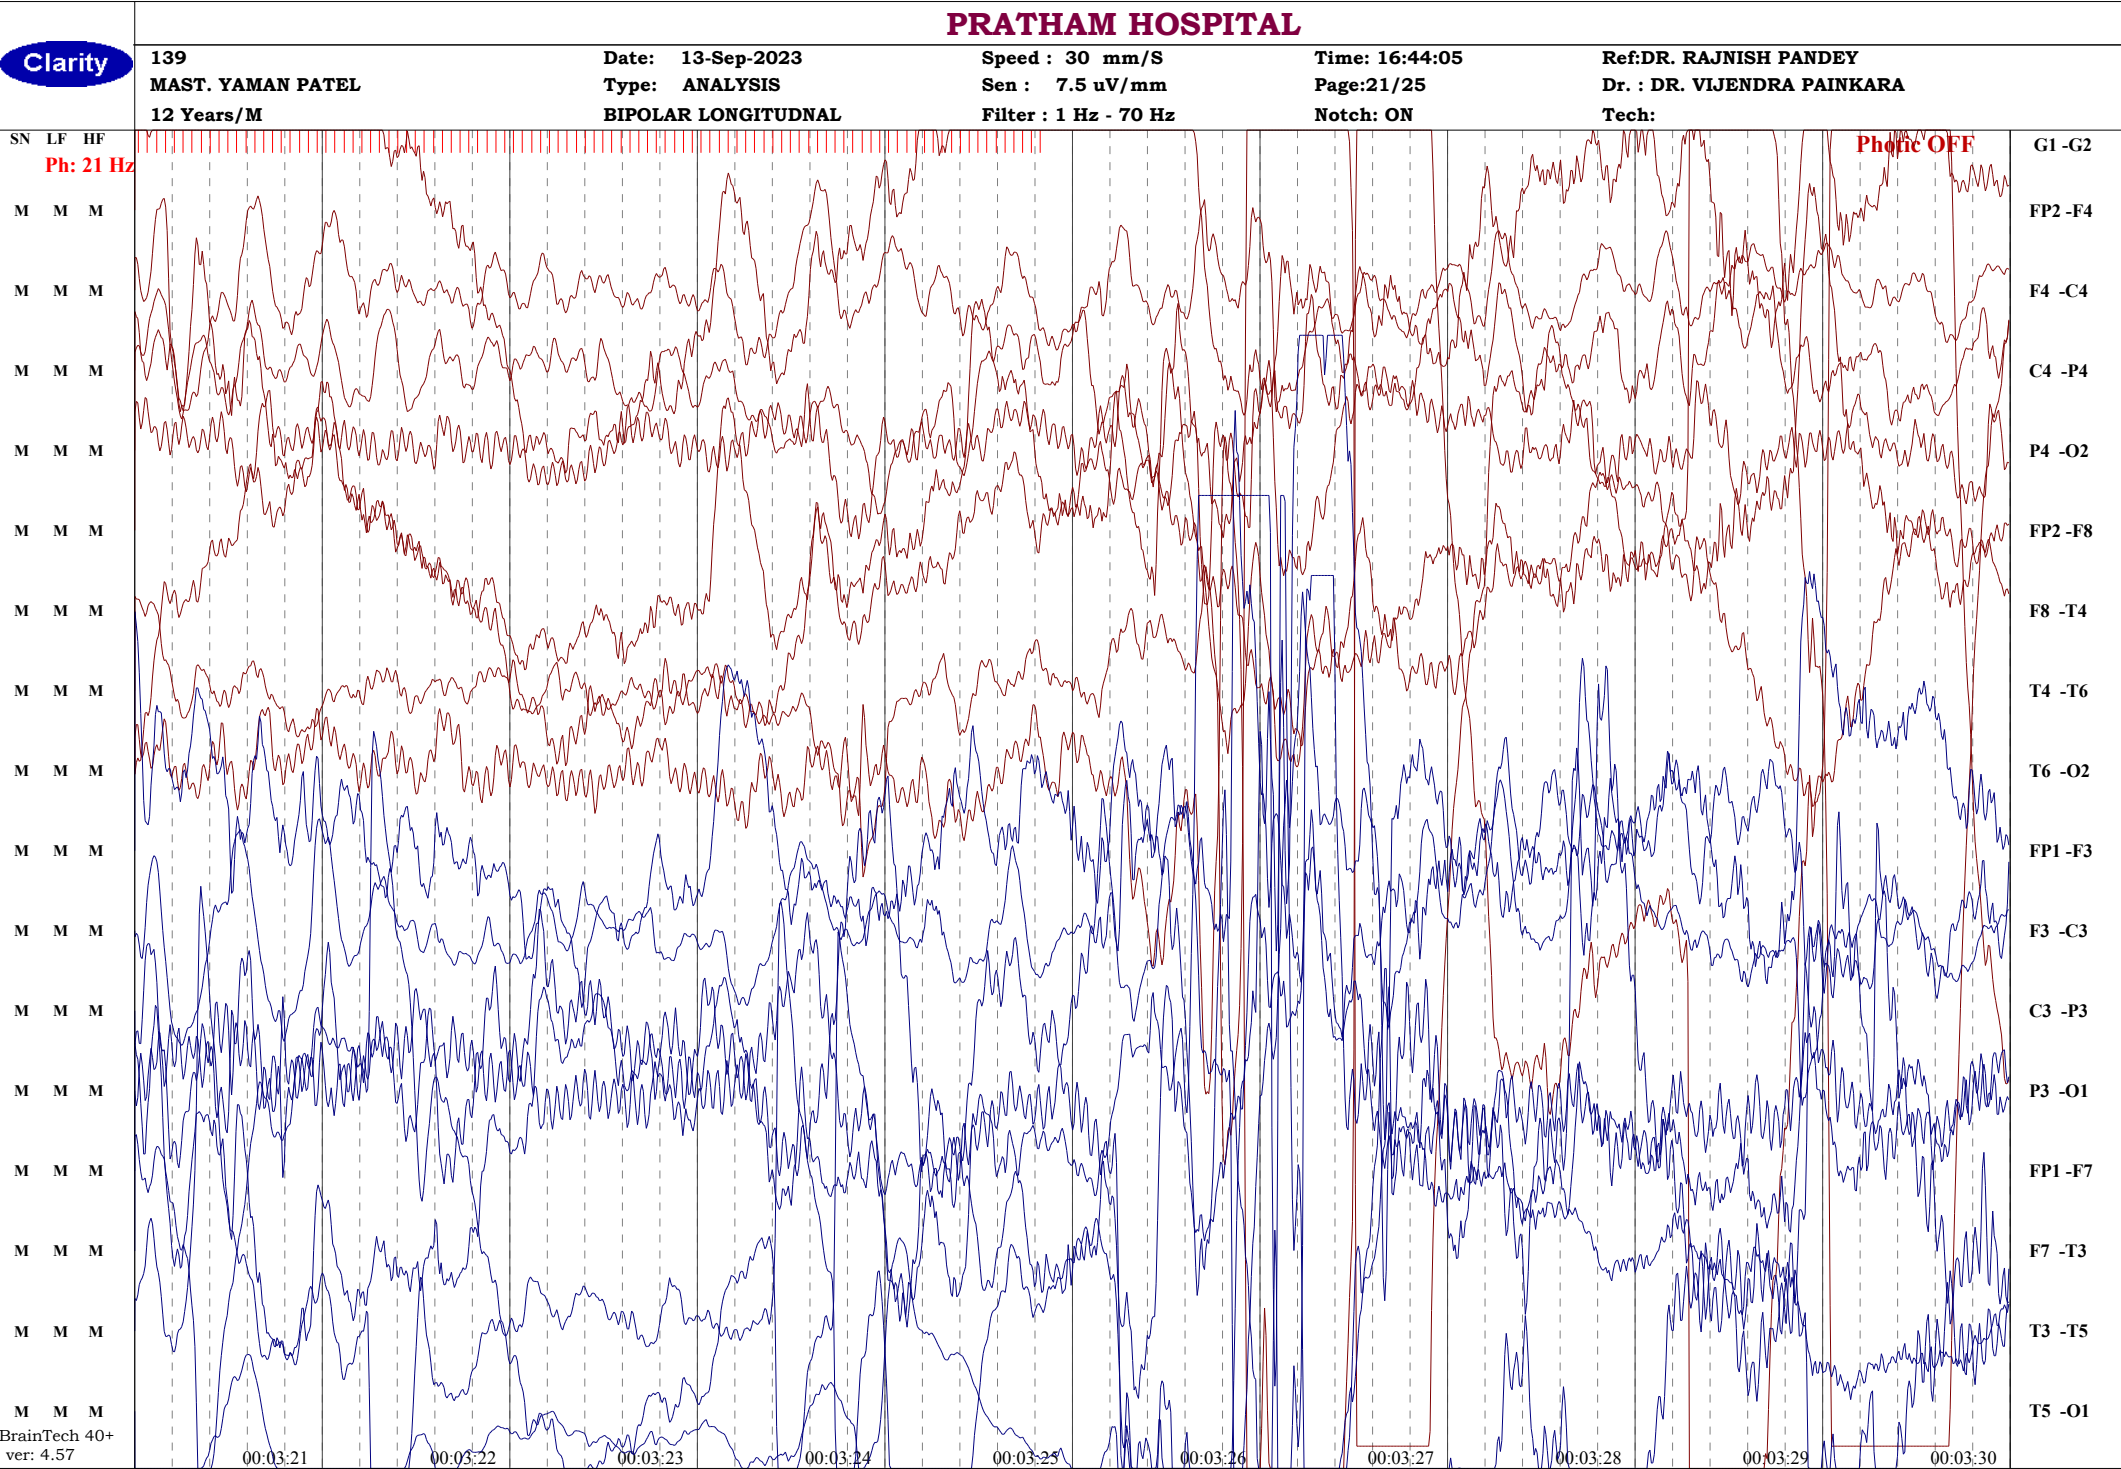

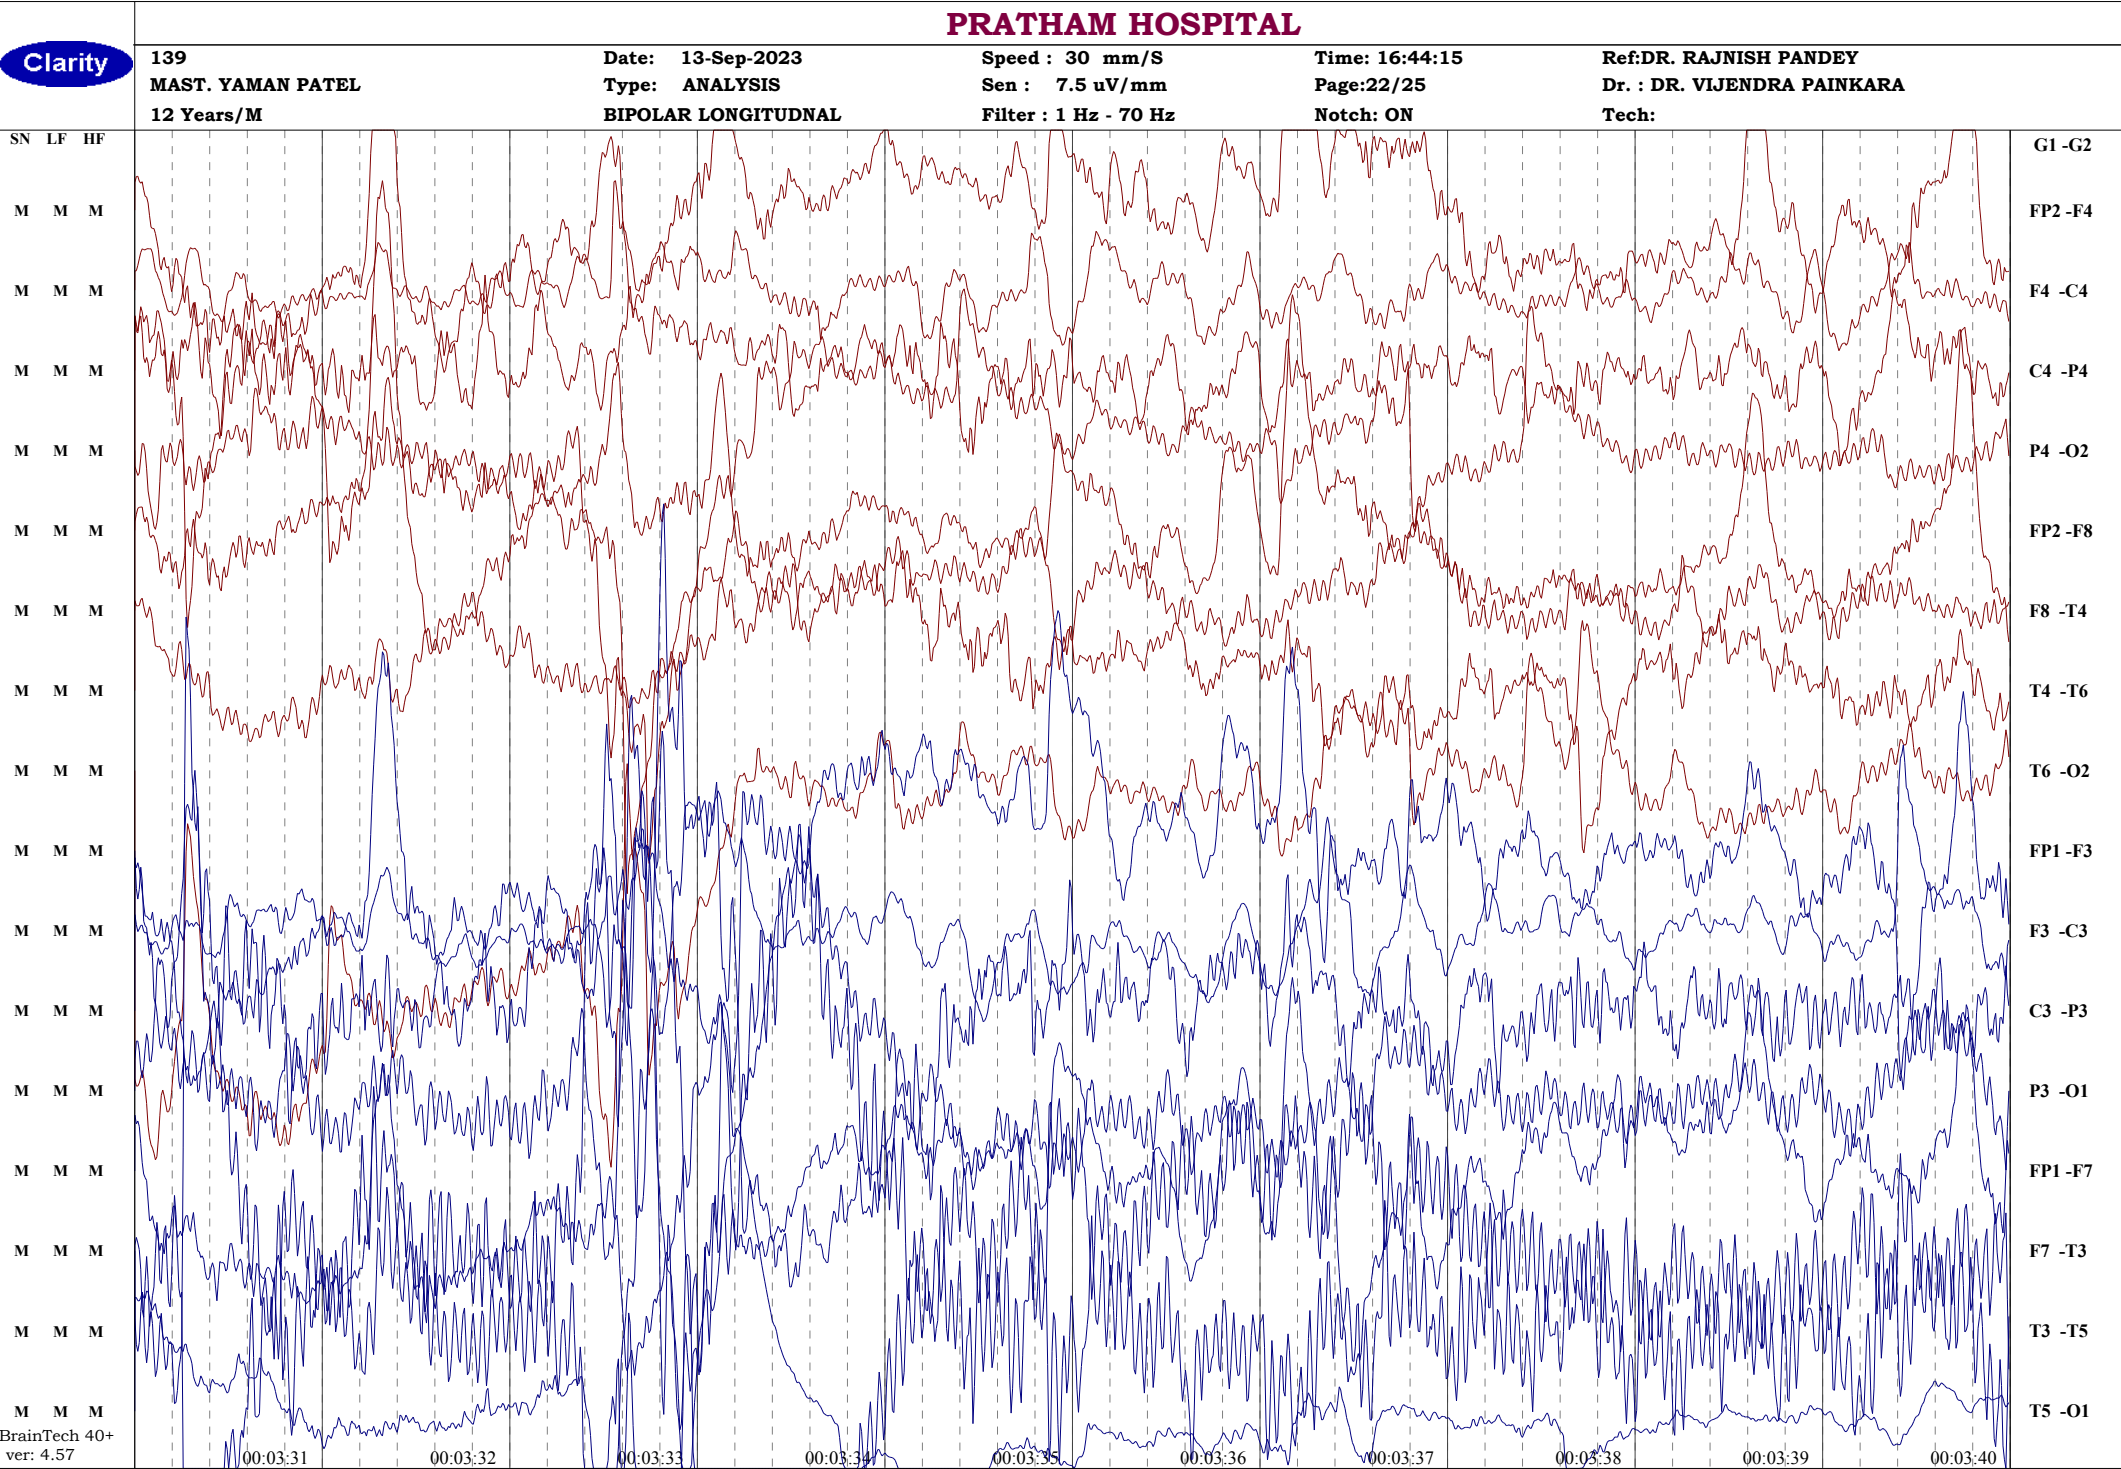

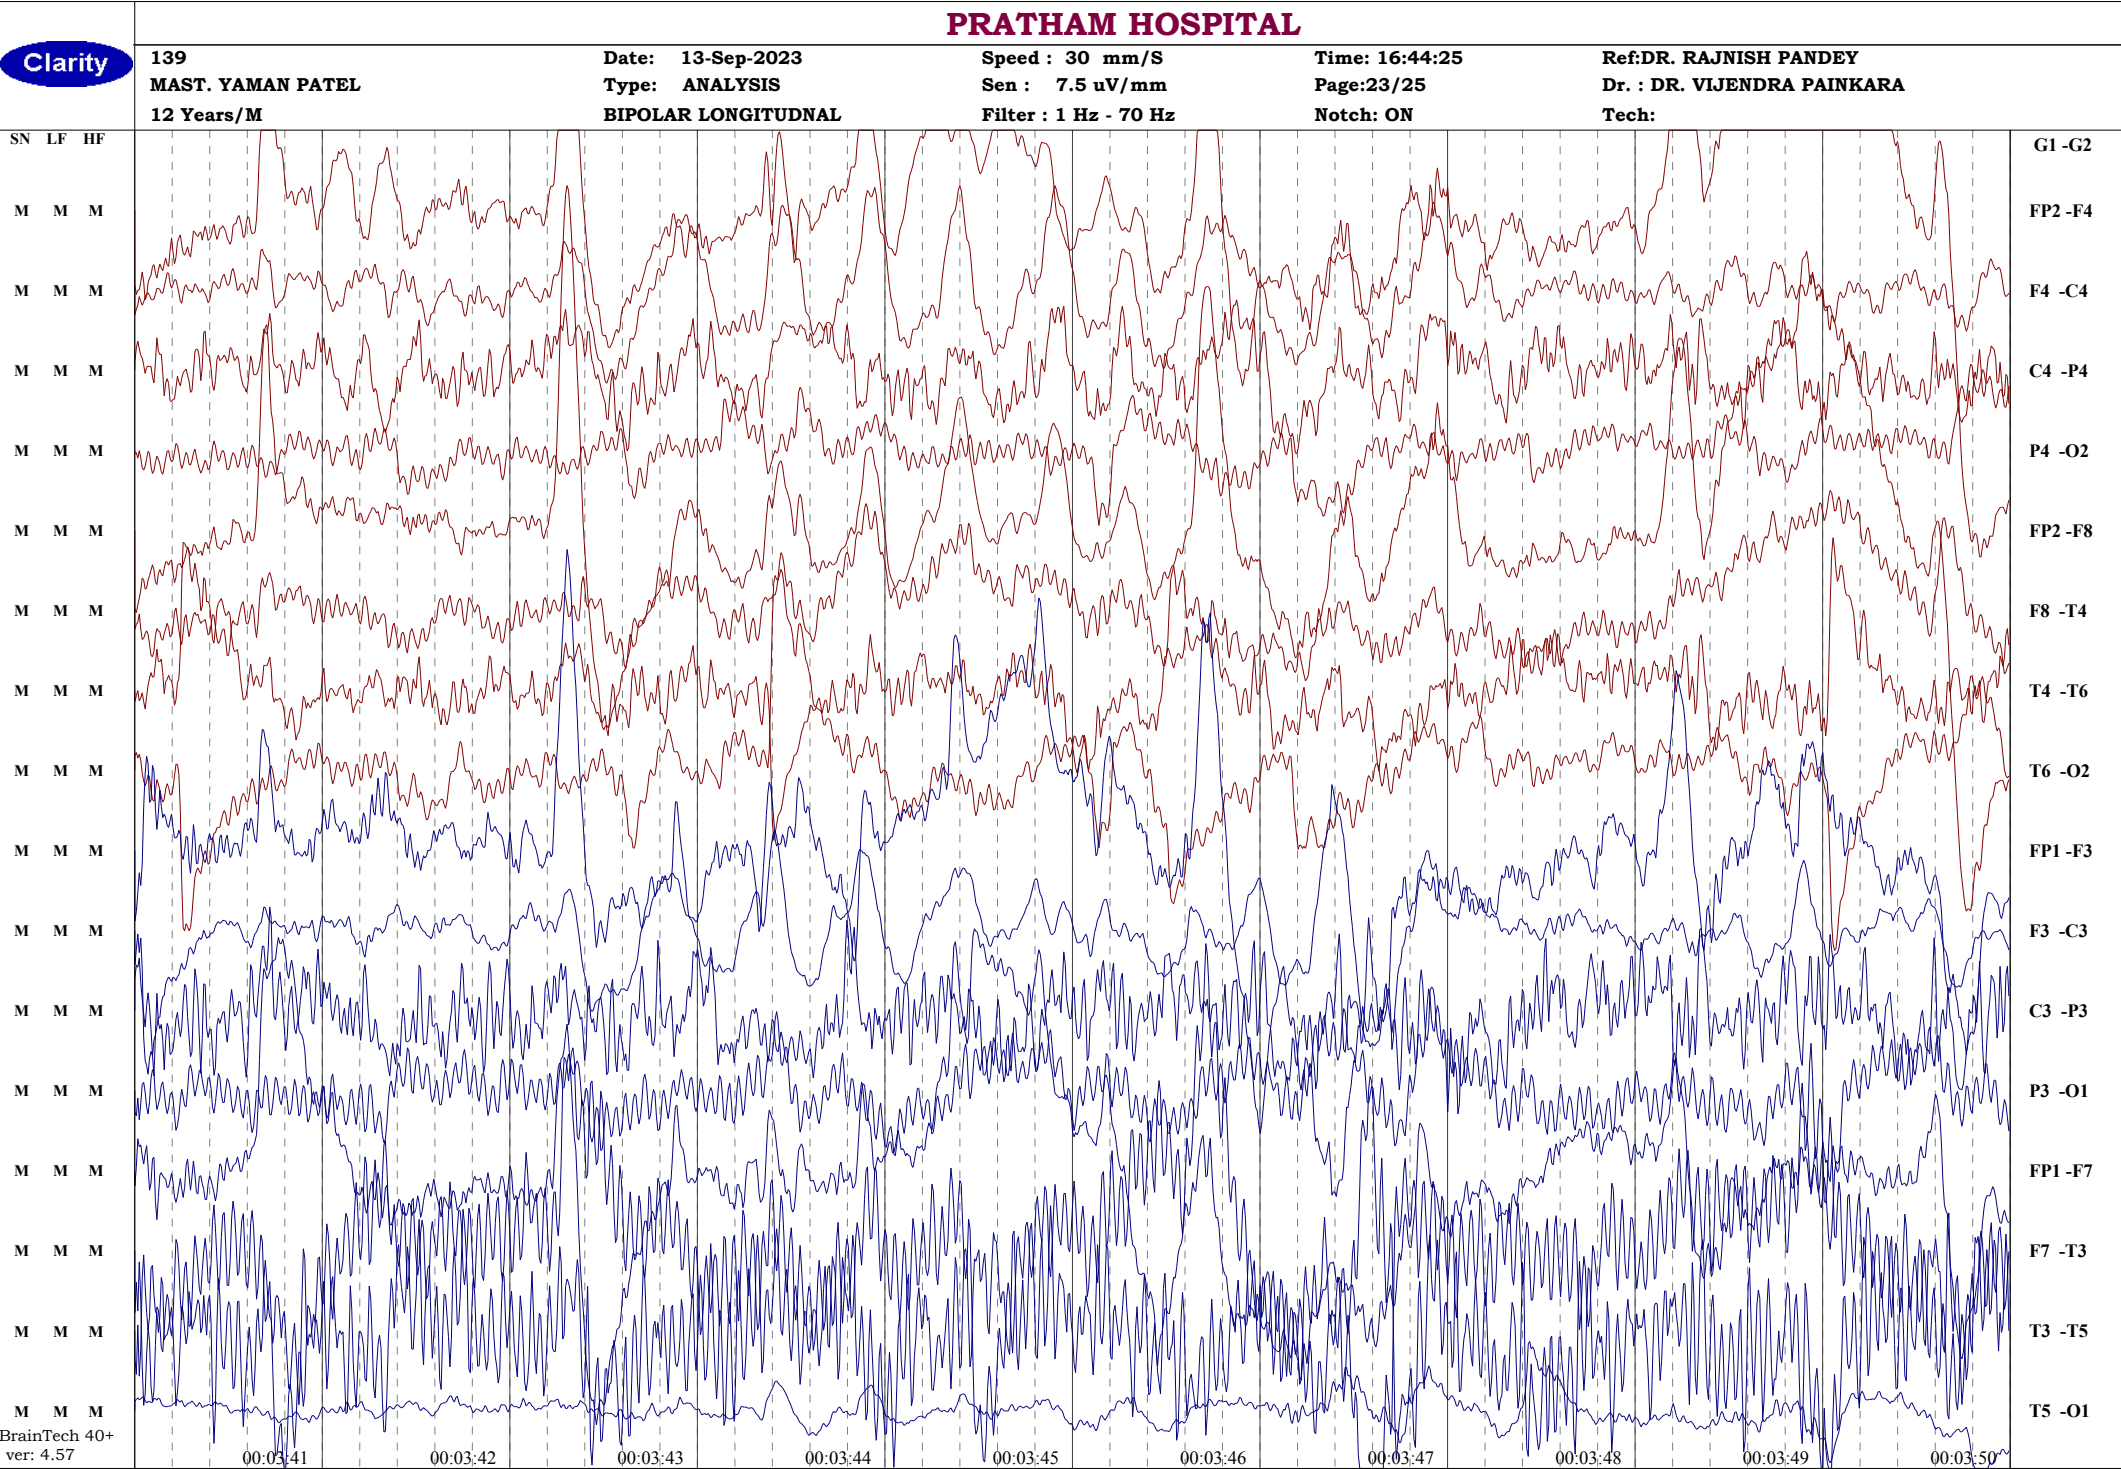

139
MAST. YAMAN PATEL
12 Years/M

Date: 13-Sep-2023
Type: ANALYSIS
BIPOLAR LONGITUDNAL

Speed : 30 mm/S
Sen : 7.5 uV/mm
Filter : 1 Hz - 70 Hz

Time: 16:44:25
Page:23/25
Notch: ON

Ref:DR. RAJNISH PANDEY
Dr. : DR. VIJENDRA PAINKARA
Tech:

