


66  
MRS. RANJUSHREE SENGUPTA  
62 Years/F

Date: 15-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 09:40:00  
Page:2/40  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

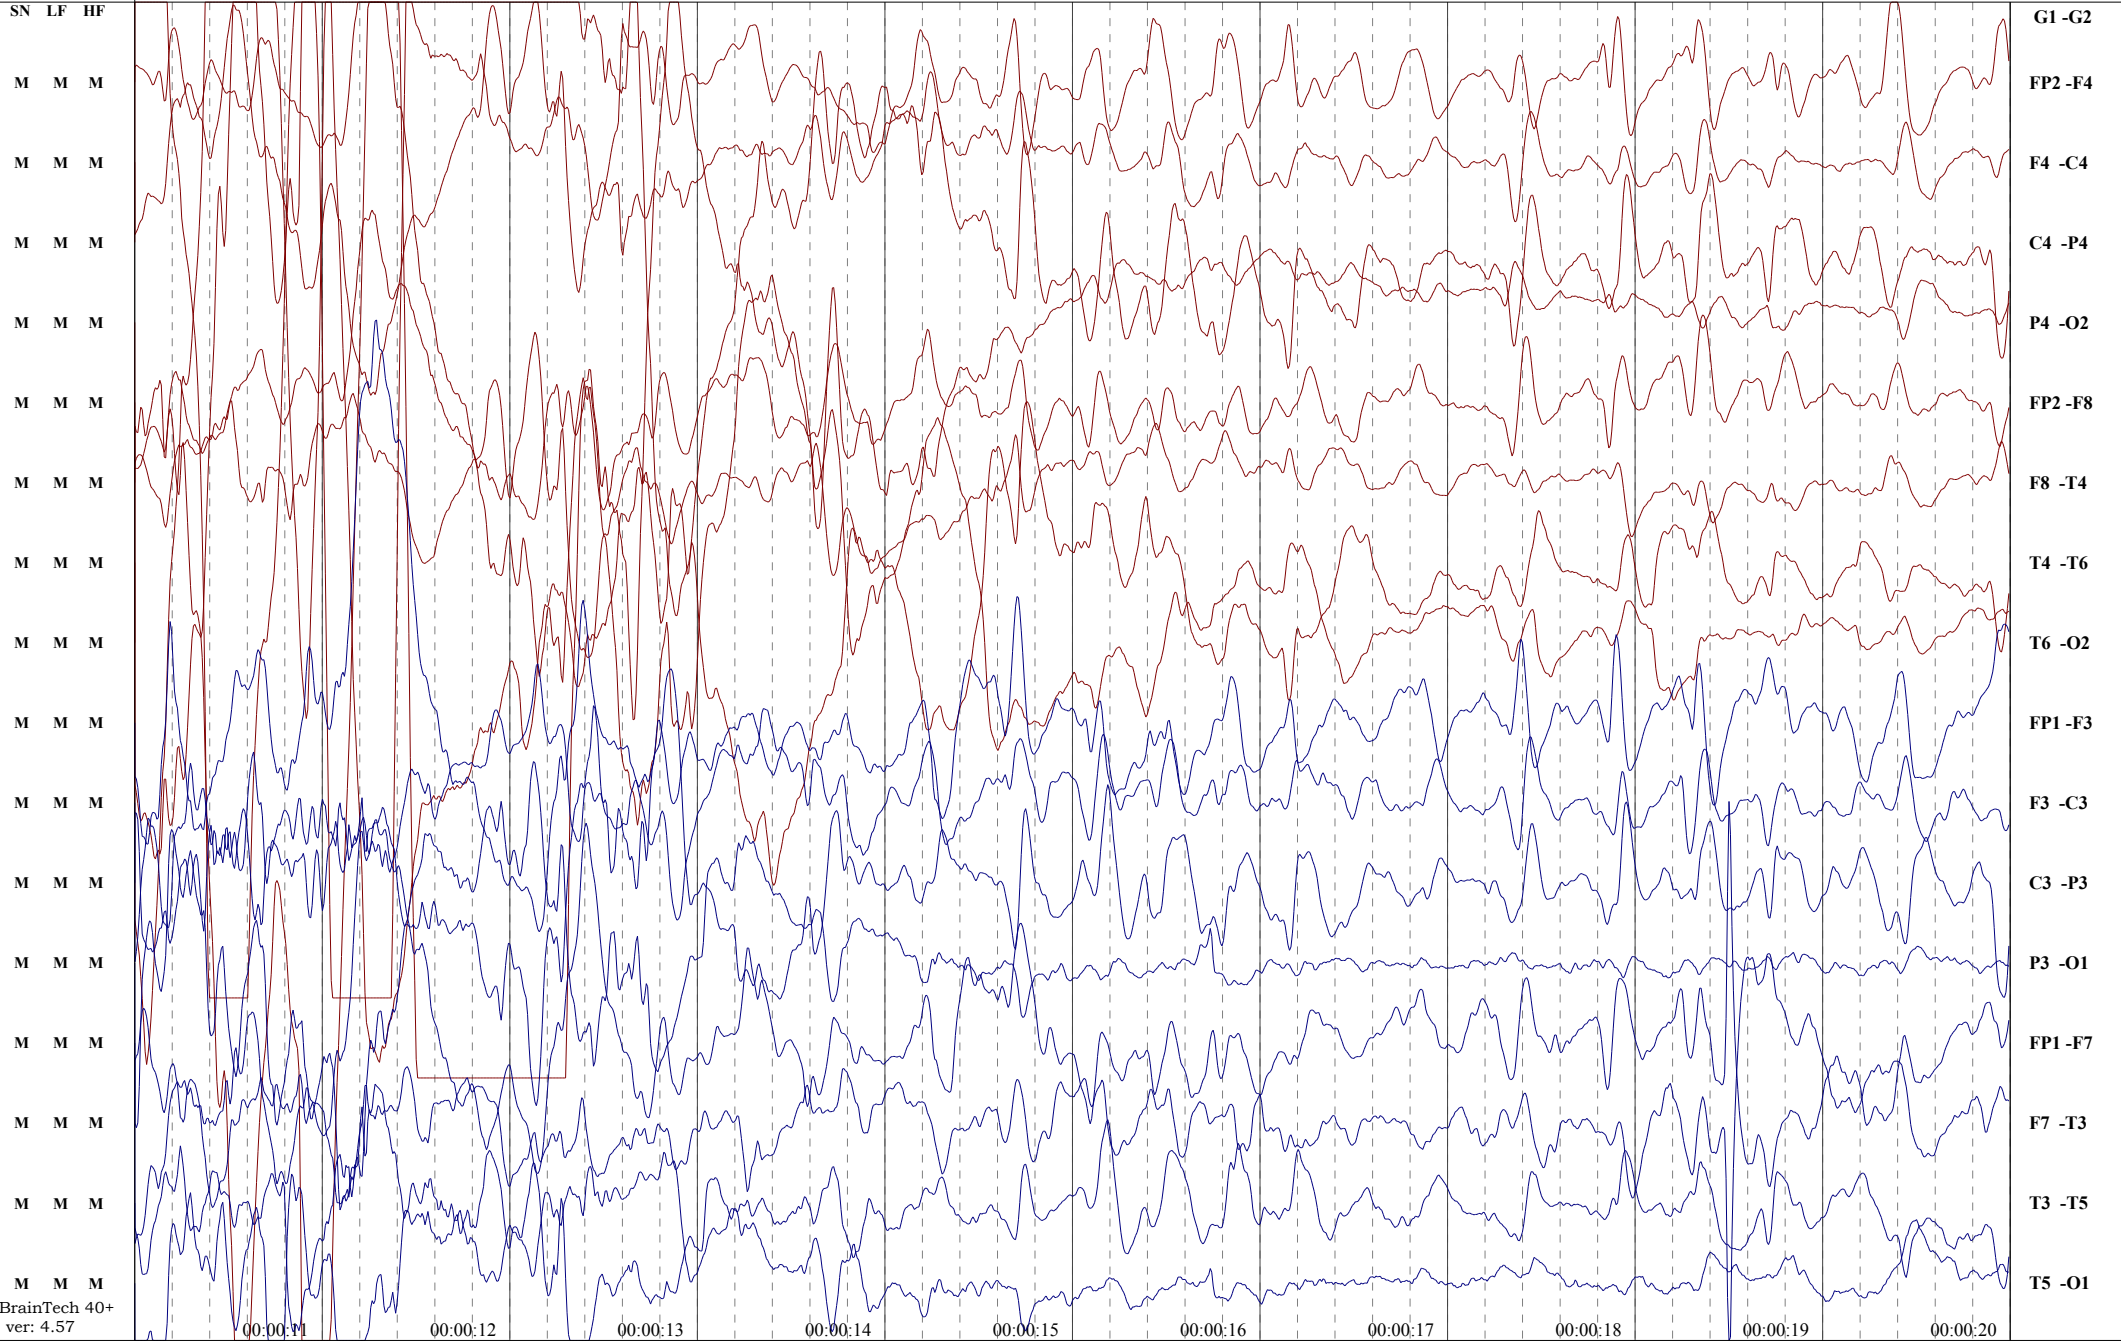


66  
MRS. RANJUSHREE SENGUPTA  
62 Years/F


Date: 15-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 09:40:10  
Page:3/40  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

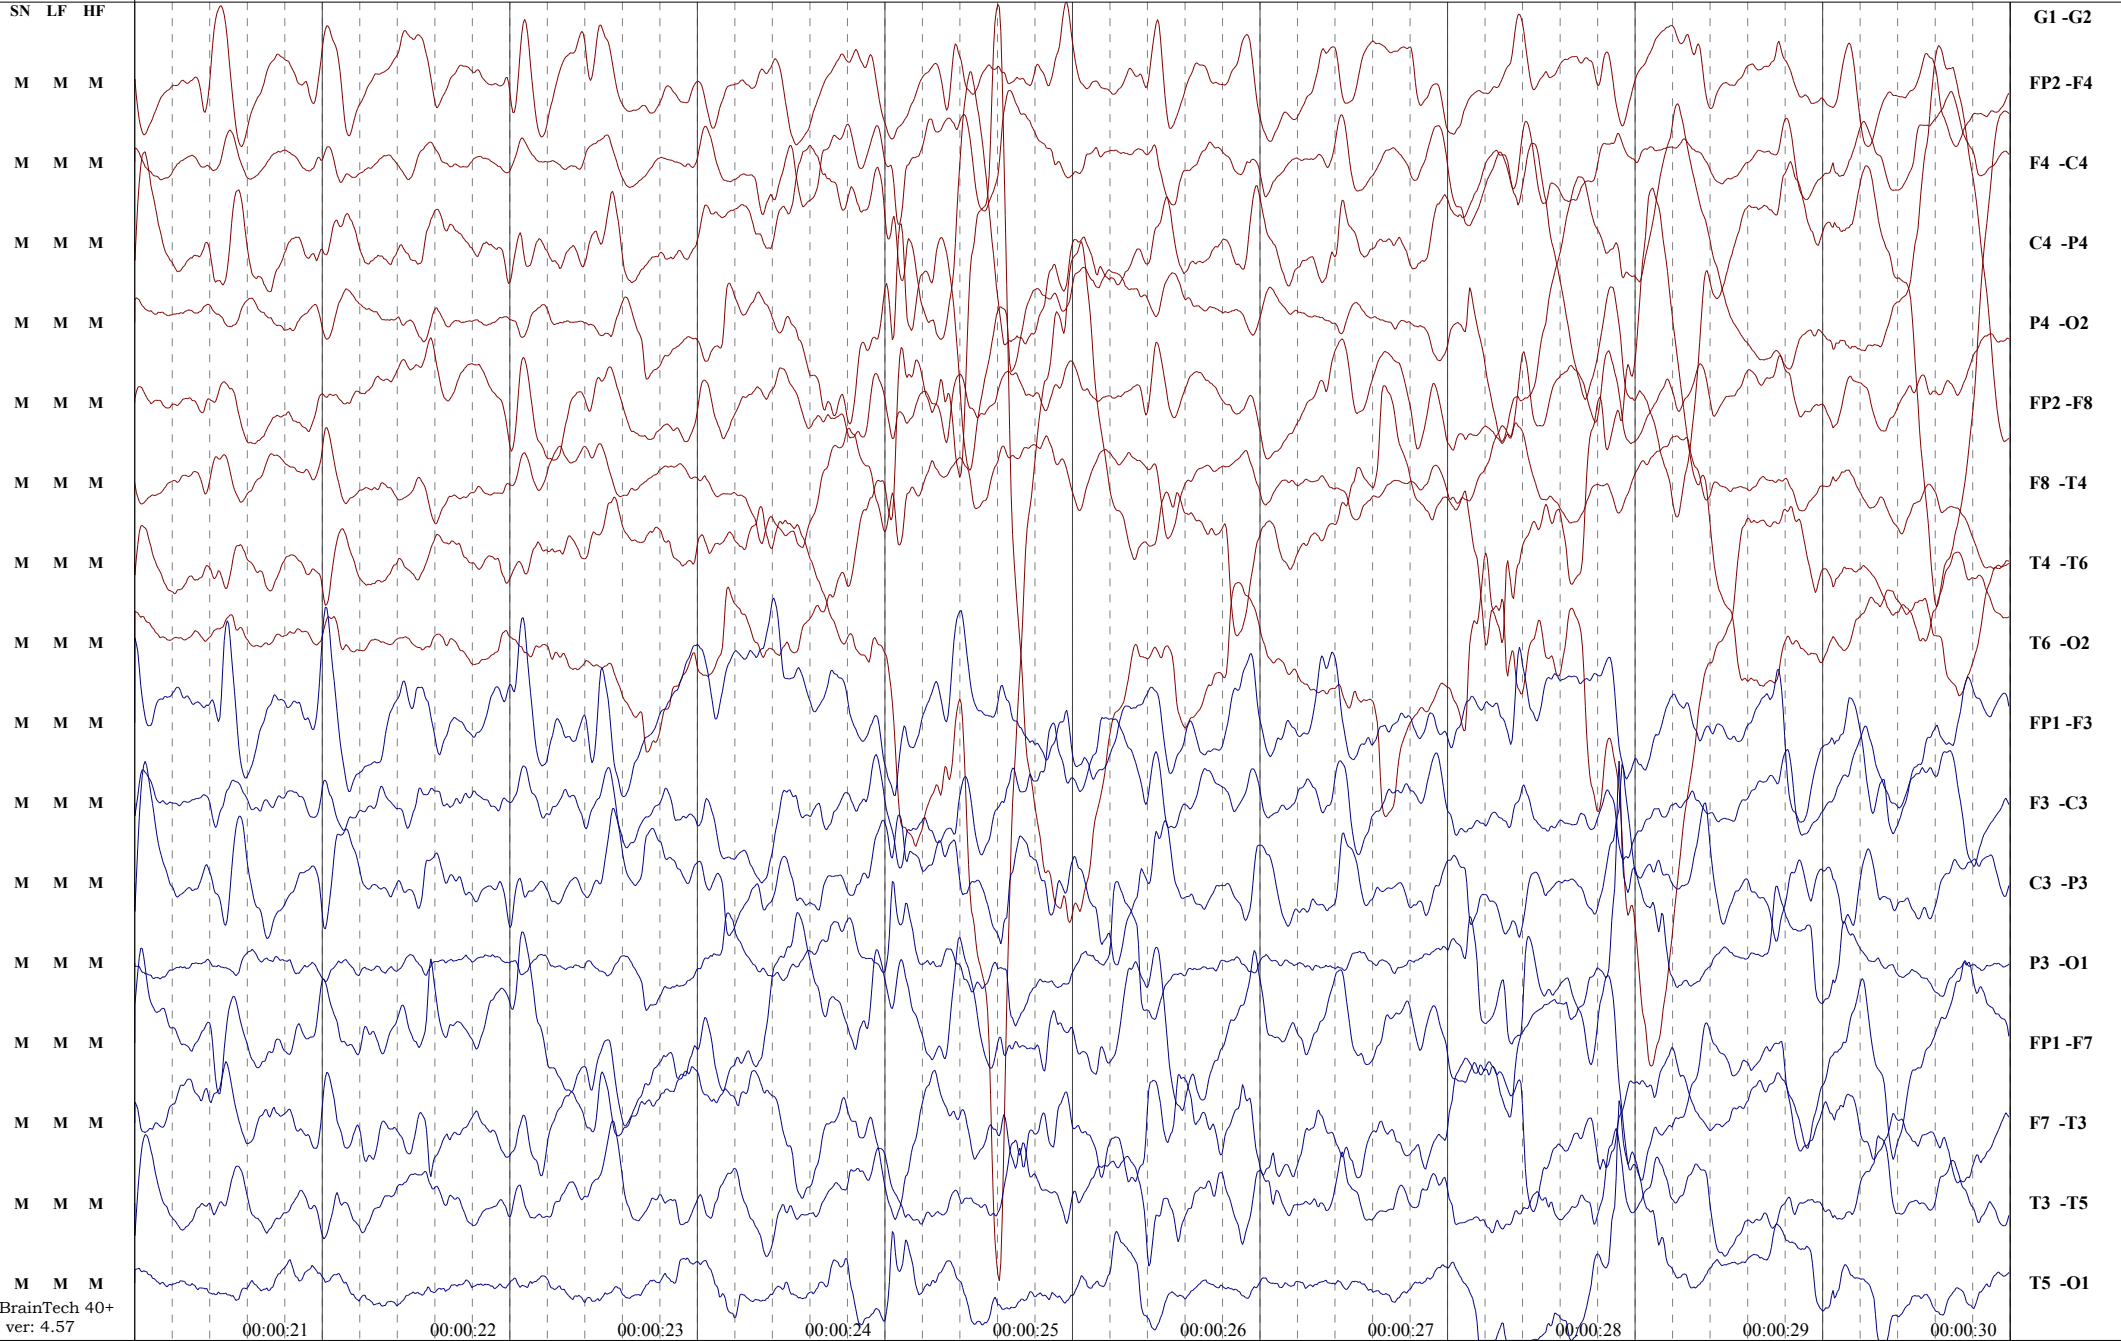

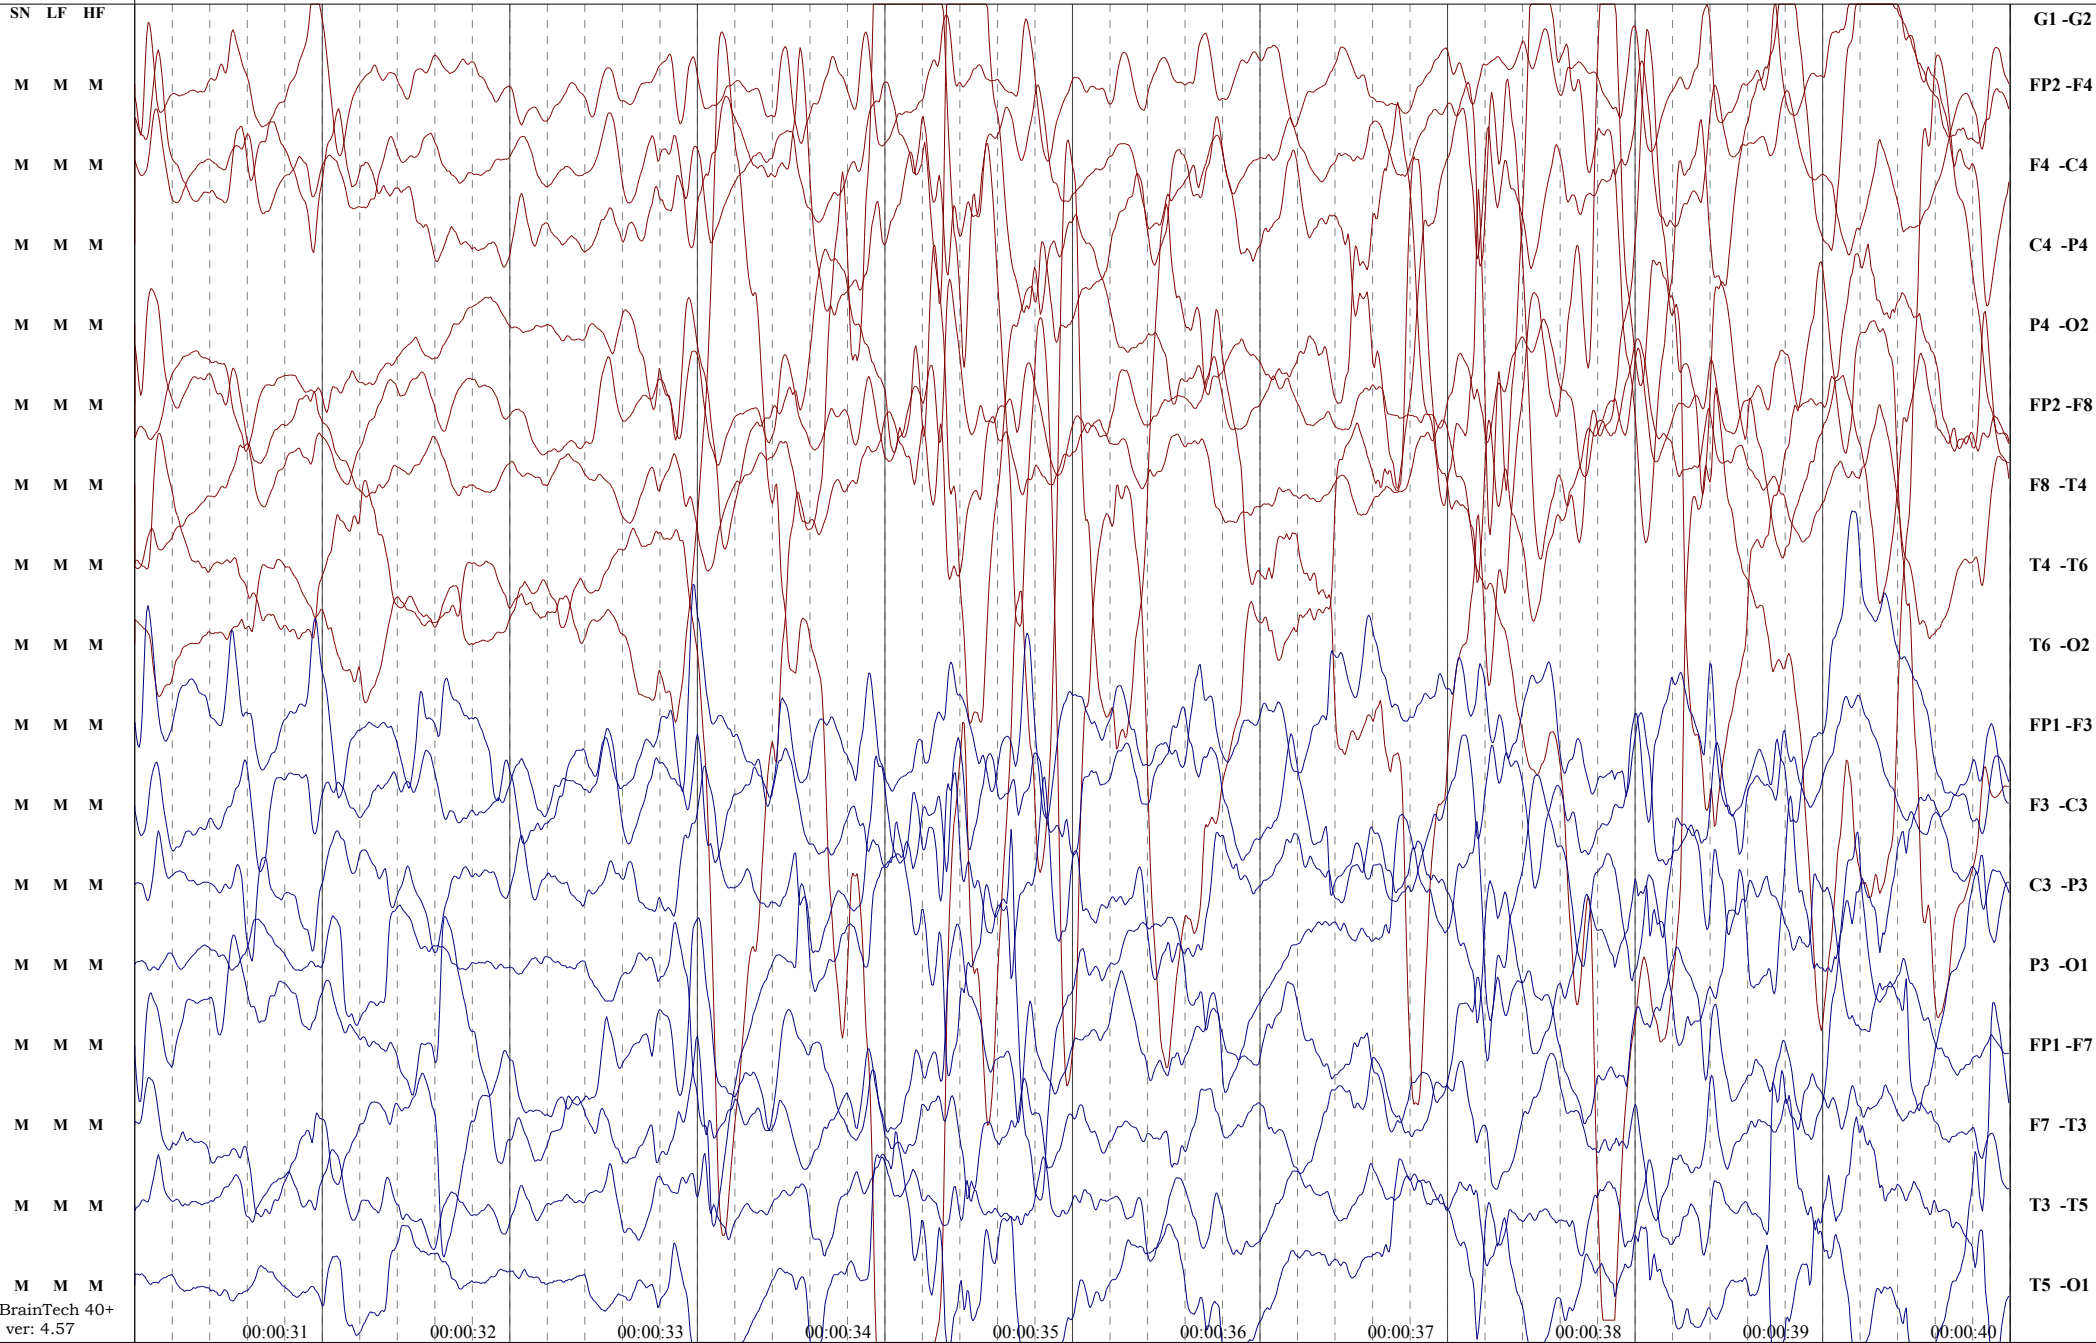






66  
MRS. RANJUSHREE SENGUPTA  
62 Years/F

Date: 15-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 09:40:40  
Page:6/40  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

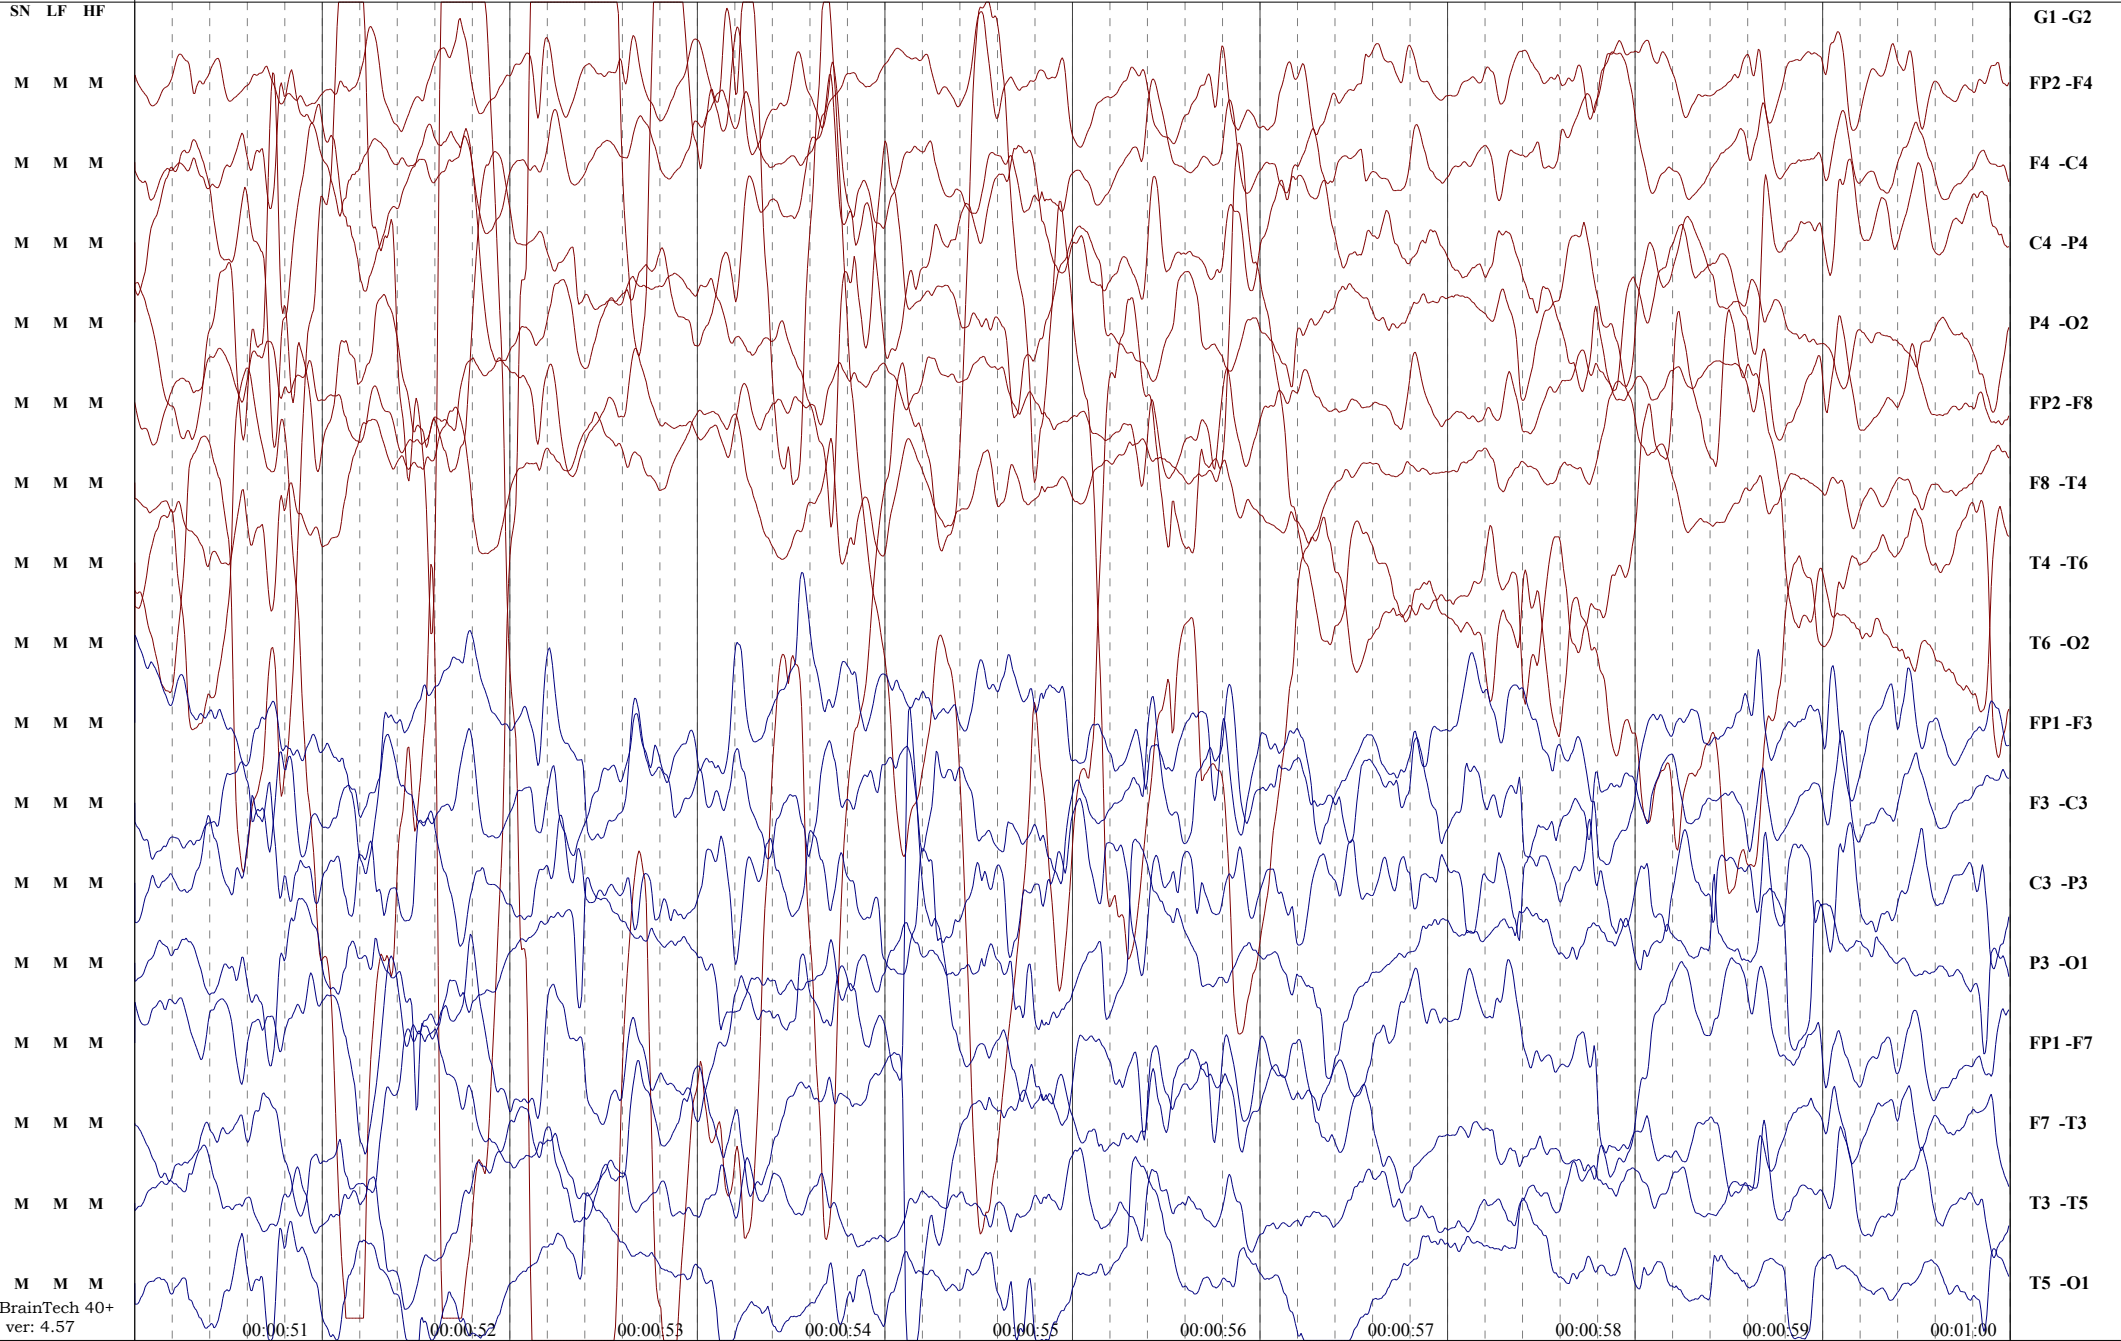


66  
MRS. RANJUSHREE SENGUPTA  
62 Years/F


Date: 15-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 09:40:50  
Page:7/40  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

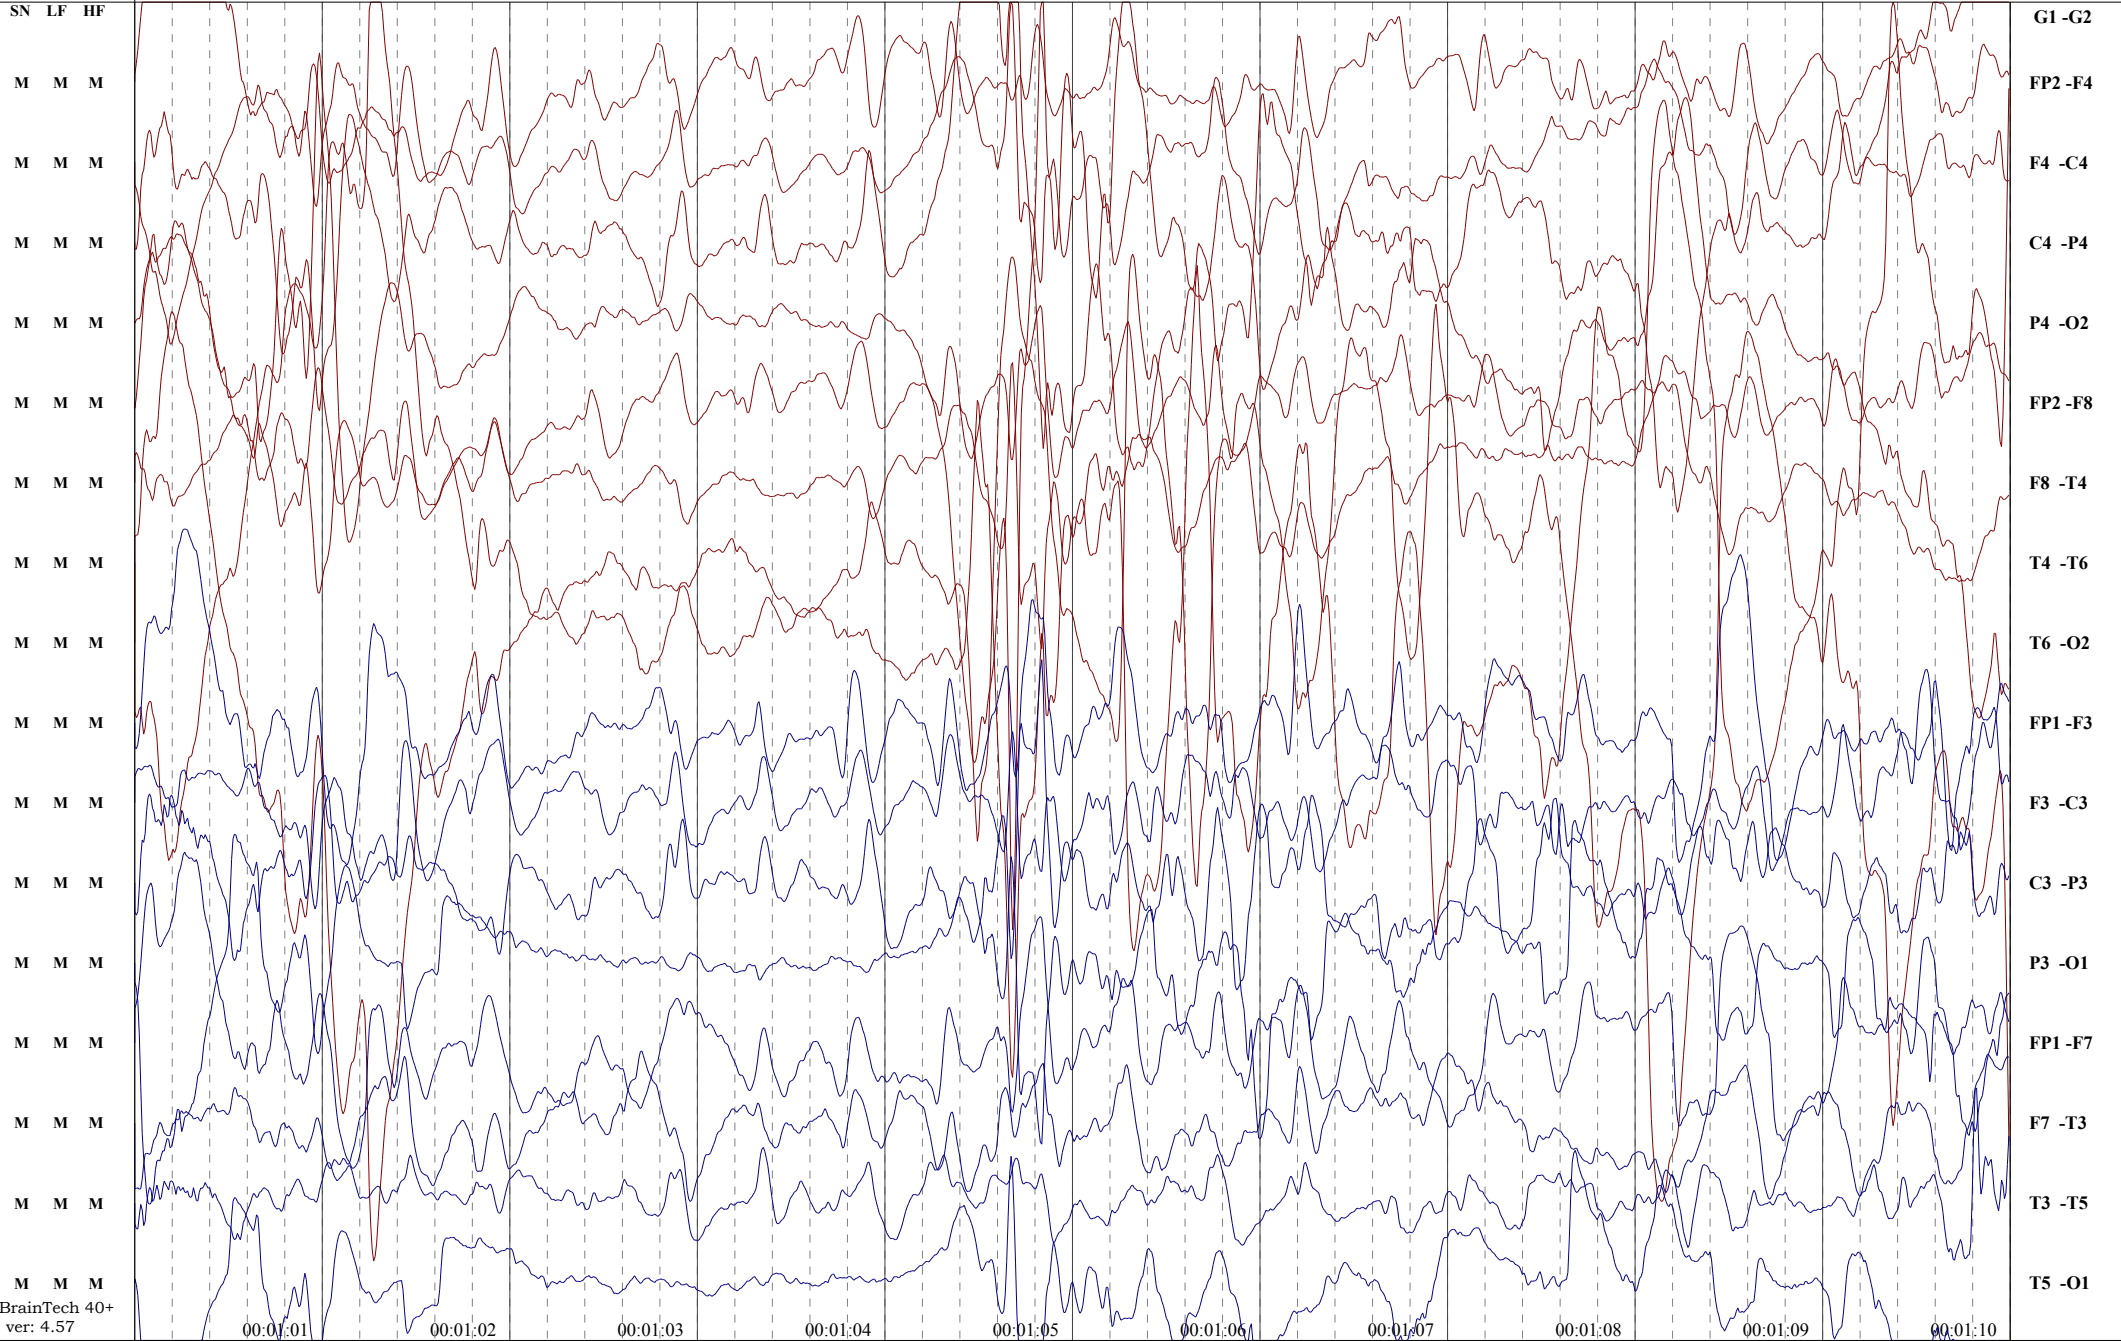

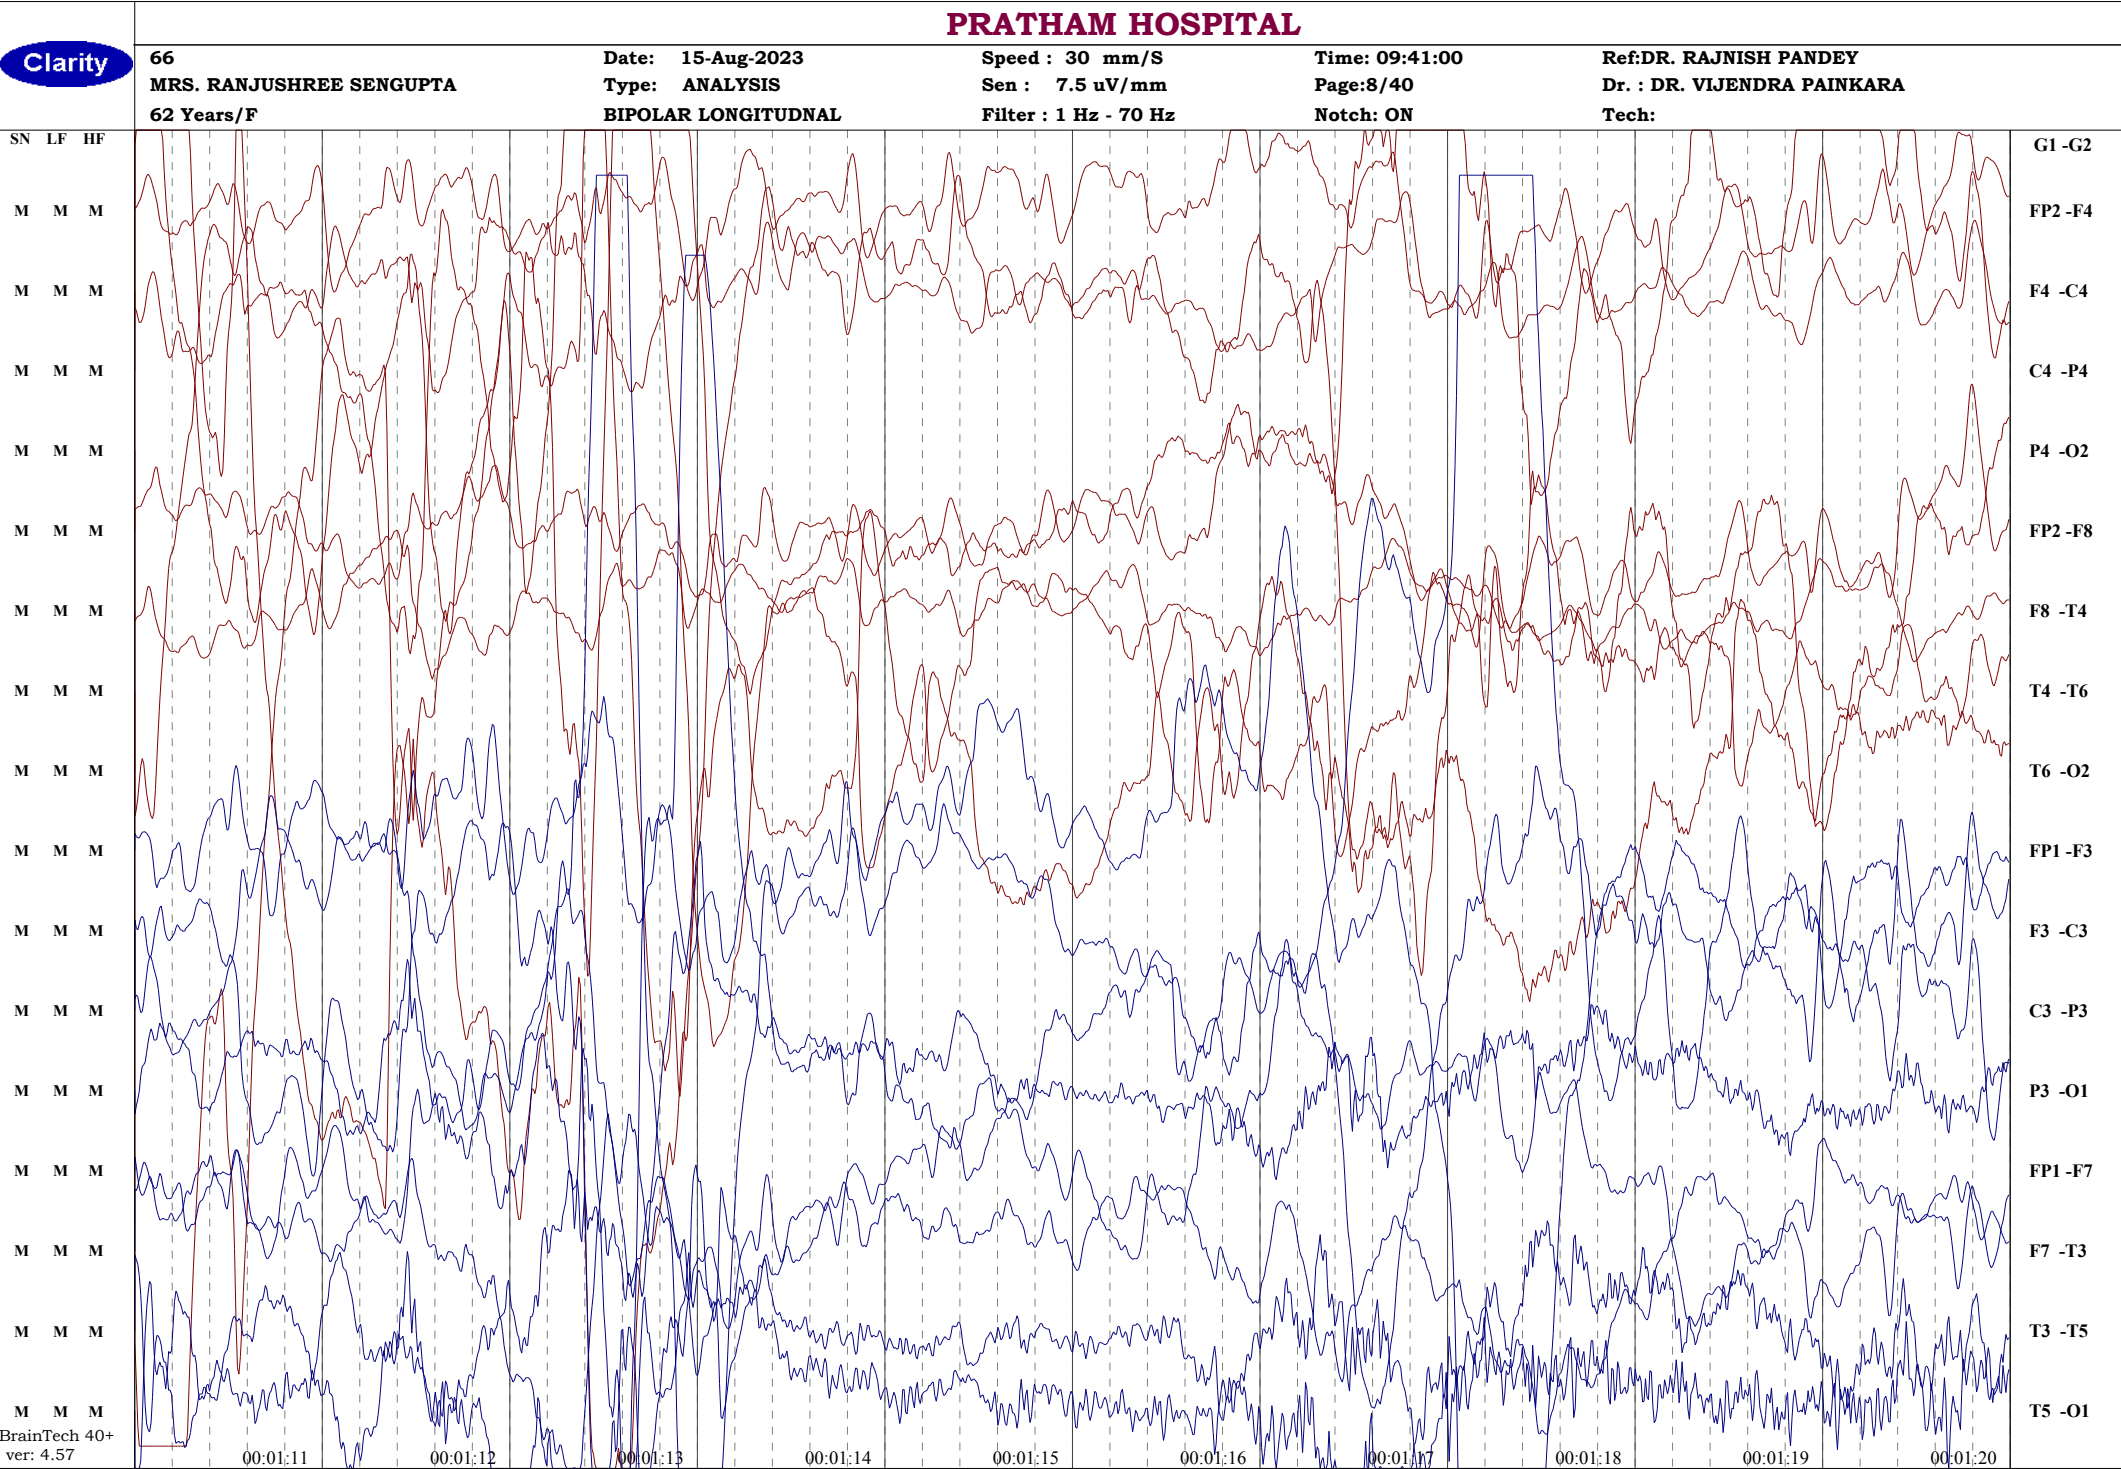




66  
MRS. RANJUSHREE SENGUPTA  
62 Years/F


Date: 15-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL


Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 09:41:10  
Page:9/40  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

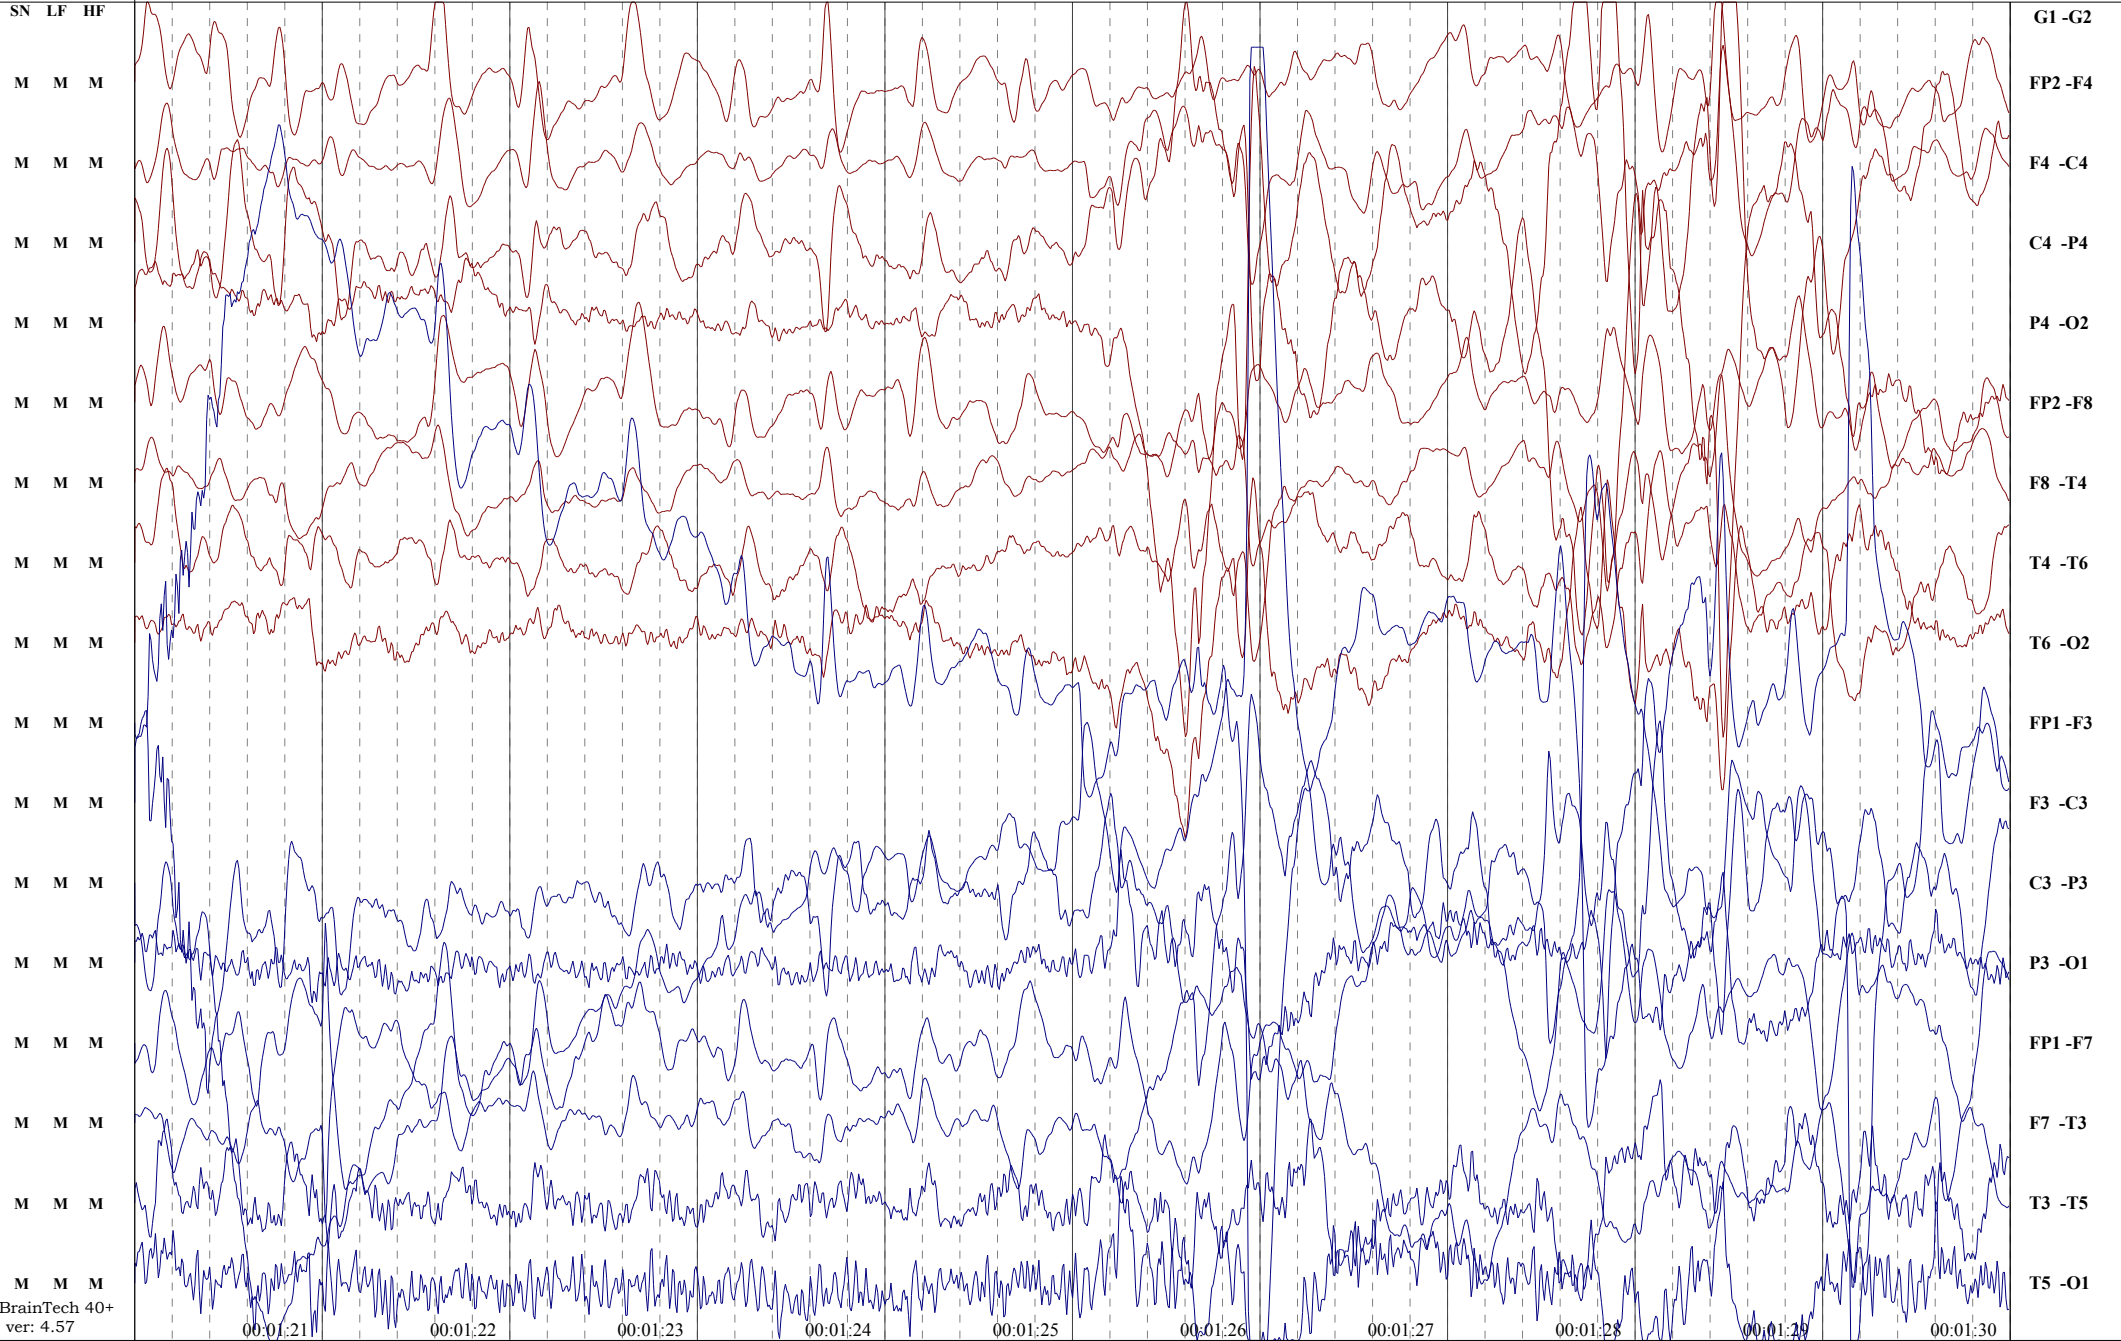

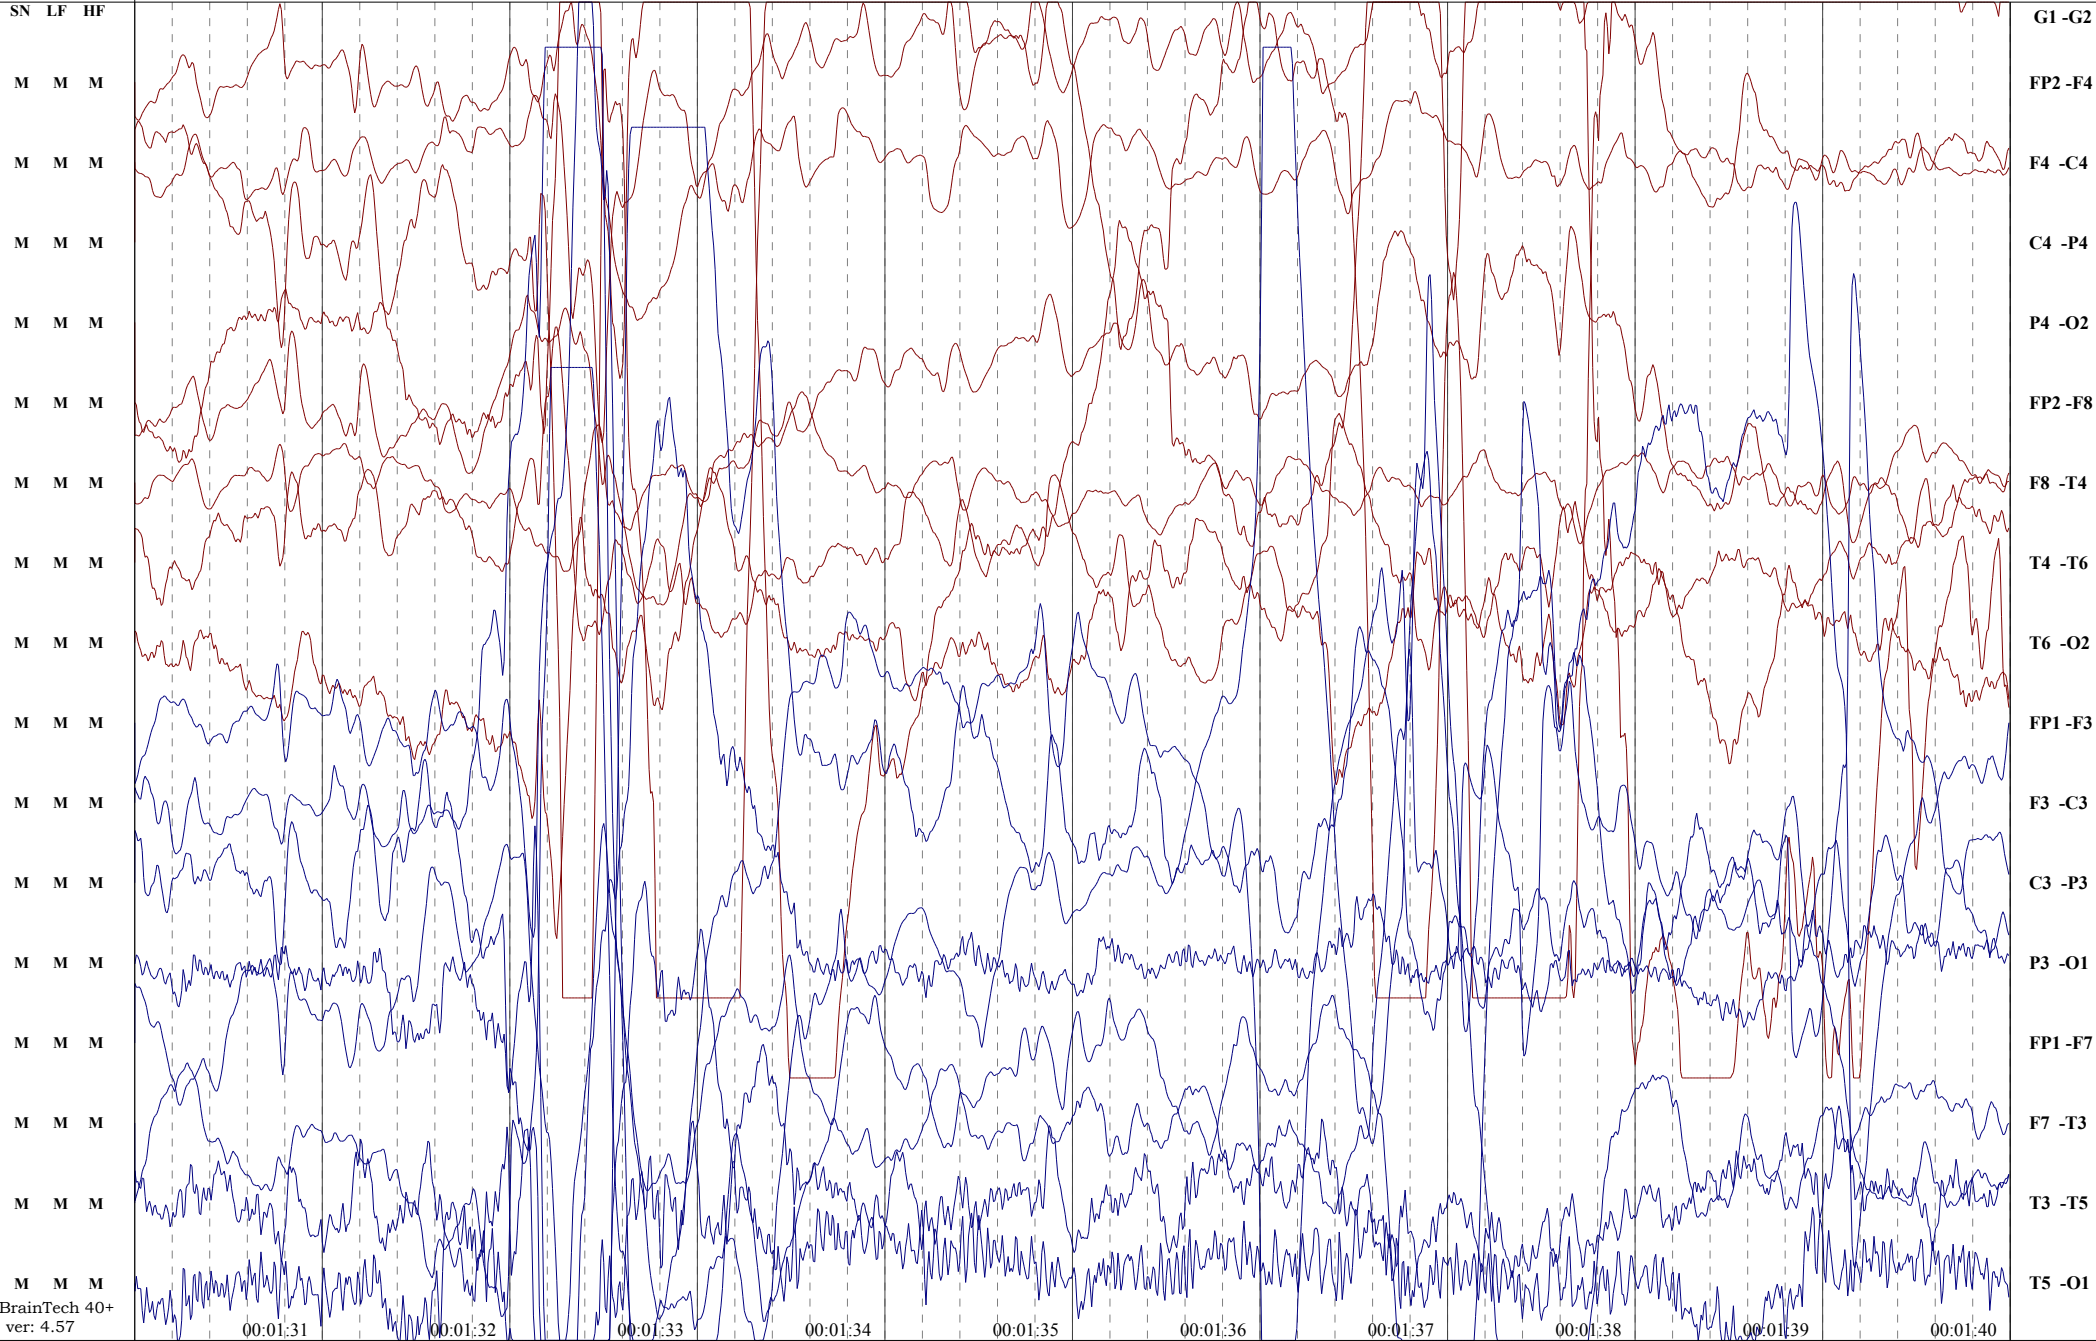


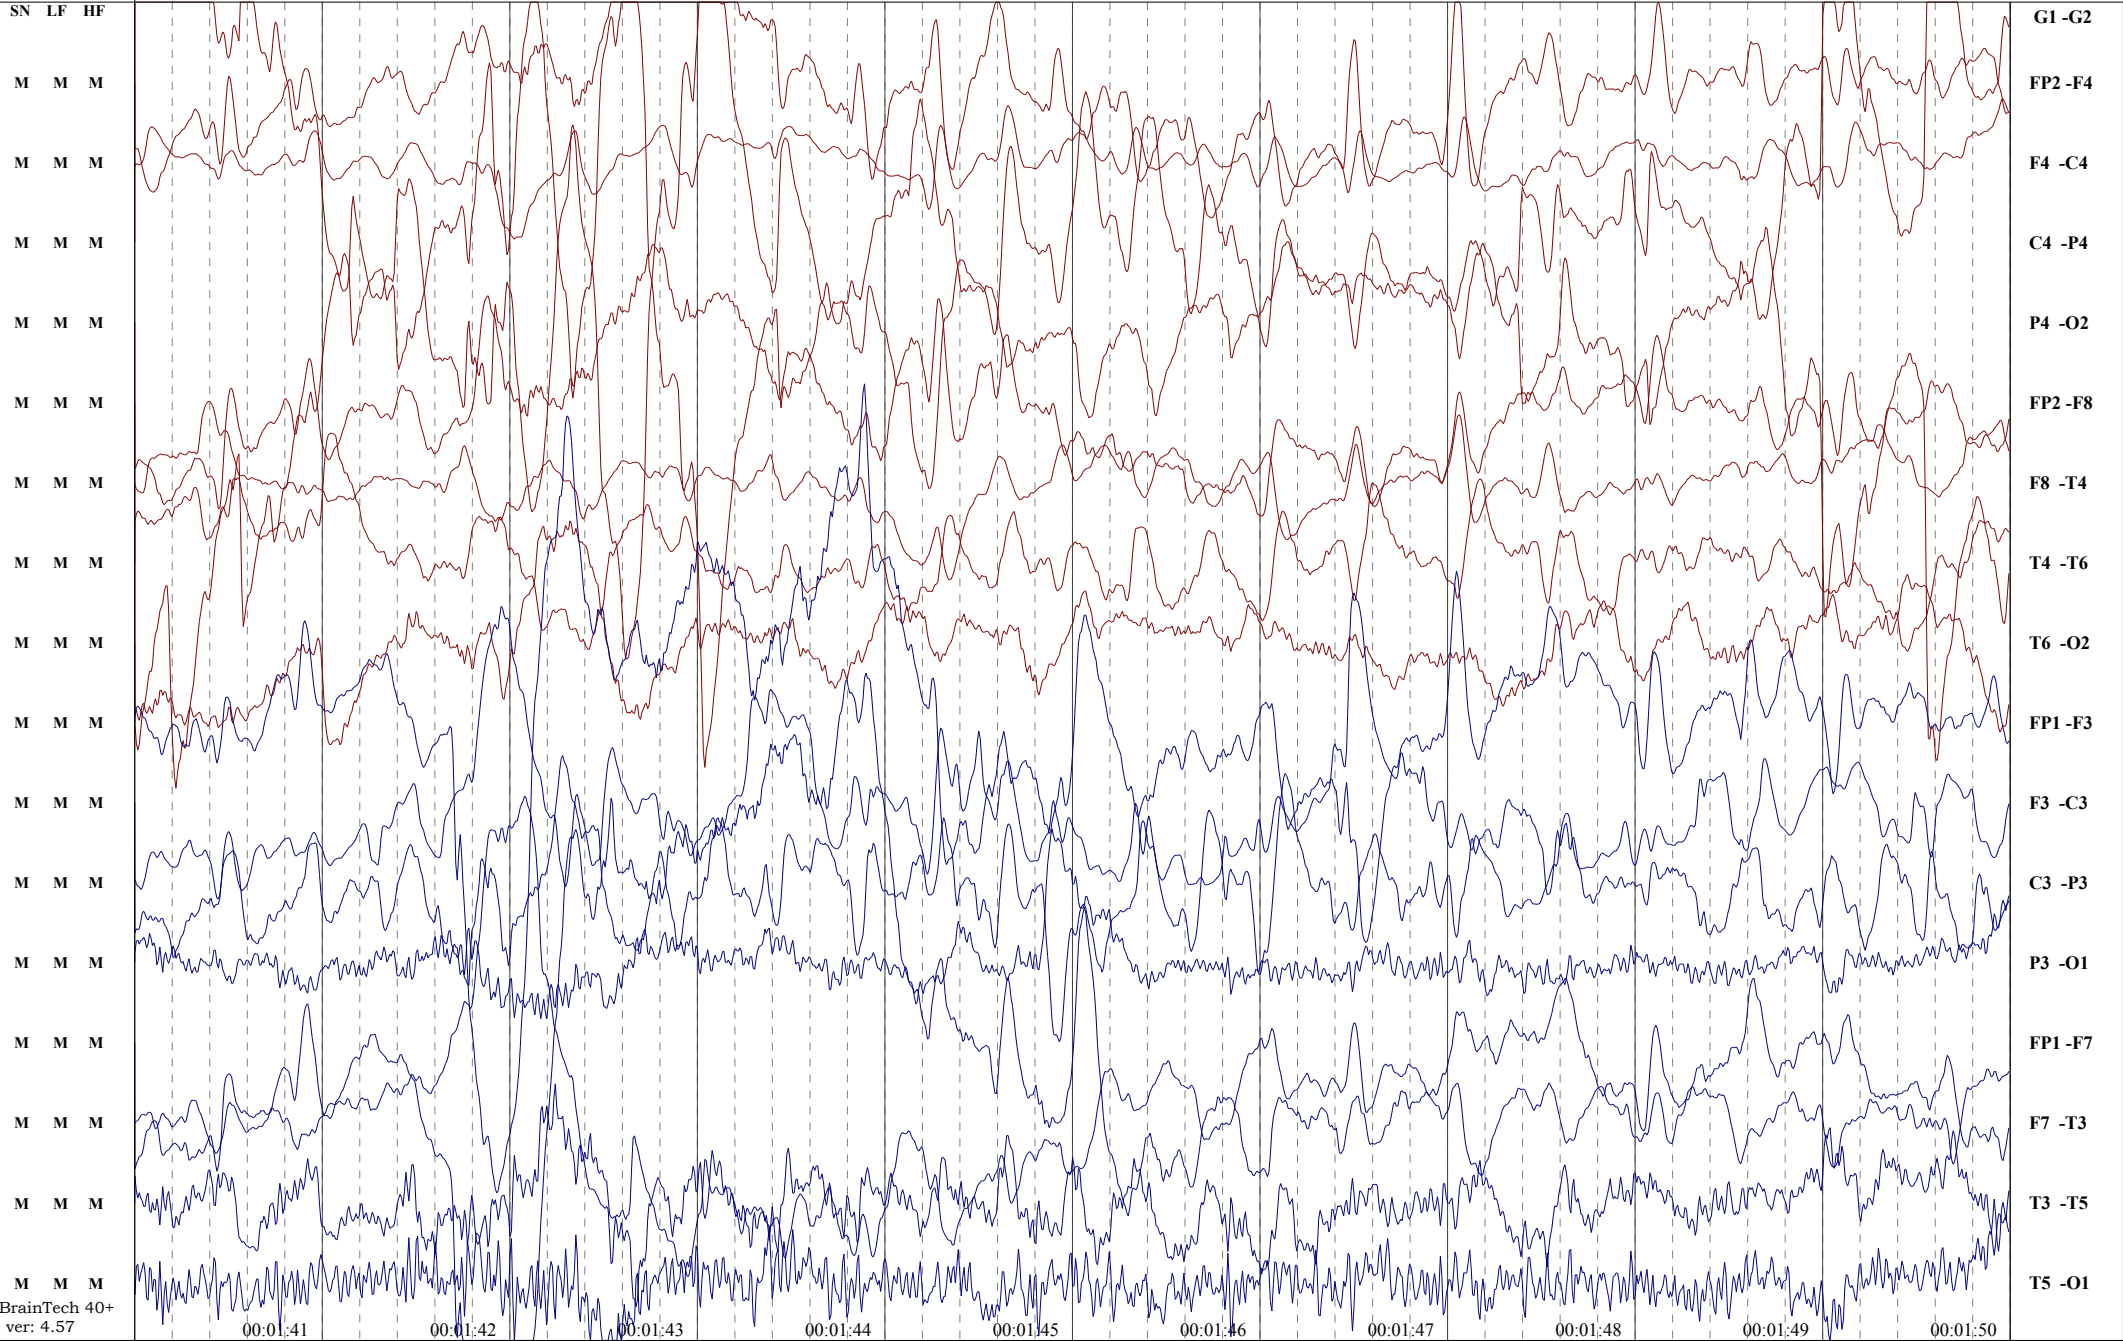










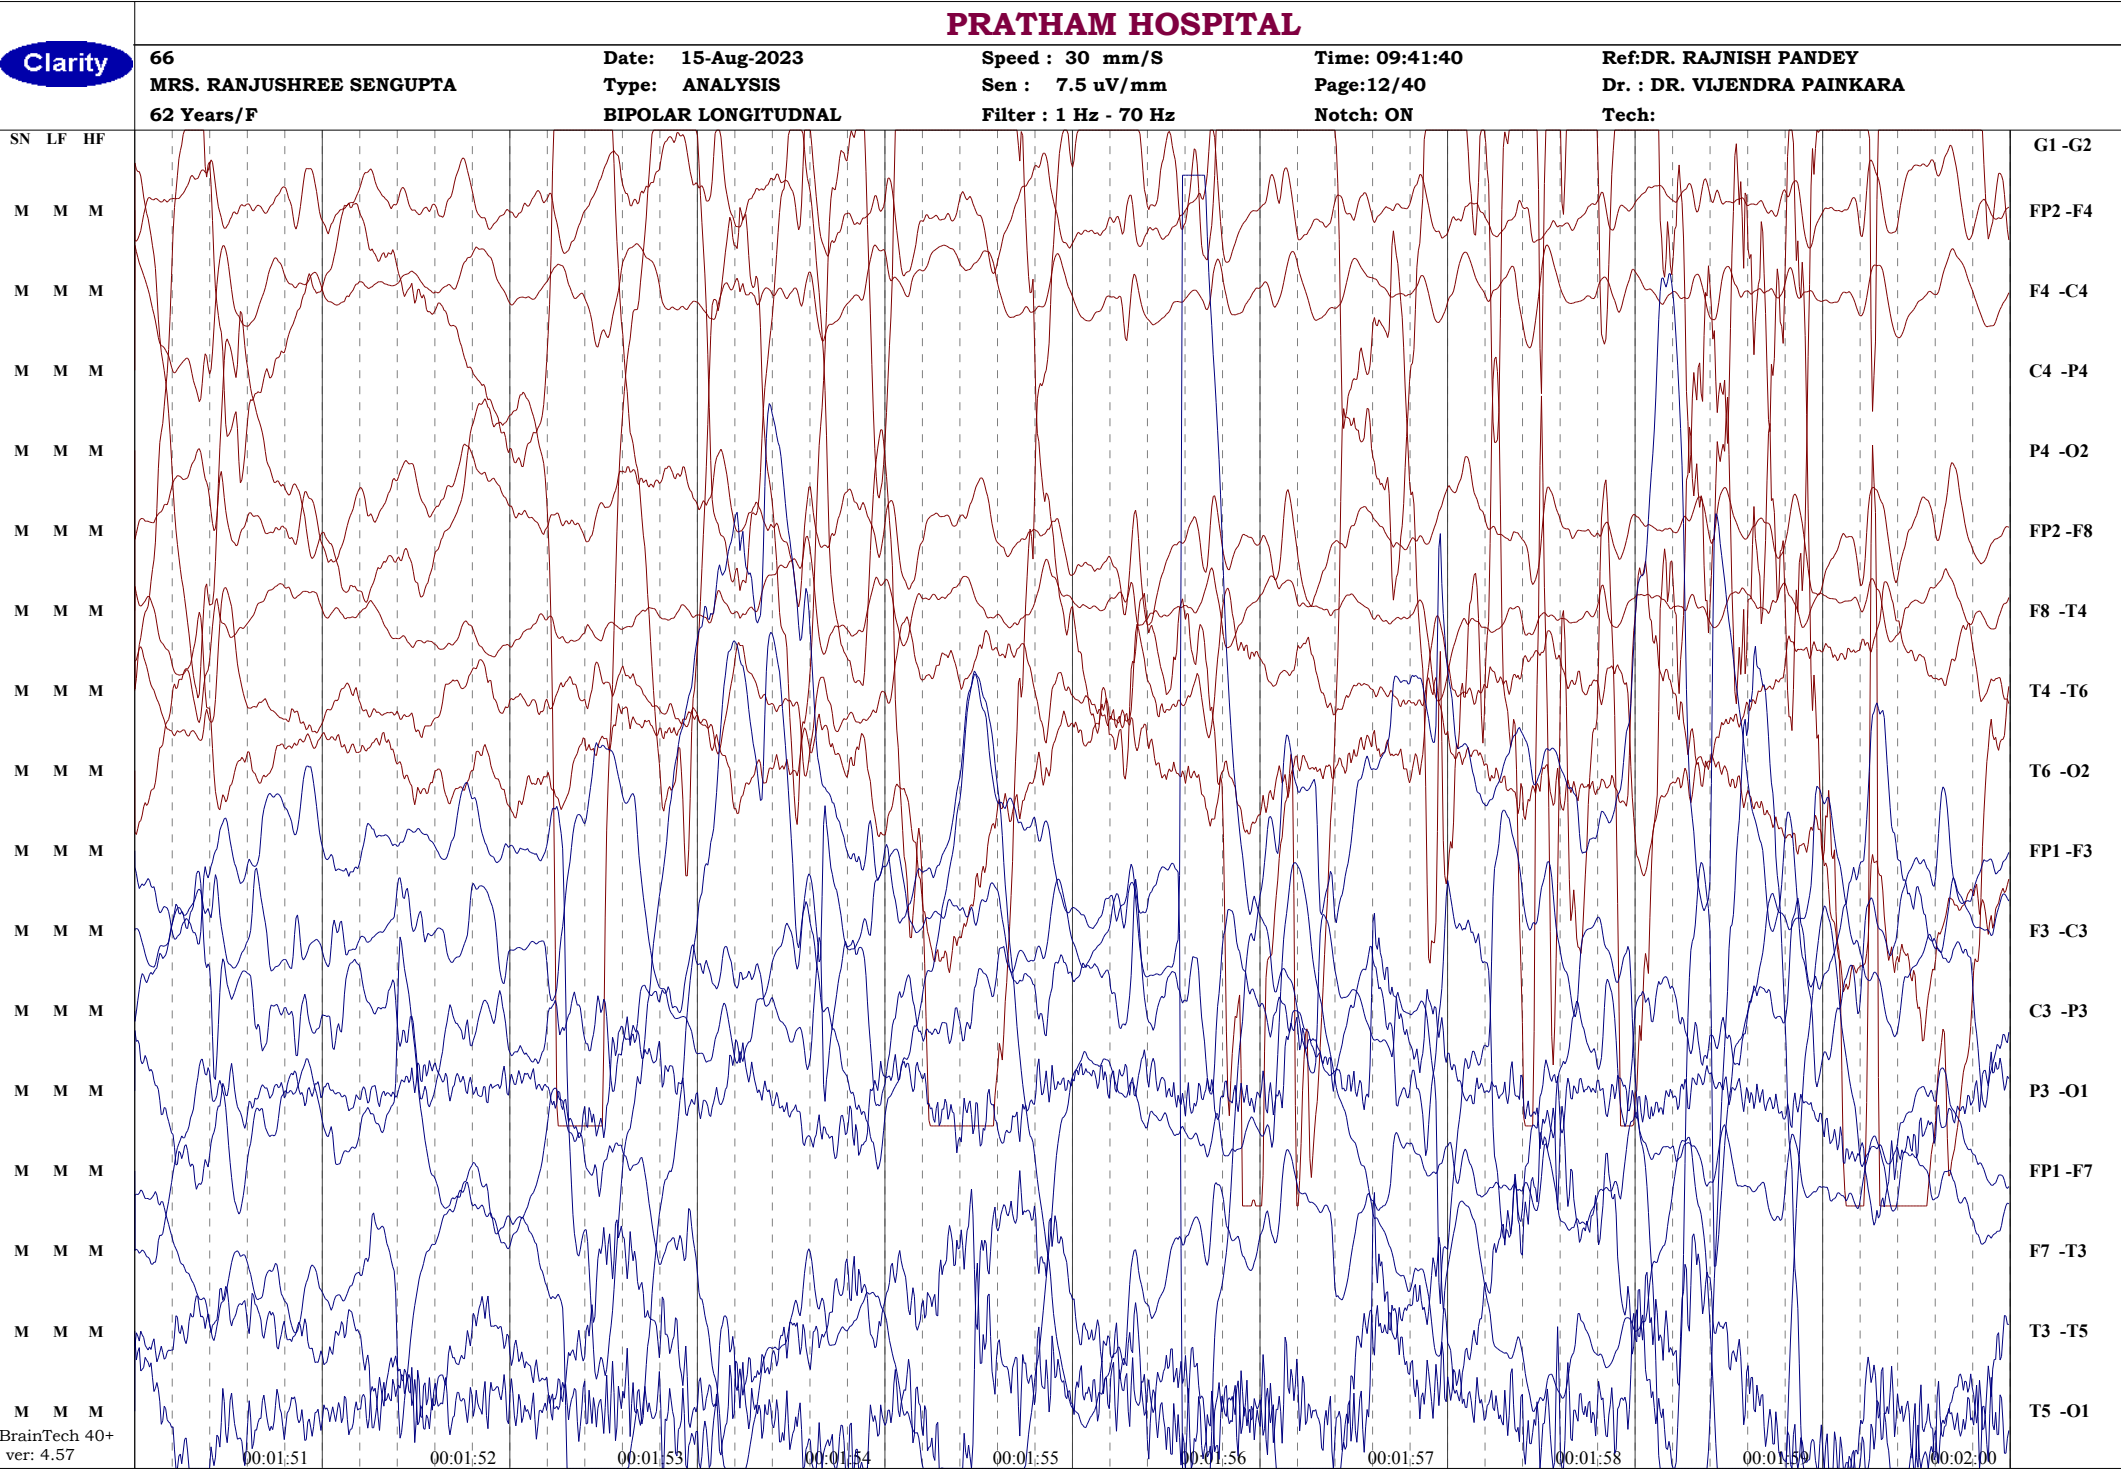

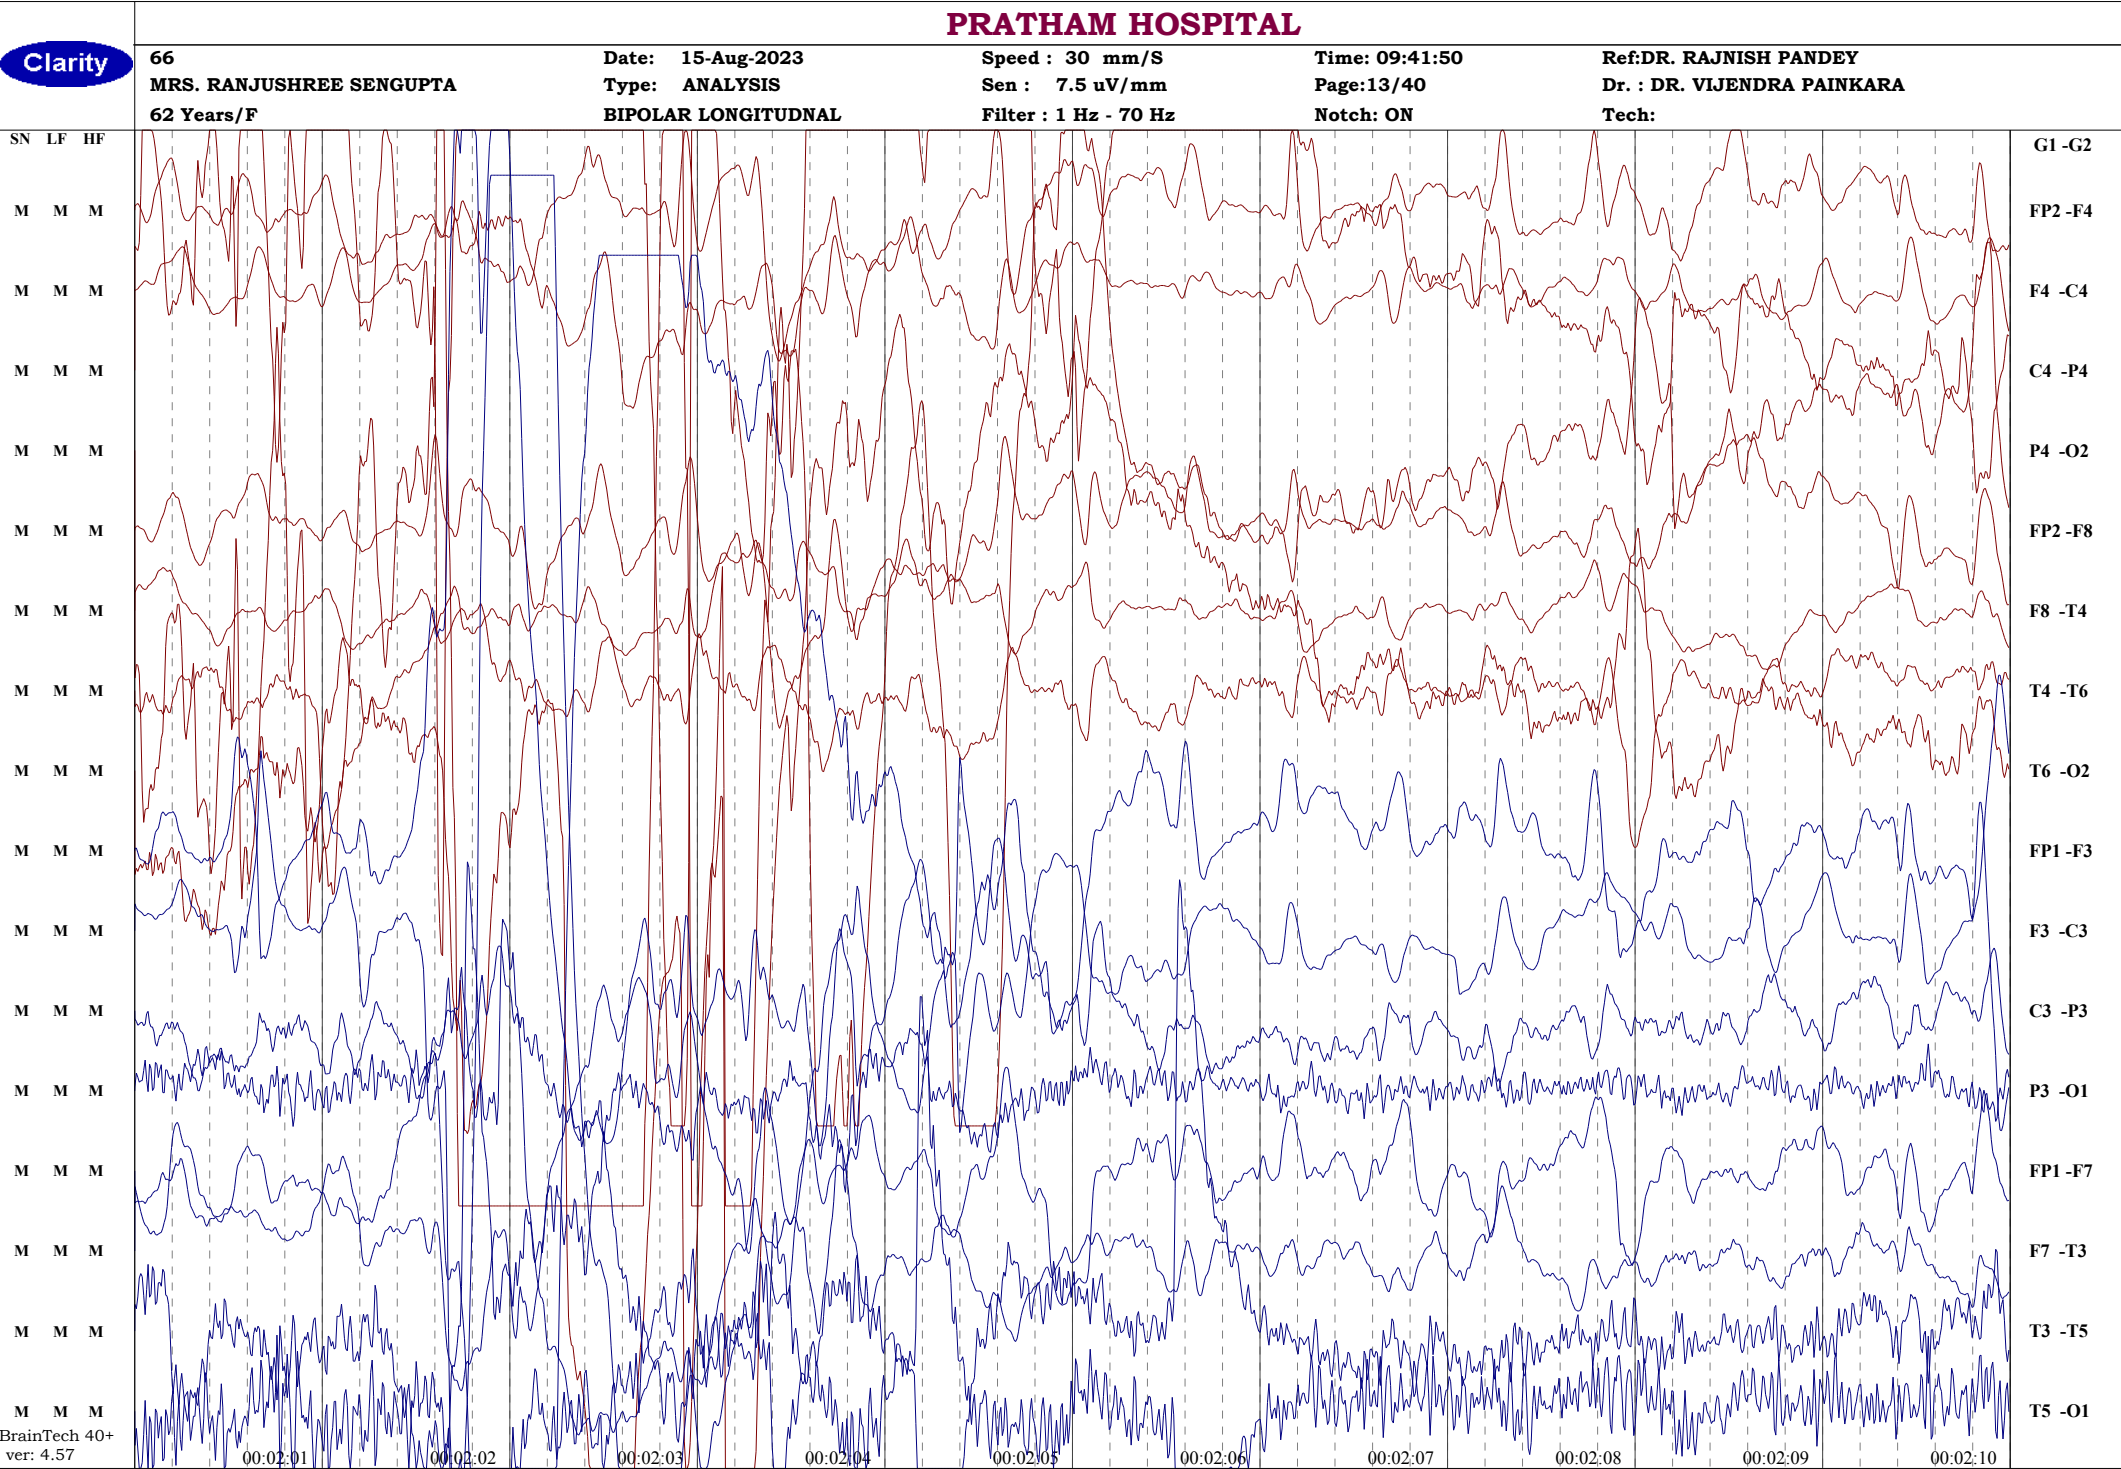


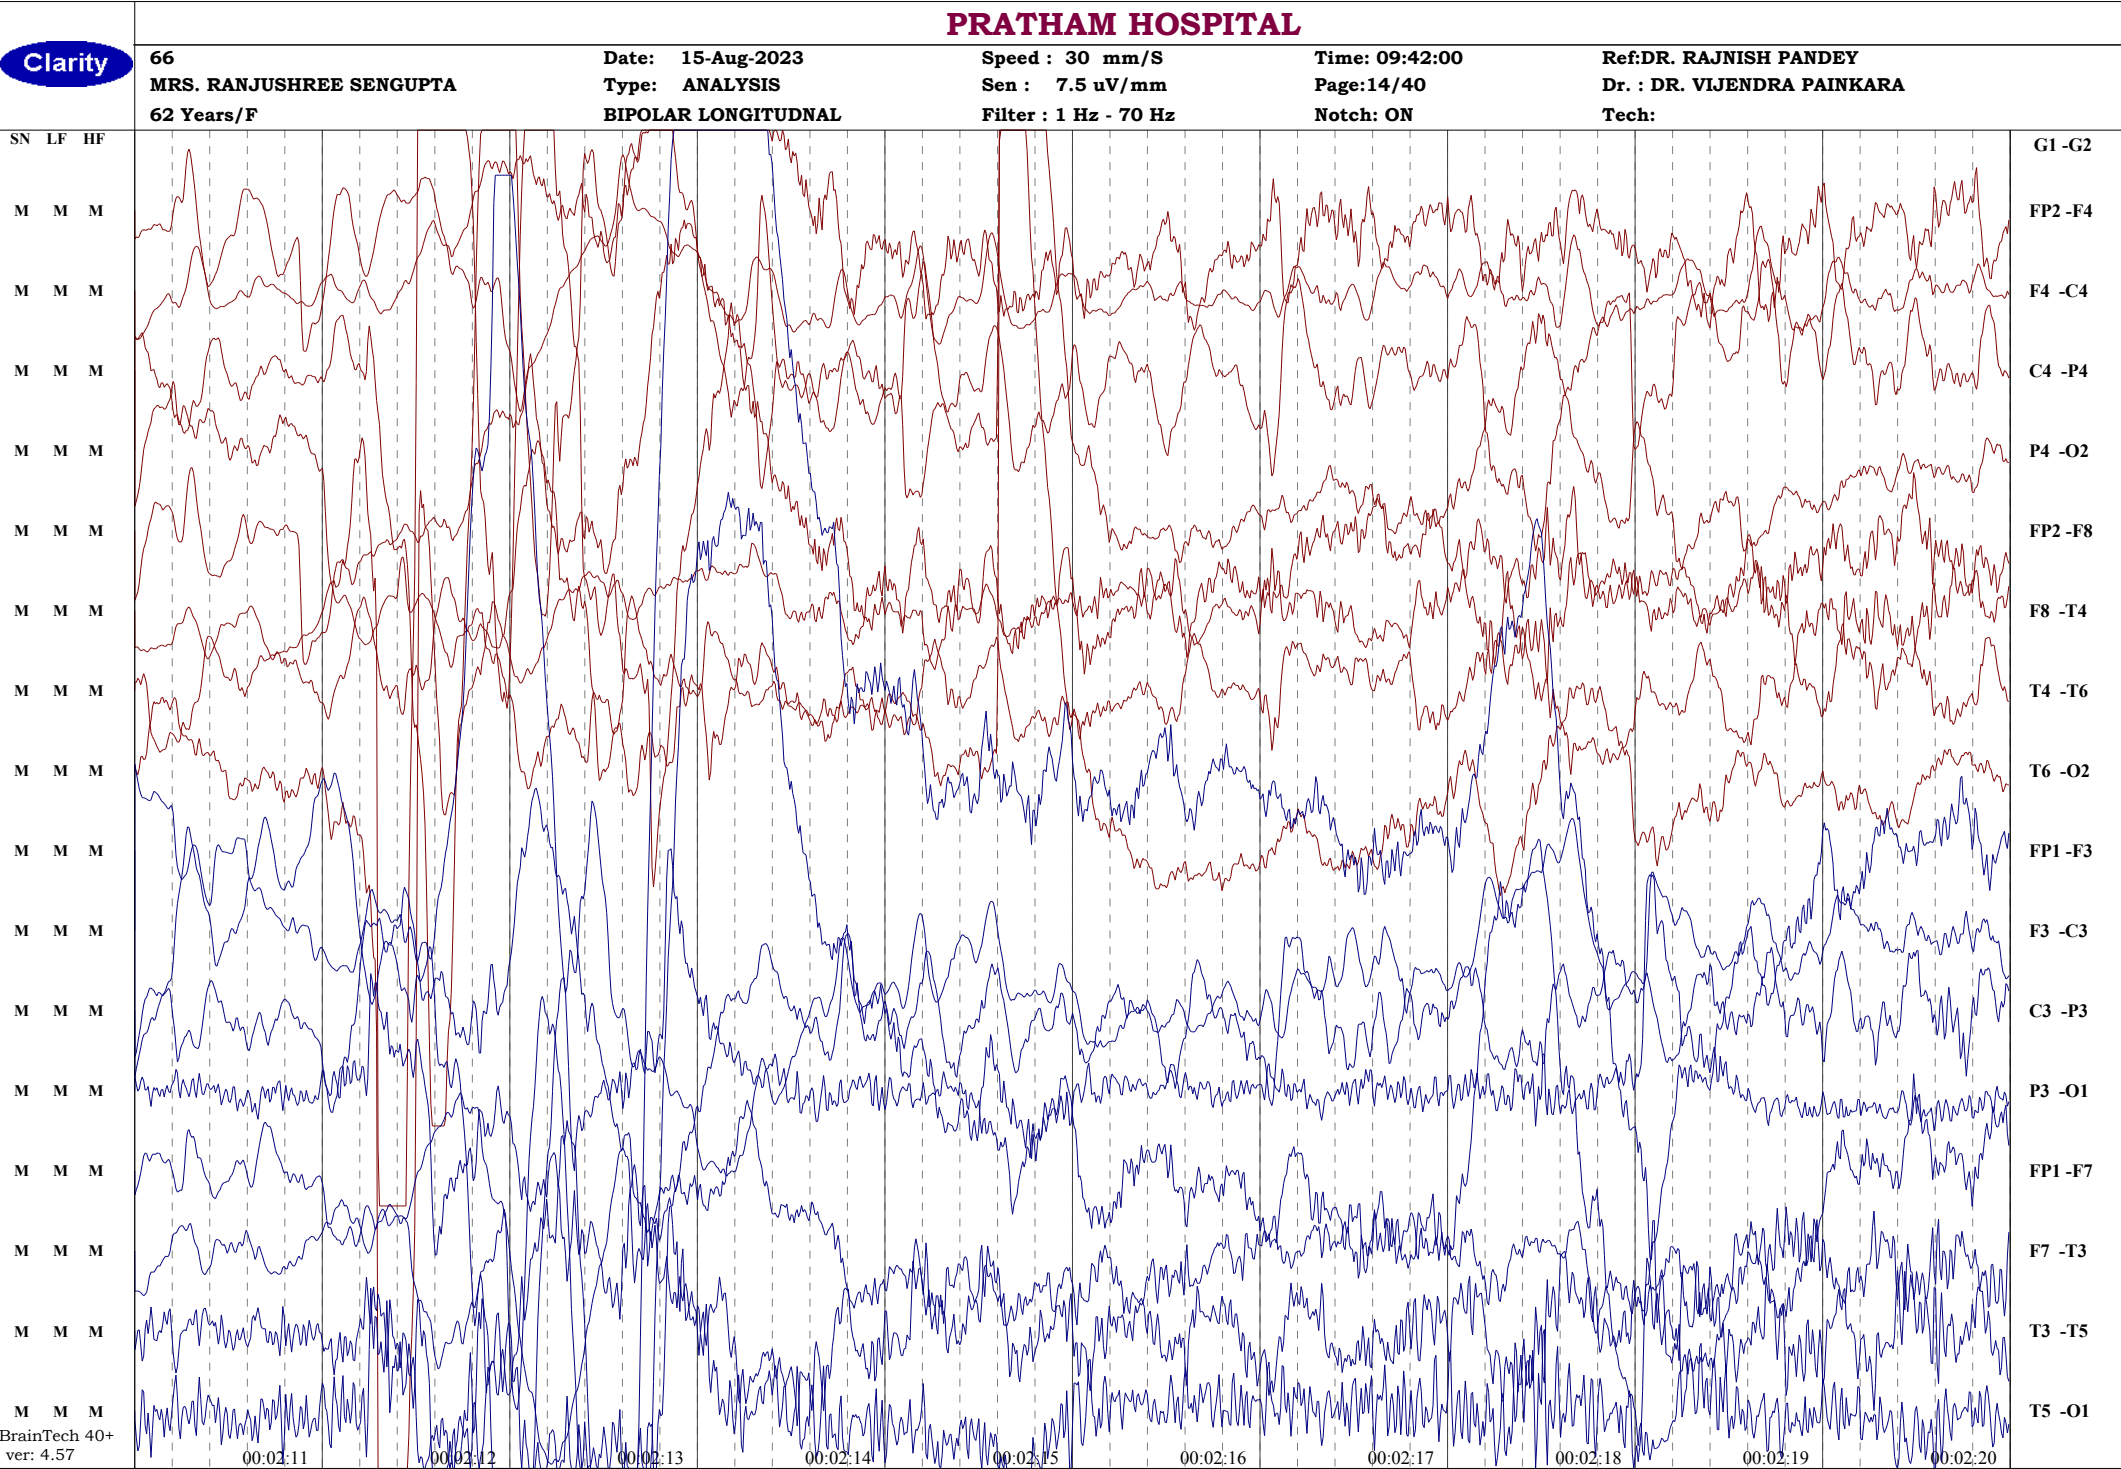



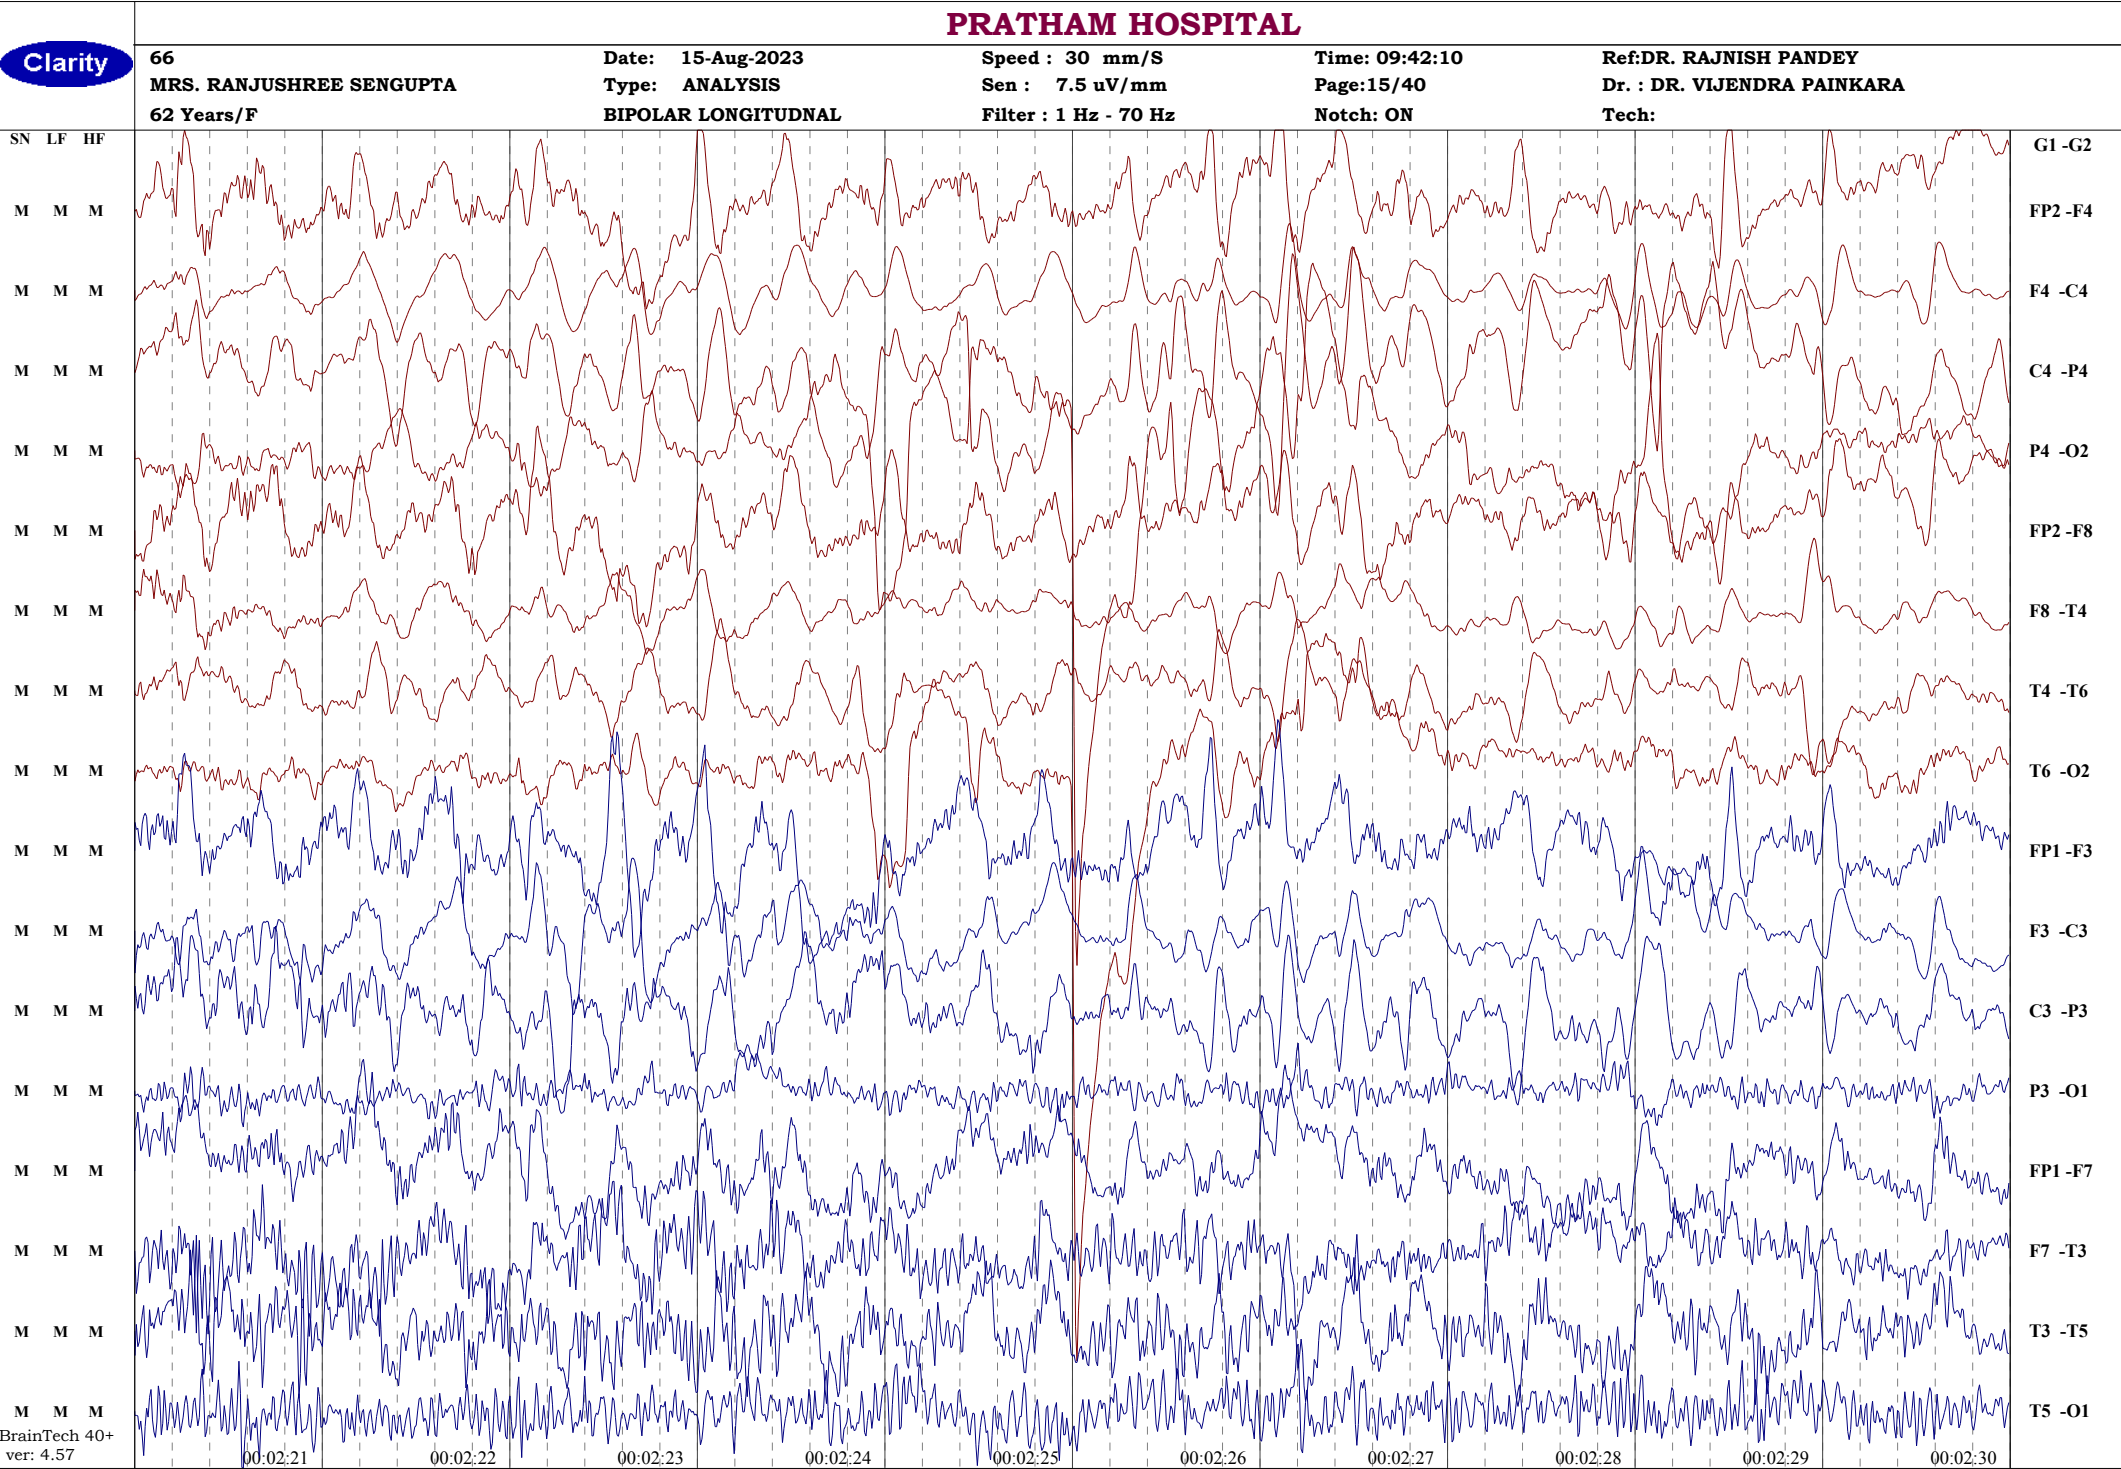



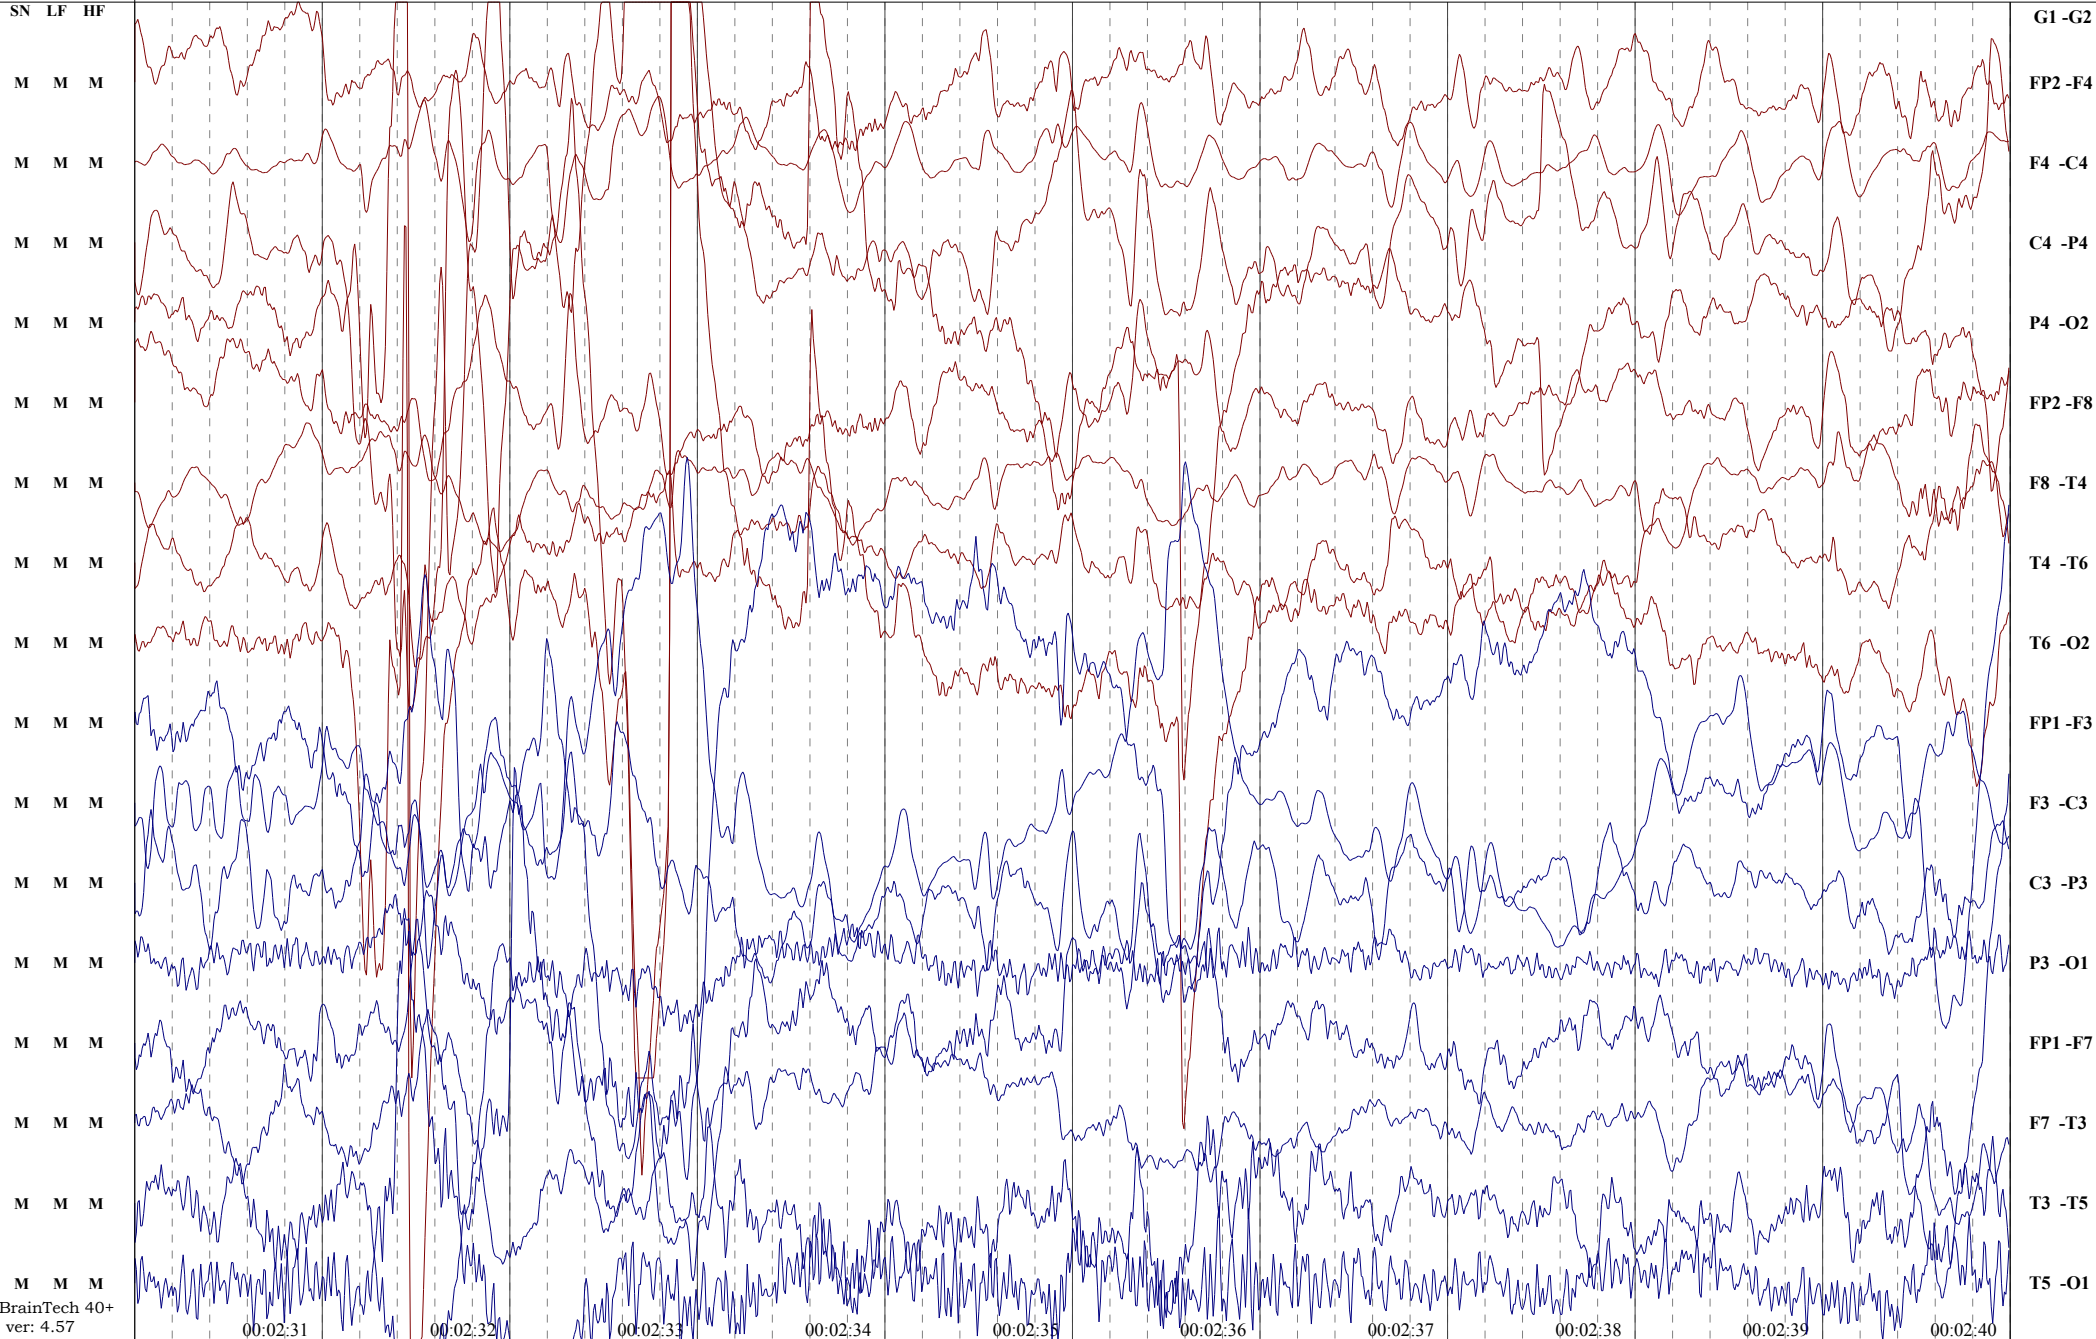

66  
MRS. RANJUSHREE SENGUPTA  
62 Years/F

Date: 15-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 09:42:30  
Page:17/40  
Notch: ON

Ref:DR. RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

