


69  
MR. NIRANJAN SAHU  
42 Years/M

Date: 17-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:46:39  
Page:3/25  
Notch: ON

Ref:DR.RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

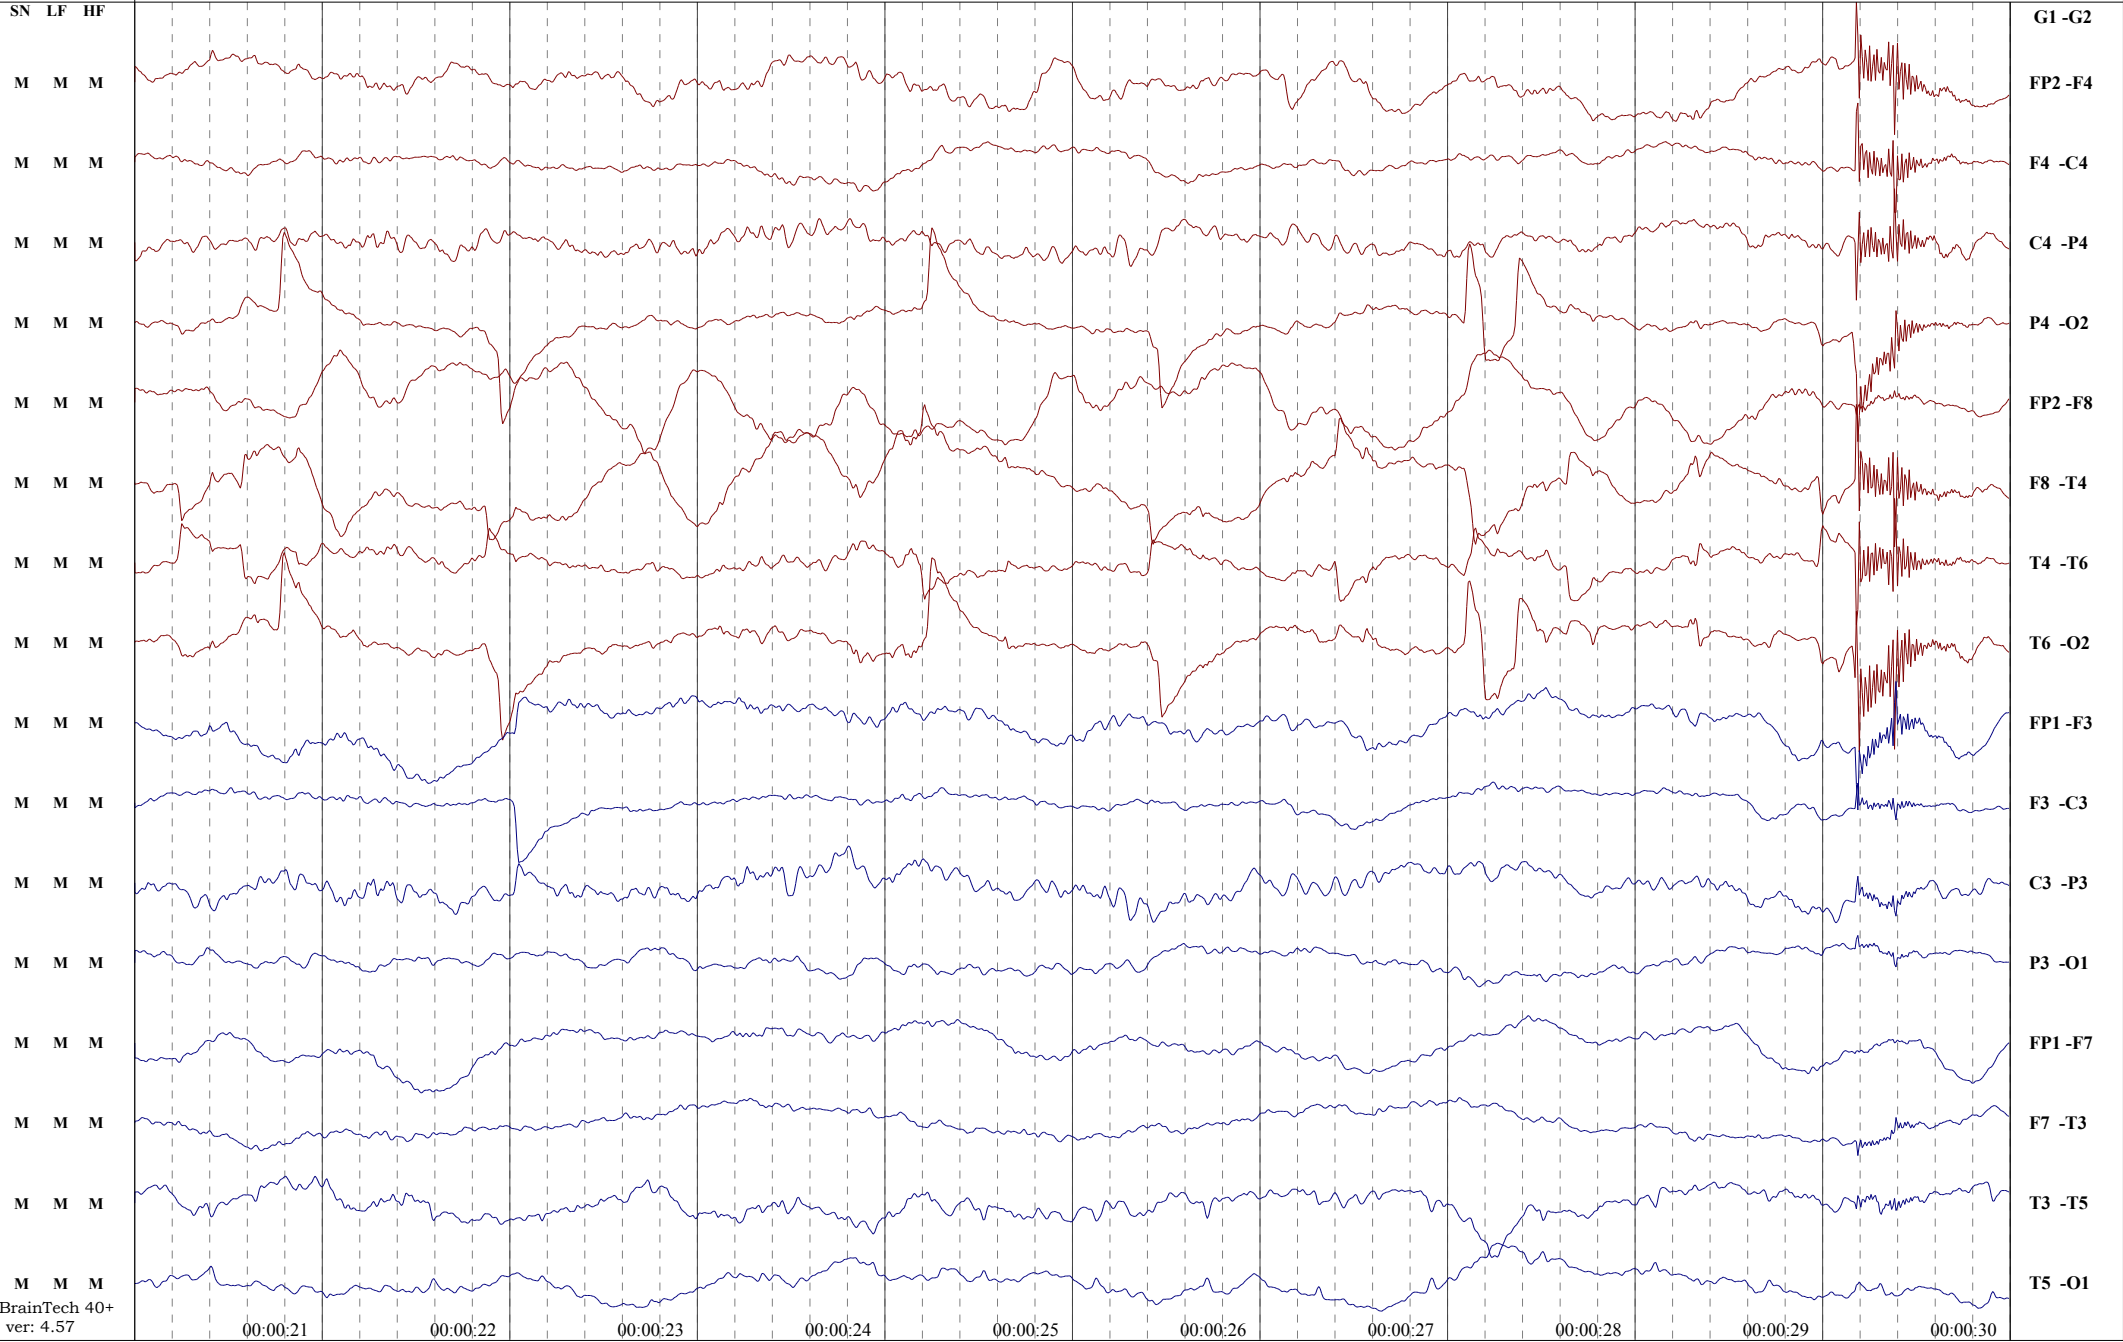


69  
MR. NIRANJAN SAHU  
42 Years/M

Date: 17-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:46:49  
Page:4/25  
Notch: ON

Ref:DR.RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

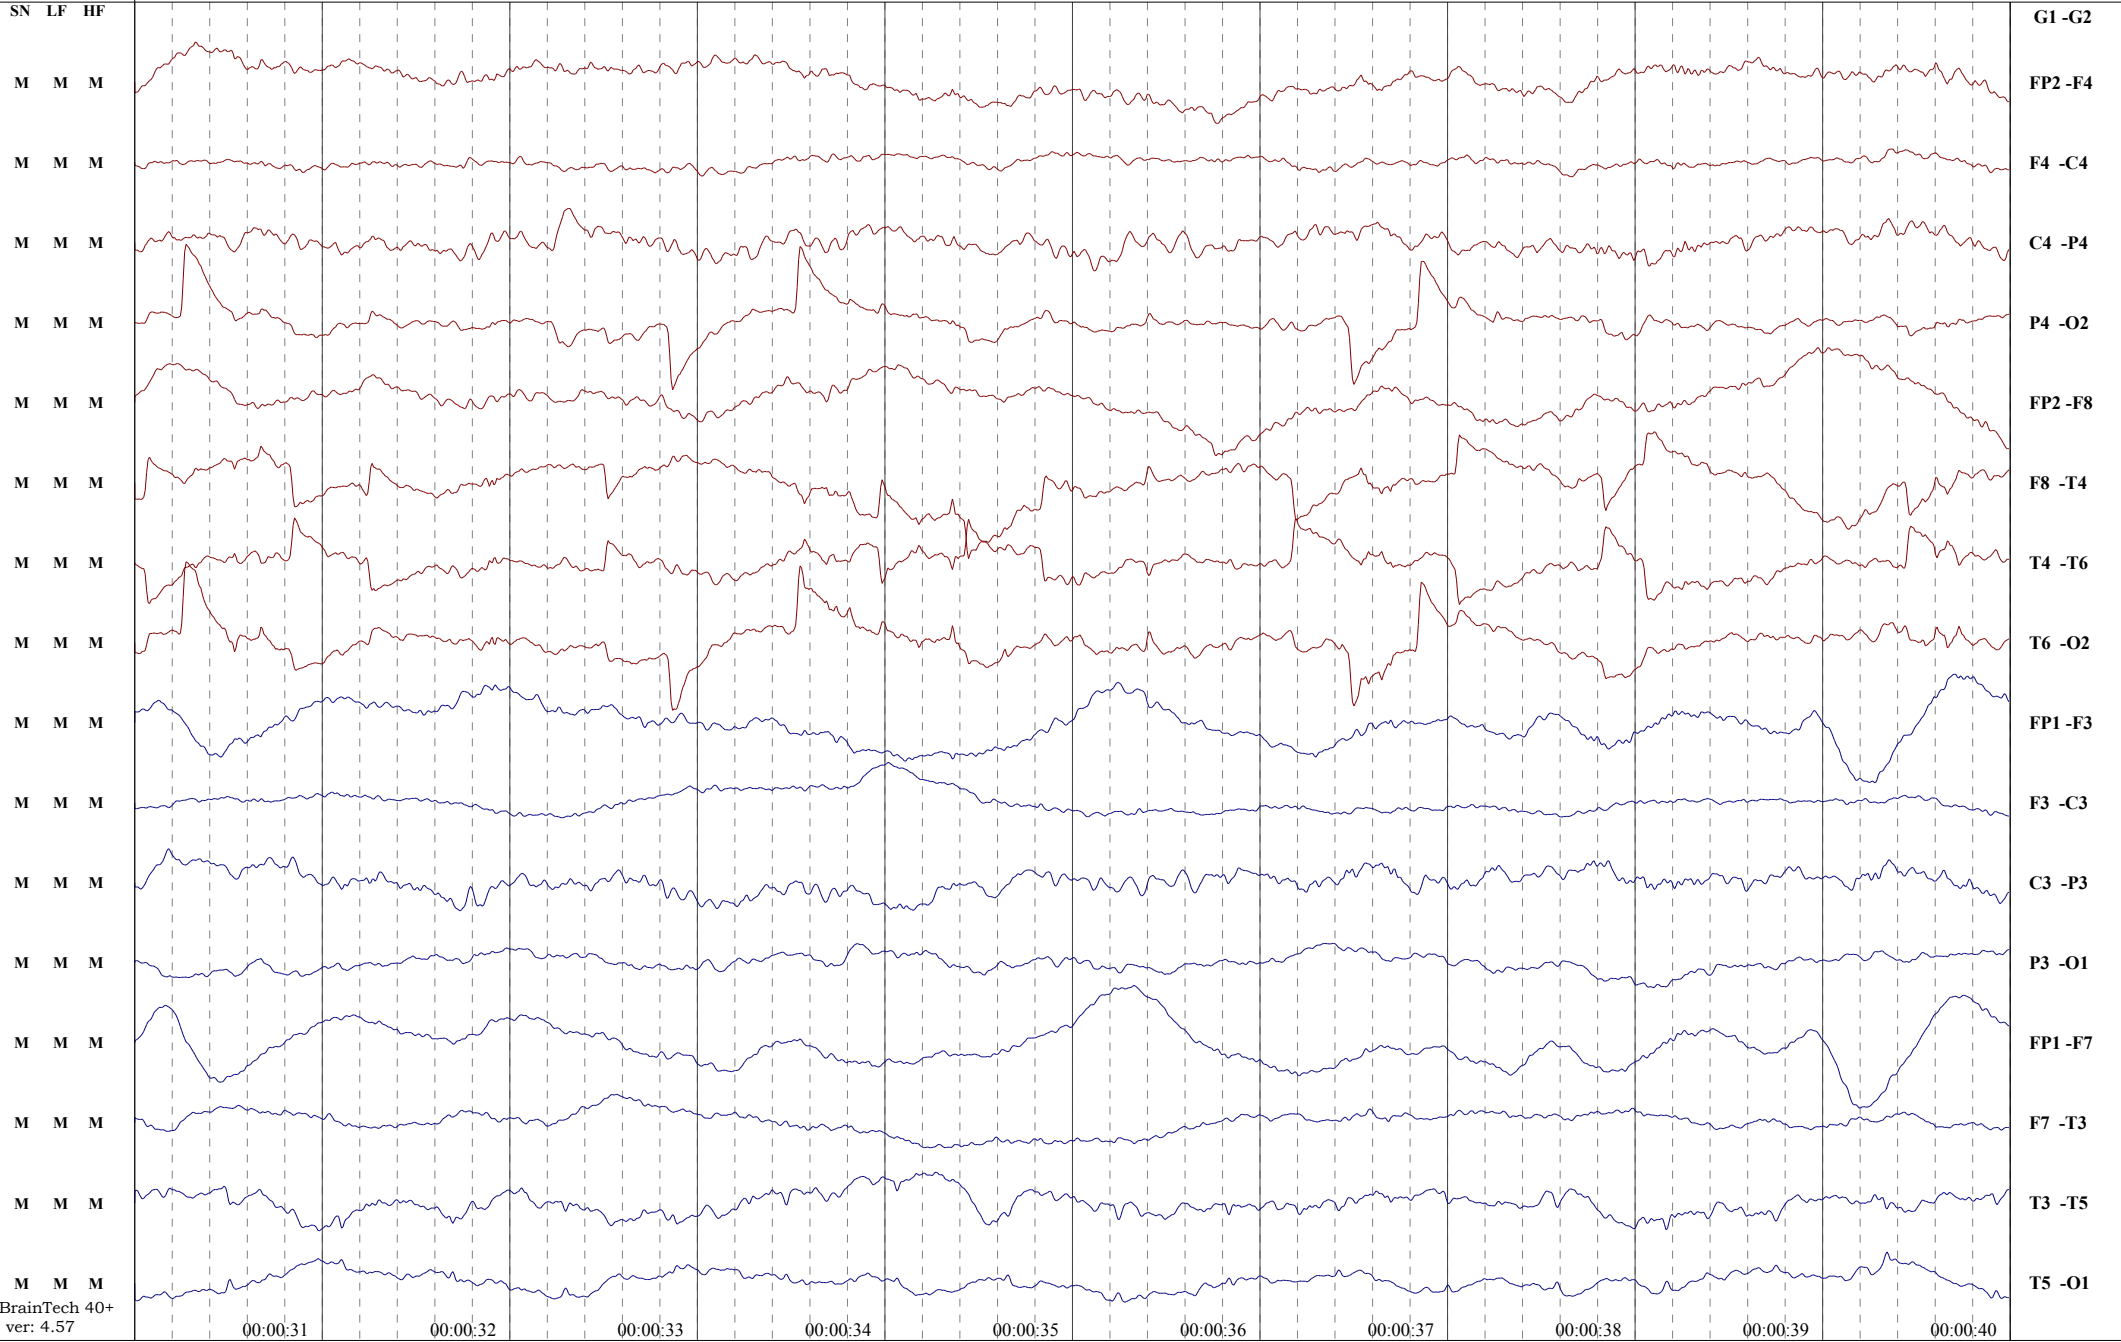


69  
MR. NIRANJAN SAHU  
42 Years/M

Date: 17-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:46:59  
Page:5/25  
Notch: ON

Ref:DR.RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

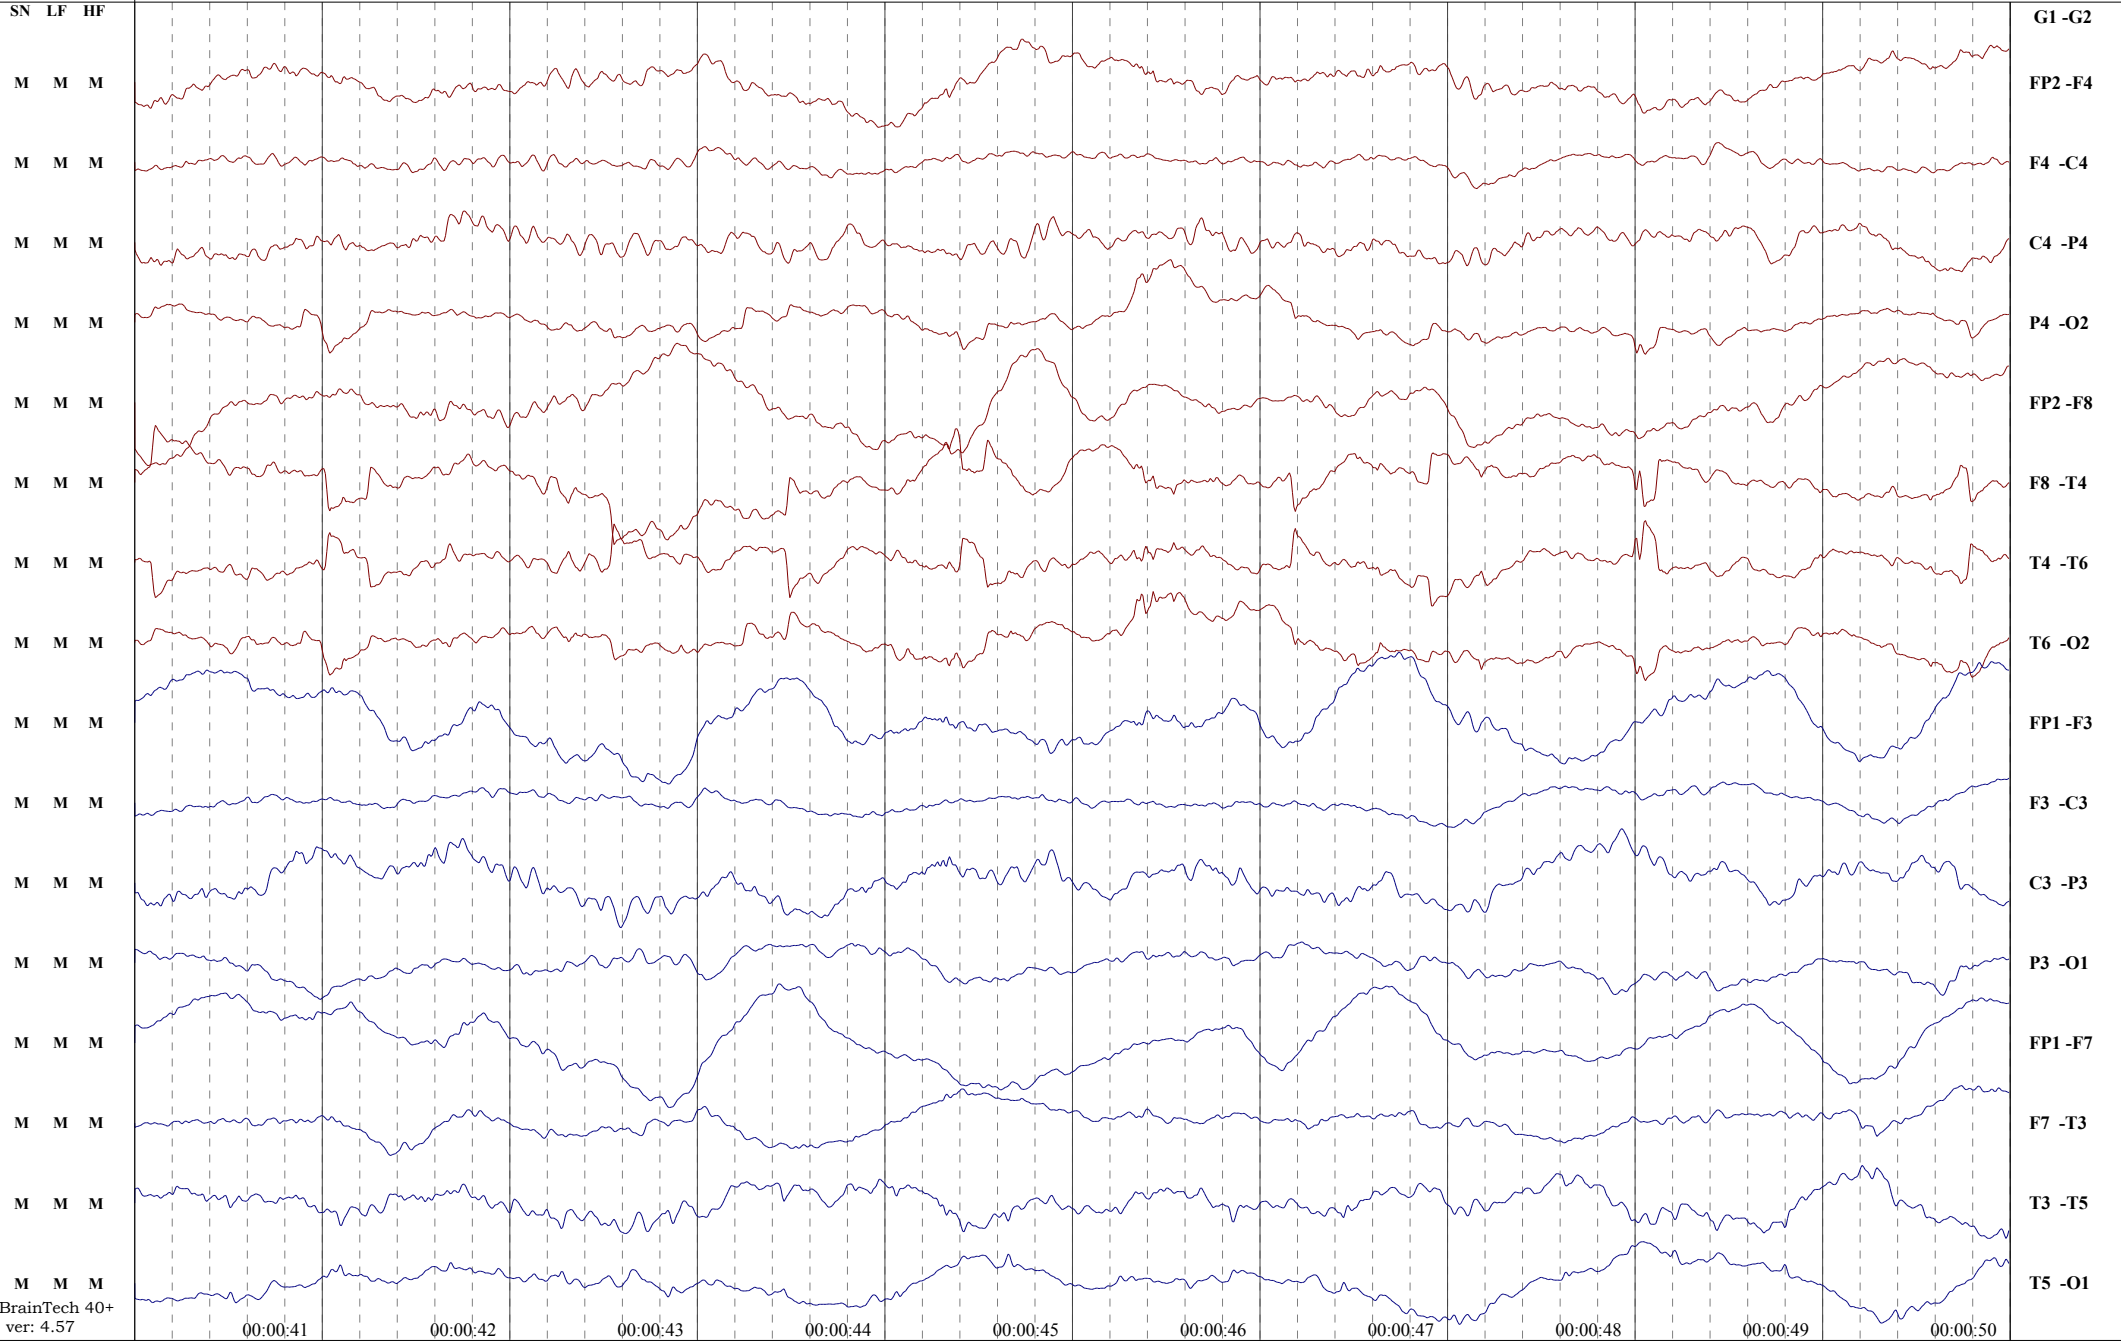


69  
MR. NIRANJAN SAHU  
42 Years/M

Date: 17-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:47:09  
Page:6/25  
Notch: ON

Ref:DR.RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

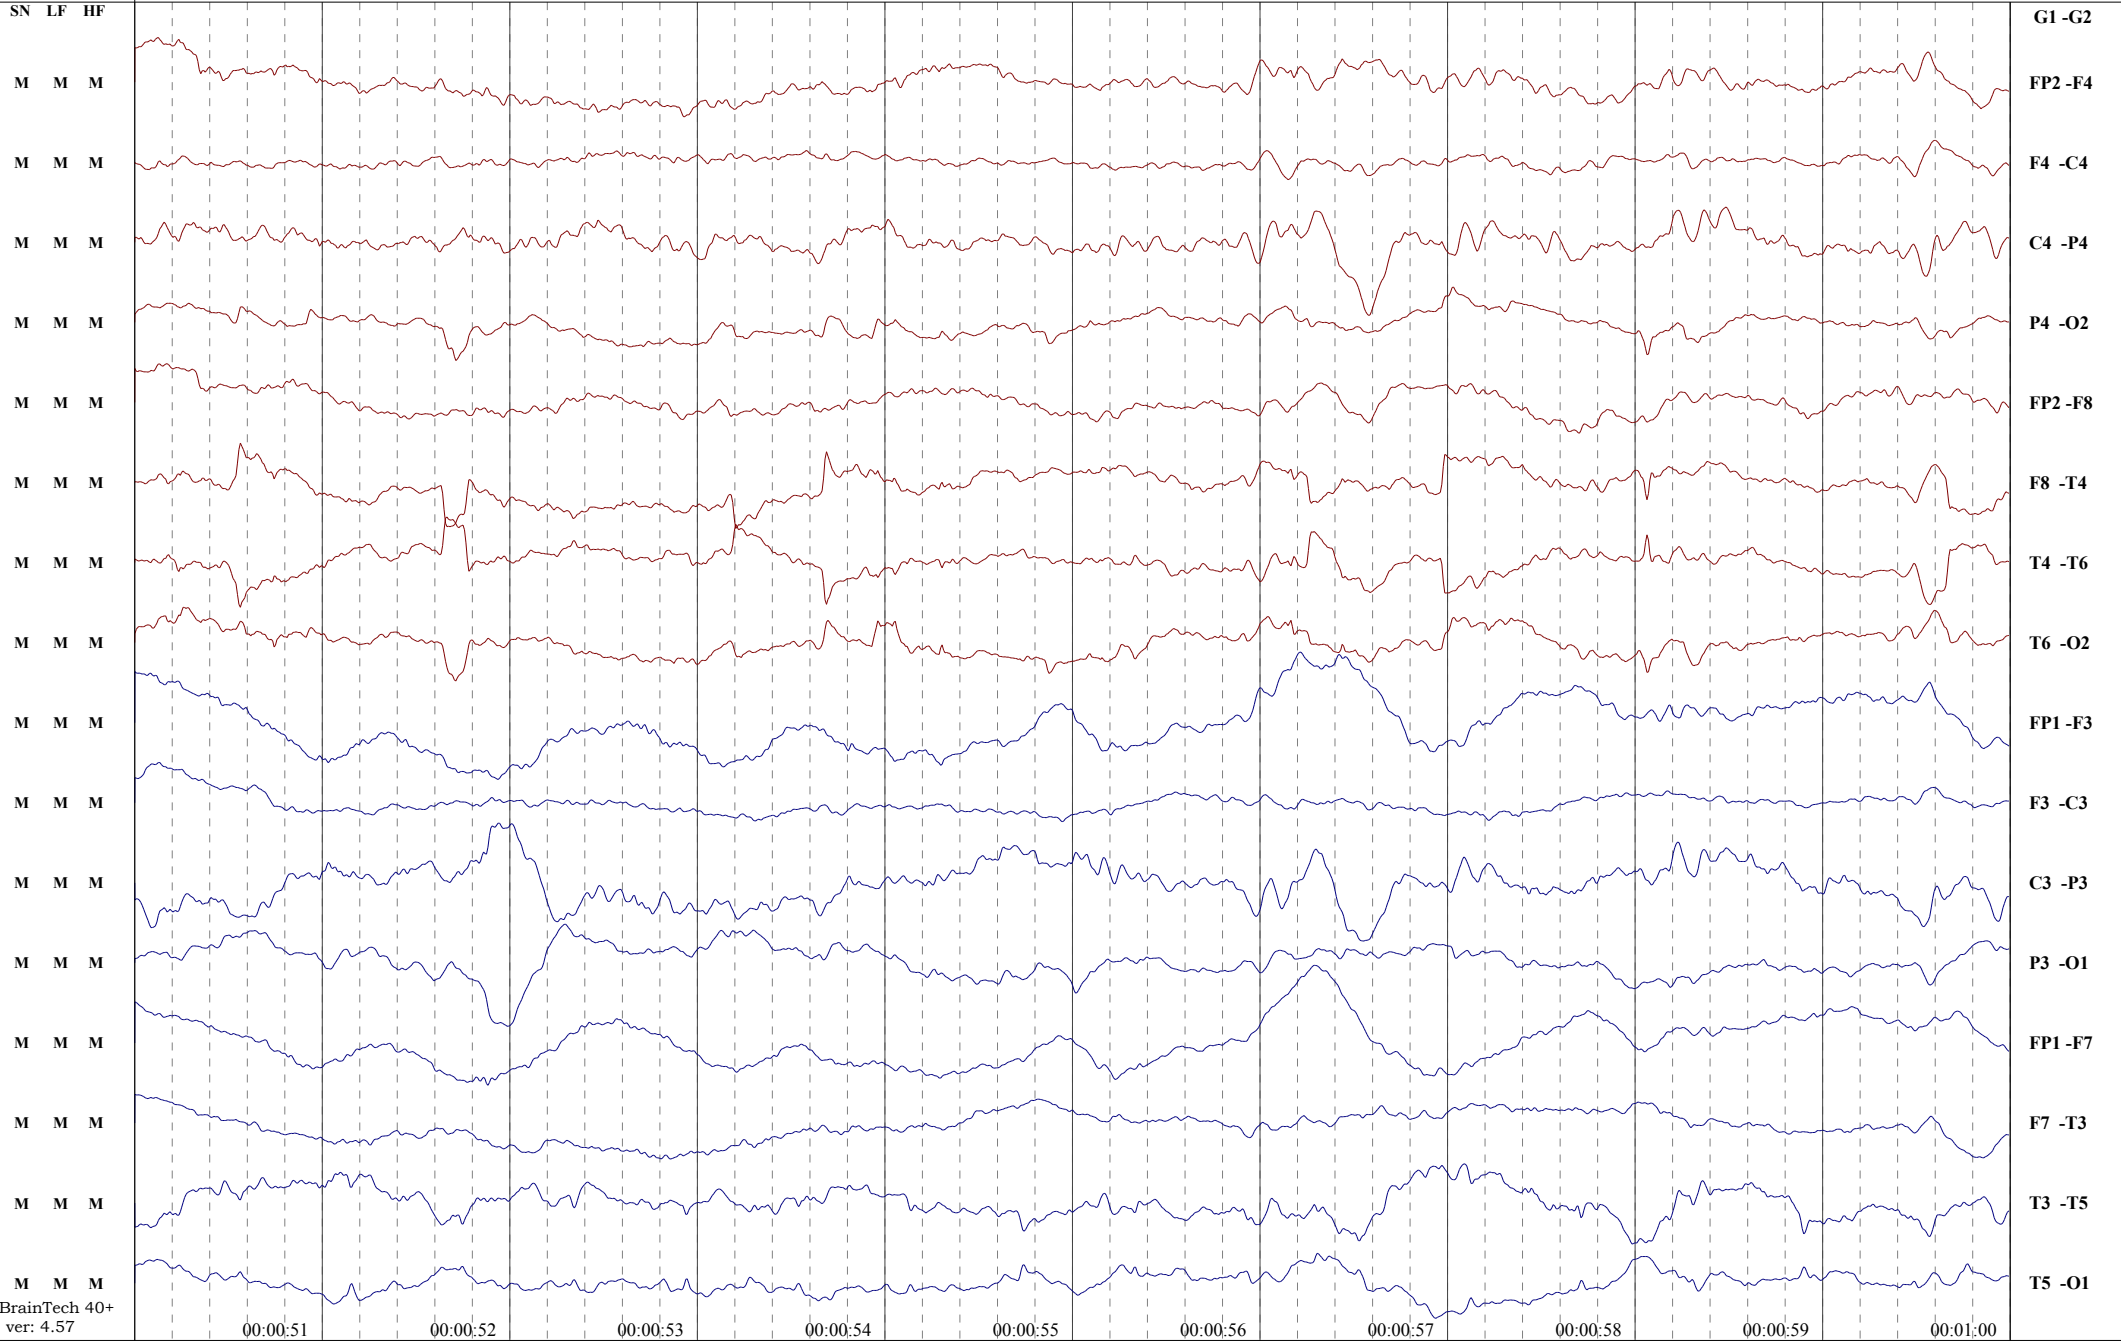


69  
MR. NIRANJAN SAHU  
42 Years/M

Date: 17-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:47:19  
Page:7/25  
Notch: ON

Ref:DR.RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

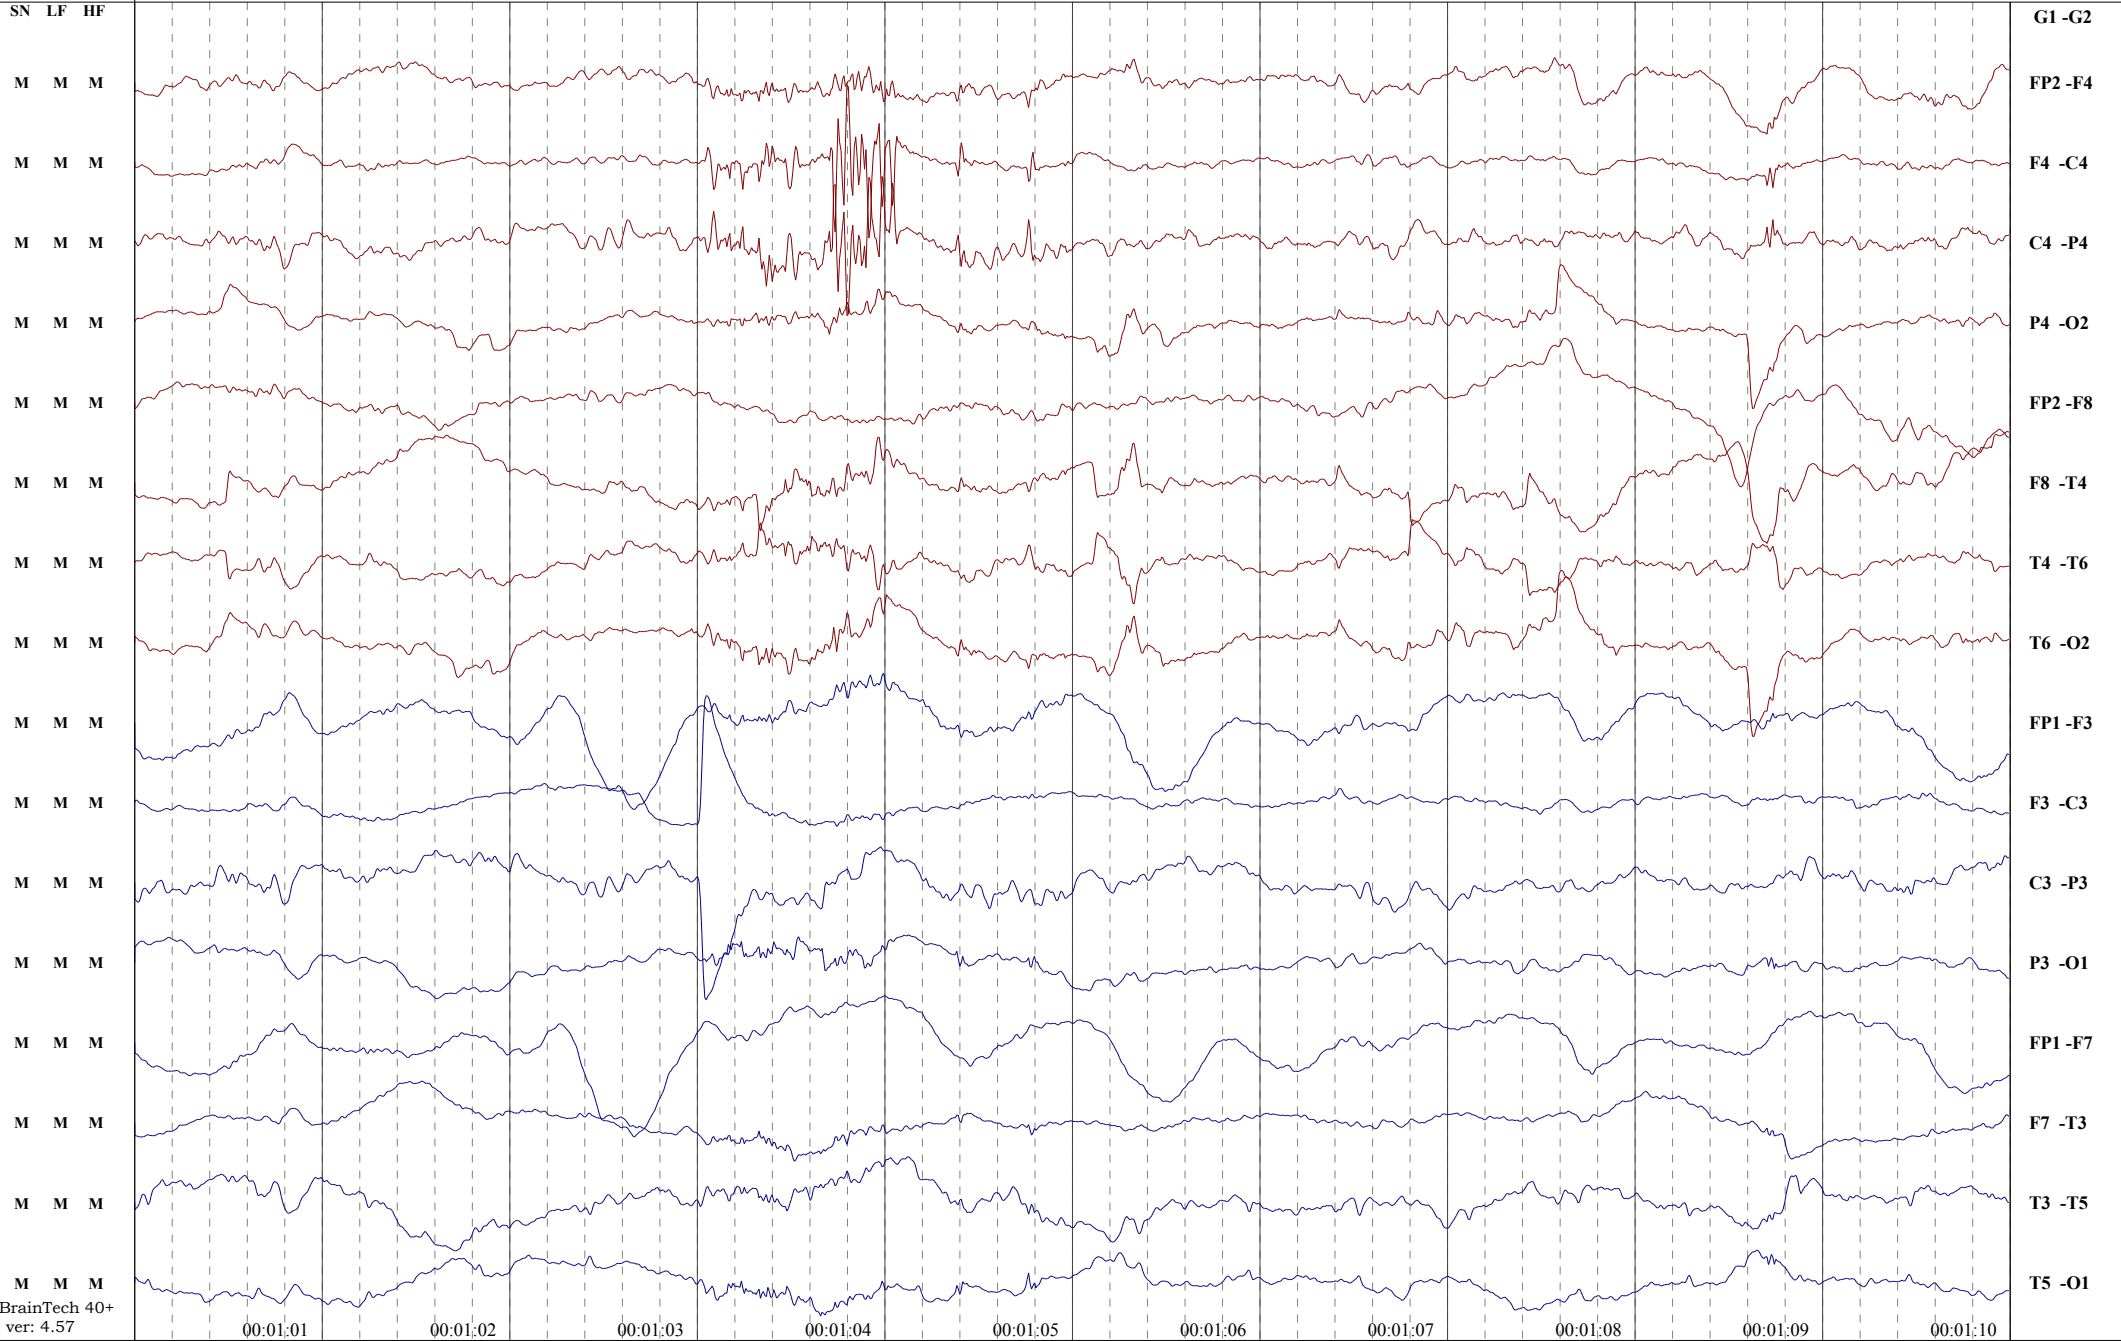

69  
MR. NIRANJAN SAHU  
42 Years/M


Date: 17-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:47:29  
Page:8/25  
Notch: ON

Ref:DR.RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

Photic ON  
Ph: 1 Hz

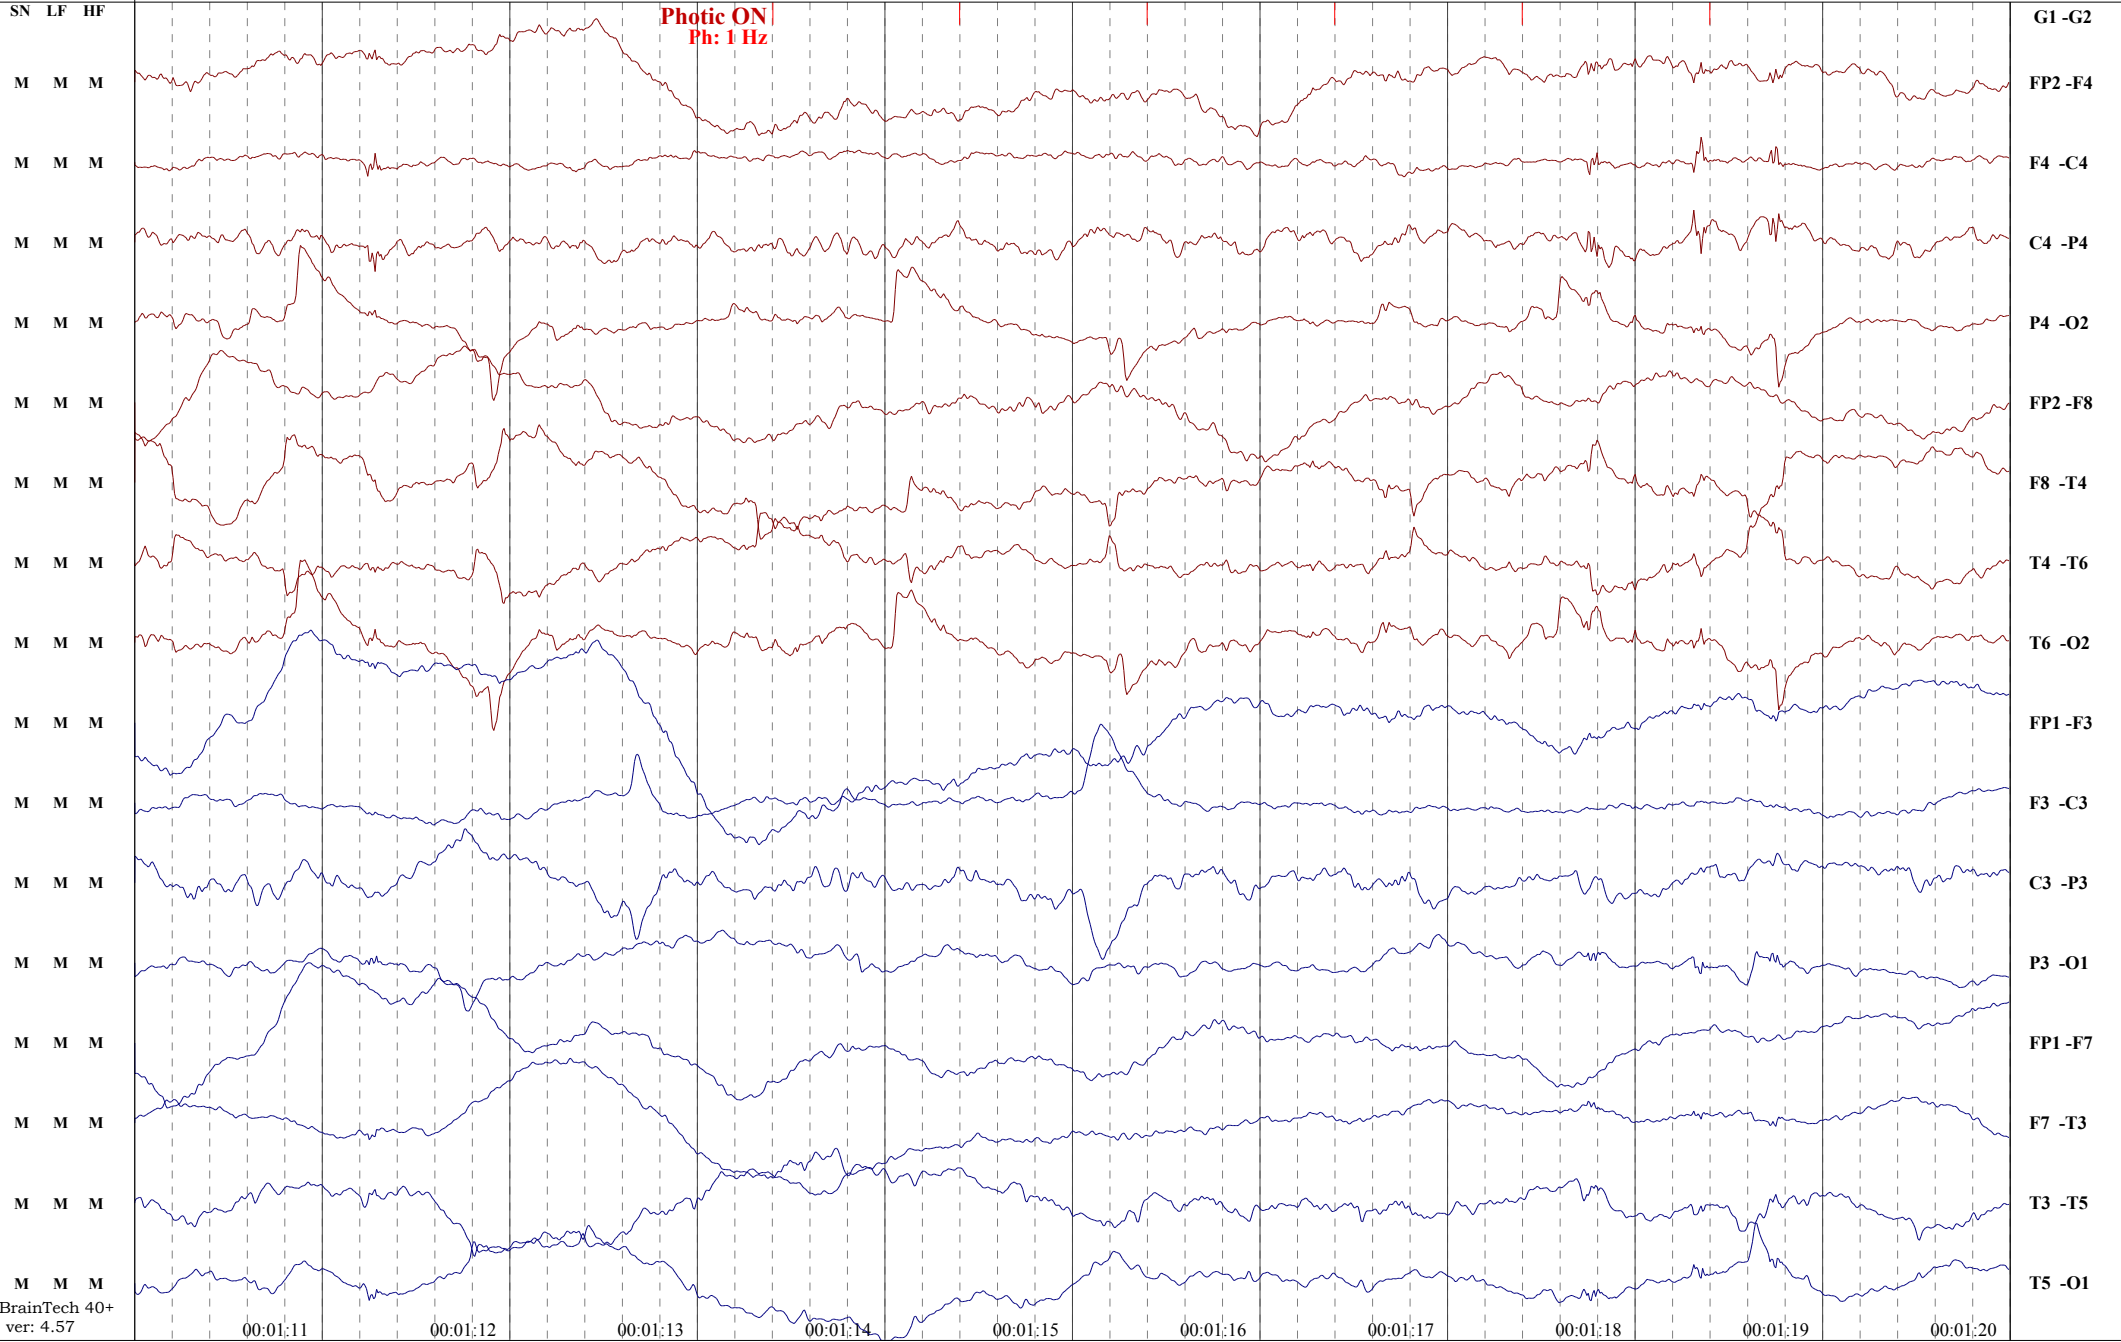




69  
MR. NIRANJAN SAHU  
42 Years/M

Date: 17-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:47:39  
Page:9/25  
Notch: ON

Ref:DR.RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

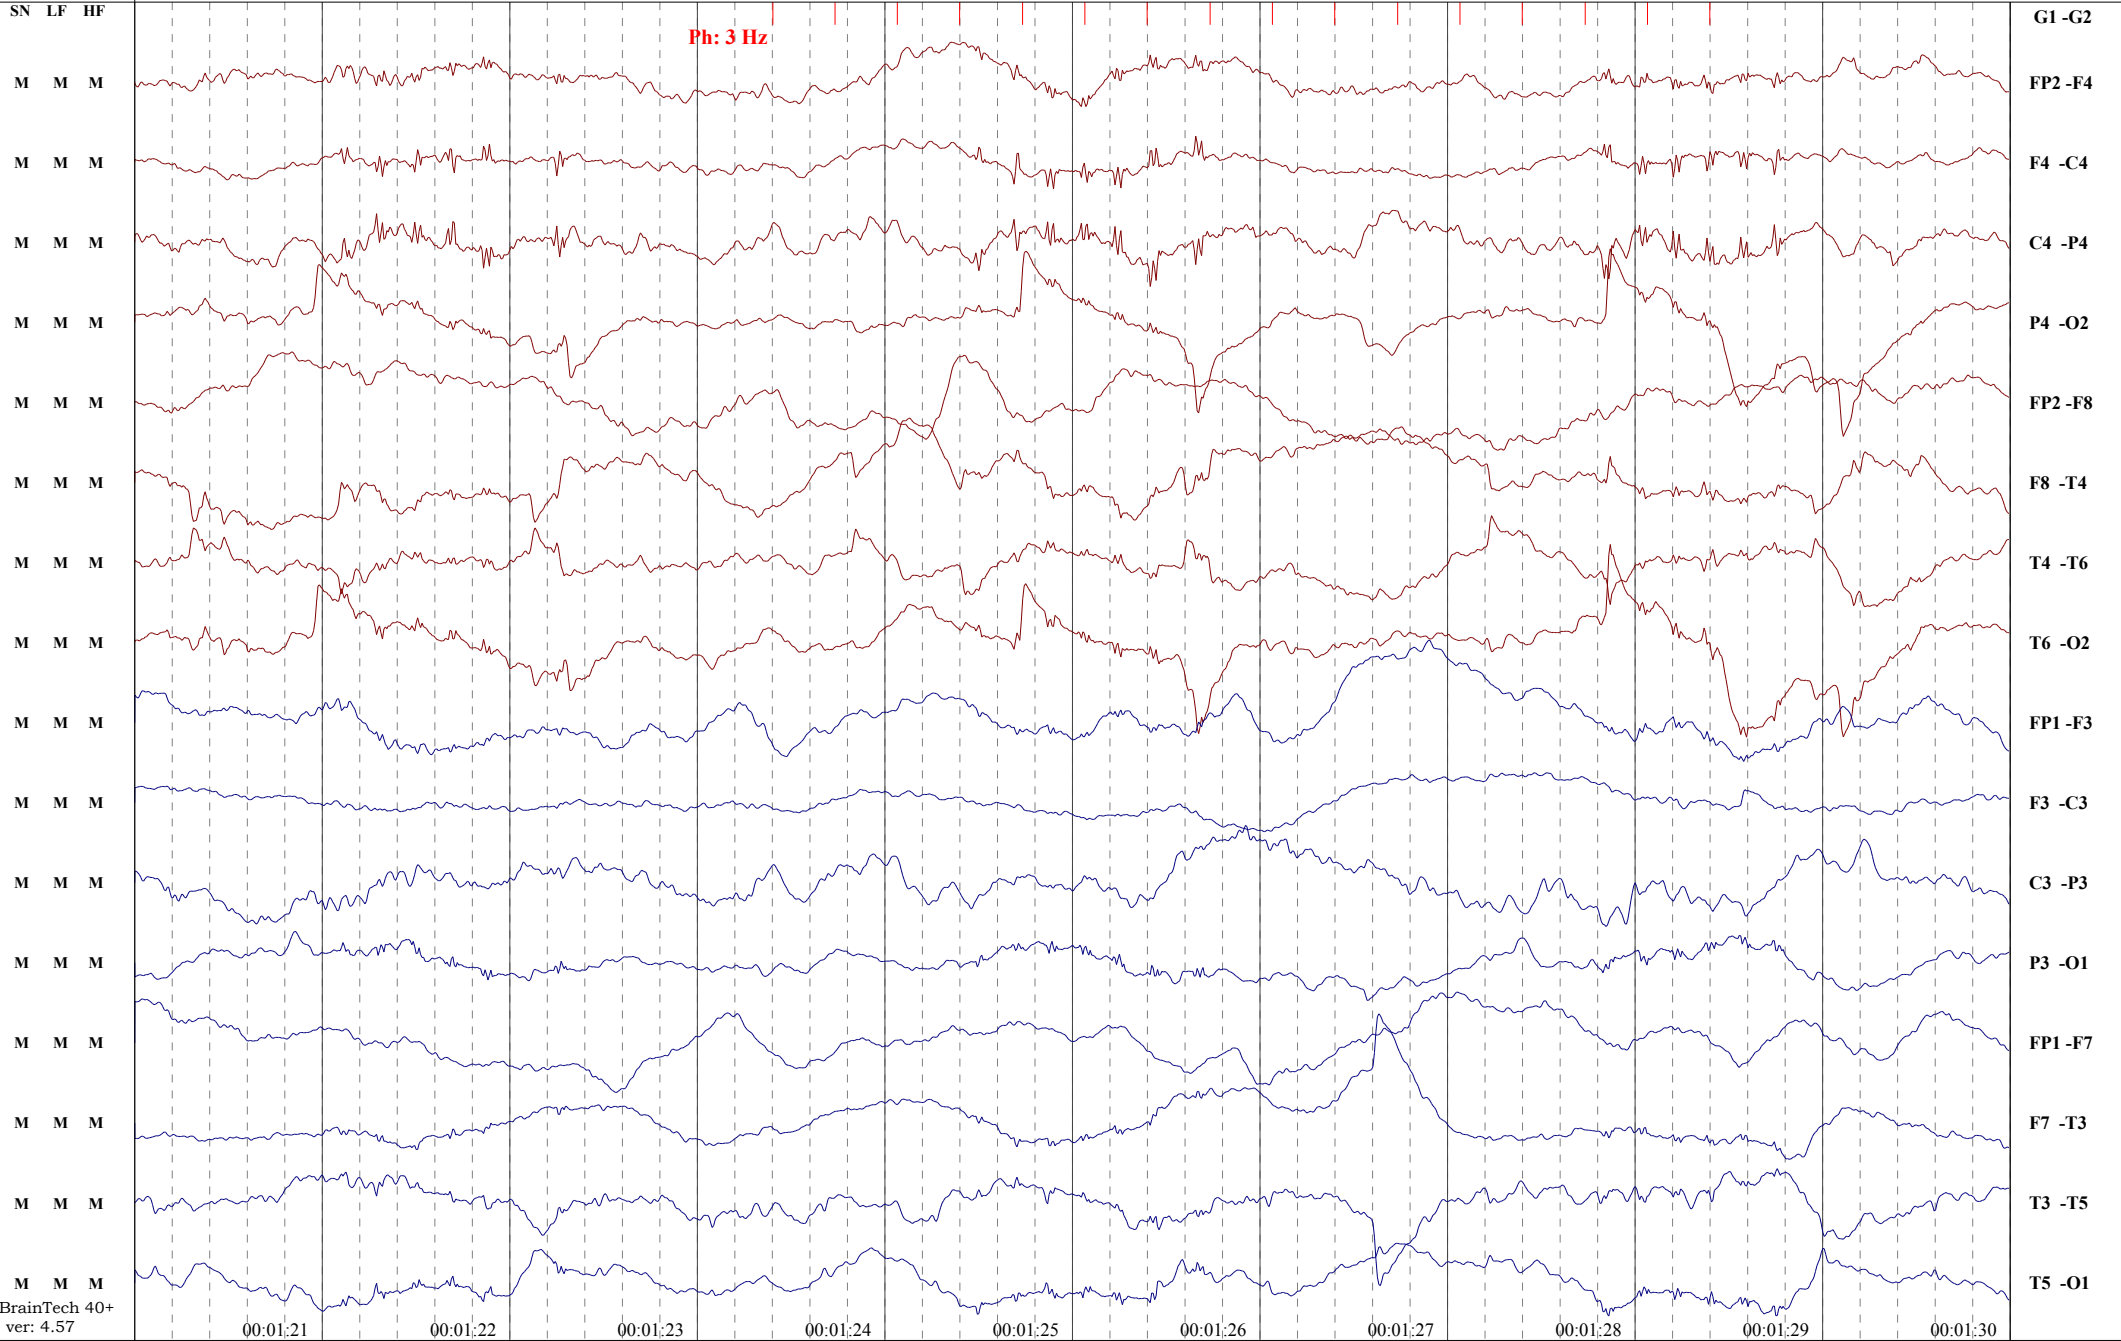


69  
MR. NIRANJAN SAHU  
42 Years/M

Date: 17-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:47:49  
Page:10/25  
Notch: ON

Ref:DR.RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

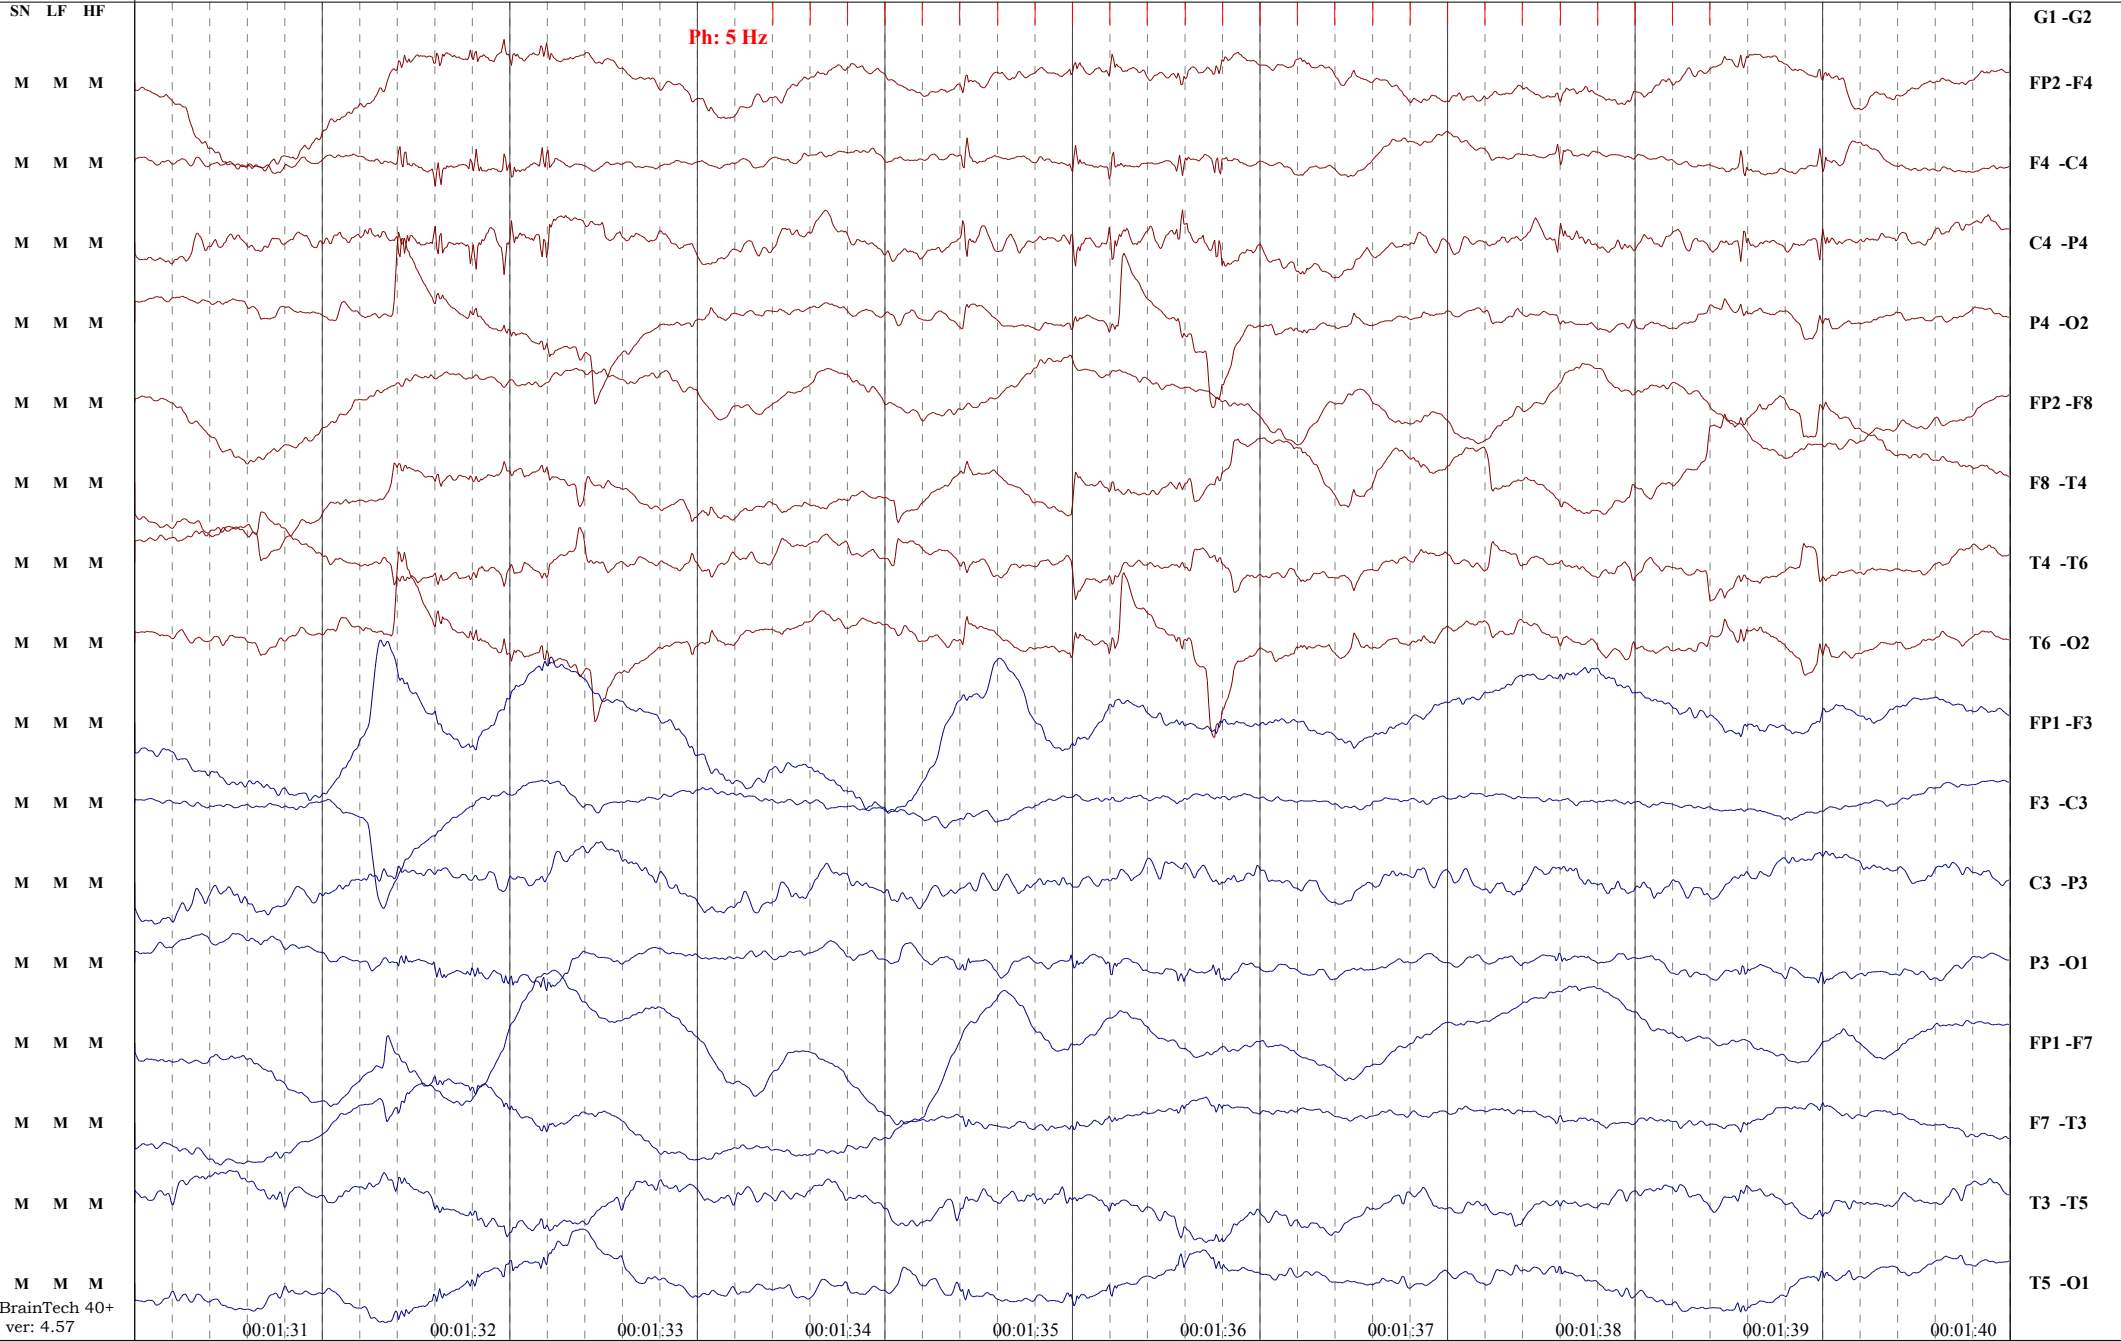




69  
MR. NIRANJAN SAHU  
42 Years/M

Date: 17-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:47:59  
Page:11/25  
Notch: ON

Ref:DR.RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

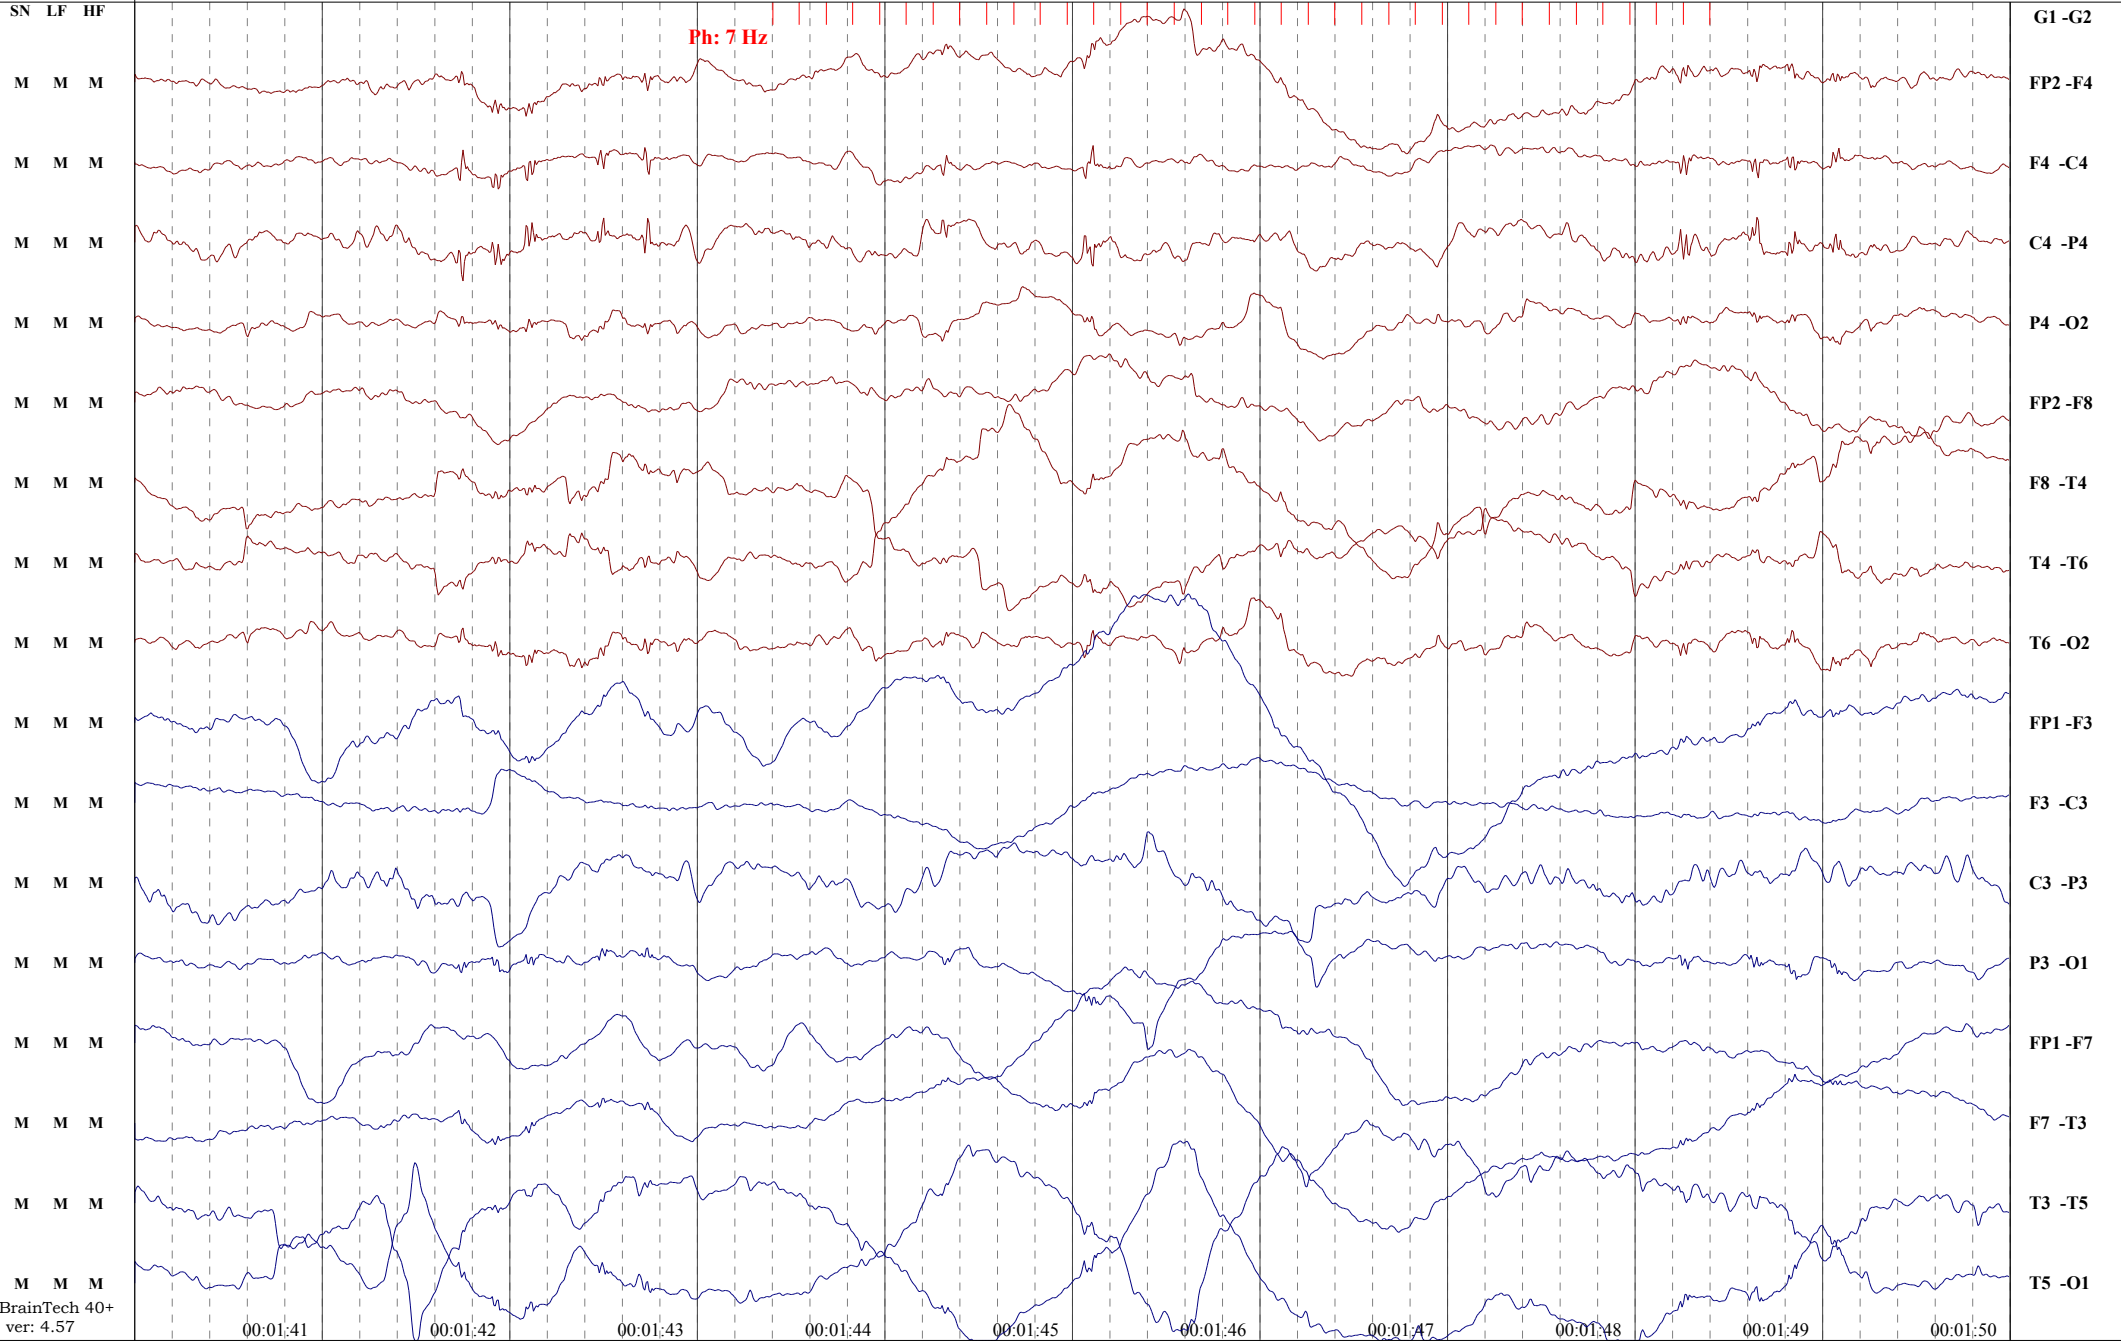


69  
MR. NIRANJAN SAHU  
42 Years/M

Date: 17-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:48:09  
Page:12/25  
Notch: ON

Ref:DR.RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

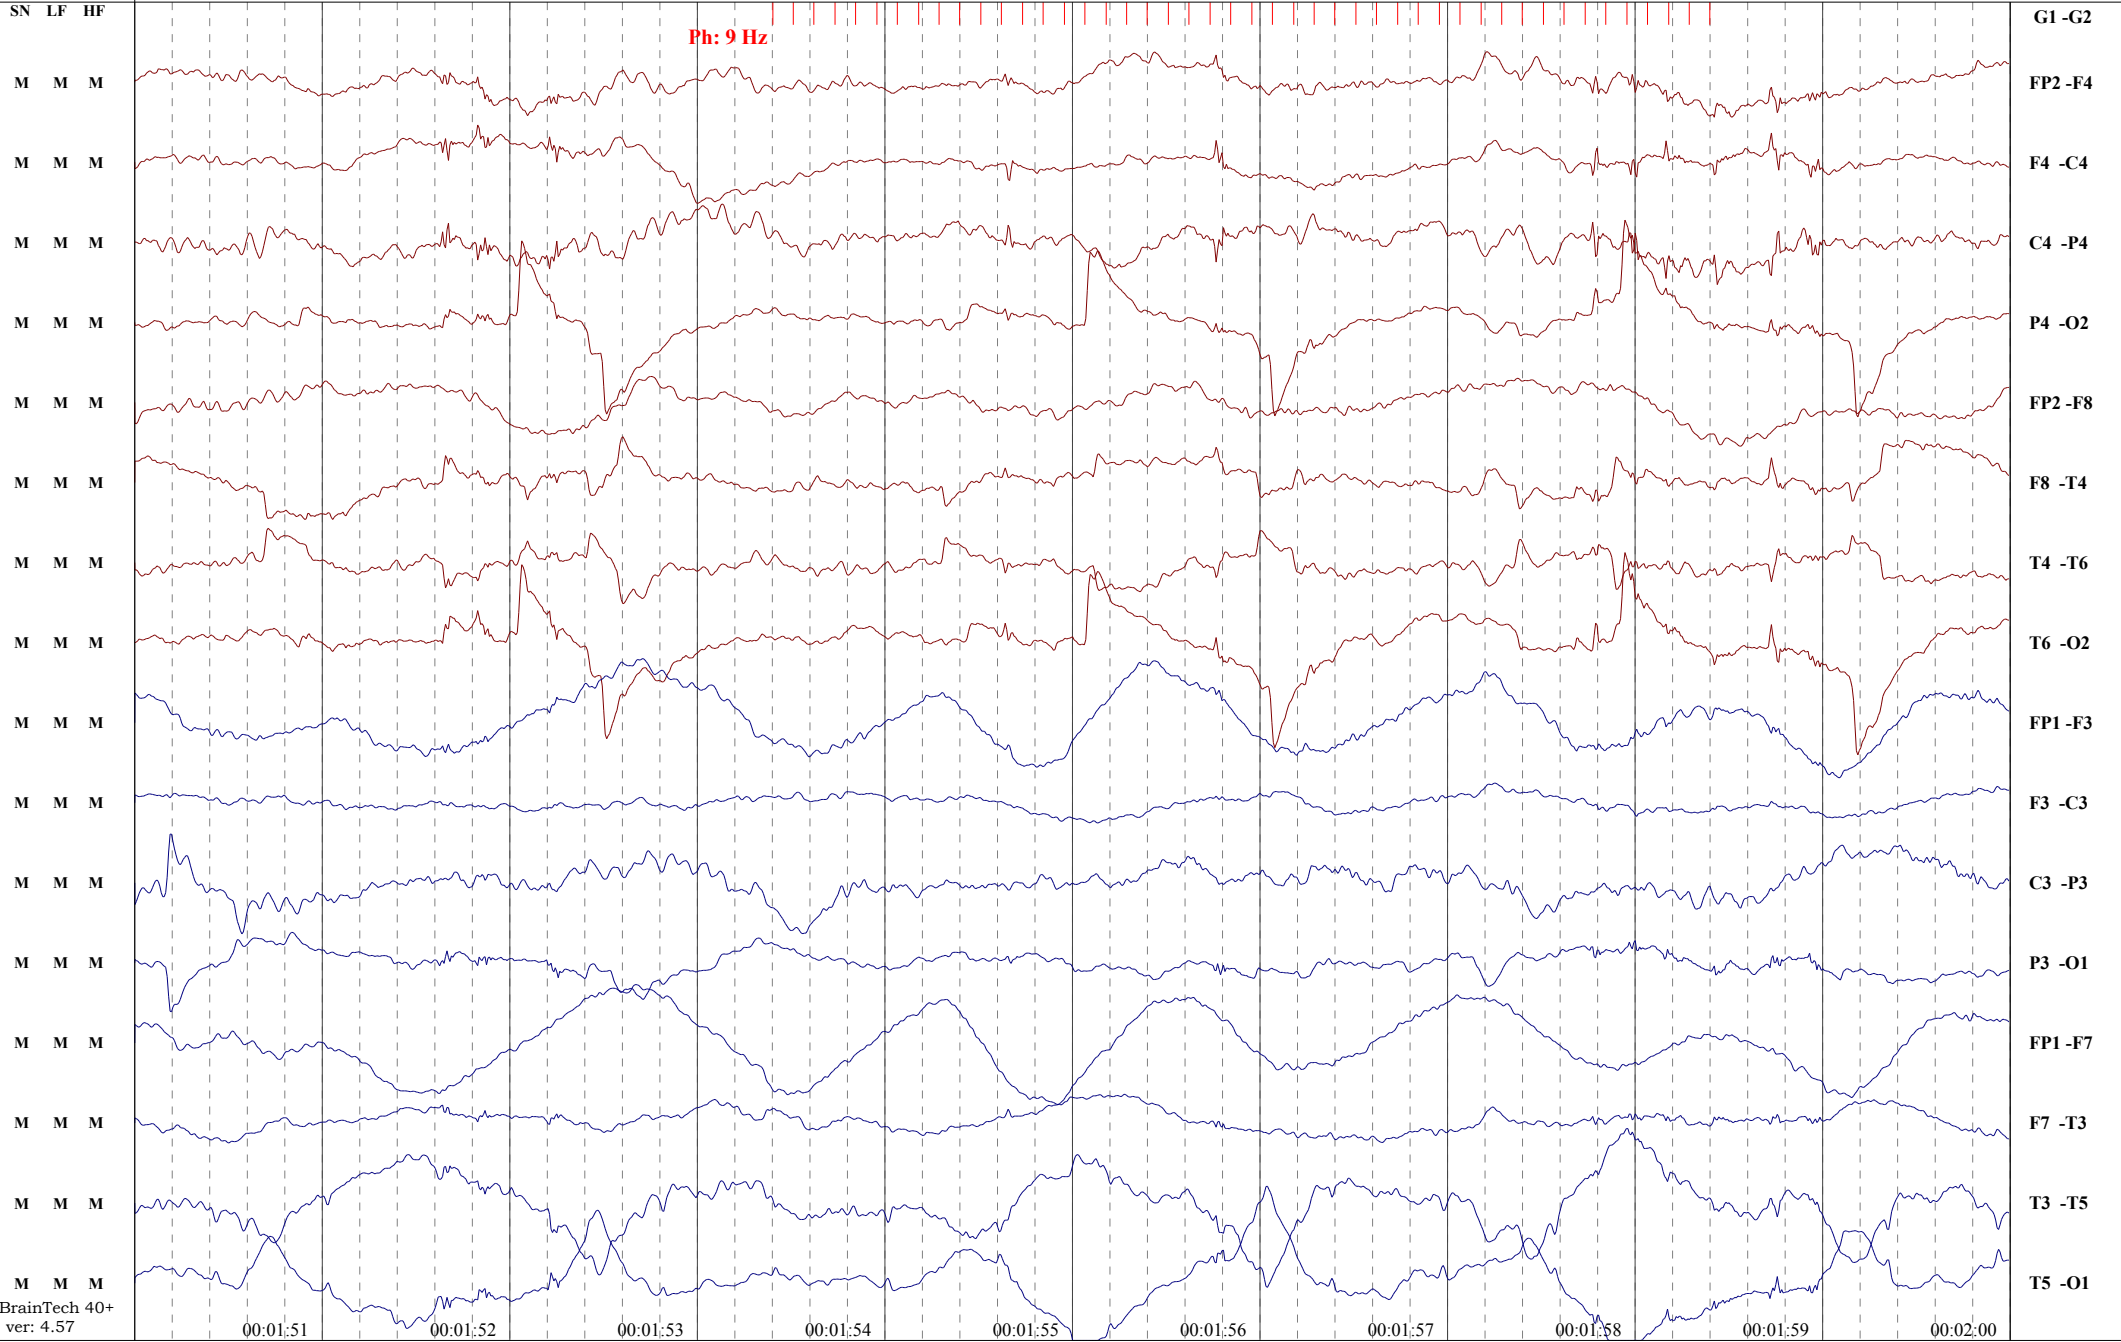


69  
MR. NIRANJAN SAHU  
42 Years/M

Date: 17-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:48:19  
Page:13/25  
Notch: ON

Ref:DR.RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

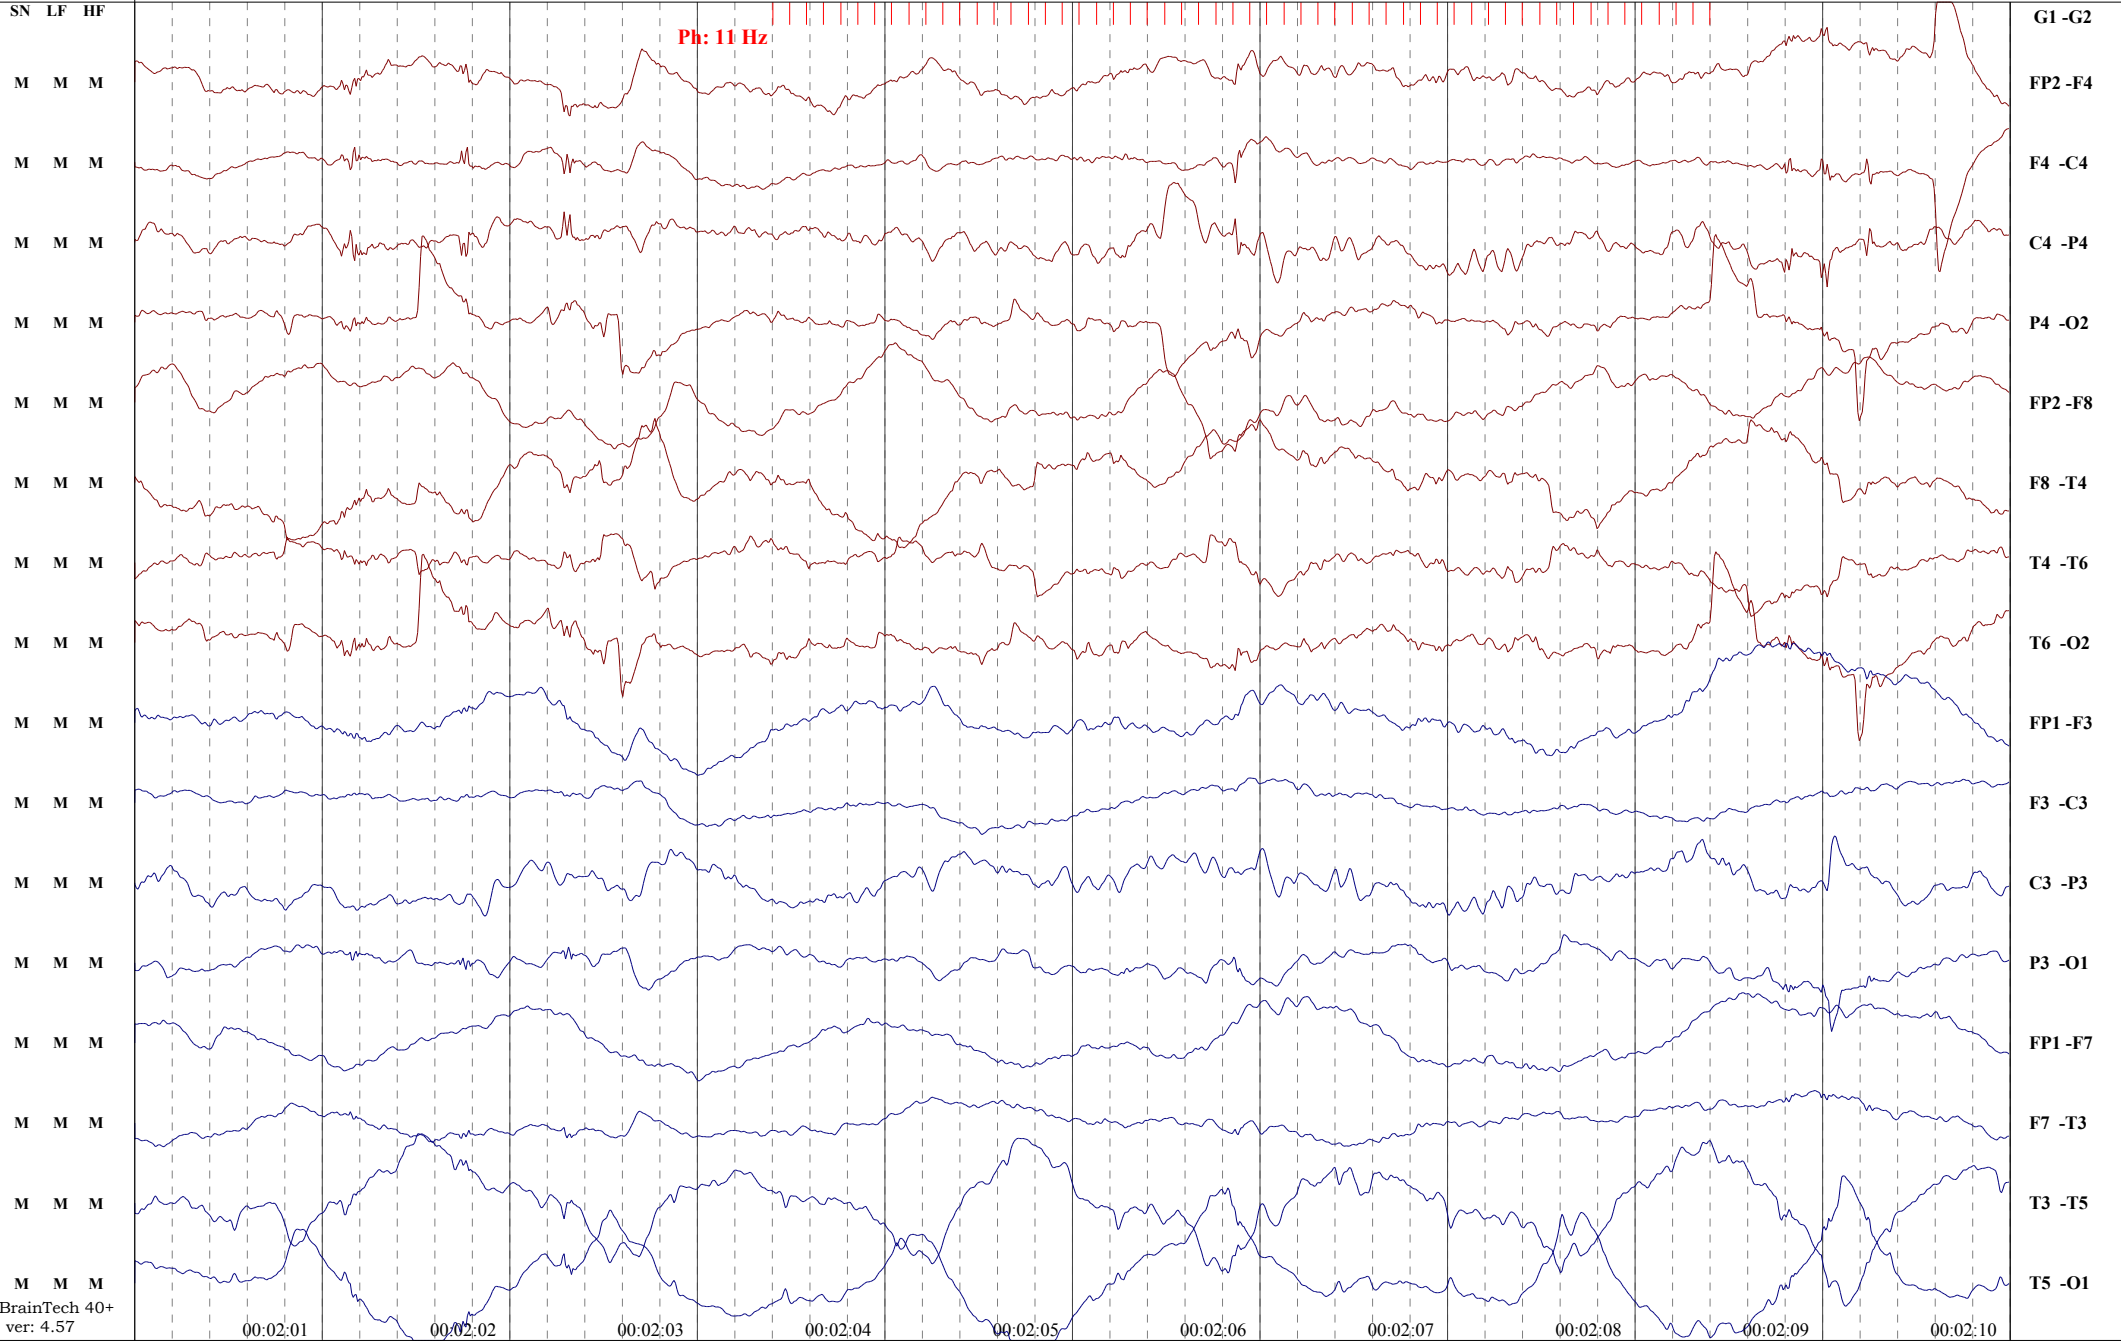


69  
MR. NIRANJAN SAHU  
42 Years/M

Date: 17-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:48:29  
Page:14/25  
Notch: ON

Ref:DR.RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

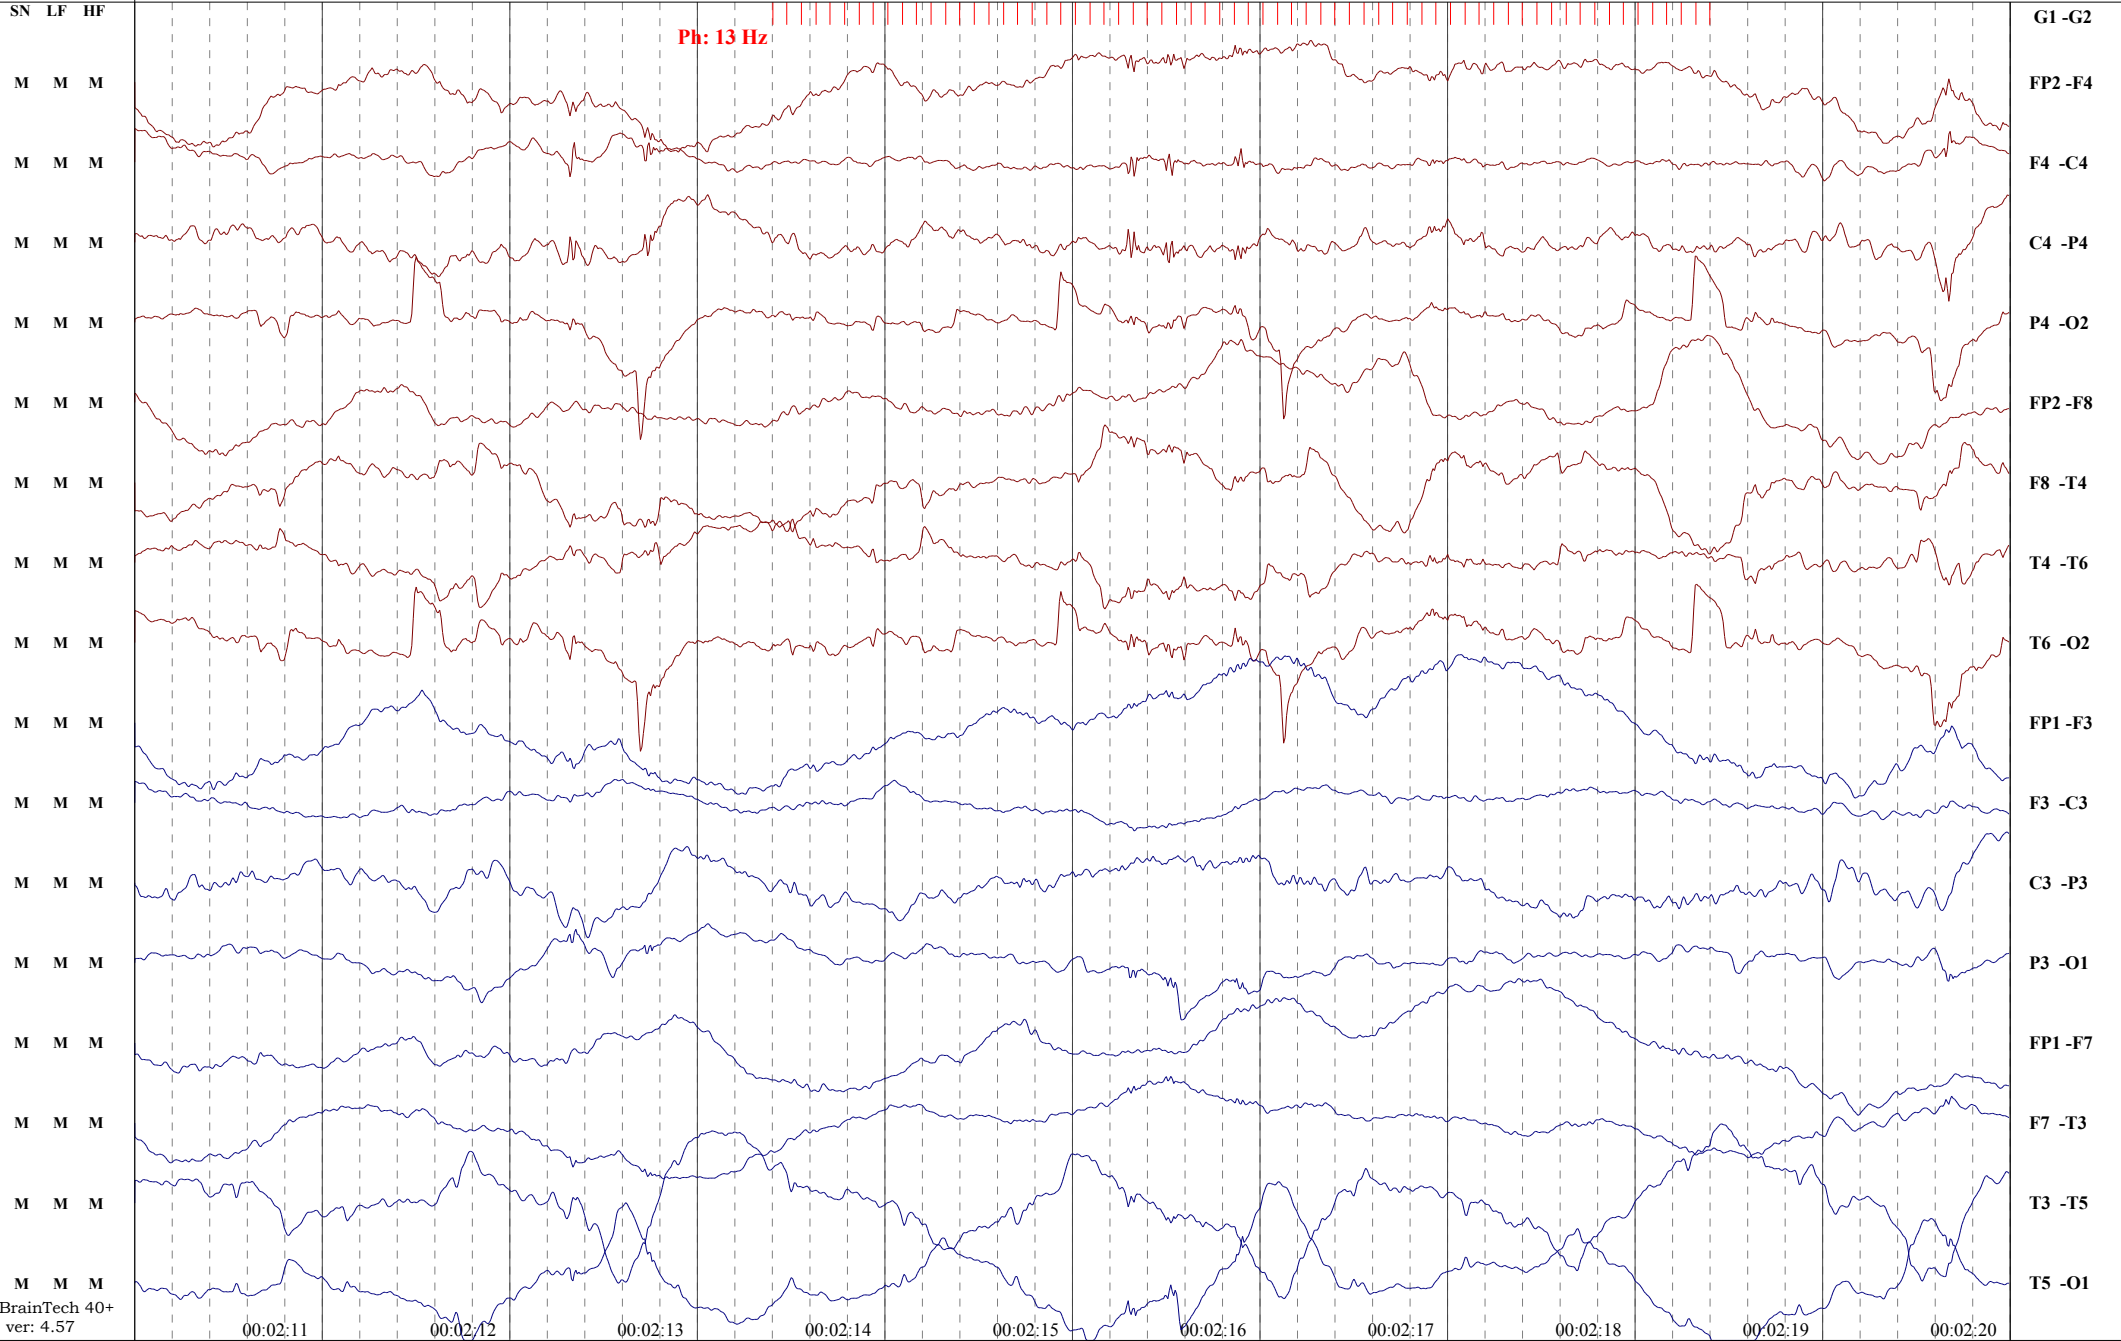


69  
MR. NIRANJAN SAHU  
42 Years/M

Date: 17-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:48:39  
Page:15/25  
Notch: ON

Ref:DR.RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

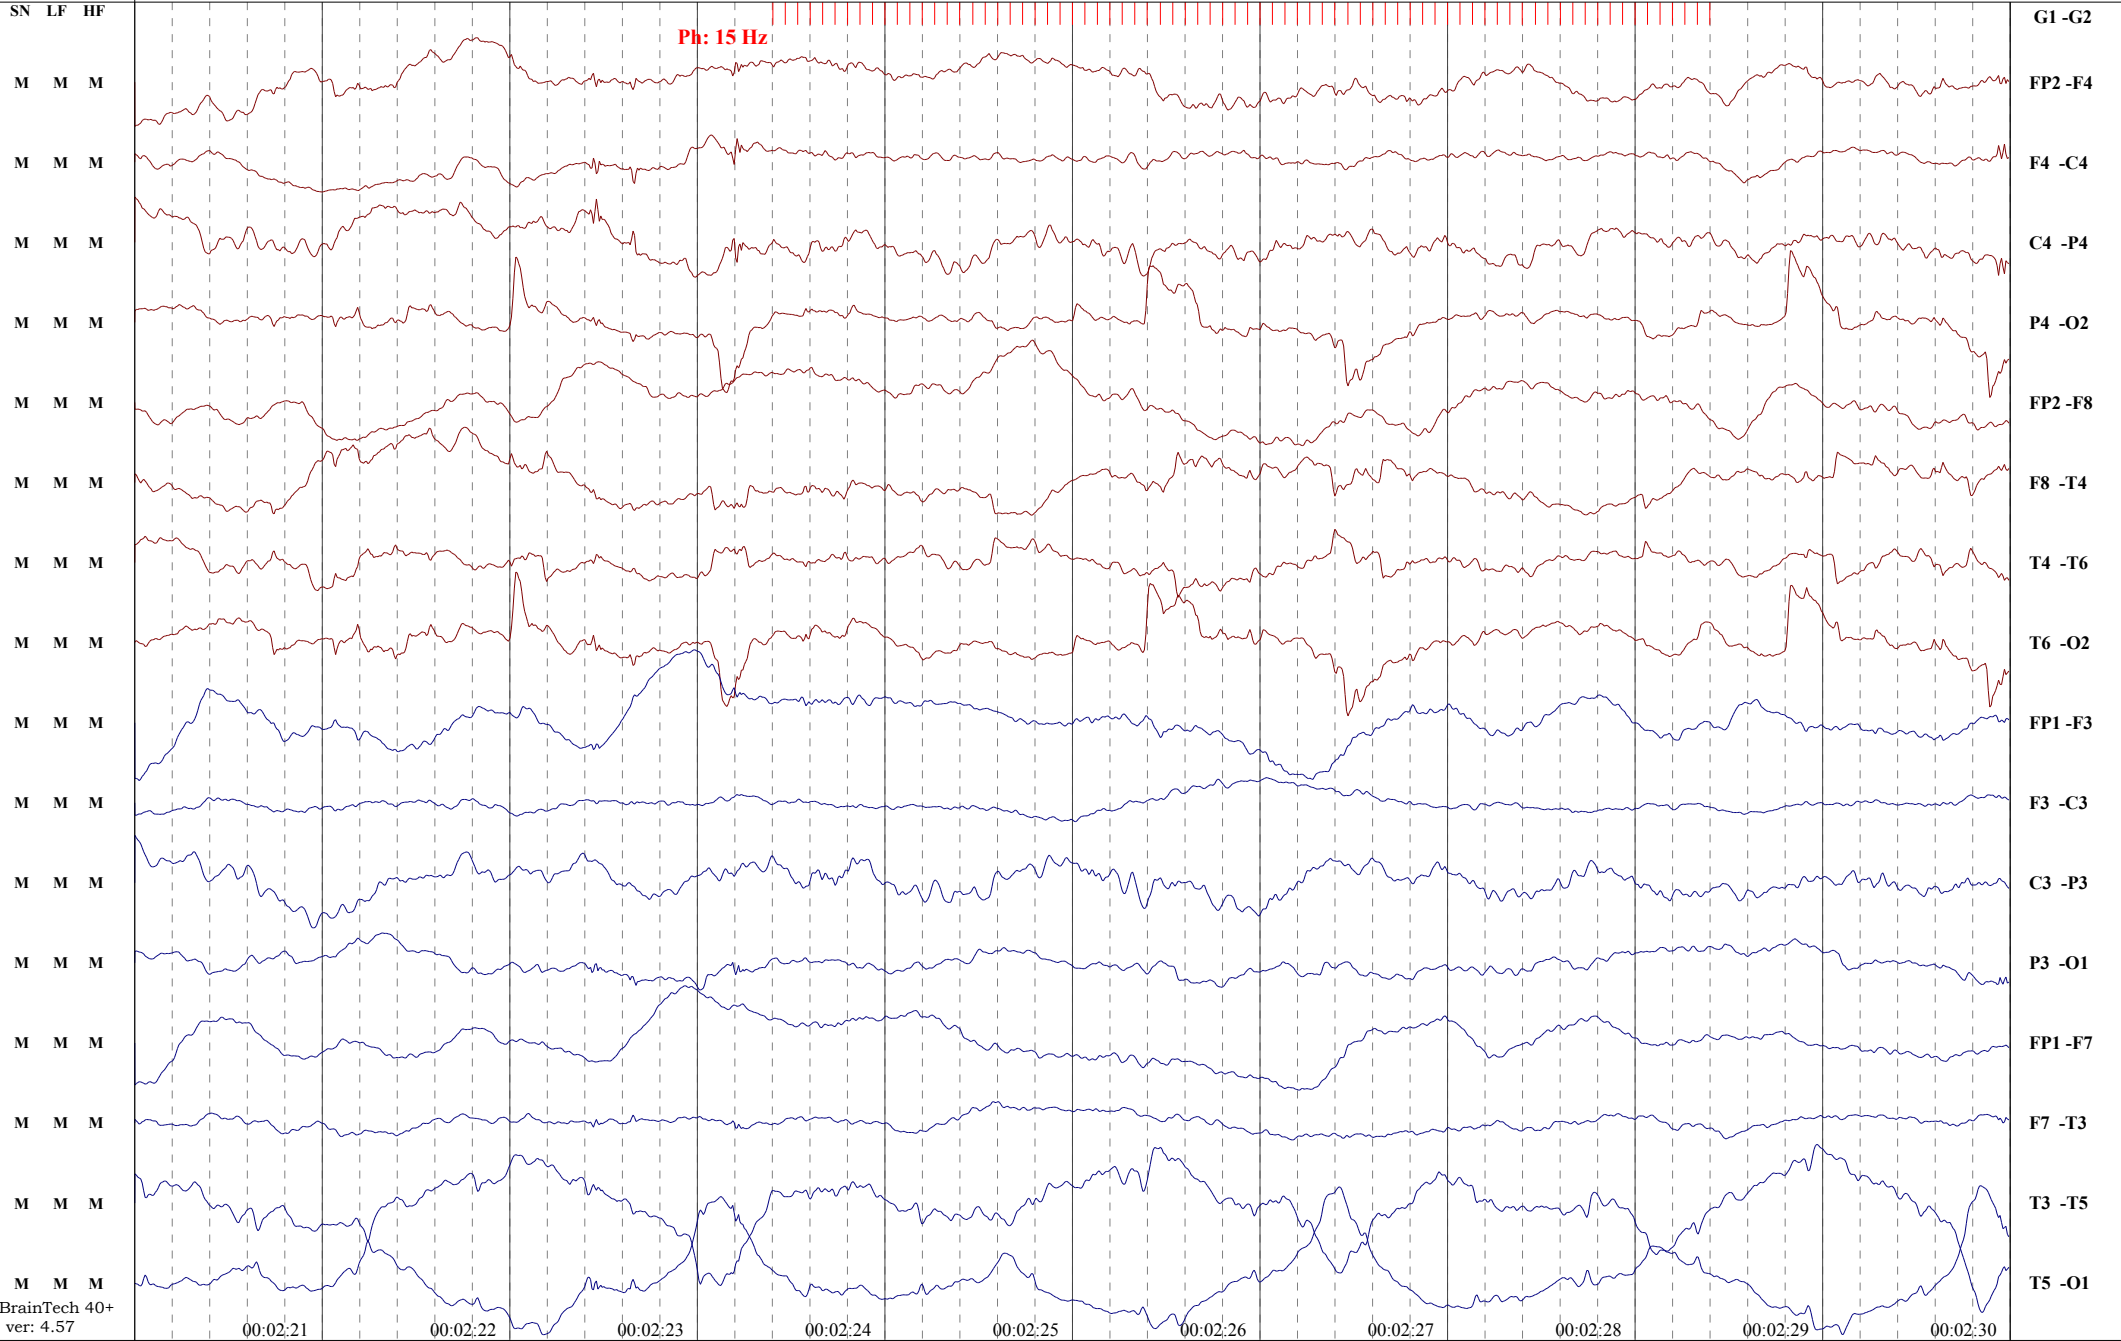


69  
MR. NIRANJAN SAHU  
42 Years/M

Date: 17-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:48:49  
Page:16/25  
Notch: ON

Ref:DR.RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

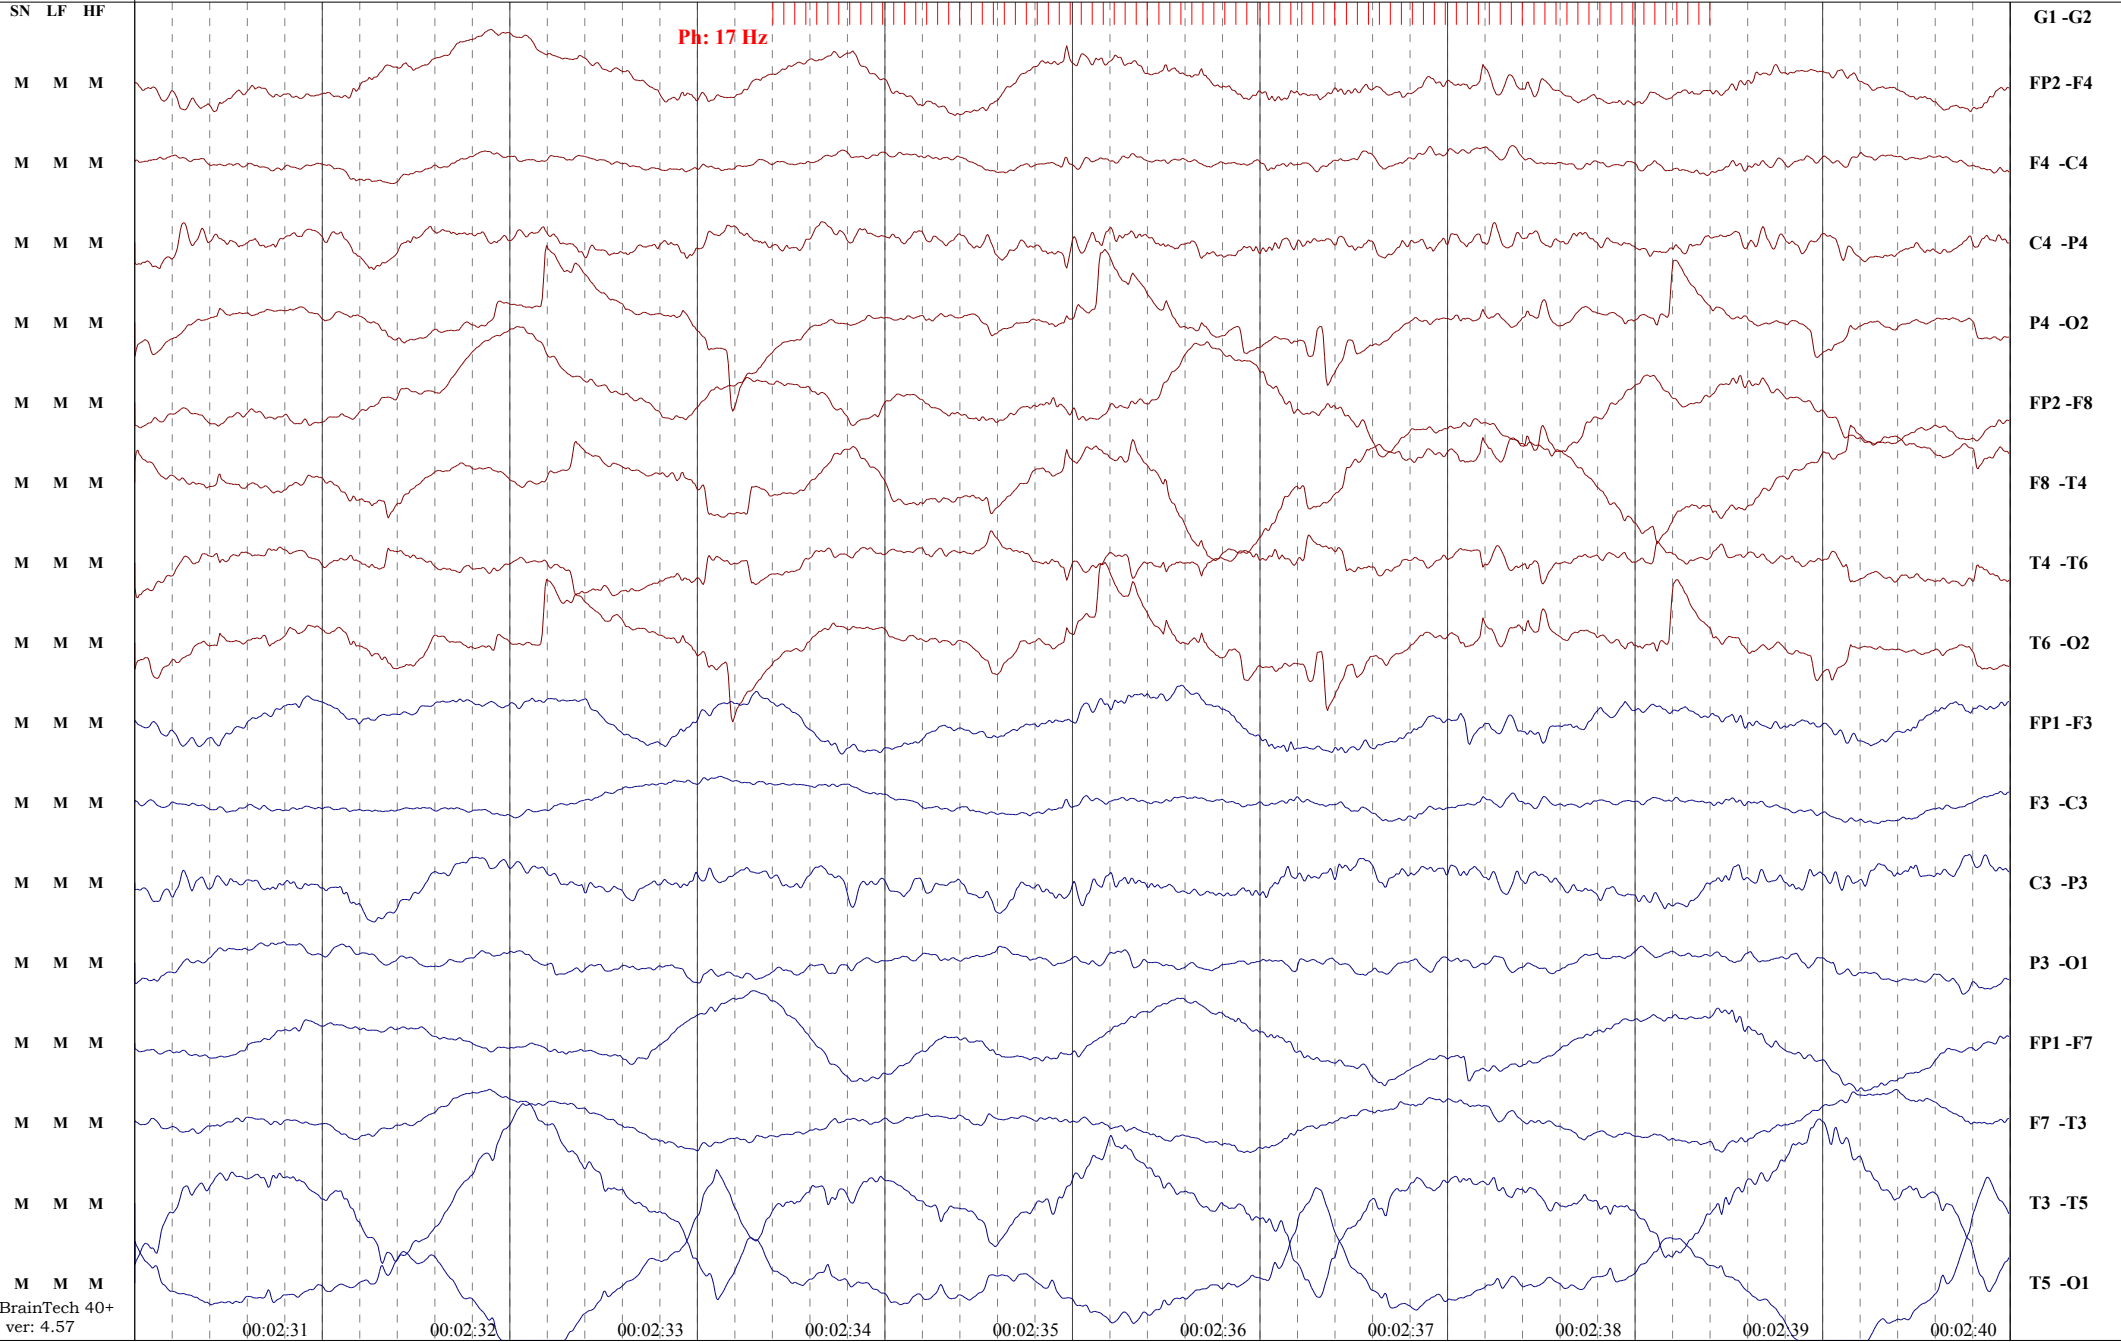




69  
MR. NIRANJAN SAHU  
42 Years/M

Date: 17-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:48:59  
Page:17/25  
Notch: ON

Ref:DR.RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

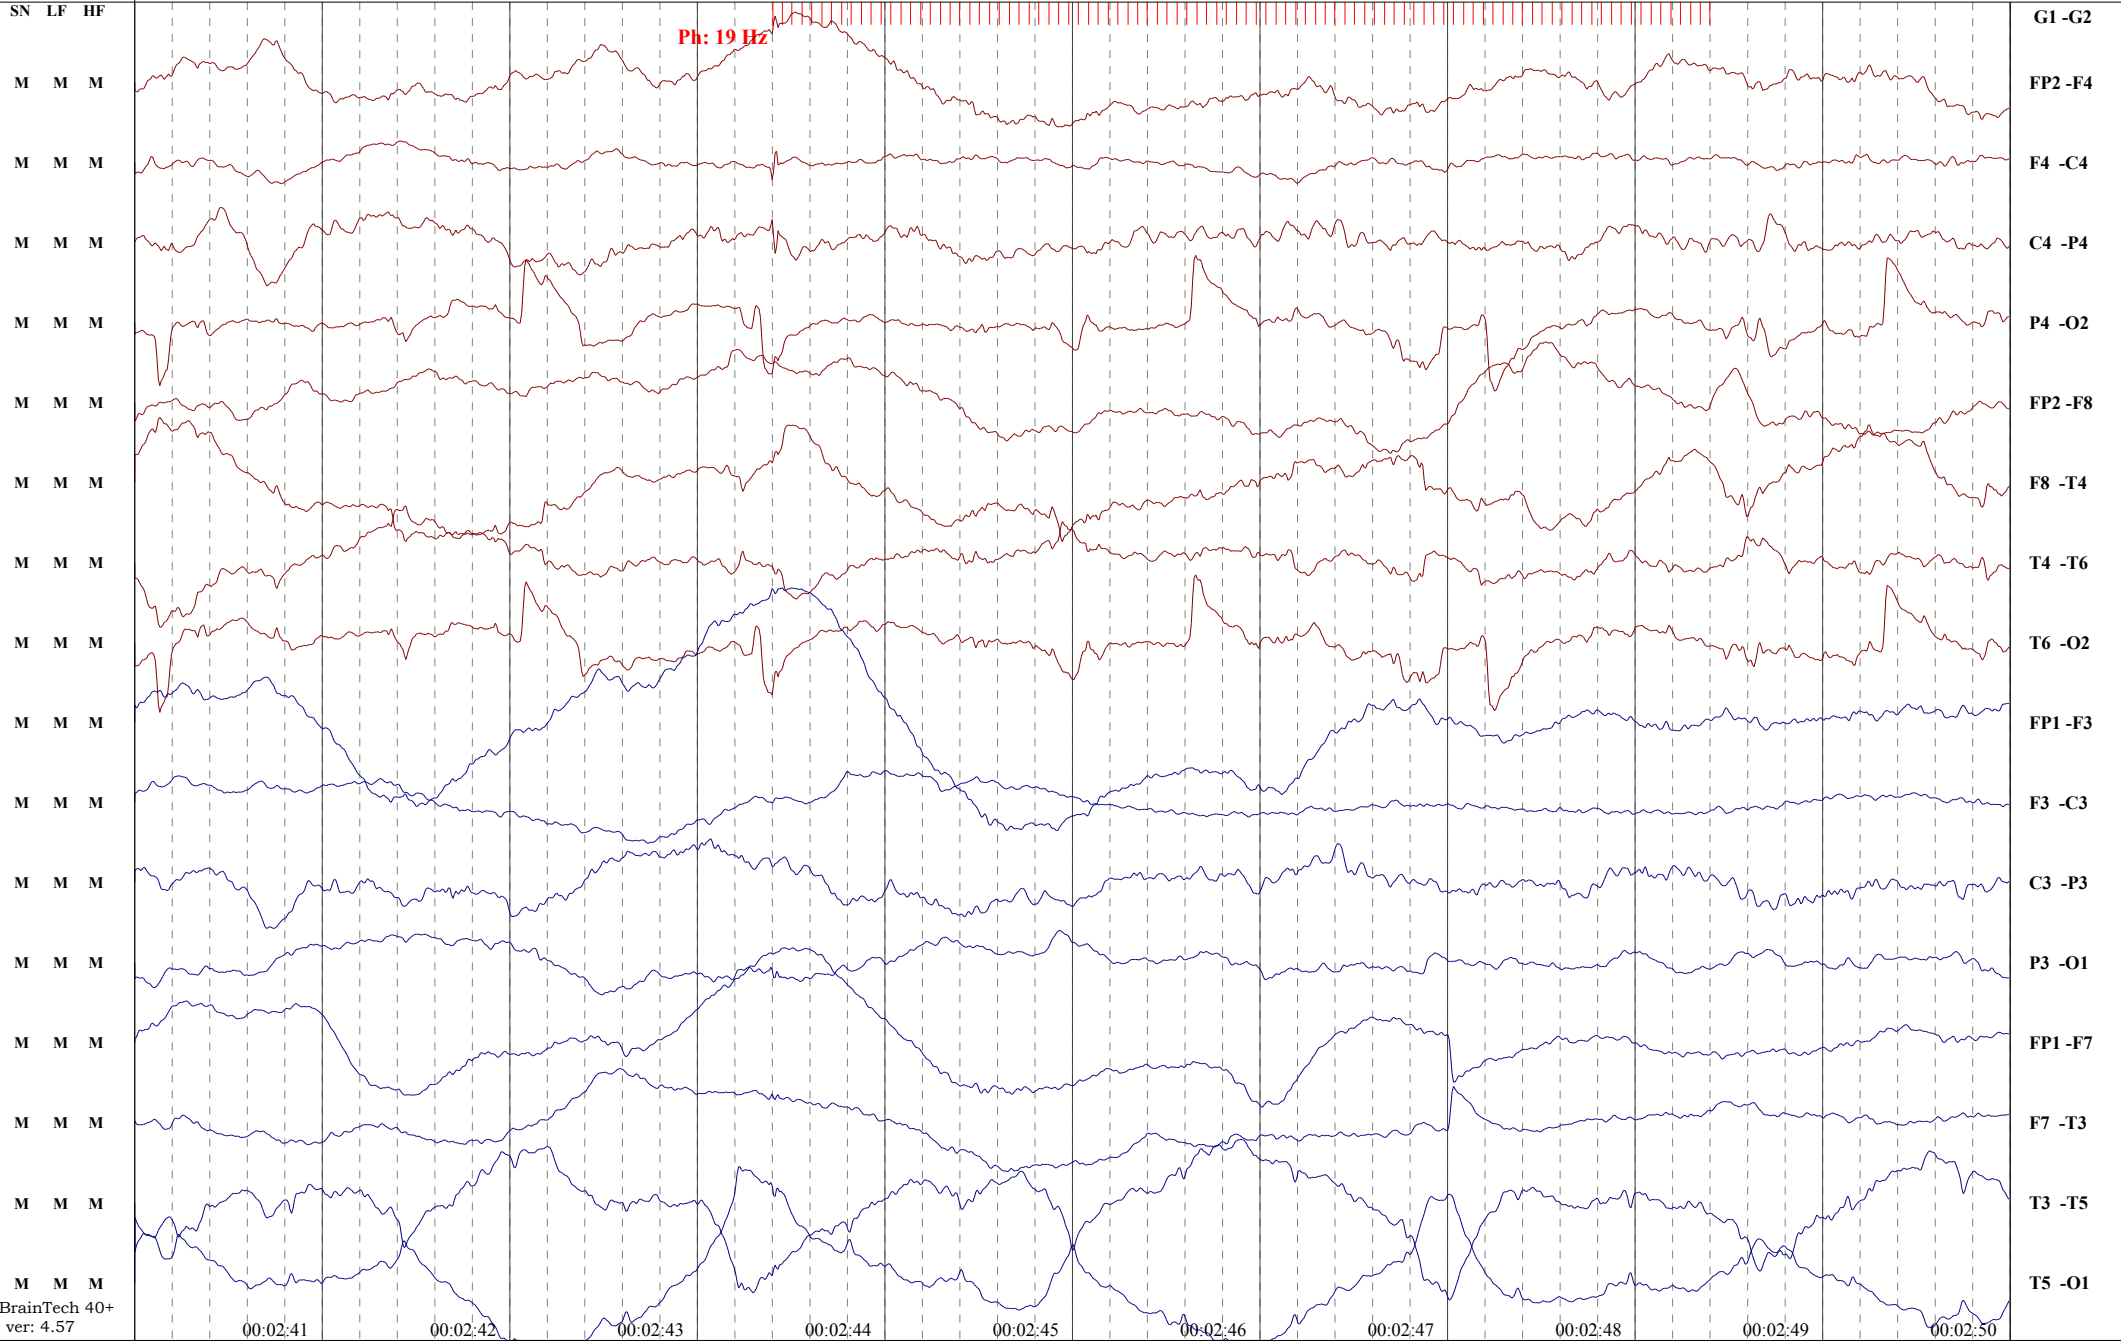


69  
MR. NIRANJAN SAHU  
42 Years/M

Date: 17-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:49:09  
Page:18/25  
Notch: ON

Ref:DR.RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

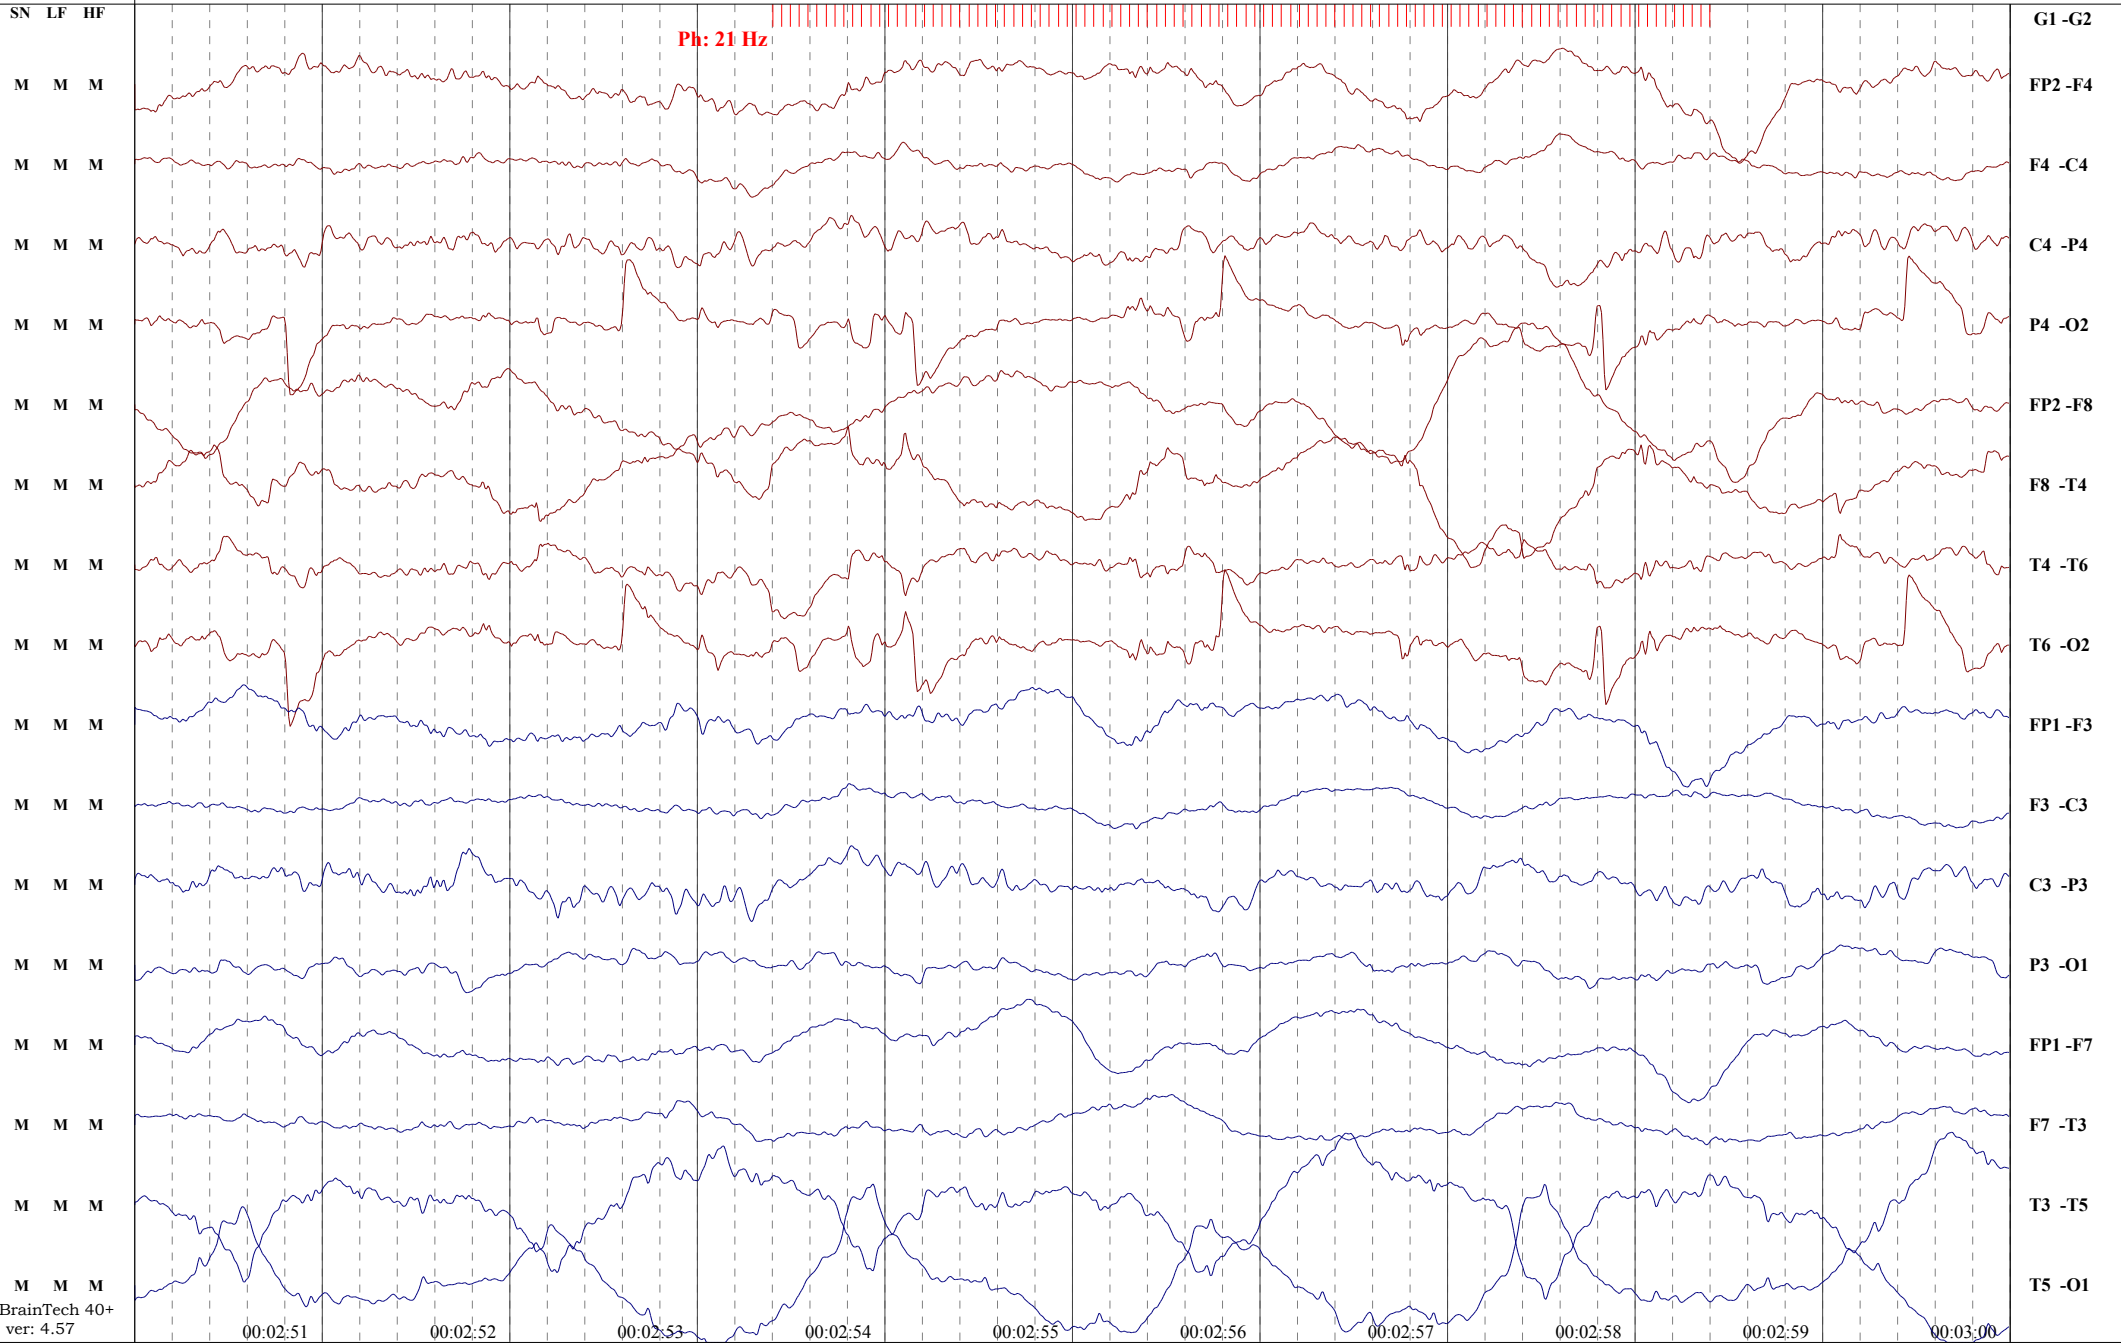

69  
MR. NIRANJAN SAHU  
42 Years/M


Date: 17-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:49:19  
Page:19/25  
Notch: ON

Ref:DR.RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

Photic OFF

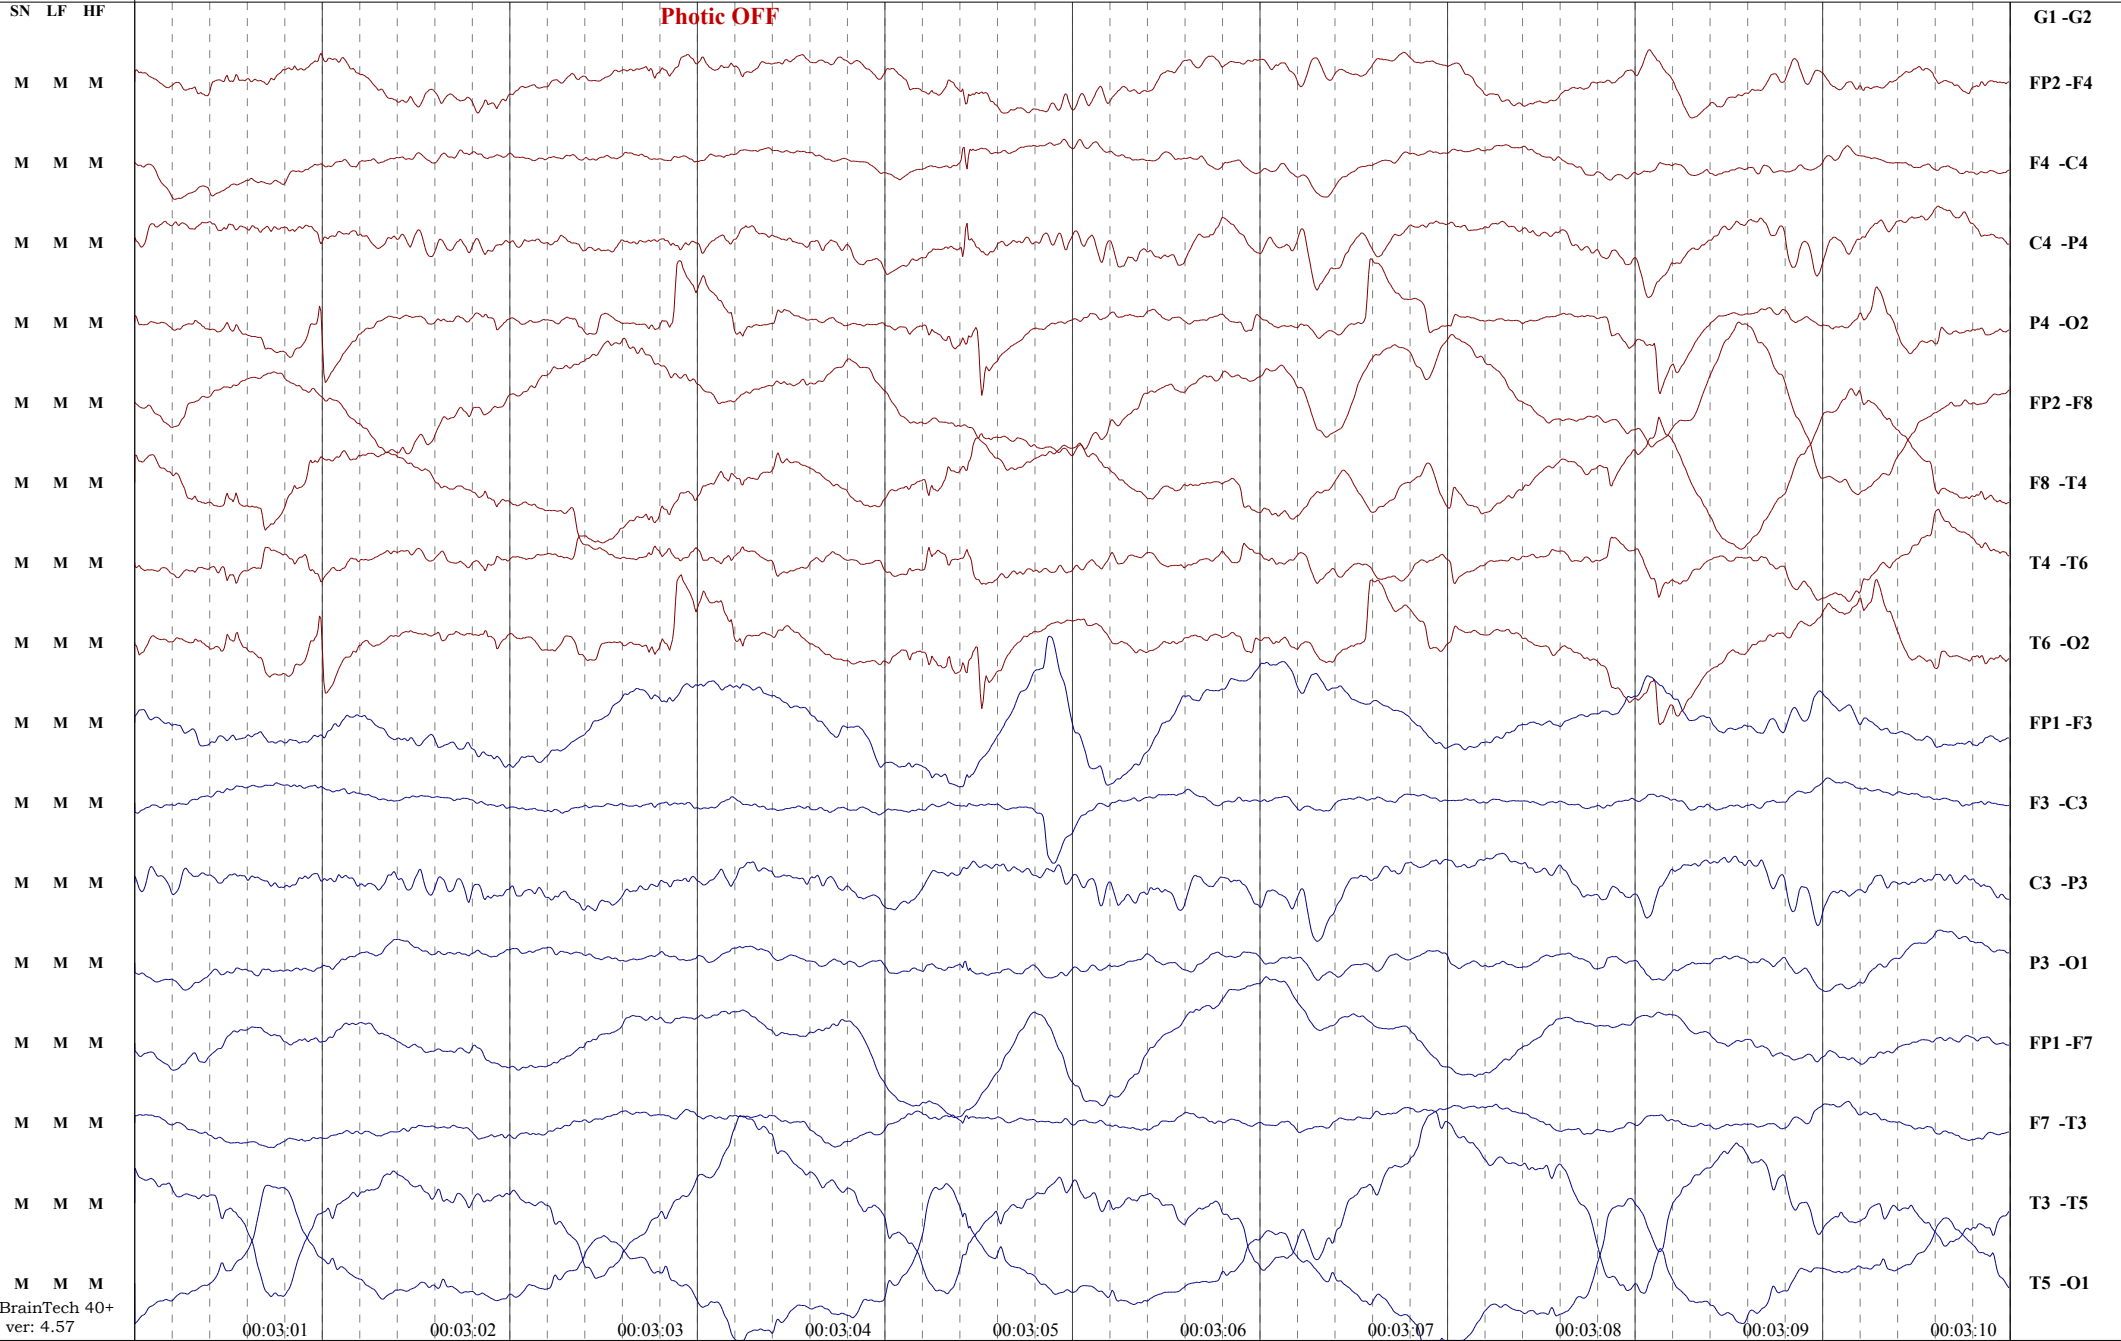


69  
MR. NIRANJAN SAHU  
42 Years/M

Date: 17-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:49:29  
Page:20/25  
Notch: ON

Ref:DR.RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

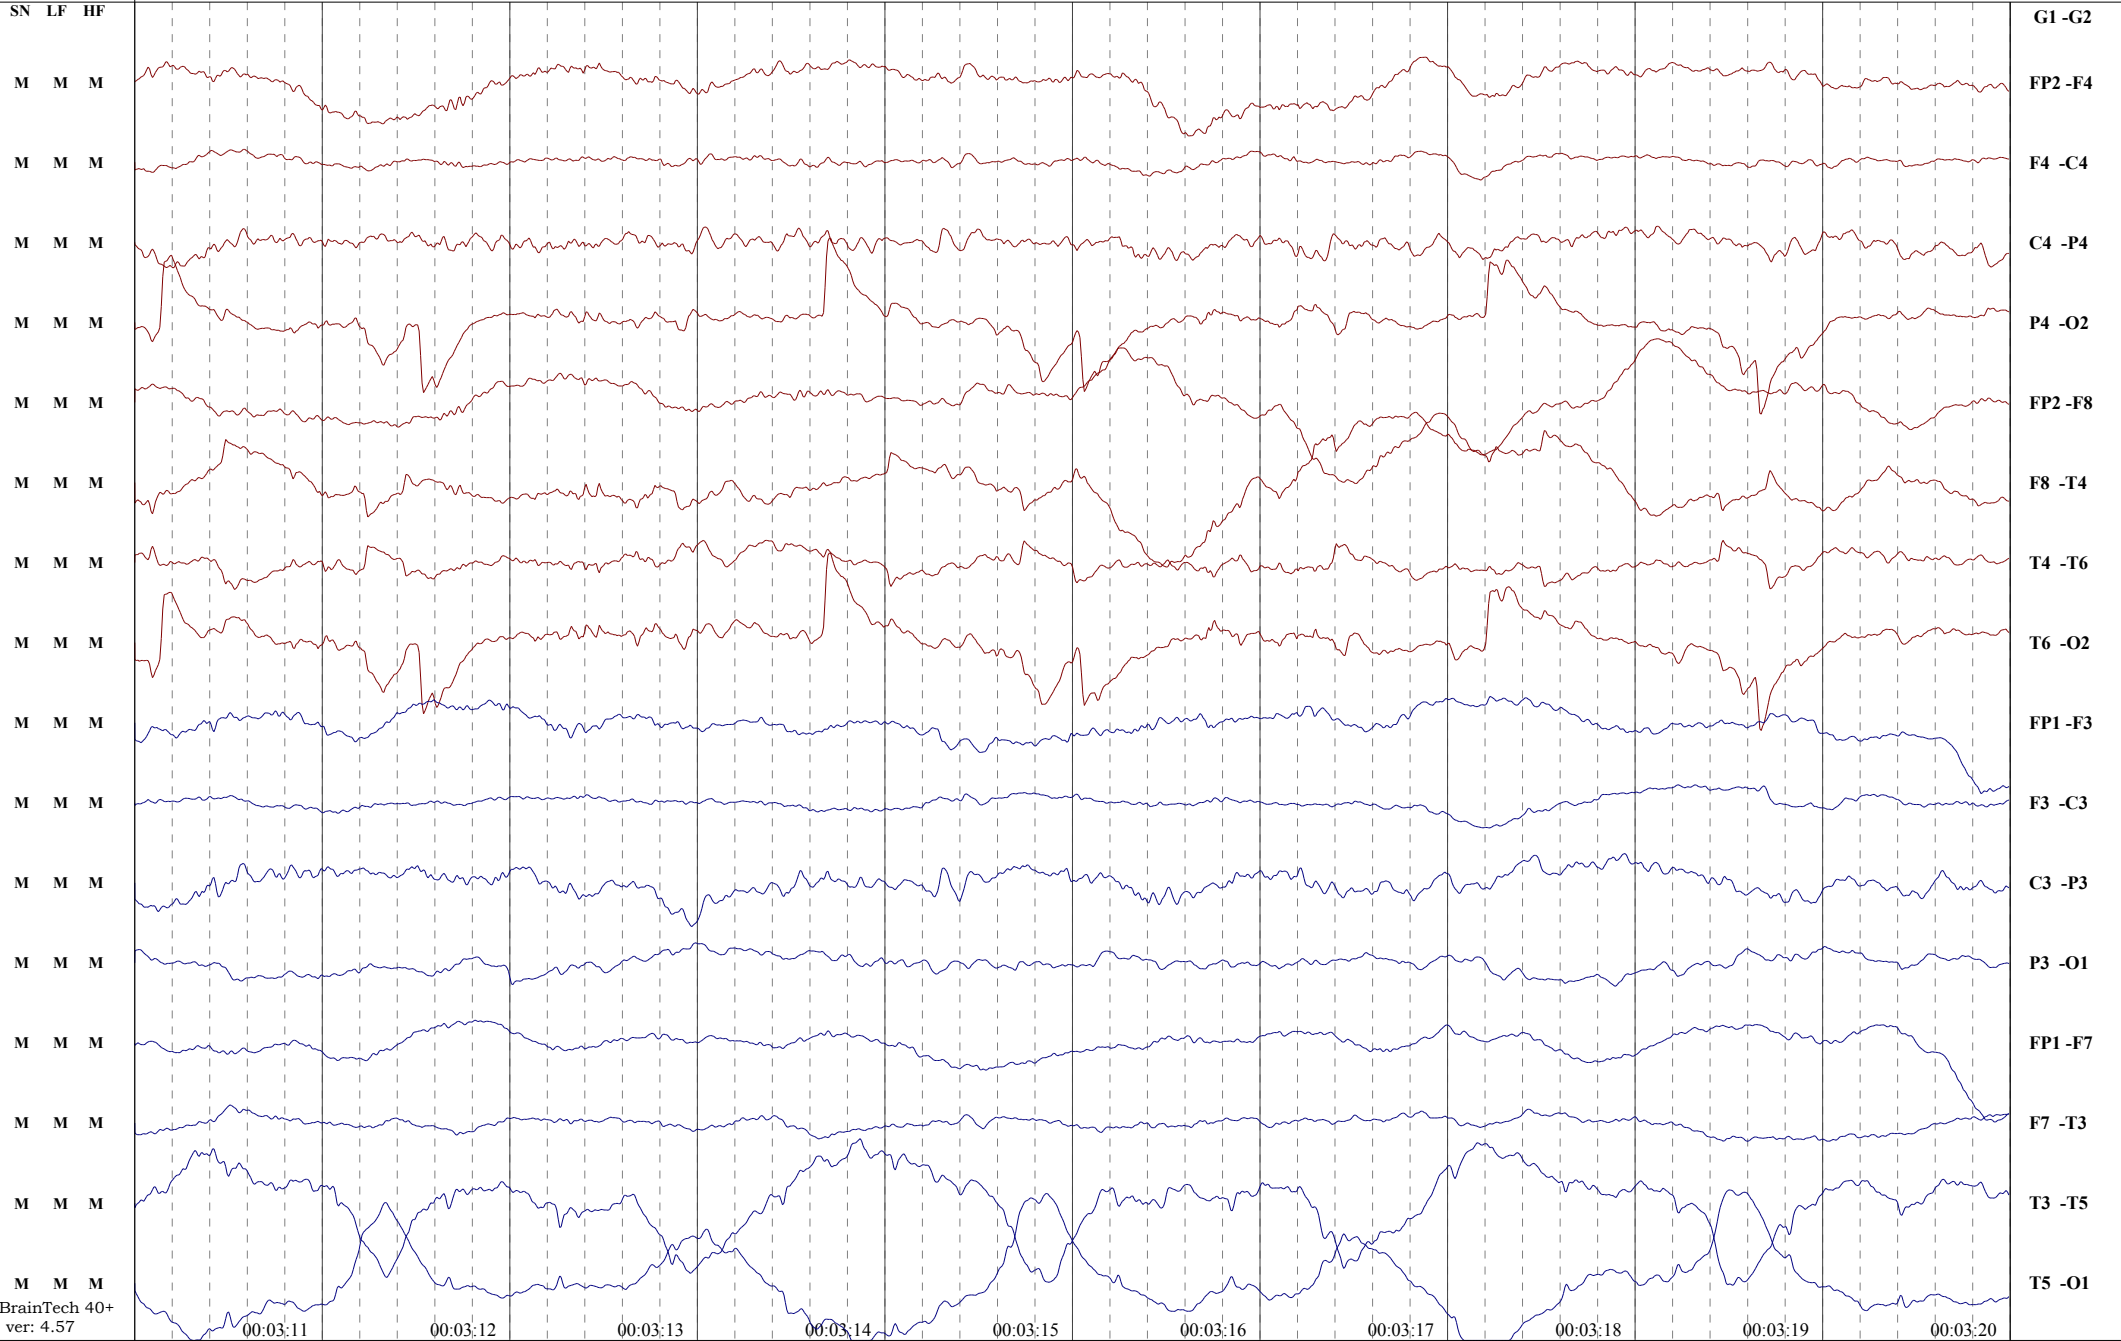


69  
MR. NIRANJAN SAHU  
42 Years/M

Date: 17-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:49:39  
Page:21/25  
Notch: ON

Ref:DR.RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

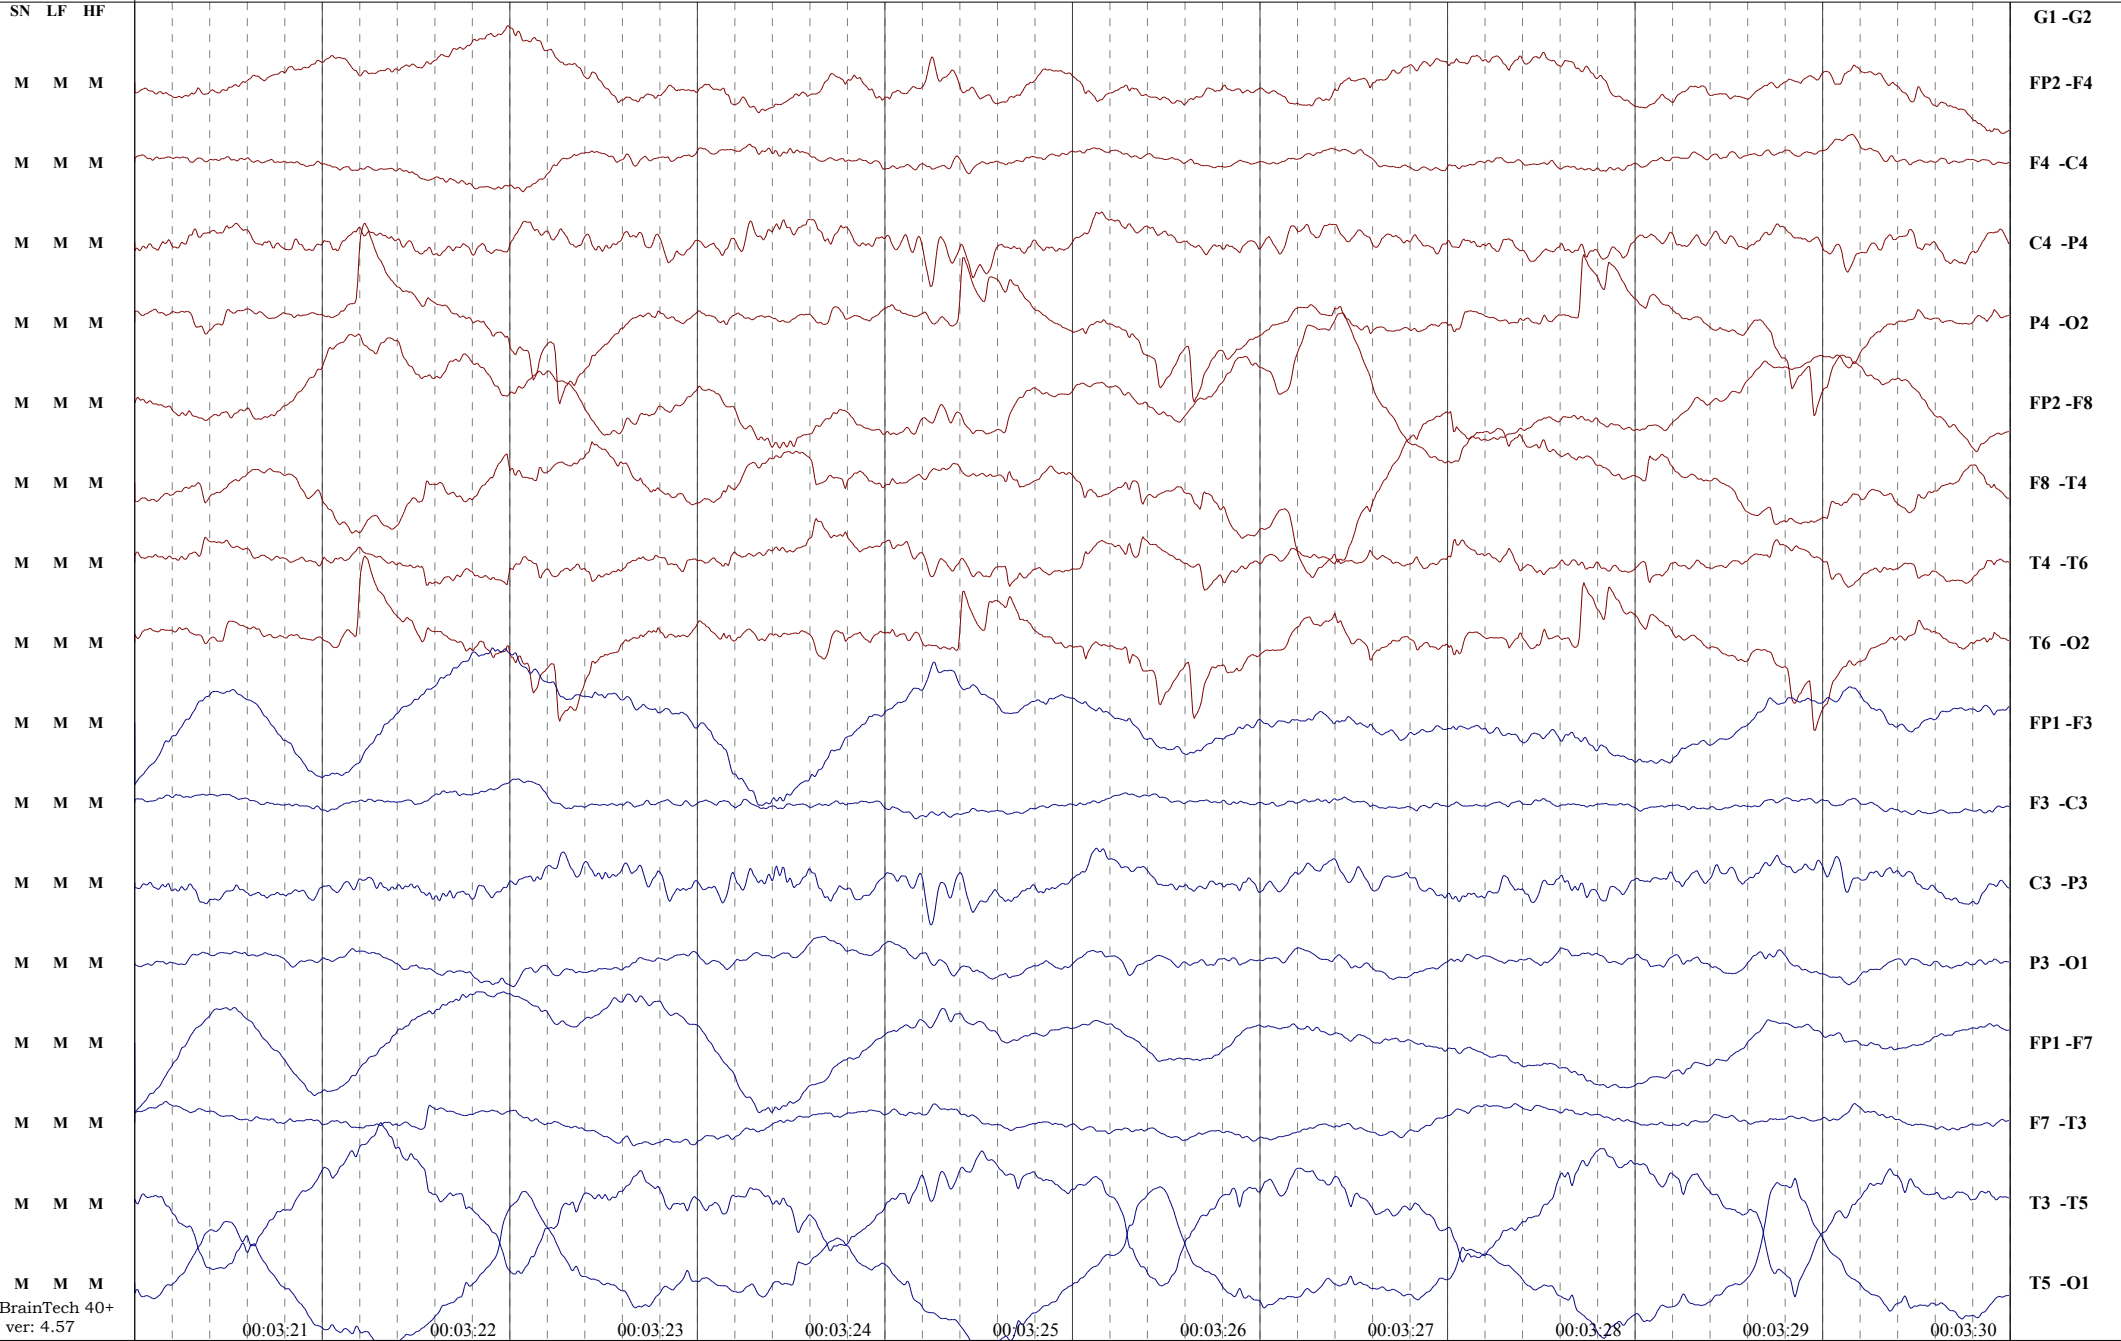


69  
MR. NIRANJAN SAHU  
42 Years/M

Date: 17-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:49:49  
Page:22/25  
Notch: ON

Ref:DR.RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

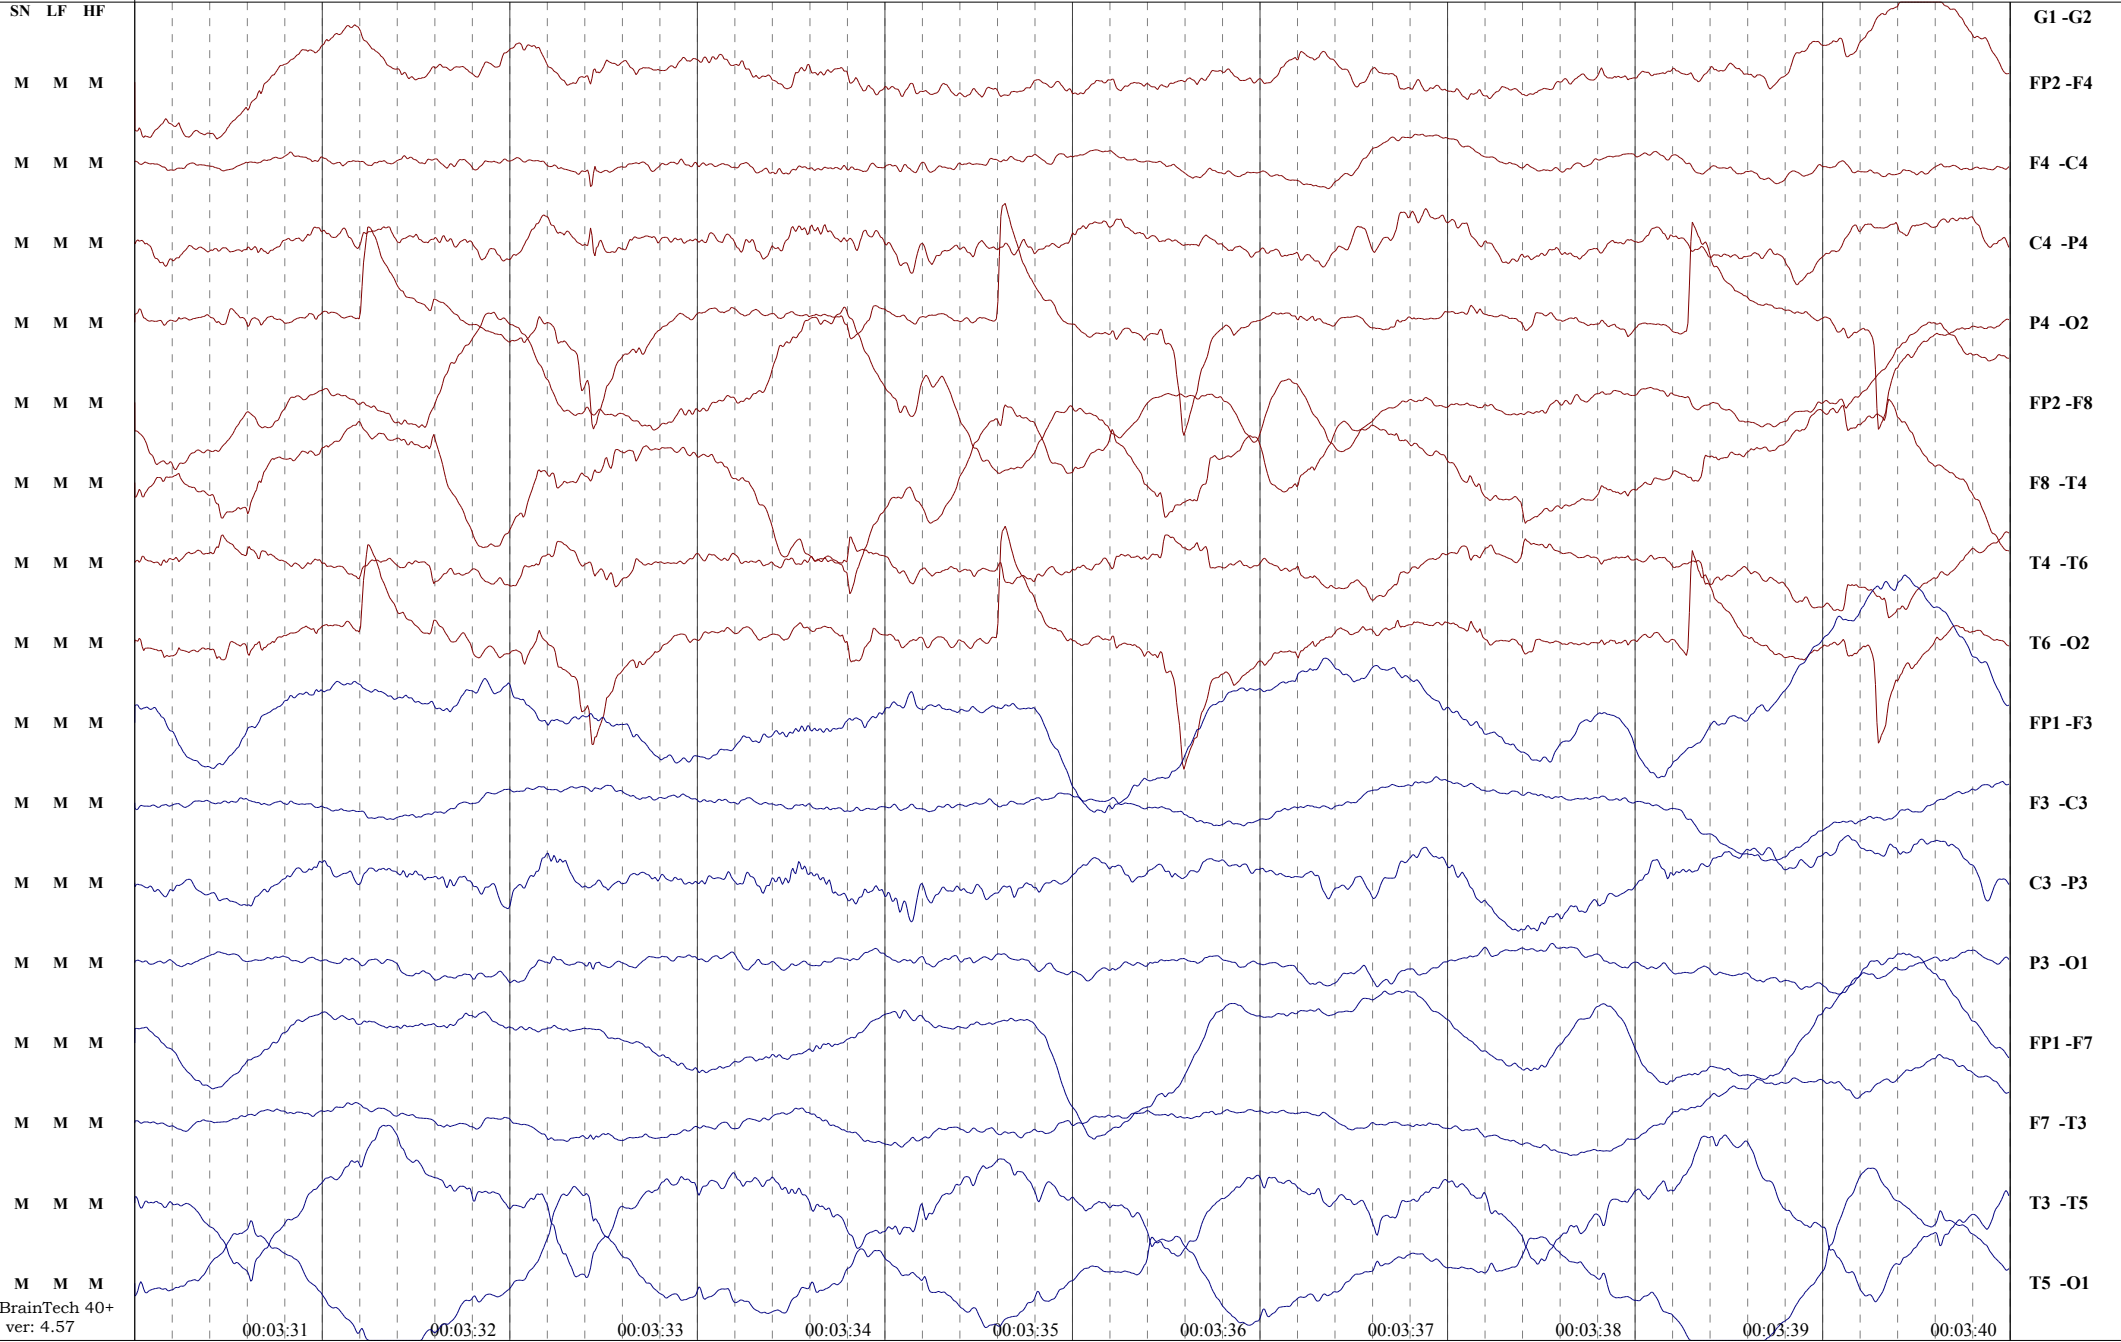



69  
MR. NIRANJAN SAHU  
42 Years/M

Date: 17-Aug-2023  
Type: ANALYSIS  
BIPOLAR LONGITUDNAL

Speed : 30 mm/S  
Sen : 7.5 uV/mm  
Filter : 1 Hz - 70 Hz

Time: 13:49:59  
Page:23/25  
Notch: ON

Ref:DR.RAJNISH PANDEY  
Dr. : DR. VIJENDRA PAINKARA  
Tech:

