

Contents

1. Description
 - 1.1 Principle of the MACS® Separation
 - 1.2 Reagent and instrument requirements
2. Protocol
 - 2.1 Overview
 - 2.2 Sample preparation
 - 2.3 Buffer preparation
 - 2.4 Magnetic labeling
 - 2.5 Magnetic separation
3. Example for elimination of dead cells from tissue using the Dead Cell Removal Kit
4. References

1. Description

This product is for research use only.

Components	10 mL Dead Cell Removal MicroBeads 25 mL 20× Binding Buffer Stock Solution
Capacity	For 10 ⁹ total cells, up to 100 separations.
Product format	Dead Cell Removal MicroBeads are supplied in buffer containing stabilizer.
Storage	Store protected from light at 2–8 °C. Do not freeze. The expiration date is indicated on the vial label.

1.1 Principle of the MACS® Separation

Dead Cell Removal MicroBeads recognize a moiety in the plasma membrane of apoptotic as well as dead cells. For the dead cell depletion, cells are magnetically labeled with Dead Cell Removal MicroBeads and passed through a separation column. The magnetically labeled dead cells are retained within the column. The unlabeled living cells run through; this cell fraction is thus depleted of dead cells. After removing the column from the magnetic field, the magnetically retained dead cells can be eluted as the positively selected cell fraction. Using the Dead Cell Removal Kit, even early apoptotic cells with an intact cellular membrane are removed. Activated cells, e.g. from a cell culture, may be labelled as well.

1.2 Reagent and instrument requirements

- Sterile, double-distilled water (ddH₂O).
▲ **Note:** Do not use deionized water for dilution!
- MACS® Columns and MACS Separators: Dead cells can be retained in the magnetic field by using MS, LS, XS, or D Columns.

Column	Max. number of labeled dead cells	Max. number of total cells	Separator
MS	10 ⁷	2×10 ⁸	MiniMACS, OctoMACS, SuperMACS II
LS	10 ⁸	2×10 ⁹	MidiMACS, QuadroMACS, SuperMACS II
XS	10 ⁹	2×10 ¹⁰	SuperMACS II
D	10 ⁹		SuperMACS II

▲ **Note:** Column adapters are required to insert certain columns into the SuperMACS™ II Separator. For details refer to the respective MACS Separator data sheet.

- (Optional) Pre-Separation Filters (30 µm) (# 130-041-407) to remove cell clumps.
- (Optional) gentleMACS™ Dissociator (# 130-093-235), gentleMACS Octo Dissociator (# 130-095-937), gentleMACS Dissociator with Heaters (# 130-096-427).
- (Optional) MACS Tissue Dissociation Kits, e.g. Tumor Dissociation Kit, mouse (130-096-730).

2. Protocol

2.1 Overview

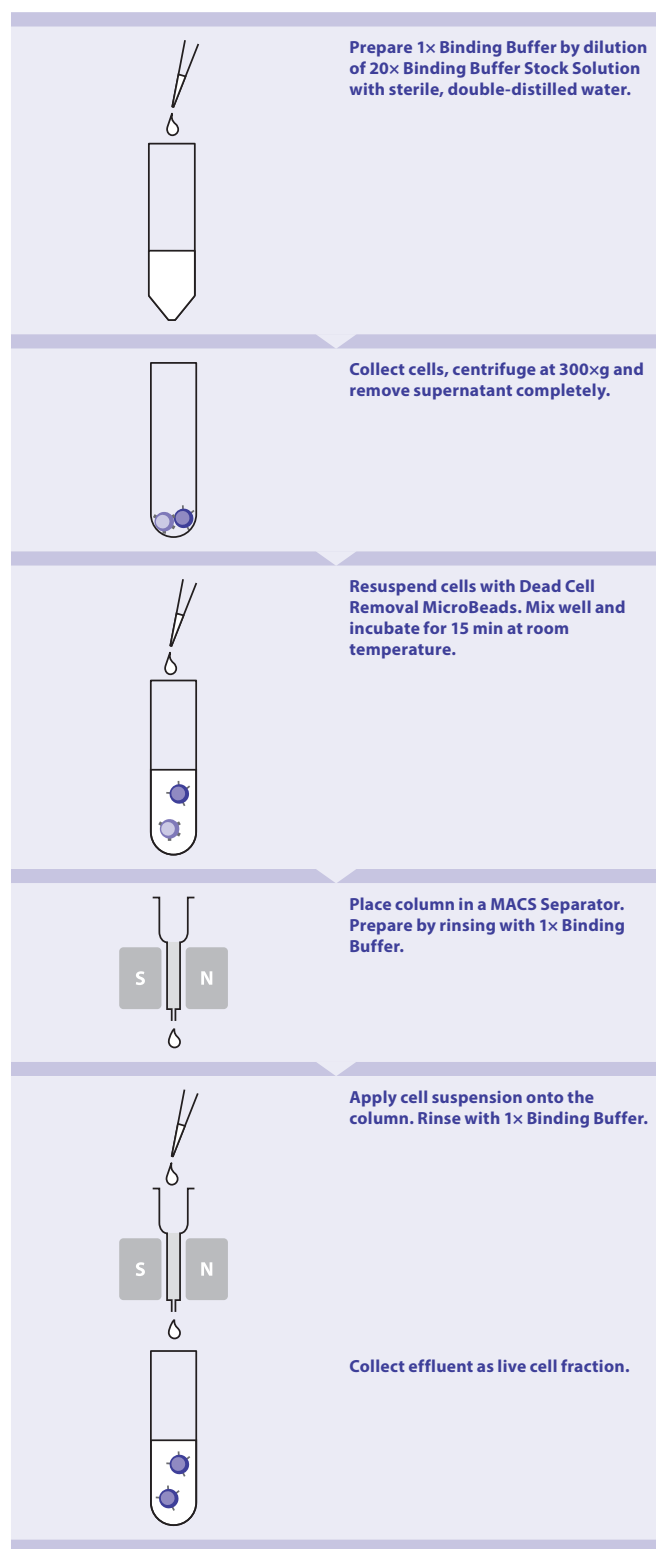


Figure 1: Elimination of dead cells using the Dead Cell Removal Kit.

2.2 Sample preparation

▲ Dead Cell Removal MicroBeads are susceptible to bacterial contamination. **Handle under sterile conditions.**

▲ When working with cell samples containing platelets, e.g., blood samples, wash samples carefully at low centrifugation speed (200×g) in order to remove platelets. Use buffer containing the ion chelator EDTA for these washing steps. Dead Cell Removal MicroBeads bind to activated platelets. Activated platelets also bind to leukocytes, e.g., monocytes. In this case, viable cells bound to activated platelets would be retained in the magnetic field and reduce the recovery of living cells.

When working with tissues, prepare a single-cell suspension using gentleMACS™ Dissociators and MACS® Tissue Dissociation Kits.

▲ Dead cells without any remnants of the plasma membranes (cell organelles without nuclei) cannot be removed using Dead Cell Removal MicroBeads due to lack of accessible antigen.

2.3 Buffer preparation

▲ Use 1× Binding Buffer prepared from 20× Binding Buffer Stock Solution supplied with the Dead Cell Removal Kit for all washing and selection steps. It is important to **use only sterile double-distilled water** for the dilution of the 20× Binding Buffer Stock Solution.

▲ **Note:** Do not use deionized water for dilution!

Prepare 1× Binding Buffer from 20× Binding Buffer Stock Solution. e.g: dilute 500 µL of 20× Binding Buffer Stock Solution with 9.5 mL of sterile, double-distilled water. Store at 2–8 °C. Alternatively, prepare 1× Binding Buffer Stock Solution by diluting 25 mL of 20× Binding Buffer with 475 mL of sterile, double-distilled water.

▲ **Note:** Handle under sterile conditions!

▲ **Note:** Binding of Dead Cell Removal MicroBeads requires Ca^{2+} . The presence of the ion chelator EDTA will abolish binding. 1× Binding Buffer is optimized for best Dead Cell Removal MicroBeads binding. The use of a different buffer may lead to poor dead cell removal efficiency.



2.4 Magnetic labeling

▲ Volumes for magnetic labeling given below are for up to 10^7 total cells. When working with fewer than 10^7 cells, use the same volumes as indicated. When working with higher cell numbers, scale up all reagent volumes and total volumes accordingly (e.g. for 2×10^7 total cells, use twice the volume of all indicated reagent volumes and total volumes).

▲ For optimal performance it is important to obtain a single-cell suspension before magnetic labeling. Pass cells through 30 µm nylon mesh (Pre-Separation Filters (30 µm), # 130-041-407) to remove cell clumps which may clog the column. Moisten filter with buffer before use.

▲ The recommended incubation temperature is 20–25 °C. Higher temperatures and/or longer incubation times may lead to non-specific cell labeling.

1. Determine cell number.
2. Centrifuge cell suspension at 300×g for 10 minutes. Aspirate supernatant completely.
3. Resuspend cell pellet in 100 µL of Dead Cell Removal MicroBeads per 10^7 total cells.

- Mix well and incubate for 15 minutes at room temperature (20–25 °C).
- (Optional) If necessary, add 1× Binding Buffer to the cell suspension to reach a minimum volume of 500 µL for separation.
- Proceed to magnetic separation (2.5).



2.5 Magnetic separation

- Choose an appropriate MACS Column and MACS Separator according to the number of total cells and the number of labeled cells. For details refer to the table in section 1.2..
- Always wait until the column reservoir is empty before proceeding to the next step.

Magnetic separation with MS or LS Columns

- Place column in the magnetic field of a suitable MACS Separator. For details refer to the respective MACS Column data sheet.
- Prepare column by rinsing with the appropriate amount of 1× Binding Buffer:
MS: 500 µL LS: 3 mL
- Apply cell suspension onto the column. Collect flow-through containing unlabeled cells (live cells).
- Wash column with the appropriate amount of 1× Binding Buffer. Collect unlabeled cells that pass through and combine with the flow-through from step 3.

MS: 4×500 µL LS: 4×3 mL

Note: Perform washing steps by adding buffer aliquots as soon as the column reservoir is empty.

- Remove column from the separator and place it on a suitable collection tube.
- Pipette the appropriate amount of buffer onto the column. Immediately flush out the magnetically labeled cells by firmly pushing the plunger into the column.
MS: 1 mL LS: 5 mL
- (Optional) To increase the efficiency of magnetic removal of dead cells, the live cell fraction can be enriched over a second MS or LS Column. Repeat the magnetic separation procedure as described in steps 1 to 6 by using a new column.
- Proceed to microscopic analysis of dead cells with membrane exclusion dyes, such as Trypan Blue or to flow cytometric analysis using Propidium Iodide Solution (# 130-093-233) or 7-AAD Staining Solution (# 130-111-568).¹

Magnetic separation with XS Columns

For instructions on the column assembly and the separation refer to the XS Column data sheet.

Depletion with D Columns

For instructions on column assembly and separation refer to the D Column data sheet.


Magnetic separation with the autoMACS® Pro Separator

- Refer to the respective user manual for instructions on how to use the autoMACS® Pro Separator.
- Buffers used for operating the autoMACS Pro Separator should have a temperature of ≥10 °C.
- The program “Depls_b” works only with **manual labeling** and only with the Chill 15 Rack. Perform manual labeling according to chapter 2.4 until step 4.
- Elution of the dead cells (labeled cells) is optional.
- The program “Depls_b” contains a 15-minute incubation timer before the separation. A countdown will be shown on the display when the run is started, and the separation will follow immediately after. This enables the incubation of the samples on the instrument, but it applies only once before starting the separation. To omit the incubation on the instrument, press **Skip**.

- Prepare and prime the instrument.
- Apply tube containing the sample in row A of the tube rack. Place tube to collect the unlabeled cell fraction (live cells) in row B and provide a tube containing 10 mL of 1× Binding Buffer in row C.
- For a standard separation choose the following program:
Depletion: Depls_b
Collect unlabeled cell fraction in row B of the tube rack. This fraction represents the live cells.
- Use the wash program **Clean**.
- (Optional) For elution of dead cells (labeled cells), press **Pos**. Cells will be eluted in tube containing 1× Binding Buffer in row C. At this step, remaining volume of 1× Binding Buffer in the tube will be 0.5mL. To discard dead cells, press **Waste**.

3. Example for elimination of dead cells from tissue using the Dead Cell Removal Kit

Dead cells were eliminated from peripheral blood mononuclear cells (PBMCs) subjected to heat-shock by using the Dead Cell Removal Kit, an LS Column, and a MidiMACS™ Separator. Dead cells were fluorescently stained with propidium iodide and analyzed using a MACSQuant® Analyzer 10.

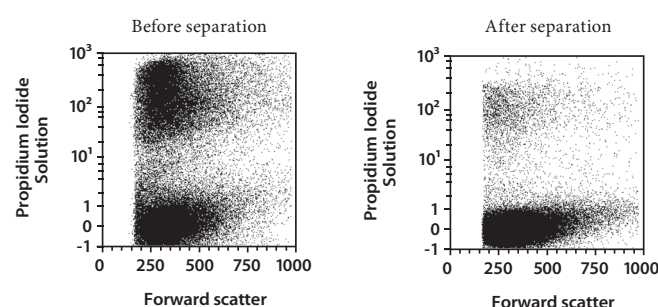

4. References

- Coder, DM (1997) Assessment of Cell Viability. In: Robinson, JP *et al.* (eds.) Current Protocols in Cytometry, p. 9.2.1-9.2.14, John Wiley & Sons Inc., New York

Refer to www.miltenyibiotec.com for all data sheets and protocols. Miltenyi Biotec provides technical support worldwide. Visit www.miltenyibiotec.com/local to find your nearest Miltenyi Biotec contact.

Legal notices

Limited product warranty

Miltenyi Biotec B.V. & Co. KG and/or its affiliate(s) warrant this product to be free from material defects in workmanship and materials and to conform substantially with Miltenyi Biotec's published specifications for the product at the time of order, under normal use and conditions in accordance with its applicable documentation, for a period beginning on the date of delivery of the product by Miltenyi Biotec or its authorized distributor and ending on the expiration date of the product's applicable shelf life stated on the product label, packaging or documentation (as applicable) or, in the absence thereof, ONE (1) YEAR from date of delivery ("Product Warranty"). Miltenyi Biotec's Product Warranty is provided subject to the warranty terms as set forth in Miltenyi Biotec's General Terms and Conditions for the Sale of Products and Services available on Miltenyi Biotec's website at www.miltenyibiotec.com, as in effect at the time of order ("Product Warranty"). Additional terms may apply. BY USE OF THIS PRODUCT, THE CUSTOMER AGREES TO BE BOUND BY THESE TERMS.

THE CUSTOMER IS SOLELY RESPONSIBLE FOR DETERMINING IF A PRODUCT IS SUITABLE FOR CUSTOMER'S PARTICULAR PURPOSE AND APPLICATION METHODS.

Technical information

The technical information, data, protocols, and other statements provided by Miltenyi Biotec in this document are based on information, tests, or experience which Miltenyi Biotec believes to be reliable, but the accuracy or completeness of such information is not guaranteed. Such technical information and data are intended for persons with knowledge and technical skills sufficient to assess and apply their own informed judgment to the information. Miltenyi Biotec shall not be liable for any technical or editorial errors or omissions contained herein.

All information and specifications are subject to change without prior notice. Please contact Miltenyi Biotec Technical Support or visit www.miltenyibiotec.com for the most up-to-date information on Miltenyi Biotec products.

Licenses

This product and/or its use may be covered by one or more pending or issued patents and/or may have certain limitations. Certain uses may be excluded by separate terms and conditions. Please contact your local Miltenyi Biotec representative or visit Miltenyi Biotec's website at www.miltenyibiotec.com for more information.

The purchase of this product conveys to the customer the non-transferable right to use the purchased amount of the product in research conducted by the customer (whether the customer is an academic or for-profit entity). This product may not be further sold. Additional terms and conditions (including the terms of a Limited Use Label License) may apply.

CUSTOMER'S USE OF THIS PRODUCT MAY REQUIRE ADDITIONAL LICENSES DEPENDING ON THE SPECIFIC APPLICATION. THE CUSTOMER IS SOLELY RESPONSIBLE FOR DETERMINING FOR ITSELF WHETHER IT HAS ALL APPROPRIATE LICENSES IN PLACE. Miltenyi Biotec provides no warranty that customer's use of this product does not and will not infringe intellectual property rights owned by a third party. BY USE OF THIS PRODUCT, THE CUSTOMER AGREES TO BE BOUND BY THESE TERMS.

Trademarks

autoMACS, gentleMACS, MACS, MACSQuant, MidiMACS, the Miltenyi Biotec logo, MiniMACS, OctoMACS, QuadroMACS, and SuperMACS are registered trademarks or trademarks of Miltenyi Biotec and/or its affiliates in various countries worldwide.

Copyright © 2020 Miltenyi Biotec and/or its affiliates. All rights reserved.