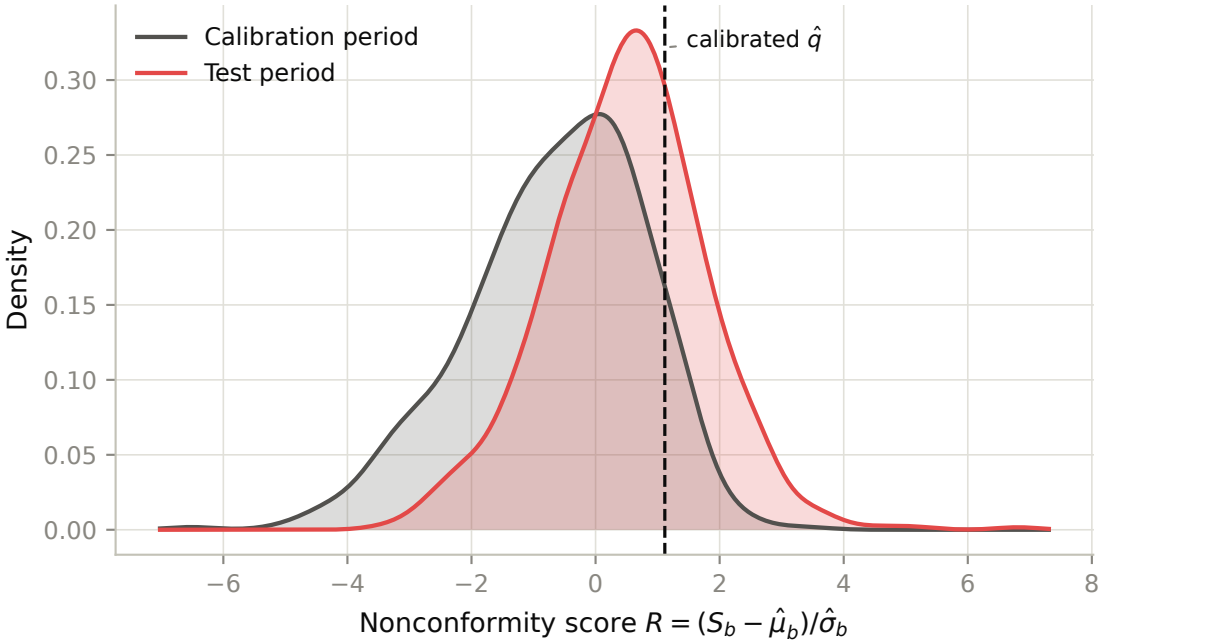
Predicted coverage 71.7% vs. observed 70.9% (from calibration-period statistics alone)
Calibration period
Test period
calibrated $\hat{q}$
Density
0.30
0.25
0.20
0.15
0.10
0.05
0.00
−6
−4
−2
0
2
4
6
8
Nonconformity score $R = (S_b - \hat{\mu}_b)/\hat{\sigma}_b$