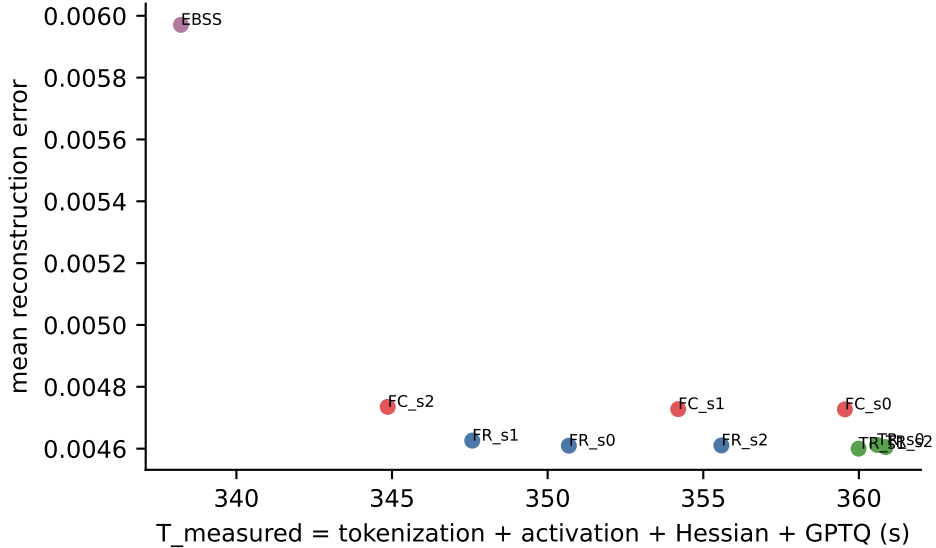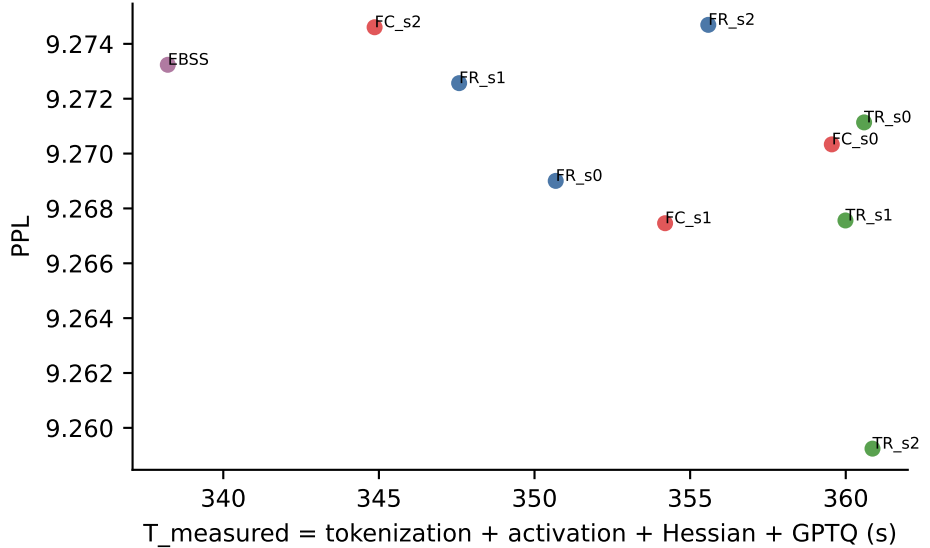Fig 6. Quality vs measured calibration cost (EBSS generation cost UNKNOWN and excluded)