
T2D Digital Twin: architecture

Team AMRIT_VIT · Digital Twin Challenge 2026 · synthetic patients only · decision support only

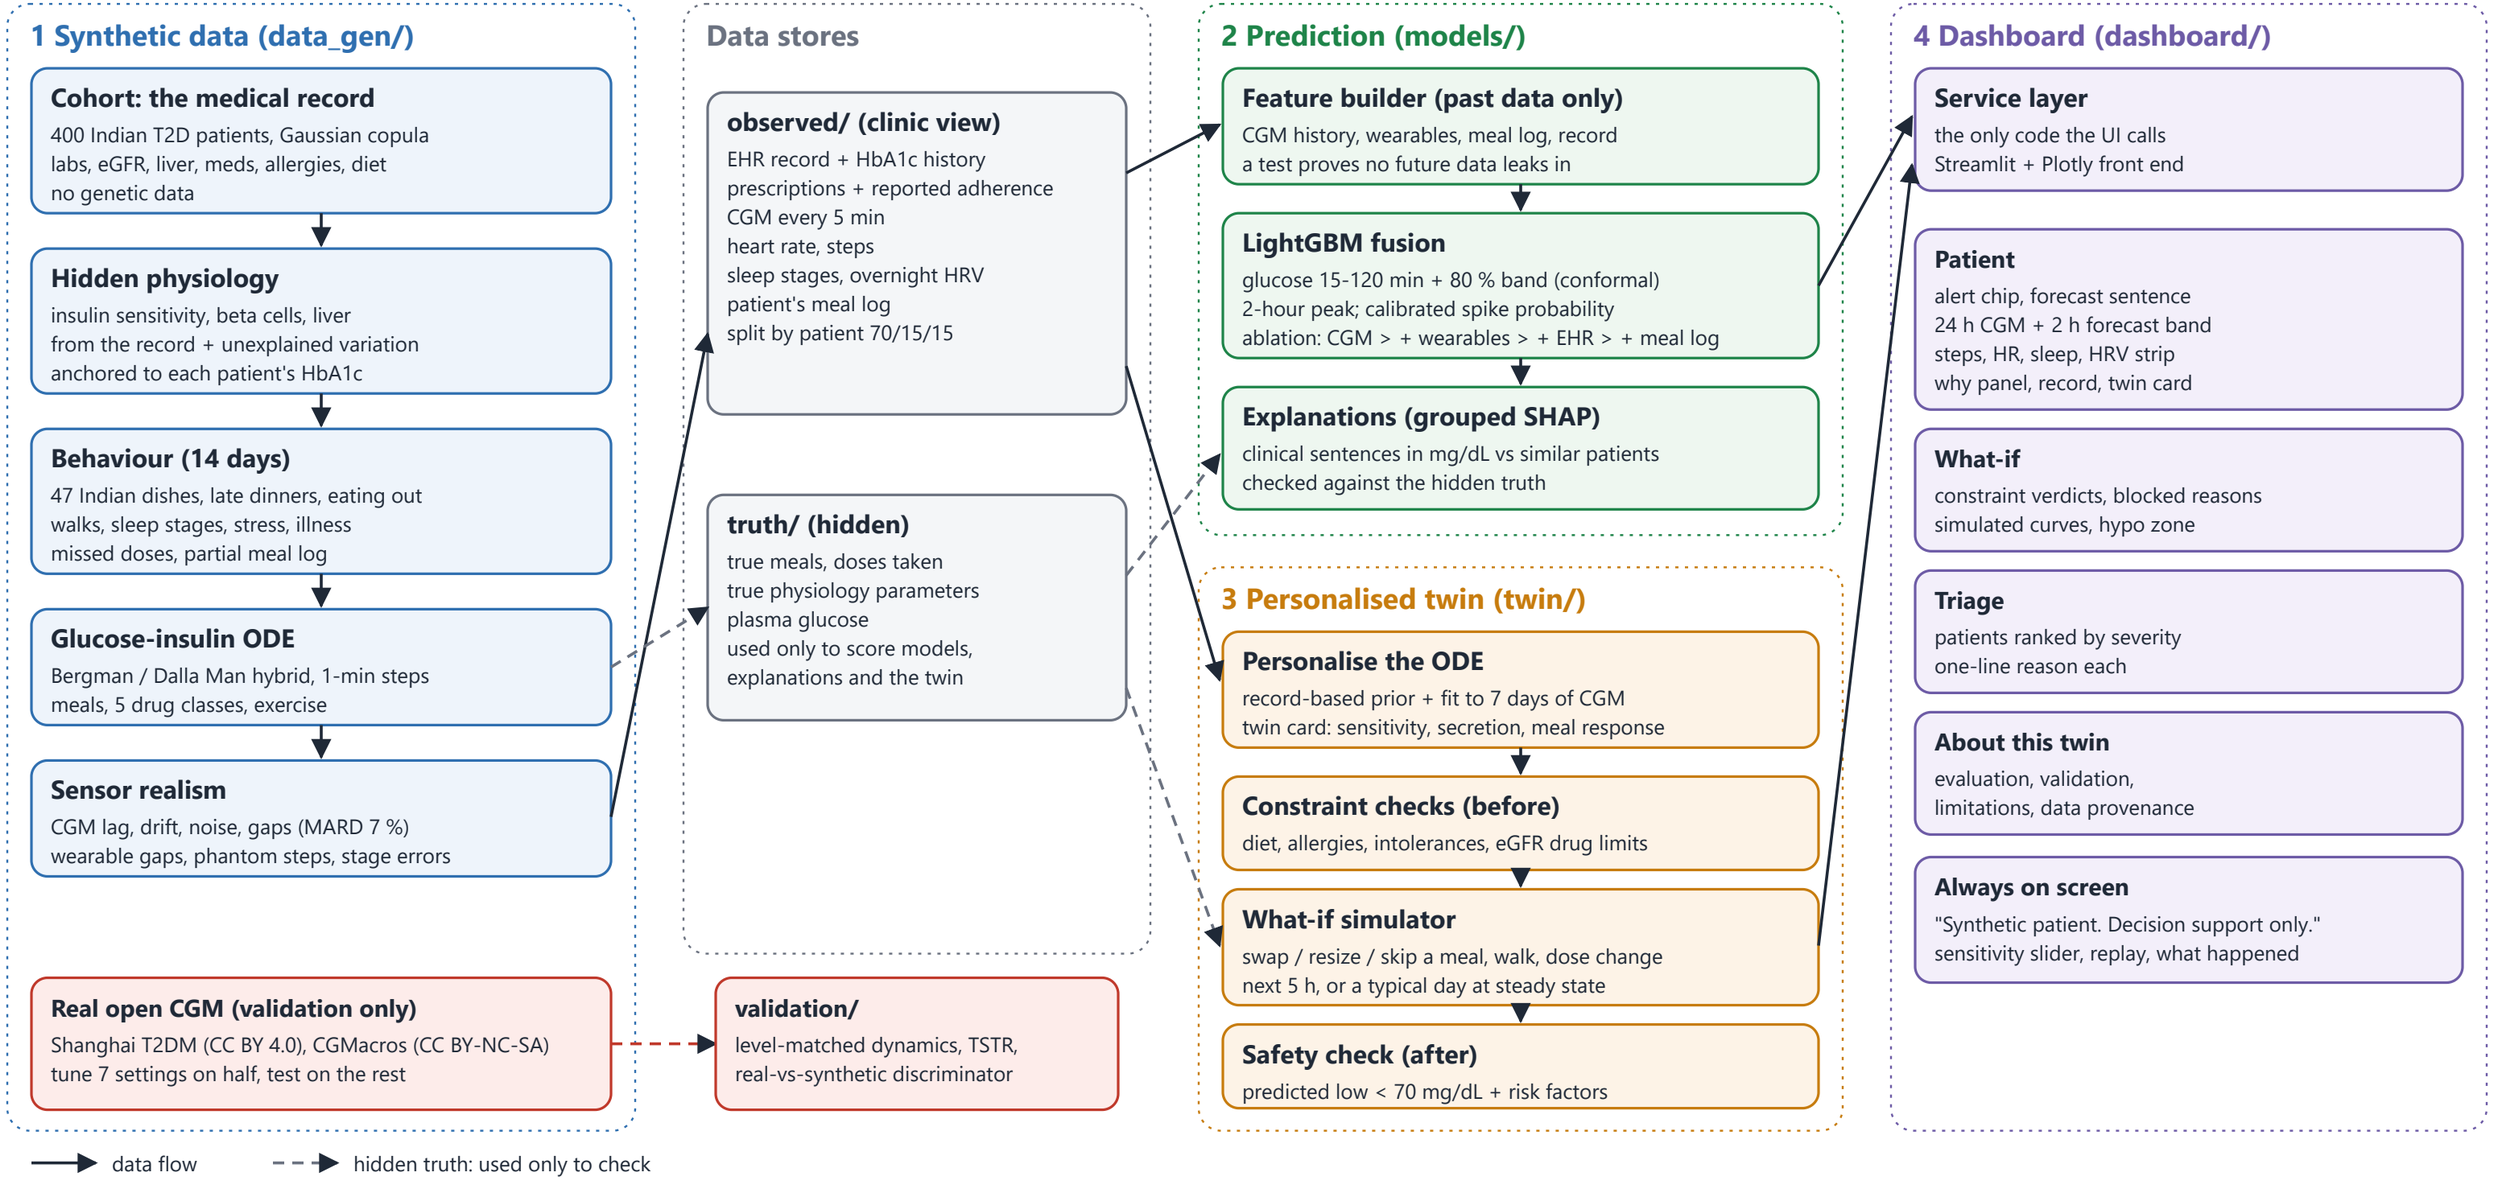

Held-out results: 92 % of spikes caught, median 80 min ahead, 0.69 false alerts/patient-day (threshold 0.5) · what-if dish swap error 13 mg/dL vs 31 for the cohort average

train-on-synthetic, test-on-real 60-min error 18.7 vs 19.9 mg/dL (no-change baseline)