


Per-block territory readouts fitted on the simulator, transported to real ECG

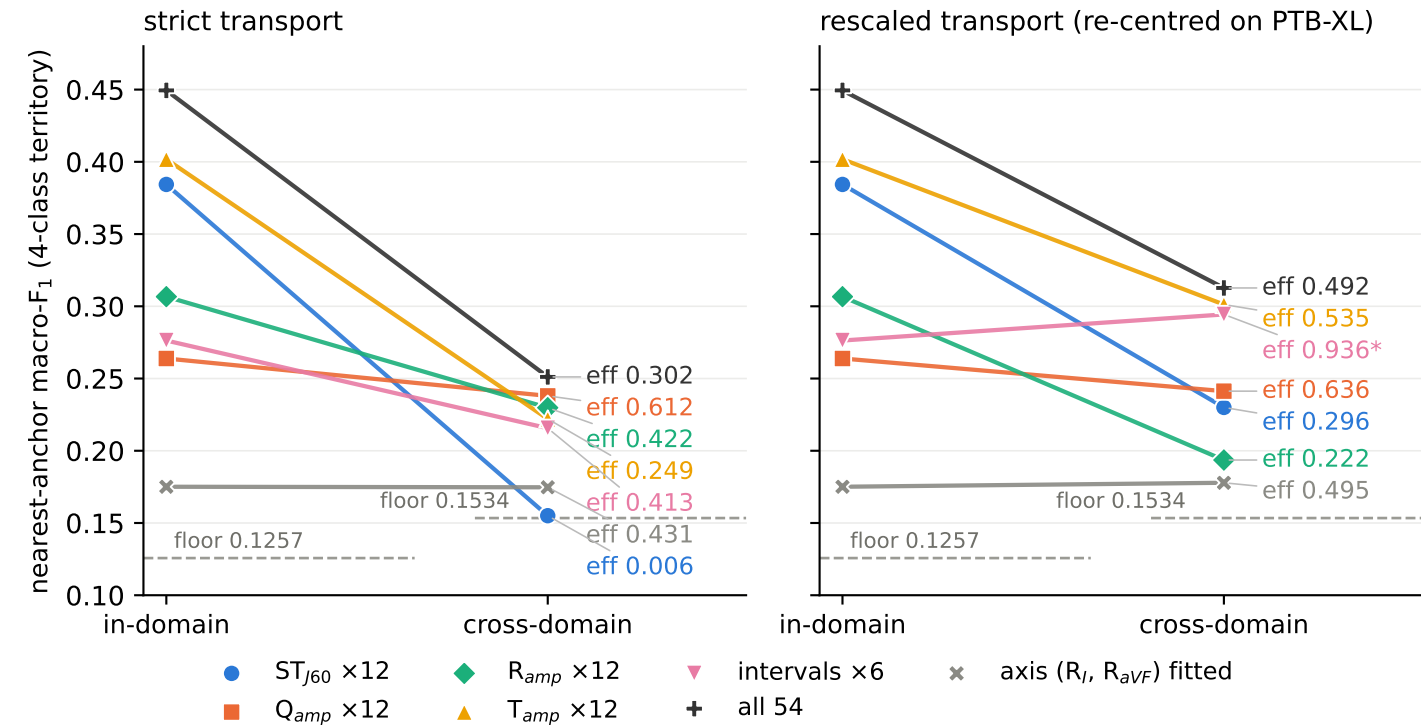

efficiency = $(F1_{cross} - floor_{cross}) / (F1_{in} - floor_{in})$. *intervals block: ~33% imputation cross-domain; efficiency not interpreted.