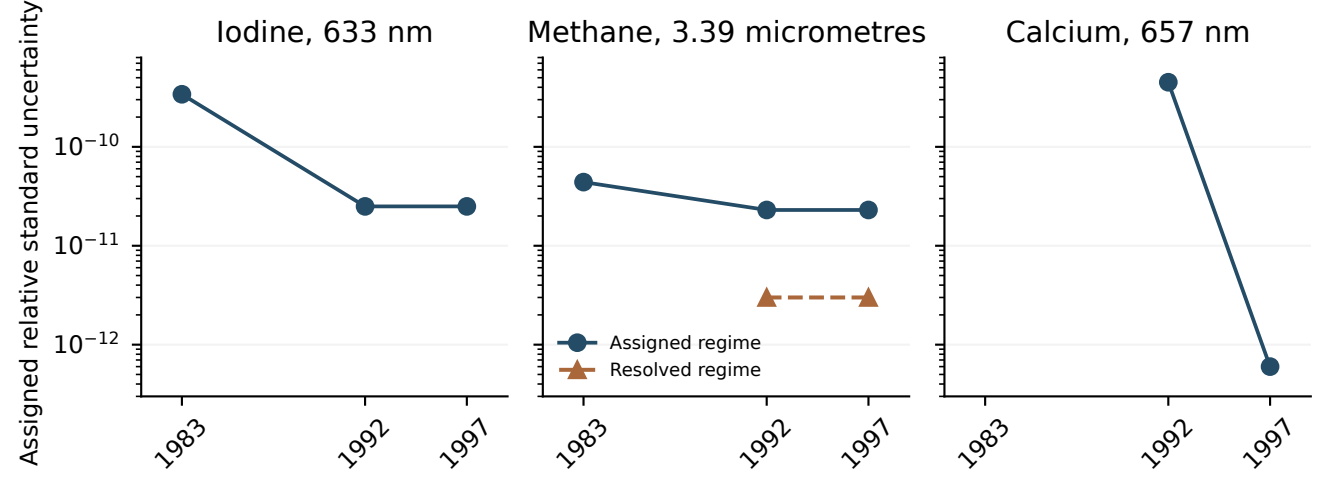
Iodine, 633 nm
Methane, 3.39 micrometres
Calcium, 657 nm
Assigned relative standard uncertainty
10^{-10}
10^{-11}
10^{-12}
1983
1992
1997
Assigned regime
Resolved regime