


Spectrum Peak Pick

Print Date : 23-02-2026 12:41:21

File Name: Metformin HCl 10ppm - RawData

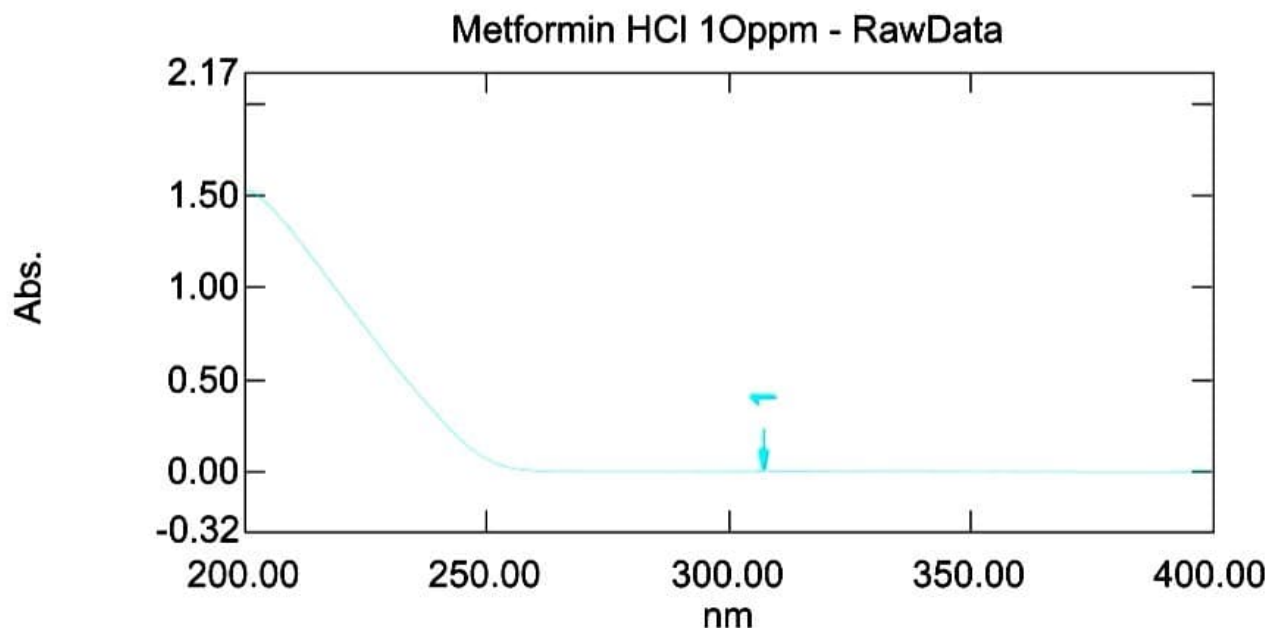

[Summary]

Data Information

Data is: Measurement Data
Data Set Name: RawData
Sample Name: Metformin HCl 10ppm
Sample ID: Metformin HCl 10ppm
Option:
Analyst:
Date/Time: 23-02-2026 12:40:23
Comments:
Parameter File Name: C:\UVVis-Data\RD sir UG 2025-26
Metformin HCl 10ppm.vspm

Software Information

Software Name: LabSolutions UV-Vis
Version: 1.14

Instrument Information

Instrument Name: UV1900I
Instrument Type: UV-1900 Series
Model (S/N): UV1900i (A12536183445)

Report File Name:

[Peak Pick Table]

Threshold: 0.001000


Number of Points: 4

No.	P/V	Wavelength nm.	Abs.	Description
1	1	307.5	0.005	

Spectrum Peak Pick

Print Date : 23-02-2026 12:37:05

File Name: Glimeperide HCl 10ppm - RawData

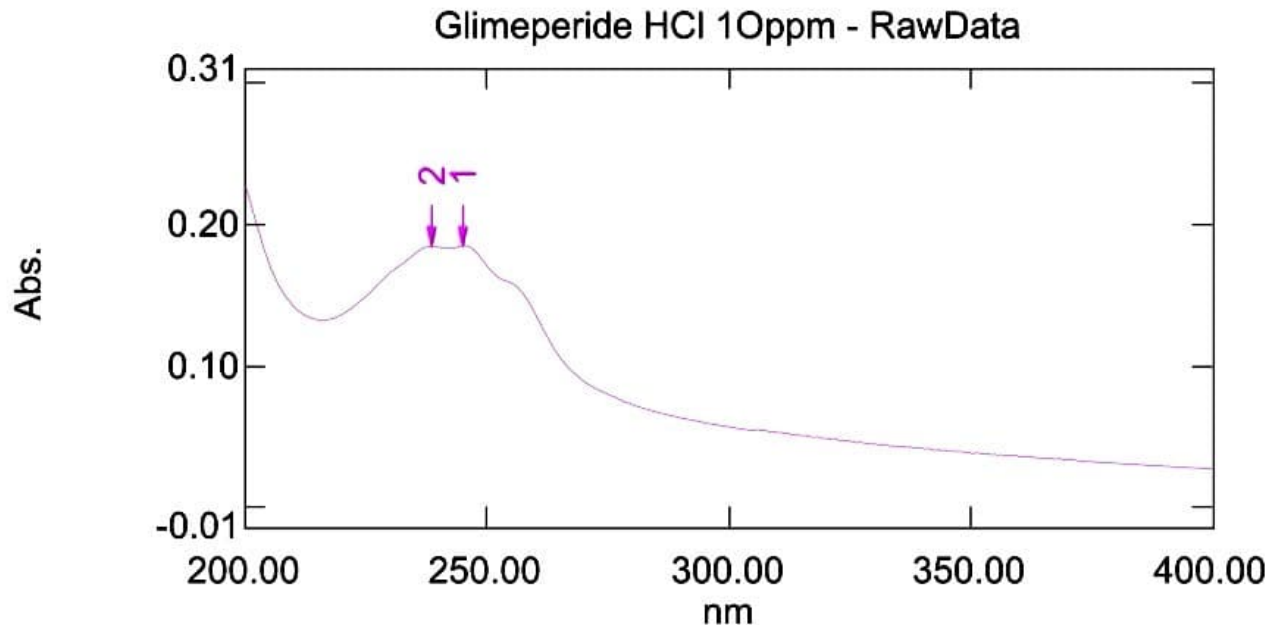

[Summary]

Data Information

Data is: Measurement Data
Data Set Name: RawData
Sample Name: Glimeperide HCl 10ppm
Sample ID: Glimeperide HCl 10ppm
Option:
Analyst:
Date/Time: 23-02-2026 12:36:15
Comments:
Parameter File Name: C:\UVVis-Data\RD sir UG 2025-26
 \Glimeperide HCL 10ppm.vspm
Report File Name:

Software Information

Software Name: LabSolutions UV-Vis
Version: 1.14

Instrument Information

Instrument Name: UV1900I
Instrument Type: UV-1900 Series
Model (S/N): UV1900i (A12536183445)

[Peak Pick Table]

Threshold: 0.001000


Number of Points: 4

No.	P/V	Wavelength nm.	Abs.	Description
1		245.0	0.185	
2		238.5	0.184	

Spectrum Active Graph

Print Date : 23-02-2026 12:25:04

File Name: Metformin NaOH 10ppm - RawData

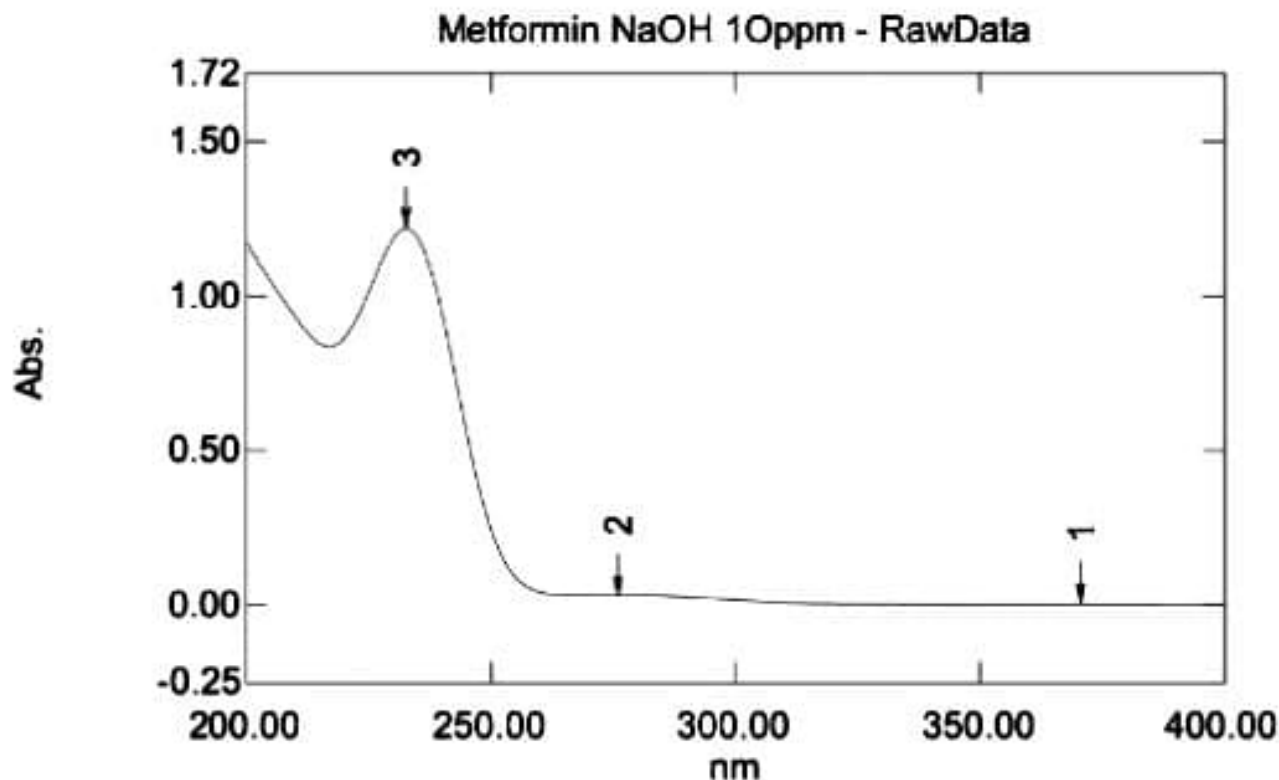

[Summary]

Data Information

Data is: Measurement Data
Data Set Name: RawData
Sample Name: Metformin NaOH 10ppm
Sample ID: Metformin NaOH 10ppm
Option:
Analyst:
Date/Time: 23-02-2026 12:23:44
Comments:
Parameter File Name: C:\UVVis-Data\RD sir UG 2025-26
Metformin NaOH 10ppm.vsp
Report File Name:

Software Information

Software Name: LabSolutions UV-Vis
Version: 1.14

Instrument Information

Instrument Name: UV1900i
Instrument Type: UV-1900 Series
Model (S/N): UV1900i (A12536183445)

[Measurement Parameters]

[Measurement]

Start: 400 nm
End: 200 nm
Data Interval: 0.5 nm
Scan Speed: Medium speed
Spectrum Type: Absorbance

[Accessories]

Accessories: None

[Advanced]

Slit Width: 1.0 nm
Light Source Switch Wavelength: 340.00 nm
S/R Switch: Standard

[Repeat]

Repeat Measurement: OFF


[Post-processing]

Spectrum Transformation: OFF
Data Processing Table: OFF
Print: OFF

Spectrum Peak Pick

Print Date : 23-02-2026 12:29:33

File Name: Glimeperide NaOH 10ppm - RawData

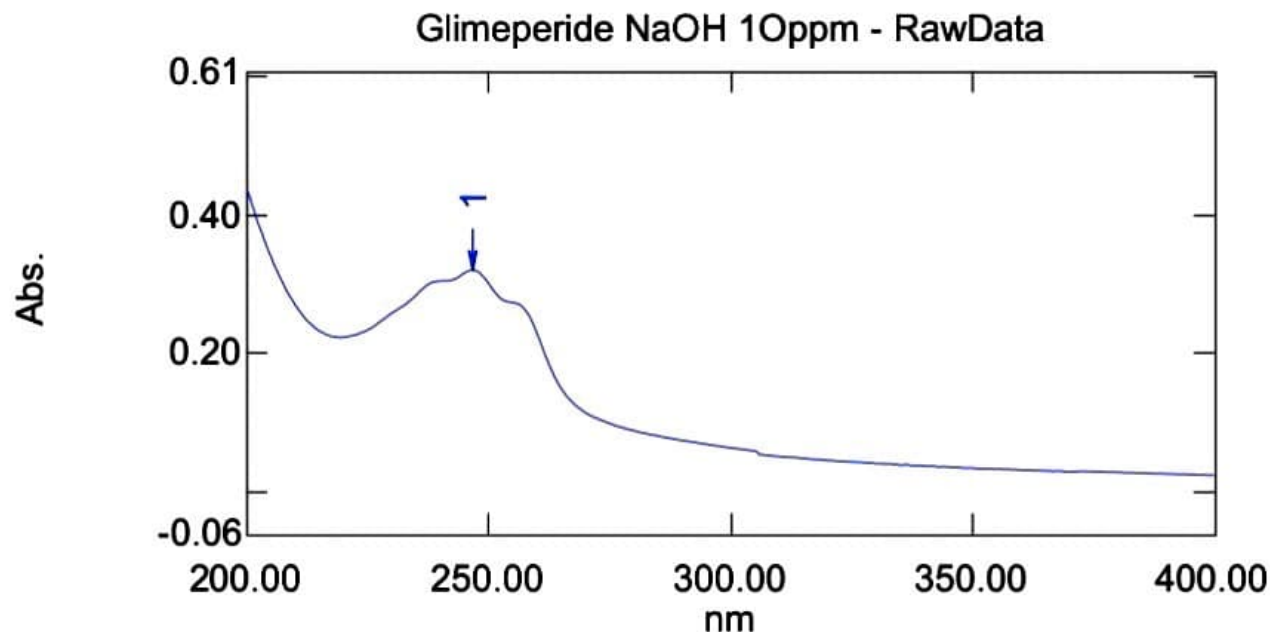

[Summary]

Data Information

Data is: Measurement Data
Data Set Name: RawData
Sample Name: Glimeperide NaOH 10ppm
Sample ID: Glimeperide NaOH 10ppm
Option:
Analyst:
Date/Time: 23-02-2026 12:28:16
Comments:
Parameter File Name: C:\UVVis-Data\RD sir UG 2025-26
\Glimeperide NaOH 10ppm.vspm
Report File Name:

Software Information

Software Name: LabSolutions UV-Vis
Version: 1.14

Instrument Information

Instrument Name: UV1900i
Instrument Type: UV-1900 Series
Model (S/N): UV1900i (A12536183445)

[Peak Pick Table]

Threshold: 0.001000


Number of Points: 4

No.	P/V	Wavelength nm.	Abs.	Description
1	1	246.5	0.320	

Spectrum Peak Pick

Print Date : 28-01-2026 15:54:01

File Name: Gilmepride C 10ppm - RawData

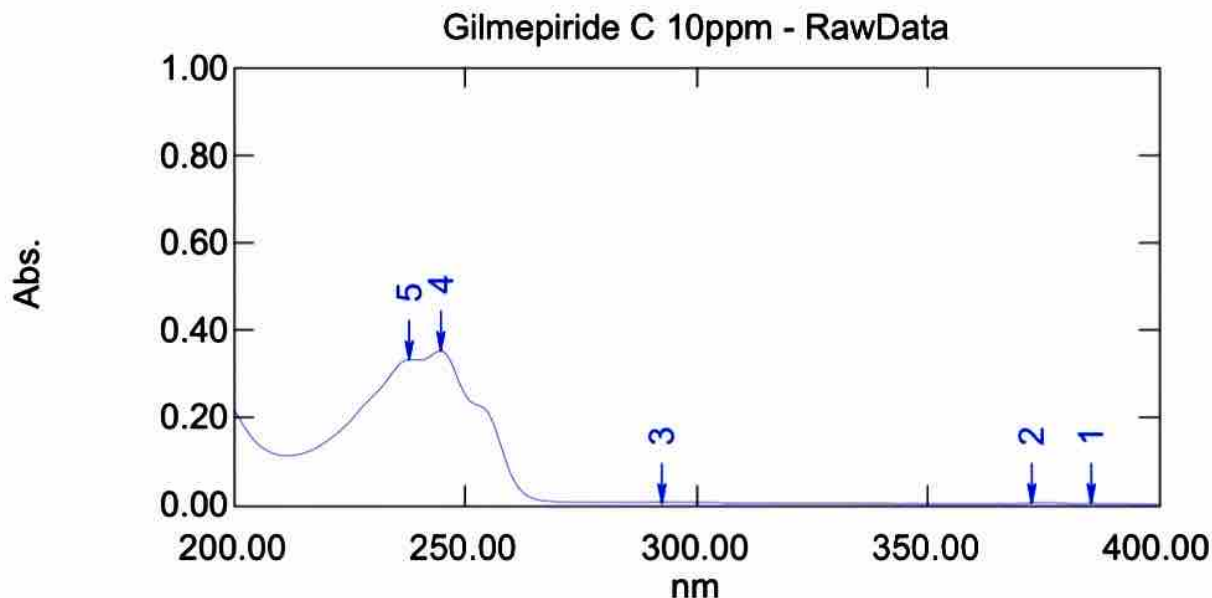

[Summary]

Data Information

Data is: Measurement Data
Data Set Name: RawData
Sample Name: Gilmepride C 10ppm
Sample ID: Gilmepride C 10ppm
Option:
Analyst:
Date/Time: 28-01-2026 15:53:04
Comments:
Parameter File Name: C:\UVVis-Data\RD sir UG 2025-26
 \Metformin C 100ppm.vspm

Software Information

Software Name: LabSolutions UV-Vis
Version: 1.14

Instrument Information

Instrument Name: UV1900i
Instrument Type: UV-1900 Series
Model (S/N): UV1900i (A12536183445)

Report File Name:

[Peak Pick Table]

Threshold: 0.001000


Number of Points: 4

No.	P/V	Wavelength nm.	Abs.	Description
1	⬆	385.5	0.003	
2	⬆	372.5	0.005	
3	⬆	292.5	0.006	
4	⬆	244.5	0.353	
5	⬆	238.0	0.333	

Spectrum Peak Pick

Print Date : 20-02-2026 16:46:04

File Name: metformin 10ppm - RawData

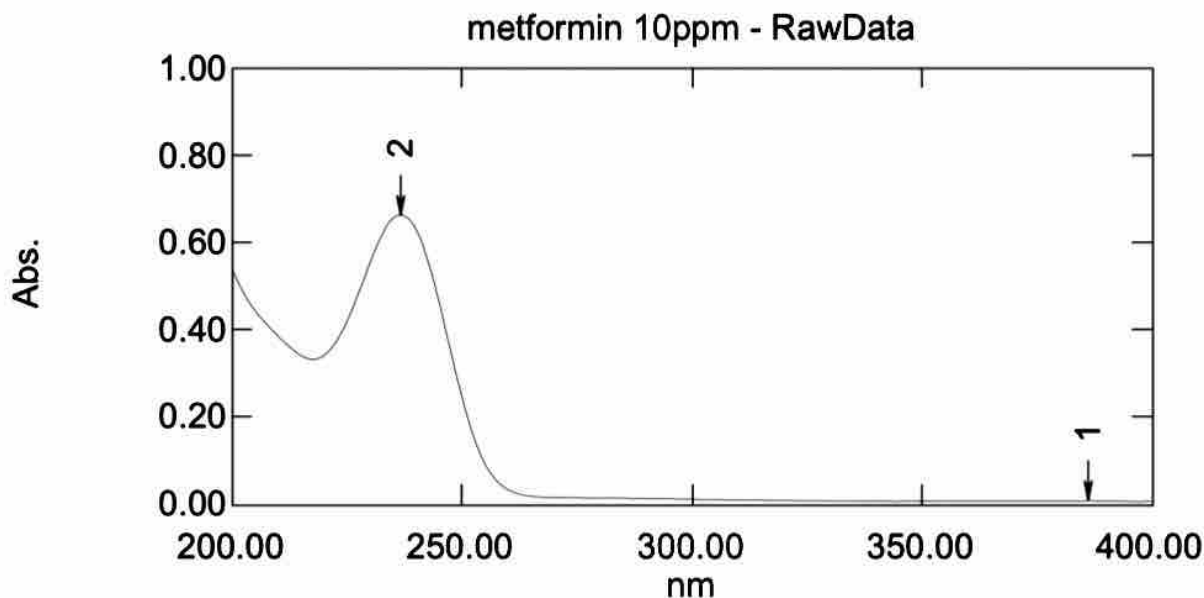

[Summary]

Data Information

Data is: Measurement Data
Data Set Name: RawData
Sample Name: metformin 10ppm
Sample ID: metformin 10ppm
Option:
Analyst:
Date/Time: 20-02-2026 16:45:23
Comments:
Parameter File Name: C:\UVVis-Data\RD sir UG 2025-26
metformin 10ppm.vspm

Software Information

Software Name: LabSolutions UV-Vis
Version: 1.14

Instrument Information

Instrument Name: UV1900i
Instrument Type: UV-1900 Series
Model (S/N): UV1900i (A12536183445)

Report File Name:

[Peak Pick Table]

Threshold: 0.001000

Number of Points: 4

No.	P/V	Wavelength nm.	Abs.	Description
1	🟢	386.5	0.008	
2	🟢	236.5	0.663	