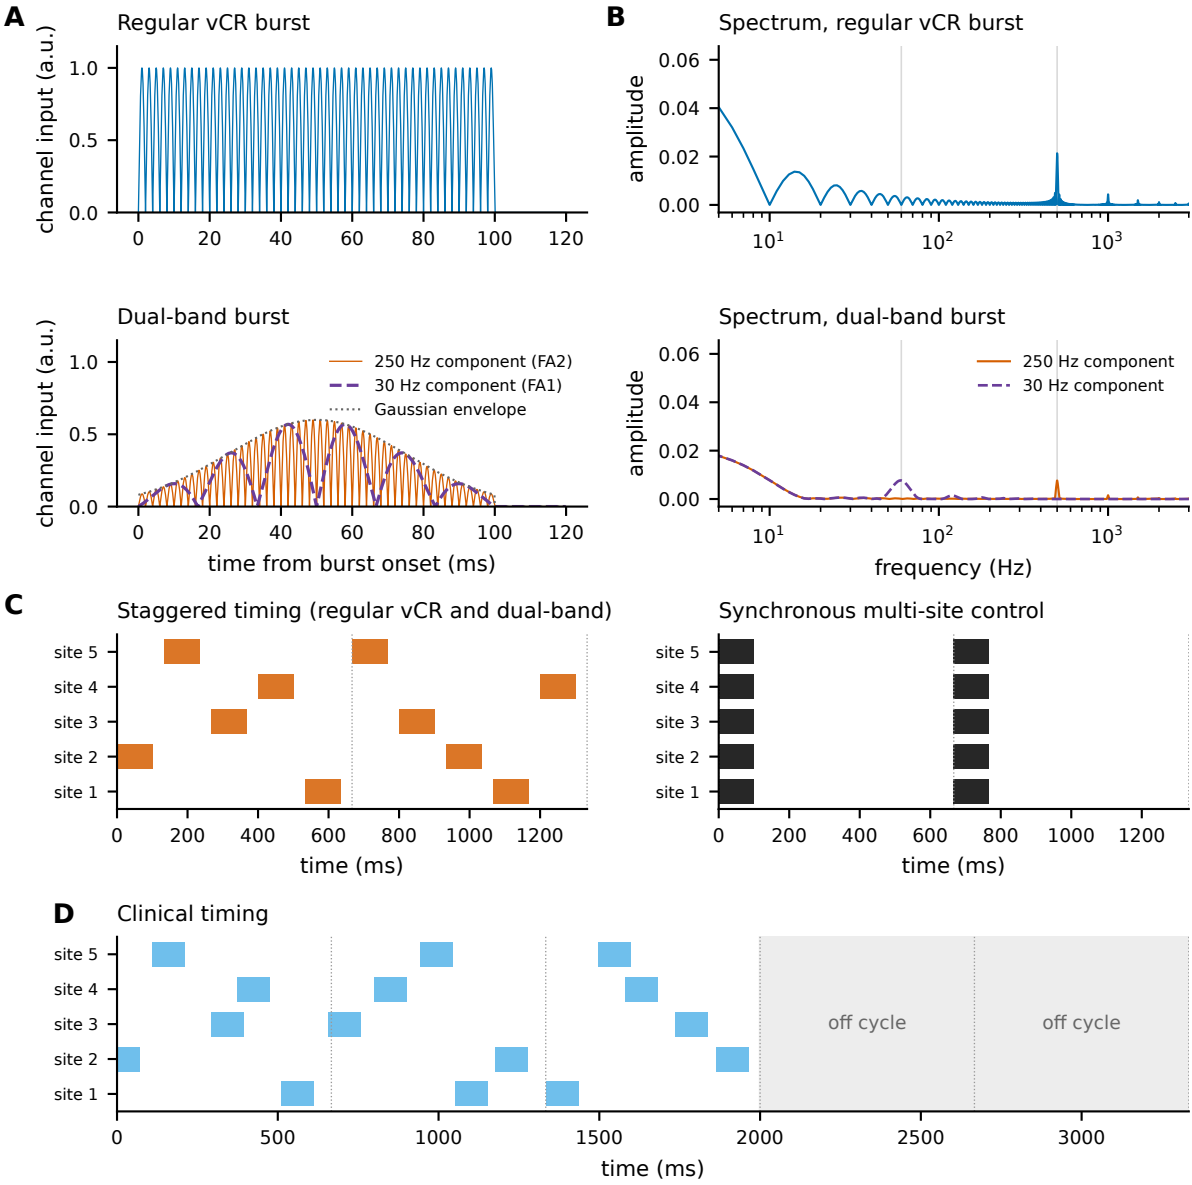

A
Regular vCR burst
channel input (a.u.)
1.0
0.5
0.0
0
20
40
60
80
100
120
B
Spectrum, regular vCR burst
amplitude
0.06
0.04
0.02
0.00
10^1
10^2
10^3
Dual-band burst
channel input (a.u.)
250 Hz component (FA2)
30 Hz component (FA1)
Gaussian envelope
time from burst onset (ms)
Spectrum, dual-band burst
amplitude
250 Hz component
30 Hz component
frequency (Hz)
C
Staggered timing (regular vCR and dual-band)
site 5
site 4
site 3
site 2
site 1
0
200
400
600
800
1000
1200
time (ms)
Synchronous multi-site control
time (ms)
D
Clinical timing
off cycle
off cycle
0
500
1000
1500
2000
2500
3000
time (ms)