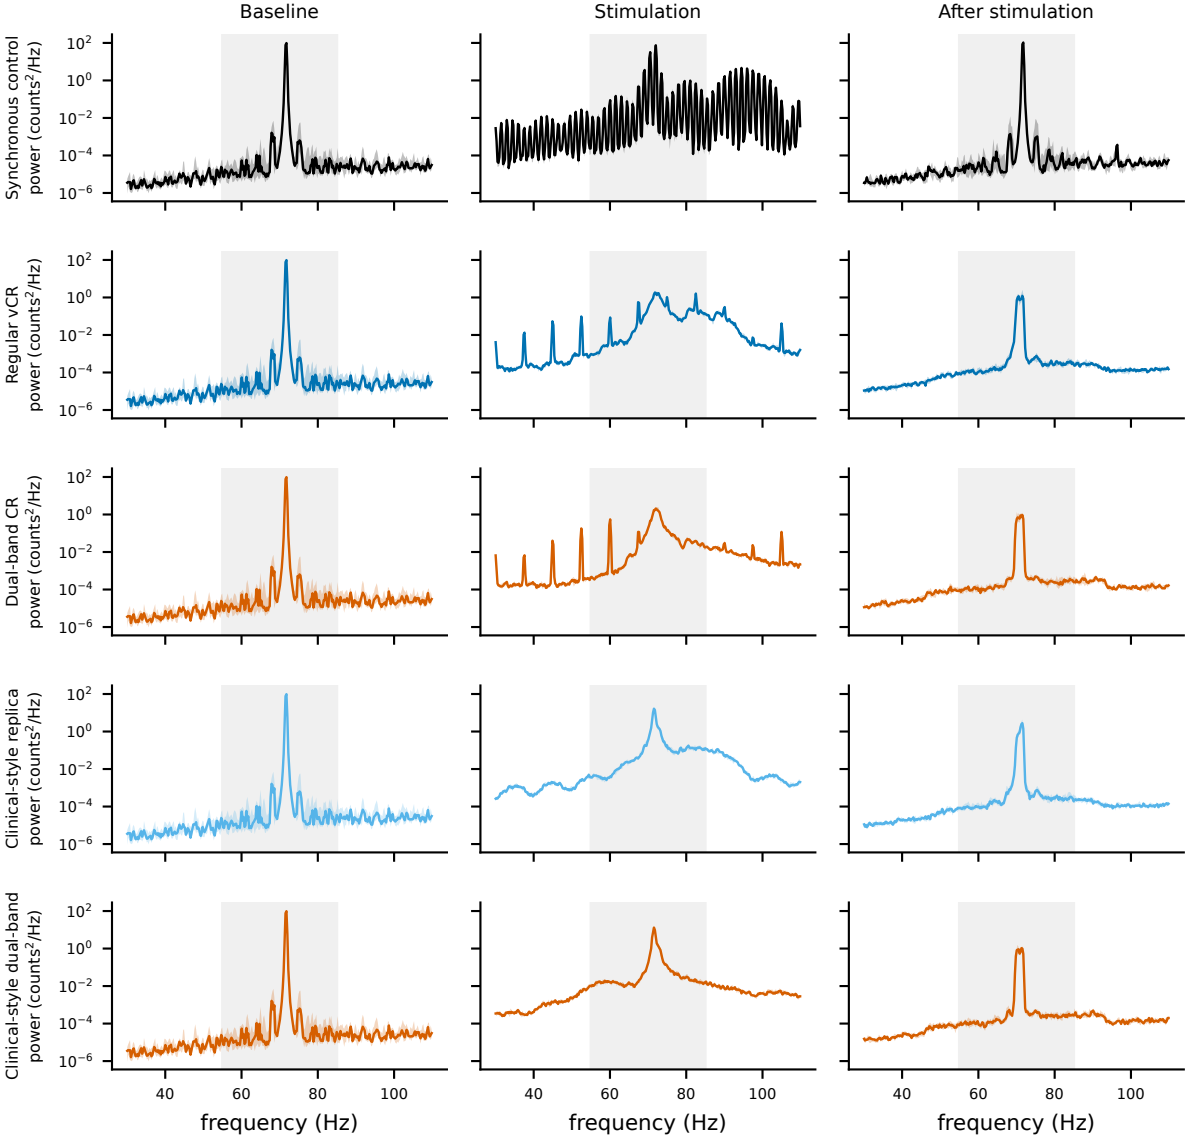

Baseline
Stimulation
After stimulation
Synchronous control
Regular vCR
Dual-band CR
Clinical-style replica
Clinical-style dual-band
power (counts²/Hz)
10^{2}
10^{0}
10^{-2}
10^{-4}
10^{-6}
40
60
80
100
frequency (Hz)