
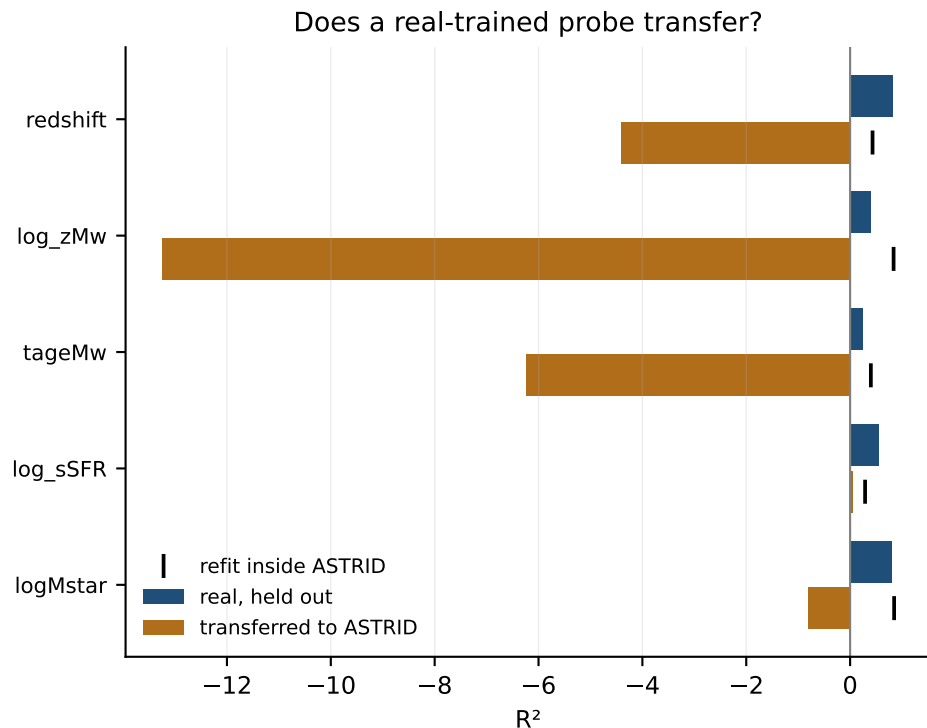


Real versus simulated: what survives the controls

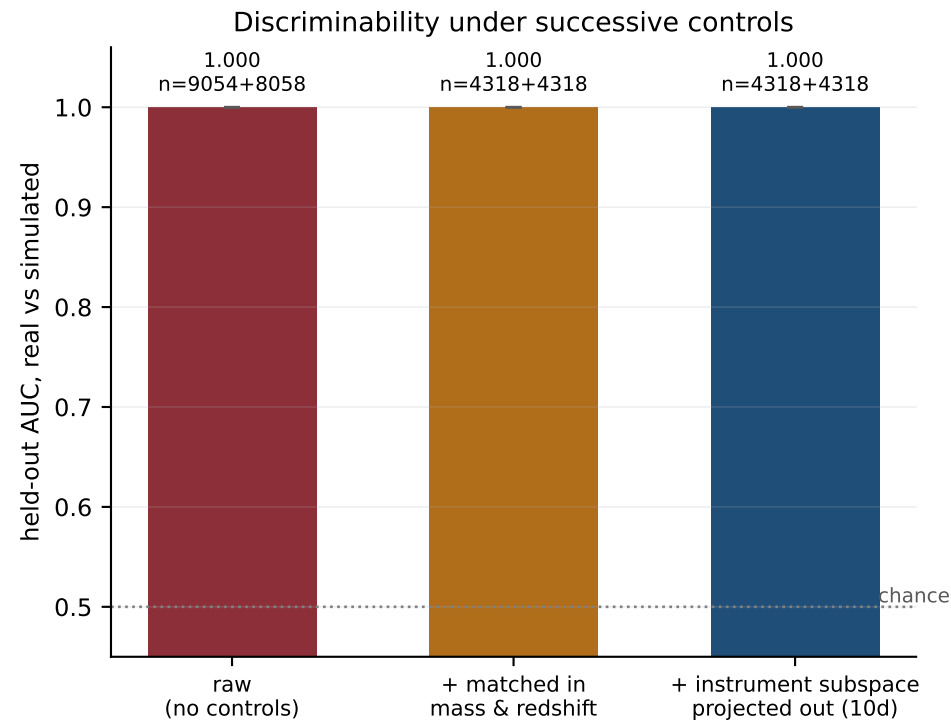

Limitation: Simulated images were not degraded to match the real PSF and noise; the confound is controlled by distribution matching plus projection of the linearly-captured instrument subspace only. Residual separation may still contain instrument signature that is nonlinearly encoded.