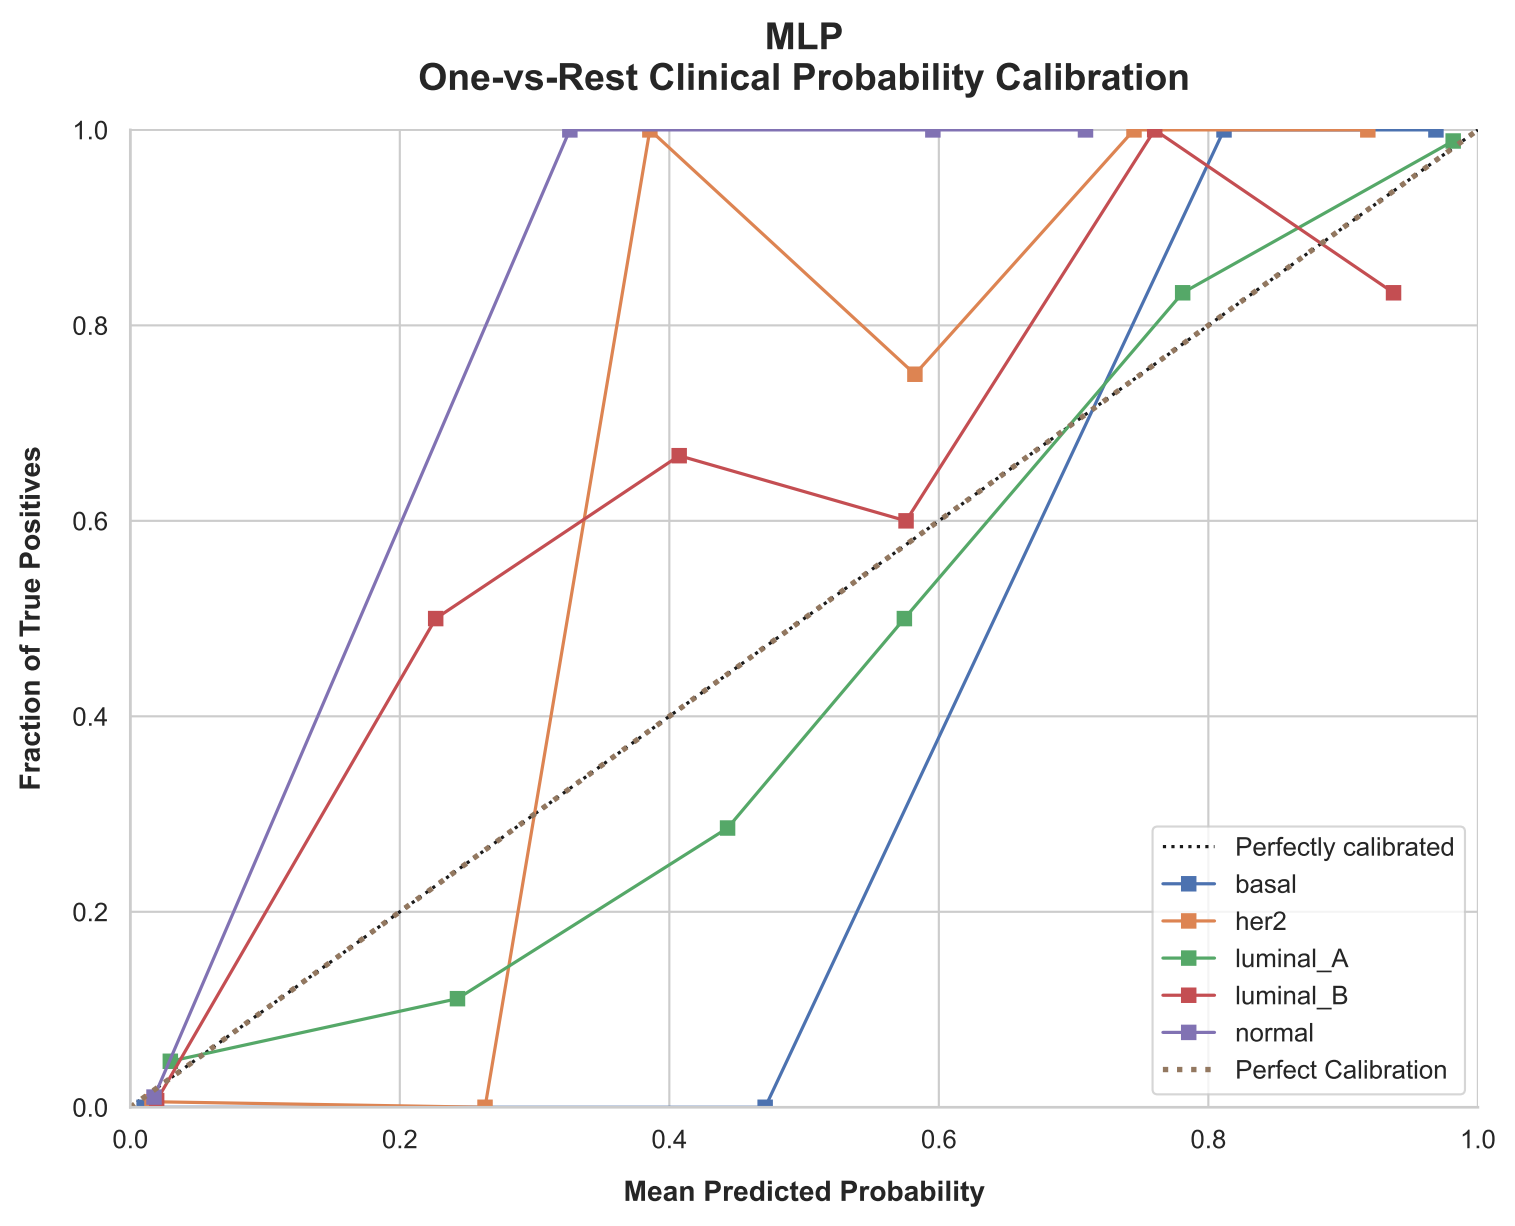
MLP
One-vs-Rest Clinical Probability Calibration
Fraction of True Positives
Mean Predicted Probability
0.0
0.2
0.4
0.6
0.8
1.0
Perfectly calibrated
basal
her2
luminal_A
luminal_B
normal
Perfect Calibration