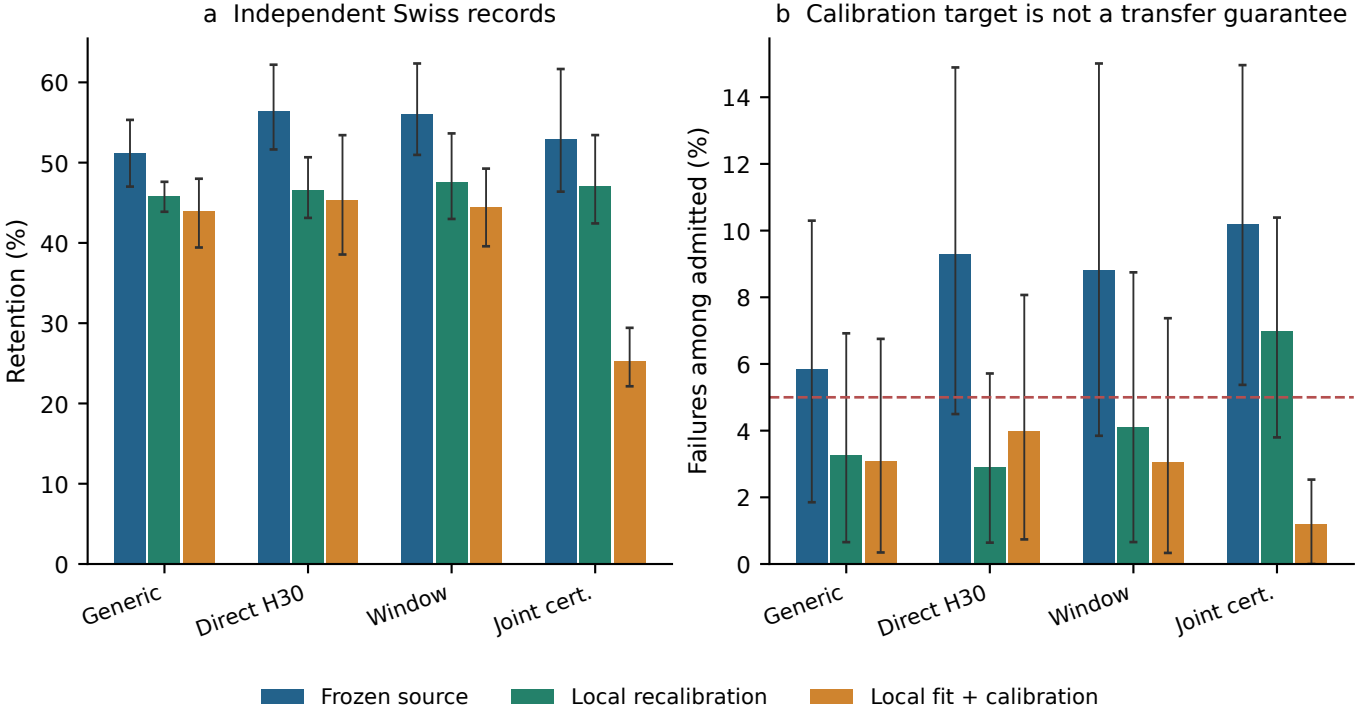
a Independent Swiss records
b Calibration target is not a transfer guarantee
Retention (%)
Failures among admitted (%)
0
10
20
30
40
50
60
0
2
4
6
8
10
12
14
Generic
Direct H30
Window
Joint cert.
Frozen source
Local recalibration
Local fit + calibration