



- 4 Four cathode-ray oscilloscope (CRO) screens each display a waveform. The screen and the time-base setting of each CRO is shown.

1

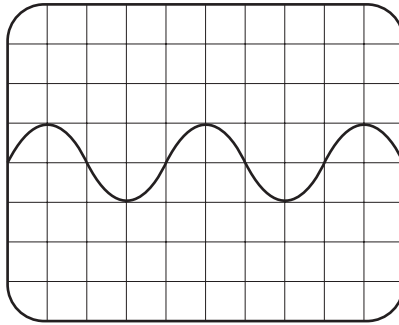


time-base setting: 0.02 s/div

2

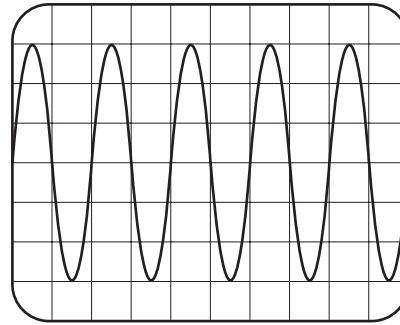


time-base setting: 0.04 s/div

3

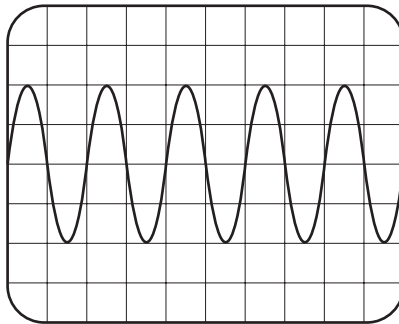

time-base setting: 0.01 s/div

4

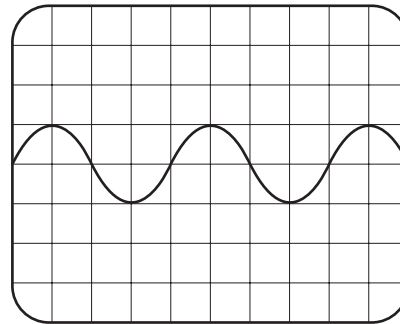

time-base setting: 0.08 s/div

Which screens show waveforms of the same frequency?

- A** 1 and 2 **B** 1 and 3 **C** 1 and 4 **D** 2 and 3