Ontario Ventilator Equipment Pool

Cleaning and Maintenance

For ResMed® Astral® 150

Questions?
Call us during business hours
Mon-Fri 8:30am-4:30pm
to speak with a Registered Respiratory Therapist
1-800-633-8977

Visit our website for more information
www.ontvep.ca



ResMed® Astral® 150 Cleaning and Maintenance
©2024 Ontario Ventilator Equipment Pool. All rights reserved.
Date of Issue: 2023-06-26. Rev. 2025-03-24

Ontario Ventilator Equipment Pool

Table 1. Cleaning frequency recommendations. More information can be found in the Astral® 150 user guide [1]

Item	DAILY	WEEKLY	MONTHLY	EVERY 6 MONTHS
MASK 	Wash by hand with mild soap*. Rinse and air dry. Before use, ensure exhalation ports are not blocked	*Did you know?* *You may only need to replace your mask cushion if you find that your mask no longer seals well*		Replace mask every 6-12 months or as indicated by manufacturer
NON-HEATED TUBING 		Wash by hand with mild soap*. Rinse well and hang to dry		
DISPOSABLE HEATED TUBING 		**Disposable - do not wash** Replace every 7 days [2] unless determined otherwise by clinical team *See "Fisher & Paykel Disposable Circuit Guide" for more information*		
MOUTHPIECE TUBING 			Replace tubing	
MOUTHPIECE FILTER 		**<u>Every 2 weeks:</u>** Replace green angled filter		
WHISPER SWIVEL II 		Wash by hand with mild soap*, rinse well and air dry [3] *Do not use solutions containing bleach or alcohol*		**<u>Every 12 months:</u>** Replace whisper swivel

©2024 Ontario Ventilator Equipment Pool. All rights reserved.
Date of Issue: 2023-06-26. Rev. 2025-03-24

Ontario Ventilator Equipment Pool

Item	DAILY	WEEKLY	MONTHLY
RESMED LEAK VALVE 	Wash by hand with warm water using mild soap* or wipe with 70% isopropyl alcohol. Rinse well and air dry [4]	Discard and replace after 7 days of use [4]	
INTERSURGICAL ACTIVE EXHALATION VALVE 		Wash by hand in warm water with mild soap as needed. Do not exceed 30 cleaning cycles.	Replace Intersurgical Active Exhalation Device
REUSABLE HUMIDIFIER CHAMBER 	Wash by hand with warm water using mild soap*. Rinse well and air dry [6]		
DISPOSABLE AUTO-FILL CHAMBER 		**Disposable - do not wash** Replace every 7 days [2] unless determined otherwise by clinical team *See "Fisher & Paykel Disposable Circuit Guide" for more information*	
WATER BAG 		Use chlorine based sterilization tablets and **COLD** water to clean bag[7] *See "Fisher & Paykel Disposable Circuit Guide" for more information*	**<u>Every 2 months:</u>** Replace water bag

©2024 Ontario Ventilator Equipment Pool. All rights reserved.
Date of Issue: 2023-06-26. Rev. 2025-03-24

Ontario Ventilator Equipment Pool

Item	WEEKLY	MONTHLY	EVERY 6 MONTHS
CIRCUIT ADAPTER 	Inspect condition of circuit adapter for moisture or contaminants [1]		Replace **single limb** or **double limb** circuit adapter [8]
AIR INLET FILTER Part Number 27939 (4pk) 		Inspect for dirt and dust [1]	Replace air inlet filter. **Do not wash or reuse** [1]
ANTIBACTERIAL FILTER 		Replace monthly or more frequently if needed. **Do not wash or reuse**	
DEVICE 	• Test alarm sounders to ensure audible alarms are functional [8] *(see instructions on next page)* • Wipe exterior of the device with a damp cloth using an approved mild cleaning solution + [8]		
CARE OF INTERNAL BATTERY		Check the charge level of the internal battery [8] 1. Disconnect from external power for 10 minutes 2. Review remaining battery capacity. Monitor battery capacity with use of device. As device ages, available battery capacity decreased 3. Restore external power after test complete	Recharge internal battery if device is not used [8]

* Soap that contains no emollients or antibacterial ingredients
+ Actichlor Plus, Bleach (1:10), Isopropanol, Cavicide™, Mikrozid™ (Cavicide™ and Mikrozid™ use monthly only) [2]

©2024 Ontario Ventilator Equipment Pool. All rights reserved.
Date of Issue: 2023-06-26. Rev. 2025-03-24

Ontario Ventilator Equipment Pool

How to Test Alarm Sounders [8] *(weekly)*

1. Press  . Alarm screen displayed.
2. Press  . Alarm volume screen displayed.
3. Press **TEST**. Alarm beeps twice and LED flashes to indicate it is working correctly. Confirm alarm beeps twice. Confirm alarm bar flashes red then yellow. Confirm mute button flashes.


How to Replace Air Inlet Filter [1] *(every 6 months)*

Located on the rear of device

1. Unlock the air filter cover by turning counter-clockwise.
2. Pull the air filter cover from the device.
3. Remove the air filter from the cover and discard.
4. Insert new filter into the cover.
5. Insert the air filter and cover back into device.
6. Turn clockwise to secure in place.





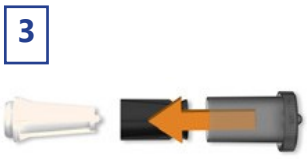







©2024 Ontario Ventilator Equipment Pool. All rights reserved.
Date of Issue: 2023-06-26. Rev. 2025-03-24

Ontario Ventilator Equipment Pool

References

1. ResMed®. (2017). *Astral ® series user guide*
2. Fisher & Paykel™ Healthcare. *RT-series breathing circuits*
3. Philips® Respironics®. (2019). *Whisper swivel II*
4. ResMed®. (2018). *ResMed ® Leak valve instruction sheet*
5. Philips® Respironics®. *Active exhalation device*
6. Fisher & Paykel™ Healthcare. (2021). *Operating instructions - H3C00 humidification chamber*
7. Fisher & Paykel™ Healthcare. (2020). *myAIRVO/myAIRVO 2 Water Bag (2-Pack) 900PT401 package insert*
8. ResMed®. (2018). *Astral ® series clinical guide*

Disclaimer

This information is provided to you for educational purposes only and should not at any time be considered a substitute for professional advice from your physician or other qualified health care professional. The VEP does not assume any responsibility for application of the content of this document or for any information that may be present in the documents or websites cited as a reference. These references are provided for informational purposes only and do not represent VEP endorsement of any company or product. Always consult your physician and/or a qualified health care professional to learn more about recommendations specific to your health needs.

640 Cataraqui Woods Drive | Unit 6 | Kingston, ON | K7P 2Y5
Tel: 613-548-6156 | Toll-Free in Ontario: 1-800-633-8977 | Fax: 613-548-6157
General Email: vep@kingstonhsc.ca | Web: www.ontvep.ca

©2024 Ontario Ventilator Equipment Pool. All rights reserved.

Date of Issue: 2023-06-26. Rev. 2025-03-24