



Independent Research Testing Center
875 Innovation Drive, Cambridge, MA 02139, USA

CERTIFICATE OF ANALYSIS (COA)


Product Name	Bacteriostatic Water 3 ml (Injectable Research Vial)
Chemical Name	Sterile water for injection with 0.9% benzyl alcohol
CAS Number	7732-18-5
Batch / Lot Number	BACTERIO3ML260607
Manufacturing Date	2026-06-07
Retest / Expiry Date	2028-06-07
Net Content	3ml per vial
Storage Conditions	Store at 15–25°C, protected from light
Appearance	Clear, colorless liquid
Molecular Formula / MW	H ₂ O / See formula

ANALYTICAL RESULTS

Test Item	Specification	Result	Method
Identification	Conforms	Conforms	LC-MS
Assay	≥98.0%	98.84%	HPLC
pH	4.5–7.5	6.5	USP <791>
Appearance	Clear, colorless liquid	Conforms	Visual
Particulate Matter	Essentially free	Conforms	Visual
Heavy Metals	≤10 ppm	<10 ppm	ICP-MS
Endotoxin	<10 EU/mg	<10 EU/mg	LAL Test

HPLC CHROMATOGRAM

DAD1A, Sig=214, 4 Ref=off

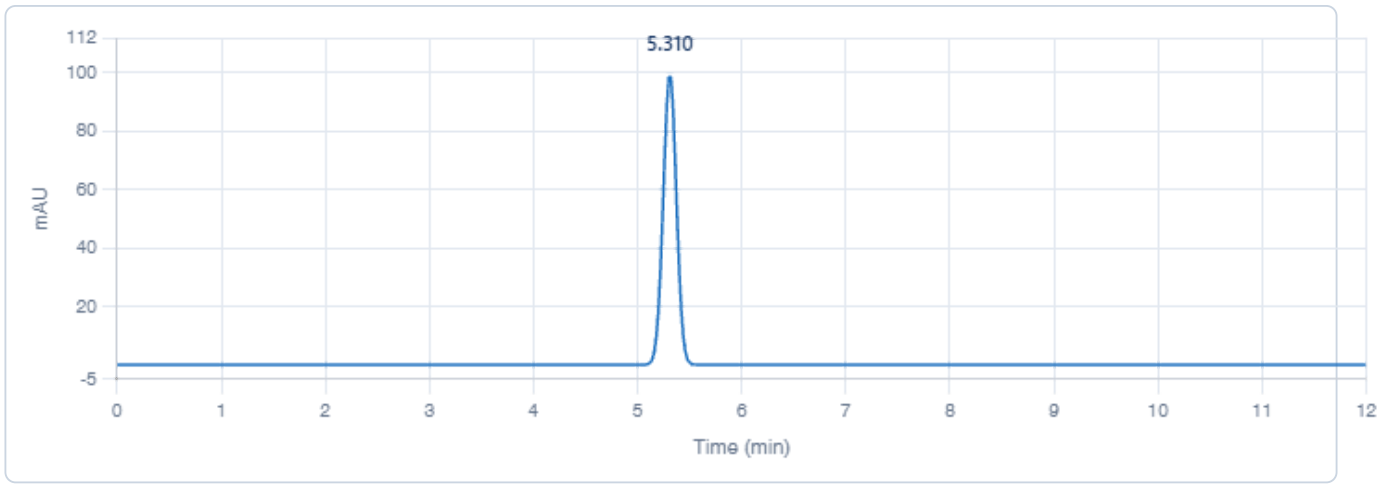

For laboratory research use only. Not for human consumption.

TESTER NAME

Dr. Michael Carter

SIGNATURE

Michael Carter

TEST DATE

2026-07-04