



Independent Research Testing Center
875 Innovation Drive, Cambridge, MA 02139, USA

CERTIFICATE OF ANALYSIS (COA)


Product Name	HCG 5000 IU (Injectable Research Vial)
Chemical Name	Human chorionic gonadotropin
CAS Number	9002-61-3
Batch / Lot Number	HCG5000IU260509
Manufacturing Date	2026-05-09
Retest / Expiry Date	2028-05-09
Net Content	5000 IU per vial
Storage Conditions	Store at 2–8°C, protected from light and moisture
Appearance	White to off-white lyophilized powder
Molecular Formula / MW	— / —

ANALYTICAL RESULTS

Test Item	Specification	Result	Method
Identification	Conforms	Conforms	LC-MS
Purity (HPLC)	≥98.0%	98.91%	HPLC
Peptide Content	95.0–105.0%	100.3%	HPLC
Appearance	White to off-white lyophilized powder	Conforms	Visual
Water Content	≤3.0%	0.8%	Karl Fischer
Heavy Metals	≤10 ppm	<10 ppm	ICP-MS
Endotoxin	<10 EU/mg	<10 EU/mg	LAL Test

HPLC CHROMATOGRAM

DAD1A, Sig=214, 4 Ref=off

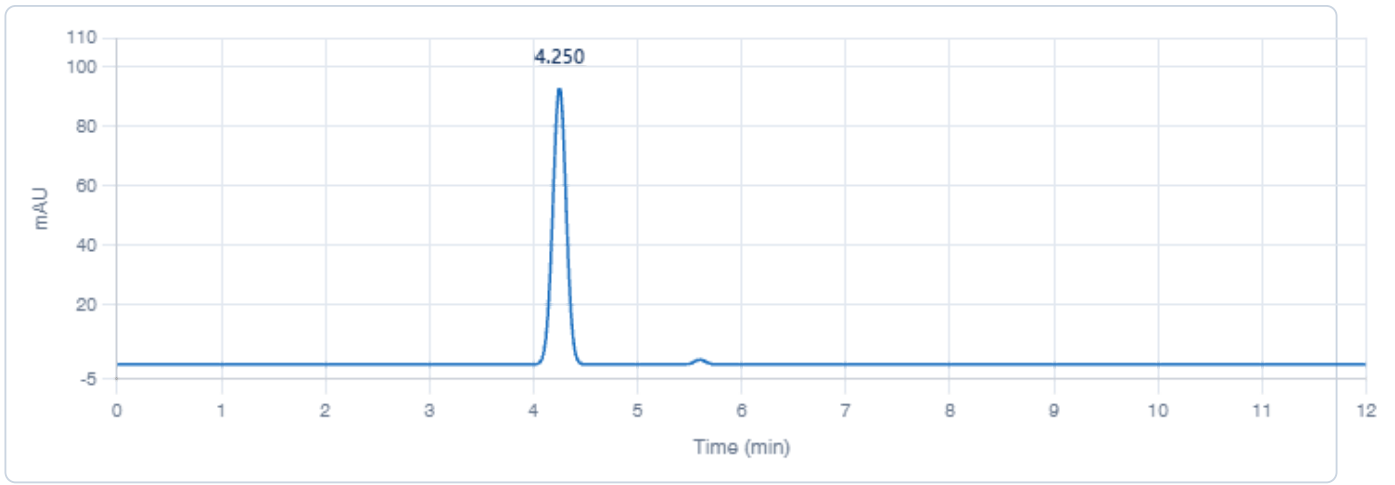

For laboratory research use only. Not for human consumption.

TESTER NAME

Dr. Michael Carter

SIGNATURE

Michael Carter

TEST DATE

2026-05-31