


P 1/2

#1628

WHI R&D: 2021.8.9.


Device-Offline

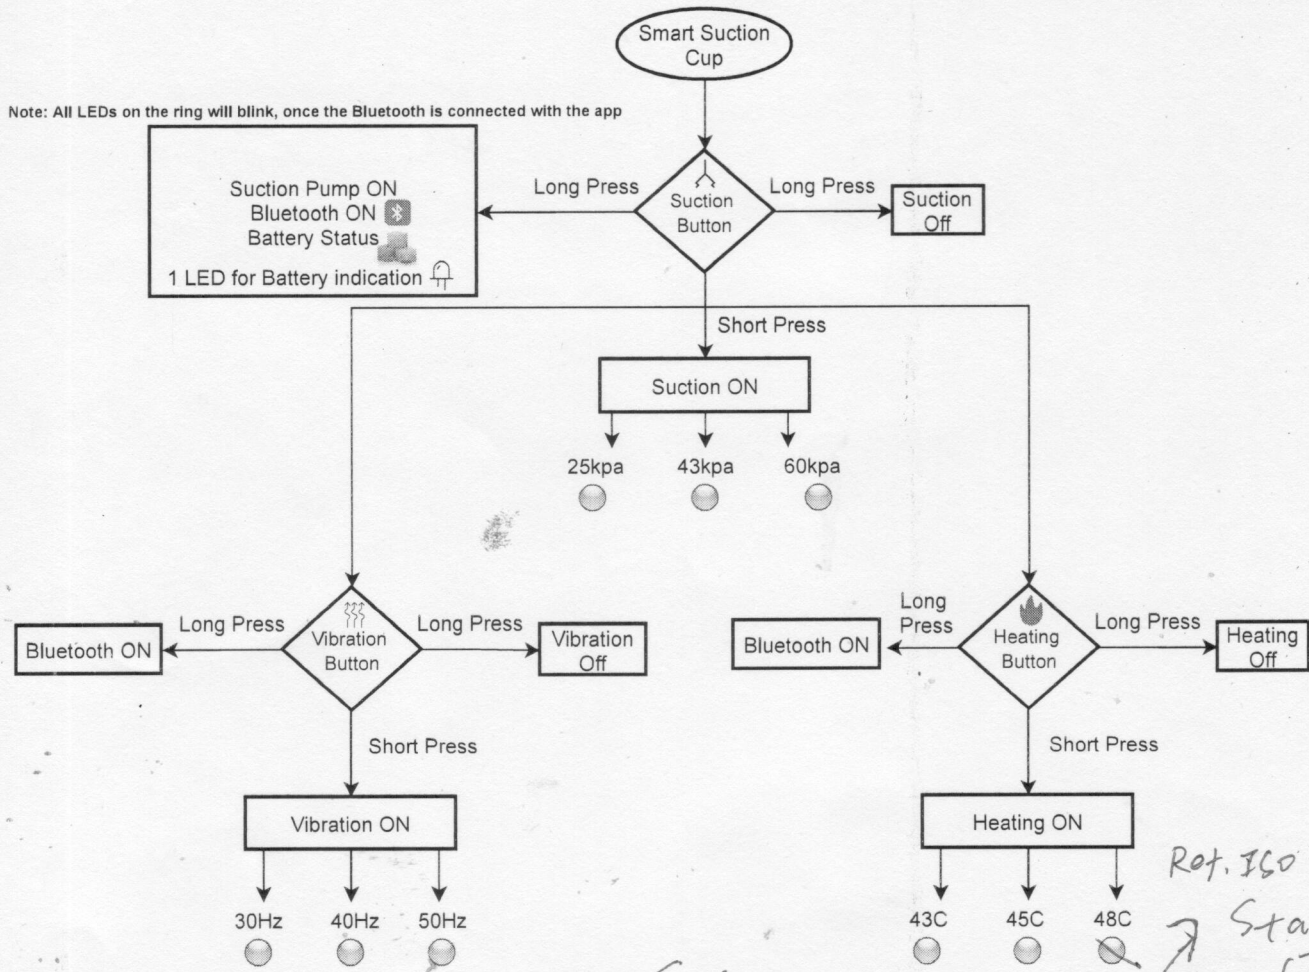



Note: Standard 5 min Timer in OFFLINE mode will start after all treatments are selected

Ref. ISO-13732-1
Standard
48C - 10 min
max

App-Online

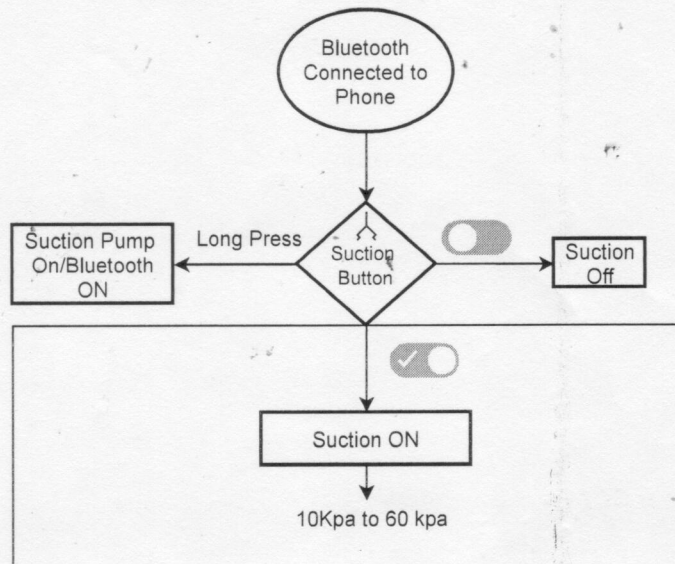


P2/2

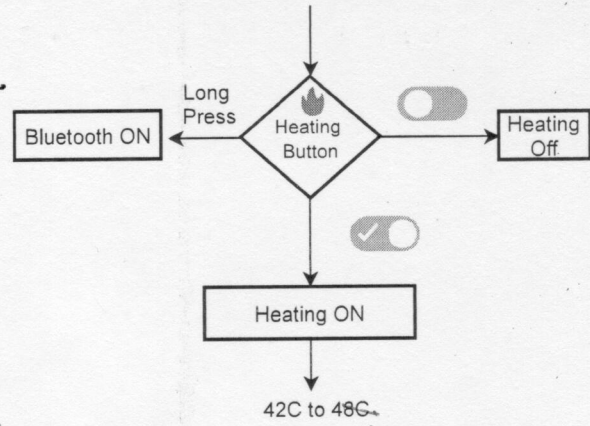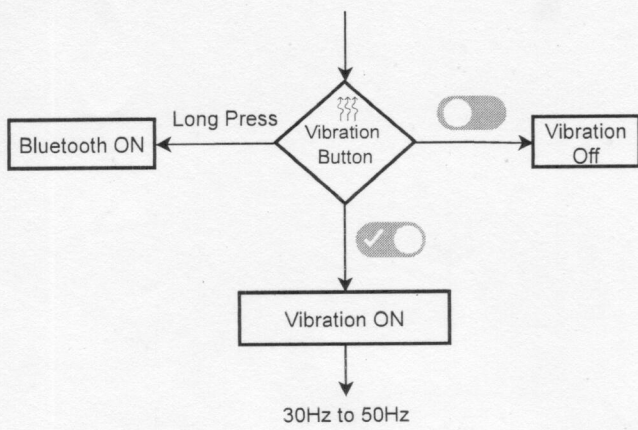

Suggested: 40C-46C-47max

Note: Slide the Timer toggle once the treatment settings are Select. Select the timer levels

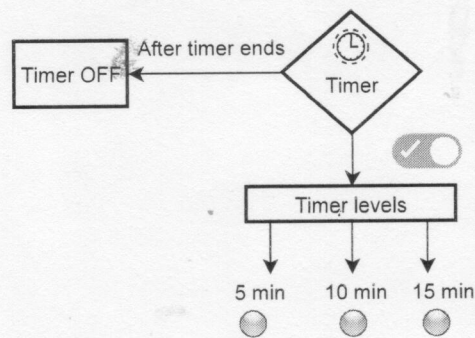

Timer mins will be displayed on the app