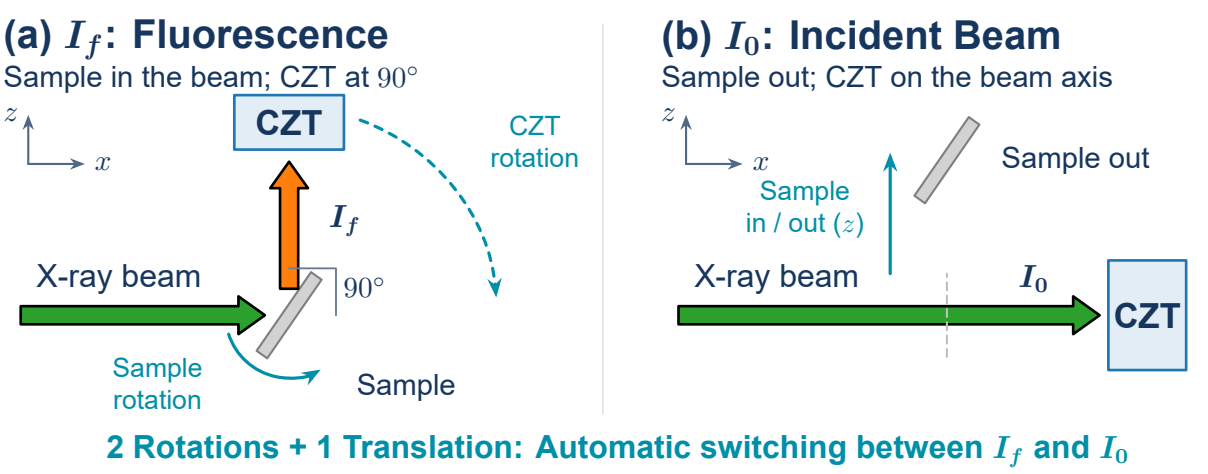
(a) I_f: Fluorescence
Sample in the beam; CZT at 90°
z
x
CZT
CZT rotation
I_f
X-ray beam
90°
Sample rotation
Sample
(b) I_0: Incident Beam
Sample out; CZT on the beam axis
z
x
Sample out
Sample in / out (z)
X-ray beam
I_0
CZT
2 Rotations + 1 Translation: Automatic switching between I_f and I_0