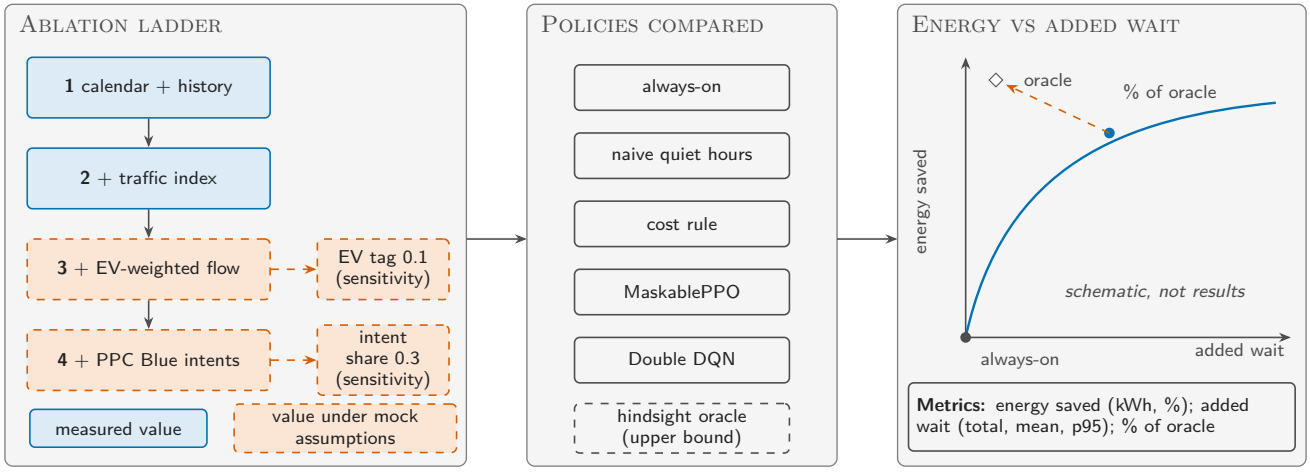


Ablation steps are scored with forecast metrics on the 2024–2025 test sample; policies are compared on the same test period. Sensitivity variants rerun a step with the changed mock parameter.