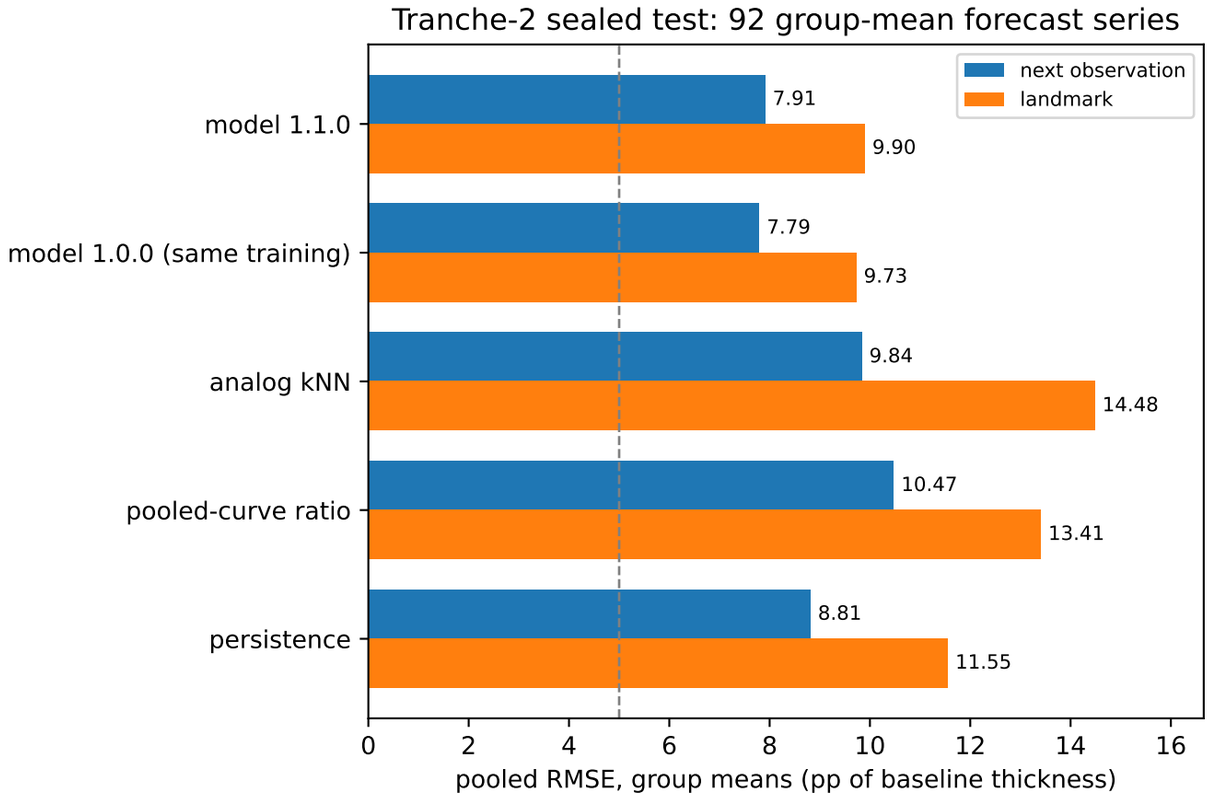
Tranche-2 sealed test: 92 group-mean forecast series
next observation
landmark
model 1.1.0
model 1.0.0 (same training)
analog kNN
pooled-curve ratio
persistence
7.91
9.90
7.79
9.73
9.84
14.48
10.47
13.41
8.81
11.55
0
2
4
6
8
10
12
14
16
pooled RMSE, group means (pp of baseline thickness)

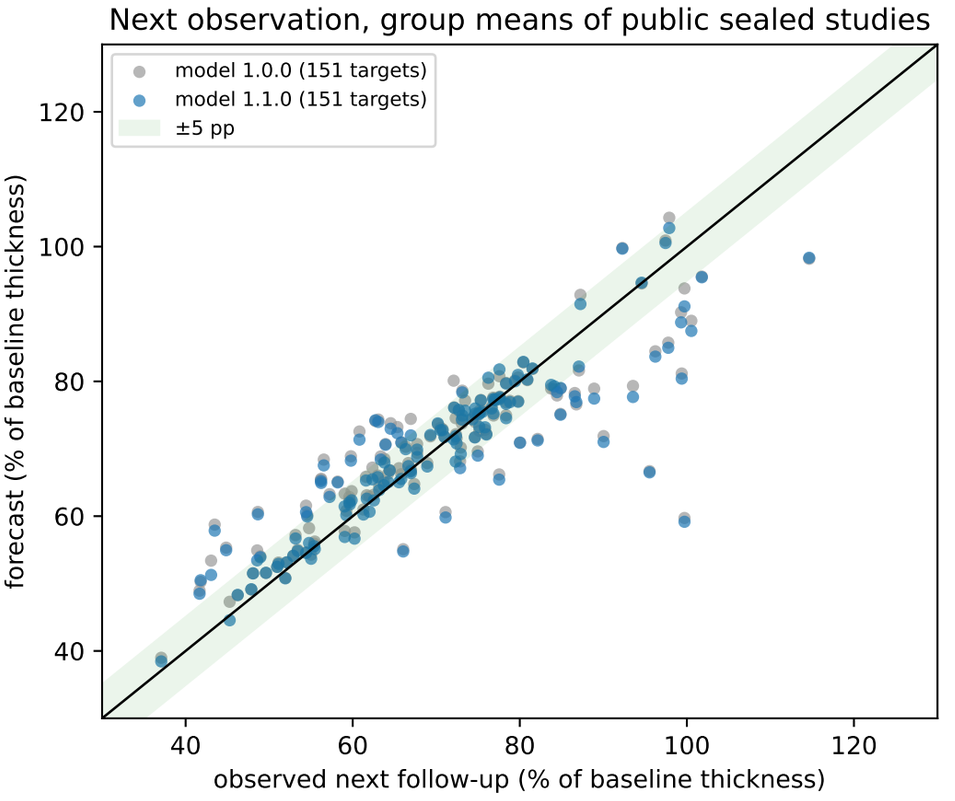
Next observation, group means of public sealed studies
model 1.0.0 (151 targets)
model 1.1.0 (151 targets)
±5 pp
forecast (% of baseline thickness)
observed next follow-up (% of baseline thickness)
40
60
80
100
120

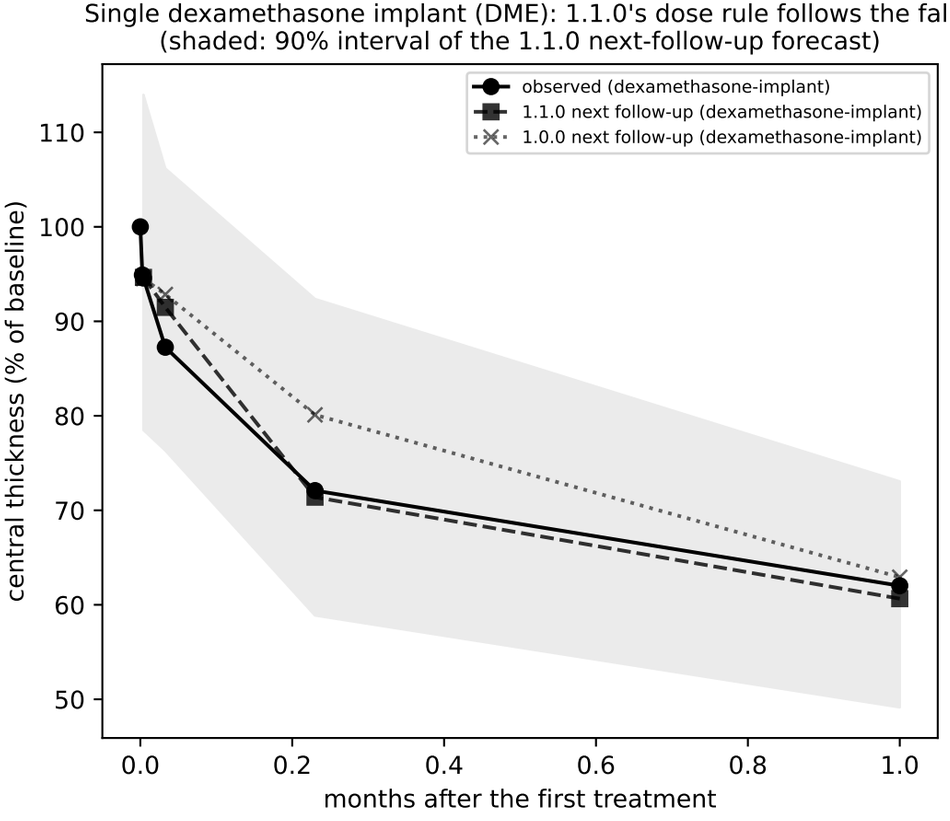
Single dexamethasone implant (DME): 1.1.0's dose rule follows the fall
(shaded: 90% interval of the 1.1.0 next-follow-up forecast)
observed (dexamethasone-implant)
1.1.0 next follow-up (dexamethasone-implant)
1.0.0 next follow-up (dexamethasone-implant)
central thickness (% of baseline)
months after the first treatment
50
60
70
80
90
100
110
0.0
0.2
0.4
0.6
0.8
1.0

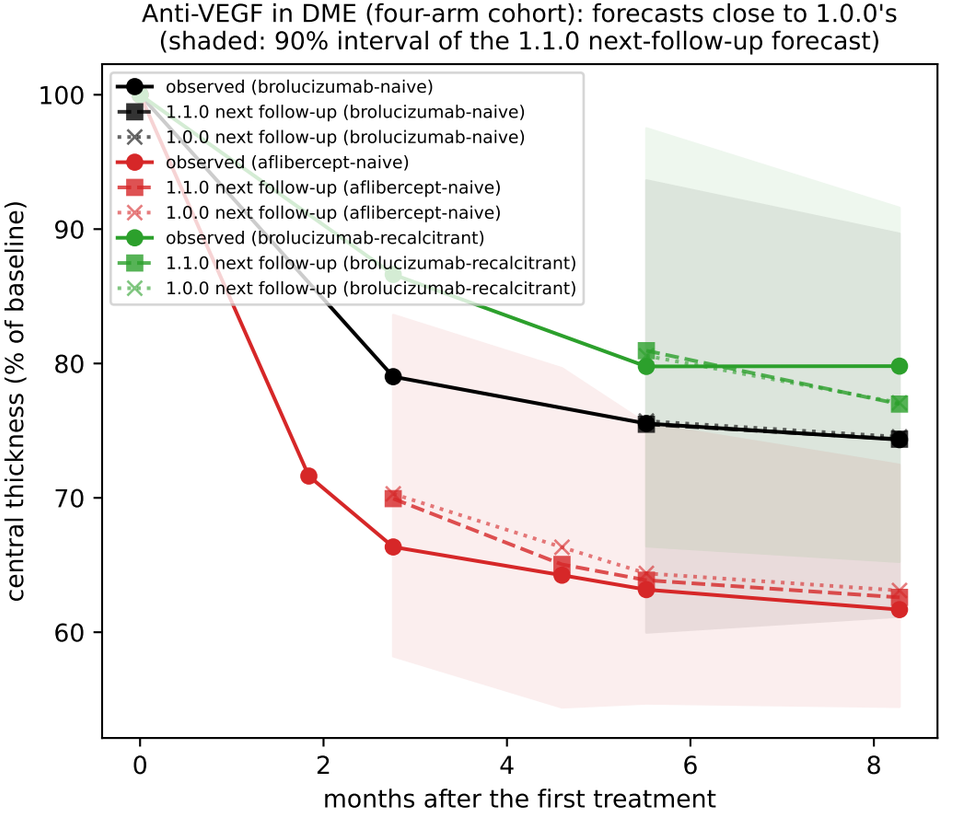
Anti-VEGF in DME (four-arm cohort): forecasts close to 1.0.0's
(shaded: 90% interval of the 1.1.0 next-follow-up forecast)
observed (brolucizumab-naive)
1.1.0 next follow-up (brolucizumab-naive)
1.0.0 next follow-up (brolucizumab-naive)
observed (aflibercept-naive)
1.1.0 next follow-up (aflibercept-naive)
1.0.0 next follow-up (aflibercept-naive)
observed (brolucizumab-recalcitrant)
1.1.0 next follow-up (brolucizumab-recalcitrant)
1.0.0 next follow-up (brolucizumab-recalcitrant)
central thickness (% of baseline)
months after the first treatment
60
70
80
90
100
0
2
4
6
8