Tranche-5 sealed test: 20 group-mean forecast series; H1–H4 pass
H5 fails: landmark 9.14 vs 8.95 pp, next observation 8.34 vs 8.28 for 1.2.0

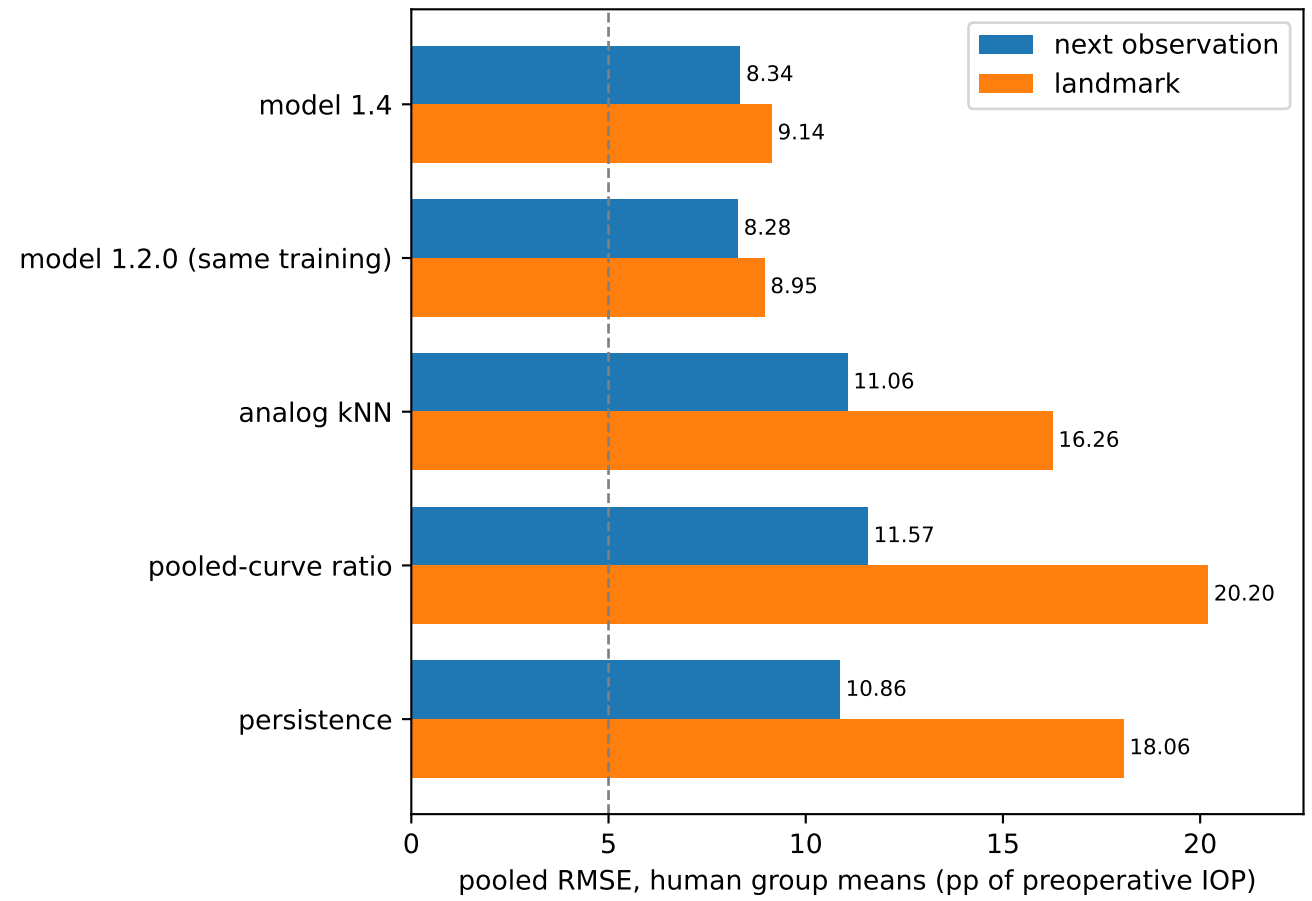

H5 rests on one study: the sub-procedure level for endoscopic cyclophotocoagulation lowered its initial state error and raised its forecast errors

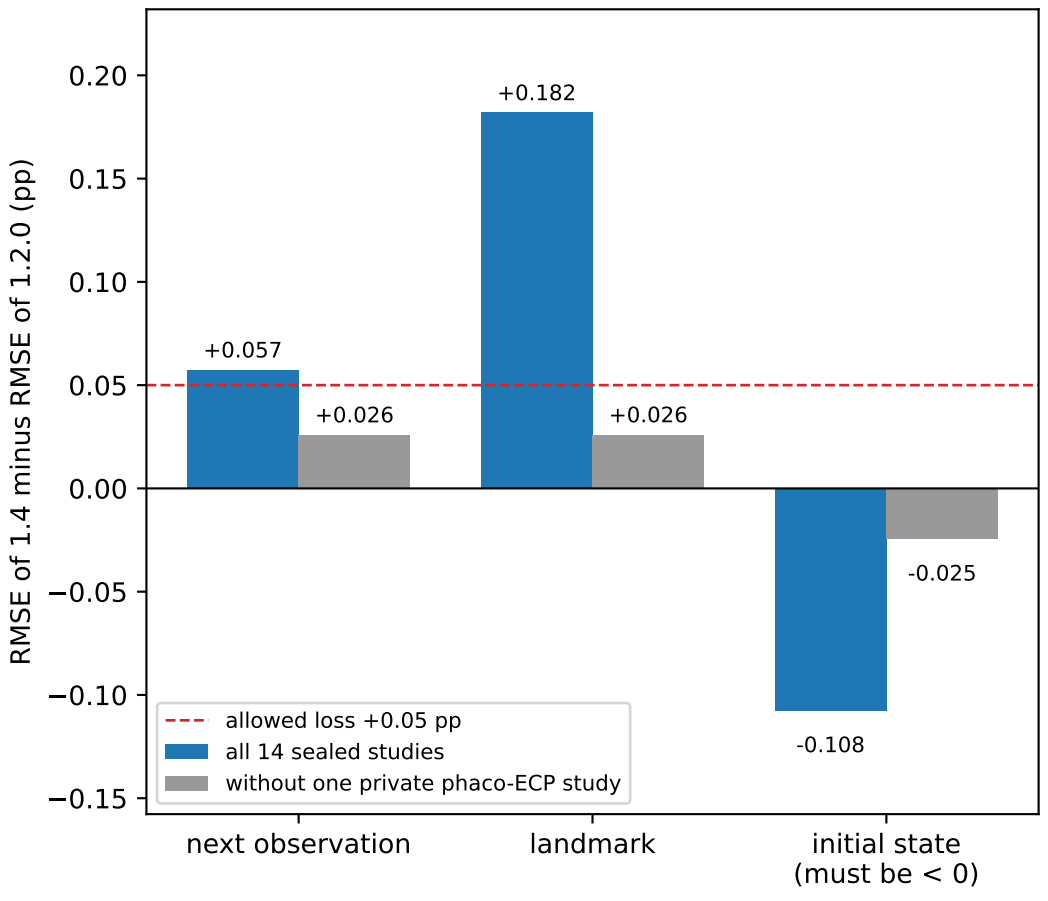

PreserFlo and XEN (two studies): the device level improves the initial state

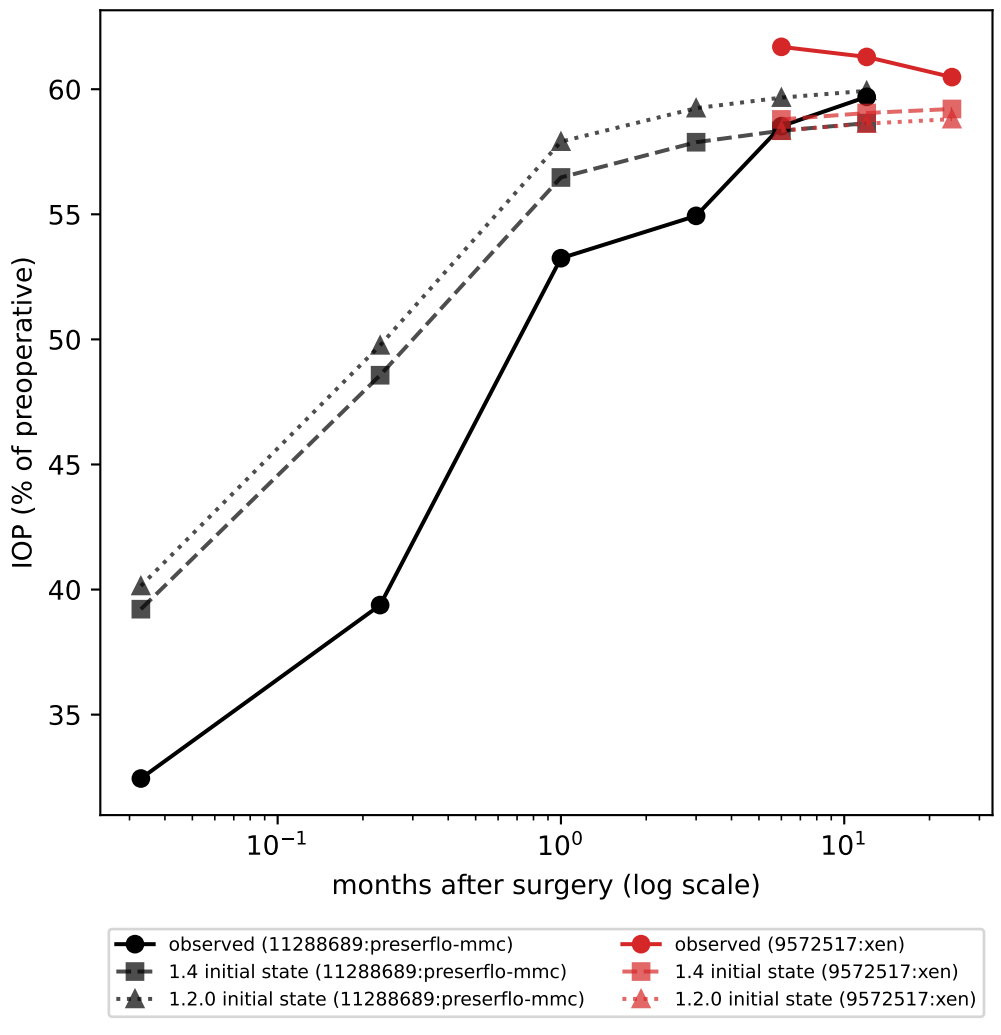
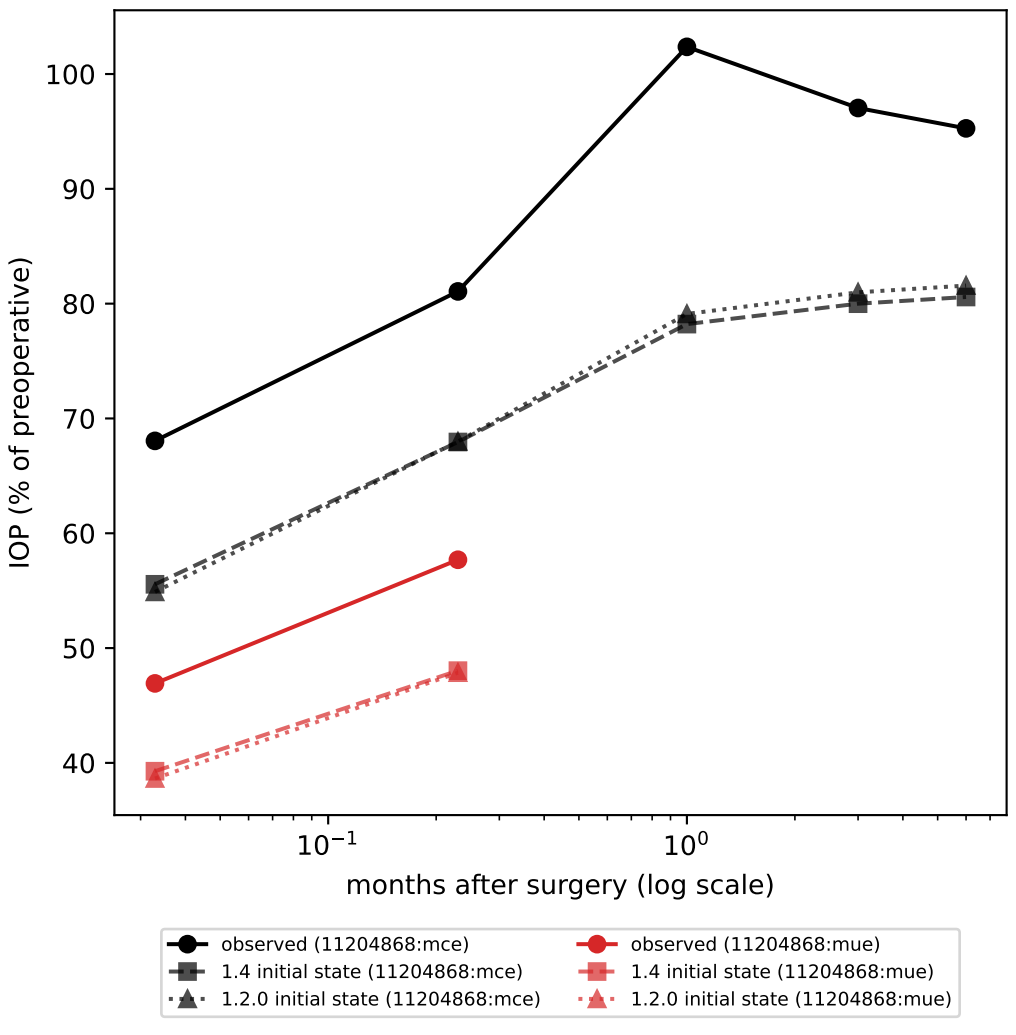
XEN45 read as 'other' by the frozen keyword rule (one study, two subgroups)