

(Fort Lauderdale, FL) Today, Congressman Alcee L. Hastings (D-Miramar) made the following statement to mark the 17th Annual National HIV Testing Day, a joint initiative between the National Association of People With AIDS (NAPWA) and the Centers for Disease Control and Prevention (CDC) aimed at promoting HIV testing.

"There are approximately 1.1 million people living in the United States with HIV/AIDS and an estimated 56,300 Americans are newly infected each year. Furthermore, according to the Centers for Disease Control and Prevention (CDC), more than one in five HIV-positive individuals are unaware that they are infected. This is truly alarming.

"I commend NAPWA and the CDC for all their hard work in making National HIV Testing Day a success year after year. We must ensure access to HIV testing that is confidential, rapid, and accurate. Combining the effectiveness of voluntary, routine screening with smart policy can help stem the transmission of, and improve the health outcomes associated with, this virus.

"Routine screening for HIV has been proven to save lives and reduce new infections. That is why I introduced in May the *Increasing Access to Voluntary Screening for HIV/AIDS and STIs Act of 2011*. Among other things, the bill requires Medicaid to cover voluntary screening for HIV/AIDS and other STIs as a mandatory service for all individuals 13 and older. It also provides states with the support they need to cover low-income individuals infected with HIV until Medicaid is expanded in 2014 under the *Patient Protection and Affordable Care Act*.

"We cannot talk about HIV testing without also addressing access to care. In providing increased funding to the AIDS Drug Assistance Program (ADAP) in the full-year Continuing Resolution for FY 2011, Congress brought much-needed relief to individuals living with HIV/AIDS who were waiting for antiretroviral treatment and other related services. However, further commitment is needed to bring an end to the ongoing ADAP funding crisis. In fact, Florida continues to lead ADAP waiting lists in 13 states nationwide with 3,581 individuals.

"This National HIV Testing Day, I pledge to continue working with my colleagues in Congress to address barriers to HIV testing and access to care, as well as secure additional funding for ADAP and other national prevention and treatment efforts. I also urge all sexually-active

Americans to get tested and know their status. HIV/AIDS is not just a personal health issue; it is a community health issue and we all have a responsibility to do our part in preventing the incidence and transmission of this disease."

Congressman Alcee L. Hastings serves as Senior Member of the House Rules Committee, Ranking Democratic Member of the U.S. Helsinki Commission, and Democratic Chairman of the Florida Delegation.

###



National Institute for Occupational Safety and Health
National Personal Protective Technology Laboratory
P.O. Box 18070
Pittsburgh, PA 15236

Procedure No. RCT-ASR-STP-0100

Revision: 1.1

Date: 3 June 2005

DETERMINATION OF STRENGTH OF HOSES AND COUPLINGS,
TYPE C, AND CE SUPPLIED-AIR RESPIRATORS
STANDARD TESTING PROCEDURE (STP)

1. PURPOSE

This test establishes the procedures for ensuring that the level of protection provided by the strength of hoses and couplings requirements on Types C and CE Supplied-Air Respirators submitted for Approval, Extension of Approval, or examined during Certified Product Audits, meet the minimum certification standards set forth in 42 CFR, Part 84, Subpart G, Section 84.63(a)(c)(d), and Subpart J, Section 84.150, Table 8; Volume 60, Number 110, June 8, 1995.

2. GENERAL

This STP describes the Determination of Strength of Hose and Coupling Type C, and CE Supplied-Air Respirators test in sufficient detail that a person knowledgeable in the appropriate technical field can select equipment with the necessary resolution, conduct the test, and determine whether or not the product passes the test.

3. EQUIPMENT/MATERIALS

3.1. The list of necessary test equipment and materials follows:

- 3.1.1. A source of compressed air (a 300 cubic foot gas cylinder) capable of delivering 250 psig or higher.
- 3.1.2. Air regulator, Model 8, from Matheson Gas Products or equivalent.
- 3.1.3. A Helicoid calibrated pressure gauge and connecting fittings or equivalent
- 3.1.4. Two sections of applicant's supplied-air hose.
- 3.1.5. A four-inch pulley, or equivalent.
- 3.1.6. An American Chain and Cable Company Model E Overhead Chain Hoist, or equivalent.
- 3.1.7. A 45 kilogram (100 pound) weight.

Approvals:	<u>1st</u> Level	<u>2nd</u> Level	<u>3rd</u> Level
------------	------------------	------------------	------------------

Procedure No. RCT-ASR-STP-0100	Revision: 1.1	Date: 3 June 2005	Page 2 of 7
--------------------------------	---------------	-------------------	-------------

- 3.1.8. Two 2-foot sections of strong rope with breaking strength above 250 lb or equivalent.
- 3.1.9. A safety cable capable of securing both ends of the hose at the coupling or equivalent.
- 3.1.10. Electric timer, calibrated to hundredths of a minute (Precision Scientific Co.) or equivalent.
- 3.1.11. A calibrated Tinius Olsen, Model LTCM, compression/tension strain gauge, or equivalent, may be substituted for the pulley, chain hoist, and weights.

4. TESTING REQUIREMENTS AND CONDITIONS

- 4.1. Prior to beginning any testing, all measuring equipment to be used must have been calibrated in accordance with the manufacturer's calibration procedure and schedule. At a minimum, all measuring equipment utilized for this testing must have been calibrated within the preceding 12 months using a method traceable to the National Institute of Standards and Technology (NIST).
- 4.2. The compressed gas cylinder must meet all applicable Department of Transportation requirements for cylinder approval as well as for retesting/requalification.
- 4.3. Normal laboratory safety practices must be observed. This includes safety precautions described in the current ALOSH Facility Laboratory Safety Manual.
 - 4.3.1. Safety glasses, lab coats, and hard-toe shoes must be worn at all times.
 - 4.3.2. Work benches must be maintained free of clutter and non-essential test equipment.
 - 4.3.3. When handling any glass laboratory equipment, lab technicians and personnel must wear special gloves which protect against lacerations or punctures.

5. PROCEDURE

Note: Reference Section 3 for equipment, model numbers and manufacturers. For calibration purposes use those described in the manufacturer's operation and maintenance manuals.

- 5.1. Use the test operating procedure as follows:
 - 5.1.1. Connect two sections of the applicant's supplied-air hose with coupling (be sure to use the safety cable).
 - 5.1.2. Secure one end of connected hoses to the proper test weight (45 kilograms-100 pounds), or to the Tinius Olsen strain gauge (within 1-foot of the coupling).
 - 5.1.3. Place air-supply hose over a four-inch pulley held suspended with a short rope

Procedure No. RCT-ASR-STP-0100	Revision: 1.1	Date: 3 June 2005	Page 3 of 7
--------------------------------	---------------	-------------------	-------------

from an overhead chain hoist, or connect the hose coupling on the other end of the hose to the opposite end of the strain gauge (within 1-foot of the coupling).

- 5.1.4. Attach one end of connected hoses to a two-stage regulator and compressed air source; attach a female quick connect coupling to the opposite end of the connected hoses.
- 5.1.5. Slowly increase air pressure within connected hoses until desired pressure is reached and check for signs of possible rupture.
- 5.1.6. Pull air-supply hose across the pulley until hose becomes taut, making certain that the coupling of the hoses is between the hoist and the weight, or both couplings and the strain gauge is between the hoist and the anchor point (See Figure 1).
- 5.1.7. Secure remaining end of the connected hoses.
- 5.1.8. Slowly raise the hook of the overhead hoist and start the timer when weight leaves the laboratory floor, or when the required weight has been reached on the strain gauge.
- 5.1.9. After five minutes, stop the timer and release the pull on the hose couplings.
- 5.1.10. Remove pressure from within connected air-supply hoses.
- 5.1.11. Examine the couplings and hoses for any indications of separation or failure.

Note: Photographs may be taken for records documentation.

Note: If the hoses pass this test then the same hoses and couplings must be used on the Tightness of Hose and Couplings and Gasoline Permeation tests.

6. PASS/FAIL CRITERIA

- 6.1. The criterion for passing this test is set forth in 42 CFR, Part 84, Subpart G, Section 84.63(a)(c)(d), and Subpart J, Section 84.150, Table 8; Volume 60, Number 110, June 8, 1995.
- 6.2. This test establishes the standard procedure for ensuring that:
 - 84.63 Test requirements; general.
 - (a) Each respirator and respirator component shall when tested by the applicant and by the Institute, meet the applicable requirements set forth in subparts H through L of this part.
 - (c) In addition to the minimum requirements set forth in subparts H through L of this part, the Institute reserves the right to require, as a further condition of approval, any additional requirements deemed necessary to establish the quality, effectiveness, and

Procedure No. RCT-ASR-STP-0100	Revision: 1.1	Date: 3 June 2005	Page 4 of 7
--------------------------------	---------------	-------------------	-------------

safety of any respirator used as protection against hazardous atmospheres.

(d) Where it is determined after receipt of an application that additional requirements will be required for approval, the Institute will notify the applicant in writing of these additional requirements, and necessary examinations, inspections, or tests, stating generally the reasons for such requirements, examinations, inspections, or tests.

84.150 Air-supply line tests; minimum requirements.

Air supply lines employed on Types C and CE supplied-air respirators shall meet the minimum test requirements set forth in Table 8 of this subpart.

Air-supply-lines used with Types C and CE, hose and couplings shall not exhibit any separation or failure when tested with a pull of 45 kg. (100 pounds) for 5 minutes and when simultaneously subjecting them to an internal air pressure of 2 times the maximum respirator-supply pressure that is specified by the applicant or at 173 kN/m.² (25 pounds per square inch) gauge, whichever is higher.

7. RECORDS\TEST SHEETS

- 7.1. All test data will be recorded on the STRENGTH OF HOSES AND COUPLINGS, TYPE C AND CE, SUPPLIED-AIR RESPIRATORS test data sheet.
- 7.2. All videotapes and photographs of the actual test being performed, or of the tested equipment shall be maintained in the task file as part of the permanent record.
- 7.3. All equipment failing any portion of this test will be handled as follows:
 - 7.3.1. If the failure occurs on a new certification application, or extension of approval application, send a test report to the RCT Leader and prepare the hardware for return to the manufacturer.
 - 7.3.2. If the failure occurs on hardware examined under an Off-the-Shelf Audit the hardware will be examined by a technician and the RCT Leader for cause. All equipment failing any portion of this test may be sent to the manufacturer for examination and then returned to NIOSH. However, the hardware tested shall be held at the testing laboratory until authorized for release by the RCT Leader, or his designee, following the standard operating procedures outlined in Procedure for Scheduling, and Processing Post-Certification Product Audits, RB-SOP-0005-00.

Procedure No. RCT-ASR-STP-0100	Revision: 1.1	Date: 3 June 2005	Page 5 of 7
--------------------------------	---------------	-------------------	-------------

**STRENGTH OF HOSES AND COUPLINGS, TYPE C AND CE,
SUPPLIED-AIR RESPIRATORS**

Project No : _____ Date:

Company :

Respirator Type:

Reference: 42 CFR, Part 84, Subpart J, Section 84.150, Table 8.

Requirement: Hose and couplings shall not exhibit any separation or failure when tested with a pull of 45 kg. (100 pounds) for 5 minutes and when simultaneously subjecting them to an internal air pressure of 2 times the maximum respirator-supply pressure that is specified by the applicant or at 173 kN/m.² (25 pounds per square inch) gauge, whichever is higher.

Test Apparatus Used: 100 lb. weight_____ / Strain Gauge

Test Data: : Hose internal air pressure - _____ (psig)

: Pounds of pull or tension - _____ (lbs.)

: Test time period - _____ (min - sec)

Evaluation: : Separation or failure occurred at a coupling: YES_____ / NO

: Separation or failure occurred in the hose: YES_____ / NO

Comments :

Test Engineer: _____ PASS_____ FAIL

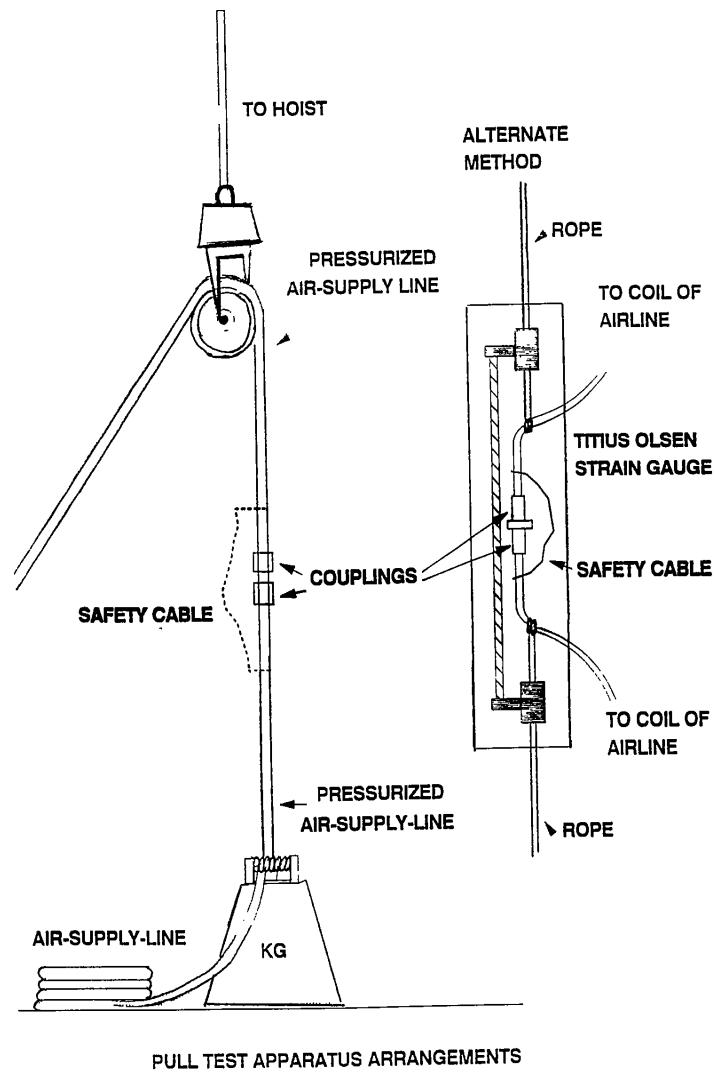


Figure 1

Pull Test Apparatus Arrangement

Procedure No. RCT-ASR-STP-0100	Revision: 1.1	Date: 3 June 2005	Page 7 of 7
--------------------------------	---------------	-------------------	-------------

Revision History

Revision	Date	Reason for Revision
1.0	27 June 2001	Historic document
1.1	3 June 2005	Update header and format to reflect lab move from Morgantown, WV No changes to method

If you want to share your comments or views on a Federal issue you can email me from this page. Please Click the link below to e-mail me. The first step will be to verify your zip code on the next page, which will bring you to a short email form to ensure that I receive your contact information.

If you need immediate assistance, please call my Newport News Office at (757) 380-1000 or my Richmond Office at (804) 644-4845 and a member of my staff will assist you.

To ensure that your correspondence is responded to as promptly as possible, please note the following before e-mailing Rep. Scott:

- **CASEWORK:** If you need assistance with a Federal Agency, please [click here](#) .
- **TOURS:** If you are planning a trip to Washington, DC and would like help scheduling Congressional tours, please [click here](#) .
- **MEDIA INQUIRIES:** If you are a member of the Press, please direct all Media Inquiries to the Press Secretary in the Washington Office (202-225-8351).
- **SCHEDULING:** If you would like to invite Congressman Scott to an event, please [click here](#) .

[E-Mail Rep. Bobby Scott](#)

If you prefer, please feel free to call or write one of my offices:

Washington, DC Office

1201 Longworth House Office Building
Washington, DC 20515
(202) 225-8351 | FAX (202) 225-8354

Hampton Roads Office

2600 Washington, Ave, Suite 1010
Newport News, VA 23607
(757) 380-1000 | FAX (757) 928-6694

Richmond Area Office

400 N 8th Street, Suite 430

Richmond, VA 23219

(804) 644-4845 | FAX (804) 648-6026

*Peer Review Framework for Predictive Analytics
in Humanitarian Response*

MODEL REPORT: Trigger for OCHA Anticipatory Action on Drought in Chad

Trigger developed by the UN OCHA Centre for Humanitarian Data

June 2023

OCHA CENTRE FOR HUMANITARIAN DATA



OCHA

centre for humdata

Model Report:

Trigger for OCHA Anticipatory Action on Drought in Chad

1. Background

This document summarizes the documentation and findings of the peer review of the model used by the UN Central Emergency Response Fund to trigger the [drought anticipatory action framework](#) in Chad. The model is a go-no-go trigger mechanism designed to anticipate humanitarian impacts of seasonal drought in a sub-region of Chad.

The review has been conducted between January and May 2023.

2. Main Findings and Recommendations

You can find all the documentation regarding the model, its application and the review process at the following links:

- The [Model Card](#) describes the version of the model that was endorsed by humanitarian action in November 2022 and was completed in January 2023.
- The [Model Evaluation Matrix](#) was completed in February 2023 by Carlos Osorio-Ramírez, Associate Professor at Universidad Nacional de Colombia.
- The [Implementation Plan](#) was completed in February 2023. It summarizes how the trigger model is used to trigger anticipatory action and the agreed activation protocol.
- The [Ethical Matrix](#) aims to identify all stakeholders and potential issues regarding the intended use of the model. The Ethical Matrix was completed in May 2023 by Anna Lena Huhn, Southern Africa Regional Anticipatory Action Advisor at the United Nations World Food Programme.

A summary of the main findings and recommendations is provided below.

2.1 Technical Review

Intended Use

Overall, the use cases are well-described and adequately explained. The documentation of the limitations of the model could be extended in its description, as is the case of the biomass anomaly and its connection with scenarios like extreme dryness or late onset.

Model Development and Documentation

It is advisable to provide further documentation on the different data sources used by the team to validate the selection of indicators and estimate the performance of the model. Also, some data is not available in a machine readable format and it would be good to explain how the team dealt with this issue.

Model Evaluation

It is unclear what is an acceptable level of accuracy for the model. The team should better articulate how the performance benchmark was established and how the performance metrics were evaluated and presented to the final stakeholders.

Operational Readiness

It would be good to expand the analysis of the missed activations of the models and the potential false alarms that the model could be providing.

2.2 Ethical Review

False Negatives

A false negative occurs when no drought impact is predicted but drought conditions occur. The team could consider additional mitigation strategies such as the use of citizen science or ground observations to complement the forecast-based trigger.

Insufficient Data

Insufficient data refers to the gaps in impact data used to verify the forecast predictions. Insufficient data might limit the precise prediction of forecasted humanitarian impact and expose local populations to adverse humanitarian impact induced by a drought event, requiring a large-scale humanitarian response ex-post. The team should consider the feasibility of adding further vulnerability layers in future iterations of the model.

False Positives

A false positive happens when drought impact is predicted but no drought conditions occur. Anticipatory action follows the 'no regret' principle, but a false alarm can still lead to inadequate resource allocation with a high potential impact on affected communities. The anticipatory action framework could indicate a precise mitigation strategy in a clearer manner.

Lack of Trust and Ownership

Lack of trust and ownership refers to the limited involvement of local and regional authorities in the model design and validation. This may lead to little ownership and trust put into the model and eventually to political blockages in activations. In future framework versions a clear strategy

for the involvement of affected populations and an approach to accountability to affected populations should be identified.

Lack of Transparency

Lack of transparency refers to the algorithms not being made available or not being transparent. The anticipatory action framework should reflect clearer strategies to engage with local leaders to better understand what is happening on the ground and obtain early buy-in. Mitigation strategy for a potential lack of transparency should be expanded in the model card and/or the anticipatory action framework.

Inaction

Inaction refers to the situation in which drought impact is predicted but no action is taken. Inaction in case of trigger activation is unlikely, given the pre-allocated financing attached to it and the UN-validated anticipatory action framework. Inaction might nevertheless be a possibility, if government or local authorities block the roll-out of interventions on the ground or in case of conflict upsurge. The team could consider adding a consensus-based decision-making option around activation or non-activation in the event of specific events or situational context not considered in the model design (e.g., higher levels of vulnerability or increase in armed conflict, etc.)

Feedback

The Centre invites individuals and organizations working in the humanitarian, academic, research and private sector to engage with us on the peer review process. Please send feedback on the Framework to centrehumdata@un.org.

383.235 Verdict -- Procedure in case of disagreement.

The jurors, after hearing the evidence, shall, by their inquest, say whether the defendants, or either of them, be guilty or not guilty of the forcible entry or detainer complained of; and shall return their inquest, signed by one of their body, to the court. If the jury do not agree, it may be discharged, and another be ordered to be summoned to meet, either immediately or at some future day to be then and there fixed and indorsed on the warrant; and this proceeding shall be continued until a jury agree.

Effective: January 2, 1978

History: Amended 1976 (1st Extra. Sess.) Ky. Acts ch. 14, sec. 315, effective January 2, 1978. -- Transferred 1952 Ky. Acts ch. 84, sec. 1, effective July 1, 1953, from C.C. sec. 459.