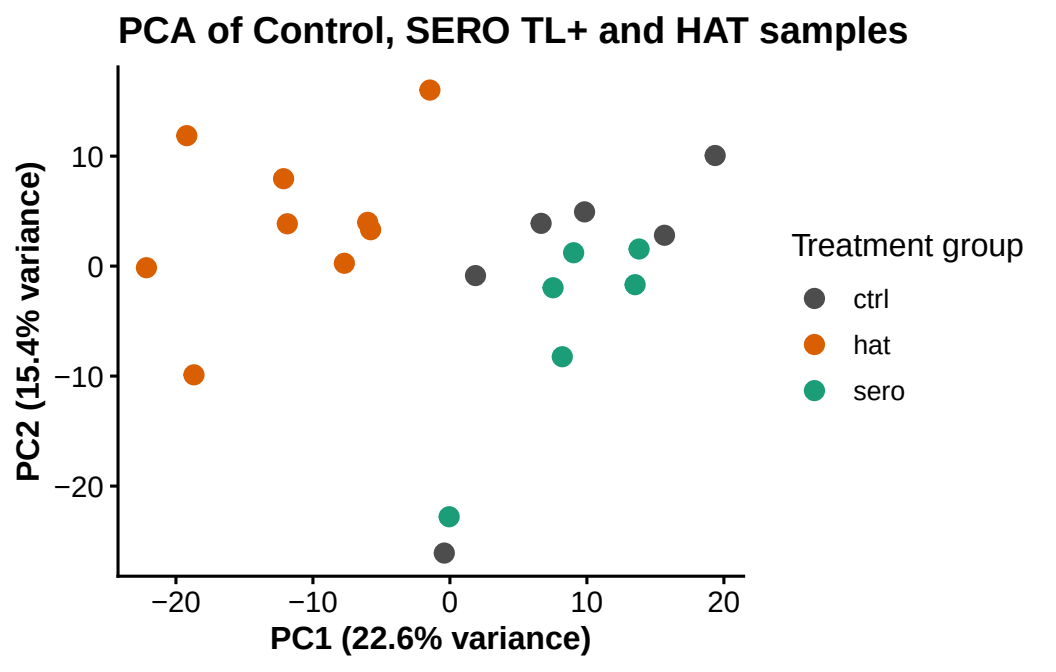
PCA of Control, SERO TL+ and HAT samples
PC2 (15.4% variance)
PC1 (22.6% variance)
10
0
−10
−20
−20
−10
0
10
20
Treatment group
ctrl
hat
sero