
Filename: LibCheck_26R266 - 2026-10-06 - 12.46.57.D5000

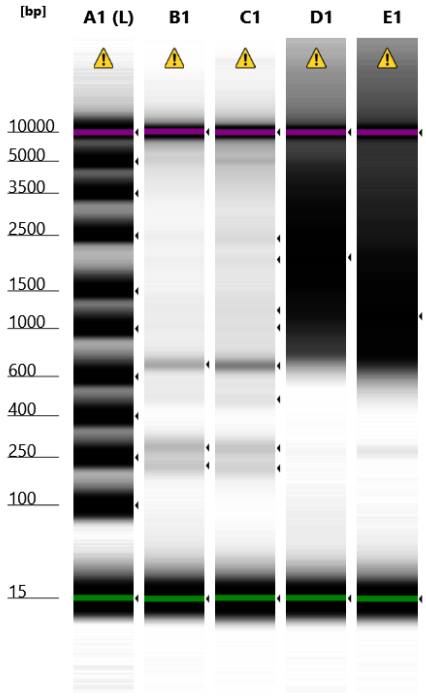


Default image (Contrast 130%)

Sample Info

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
A1	37.8	Ladder	⚠	Caution! Expired ScreenTape device (used after two weeks of first use); Ladder
B1	0.650	26R266 Lib 1 (sample 1 +enrichment)	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)
C1	1.12	26R266 Lib 2 (sample 2 +enrichment)	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)
D1	6.61	26R266 Lib 3 (sample 1)	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)
E1	7.35	26R266 Lib 4 (sample 2)	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)

A1: Ladder

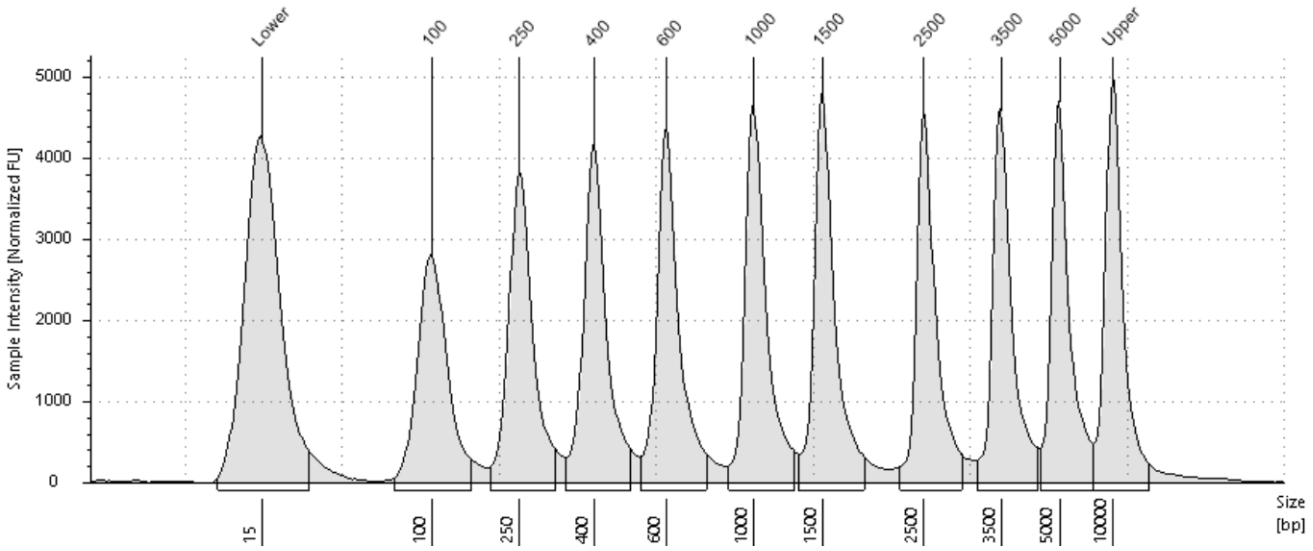


Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
A1	37.8	Ladder	⚠	Caution! Expired ScreenTape device (used after two weeks of first use); Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.16	-	632	-		Lower Marker
100	3.79	-	58.4	10.05		
250	4.21	-	25.9	11.15		
400	4.40	-	16.9	11.65		
600	4.43	-	11.4	11.74		
1000	4.50	-	6.92	11.91		
1500	4.43	-	4.54	11.72		
2500	4.02	-	2.47	10.65		
3500	4.01	-	1.76	10.62		
5000	3.97	-	1.22	10.51		
10000	3.25	3.25	0.500	-		Upper Marker

B1: 26R266 Lib 1 (sample 1 +enrichment)

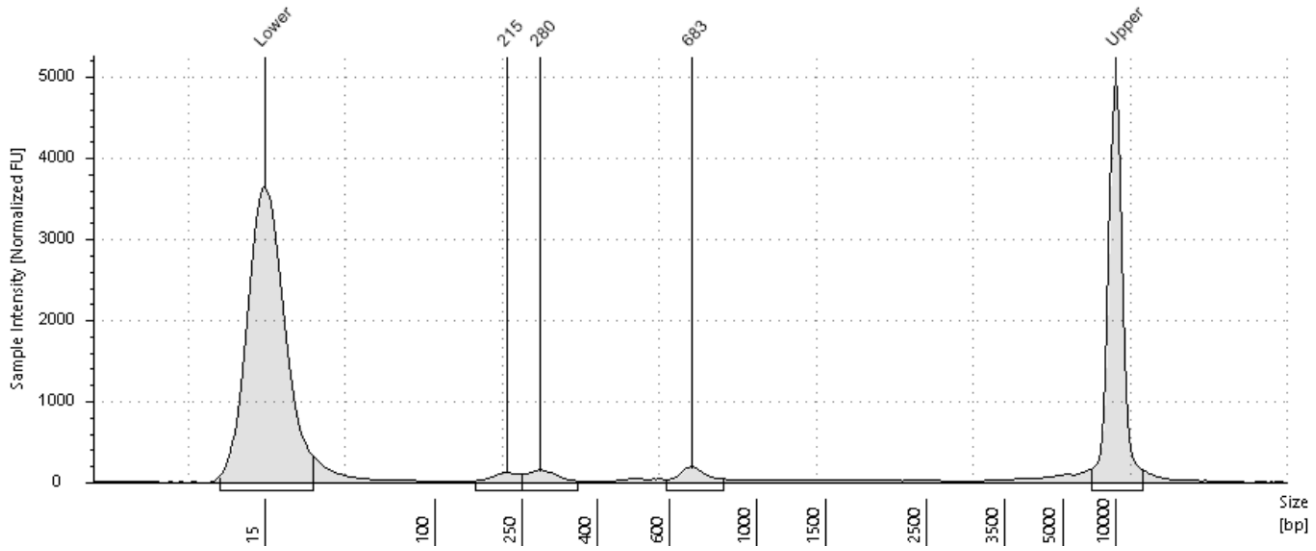


Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
B1	0.650	26R266 Lib 1 (sample 1 +enrichment)	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)

Peak Table


Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.27	-	644	-		Lower Marker
215	0.159	-	1.14	24.54		
280	0.239	-	1.31	36.82		
683	0.251	-	0.565	38.64		
10000	3.25	3.25	0.500	-		Upper Marker

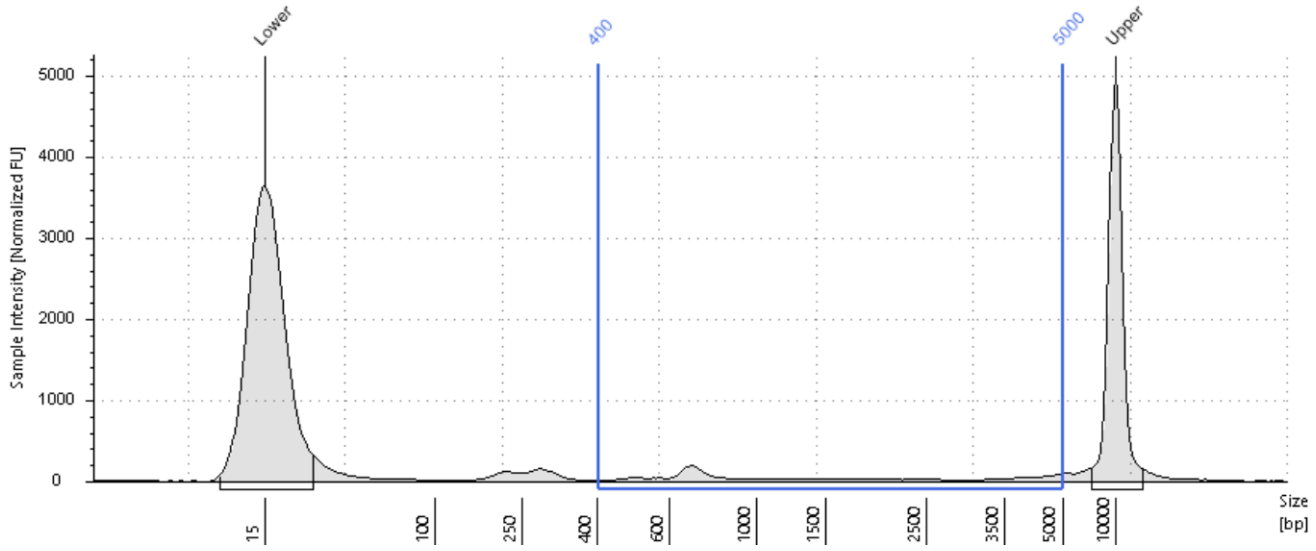

Region Table

From [bp]	To [bp]	Average Size [bp]	Conc. [ng/µl]	Region Molarity [nmol/l]	% of Total	Region Comment	Color
400	5000	1790	0.771	1.21	41.83		

C1: 26R266 Lib 2 (sample 2 +enrichment)

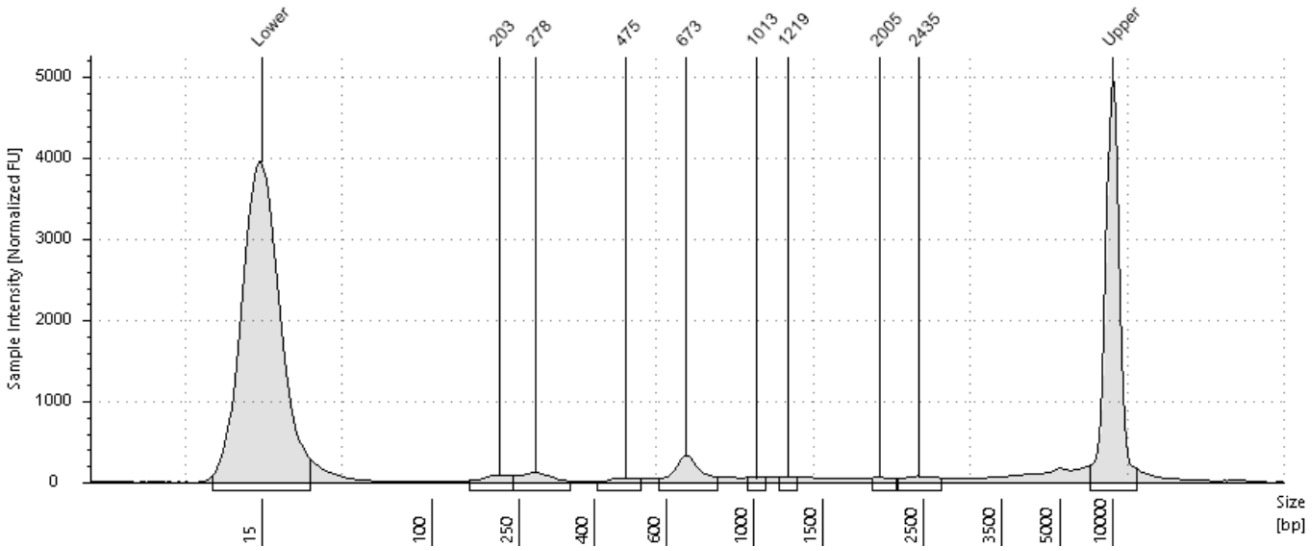


Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
C1	1.12	26R266 Lib 2 (sample 2 +enrichment)	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)

Peak Table


Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.27	-	745	-		Lower Marker
203	0.128	-	0.969	11.40		
278	0.198	-	1.09	17.58		
475	0.0731	-	0.237	6.51		
673	0.429	-	0.980	38.16		
1013	0.0518	-	0.0787	4.61		
1219	0.0546	-	0.0689	4.86		
2005	0.0629	-	0.0482	5.60		
2435	0.127	-	0.0802	11.29		
10000	3.25	3.25	0.500	-		Upper Marker

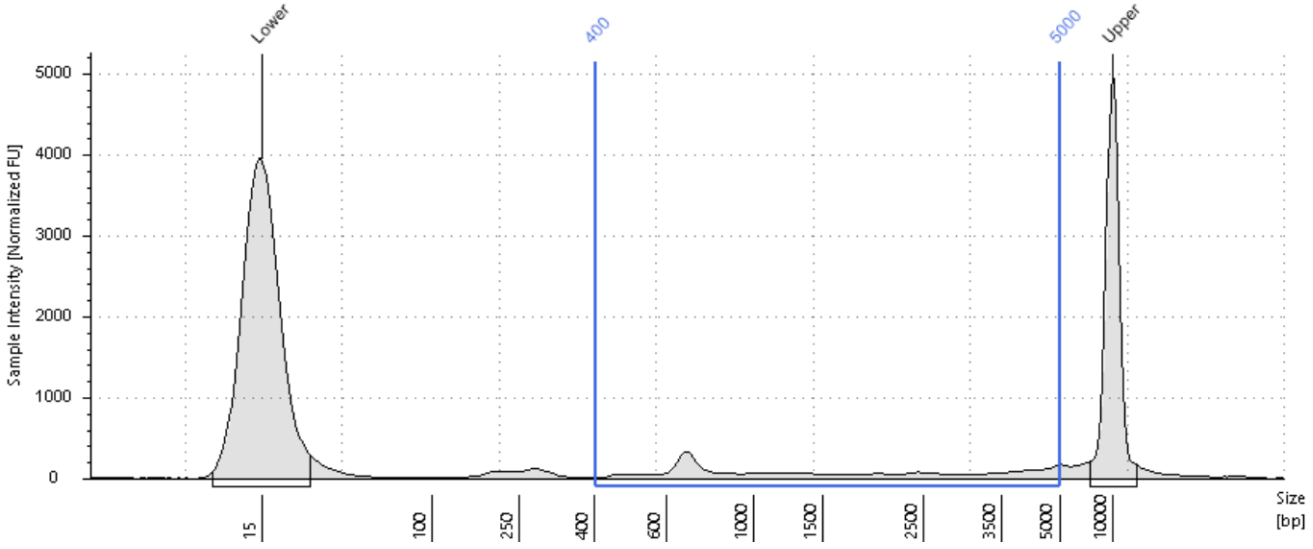

Region Table

From [bp]	To [bp]	Average Size [bp]	Conc. [ng/µl]	Region Molarity [nmol/l]	% of Total	Region Comment	Color
400	5000	1923	1.53	2.14	58.99		

D1: 26R266 Lib 3 (sample 1)

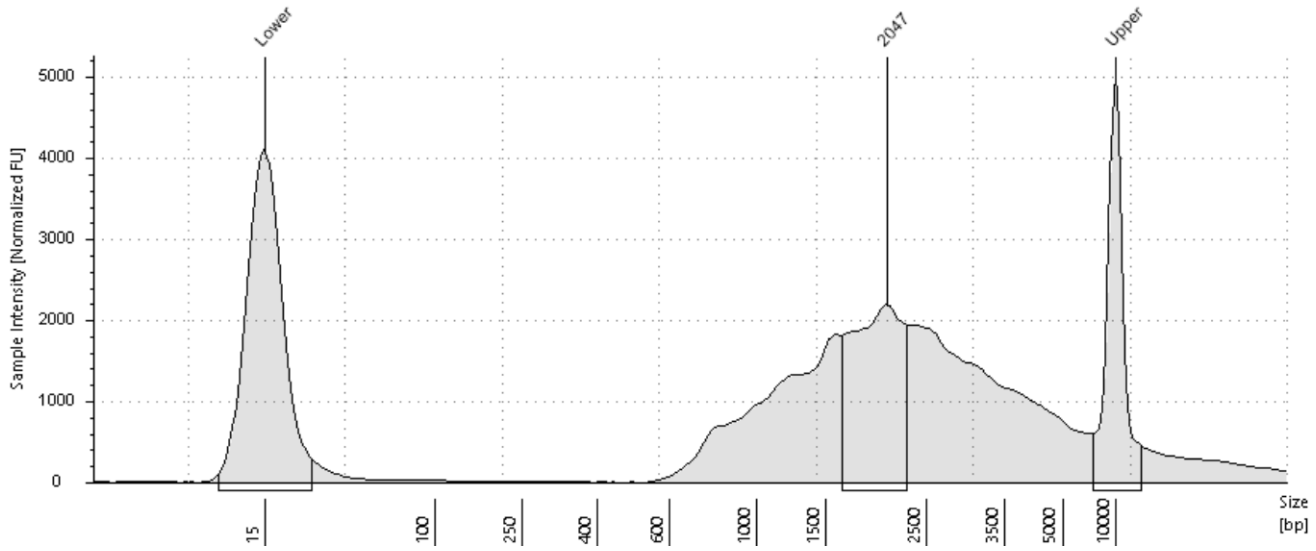


Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
D1	6.61	26R266 Lib 3 (sample 1)	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)

Peak Table


Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.77	-	796	-		Lower Marker
2047	6.61	-	4.97	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

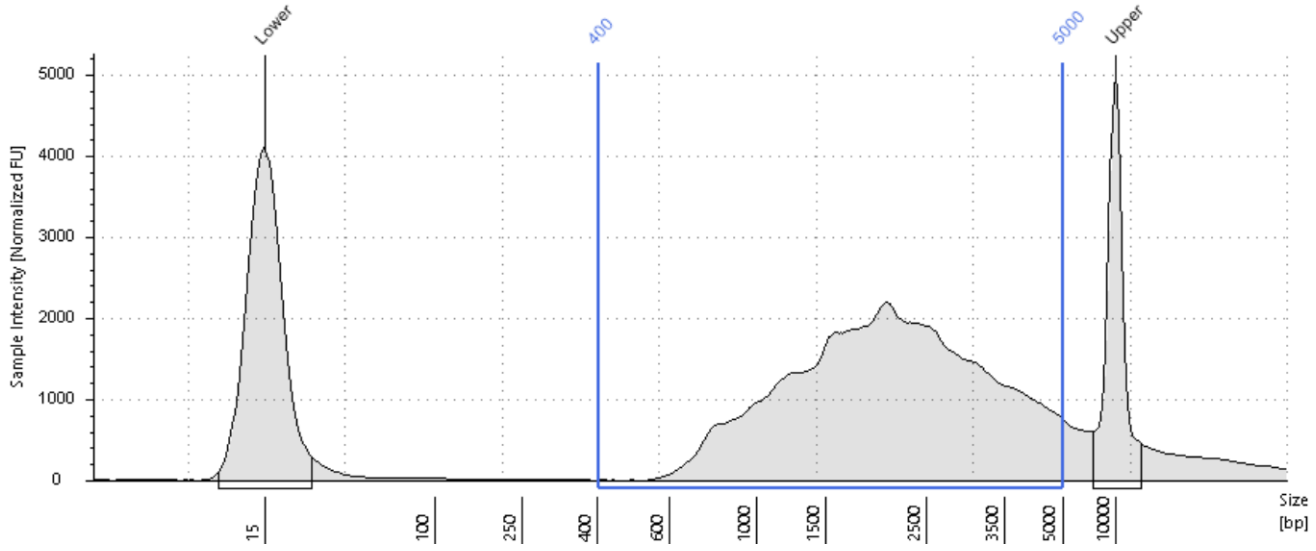

Region Table

From [bp]	To [bp]	Average Size [bp]	Conc. [ng/µl]	Region Molarity [nmol/l]	% of Total	Region Comment	Color
400	5000	2221	25.6	22.2	86.28		

E1: 26R266 Lib 4 (sample 2)

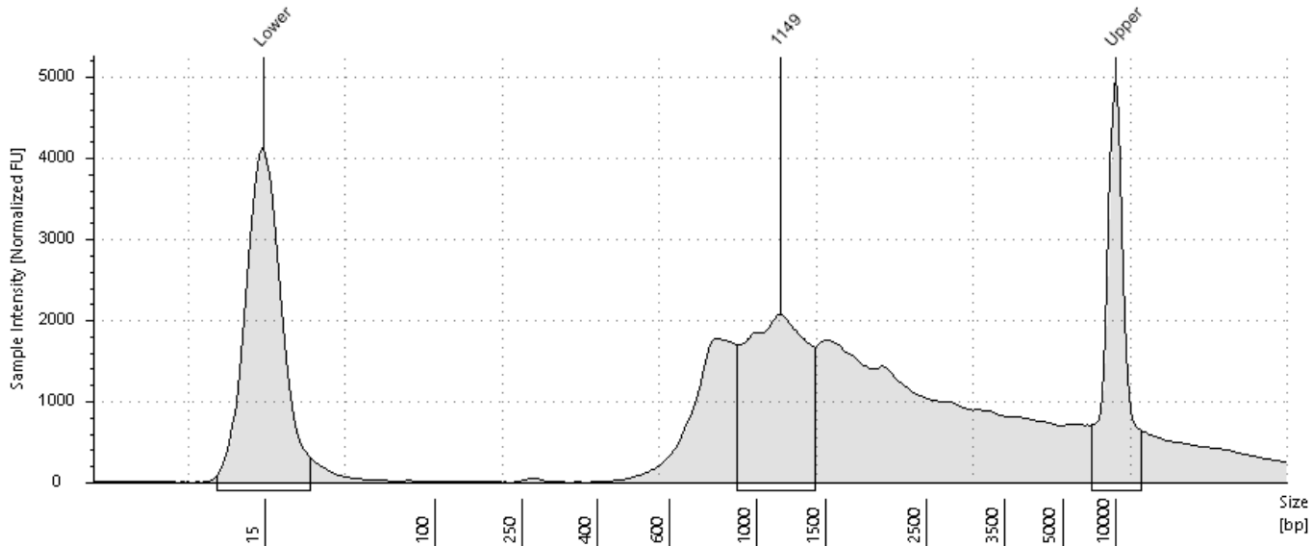


Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
E1	7.35	26R266 Lib 4 (sample 2)	⚠	Caution! Expired ScreenTape device (used after two weeks of first use)

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.47	-	766	-		Lower Marker
1149	7.35	-	9.83	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

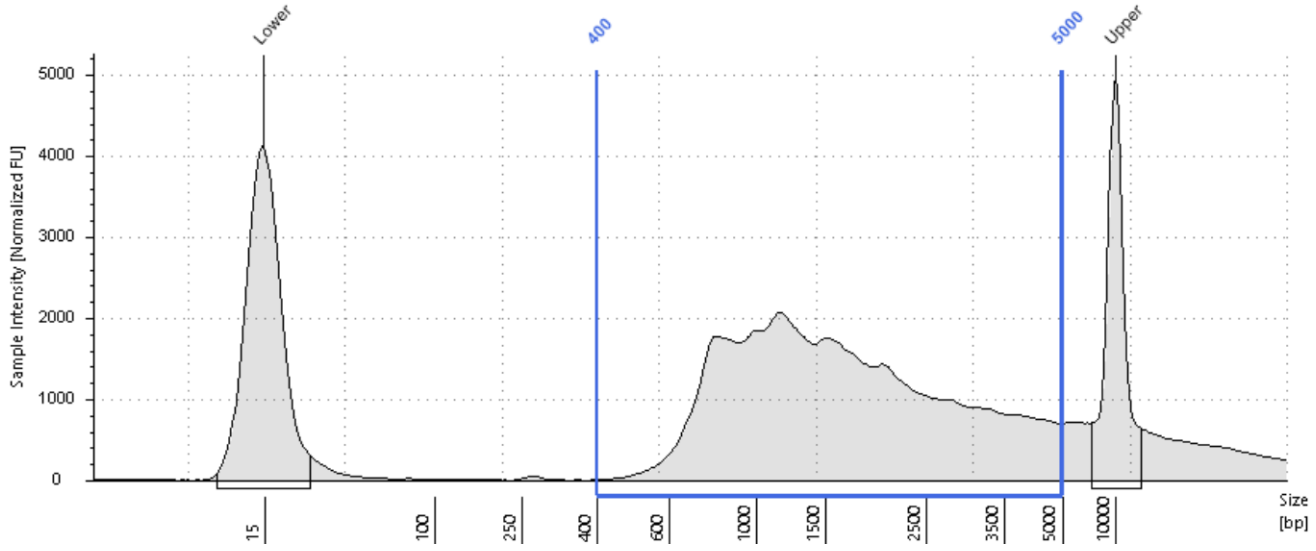

Region Table

From [bp]	To [bp]	Average Size [bp]	Conc. [ng/µl]	Region Molarity [nmol/l]	% of Total	Region Comment	Color
400	5000	1832	25.1	28.3	81.21		