PRESSURE TRANSDUCER CALIBRATION DATA

MICRON INSTRUMENTS

Customer	*Date*
TELEDYNE WEBB	27 FEB 14
Model Number	*Serial Number*
141698-2000A	96645

Diaphragm Materials	*Excitation*	*Pressure Range*	*Excitation Type*
TITANIUM	5 VDC	2000 PSIA	Constant Voltage

Pressure Calibration Data all readings are in mV DC

Date of Pressure Calibration 22 JUL 13

STATIC ERROR BAND ± 0.07% FS BFSL

Pressure	Increase	Decrease	Ideal	Linearity (%FS)	Hysteresis (%FS)
0 PSIA	-1.12	-1.16	-1.12		0.04%
1000 PSIA	50.20	50.09	50.07	0.13%	0.11%
2000 PSIA	101.25		101.25		
SENSITIVITY	102.37				

Thermal Calibration Data all readings are in mV DC

Date of Thermal Calibration 22 JUL 13

	Low Temp.	Ambient	High Temp	Temperature Range	Thermal Balance Shift	Thermal Sensitivity Shift
Temperature	30 °F	75 °F	130 °F			
0 PSIA	-1.15	-1.16	-1.48	30°F to 75°F	-0.01%FS	0.00%FS
2000 PSIA	101.29	101.28	100.48	75°F to 130°F	-0.31%FS	-0.47%FS
Sensitivity	102.44	102.44	101.96	AVERAGE	± 0.002% FS/°F	± 0.002% FS/°F

Notes

DATE OF LAST MEASUREMENT:
10 DEC 13
BALANCE OUTPUT:
-0.76 mV DC

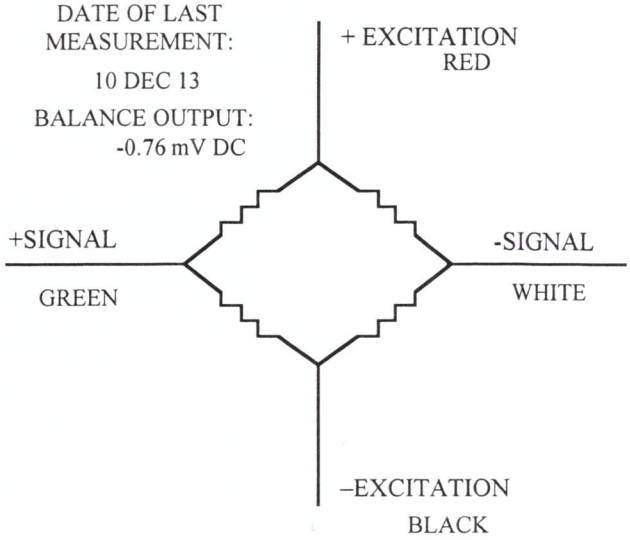

INPUT RESISTANCE 1897 Ohms
OUTPUT RESISTANCE 825 Ohms

Data Entered and Reviewed By	*Date Data Entered*
Dennis Adkinson	29 July 2013

4509 Runway Streeet, Simi Valley, CA 93063 (805) 522-4676 • FAX (805) 522-4982 • e-mail sensors@microninstruments.com 000635