Onyx Research
sales@onyxhealth.net
+44 7404 932 343

DOCUMENT NUMBER	REVISION	DATE OF RELEASE	DISPOSITION
OR-COA-2026-039	**1.0**	**02/09/2026**	**Conforms**

CERTIFICATE OF ANALYSIS

ONYX RESEARCH

01 SAMPLE IDENTIFICATION

Product / Sample	**Onyx Retatrutide 40 mg / 3 mL**	Batch Number	**RE010926C**
Substance	**Retatrutide**	Manufacture Date	**01/09/2026**
Product Form	**Pre-Filled Cartridge**	Retest Date	**01/09/2027**

02 ANALYTICAL RESULTS

NO.	TEST	METHOD	METHOD ID	SPECIFICATION	RESULT	CONFORMITY
01	**Appearance**	Visual examination	TM001.0	Clear liquid	Clear liquid	**Pass**
02	**Identity**	LC-MS	TM002.0	4731.33 ± 0.60 Da	4731.86 Da	**Pass**
03	**Assay**	HPLC-PDA	TM004.1	>13.33 mg/mL >40 mg/3 mL	13.68 mg/mL 41.04 mg/3 mL	**Pass**
04	**Purity**	HPLC-PDA	TM003.2	>98%	98.73%	**Pass**

Results relate only to the sample identified above and to the specifications in force on the date of release.

03 CONCLUSION


The batch conforms to the stated specifications.

The sample was analysed according to validated laboratory procedures.

Onyx Research
sales@onyxhealth.net
+44 7404 932 343


04 CHROMATOGRAPHIC AND SPECTROMETRIC DATA

FIGURE 1 HPLC CHROMATOGRAM

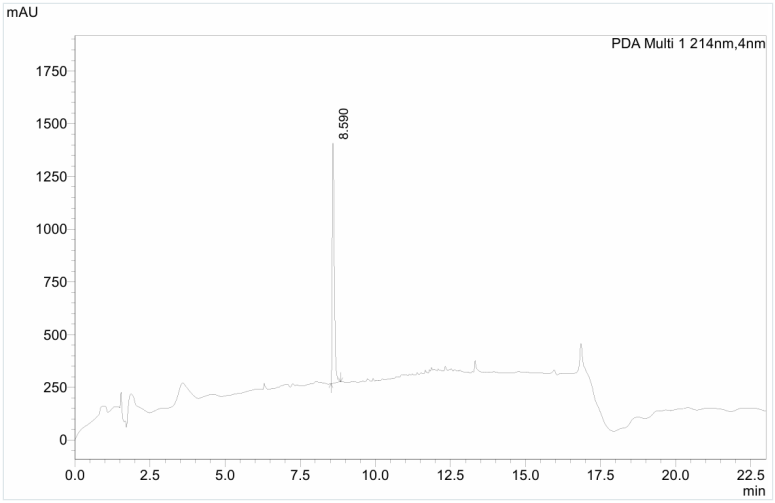

Representative HPLC chromatogram demonstrating the chromatographic profile of the analysed sample.

FIGURE 2 LC-MS SPECTRUM

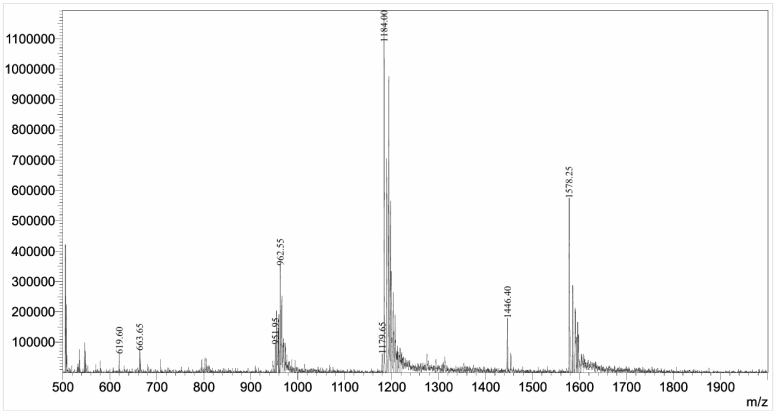

Representative LC-MS spectrum confirming the molecular mass profile of the analysed sample.

Analytical testing was performed by an independent third-party contract laboratory. The full laboratory report for batch RE010926C is retained on file by Onyx Research and is available on request. This Certificate of Analysis applies exclusively to the batch identified above, and the reported results relate solely to the sample submitted for testing. Partial reproduction of this document is prohibited without the prior written authorisation of Onyx Research.

For research use only. Not for human or veterinary use. Not for diagnostic or therapeutic purposes.

END OF CERTIFICATE OR-COA-2026-039