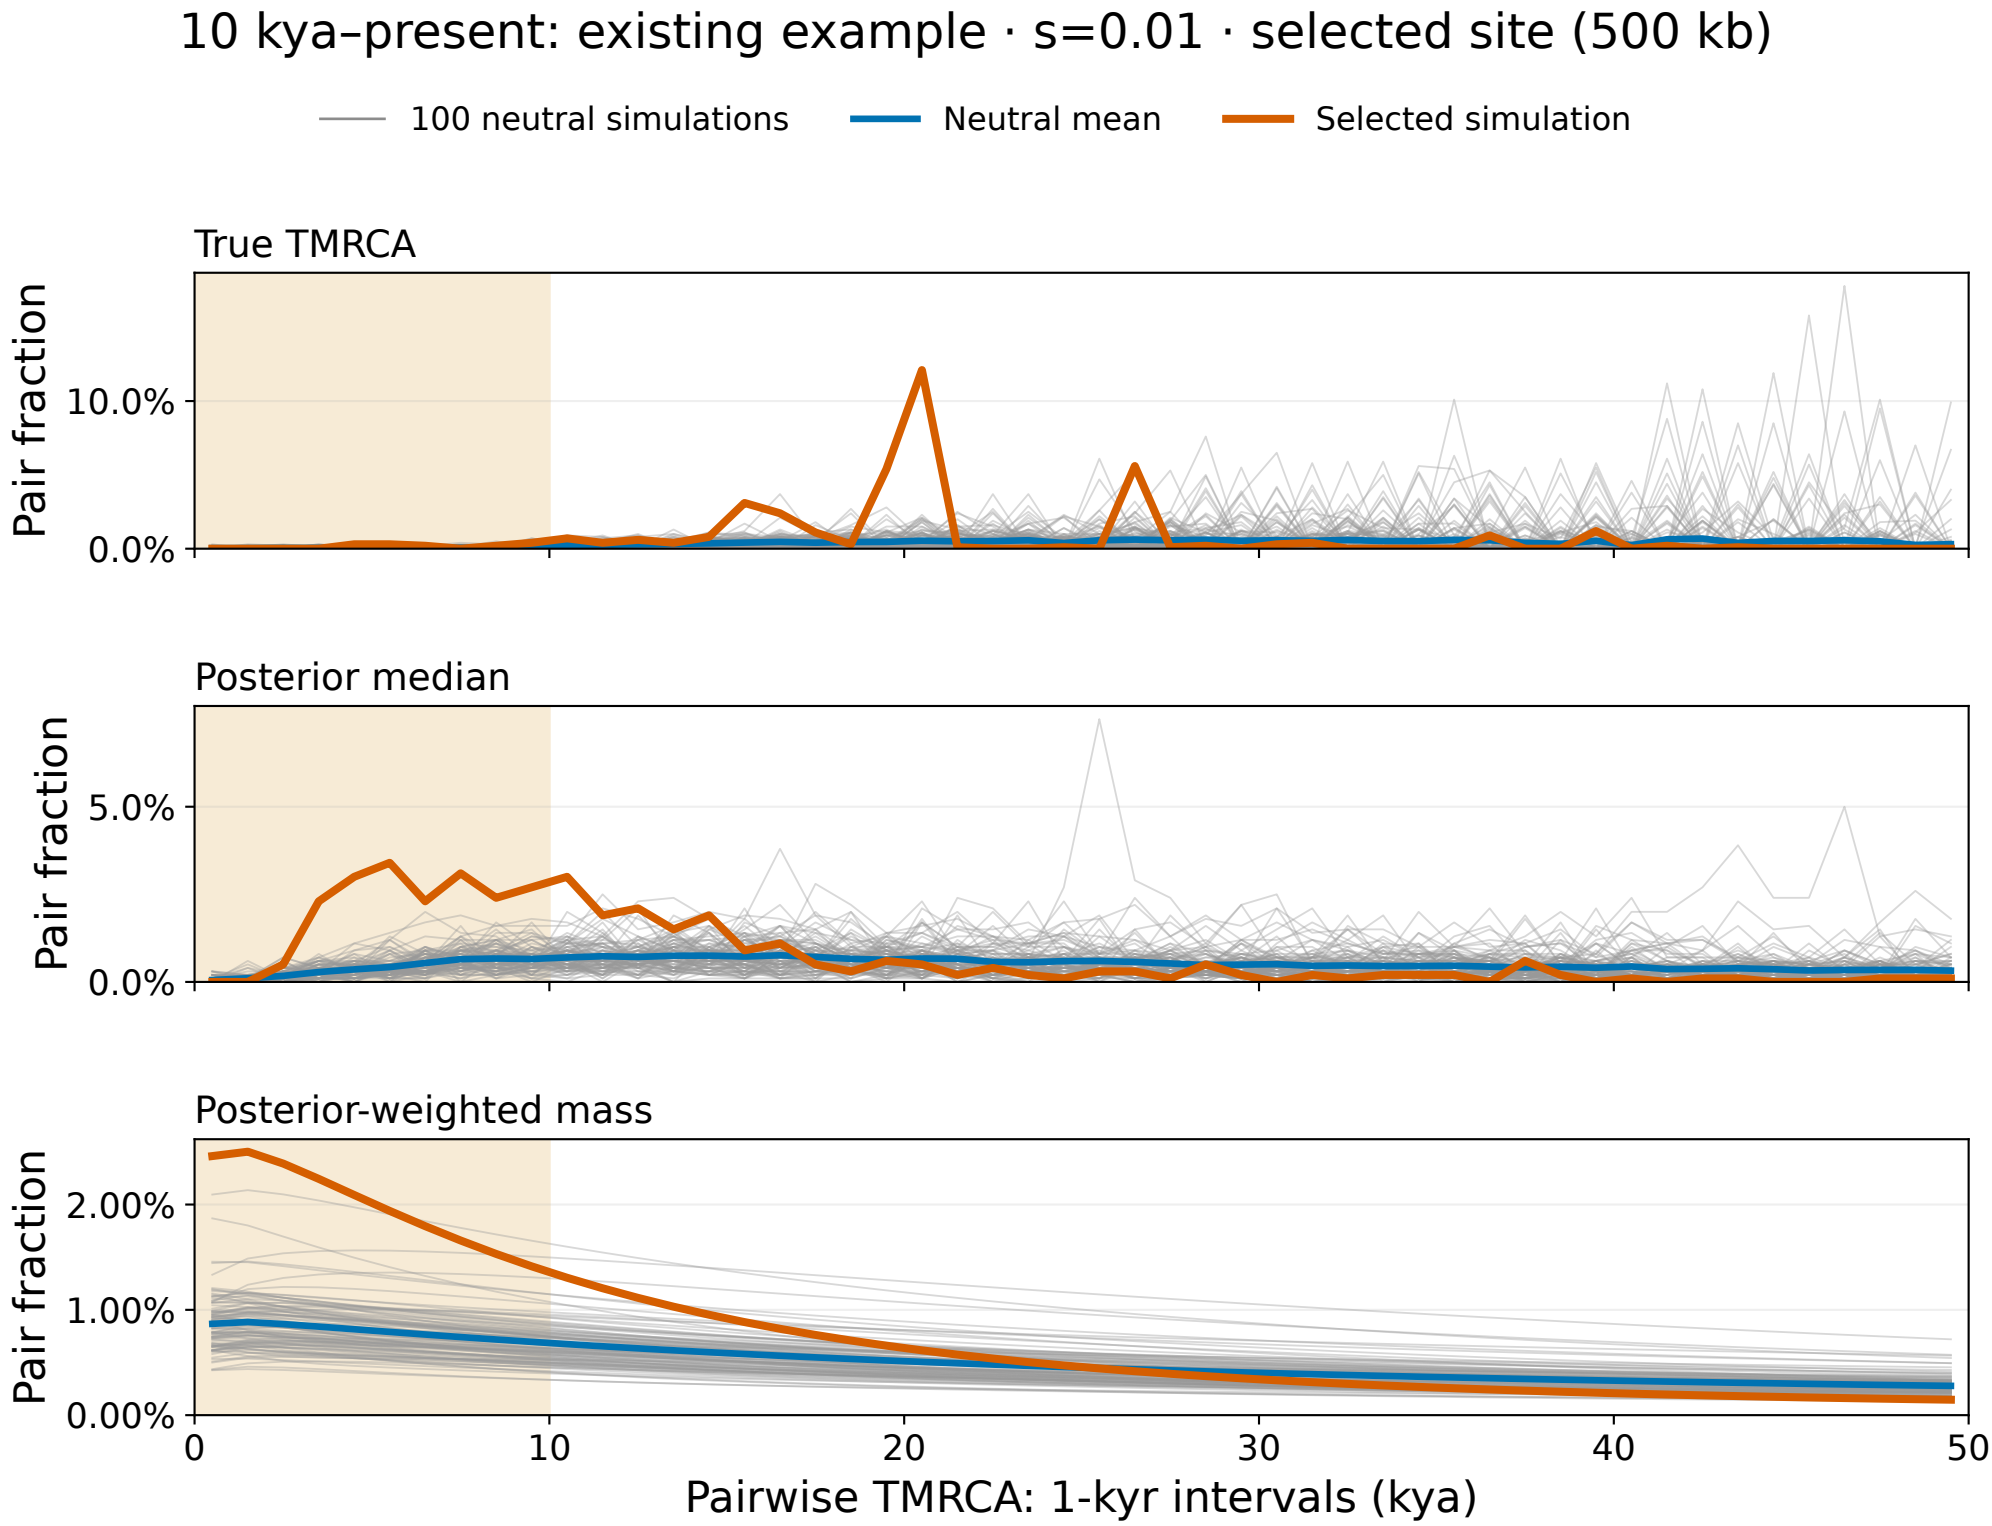


Same 1,000 pairs for all methods · 50 held-out + 50 calibration neutrals · descriptive comparison