



[I-21/36/2026-W&M Section]

GOVERNMENT OF INDIA/भारत सरकार
MINISTRY OF CONSUMER AFFAIRS, FOOD AND PUBLIC DISTRIBUTION
उपभोक्ता मामले, खाद्य एवं सार्वजनिक वितरण मंत्रालय
DEPARTMENT OF CONSUMER AFFAIRS/ उपभोक्ता मामले विभाग
LEGAL METROLOGY DIVISION/ विधिक मापविज्ञान प्रभाग

Krishi Bhawan/कृषि भवन, नई दिल्ली

Dated/दिनांक:- 03.03.2026

Certificate of Approval of Model/ मॉडल का अनुमोदन प्रमाणपत्र

Whereas the Central Government, after considering the report submitted to it by the prescribed authority along with the OIML-CS certificate: R76/1992-DE1-04.04 Revision 3 issued by PTB Germany is satisfied that the model described in the said report (see the figure given below), is in conformity with the provisions of the Legal Metrology Act 2009 (1 of 2010) and the Legal Metrology (Approval of Models) Rules, 2011 and the said model is likely to maintain its accuracy over periods of sustained use and to render accurate service under varied conditions;

Now, therefore, in exercise of the powers conferred by section 22 of the Legal Metrology Act, 2009 (1 of 2010) read with sub-rule (6) of rule 8 and sub-rule (4) of rule 11 of the Legal Metrology (Approval of Models) Rules, 2011, the Central Government hereby issues the certificate of approval of the model of Non Automatic Weighing Instrument of Series: "XS" for accuracy class II and with brand name "METTLER TOLEDO" (hereinafter referred to as the said model), manufactured by M/s Mettler-Toledo AG Im Langacher, 8606 Greifensee, Switzerland and imported & marketed in India without any alteration before or after sale by M/s Mettler-Toledo India Private Limited Amar Hill, Sakhi Vihar Road, Powai. Mumbai 400072 which is assigned the approval mark IND/09/26/ 88 (the picture of the model is given below as Figure 1).

Figure 1



**Technical Data:**

Accuracy Class	II
Temperature range	10°C ...30°C
Max	210 g ... 64100 g
verification scale interval e	0.01g... 1 g
Actual Scale Interval “e”	0.001...1g
number of verification scale intervals n	≤ 81000
Display	LCD
Power Supply	230 V – AC & 12 V Dc
tare-balancing range	≤ 100% of Max

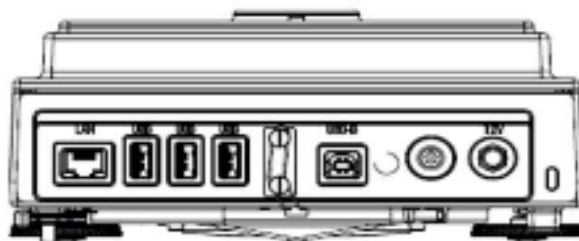


Figure-2

Sealing is done by passing the sealing wire through the holes provided on the body of the machine. A lead seal is put at the end of the wire for stamping purposes (a typical schematic diagram of sealing provision to prevent the fraudulent practice of the model is given above as Figure (2). A dip switch has been provided in the motherboard/PCB to disable access to external calibration.



[F.No.I-21/36/2026-W&M Section]

ASHUTOSH Digitally signed by
AGARWAL ASHUTOSH AGARWAL
Date: 2026.03.03
16:43:41 +05'30'

Director (Legal Metrology) to Govt. of India/ निदेशक (विधिक माप विज्ञान) भारत सरकार
(Ashutosh Agarwal/आशुतोष अग्रवाल)
Phone/दूरभाष 01123389489
Email/ई-मेल: dirwm-ca@nic.in

Online application no. 23580