

- ☐ Analytical
☒ Medical
☐ Testing Machine/Big Range
☐ Balance

TECHNICAL SERVICE REPORT

CUSTOMER NAME: CARAGA REGIONAL HOSPITAL ADDRESS: SURIGAO CITY
SERVICE REQUESTED BY: DEPARTMENT: X-RAY ROOM
EQUIPMENT/MODEL: MOBILEART EVOLUTION MX8v SERIAL NO.: MQ00005F4030

SERVICE CATEGORY

☒ WARRANTY ☐ CHECKUP/REPAIR ☒ PREVENTIVE MAINTENANCE ☐ INSTALLATION ☐ OTHERS

COMPLAINT:**ACTIONS TAKEN****SCHEDULED PREVENTIVE MAINTENANCE UNDER SERVICE CONTRACT - 1ST YEAR, 1ST VISIT**

- Performed test x-ray exposure, unit working normally with no errors encountered
- Checked and cleaned whole unit, charging test: OK
- Checked mechanical movements, applied WD-40 lubricant to moving gears and parts.
- Checked and cleaned x-ray tube & collimator assy
- Checked wire rope, OK
- Checked and cleaned boards & fuses: OK
- Checked 20pcs batteries & CMOS battery: 3.051 OK
- Checked 9 volt batteries, and tested emergency break release button, OK
- Performed x-ray tube calibration (small & large focus): OK
- Performed battery detection & voltage drop: OK
- Verified overall exposure count: 1,423 exposures
- Checked DR system, logs and storage
- Tested x-ray exposure and image acquisition: OK

- Endorsed to end-user

REMARKS/RECOMMENDATIONS

UNIT IN GOOD WORKING CONDITION

SUBMITTED ORIGINAL DOCUMENTS

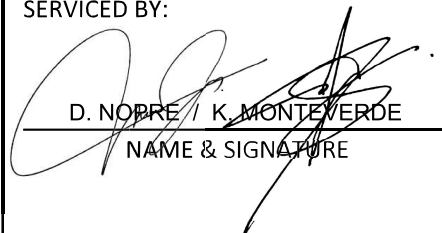
- ☐ STICKER ☐ CALIBRATION CERTIFICATE ☐ PM CERTIFICATE ☐ COMPLETION REPORT
☐ SYSTEM CHECK ☐ IQ DOCUMENTS ☐ OQ DOCUMENTS ☐ PM DOCUMENTS
☐ SERVICE REPORT ☐ CALIBRATION DATA (MEDICAL) ☐ INVOICE/BILLING ☐ DELIVERY RECEIPT

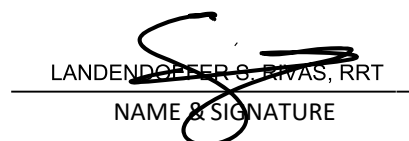
PARTS SUPPLIED/RECOMMENDED

ITEM NO.	PART NUMBER	DESCRIPTION	QTY	DELIVERY RECEIPT

DATE OF SERVICE	TIME STARTED	TIME FINISHED	BILLING STATEMENT
05/12/2026	9:00AM	11:00AM	SALES INVOICE
			PURCHASE ORDER
			AS PER W.

SERVED BY:**ACKNOWLEDGED BY:**


D. NOBRE / K. MONTEVERDE
NAME & SIGNATURE


LANDENDOPFER S. RIVAS, RRT
NAME & SIGNATURE

CONTACT NO:**EMAIL ADD:**

crhradiologyfebruary2021@gmail.com

WHITE: Customer Accounting

PINK: SPC Service Dept

GREEN: Customer End User

YELLOW: SPC Accounting