

TECHNICAL SERVICE REPORT

CUSTOMER NAME: ACEMC-SARIAYA ADDRESS: SARIAYA, QUEZON
SERVICE REQUESTED BY: End-User DEPARTMENT: Cathlab Department
EQUIPMENT/MODEL: TRINIAS UNITY C16 with Hemodynamics SERIAL NO.: M1EFD34D5001

SERVICE CATEGORY

☐ WARRANTY ☐ CHECKUP/REPAIR ☒ PREVENTIVE MAINTENANCE ☐ INSTALLATION ☐ OTHERS

COMPLAINT: FAILED TO DETECT BALL CALIBRATION FOR 3D/CT PROCEDURES

ACTIONS TAKEN

- 1.) CLEANED THE UNIT FROM DUST AND CLEAN THE LARGE MONITOR SCREEN PROTECTOR USING WATER AND CLEAN CLOTH
 - 2.) ADJUSTED ORTHOGONAL POSITION OF THE C-ARM WITH RESPECT TO THE TABLE FOR 3D/CT PROCEDURES.
 - 3.) CHECKED MECHANICAL MOVEMENTS OF THE C-ARM AND TABLE. OK
 - 4.) CHECKED COLLIMATOR CENTERING AND LEAF OPENING. OK
 - 5.) TOP UP COOLING WATER AND COOLANT FOR X-RAY TUBE HEAT EXCHANGER AND FPD COOLER.
 - 6.) PERFORMED X-RAY TUBE FILAMENT CALIBRATION OF LARGE AND SMALL FOCAL SPOT. OK
 - 7.) PERFORMED FPD CALIBRATION FOR GAIN AND OFFSET. OK
 - 8.) PERFORMED 3D/CT CALIBRATION FOR AIR, BALL PHANTOM AND TABLE CALIBRATION. OK
 - 9.) CHECKED 3D ROADMAP FUNCTION OF 3D/CT. OK
 - 10.) TIGHTENED TABLE RAIL BOLTS FOR CONTROLS & MAVIG SKIRT. OK
 - 11.) TOTAL NUMBER OF X-RAY EXPOSURE SINCE INSTALLATION (2023-2026) = 684,024.
- FOR HEMODYNAMICS.

A.) CHECKED ECG WAVEFORM FROM GROUNDING. OK

B.) CHECKED AO PRESSURE OUTPUT. OK

C.) CHECKED SPO2 & NIBP READINGS. OK

NOTE: FOR 100kVA MAIN UPS FOR CATHLAB. MAIN BATTERIES FOR REPLACEMENT. CRITICAL ERRORS ON WINDOWS LOGS SAYS WINDOWS HAS BEEN REBOOTED WITHOUT CLEANLY SHUTTING DOWN. ALREADY 2 Years Past being used

REMARKS/RECOMMENDATIONS

-UNIT IN GOOD WORKING CONDITION . Quotation of batteries of main UPS 100kVA to follow.

-NEXT PMS IS AUGUST 2026

SUBMITTED ORIGINAL DOCUMENTS


☒ STICKER ☐ CALIBRATION CERTIFICATE ☐ PM CERTIFICATE ☐ COMPLETION REPORT
☐ SYSTEM CHECK ☐ IQ DOCUMENTS ☐ OQ DOCUMENTS ☐ PM DOCUMENTS
☒ SERVICE REPORT ☐ CALIBRATION DATA (MEDICAL) ☐ INVOICE/BILLING ☐ DELIVERY RECEIPT

PARTS SUPPLIED/RECOMMENDED

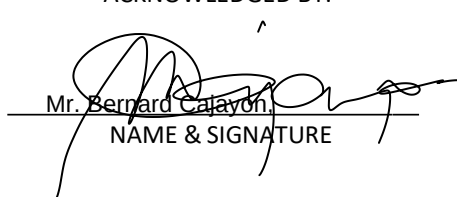
ITEM NO.	PART NUMBER	DESCRIPTION	QTY	DELIVERY RECEIPT
1		BATTERIES FOR 100kVA UPS	1 Set	For Replacement

DATE OF SERVICE	TIME STARTED	TIME FINISHED	BILLING STATEMENT
	8:30AM		SALES INVOICE
MAY 12, 2026	11:00AM	8:00PM	PURCHASE ORDER
			AS PER CONTRACT

SERVED BY:


Engr. Robert Rio / A. Enriquez
NAME & SIGNATURE

ACKNOWLEDGED BY:


Mr. Bernard Calayon
NAME & SIGNATURE

CONTACT NO:

EMAIL ADD: