

- ☐ Analytical
☒ Medical
☐ Testing Machine/Big Range
☐ Balance

TECHNICAL SERVICE REPORT

CUSTOMER NAME: MP ANALYSIS AND LABORATORY INC., ADDRESS: BACOLOD CITY
 SERVICE REQUESTED BY: END-USER DEPARTMENT: RADIOLOGY
 EQUIPMENT/MODEL: EZYRAD PRO MOBILE TRUCK SERIAL NO.: 3M993BC5B002

SERVICE CATEGORY

☐ WARRANTY ☒ CHECKUP/REPAIR ☐ PREVENTIVE MAINTENANCE ☐ INSTALLATION ☐ OTHERS _____ P.O.

COMPLAINT: CONTINUED THE REPAIR OF THE X-RAY MACHINE DUE ERROR F61

ACTIONS TAKEN

-REMOUNTED THE NEW X-RAY TUBE
 -REMOUNTED THE COLLIMATOR
 -CONNECTED THE LOW-VOLTAGE CABLE TO THE TUBE
 -CHECKED OUTLET POWER SUPPLY; 205.4VAC
 -CHECKED AVR OUTPUT; 218.1VAC
 -REGREASED THE HIGH-VOLTAGE CABLES FOR THE ANODE AND CATHODE, THEN CONNECTED THEM TO THE ANODE AND CATHODE TERMINALS OF THE X-RAY TUBE
 -REMOVED THE ORIGINAL INVERTER UNIT-C2 AND INSTALLED THE BRAND-NEW INVERTER UNIT-C2 SENT BY THE OFFICE
 -PERFORMED A TEST EXPOSURE, AND ERROR F61 NO LONGER APPEARED
 -PERFORMED 2 POINTS AND POINT TO POINT CALIBRATION
 -TESTED UNDER NORMAL EXPOSURE AND OBSERVED THAT WHEN THE mAs WAS INCREASED TO 12 mAs, WETHER AT LOW KV OR HIGH KV, A NEW ERROR (F21) APPEARED
 -REMOVED THE ORIGINAL XCONT AND NEX-SH ASSY AND INSTALLED THE BRAND-NEW XCONT AND NEX-SH ASSY BOARDS SENT BY THE OFFICE; -PERFORMED ANOTHER 2 POINT AND POINT TO POINT CALIBRATION
 -PERFORMED ANOTHER TEST UNDER NORMAL EXPOSURE WHERE LOW AND HIGH KV AND 12mAs WERE APPLIED; THE F21 ERROR NO LONGER APPEARED;
 -FURTHER VERIFIED BY INCREASING THE mAs UP TO 30, COMBINED WITH LOW AND HIGH KV; NO F21 ERROR APPEARED

REMARKS/RECOMMENDATIONS

TOMORROW, THE COLLIMATOR WILL BE ALLIGNED WITH RESPECT TO THE CASSETTE STAND / UNIT IS IN WORKING GOOD CONDITION

SUBMITTED ORIGINAL DOCUMENTS

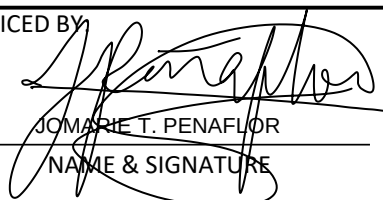
☐ STICKER ☐ CALIBRATION CERTIFICATE ☐ PM CERTIFICATE ☐ COMPLETION REPORT
☐ SYSTEM CHECK ☐ IQ DOCUMENTS ☐ OQ DOCUMENTS ☐ PM DOCUMENTS
☒ SERVICE REPORT ☐ CALIBRATION DATA (MEDICAL) ☐ INVOICE/BILLING ☐ DELIVERY RECEIPT

PARTS SUPPLIED/RECOMMENDED

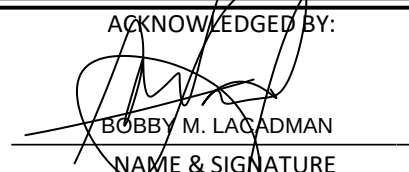
ITEM NO.	PART NUMBER	DESCRIPTION	QTY	DELIVERY RECEIPT

DATE OF SERVICE	TIME STARTED	TIME FINISHED	BILLING STATEMENT
MAY 13, 2026	10:00 A.M	7:50 P.M	SALES INVOICE
			PURCHASE ORDER
			P.O.

SERVICED BY:


 JOMARIE T. PENAFLO
 NAME & SIGNATURE

ACKNOWLEDGED BY:


 BOBBY M. LACADMAN
 NAME & SIGNATURE

CONTACT NO:

1_purchasing2008@hotmail.com/medicalpla;

EMAIL ADD:

robertlacadman1015@gmail.com

WHITE: Customer Accounting

PINK: SPC Service Dept

GREEN: Customer End User

YELLOW: SPC Accounting