

- ☐ Analytical
☒ Medical
☐ Testing Machine/Big Range
☐ Balance

TECHNICAL SERVICE REPORT

CUSTOMER NAME: CARAGA REGIONAL HOSPITAL ADDRESS: SURIGAO CITY
SERVICE REQUESTED BY: DEPARTMENT: RADIOLOGY
EQUIPMENT/MODEL: R/F SYSTEM / FLEXAVISION F4 SERIAL NO.: MQC353CE3003

SERVICE CATEGORY

☒ WARRANTY ☐ CHECKUP/REPAIR ☒ PREVENTIVE MAINTENANCE ☐ INSTALLATION ☐ OTHERS

COMPLAINT:**ACTIONS TAKEN**

SCHEDULED PREVENTIVE MAINTENANCE UNDER WARRANTY - 2ND YEAR, 1ST VISIT

- Performed testing of unit, working and no errors encountered
- Checked and cleaned the unit
- Checked mechanical movements and applied lubricants
- Checked and cleaned generator cabinet, boards and fuses; good
- Checked and cleaned stand and table
- Checked and cleaned CH200M, applied lubricant to bearings and railings
- Checked x-ray tube and collimator assy
- Checked CMOS battery: 3.032
- Checked and cleaned SDR system and cleaned PC
- Checked x-ray tube alignment with respect to stand and table
- Performed x-ray tube calibration for tube 1 and tube 2
- Verified overall exposure count: Tube 1 = 4,156 exposures, Tube 2 = 25,518
- Checked APR settings
- Tested xray exposure and image acquisition
- Addressed other end-user concerns
- Endorsed to end-user

REMARKS/RECOMMENDATIONS

UNIT IN GOOD WORKING CONDITION

SUBMITTED ORIGINAL DOCUMENTS

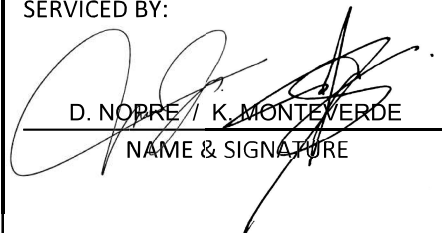
- ☐ STICKER ☐ CALIBRATION CERTIFICATE ☐ PM CERTIFICATE ☐ COMPLETION REPORT
☐ SYSTEM CHECK ☐ IQ DOCUMENTS ☐ OQ DOCUMENTS ☐ PM DOCUMENTS
☐ SERVICE REPORT ☐ CALIBRATION DATA (MEDICAL) ☐ INVOICE/BILLING ☐ DELIVERY RECEIPT

PARTS SUPPLIED/RECOMMENDED

ITEM NO.	PART NUMBER	DESCRIPTION	QTY	DELIVERY RECEIPT

DATE OF SERVICE	TIME STARTED	TIME FINISHED	BILLING STATEMENT
05/11/2026	7:00PM	10:00PM	SALES INVOICE
			PURCHASE ORDER
			AS PER W.

SERVED BY:**ACKNOWLEDGED BY:**


D. NOPRE / K. MONTEVERDE
NAME & SIGNATURE


LANDENDER S. RIVAS, RRT
NAME & SIGNATURE

CONTACT NO:**EMAIL ADD:**

crhradiologyfebruary2021@gmail.com

WHITE: Customer Accounting

PINK: SPC Service Dept

GREEN: Customer End User

YELLOW: SPC Accounting