


Sample-rate and resampling ablation

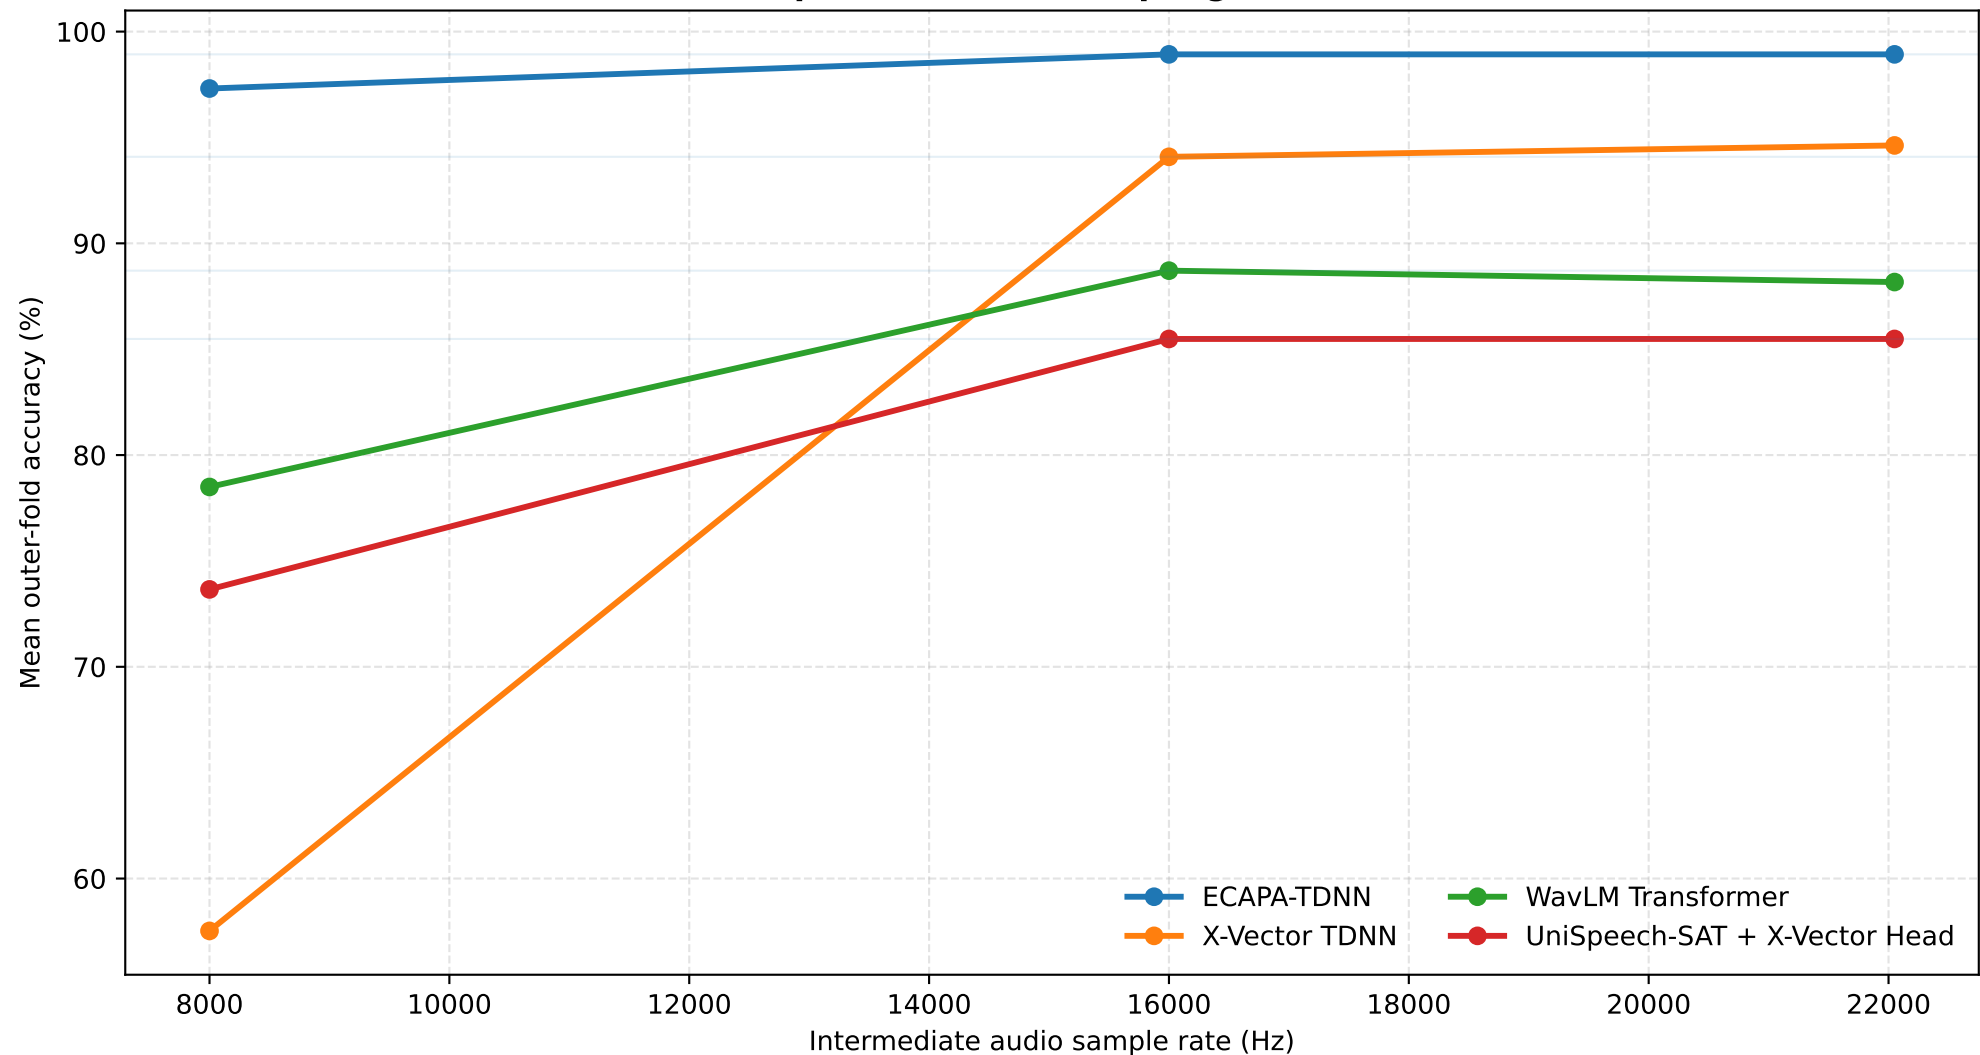

Clean-trained classifier; transformed held-out test clips only. Two correlated outer folds; descriptive comparison.