

Case 1: Bilirubin fractions transferred as same values

Icteric ICU sample: True Total 24.04, Direct- 16.0, Indirect- 8.04 mg/dL; all three committed as 2.2 mg/dL. Intercepted before release.

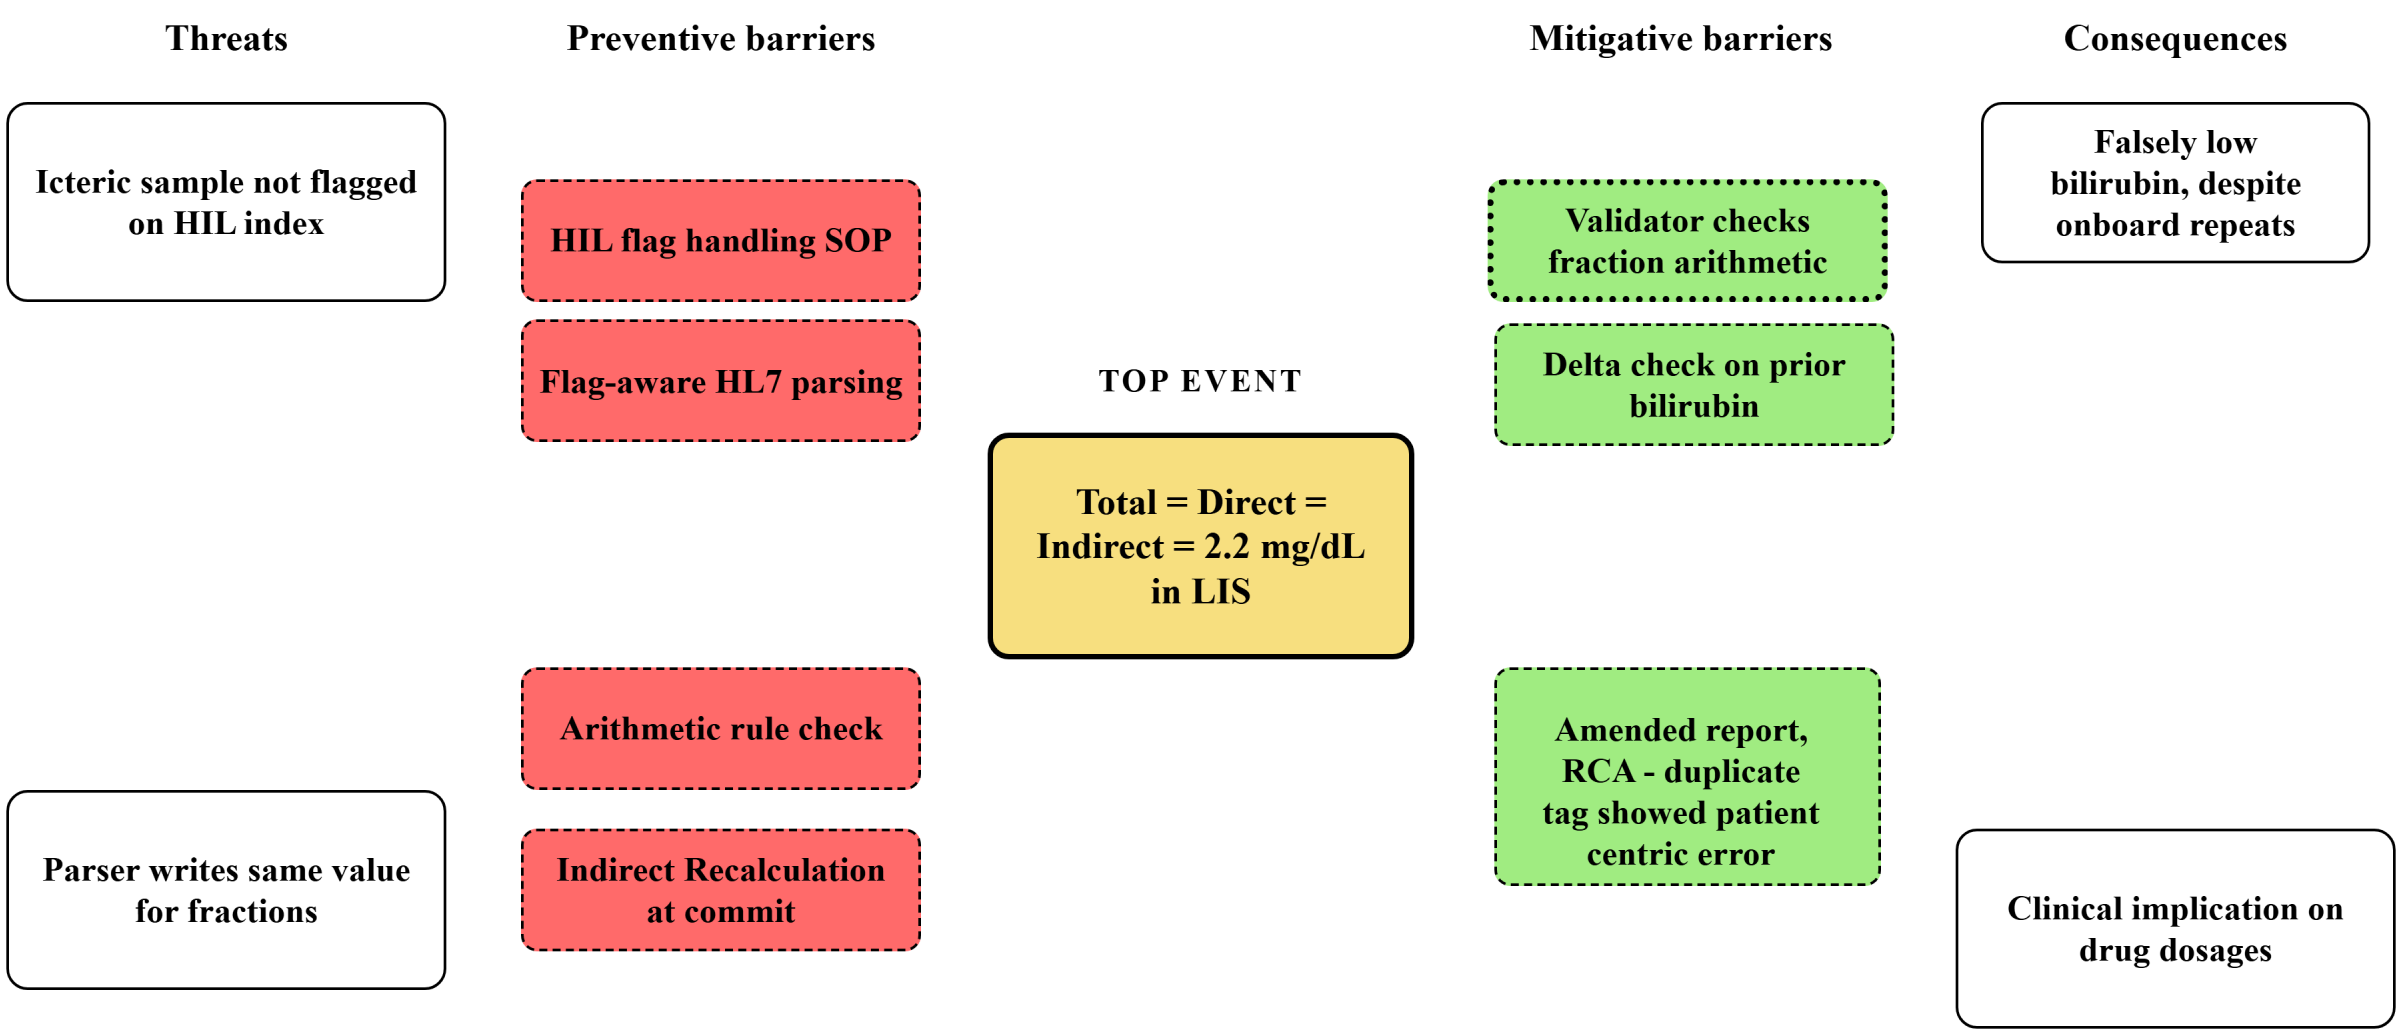

Case 2: Reference intervals reverted after an LIS change

After an LIS configuration event, ranges reverted to obsolete cut-offs, giving wrong H and L flags. Intercepted before release.

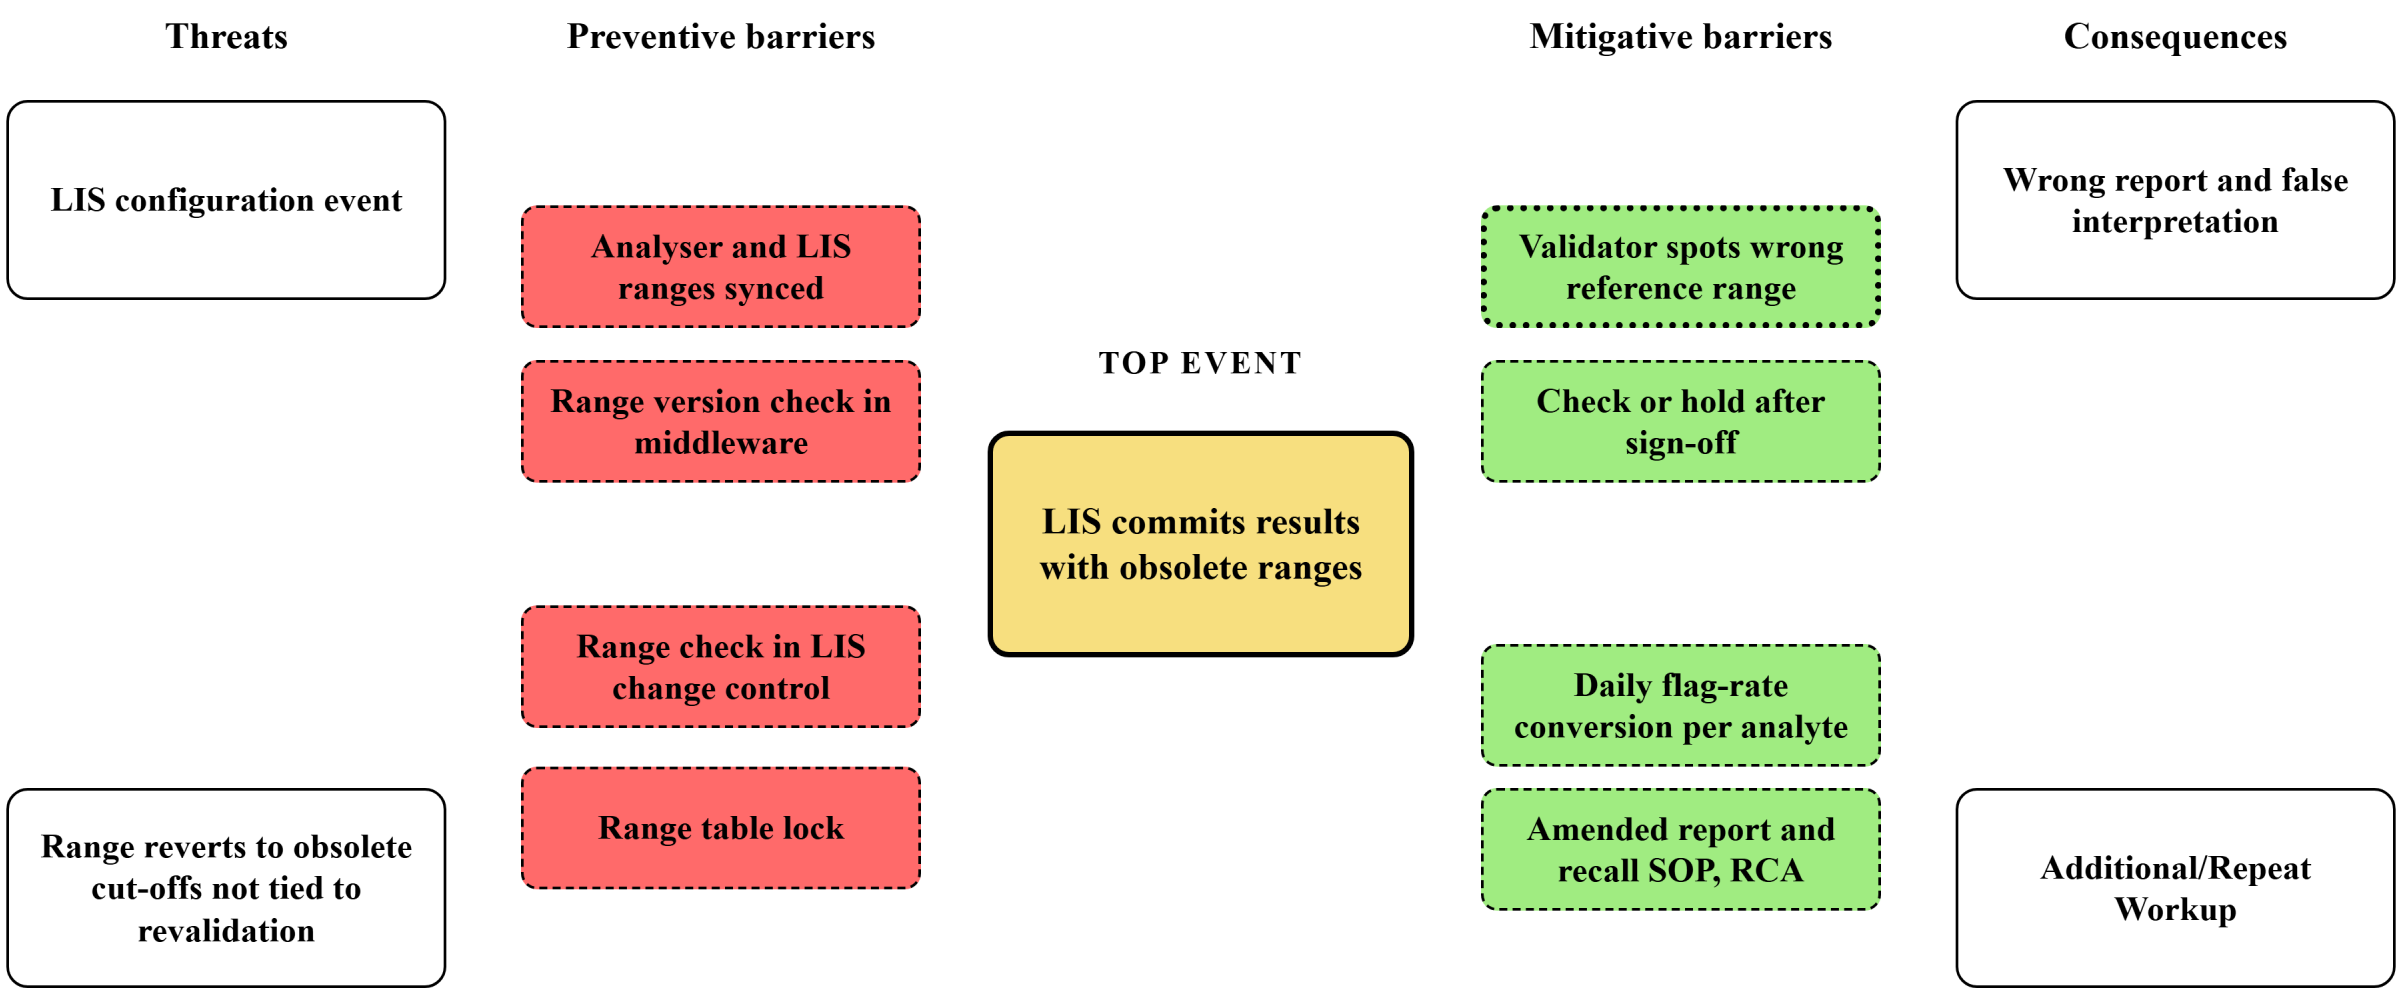

Case 3: AST and ALT committed above linearity

Activity above the measuring range committed as 1000 IU/L without dilution; true value about 1500 IU/L. Intercepted before release.

