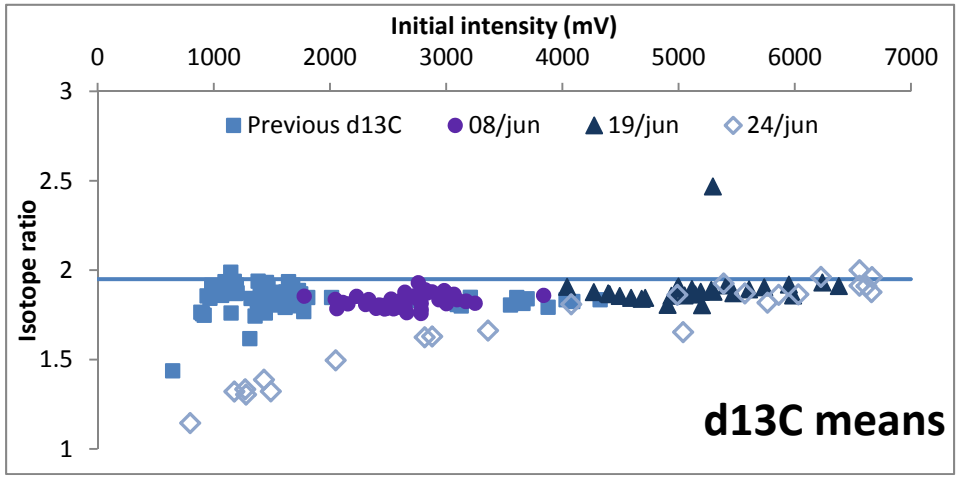
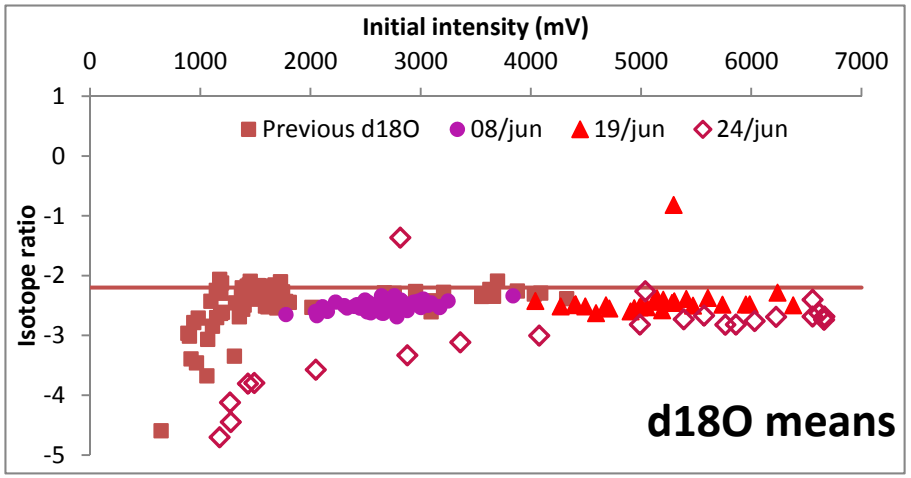




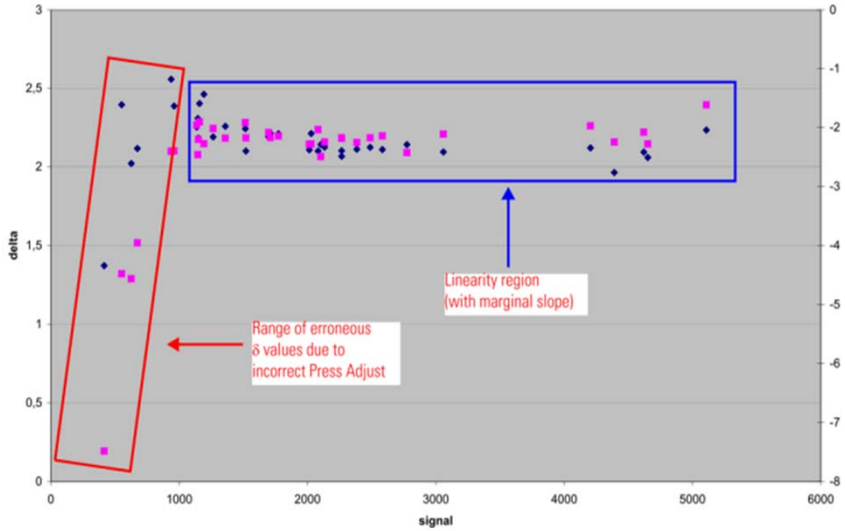


Figure 5-11. δ vs. Signal*

* Both the range of erroneous δ values and the linearity region are general properties, that is they occur in every carbonate measurement (^{13}C and ^{18}O).

Below a certain voltage, usually around 1.5 to 2 V, the δ value drops considerably below the real value. This lower limit of the lower range depends largely on the Press Adjust and Reference Refill parameters.