

# xMAPr - manual

Stephan Michalik

2023-04-04




# Contents

<b>1</b>	<b>Preamble</b>	<b>5</b>
<b>2</b>	<b>Introduction</b>	<b>7</b>
<b>3</b>	<b>Installation</b>	<b>9</b>
3.1	Download xMAPr from GitHub and run locally . . . . .	9
<b>4</b>	<b>xMAPr</b>	<b>11</b>
4.1	xMAPr Analysis . . . . .	11
<b>5</b>	<b>used R-packages for xMAPr</b>	<b>47</b>



# Chapter 1

## Preamble

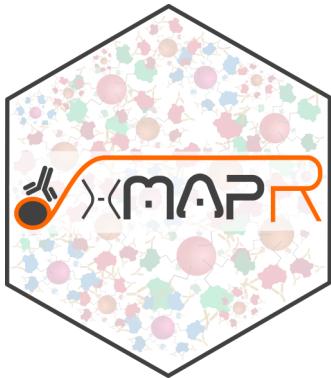

Every human being has a highly specific mixture of antibody specificities in the blood, which reflecting the individual history of interactions with body-foreign substances like virulence factors of pathogens.

The determination of antigen-specific antibody content is a central quantitative measure for diagnostics and vaccine development. The **xMAPr app** was designed to analyze xMAP® technology derived serological assay data measured in serial dilutions (hyper-dynamic-range [HDR] data).

xMAPr was developed under GNU GENERAL PUBLIC LICENSE Version 3.

**You may adjust the font size in your browser by using the zoom in and zoom out functionality of your browser.**

operating system	shortcut	function
MacOS	Cmd & +	<i>zoom in (larger font)</i>
MacOS	Cmd & -	<i>zoom out (smaller font)</i>
Windows	Strg & +	<i>zoom in (larger font)</i>

operating system	shortcut	function
Windows	Strg & -	<i>zoom out (smaller font)</i>

## Chapter 2

# Introduction

Measuring the antibody response to multiple antigens in biofluids can be achieved using the xMAP® technology supplied by Luminex®. For the multiplexing assay all antigens are covalently bound to small paramagnetic particles (MagPlex™) of unique fluorescence dye combination making it possible to distinguish between the mixed spheres in the full assay.

The immune response to some antigens can be extremely strong and extremely weak to others. Thus, the quantitative dynamic range of analysis extends over several orders of magnitude. In a standard measurement, the patient's plasma/serum is diluted 1000-fold and / or 10000-fold. Since this commonly used approach carries the risk of generating quantitative data close to the detection limit when including multiple antigens with a wide variance in the expected antibody responses. This results in error prone data sets making the interpretation of the data very difficult. An advanced approach has been developed to overcome this issue including a serial dilution based measurement of samples granting results derived from the linear range of each antigen.

inspect workflow flow chart

The resulting complex data set could not be analyzed to date. Therefore, an iterative analysis procedure was developed and implemented using the programming language R and the shiny framework resulting the the **xMAPr app**.

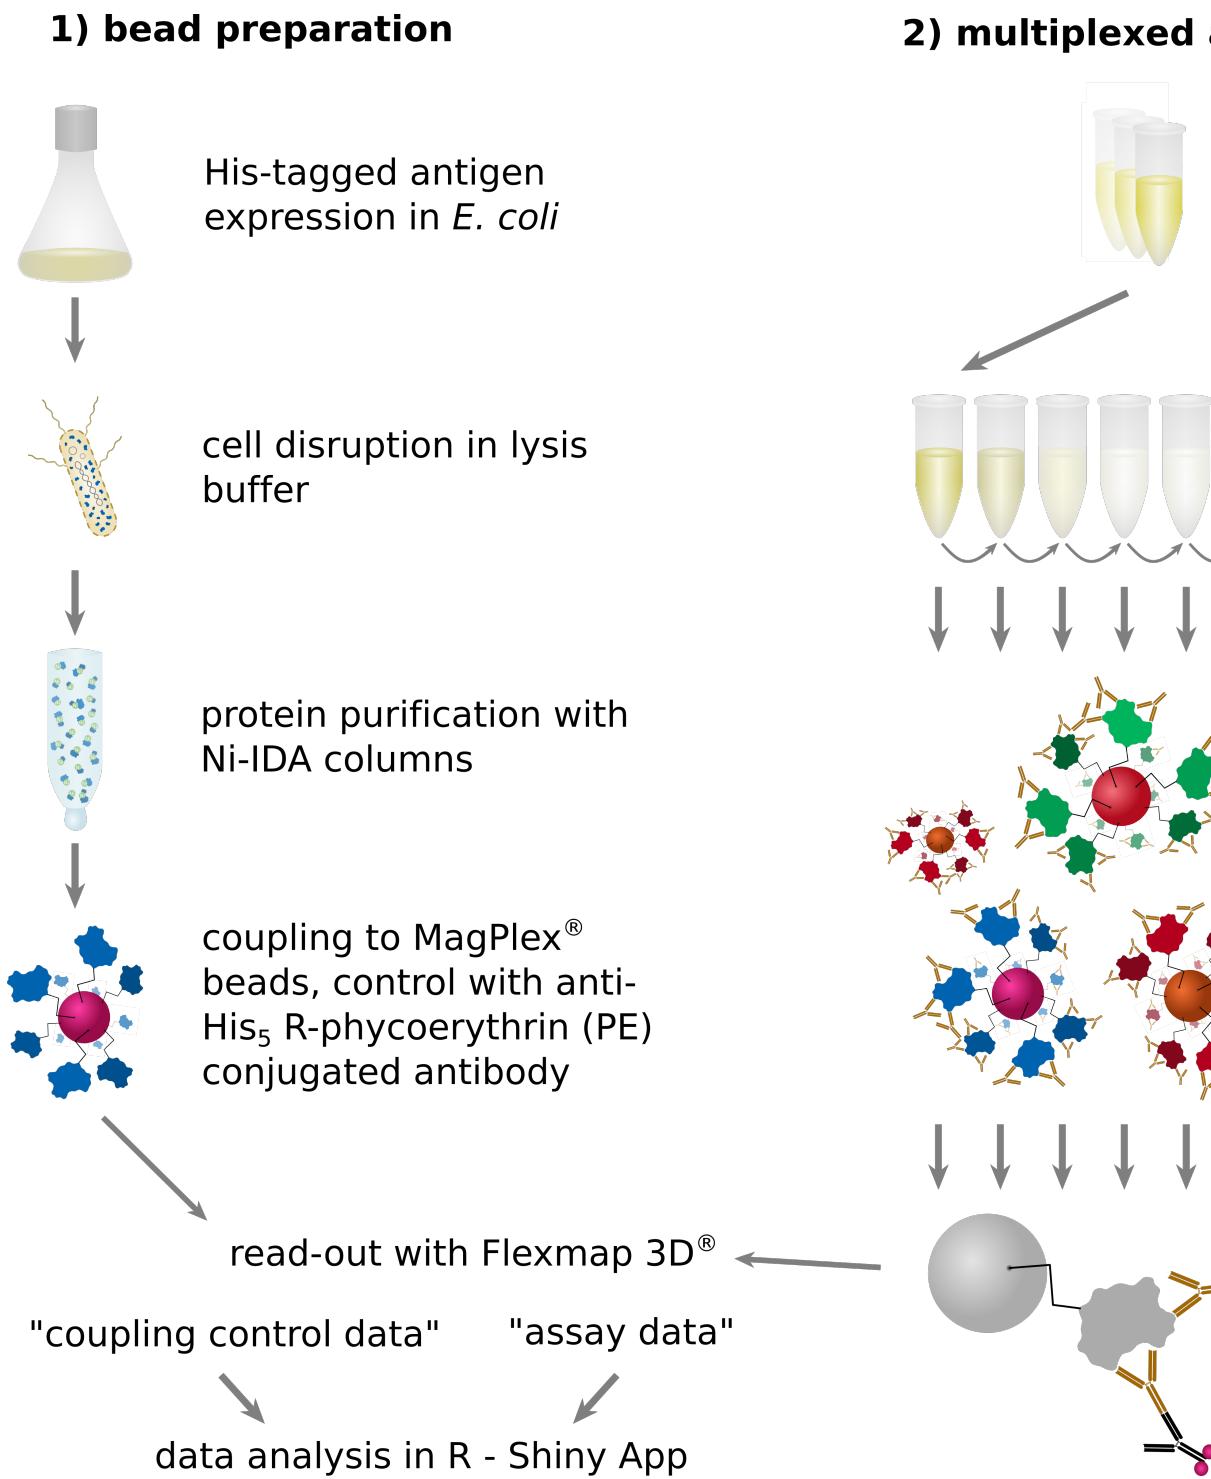


Figure 2.1: serological assay workflow using the xMAP® technology

# Chapter 3

## Installation

### 3.1 Download xMAPr from GitHub and run locally

#### 3.1.1 Requirements

- R (min. version 3.5.1) <https://cran.r-project.org>
- RStudio Desktop (min. version 1.1.414) <https://www.rstudio.com/products/rstudio-desktop/>
- **Windows user MUST install RTools** <https://cran.r-project.org/bin/windows/Rtools/> on C: drive (final path: C:\RTools)

other demanding R packages will be installed on the first startup of the xMAPr app (this might take a while)

#### 3.1.2 Running the app locally<sup>1</sup>

1. download the app from github [https://github.com/stemicha/xMAPr\\_app](https://github.com/stemicha/xMAPr_app) by using the **clone or download** button
2. after extracting the zip file please open the **ui.R** or **server.R** in RStudio
3. select **Run external**
4. press **Run App** to start the app (first run will take a while, due to package installations)

---

<sup>1</sup>xMAPr app perform best with Firefox or Chrome web browser



# Chapter 4

## xMAPr

xMAPr was developed to analyze and visualize data from bead-based experiments performed with the xMAP® technology. The whole basis of the analysis is the utilization of serial dilutions per sample to avoid saturation effects. Figure 4.1 illustrates the mode of operation of xMAPr.

```
[inspect xMA
```

### 4.1 xMAPr Analysis

#### 4.1.1 xPONENT® raw data processing

For the analysis several files are mandatory. After you performed the serological assay including a coupling control the resulting csv-files can be exported using the xPONENT® software from Luminex® (Figure 4.2). The resulting files can be imported into xMAPr, which will automatically generate the correct input files for the analysis.

```
inspect xPonent csv-file export
```

The generated raw input files can be inspected and manipulated after preparation since they are stored as easily accessible txt-files in case of naming errors or removal of specific samples for the later analysis (e.g. included standard wells to monitor the inter-plate reproducibility).

If multiple csv-files should be used for the generation of the xMAPr input files, make sure to store them all in one folder for the upload selection. When all necessary files are selected start processing the data by clicking on the “Run data processing”-button. When processing is done you can download the raw txt-files as a zip-folder by clicking on the green download button.

```
inspect xMAPr xPONENT® raw file processing screenshot
```

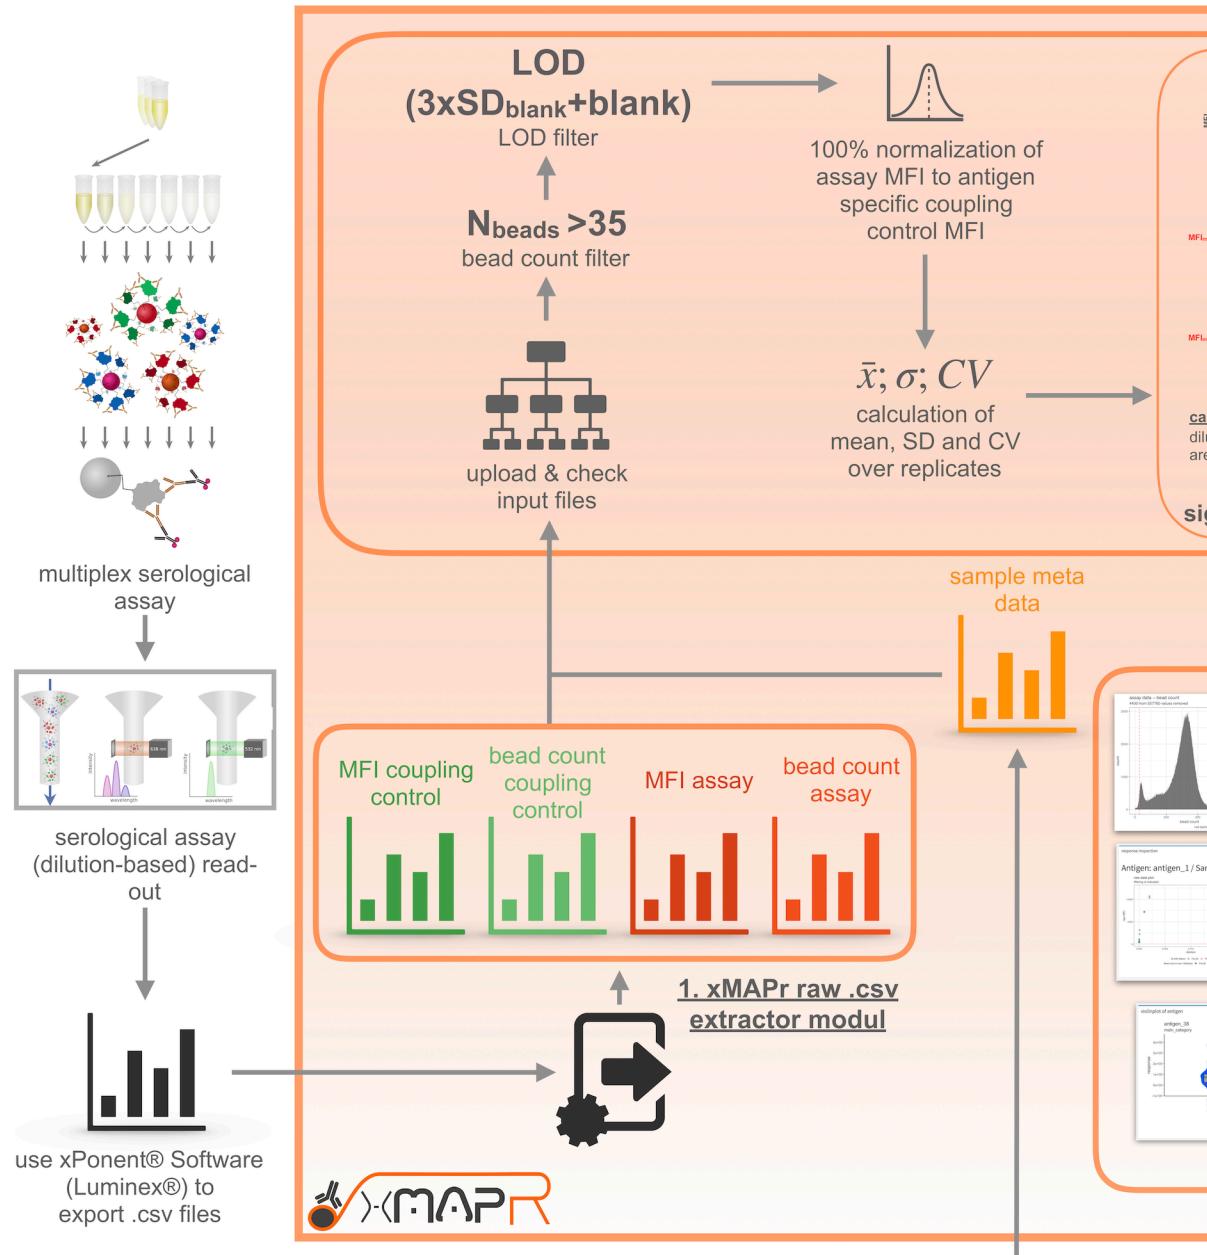


Figure 4.1: xMAPr workflow depicted as flow chart

The screenshot shows the Luminex xPONENT software interface. The top navigation bar includes 'User:' (redacted), 'Log Off', and tabs for Home, Samples, Batches (selected), Results, Protocols, and Tools. The left sidebar has buttons for Current Batch, Saved Batches (selected), LIS Results, and Reports. The main content area displays 'Saved Batches' with instructions to select a batch for details, export, approve, or replay. It features a 'Filter' button, a status indicator 'Filter is OFF', and a 'Clear' button. Below this is a table titled 'Completed Batches' listing 14 entries. The table columns are Name, Protocol, Protocol Version, Date, and Status. The last entry in the table is partially cut off. At the bottom is a toolbar with buttons for Reacquire, Save Prtcl, Plate Layout, Approve, Exp Results (highlighted with a red arrow), and Import.

Name	Protocol	Protocol Version	Date	Status
180402_TM_pools_I...	TM_SHIP_2_IgA	1	4/2/2018 2:43 PM	Compl
180402_TM_pools_I...	TM_SHIP_2_IgA	1	4/2/2018 1:19 PM	Compl
180402_TM_pools_I...	TM_SHIP_2_IgA	1	4/2/2018 11:55 AM	Compl
180329_TM_pools_I...	TM_SHIP_2_IgA	1	3/29/2018 5:38 PM	Compl
180329_TM_pools_I...	TM_SHIP_2_IgA	1	3/29/2018 4:16 PM	Compl
180329_TM_pools_I...	TM_SHIP_2_IgA	1	3/29/2018 2:54 PM	Compl
180329_TM_pools_I...	TM_SHIP_2_IgA	1	3/29/2018 1:32 PM	Compl
180329_TM_pools_I...	TM_SHIP_2_IgA	1	3/29/2018 12:10 PM	Compl
180329_TM_pools_I...	TM_SHIP_2_IgA	1	3/29/2018 10:48 AM	Compl
180328_TM_pools_I...	TM_SHIP_2_IgA	1	3/28/2018 5:45 PM	Compl
180328_TM_pools_I...	TM_SHIP_2_IgA	1	3/28/2018 4:24 PM	Compl
180328_TM_pools_I...	TM_SHIP_2_IgA	1	3/28/2018 3:01 PM	Compl
180328_TM_pools_I...	TM_SHIP_2_IgA	1	3/28/2018 1:39 PM	Compl

Figure 4.2: xPONENT csv-file export

**xPonent raw file input**

**set name for processed output**  
raw\_processed\_output

**Sample column separator for assay RAW xPonent csv input files**  
?

- pipe
- underscore
- dash

example: Sample1\_1\_10000 = Sample > Replicate > Xfold Dilution (Separator = \_)

**assay data**

**Upload assay raw CSVs here**

Browse... 4 files  
Upload complete

**coupling control data**

**Upload coupling control raw CSVs here**

Browse... 180402\_TM\_pools  
Upload complete

**download processed data:**

**download processed raw data**

zipped folder is ready for download

**converted data frames**

	Sample	Replicate	Dilution	Analyte
1	IgGt-EB01	1	50	77269
2	IgGt-EB01	1	200	61203
3	IgGt-EB01	1	800	47431.5
4	IgGt-EB01	1	3200	31971
5	IgGt-EB01	1	12800	16304.5
6	IgGt-EB01	1	51200	6561
7	IgGt-EB01	1	204800	1485.5
8	IgGt-Blank	1		51
9	IgGt-AD01	1	50	61317.5
10	IgGt-AD01	1	200	34915
11	IgGt-AD01	1	800	16218.5
12	IgGt-AD01	1	3200	5938
13	IgGt-AD01	1	12800	3411
14	IgGt-AD01	1	51200	828
15	IgGt-AD01	1	204800	244.5
16	IgGt-Blank	2		49
17	IgGt-CF01	1	50	90071
18	IgGt-CF01	1	200	65881.5

Showing 1 to 18 of 344 entries

Figure 4.3: xMAPr xPONENT® raw file processing screenshot

### 4.1.2 xMAPr analysis pipeline

the resulting files from the raw file processing step are mandatory for the analysis with xMAPr:

1. assay MFI file
2. assay bead count file
3. coupling control MFI file
4. coupling control bead count file
5. sample meta data (additional file, which provides all the sample meta data !)

In addition to the above mentioned files several parameters can be set (figure 4.4).

inspect xMAPr analysis pipeline screenshot

If a naming parameter does not fit the input data frames the pipeline will detect that and will report the error in a pop-up error message.

#### What will be checked?

- is the used dilution name found in assay data header
- is the used dilution name found in assay bead count data header
- is the used dilution name found in assay data header
- is the used replicate name found in assay bead count data header
- is the used sample name found in assay data header
- is the used sample name found in assay bead count data header
- is the used sample name found in meta data header
- is the used blank name found in assay data first column
- is the used blank name found in assay bead count data first column
- is the used antiTag name found in coupling control data first column
- is the used antiTag name found in coupling control bead count data first column
- is the used blank name found in coupling control data first column
- is the used blank name found in coupling control bead count data first column
- do assay data and control coupling data share the same number of antigens or antigens and do they have the same order
- do assay bead count data and control coupling bead count data share the same number of antigens and do they have the same order
- do control coupling bead count data and control coupling data share the same number of antigens or antigens and do they have the same order
- is the used number of dilutions below 5 (min. 5 different dilutions required !)

In the first instance of the pipeline, the data are corrected for their measurement background, bead count and normalized to their respective coupling efficiency. This is followed by the process of sequential multiple regression.

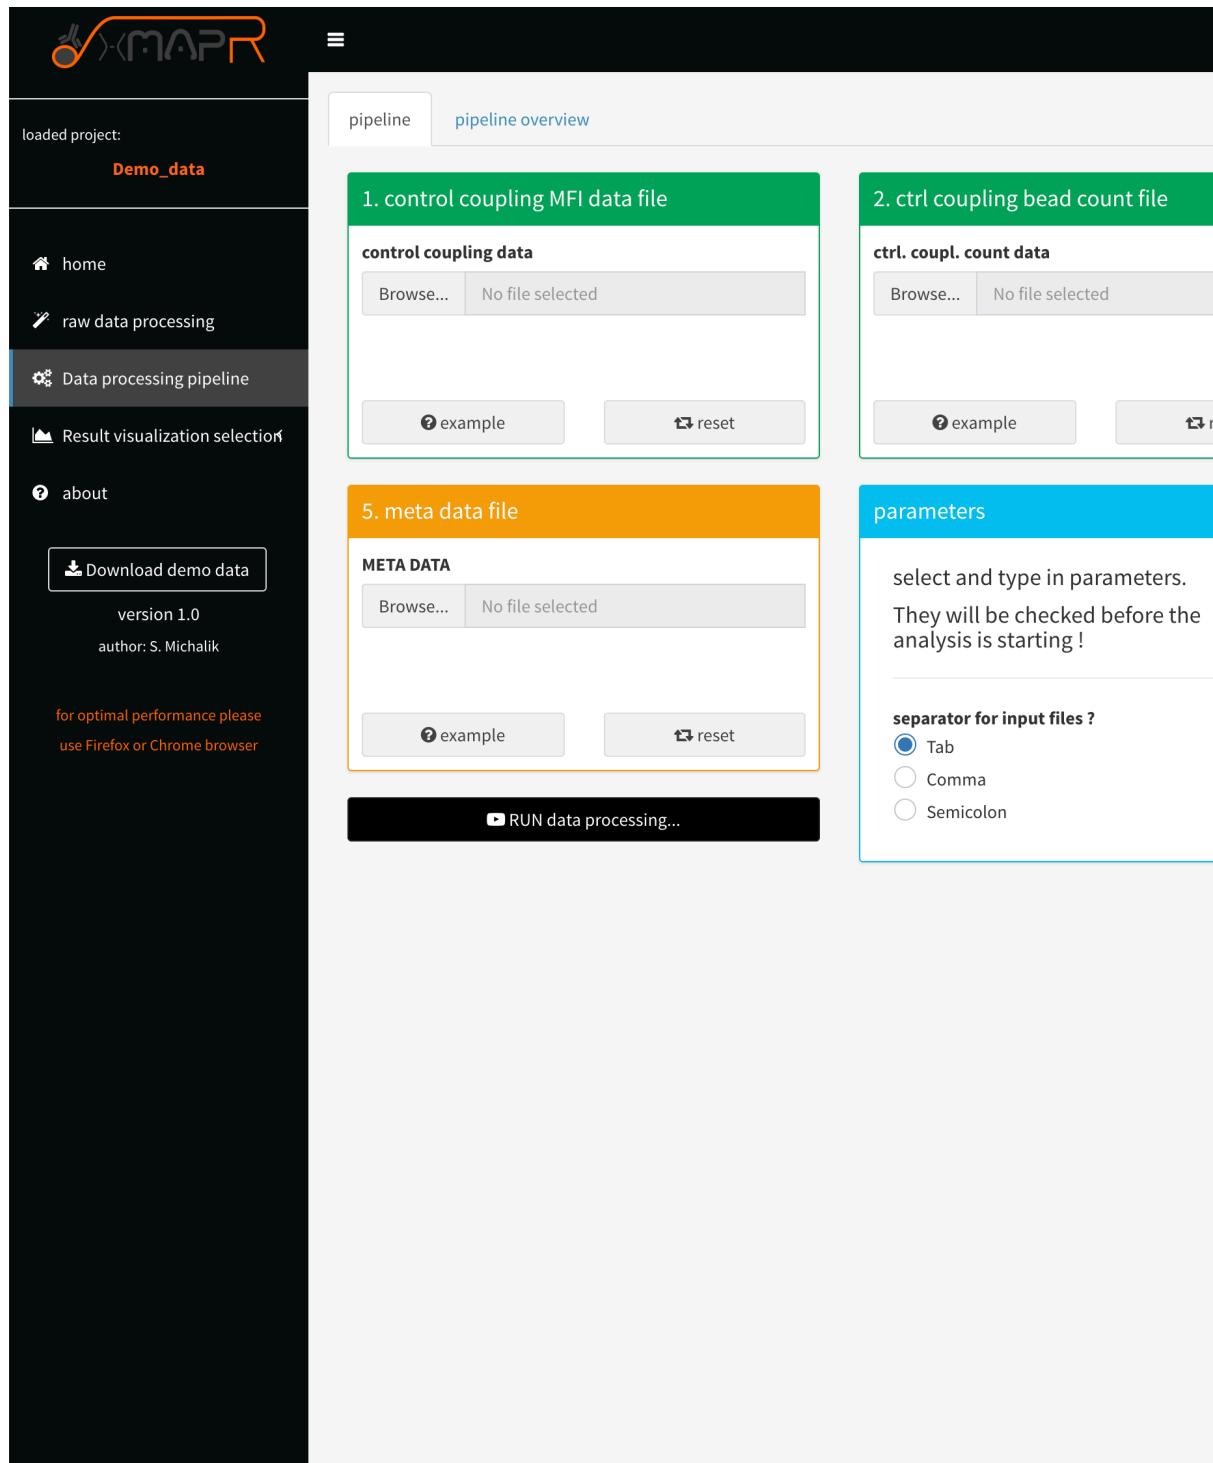


Figure 4.4: xMAPr analysis pipeline screenshot

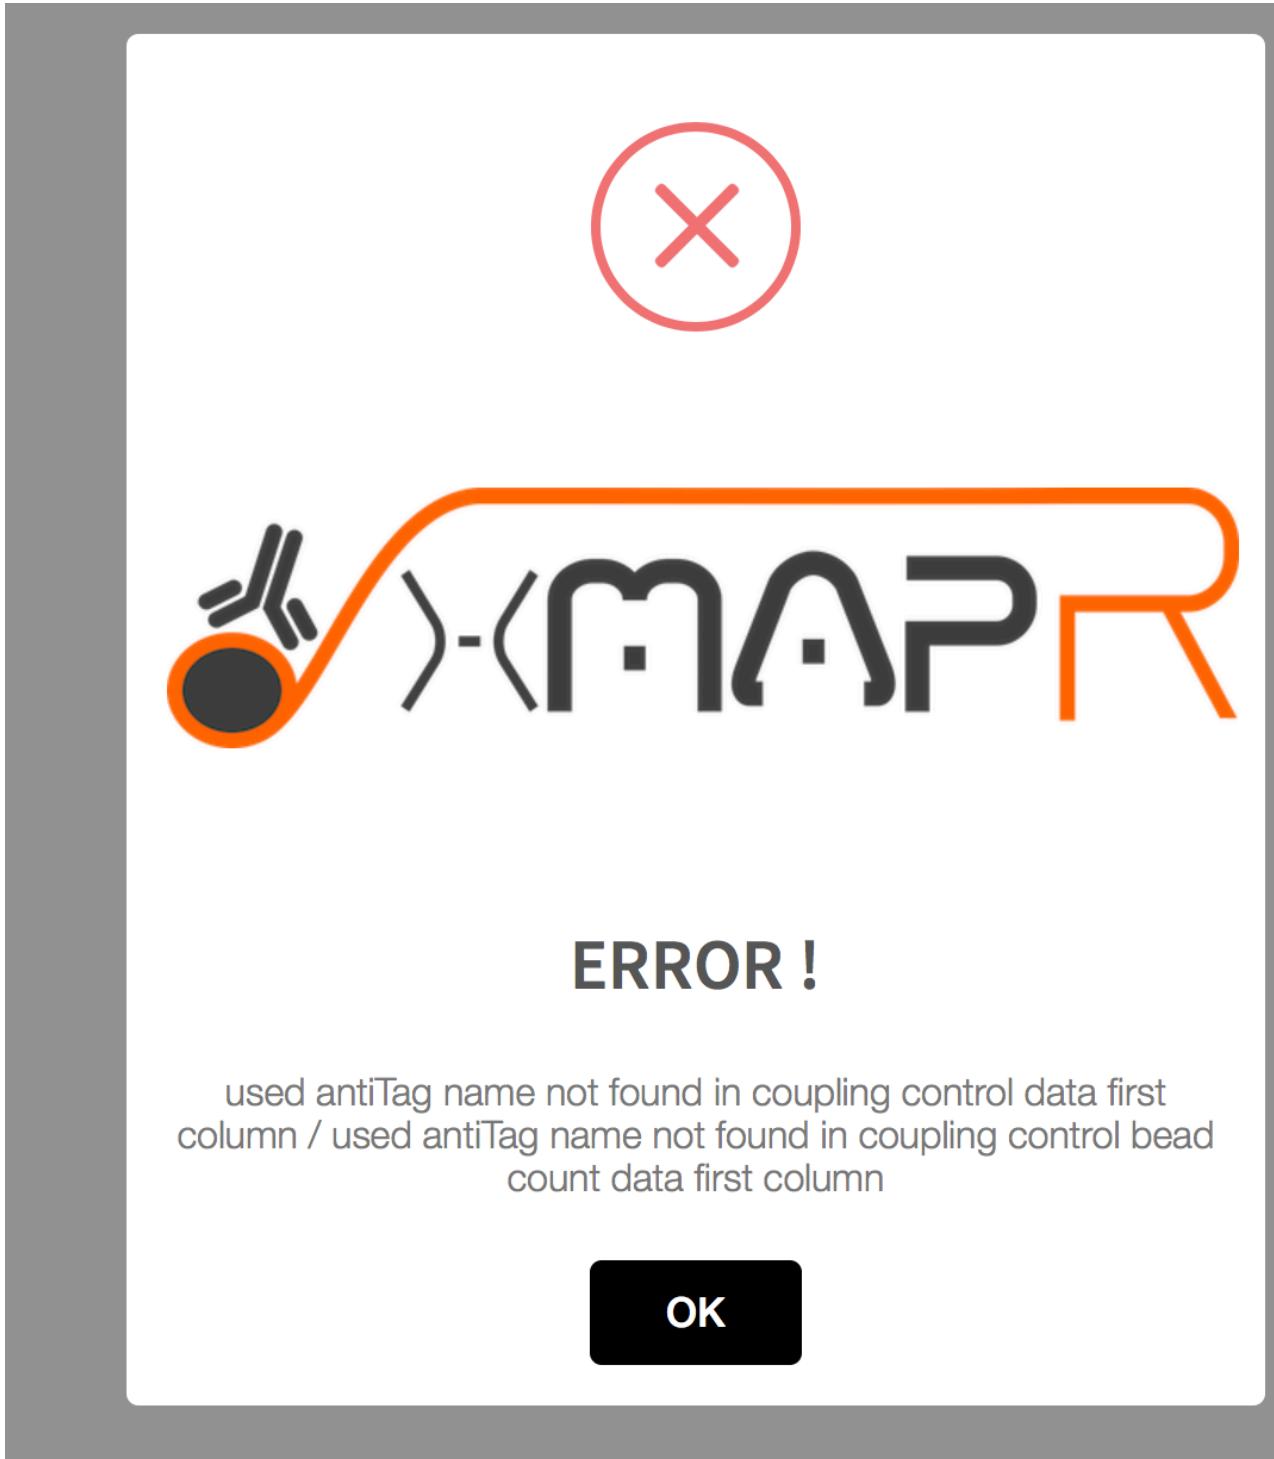


Figure 4.5: xMAPr anaylsis pipeline error pop-up (used antiTag name was wrong)

Here, a saturation curve regression model is first assumed and calculated by means of “non-least squared”. If such a calculation is not possible, a linear regression is assumed. If this calculation is successful, even a 50-fold dilution of the patient sample is still in the linear range and the respective antigen thus shows a very low immune response. In order to obtain individual quantitative values per patient and antigen, the different individual regression curves had to be converted into a meaningful value, whereby the antibody titer, which is represented over the individual dilution stages, represents the most important quantitative quantity. Here, in the saturation curve model, the half-maximal intensity was multiplied by the reciprocal dilution at the half-maximal intensity (e.g., `half maximal norm. MFI intensity = 50 & dilution at half maximalnorm. MFI intensity = 0.001 --> 50 * (1 / 0.001) = immune response of 50,000`). Linear regression multiplies the first serial dilution step by the intensity at that step. This results in a very small quantitative value.

xMAPr will perform multiple regression modeling on the data of each sample/antigen combination and subsequently decide which fit type is most characteristic for the sample/antigen specific data (decision tree figure 4.6)

#### 4.1.2.1 Decision tree

The decision tree was build to elucidate the best fit for the data.

inspect xMAPr decision tree

### 4.1.3 xMAPr data inspection

In addition to the data analysis pipeline xMAPr possess a interactive data inspection modul, which allows the user to easily check the fits and the resulting response values.

#### 4.1.3.1 global analysis inspection (Screenshots)

inspect xMAPr anaylsis output data inspection » global overview

The `overview of responses` (figure 4.7) tab depicts the used fit count histogram (figure 4.7 **left plot**), which should have a majority of `nls` (non-least squared) fits (saturation curve fits).

A `nls_with_exclusion` fit - is a nls fit that appears to posses a signal drop in the first sample dilutions in the measured curve. This happens if the secondary antibody **did not saturate the bound sample antibodies on the bead**. Therefore the automatic detection of a signal drops in the dilution response curve will flagged and not use the responsible data points for the fit (`nls_wih_exclusion`).

If linear fits were used for the majority of curve fittings the used serial dilution range did not end up in a saturation making a saturation curve fit impossible.

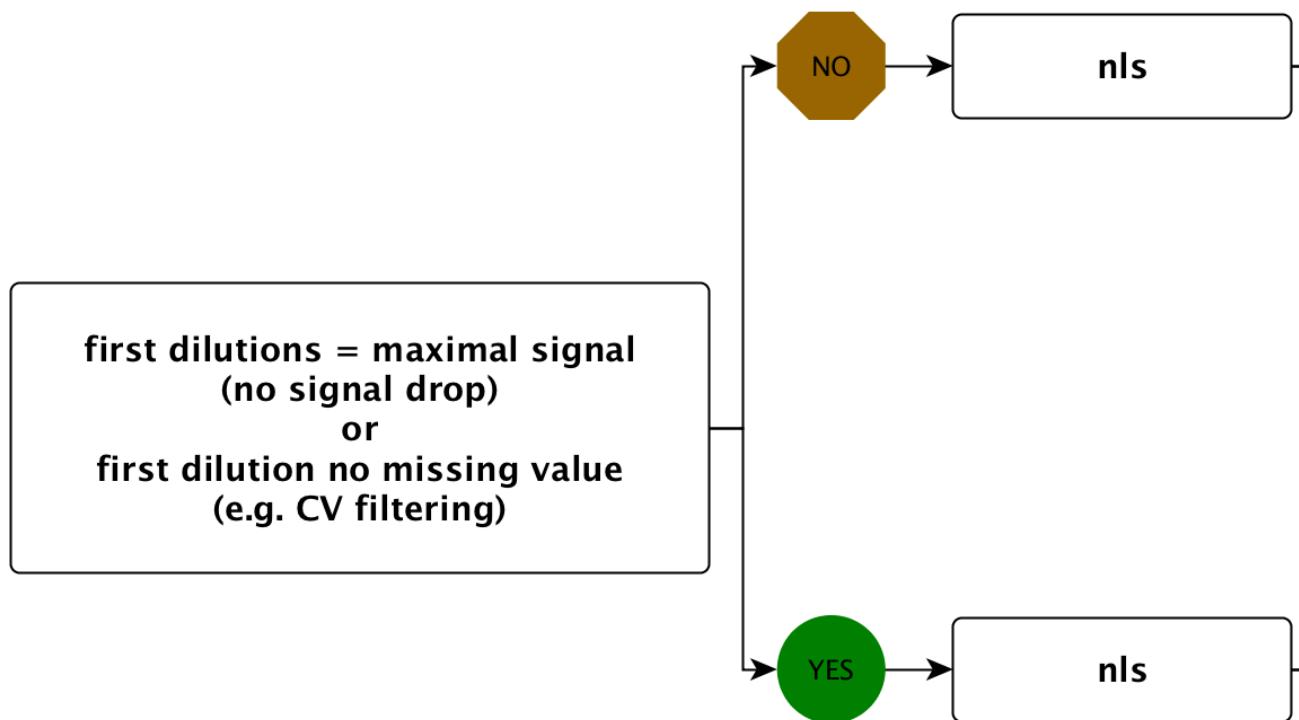


Figure 4.6: xMAPr decision tree

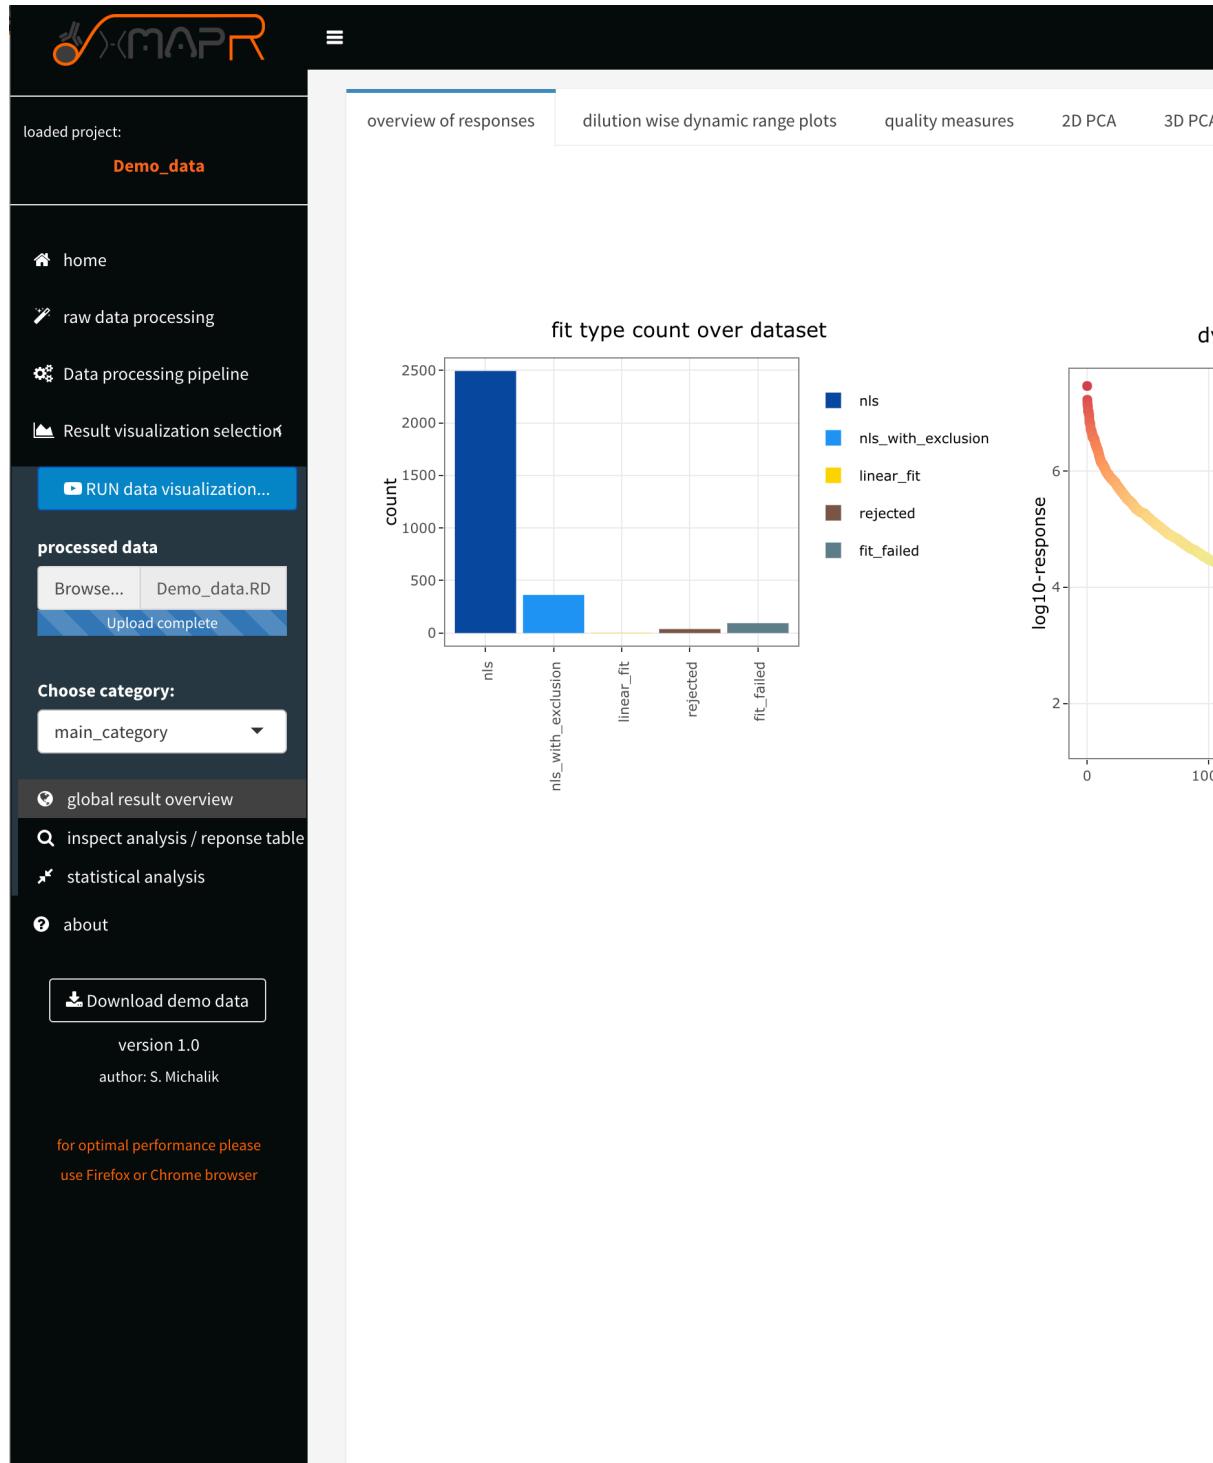


Figure 4.7: xMAPr anaylsis output data inspection » global overview

The resulting response data should be used carefully ! In that case a one dilution data analysis is more reasonable.

The dynamic range of responses plot (figure 4.7 **center plot**) depicts the dynamic range which is covered by the data over all sample and antigen combinations used.

inspect xMAPr anaylsis output data inspection » global overview (interactive hover feature)

The fit type histogram ((figure 4.7 **right plot**) displays the used fit histogram in correlation to the calculated response. In the example screenshot it apparent that the *nls\_with\_exclusion* is primarily being used in the high response range. This makes sense since a high sample antibody titer against one antigen is resulting in a very high load of the sample antibodies on the individual bead. Thus a signal drop in the very first dilutions (low sample dilution) are more likely to happen.

The **dilution wise dynamic range plots** (figure 4.9) tab depicts intensity ranked order of sample/antigen combinations (x-axis) versus log. MFI (median fluorescence intensity) (y-axis). The plot is being used for visually estimating the saturation effect (upper and lower LOD) in each dilution used.

inspect xMAPr anaylsis output data inspection » dynamic range dilution wise

#### 4.1.3.2 global analysis inspection: quality check of data (Screenshots)

It is important to evaluate the data quality (figure 4.10; **quality measures > general overview**). Therefore basic measures like the bead count or coefficient of variation between technical replicates are very informative in terms of quality. A bead count below **35 beads** results by default (factory suggestion) in a missing value since the MFI (Median fluorescence intensity) is unsure using only 35 beads or below. The CV cut-off can be set in the pipeline settings (figure 4.4)

inspect xMAPr quality measures: bead count and CV histograms

Since a EDC-NHS coupling of the carboxylated beads with the desired antigens is being used the coupling efficiency might be varying due to the differences in amino acid composition and length of the antigens. The coupling control plot (figure 4.11) displays in a ranked fasion the coupling efficiency measured with a detection antibody directed against the recombinant tag the antigens. The interactive hover feature returns the absolute value measured for each antigen.

The MFI of the coupling control (**quality measures > coupling control**) represents the loading of the beads with the individual antigens, which can be different but should not be very low to keep a certain dynamic range for the detection of the antibody titer.

inspect xMAPr quality measures: MFI of coupling control

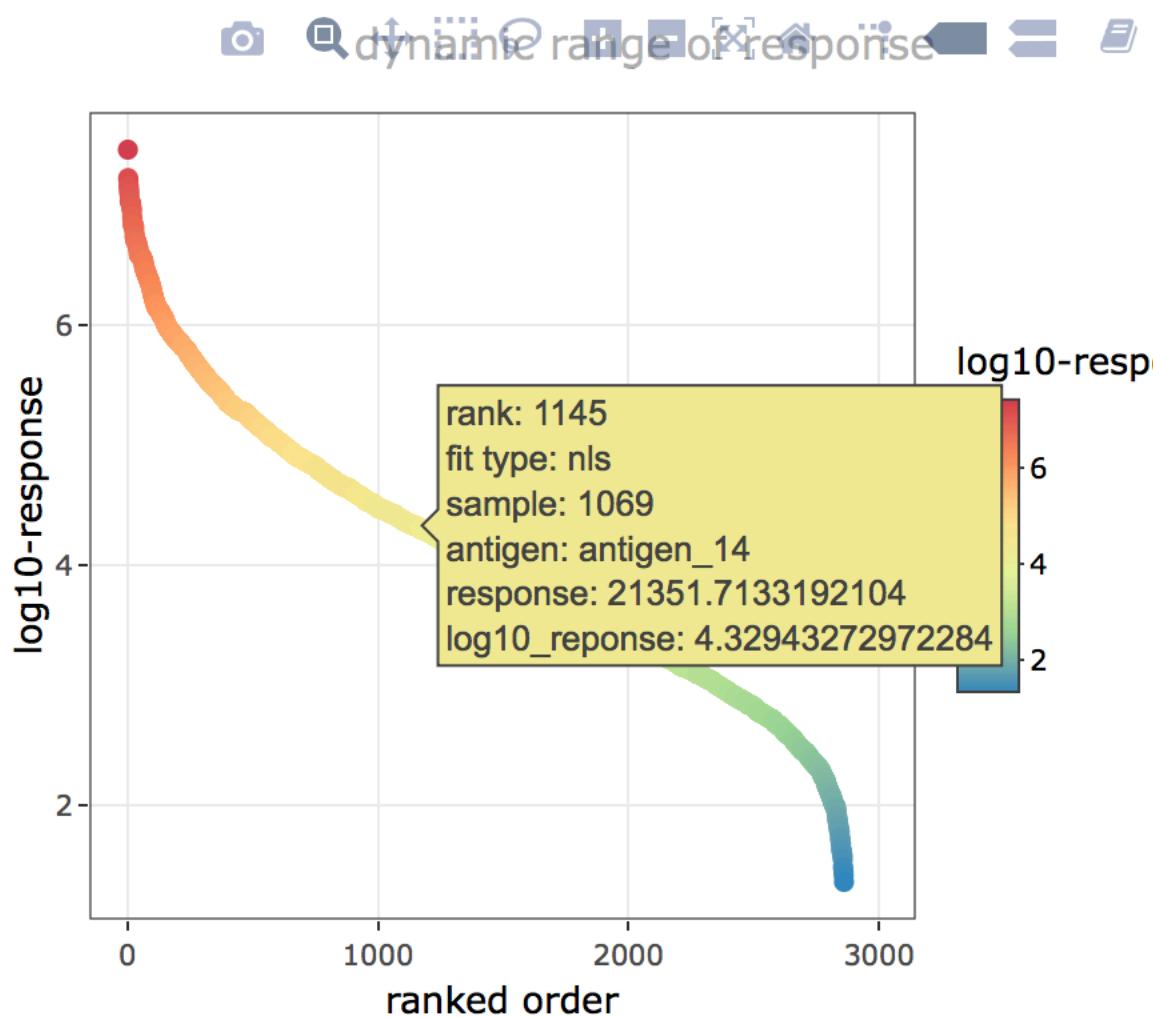


Figure 4.8: xMAPr analysis output data inspection » global overview (interactive hover feature)

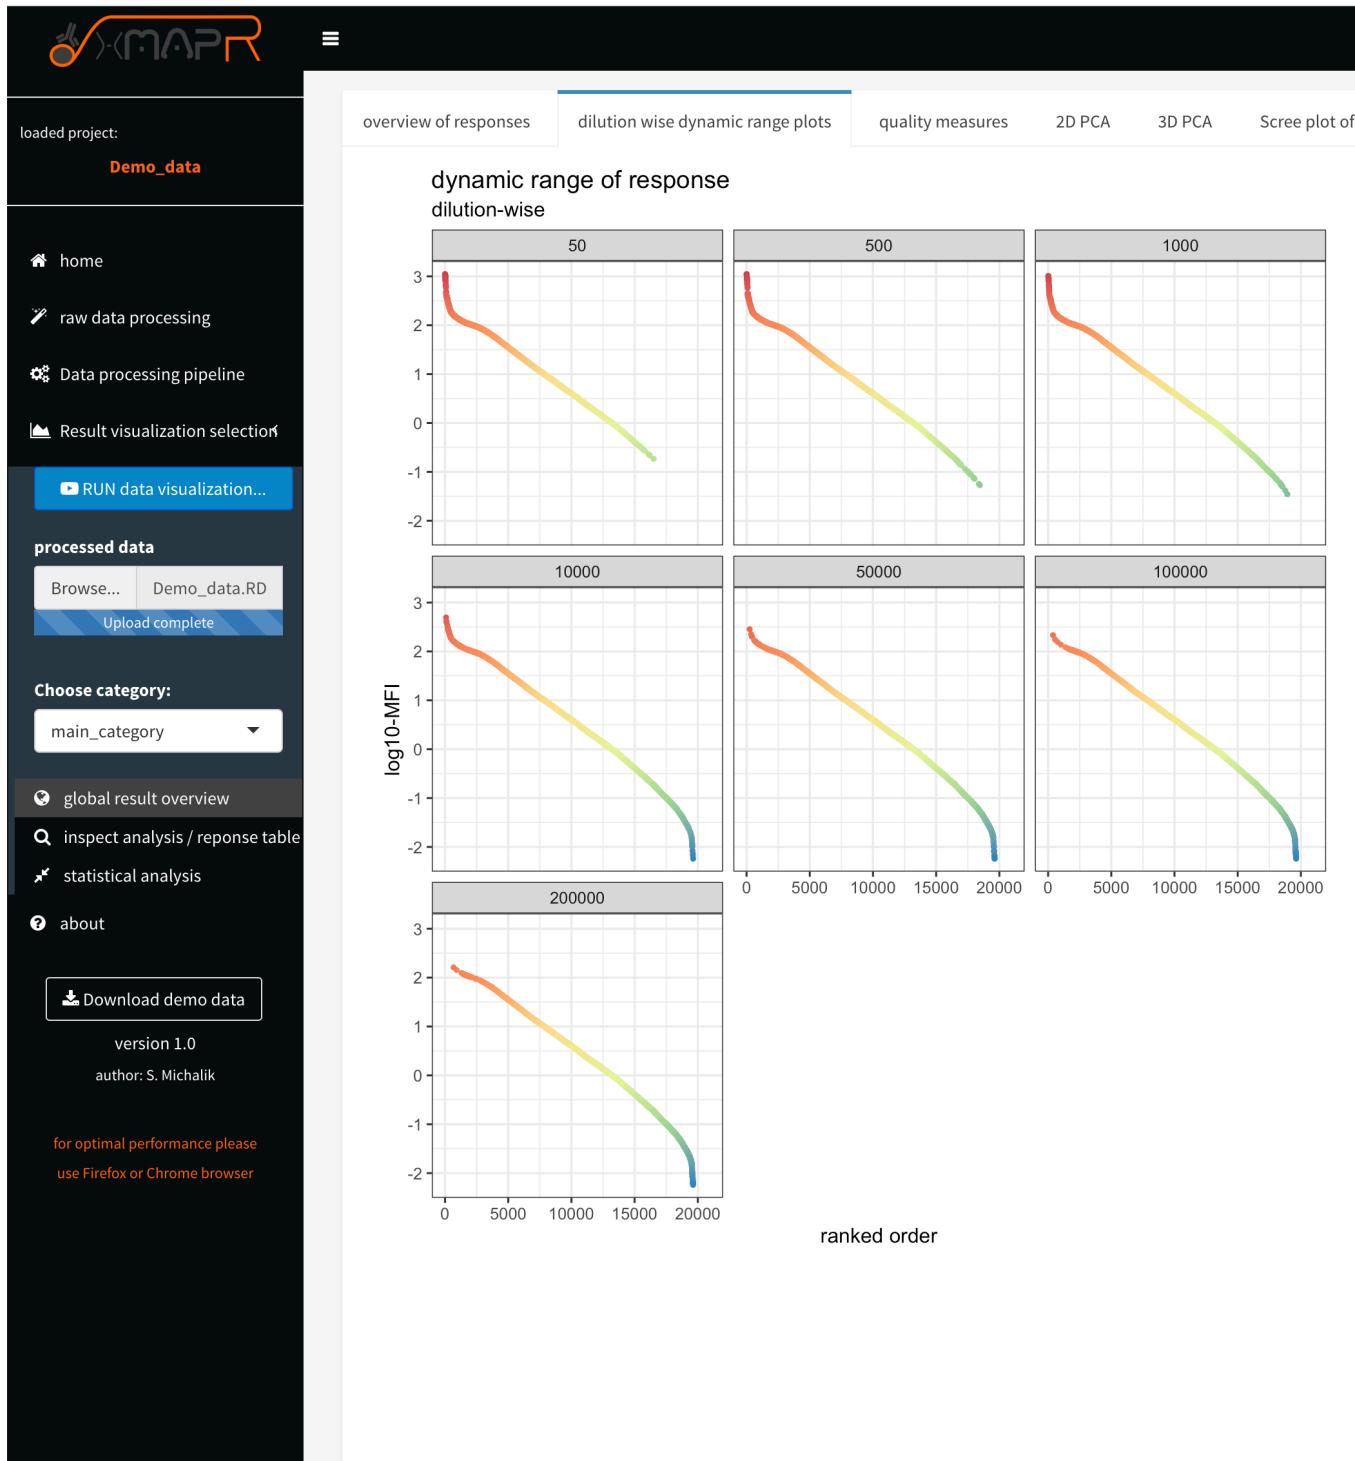


Figure 4.9: xMAPr anaylsis output data inspection » dynamic range dilution wise

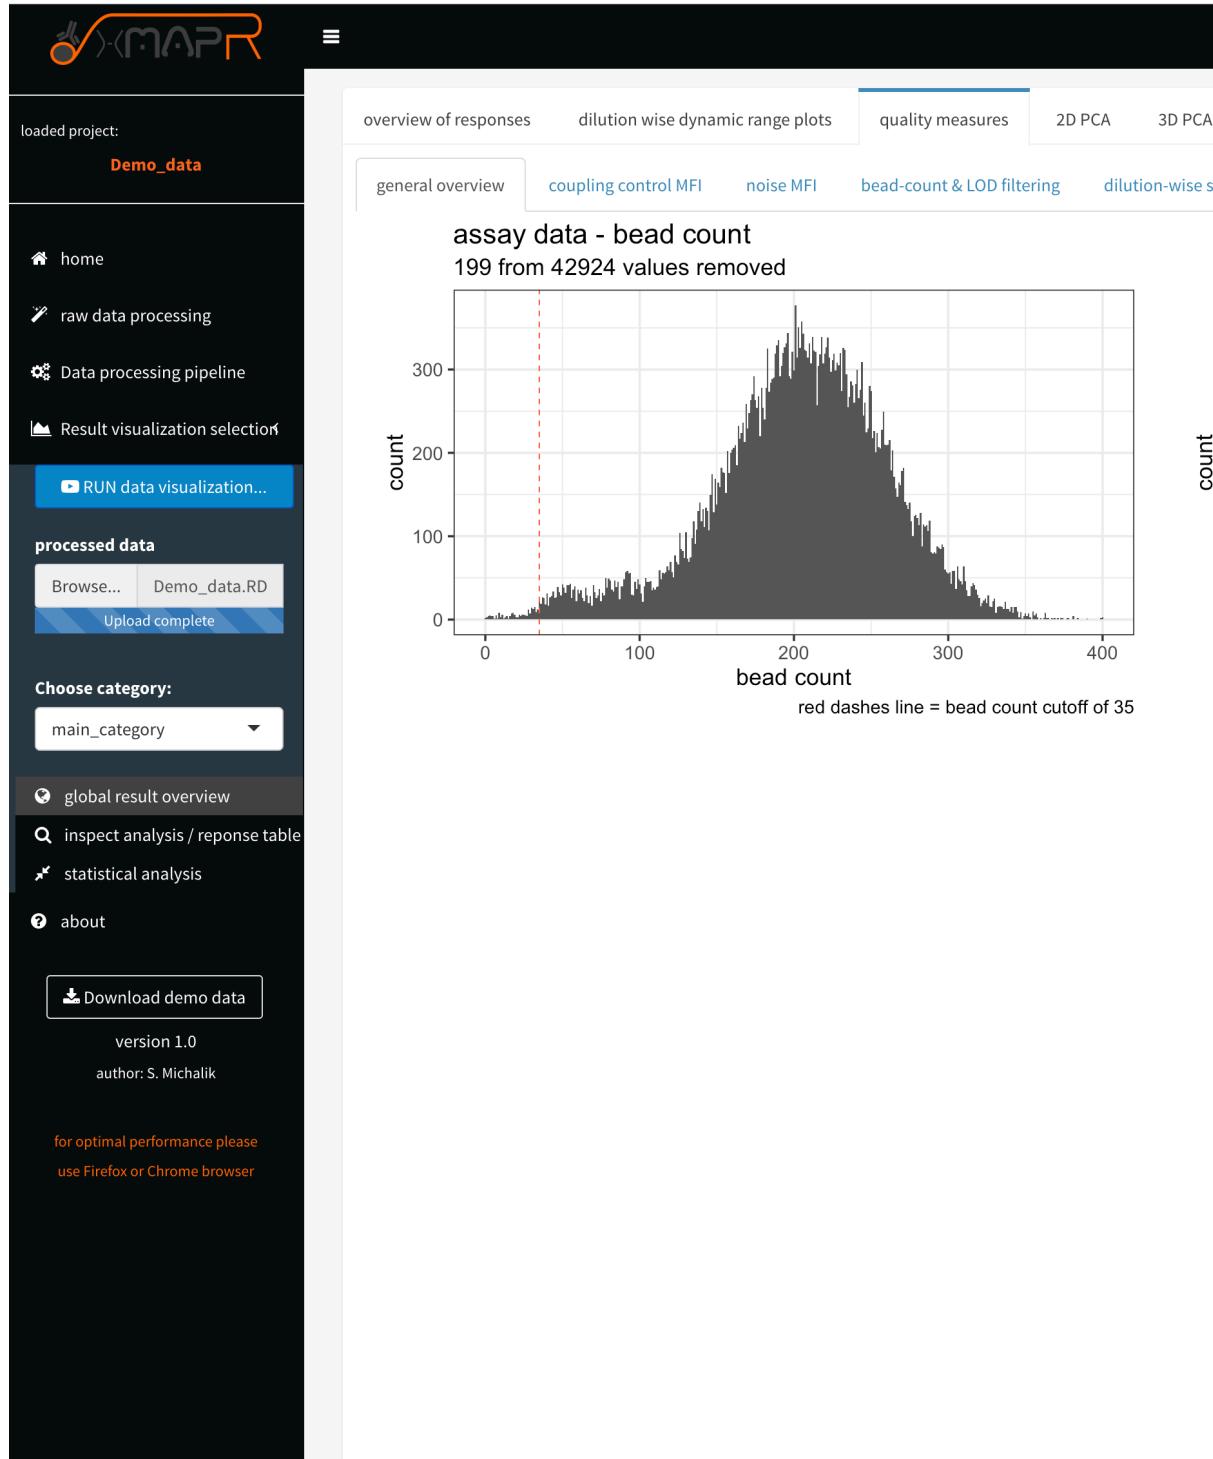


Figure 4.10: xMAPr quality measures: bead count and CV histograms

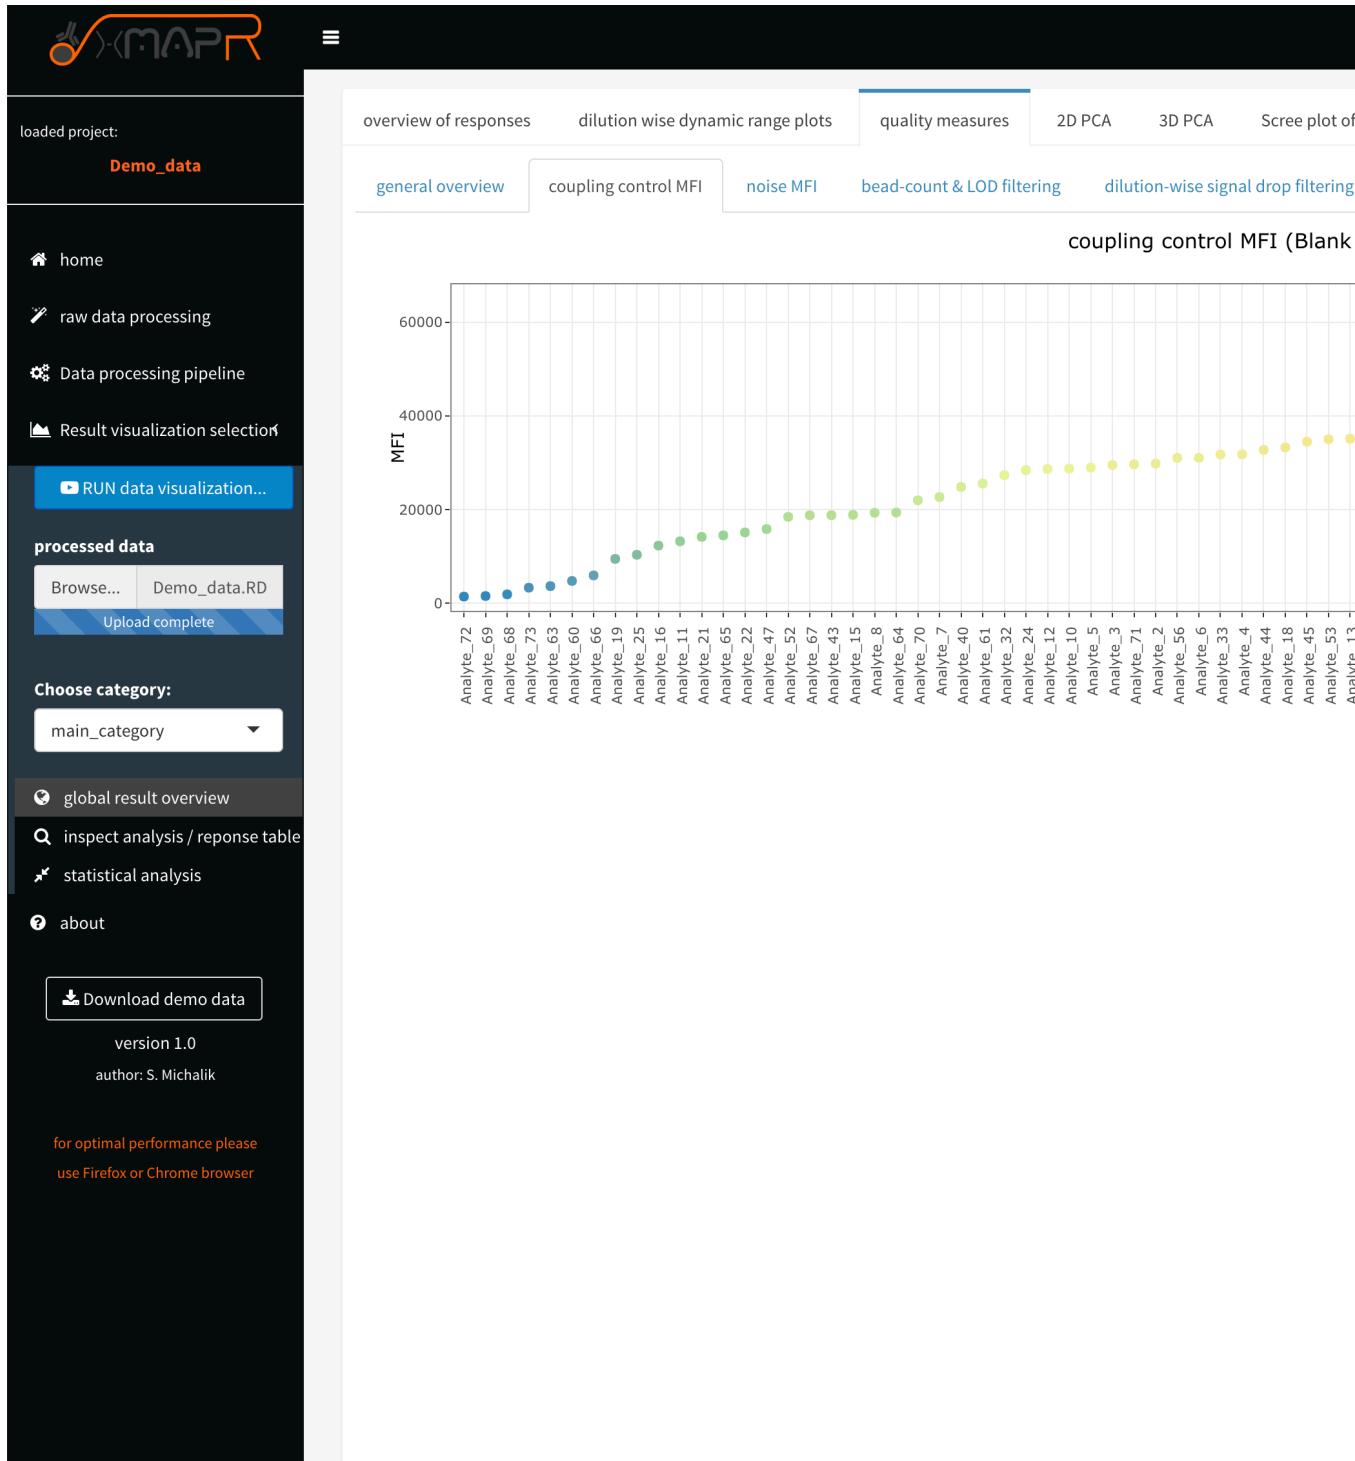


Figure 4.11: xMAPr quality measures: MFI of coupling control

The noise MFI (figure 4.12) (`quality measures > noise MFI`) depicts the ranked ordered mean BLANK values + 3 x SD of the BLANK values, which is being used to estimate the LOD (limit of detection) for each antigen. Again the interactive hover feature show details for each entigen.

inspect xMAPr quality measures: LOD...limit of detection

The stacked barplots (figure 4.13) (`quality measures > bead-count and LOD filtering`) are displaying the filtering for low bead count, for CV filtering with the used cut-off and showing how many fits failed or get rejected.

inspect xMAPr quality measures: stacked barplots of value filtering

The implemented signal drop detection alg. uses the maximum value of the measured data points and inspect the data points with a lower dilution beginning from the maximal MFI data point (`quality measures > dilution-wise signal drop filtering`). For example signal drops in the first dilution step of the serial dilution range is normal. But also having a huge amount of signal drops in later dilutions is the result of using a low concentration of the detection antibody or the dilution steps were not well choosen.

“xMAPr quality measures: stacked barplots of dilution-wise signal drop detection

The interative hover feature (figure 4.14) displays information like which antigen, the count of filtered values and what is the percentage of filtered values form the data matrix. Making it easy to identify problematic antigen or sample candidates.

inspect xMAPr quality measures: NA (missing) value heatmap

The missing value heatmap (figure 4.16) (`quality measures > heatmap of NA values`) depicts in a compact format where and how many values are missing the the dataset after the response calculation was performed.

inspect xMAPr quality measures: bead count heatmap

The bead count heatmap (figure 4.17) (`quality measures > bead count heatmap`) is designed for quickly identifying problematic antigens or patient samples over the dilution series, which also often resulting in a low bead count.

#### **4.1.3.3 global data analysis: PCA & heatmap**

A first look at the data can be performed in the xMAPr app. A PCA (principle component analysis) is automatically generated plotted and colored based on the selected meta data.

inspect xMAPr anaylsis output data inspection » 2D-PCA of data colored by selected meta data

The principle component analysis is performed using the factomineR package with missing values removed. The data centering was done by subtracting the

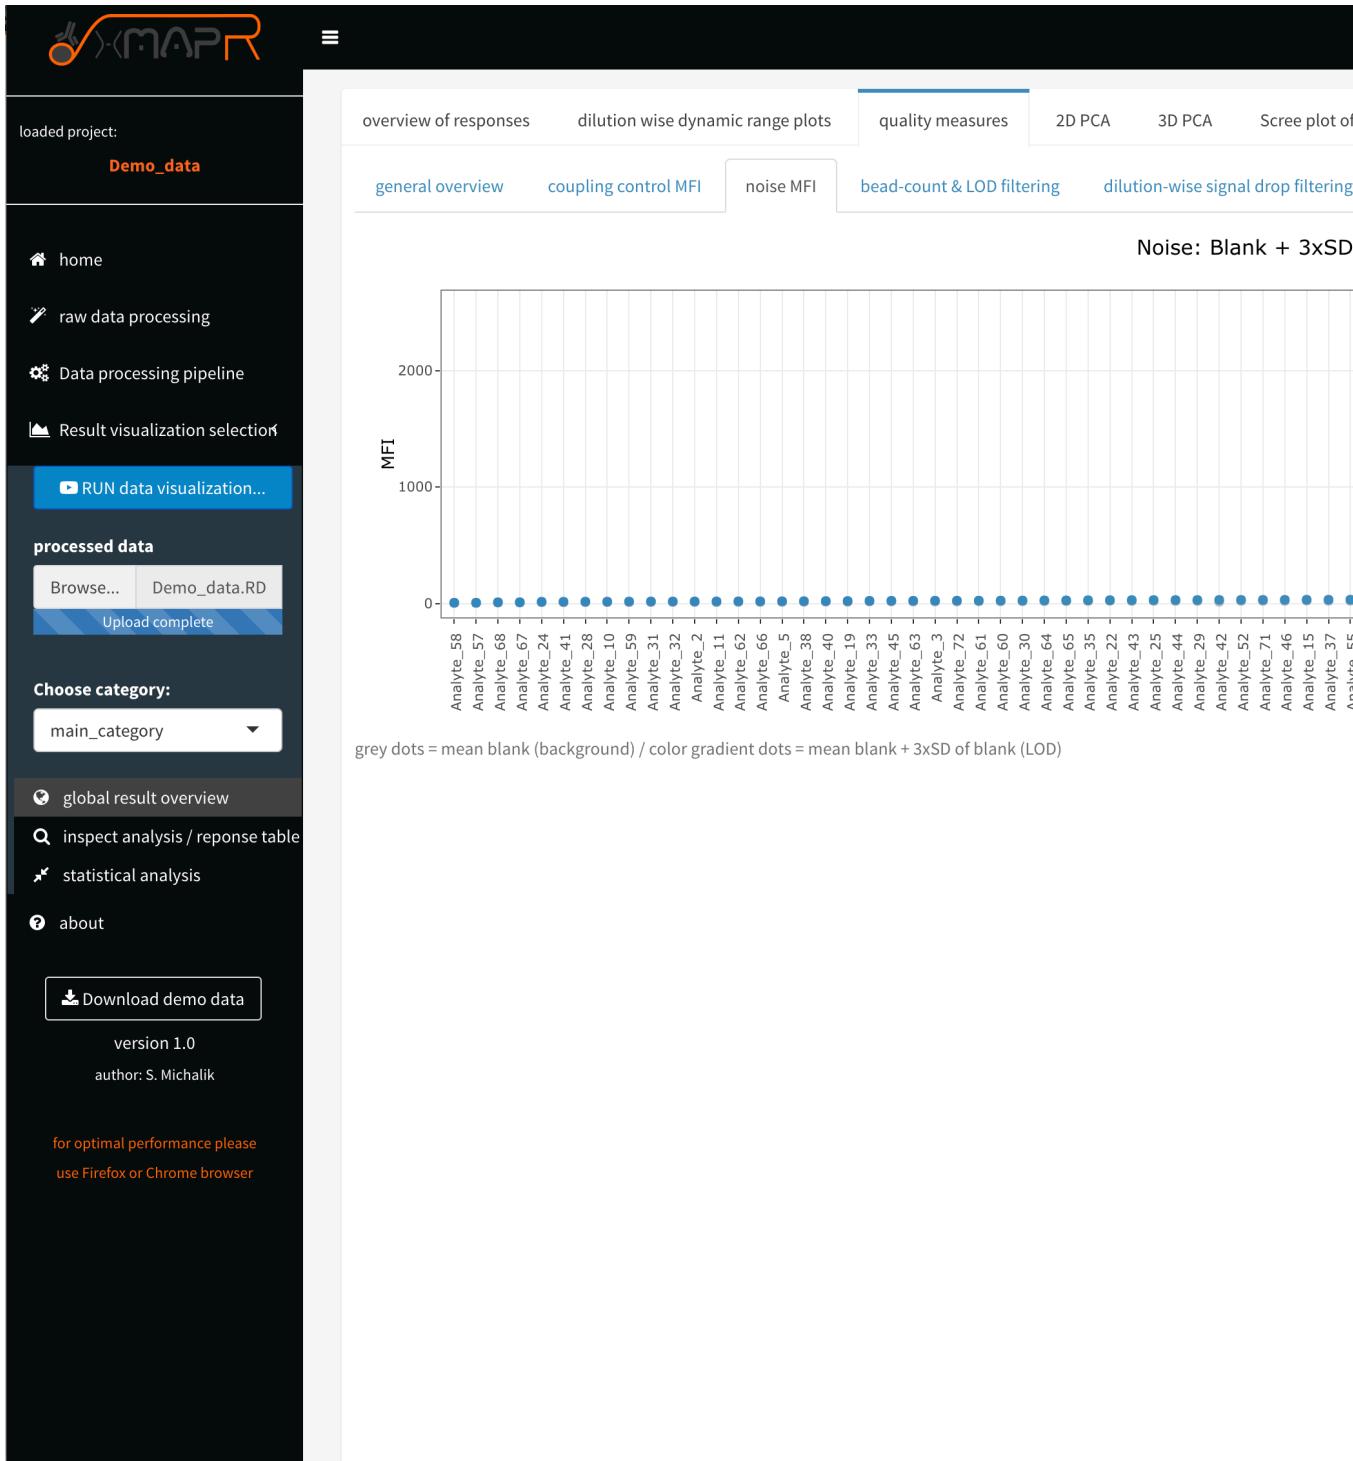


Figure 4.12: xMAPr quality measures: LOD...limit of detection

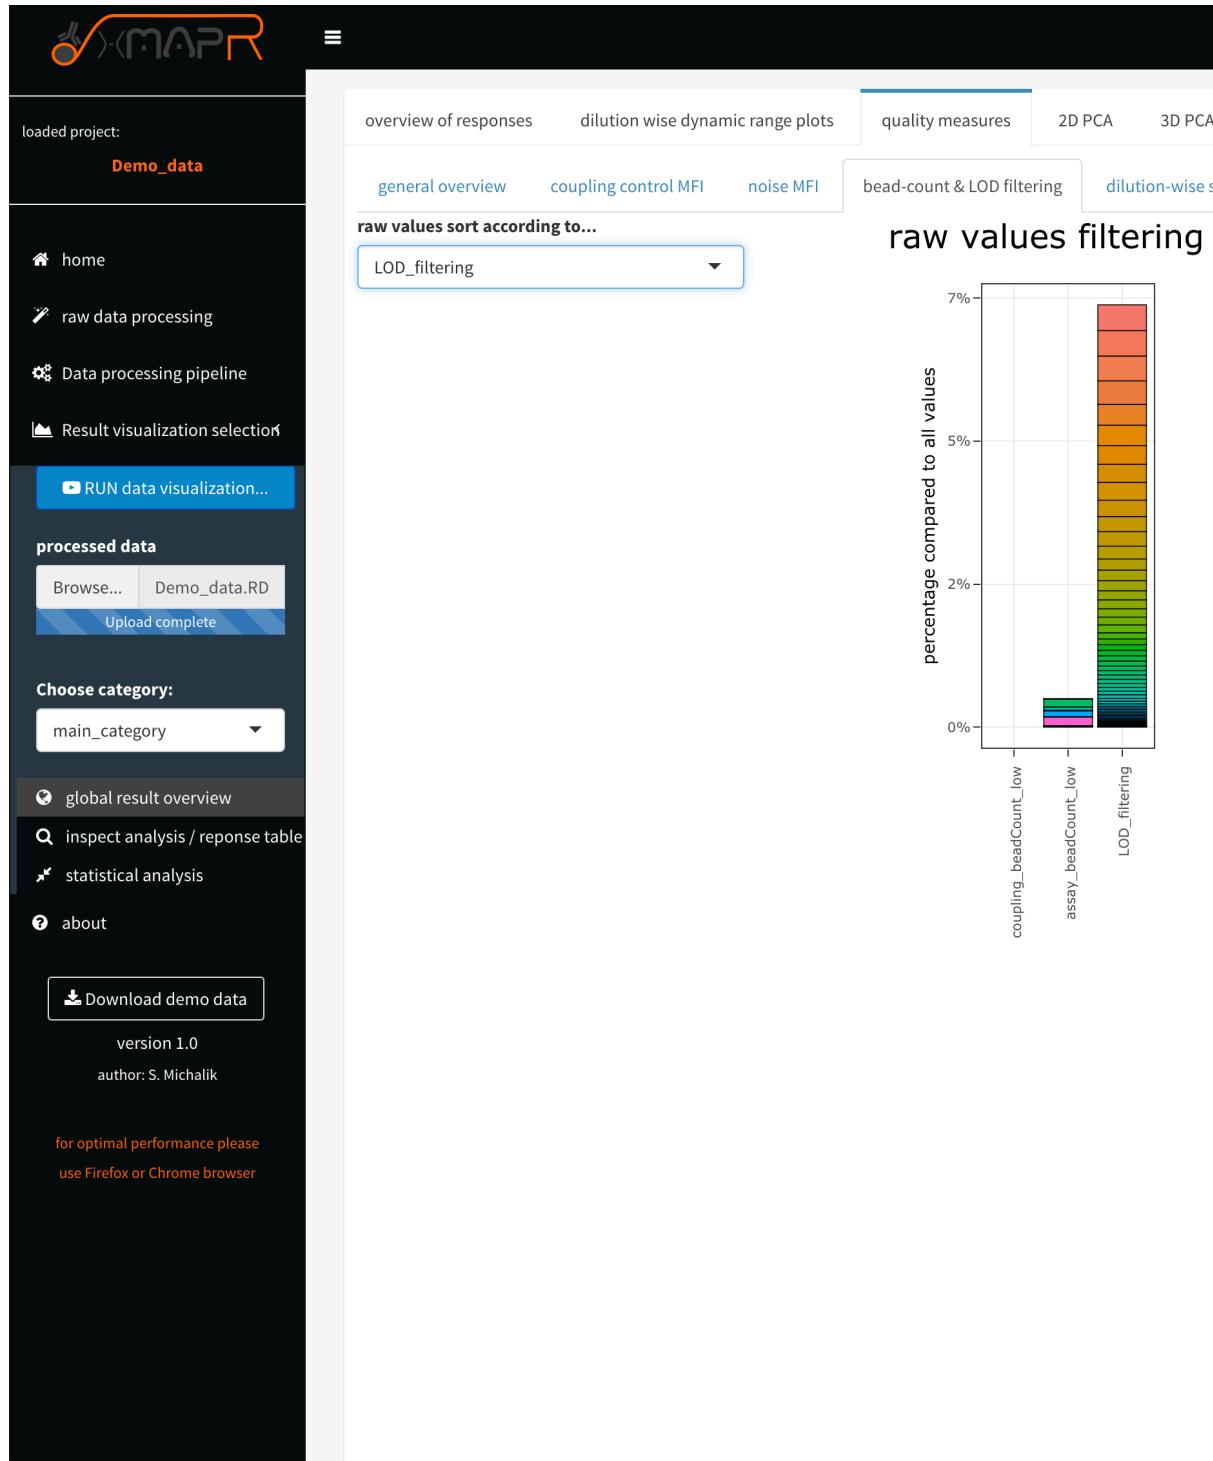


Figure 4.13: xMAPr quality measures: stacked barplots of value filtering

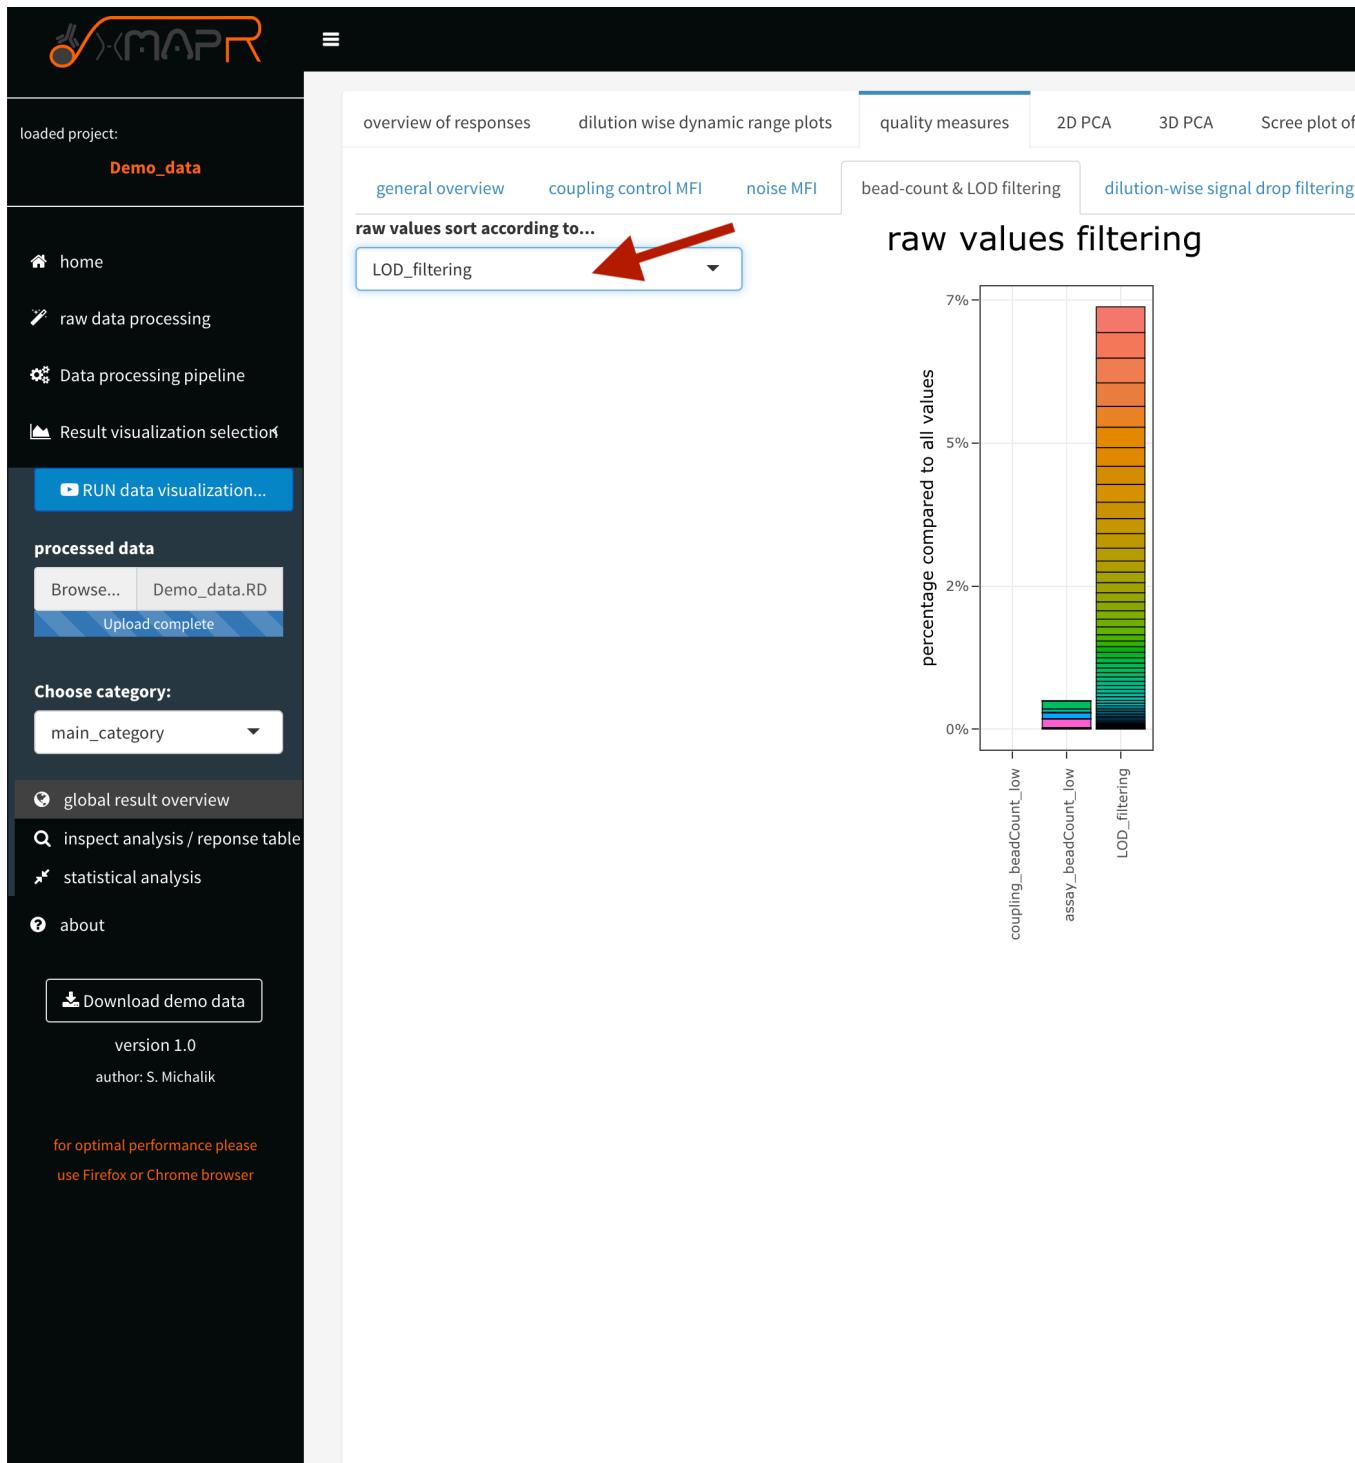


Figure 4.14: xMAPr quality measures: stacked barplots of value filtering (interactive hover)

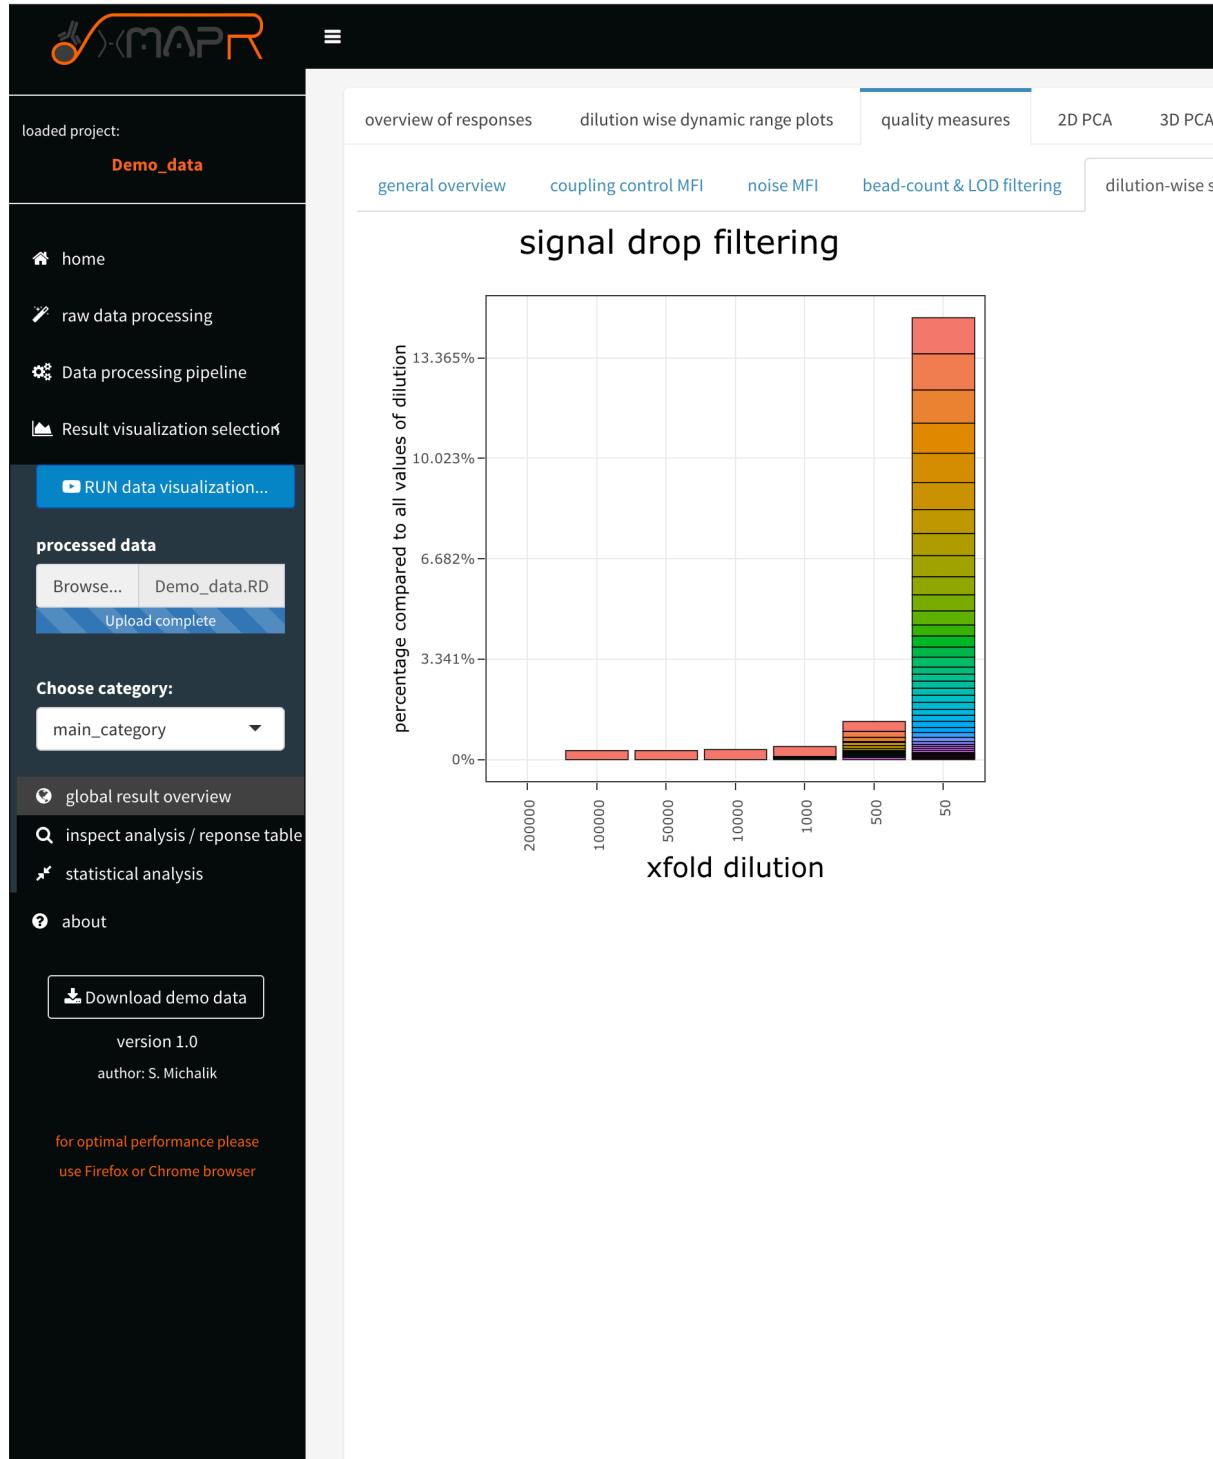


Figure 4.15: xMAPr quality measures: stacked barplots of dilution-wise signal drop detection (interactive hover)

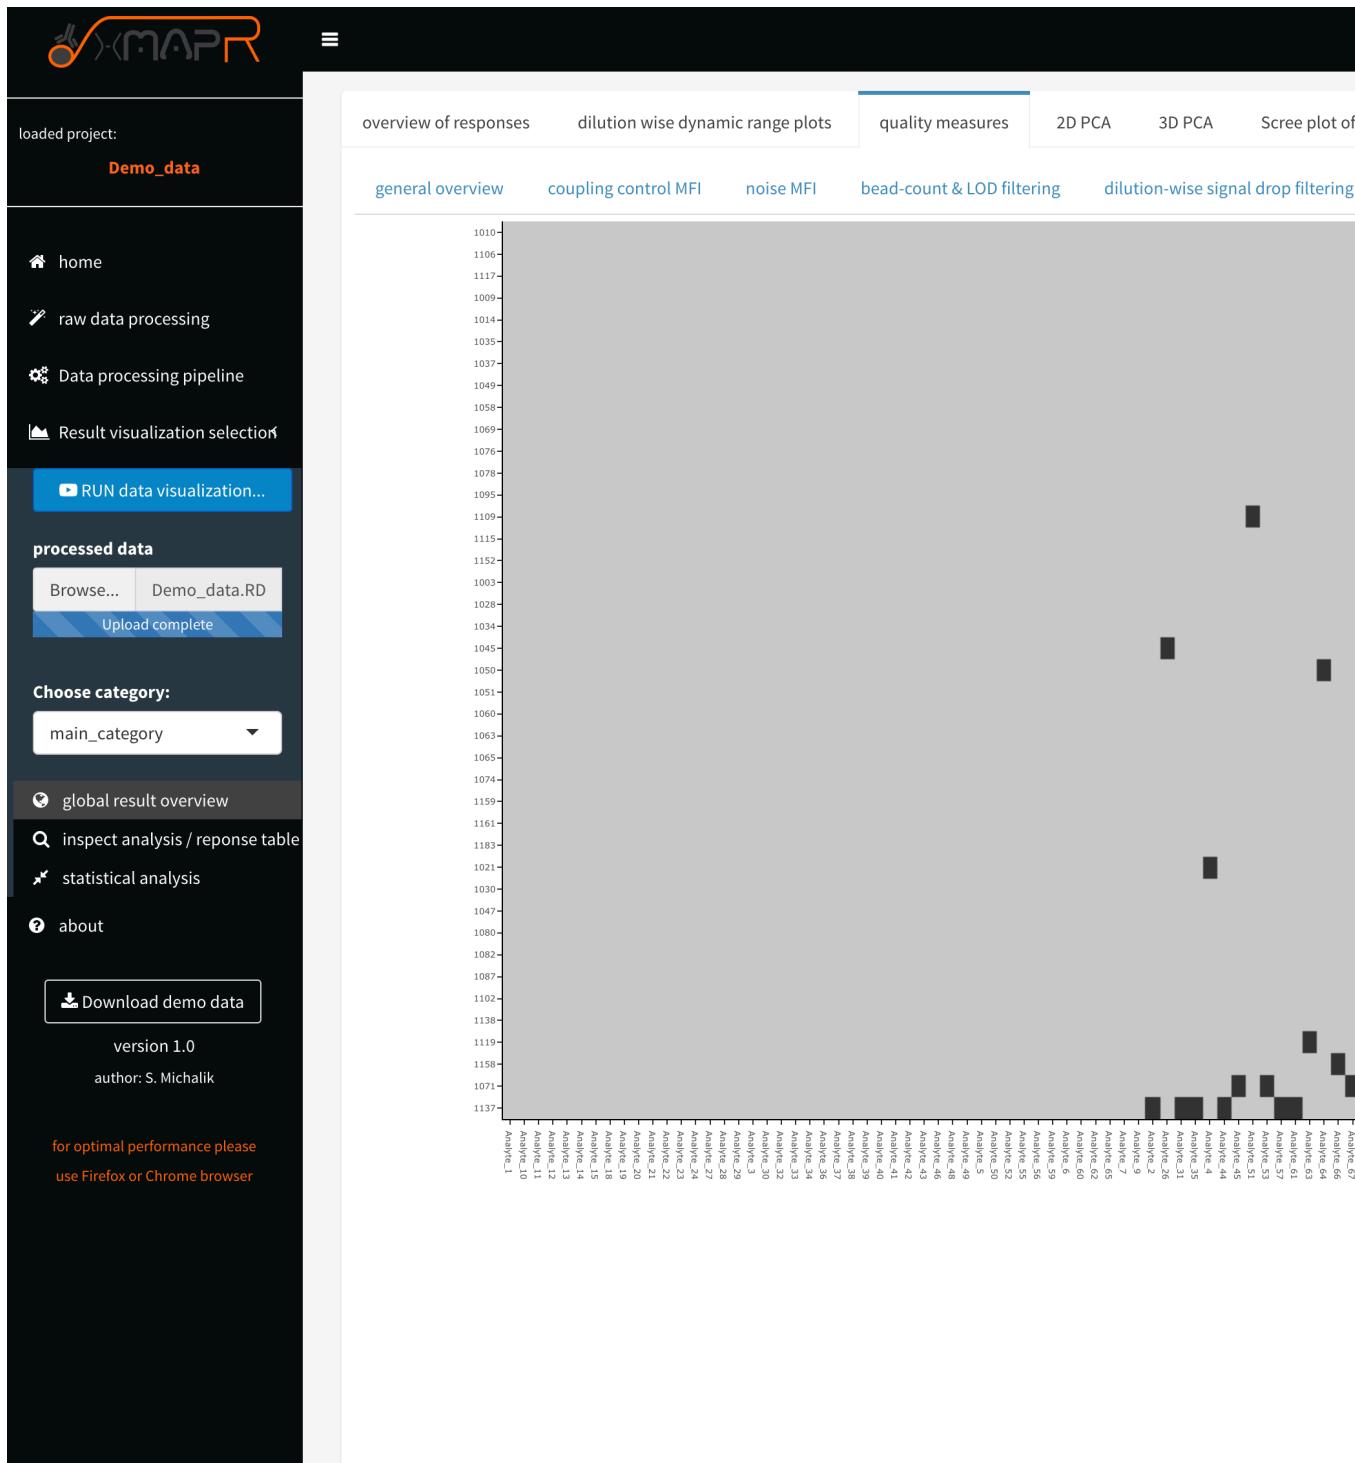


Figure 4.16: xMAPr quality measures: NA (missing) value heatmap



Figure 4.17: xMAPr quality measures: bead count heatmap

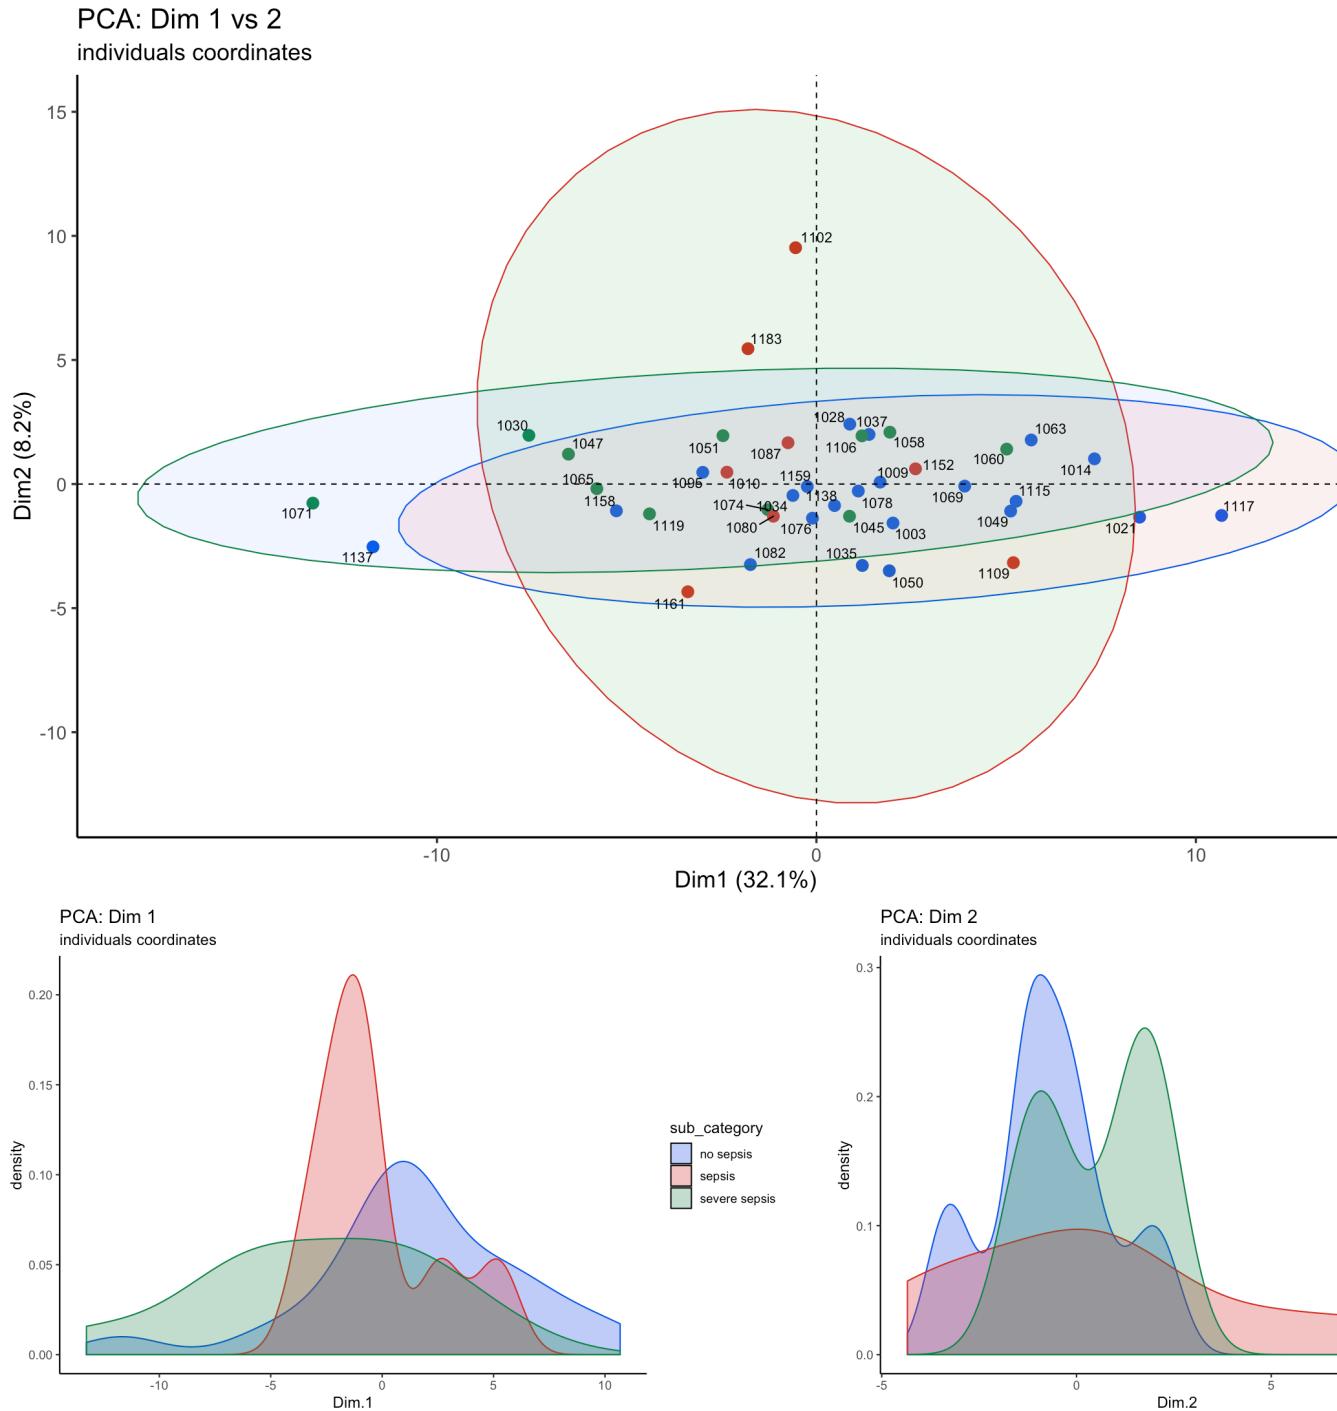


Figure 4.18: xMAPr analysis output data inspection » 2D-PCA of data colored by selected meta data

column means (omitting NAs) of the data from their corresponding columns. To unify variances scaling of data was done by dividing the (centered) columns of the data by their standard deviations. The 2D PCA (figure 4.18) (2D PCA) displays the resulting PCA plot. 1D density plots supporting the interpretation of the PCA results.

The PCA dimension for the plot can be selected using the *knobs*. Furthermore advanced plot adjustment like group ellipsis can be set as well using the “*wrench*” button.

inspect xMAPr analysis output data inspection » interactive 3D-PCA colored by selected meta data

The 3D PCA (figure 4.19) (3D PCA) displays the resulting PCA plot in the first 3 dimensions.

inspect xMAPr analysis output data inspection » screeplot of PCA analysis

The Screeplot visualize the variances of dimensions of the PCA (figure 4.20) (Scree plot of PCA).

inspect xMAPr analysis output data inspection » response heatmap

The heatmap (figure 4.21) (heatmap (response data)) displays the clustered heatmap of the calculated response data. If a sample or a antigen possess only NA values it is excluded from the heatmap, which is indicated in the grey text below the “*download heatmap*” button. The heatmap is fully interactive with hover information feature, zoom and screenshot feature. Furthermore the heatmap can be download in its interactive form as html using the “*download heatmap*” button. Several parameters can be set like number of clusters of rows and columns or cluster methods to name a few.

#### 4.1.3.4 single antigen/sample inspection (Screenshots)

inspect xMAPr analysis output data inspection » single antigen/sample combination fit inspection

The single result view (figure 4.22) (inspect analysis/response table) enables a inspection of the data down to raw data level by displaying the results on a antigen/sample combination basis. The upper panel displays the different presentations of the data.

The **left plot** displays the raw data and the dashed red line indicate the LOD. In addition detected signal drops were marked with a blue cross.

The **center plot** displays the calculated curve and the curve point, which is being used for the response calculation. The dashed violet vertical line indicating the lower and upper end of the used dilution steps.

The **right plot** displays the residuals from the used fit.

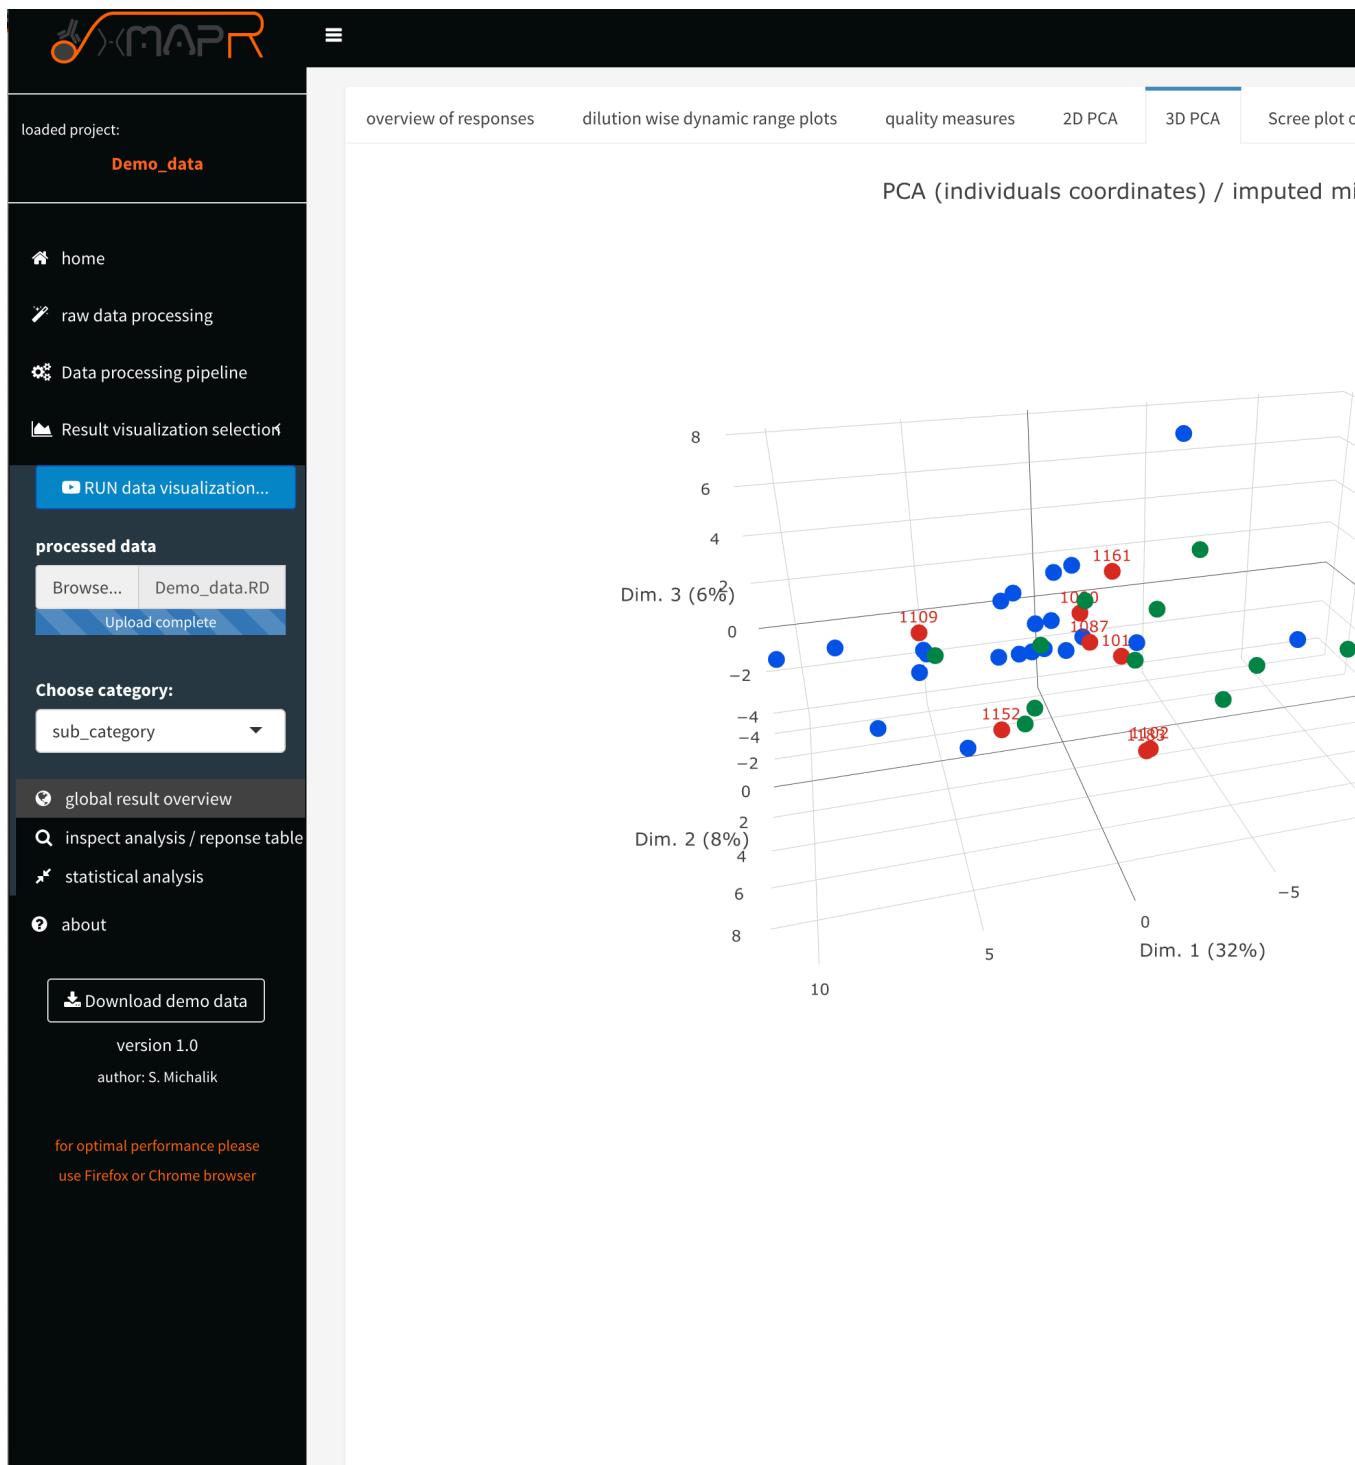


Figure 4.19: xMAPr analysis output data inspection » interactive 3D-PCA colored by selected meta data



Figure 4.20: xMAPr anaylsis output data inspection » screepplot of PCA analysis

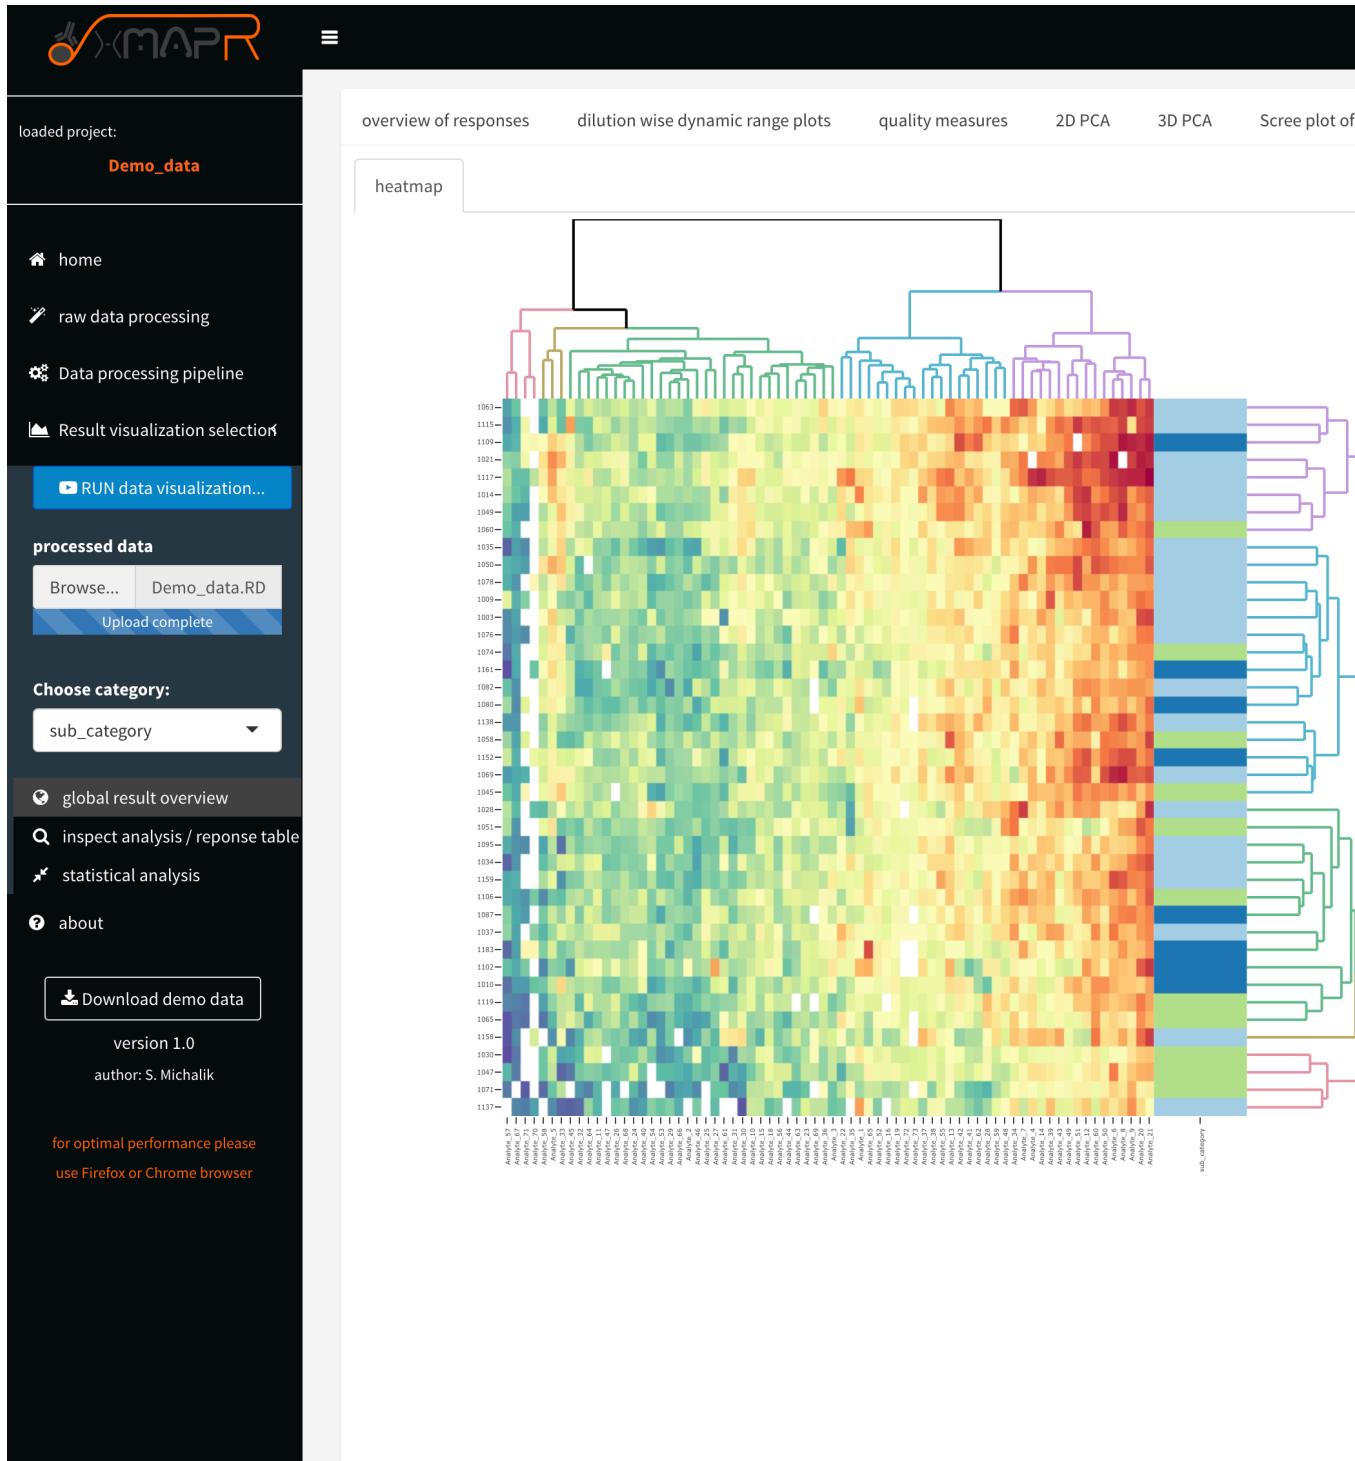


Figure 4.21: xMAPr analysis output data inspection » response heatmap

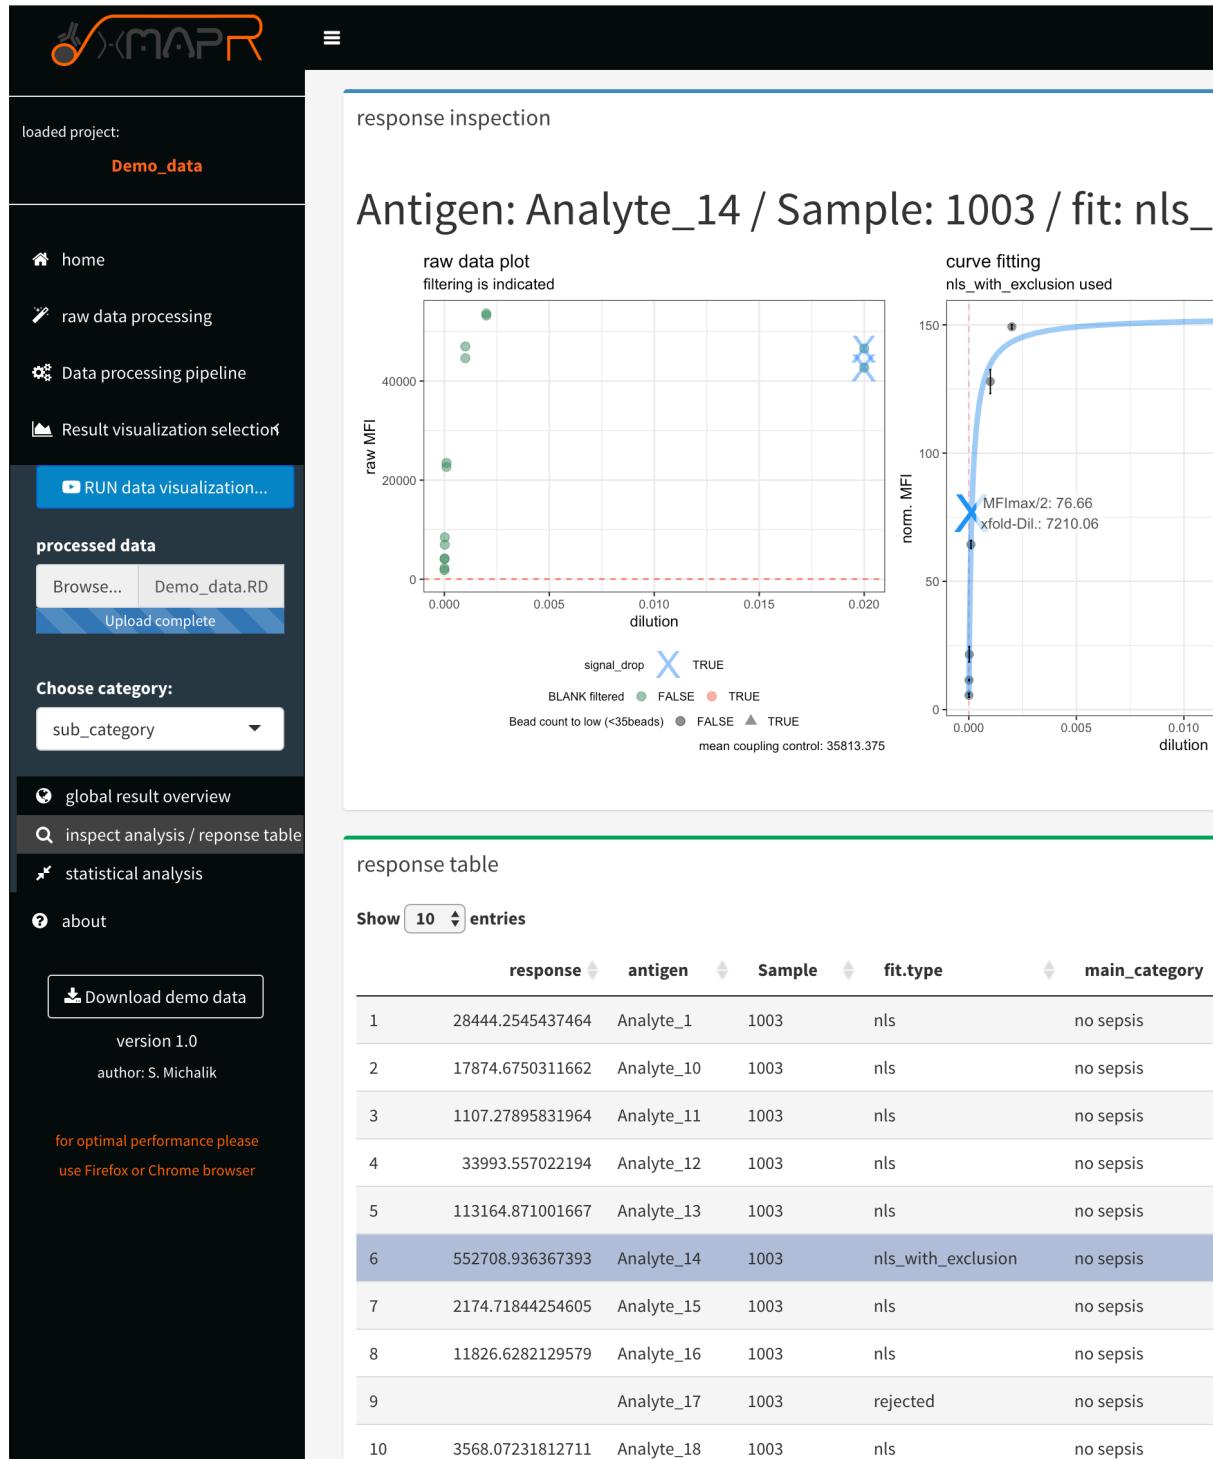


Figure 4.22: xMAPr analysis output data inspection » single antigen/sample combination fit inspection

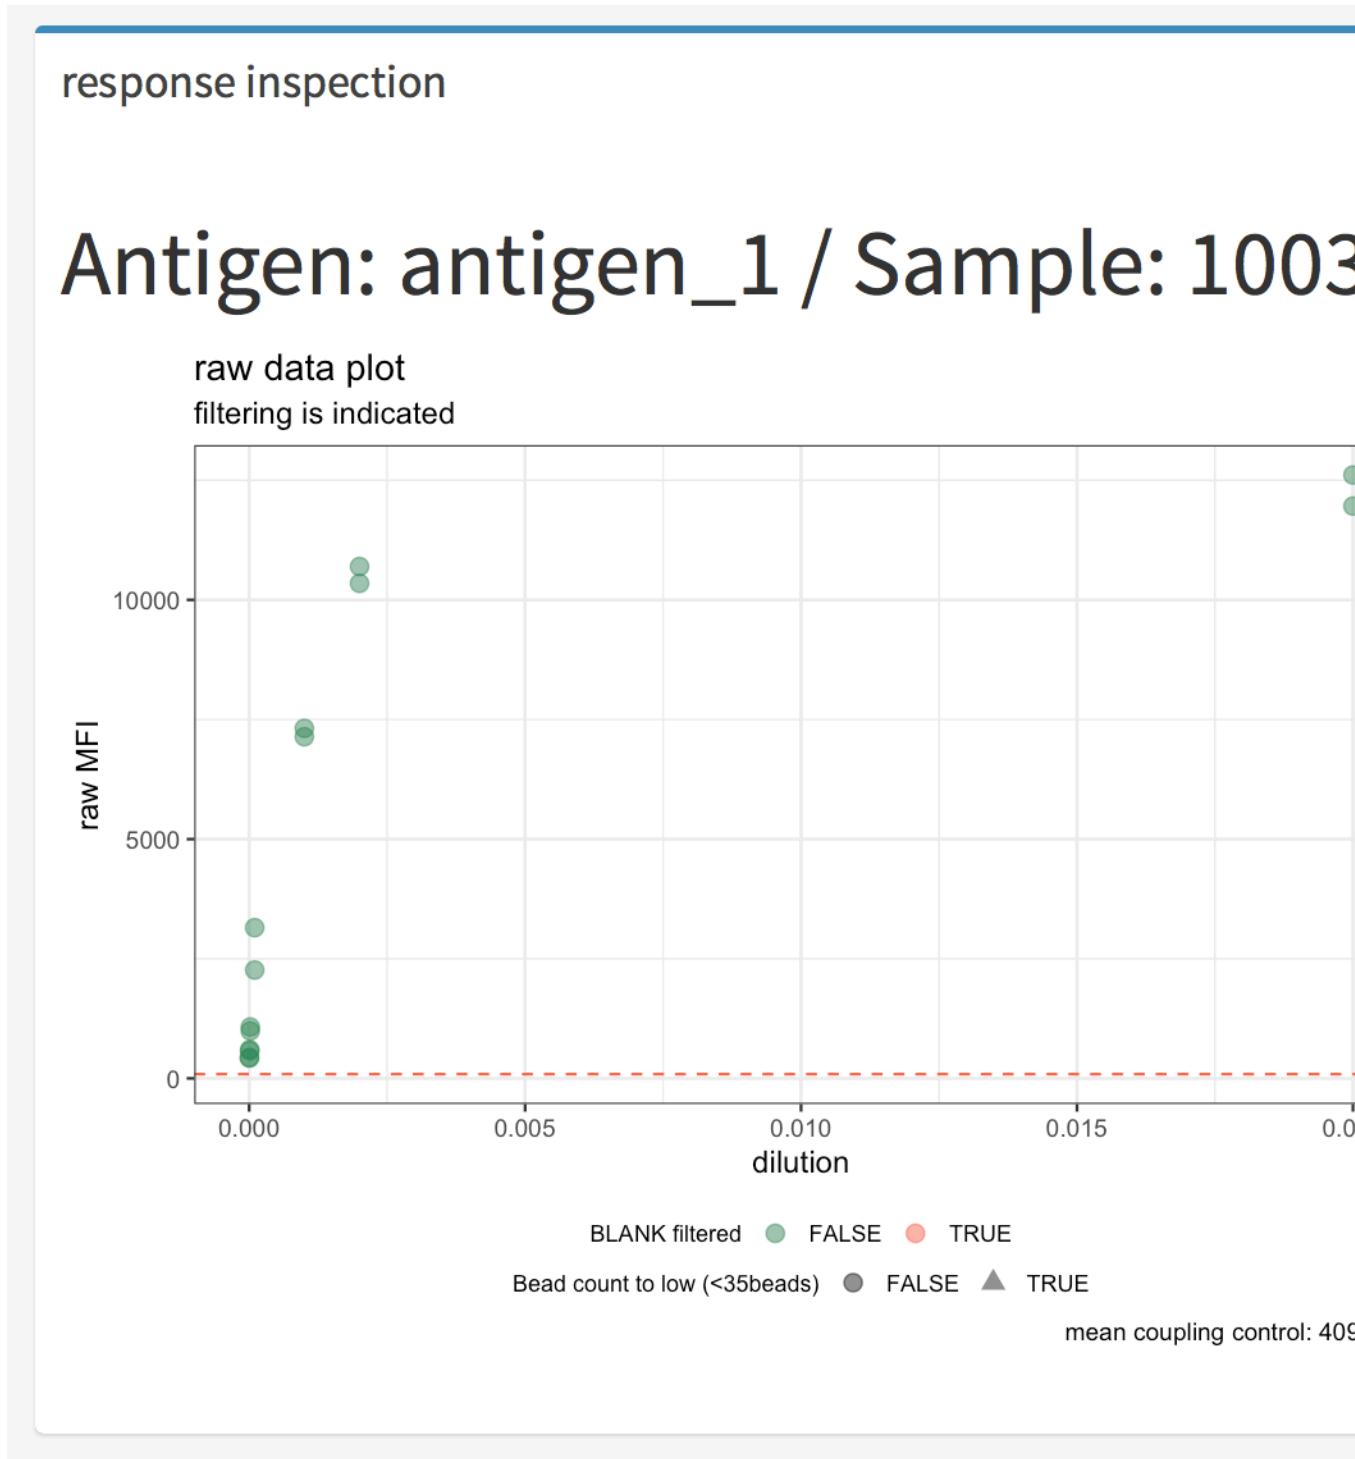


Figure 4.23: xMAPr analysis output data inspection » single antigen/sample combination fit inspection (antigen selection)

inspect xMAPr analysis output data inspection » single antigen/sample combination fit inspection (antigen selection)

inspect xMAPr analysis output data inspection » single antigen/sample combination fit inspection (log. scale)

When hitting the e.g. log. scale buttons the plots were generated using a log. scale on the selected axis (figure 4.24).

One method to choose the antigen and sample which should plotted are the drop down selection list (figure 4.23). In the elements the desired selection can also being typed in.

Another method to choose the antigen and sample which should plotted is to use the interactive data table in the lower panel of the inspect analysis/reponse (figure 4.25. The desired antigen/sample combination can be directly selected inside the table and when looking for a antigen or sample the search field is very helpful.

inspect xMAPr analysis output data inspection » single antigen/sample combination fit inspection (interactive data table)

In addition if the `highlight select antigen/sample combination in global plots?` is being switch on the selected antigen/sample combination is being marked in the global plots (figure 4.26 & 4.27).

xMAPr analysis output data inspection » single antigen/sample combination marked in global dynamic range plots over dilutions

xMAPr analysis output data inspection » single antigen/sample combination marked in global dynamic range plots

#### 4.1.3.5 statistical analysis of calculated response data (Screenshots)

The statistical data analysis is based on samples groups defined by the selected meta data. A wilcox rank sum test is performed using multiple test correction if the number of groups are more than two. The test statistics with p-value, adjusted p-value and confidence intervals etc. can be interactively inspected and the data is plotted using a violin plot with a bars indicating significant changes.

inspect xMAPr analysis output data inspection » statistical analysis using a wilcox ranked sum test on sample reponse data and the the selcted meta data for grouping

inspect xMAPr analysis output data inspection » statistical analysis using a wilcox ranked sum test on sample reponse data and the the selcted meta data for grouping (meta data selection)

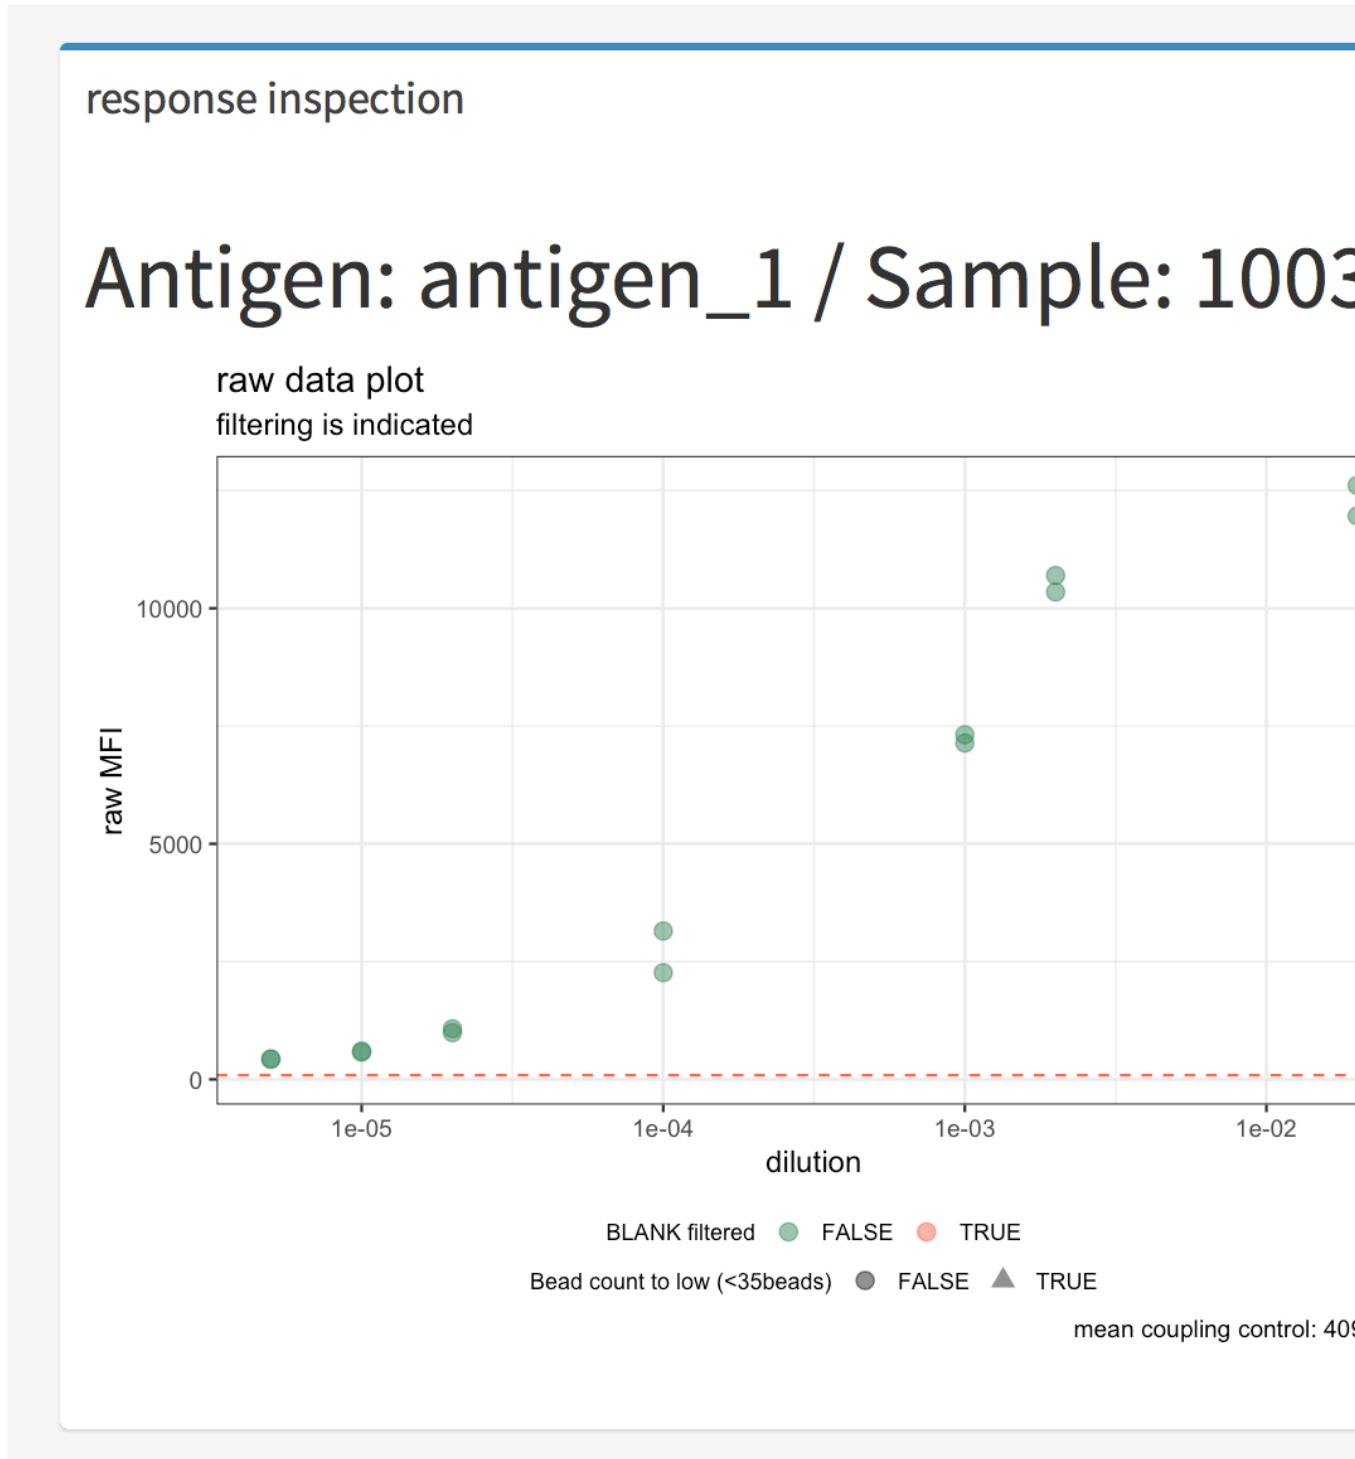


Figure 4.24: xMAPr analysis output data inspection » single antigen/sample combination fit inspection (log. scale)

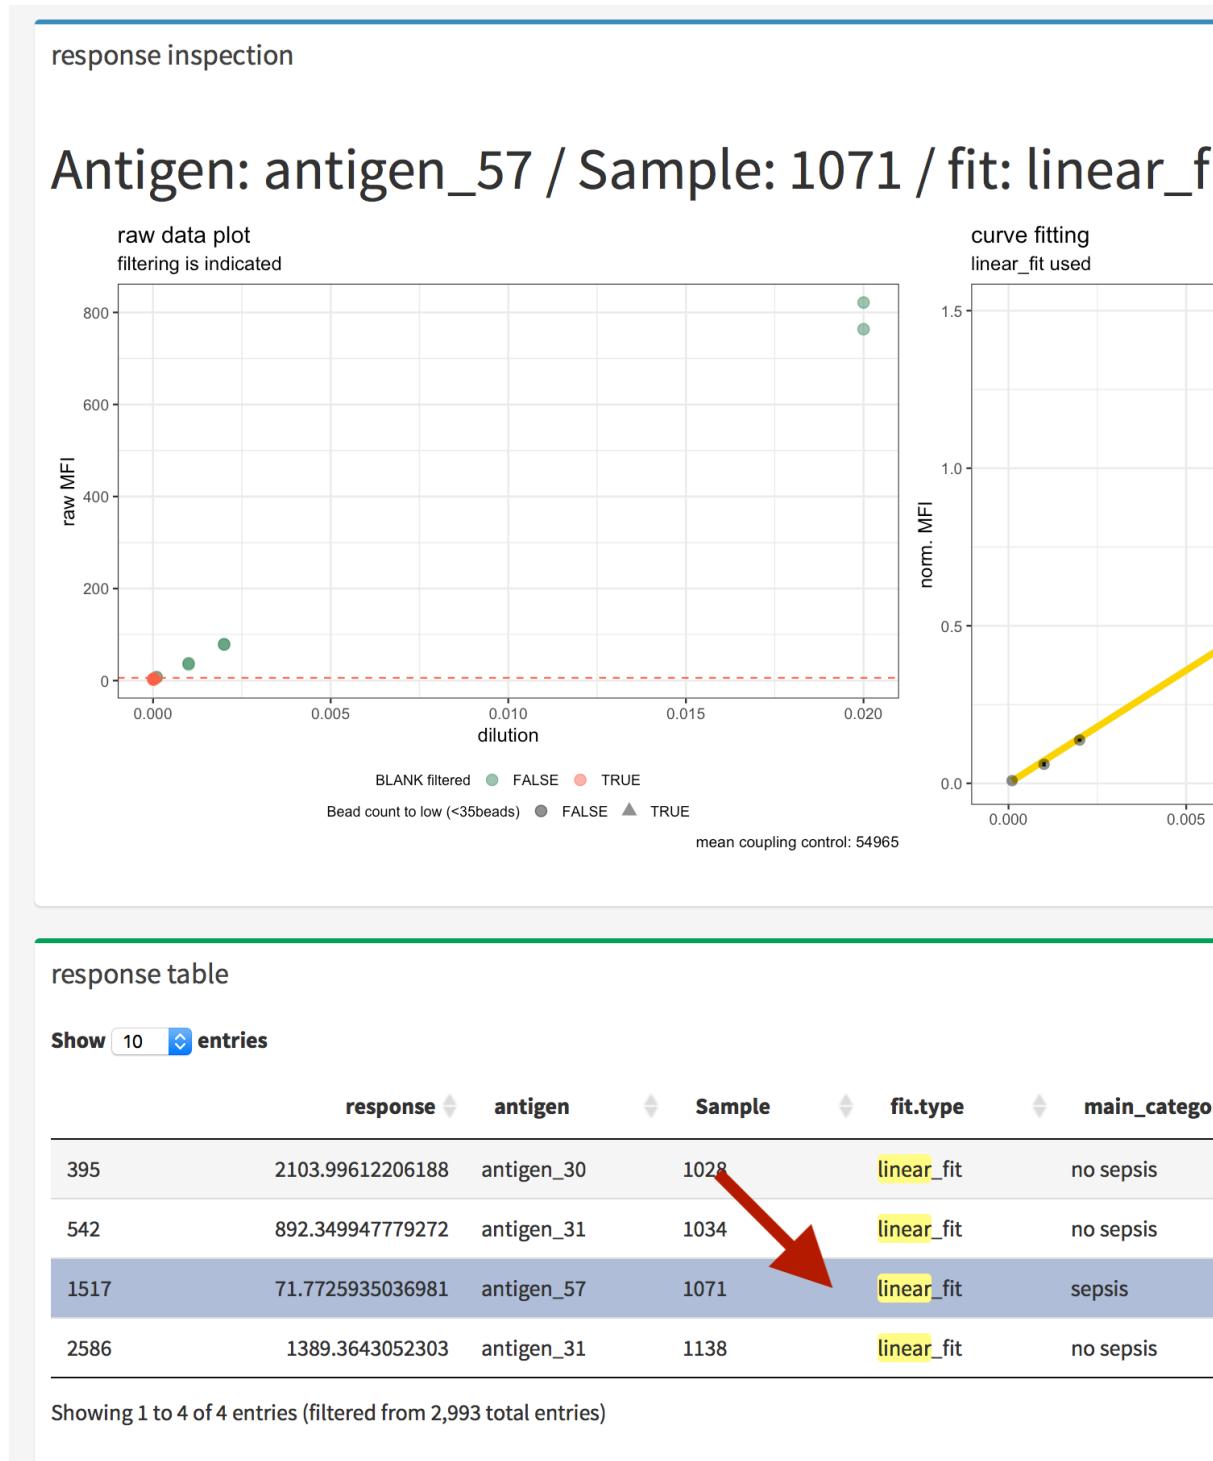


Figure 4.25: xMAPr analysis output data inspection » single antigen/sample combination fit inspection (interactive data table)

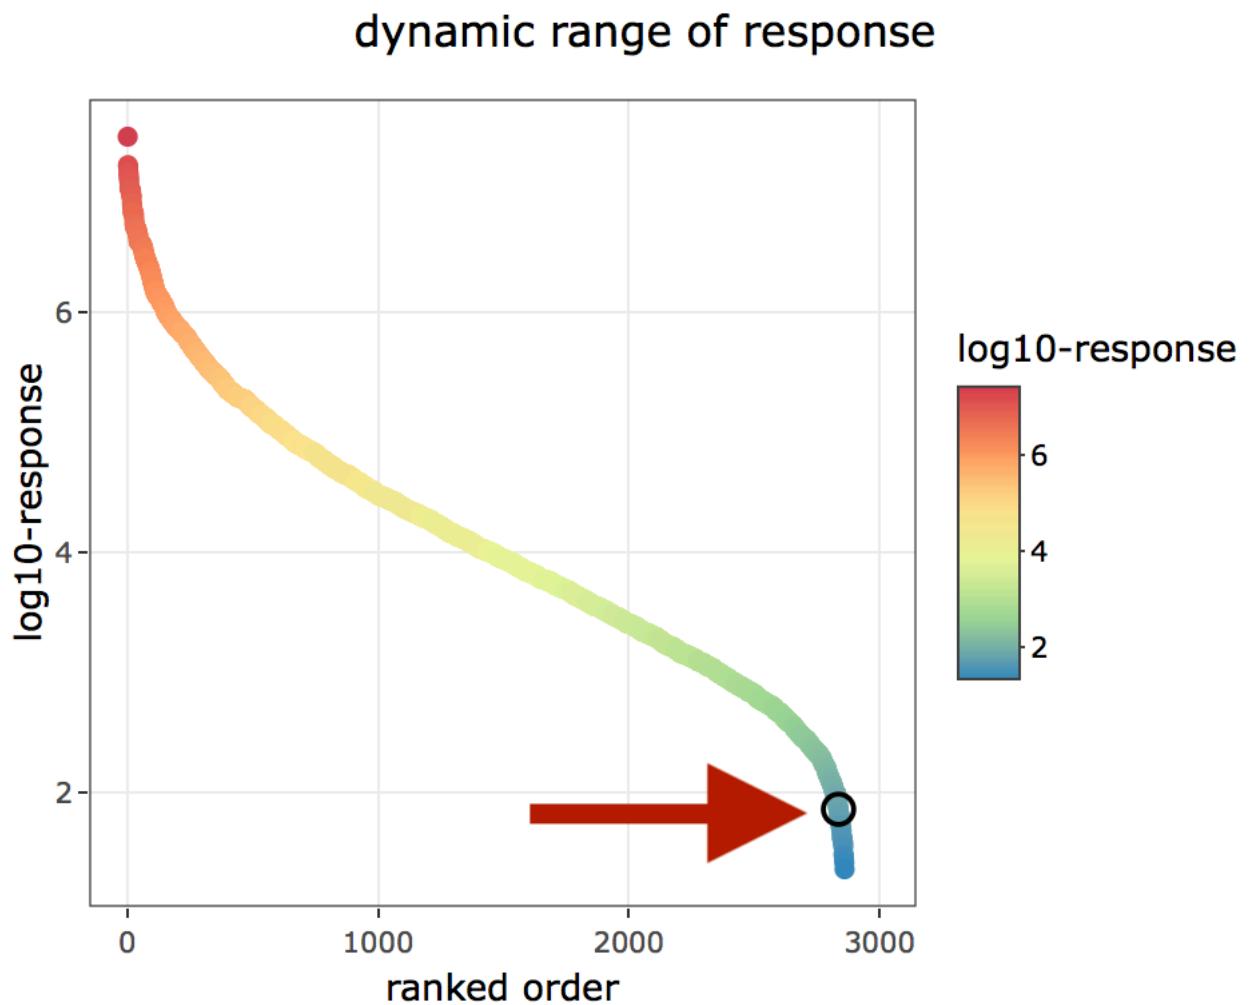


Figure 4.26: xMAPr analysis output data inspection » single antigen/sample combination marked in global dynamic range plots over dilutions

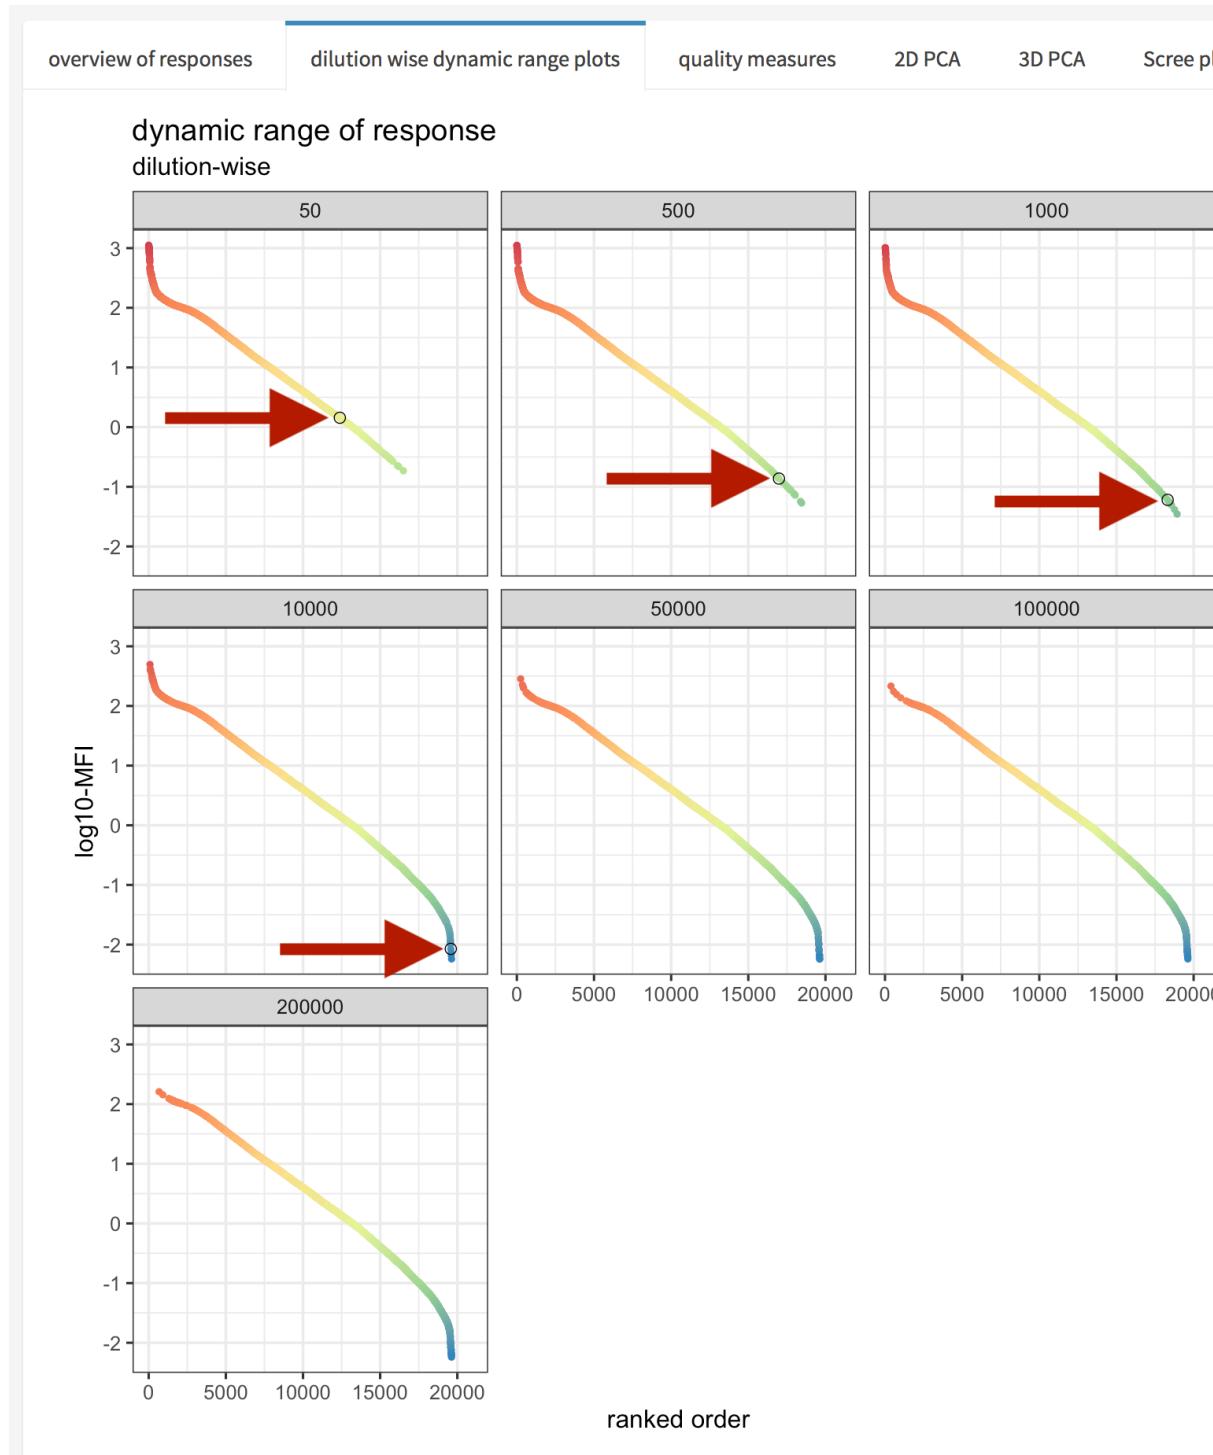


Figure 4.27: xMAPr analysis output data inspection » single antigen/sample combination marked in global dynamic range plots

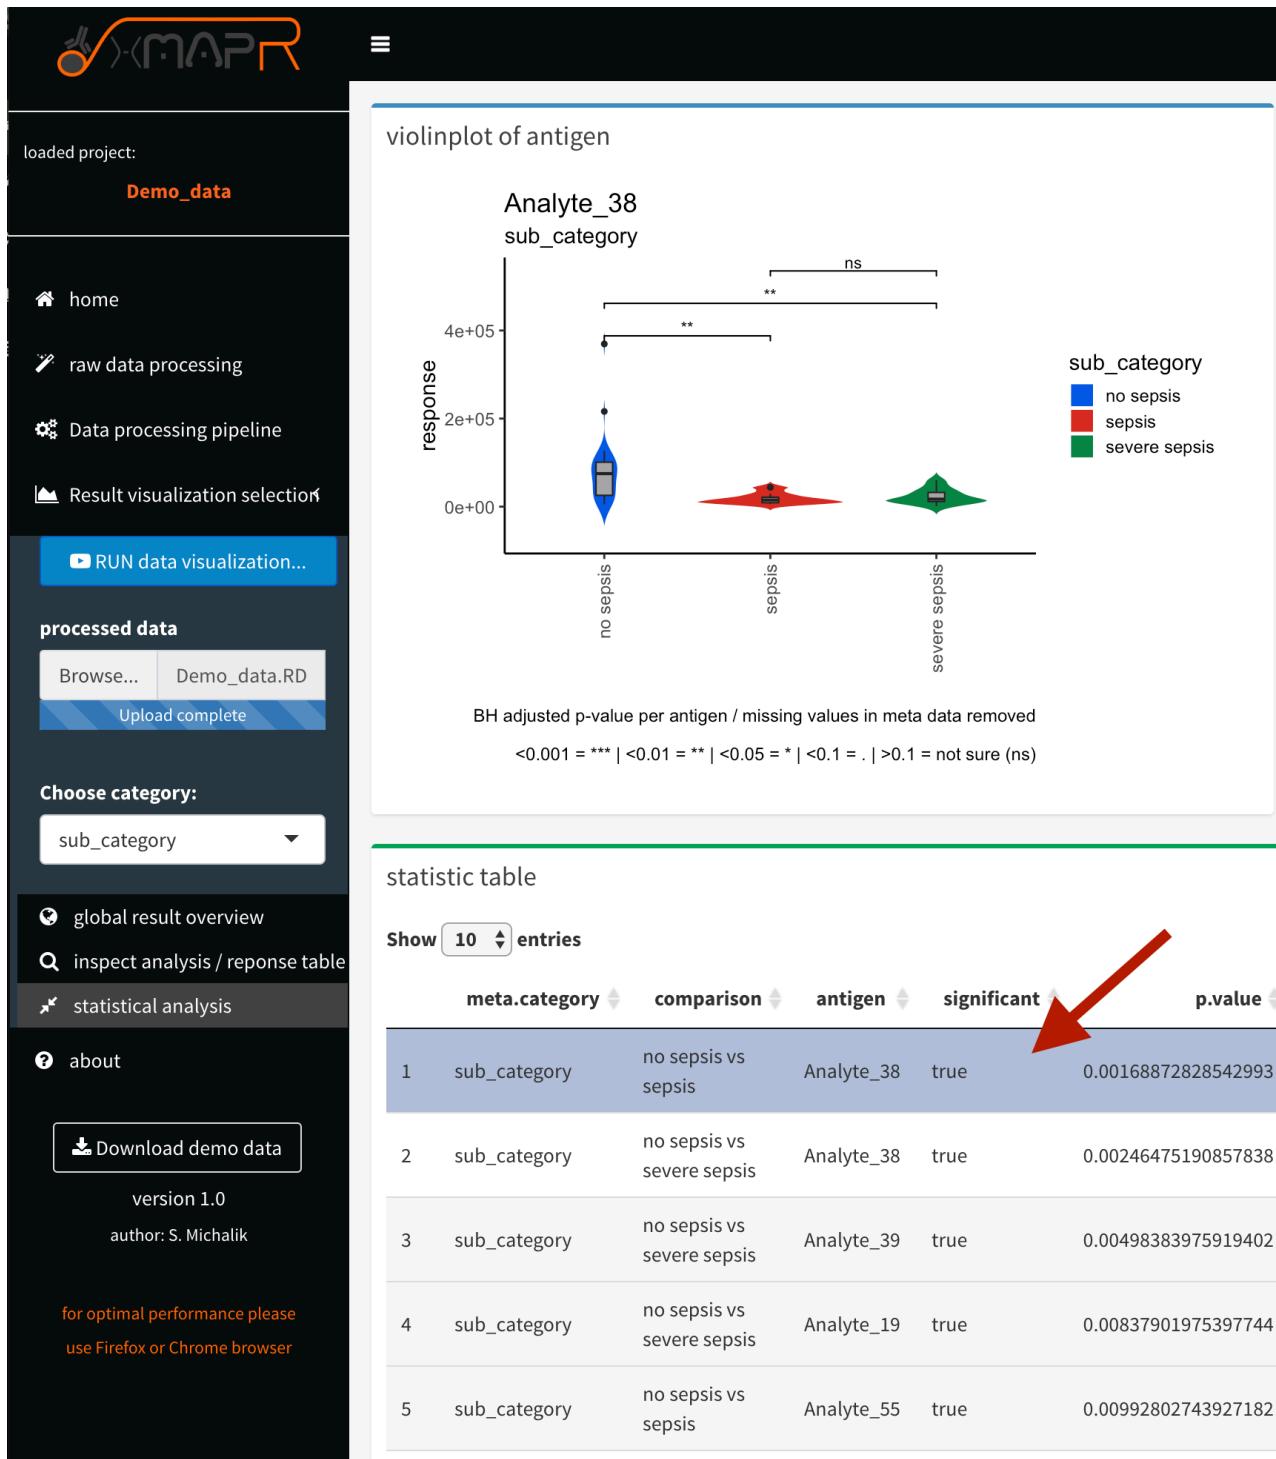


Figure 4.28: xMAPr analysis output data inspection » statistical analysis using a wilcoxon ranked sum test on sample response data and the selected meta data for grouping

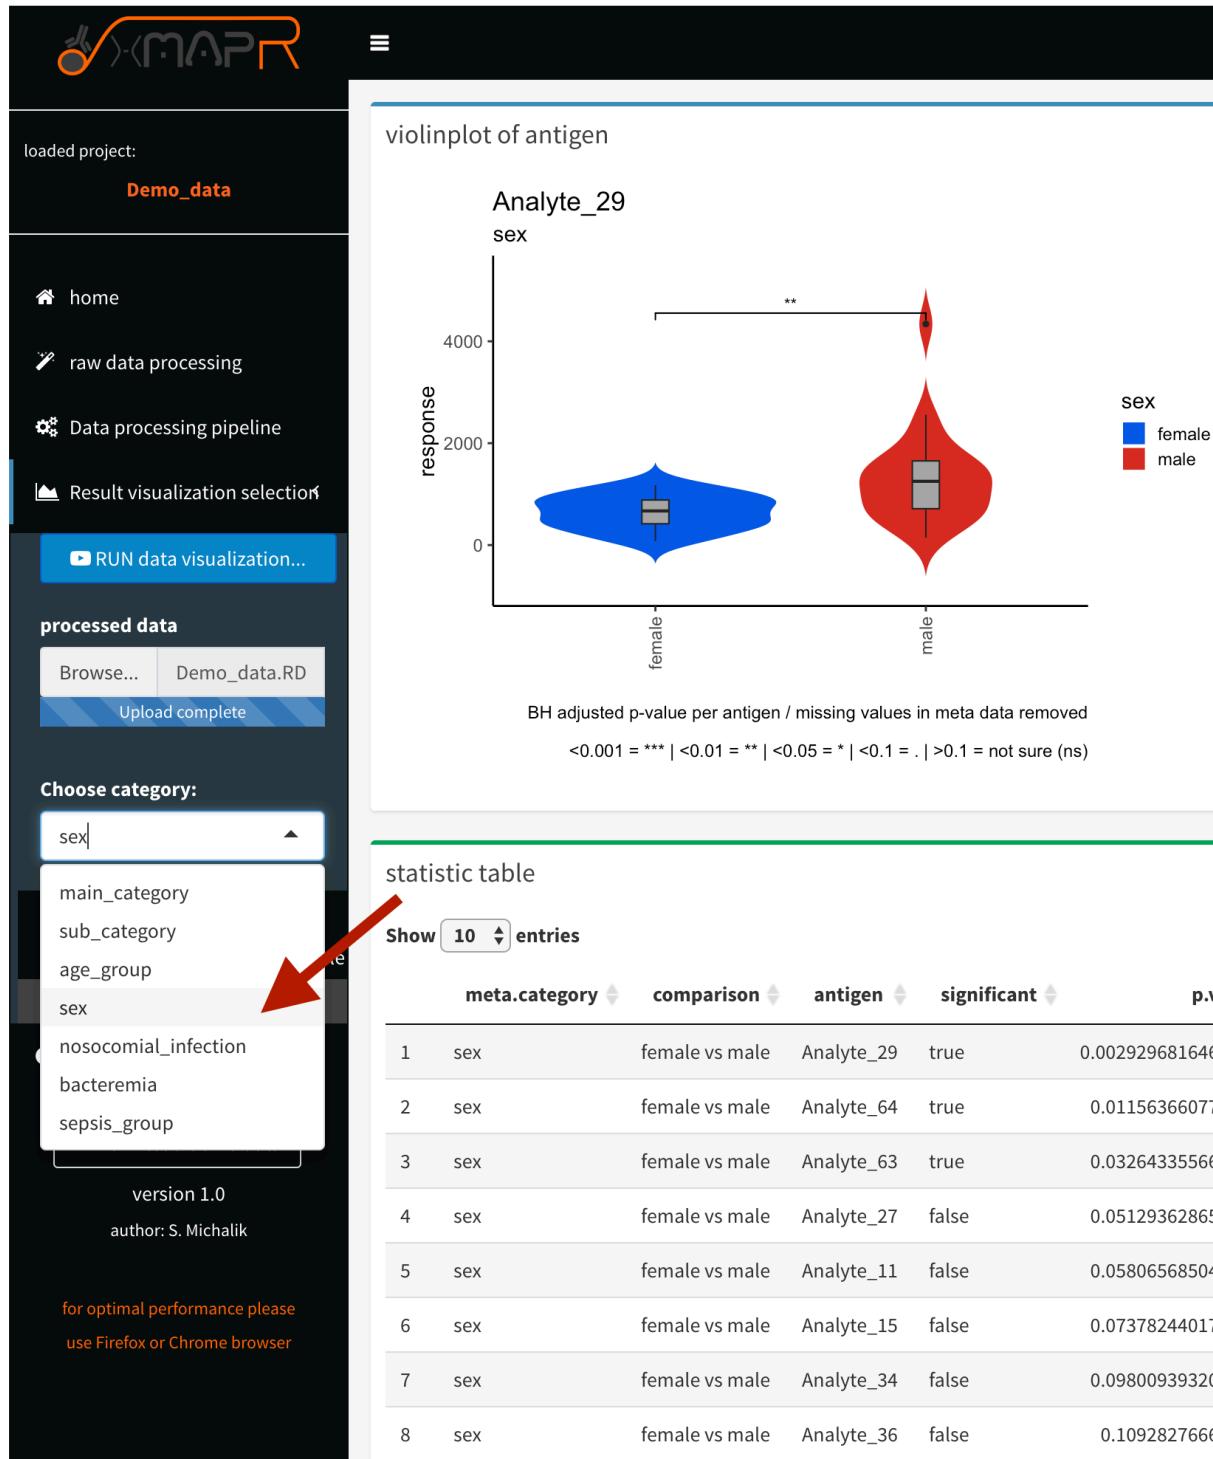


Figure 4.29: xMAPr analysis output data inspection » statistical analysis using a wilcoxon ranked sum test on sample response data and the selected meta data for grouping (meta data selection)

# Chapter 5

## used R-packages for xMAPr

- R: A Language and Environment for Statistical Computing (R Core Team [2022])
- bookdown: Authoring Books and Technical Documents with R Markdown (Xie [2023a])
- rmarkdown: Dynamic Documents for R (Allaire et al. [2023])
- data.table: Extension of `data.frame` (Dowle and Srinivasan [2023])
- DT: A Wrapper of the JavaScript Library ‘DataTables’ (Xie et al. [2023])
- factoextra: Extract and Visualize the Results of Multivariate Data Analyses (Kassambara and Mundt [2020])
- FactoMineR: Multivariate Exploratory Data Analysis and Data Mining (Husson et al. [2022])
- ggrepel: Automatically Position Non-Overlapping Text Labels with ‘ggplot2’ (Slowikowski [2023])
- ggsignif: Significance Brackets for ‘ggplot2’ (Ahlmann-Eltze and Patil [2022])
- gridExtra: Miscellaneous Functions for “Grid” Graphics (Auguie [2017])
- heatmaply: Interactive Cluster Heat Maps Using ‘plotly’ (Galili and O’Callaghan [2023])
- knitr: A General-Purpose Package for Dynamic Report Generation in R (Xie [2023b])
- magrittr: A Forward-Pipe Operator for R (Bache and Wickham [2022])
- minpack.lm: R Interface to the Levenberg-Marquardt Nonlinear Least-Squares Algorithm Found in MINPACK, Plus Support for Bounds (Elzhov et al. [2023])
- plotly: Create Interactive Web Graphics via ‘plotly.js’ (Sievert et al. [2022])
- RColorBrewer: ColorBrewer Palettes (Neuwirth [2022])
- reshape: Flexibly Reshape Data (?)
- reshape2: Flexibly Reshape Data: A Reboot of the Reshape Package (?)

- rlang: Functions for Base Types and Core R and ‘Tidyverse’ Features (Henry and Wickham [2023])
- scales: Scale Functions for Visualization (Wickham and Seidel [2022])
- shiny: Web Application Framework for R (Chang et al. [2022])
- shinyalert: Easily Create Pretty Popup Messages (Modals) in ‘Shiny’ (Attali and Edwards [2021])
- shinyBS: Twitter Bootstrap Components for Shiny (Bailey [2022])
- shinydashboard: Create Dashboards with ‘Shiny’ (Chang and Borges Ribeiro [2021])
- shinyFiles: A Server-Side File System Viewer for Shiny (Pedersen et al. [2022])
- shinyjs: Easily Improve the User Experience of Your Shiny Apps in Seconds (Attali [2021])
- shinyWidgets: Custom Inputs Widgets for Shiny (Perrier et al. [2023])
- tidyverse: Easily Install and Load the ‘Tidyverse’ (Wickham [2023])

# Bibliography

Constantin Ahlmann-Eltze and Indrajeet Patil. *ggsignif: Significance Brackets for ggplot2*, 2022. URL <https://CRAN.R-project.org/package=ggsignif>. R package version 0.6.4.

JJ Allaire, Yihui Xie, Jonathan McPherson, Javier Luraschi, Kevin Ushey, Aron Atkins, Hadley Wickham, Joe Cheng, Winston Chang, and Richard Iannone. *rmarkdown: Dynamic Documents for R*, 2023. URL <https://CRAN.R-project.org/package=rmarkdown>. R package version 2.20.

Dean Attali. *shinyjs: Easily Improve the User Experience of Your Shiny Apps in Seconds*, 2021. URL <https://deanattali.com/shinyjs/>. R package version 2.1.0.

Dean Attali and Tristan Edwards. *shinyalert: Easily Create Pretty Popup Messages (Modals) in Shiny*, 2021. URL <https://github.com/daattali/shinyalert><https://daattali.com/shiny/shinyalert-demo/>. R package version 3.0.0.

Baptiste Auguie. *gridExtra: Miscellaneous Functions for "Grid" Graphics*, 2017. URL <https://CRAN.R-project.org/package=gridExtra>. R package version 2.3.

Stefan Milton Bache and Hadley Wickham. *magrittr: A Forward-Pipe Operator for R*, 2022. URL <https://CRAN.R-project.org/package=magrittr>. R package version 2.0.3.

Eric Bailey. *shinyBS: Twitter Bootstrap Components for Shiny*, 2022. URL <https://ebailey78.github.io/shinyBS>. R package version 0.61.1.

Winston Chang and Barbara Borges Ribeiro. *shinydashboard: Create Dashboards with Shiny*, 2021. URL <http://rstudio.github.io/shinydashboard/>. R package version 0.7.2.

Winston Chang, Joe Cheng, JJ Allaire, Carson Sievert, Barret Schloerke, Yihui Xie, Jeff Allen, Jonathan McPherson, Alan Dipert, and Barbara Borges. *shiny: Web Application Framework for R*, 2022. URL <https://shiny.rstudio.com/>. R package version 1.7.4.

- Matt Dowle and Arun Srinivasan. *data.table: Extension of ‘data.frame’*, 2023. URL <https://CRAN.R-project.org/package=data.table>. R package version 1.14.8.
- Timur V. Elzhov, Katharine M. Mullen, Andrej-Nikolai Spiess, and Ben Bolker. *minpack.lm: R Interface to the Levenberg-Marquardt Nonlinear Least-Squares Algorithm Found in MINPACK, Plus Support for Bounds*, 2023. URL <https://CRAN.R-project.org/package=minpack.lm>. R package version 1.2-3.
- Tal Galili and Alan O’Callaghan. *heatmaply: Interactive Cluster Heat Maps Using plotly and ggplot2*, 2023. URL <https://CRAN.R-project.org/package=heatmaply>. R package version 1.4.2.
- Lionel Henry and Hadley Wickham. *rlang: Functions for Base Types and Core R and Tidyverse Features*, 2023. URL <https://CRAN.R-project.org/package=rlang>. R package version 1.1.0.
- Francois Husson, Julie Josse, Sebastien Le, and Jeremy Mazet. *FactoMineR: Multivariate Exploratory Data Analysis and Data Mining*, 2022. URL <http://factominer.free.fr>. R package version 2.7.
- Alboukadel Kassambara and Fabian Mundt. *factoextra: Extract and Visualize the Results of Multivariate Data Analyses*, 2020. URL <http://www.sthda.com/english/rpkgs/factoextra>. R package version 1.0.7.
- Erich Neuwirth. *RColorBrewer: ColorBrewer Palettes*, 2022. URL <https://CRAN.R-project.org/package=RColorBrewer>. R package version 1.1-3.
- Thomas Lin Pedersen, Vincent Nijs, Thomas Schaffner, and Eric Nantz. *shinyFiles: A Server-Side File System Viewer for Shiny*, 2022. URL <https://github.com/thomasp85/shinyFiles>. R package version 0.9.3.
- Victor Perrier, Fanny Meyer, and David Granjon. *shinyWidgets: Custom Inputs Widgets for Shiny*, 2023. URL <https://CRAN.R-project.org/package=shinyWidgets>. R package version 0.7.6.
- R Core Team. *R: A Language and Environment for Statistical Computing*. R Foundation for Statistical Computing, Vienna, Austria, 2022. URL <https://www.R-project.org/>.
- Carson Sievert, Chris Parmer, Toby Hocking, Scott Chamberlain, Karthik Ram, Marianne Corvellec, and Pedro Despouy. *plotly: Create Interactive Web Graphics via plotly.js*, 2022. URL <https://CRAN.R-project.org/package=plotly>. R package version 4.10.1.
- Kamil Slowikowski. *ggrepel: Automatically Position Non-Overlapping Text Labels with ggplot2*, 2023. URL <https://github.com/slowkow/ggrepel>. R package version 0.9.3.
- Hadley Wickham. *tidyverse: Easily Install and Load the Tidyverse*, 2023. URL <https://CRAN.R-project.org/package=tidyverse>. R package version 2.0.0.

- Hadley Wickham and Dana Seidel. *scales: Scale Functions for Visualization*, 2022. URL <https://CRAN.R-project.org/package=scales>. R package version 1.2.1.
- Yihui Xie. *bookdown: Authoring Books and Technical Documents with R Markdown*, 2023a. URL <https://CRAN.R-project.org/package=bookdown>. R package version 0.33.
- Yihui Xie. *knitr: A General-Purpose Package for Dynamic Report Generation in R*, 2023b. URL <https://yihui.org/knitr/>. R package version 1.42.
- Yihui Xie, Joe Cheng, and Xianying Tan. *DT: A Wrapper of the JavaScript Library DataTables*, 2023. URL <https://github.com/rstudio/DT>. R package version 0.27.