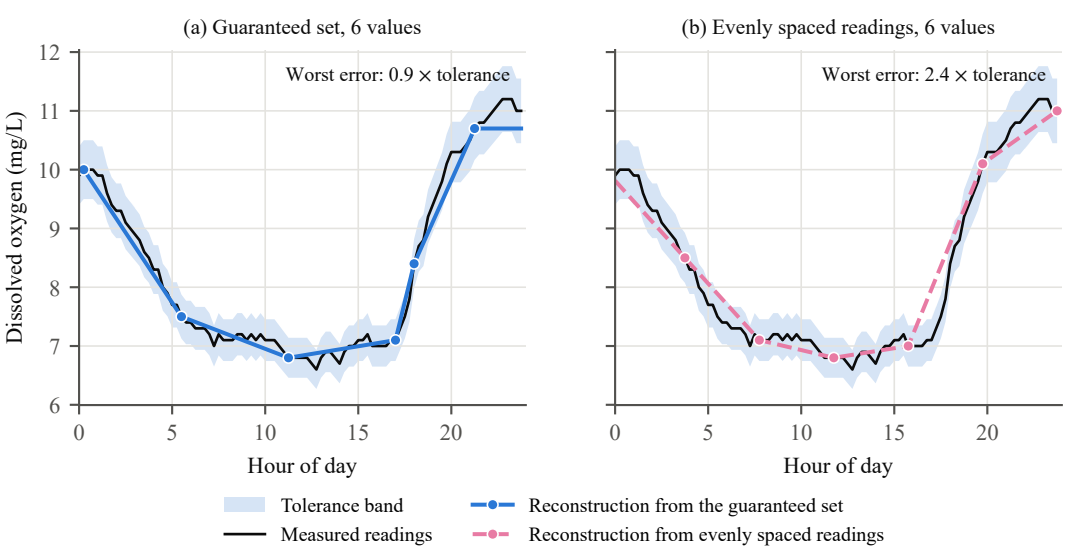
(a) Guaranteed set, 6 values
(b) Evenly spaced readings, 6 values
Worst error: 0.9 × tolerance
Worst error: 2.4 × tolerance
Dissolved oxygen (mg/L)
12
11
10
9
8
7
6
0
5
10
15
20
Hour of day
Hour of day
Tolerance band
Measured readings
Reconstruction from the guaranteed set
Reconstruction from evenly spaced readings