

COMMISSION ÉLECTROTECHNIQUE INTERNATIONALE
NORME DE LA CEI

INTERNATIONAL ELECTROTECHNICAL COMMISSION
IEC STANDARD

Publication 268-1
Deuxième édition — Second edition
1985

Equipements pour systèmes électroacoustiques
Première partie : Généralités

Sound system equipment
Part 1: General



- teknologisk service
- salg af elektrotekniske standarder
- abonnement på standardiseringsudvalg

DANSK ELEKTROTEKNISK KOMITE Tlf.: 31 57 50 50
Strandgade 36, 1401 København K Fax: 31 57 63 50



© CEI 1985

Aalborg universitetscenter
Universitetsbiblioteket

13 JUNI 1991

Droits de reproduction réservés — Copyright - all rights reserved

Bureau Central de la Commission Electrotechnique Internationale

3, rue de Varembé
Genève, Suisse

Le prix imprimé dans cette publication n'est plus valable. Veuillez consulter l'édition actuelle du Catalogue de la CEI.
The price printed in this publication is no longer valid. Please consult the current edition of the IEC Catalogue.

COMMISSION ÉLECTROTECHNIQUE INTERNATIONALE
NORME DE LA CEI

INTERNATIONAL ELECTROTECHNICAL COMMISSION
IEC STANDARD

Publication 268-1

Deuxième édition — Second edition

1985

Equipements pour systèmes électroacoustiques
Première partie : Généralités

Sound system equipment
Part 1: General



© CEI 1985

Droits de reproduction réservés — Copyright - all rights reserved

Aucune partie de cette publication ne peut être reproduite ni utilisée sous quelque forme que ce soit et par aucun procédé, électronique ou mécanique, y compris la photocopie et les microfilms, sans l'accord écrit de l'éditeur.

No part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the publisher.

Bureau Central de la Commission Electrotechnique Internationale

3, rue de Varembé
Genève, Suisse

Aalborg Universitetsbibliotek

530003023779

Prix Frs. 46



SOUND SYSTEM EQUIPMENT

Part 1: General

1. Scope

This standard applies to sound systems of any kind, and to the parts of which they are composed or which are used as auxiliaries to such systems.

This standard deals with the determination of the performance of sound system equipment, the comparison of these types of equipment and the determination of their proper practical application, by listing the characteristics which are useful for their specification and laying down uniform methods of measurements for these characteristics.

The standard is confined to a description of the different characteristics and the relevant methods of measurement; it does not in general specify performance (except in Part 10).

The complete standard consists of the following parts, in which the characteristics of various parts of sound systems and their methods of measurement are specified; some parts include preferred values:

- Part 1: General.
(Uniform characteristics and methods of measurement)
- Part 2: Explanation of General Terms.
(Explanation of general terms and calculation methods)
- Part 3: Sound System Amplifiers.
(Amplifiers forming part of a sound system for professional and domestic applications)
- Part 4: Microphones.
(Microphones in professional and domestic applications)
- Part 5: Loudspeakers.
(Loudspeakers in professional and domestic applications, treated as entirely passive elements)
- Part 6: Auxiliary Passive Elements.
(Attenuators, transformers, filters and equalizers, applied as separate units to be combined with other separate sound system units)
- Part 7: Headphones and Headsets.
(Headphones and headsets intended to be used on the human ear)
- Part 8: Automatic Gain Control Devices.
(Limiters and compressors)
- Part 9: Artificial Reverberation, Time Delay and Frequency Shift Equipment.
(Devices commonly employed to achieve special effects in sound systems)
- Part 10: Programme Level Meters
(Peak programme meters and vu-indicators)

- Part 11: Connectors for the Interconnection of Sound System Components.
(Application of connectors for the interconnection between parts of a sound system)
- Part 12: Circular Connectors for Broadcast and Similar Use.
(Application of connectors for the interconnection between parts of a broadcast or similar professional system)
- Part 13: Listening Test on Loudspeakers.
(Listening tests and objective methods for rating the quality of the transmission systems)
- Part 14: Circular and Elliptical Loudspeakers; Outer Frame Diameters and Mounting Dimensions.
(Dimensional characteristics of single moving-coil (dynamic) loudspeakers)
- Part 15: Preferred Matching Values for the Interconnection of Sound System Components.
(Preferred electrical values for the correct interconnection of sound system components)

2. Units and system of measurement

The International System of Units (SI units) as given in IEC Publication 27: Letter Symbols to be Used in Electrical Technology, is used exclusively in this standard.

3. Frequencies of measurement

If measurements are to be made at discrete frequencies, then these shall be the frequencies specified as preferred frequencies for acoustical measurements in ISO Standard 266, reproduced in Table I. If a measurement relates to a reference frequency, then, in the absence of a clear reason to the contrary, this shall be the standard reference frequency of 1 000 Hz.

If a measurement is to be made using only one signal frequency, the signal frequency shall be the chosen reference frequency. If measurements are to be made at a number of different frequencies, the chosen reference frequency shall be included, the other frequencies being so chosen that the results of the measurements give an adequate representation of the behaviour of the characteristics over the whole of the effective frequency range.

If measurements are to be made in frequency bands of constant relative bandwidth, preference shall be given to the one-octave and one-third octave bands mentioned in Sub-clause 6.2.3.

4. Quantities to be specified and their accuracy

Unless otherwise stated, the values of voltage, current, sound pressure, etc., mentioned in this standard are assumed to be r.m.s. quantities. For most purposes it is sufficient to measure electrical quantities with an accuracy of ± 0.15 dB and acoustical quantities with an accuracy of ± 1 dB. The accuracy of measurement required depends only on the purpose for which the results are to be used.

5. Marking and symbols for marking

5.1 Marking

Terminals and controls shall be adequately marked to give information regarding their function, characteristics and polarity.

The marking shall be such that it must be possible to adjust the controls and to identify their positions with sufficient accuracy in connection with the information given in the user instructions.

5.2 Symbols for marking

Marking should preferably be composed of letter symbols, signs, numbers and colours, which are internationally intelligible. Reference is made to IEC Publication 27, IEC Publication 617: Graphical Symbols for Diagrams, and IEC Publication 417: Graphical Symbols for Use on Equipment. Index, Survey and Compilation of the Single Sheets.

Markings not included in the above-mentioned standards shall be clearly explained in the user instructions.

6. Filters, weighting curves and meters for noise specification and measurement

A specification of noise or signal-to-noise ratio shall refer to noise measured by one of the following methods:

6.1 Wide-band measurement

The filter shall be a band-pass filter having a frequency response within the limits shown in Figure 5, page 24. (This is identical to the wide-band filter specification in CCIR Recommendation 468-3.)

A band-pass filter which has a substantially constant transmission factor between 22.4 Hz and 22.4 kHz, decreasing outside this frequency band at the rates specified for octave-band filters having mid-band frequencies of 31.5 Hz and 16 000 Hz specified in IEC Publication 225: Octave, Half-octave and Third-octave Band Filters intended for the Analysis of Sound and Vibrations, has a response falling within the limits of this specification.

Note. — Care should be taken when there may be strong signals just above or below the band-limits since in this case the results will depend, to some degree, on the individual frequency response of the filter actually used.

6.2 Weighted measurements

6.2.1 Noise (A-weighting) or signal-to-noise (A-weighting) ratio

The filter used shall have A-weighting characteristics with tolerances type 1 as specified for sound level measurements in IEC Publication 651: Sound Level Meters. The meter shall be a true r.m.s. meter as described in Publication 651 for sound level meters type 1; the dynamic characteristic designated "S" shall be used.

Note. — A-weighted measurements are particularly appropriate where the noise output from the equipment in the absence of a programme is concerned.

6.2.2 Noise (*psophometric*) or signal-to-noise (*psophometric*) ratio

The filter and meter used shall have the characteristics described in Appendix A, which are identical to those specified in CCIR Recommendation 468-3.

Notes 1. — The word “*psophometric*” may be abbreviated to “*ps*” (see CCITT Recommendation J.16) if no confusion may arise.

2. — Psophometric measurements are particularly appropriate where the disturbing effect of the noise output from the system in the presence of a programme is concerned.

6.2.3 Octave/third-octave band measurements

The filters shall have characteristics as specified for octave or third-octave band filters in IEC Publication 225. The meter shall be a true r.m.s. meter as described in IEC Publication 651 for sound level meters, type 1. When measuring in narrow bands, particularly at low frequencies, it is recommended that the instruments should conform dynamically to the characteristics designated “S” for the sound level meter.

7. Simulated programme signal

A signal, whose mean power spectral density closely resembles the average of the mean power spectral densities of a wide range of programme material, including both speech and music of several kinds, is stationary weighted Gaussian noise without amplitude limiting, the weighted power spectrum being in accordance with Table II and Figure 1, page 22, when measured with third-octave filters in accordance with IEC Publication 225.

Such a signal may be obtained from a pink-noise source by means of the filter circuit shown in Figure 2, page 22.

Measurements made with narrow-band signals shall, if appropriate, be made with the relative level in each frequency band corresponding to that indicated in Table II and Figure 1. (Measurements and characteristics related to the use of this signal, especially for amplifiers and loudspeakers, are under consideration.)

Note. — It should be noted that the power level of the signal measured over the full frequency range is approximately 12.5 dB higher than the indicated zero relative level, which is measured over $\frac{1}{3}$ octave.

8. Climatic conditions

Measurements and mechanical checks may be carried out at any combination of temperature, humidity and air pressure within the following limits:

- Ambient temperature: 15 °C to 35 °C, preferably at 20 °C
- Relative humidity: 25% to 75%
- Air pressure: 86 kPa to 106 kPa (860 mbar to 1 060 mbar)

If the manufacturer finds it necessary to specify climatic conditions differing from the above these should be chosen from IEC Publication 68: Basic Environmental Testing Procedures, and the measurements shall be made under these specified conditions.

The conditions mentioned above represent those under which the equipment is required to meet its specification. Over a wider range the equipment may operate but not meet all of its specifications and it may be permissible to store the equipment under much more extreme conditions.

For a more complete discussion of these concepts, reference is made to IEC Publication 68.

9. Individual specification and type specification

Values may be specified either for a general type or for an individual sample of this type.

In the first case, the manufacturer shall state whether the specified values are:

- limits,
- statistical “worst case” values (see note),
- average values (see note).

Note. — These values are derived from measurements on a batch and accompanied by the data required to render them significant, see the relevant ISO standards on sampling procedures.

10. Graphical presentation of data

10.1 General

The relation between two or more quantities is often more clearly presented as a graph rather than as a table.

When the results of a point-to-point measurement for an individual sample are presented as a continuous curve, the measured points shall be clearly indicated. Extrapolated or intermediate curves based on theoretical expectations or other information presented, but not based on direct measurement, shall be clearly distinguished from measurement curves, for example by another style of drawing.

Where appropriate, data may be presented as a line or band spectrum of constant bandwidth or constant proportional bandwidth. The bandwidth used shall be stated. Preference shall be given to one octave and one-third octave bands as mentioned in Sub-clause 6.2.3.

10.2 Scales

Linear or logarithmic scales are recommended for graphical presentation. Other kinds of scales, such as double logarithmic and combinations of linear and logarithmic, should be avoided. Linear decibel scales are equivalent to logarithmic scales.

Where quantities represented by abscissa and ordinate are of the same kind, the same unit length should be used for both. A remote zero point in linear scales should be avoided as far as possible. The zero reference in a decibel scale should, if possible, be the rated value.

10.3 Logarithmic scales and polar diagrams

For logarithmic frequency scales and polar level diagrams reference is made to I E C Publication 263: Scales and Sizes for Plotting Frequency Characteristics and Polar Diagrams.

10.3.1 Logarithmic frequency scales

For graphs in which a level (in decibels) is plotted against frequency on a logarithmic scale, the scale proportions shall be those for which the length for a 10:1 frequency ratio is equal to the length for a level difference of 50 dB on the ordinate scale.

Note. — The alternative values of level difference (10 dB and 25 dB per decade) given in I E C Publication 263 are not prohibited.

10.3.2 Polar level diagrams

For polar plots in which a level in decibels is shown increasing outward along a radius on a linear scale, the maximum level shall preferably be plotted on, or within 2.5 dB of, the reference circle whose radius corresponds to a difference in level of 25 dB. The tolerance limits on the radius of the reference circle correspond to ± 0.25 dB. These requirements apply for whatever length is chosen to represent 1 dB.

For an absolute level, when the radius of the reference circle corresponds to 25 dB, the level assigned to the reference circle shall be a multiple of 5 dB.

Note. — If it is necessary to plot a characteristic over a range greater than 25 dB, then a difference in level of 50 dB should be used.

11. Personal safety and prevention of spread of fire

Reference is made to IEC Publication 65: Safety Requirements for Mains Operated Electronic and Related Apparatus for Household and Similar General Use, or to other appropriate IEC safety standards.

12. Measurements in a uniform alternating magnetic field

12.1 Method of producing a uniform alternating magnetic field

A convenient and fairly accurate method of producing a uniform alternating magnetic field makes use of the arrangement of three square coils according to Figure 3, page 23, in which $a = 0.375 b$, where a is the distance between the coils and b the dimension of the side of each coil. The coils are supplied with a current at the required frequency.

Between the three coils 1, 2 and 3 having turns in the ratios of:

$$\frac{n_1}{100} = \frac{n_2}{36} = \frac{n_3}{100}$$

when the same current I flows through each coil in the same direction, a field is produced that may be considered to be uniform to within $\pm 2\%$, inside a spherical space having a diameter of $d = 0.5 b$, the centre of which coincides with the geometrical centre of coil 2.

The resulting magnetizing force H and field strength B will be approximately:

$$H = 1.35 \frac{n_1 I}{b} \text{ A/m} \quad B = 1.70 \frac{n_1 I}{b} \mu\text{T}$$

The magnetic field strength shall be measured before the device is placed into the field. This can be done with a search coil, in accordance with Sub-clause 12.2.

12.2 Measuring the magnetic field strength

For measuring the magnetic field strength, the use of a search coil, according to Figure 4, page 23, is recommended, which will produce an e.m.f. of 1 mV in a magnetic field with a strength of 1 A/m at a frequency of 50 Hz, the voltage being proportional to both the magnetic field strength and the frequency.

The search coil output voltage should also be measured with the magnetic field switched off. If the output voltage under these conditions exceeds one third of the output voltage with the field present, a selective measurement is required. If possible, the search coil output voltage should be measured using a voltmeter with balanced input.

12.3 Positioning the sample

The sample under test shall be placed in the magnetic field and the position of the sample relative to the pattern of the field shall be varied until the interference is at maximum.

The sample under test shall not project from the spherical space of diameter d .

TABLE I

Frequencies conforming to ISO Standard 266

The table may be extended in either direction by successive multiplication or division by 1 000. The sign \times indicates in each column the geometric mean frequencies of the filters mentioned in Clause 6.

Preferred frequencies	$1/1$ octave	$1/2$ octave	$1/3$ octave	Preferred frequencies	$1/1$ octave	$1/2$ octave	$1/3$ octave	Preferred frequencies	$1/1$ octave	$1/2$ octave	$1/3$ octave
16	\times	\times	\times	160			\times	1 600			\times
18				180		\times		1 800			
20			\times	200			\times	2 000			
22.4		\times		224				2 240		\times	
25			\times	250	\times	\times	\times	2 500			
28				280				2 800		\times	
31.5	\times	\times	\times	315			\times	3 150			
35.5				355		\times		3 550			
40			\times	400			\times	4 000		\times	
45		\times		450				4 500			
50			\times	500	\times	\times	\times	5 000			
56				560				5 600		\times	
63	\times	\times	\times	630			\times	6 300			
71				710		\times		7 100			
80			\times	800			\times	8 000		\times	
90		\times		900				9 000			
100				1 000	\times	\times	\times	10 000			
112				1 120				11 200			
125	\times	\times	\times	1 250			\times	12 500			
140				1 400		\times		14 000			
160			\times	1 600			\times	16 000	\times	\times	\times

Note. — The exact preferred frequencies calculated from $1 000 \times 10^{3n/10}$ for octave band filters, $1 000 \times 10^{3n/20}$ for half-octave band filters and $1 000 \times 10^{n/10}$ for third-octave band filters where n is a positive or negative integer, or zero, are to be used for the design of filters rather than the nominal values given in the table.

For normal acoustical measurements, the difference between the nominal and the exact frequencies is negligible.

TABLE II

Power spectrum of simulated programme signal

Frequency (Hz)	Relative level (dB)	Tolerance limits (dB)		Frequency (Hz)	Relative level (dB)	Tolerance limits (dB)	
		+	-			+	-
20	-13.5	3.0	3.0	630	0	0.5	0.5
25	-10.2	2.0	2.0	800	0	0.5	0.5
31.5	-7.4	1.0	1.0	1 000	-0.1	0.6	0.6
40	-5.2	1.0	1.0	1 250	-0.3	0.7	0.7
50	-3.5	1.0	1.0	1 600	-0.6	0.8	0.8
63	-2.3	1.0	1.0	2 000	-1.0	1.0	1.0
80	-1.4	1.0	1.0	2 500	-1.6	1.0	1.0
100	-0.9	0.8	0.8	3 150	-2.5	1.0	1.0
125	-0.5	0.6	0.6	4 000	-3.7	1.0	1.0
160	-0.2	0.5	0.5	5 000	-5.1	1.0	1.0
200	-0.1	0.5	0.5	6 300	-7.0	1.0	1.0
250	0	0.5	0.5	8 000	-9.4	1.0	1.0
315	0	0.5	0.5	10 000	-11.9	1.0	1.0
400	0	0.5	0.5	12 500	-14.8	1.5	1.5
500	0	0.5	0.5	16 000	-18.2	2.0	2.0
630	0	0.5	0.5	20 000	-21.6	3.0	3.0


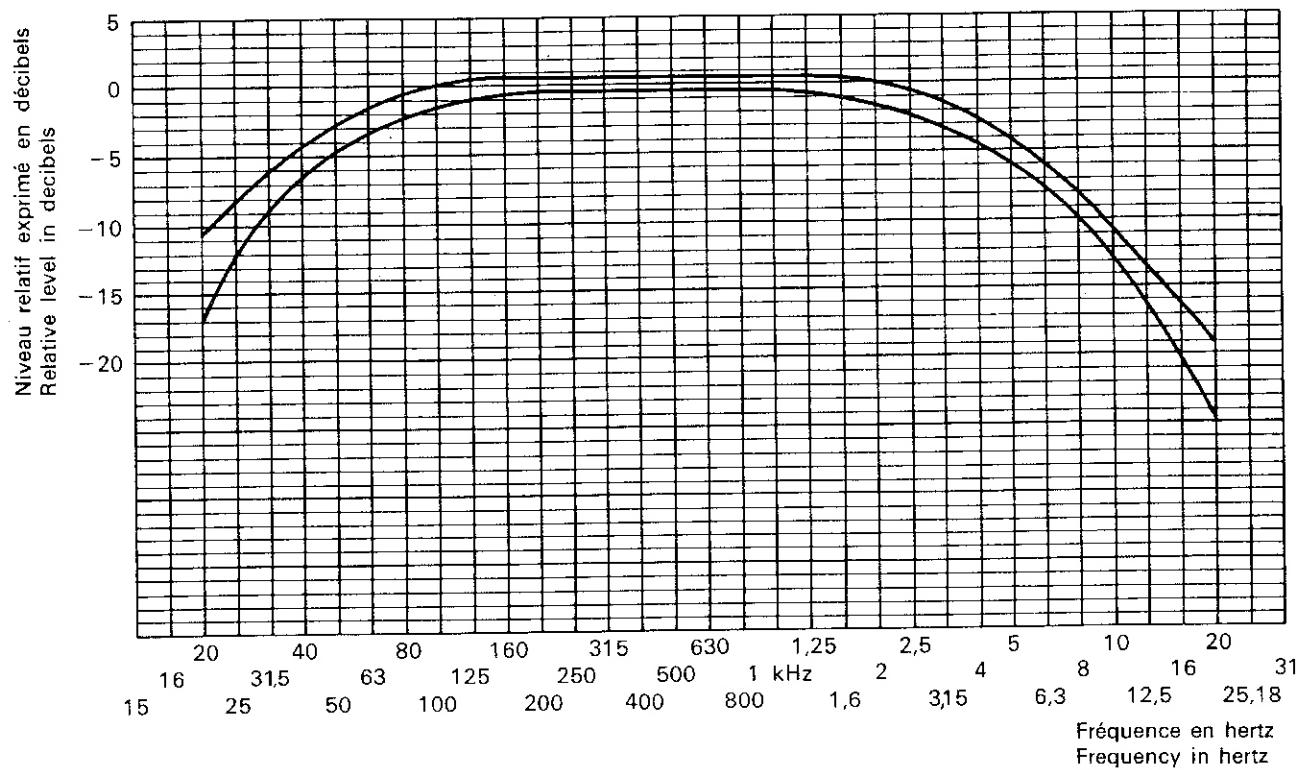


FIG. 1. — Spectre de puissance d'un signal pour simulation de programme.
Power spectrum of simulated programme signal.

446/81

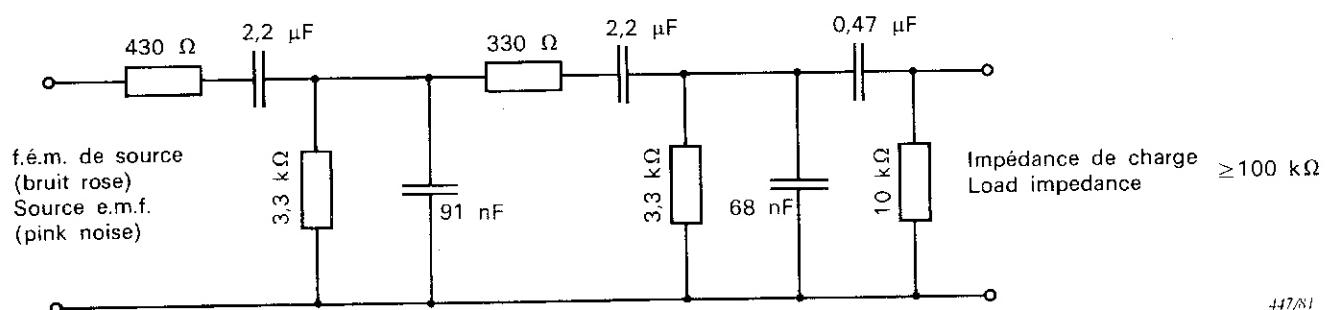

La valeur de l'impédance de sortie de la source doit être comprise dans la valeur de la première résistance (430Ω). L'effet de l'impédance de charge peut être pris en compte en réglant la valeur de la résistance de $10 \text{ k}\Omega$.

Il convient que la tangente de l'angle de perte des condensateurs ne soit pas supérieure à 0,005.

The output impedance of the source shall be included in the value of the first resistor (430Ω). The effect of the load impedance may be taken into account by adjusting the value of the $10 \text{ k}\Omega$ resistor.

The tangent of loss angle of the capacitors shall not exceed 0,005.

FIG. 2. — Filtre destiné au signal pour simulation de programme (source de bruit rose).
Filter for simulated programme signal (for pink-noise source).

447/81

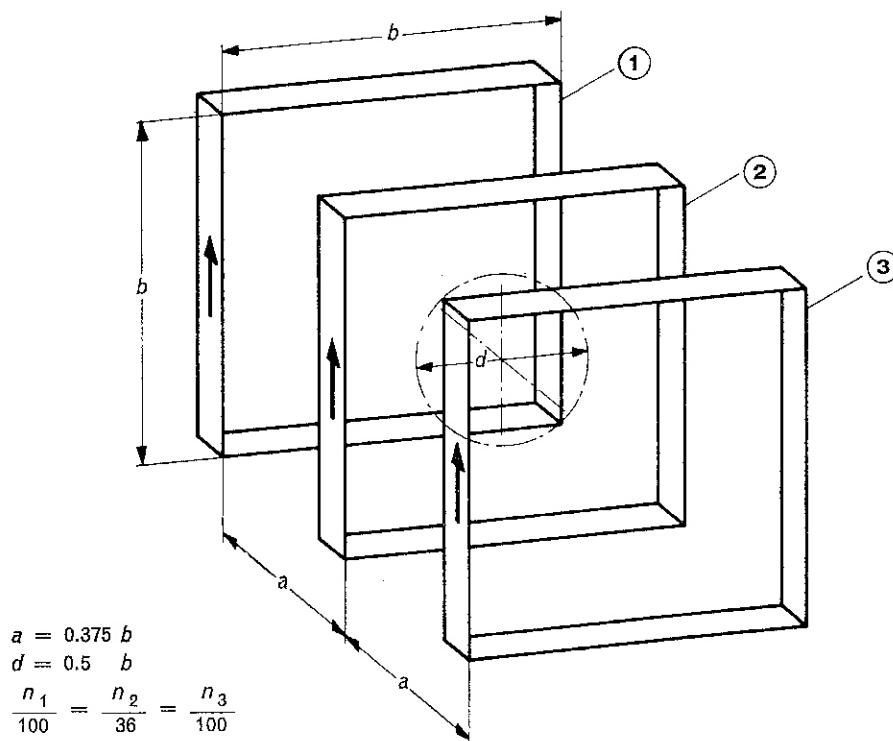


FIG. 3. — Disposition des trois bobines pour la production d'un champ magnétique alternatif uniforme.

Arrangement of three coils for the production of a uniform alternating magnetic field.

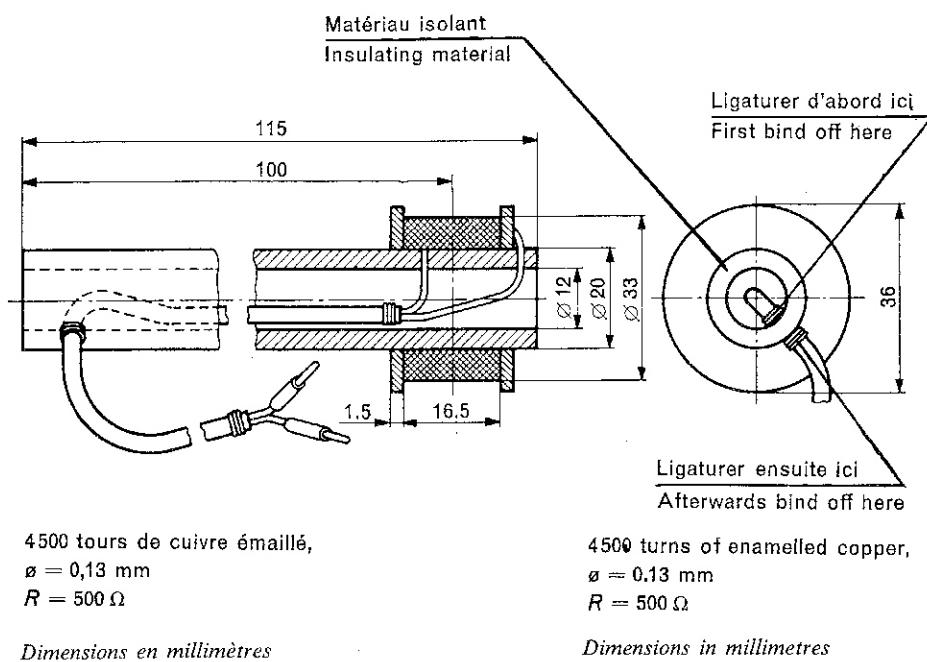


FIG. 4. — Bobine exploratrice pour la mesure de l'intensité des champs magnétiques.
Search coil for measuring the magnetic field strength.

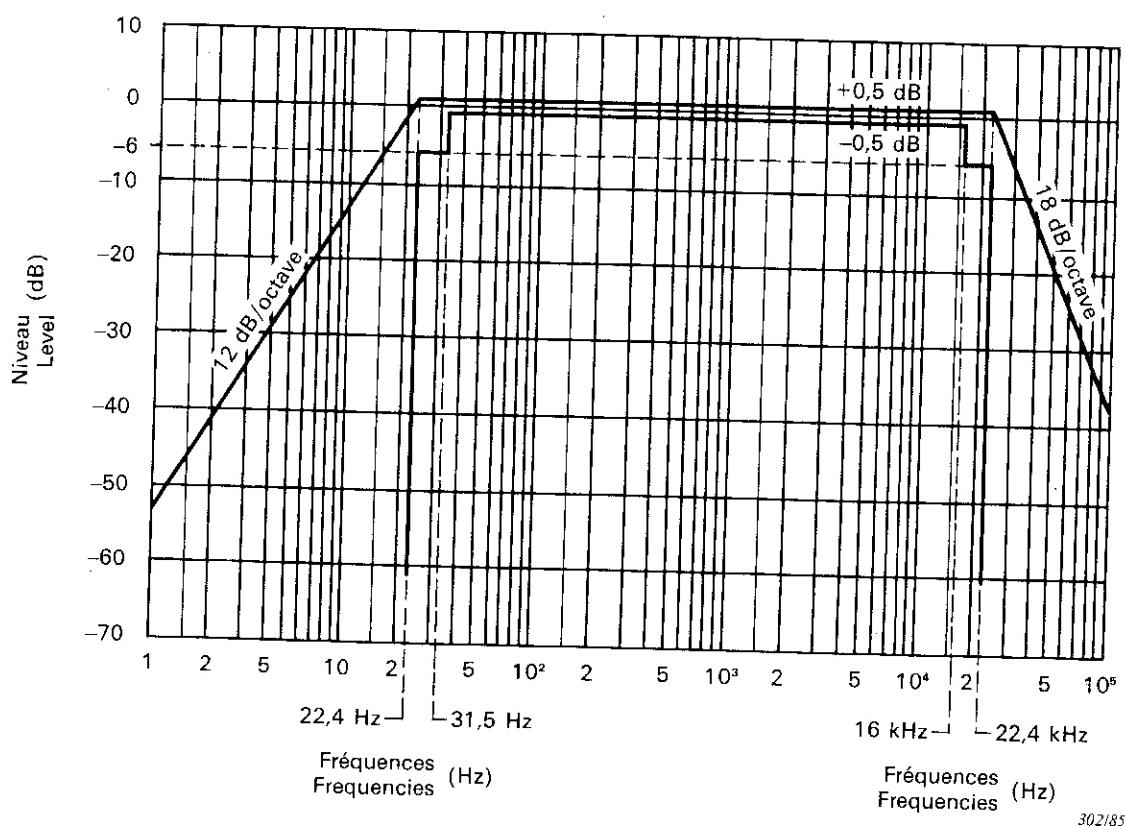


FIG. 5. — Filtre passe-bande pour mesure de bruit en bande large
(Limites de la réponse amplitude-fréquence). (Voir paragraphe 6.1.)
Band-pass filter for wide-band noise measurement (amplitude/frequency response
limits, see Sub-clause 6.1).

APPENDIX A

NOISE WEIGHTING NETWORK AND QUASI-PEAK METER

Note. — This weighting network and meter are in accordance with CCIR Recommendation 468-3.

A1. Weighting network

The nominal response curve of the weighting network is defined in Figure A1, page 29, which is the theoretical response of the passive network shown in Figure A2, page 29. Table AI gives the values of this response at various frequencies.

The permissible differences between the response curve of measuring networks and this nominal curve are shown in the last column of Table AI and in Figure A3, page 31.

Note. — The whole instrument is calibrated at 1 kHz (see Sub-clause A2.6). In order to make accurate measurements at frequencies giving maximum gain it would be useful to reduce the tolerance at 1 kHz (for instance: ± 0.2 dB).

TABLE AI

Frequency (Hz)	Response (dB)	Tolerance (dB)
31.5	- 29.9	± 2.0
63	- 23.9	± 1.4
100	- 19.8	± 1.0
200	- 13.8	$\pm 0.85^{1)}$
400	- 7.8	$\pm 0.7^{1)}$
800	- 1.9	$\pm 0.55^{1)}$
1 000	0	± 0.5
2 000	+ 5.6	$\pm 0.5^{1)}$
3 150	+ 9.0	$\pm 0.5^{1)}$
4 000	+ 10.5	$\pm 0.5^{1)}$
5 000	+ 11.7	± 0.5
6 300	+ 12.2	0
7 100	+ 12.0	$\pm 0.2^{1)}$
8 000	+ 11.4	$\pm 0.4^{1)}$
9 000	+ 10.1	$\pm 0.6^{1)}$
10 000	+ 8.1	$\pm 0.8^{1)}$
12 500	0	$\pm 1.2^{1)}$
14 000	- 5.3	$\pm 1.4^{1)}$
16 000	- 11.7	$\pm 1.65^{1)}$
20 000	- 22.2	± 2.0
31 500	- 42.7	{ + 2.8 ¹⁾ - ∞

¹⁾ The tolerances are obtained by a linear interpolation on a logarithmic graph on the basis of values specified for the frequencies used to define the mask, i.e. 31.5 Hz, 100 Hz, 1 000 Hz, 5 000 Hz, 6 300 Hz, and 20 000 Hz.

Note. — This table is in accordance with CCIR Recommendation 468-2.



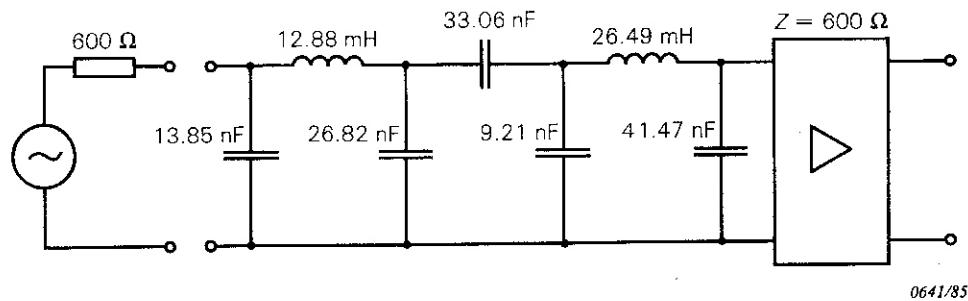


FIG. A1. — Weighting network.

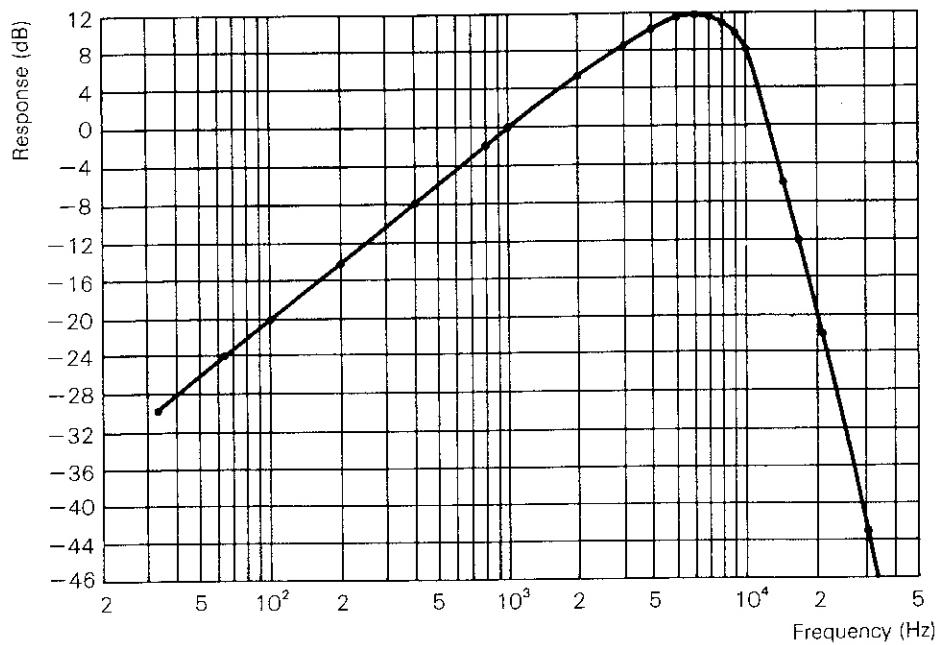

(A tolerance of at most 1% on the component values and a Q-factor of at least 200 at 10 000 Hz are sufficient to meet the tolerances given in Table AI.)

FIG. A2. — Frequency response of the weighting network shown in Figure A1.

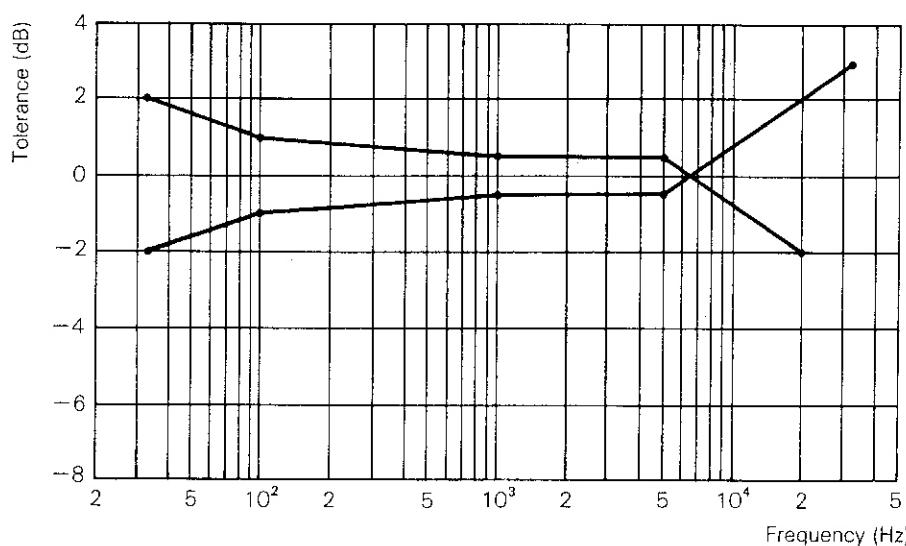

330/82

Note. — This figure is in accordance with CCIR Recommendation 468-2.

FIG. A3. — Maximum tolerances for the frequency response of the weighting network value.

A2. Characteristics of the measuring device

A quasi-peak value method of measurement shall be used, defined by the time-response characteristic of the measuring set, as described in Table AII.

The required dynamic performance of the measuring set may be realized in a variety of ways. It is defined by the performance of the measuring set as described by the following characteristics.

Note. — After full-wave rectification of the input signal, a possible arrangement would consist of two peak rectifier circuits of different time-constants connected in tandem.

TABLE AII

Burst duration (ms)	1 ¹⁾	2 ¹⁾	5	10	20	50	100	200
Amplitude reference steady signal reading								
(%)	17.0	26.6	40	48	52	59	68	80
(dB)	-15.4	-11.5	-8.0	-6.4	-5.7	-4.6	-3.3	-1.9
Limited values								
-- lower limit	13.5	22.4	34	41	44	44	50	68
(%)	-17.4	-13.0	-9.3	-7.7	-7.1	-6.0	-4.7	-3.3
-- upper limit	21.4	31.6	46	55	60	68	78	92
(%)	-13.4	-10.0	-6.6	-5.2	-4.4	-3.3	-2.2	-0.7

¹⁾ The use of burst durations less than 5 ms is not mandatory.

A2.1 Dynamic characteristic in response to single tone-bursts

Method of measurement

Single bursts of 5 kHz tone are applied to the input at an amplitude such that the steady signal would give a reading of 80% of full scale. The burst should start at the zero-crossing of the 5 kHz tone and should consist of an integral number of full periods. The limits of reading corresponding to each duration of tone-burst are given in Table AII.

The tests should be performed both without adjustment of the attenuators, the readings being observed directly from the instrument scale and also with the attenuators adjusted for each burst duration to maintain the reading as nearly constant at 80% of full scale as the attenuator steps will permit.

Unless otherwise specified, measurements should be made through the weighting network.

A2.2 Dynamic characteristic in response to repetitive tone-bursts

Method of measurement

A series of 5 ms bursts of 5 kHz tone starting at zero-crossing is applied to the input at an amplitude such that the steady signal would give a reading of 80% of full scale. The limits of the reading corresponding to each repetition frequency are given in Table AIII.

The tests should be performed without adjustment of the attenuators but the characteristic should be within tolerance on all ranges.

TABLE AIII

Number of bursts per second	2	10	100
Amplitude reference steady signal reading (%) (dB)	48 -6.4	77 -2.3	97 -0.25
Limiting values:			
— lower limit (%) (dB)	43 -7.3	72 -2.9	94 -0.5
— upper limit (%) (dB)	53 -5.5	82 -1.7	100 -0.0

A2.3 Overload characteristics

The overload capacity of the measuring set should be more than 20 dB with respect to the maximum indication of the scale at all settings of the attenuators. The term "overload capacity" refers both to absence of clipping in linear stages and to retention of the law of any logarithmic or similar stage which may be incorporated.

Method of measurement

Isolated 5 kHz tone-bursts of 0.6 ms duration starting at zero-crossing are applied to the input at an amplitude giving full scale reading using the most sensitive range of the

instrument. The amplitude of the tone-bursts is decreased in steps by a total of 20 dB while the readings are observed to check that they decrease by corresponding steps within an overall tolerance of ± 1 dB. The test is repeated for each range.

A2.4 *Reversibility error*

The difference in reading when the polarity of an asymmetrical signal is reversed shall be not greater than 0.5 dB.

Method of measurement

1 ms rectangular d.c. pulses with a pulse repetition rate of 100 pulses per second or less are applied to the input in the unweighted mode, at an amplitude giving an indication of 80% of full scale. The polarity of the input signal is then reversed and the difference in indication is noted.

A2.5 *Overswing*

The reading device shall be free from excessive overswing.

Method of measurement

1 kHz tone is applied to the input at an amplitude giving a steady reading of 0.775 V or 0 dB (see Sub-clause A2.6). When this signal is suddenly applied, the overswing shall be less than 0.3 dB.

A2.6 *Calibration*

The instrument shall be calibrated such that a steady input signal of 1 kHz sine wave at 0.775 V r.m.s, having less than 1% total harmonic distortion shall give a reading of 0.775 V (0 dB). The scale should have a calibrated range of at least 20 dB with the indication corresponding to 0.775 V (or 0 dB) between 2 dB and 10 dB below full scale.

A2.7 *Input impedance*

The instrument should have an input impedance $\geq 20 \text{ k}\Omega$ and if an input termination is provided then this should be $600 \Omega \pm 1\%$.

**Publications de la C E I préparées
par le Comité d'Etudes n° 84 ***

- 268: — Equipements pour systèmes électroacoustiques.
- 268-1 (1985) Première partie: Généralités.
- 268-2 (1971) Deuxième partie: Définition des termes généraux.
Modification n° 1 (1975).
- 268-3 (1969) Troisième partie: Amplificateurs pour systèmes électroacoustiques.
Modification n° 1 (1978).
- 268-3A (1970) Premier complément.
- 268-3B (1977) Deuxième complément.
- 268-3C (1978) Troisième complément.
- 268-4 (1972) Quatrième partie: Microphones.
- 268-5 (1972) Cinquième partie: Haut-parleurs.
- 268-5A (1980) Premier complément.
- 268-6 (1971) Sixième partie: Éléments auxiliaires passifs.
- 268-7 (1984) Septième partie: Casques et casques microphoniques.
- 268-8 (1973) Huitième partie: Dispositifs de commande automatique de gain.
- 268-9 (1977) Neuvième partie: Equipements de réverbération artificielle, de retard et de transposition de fréquence.
- 268-10 (1976) Dixième partie: Appareils de mesure du niveau de la modulation.
- 268-10A (1978) Premier complément.
- 268-11 (1985) Onzième partie: Connecteurs pour l'interconnexion des éléments de systèmes électroacoustiques.
- 268-12 (1975) Douzième partie: Connecteurs circulaires pour radiodiffusion et usage analogue.
- 268-13 (1985) Treizième partie: Essai d'écoute des haut-parleurs.
- 268-14 (1980) Quatorzième partie: Haut-parleurs circulaires et elliptiques; diamètres extérieurs du saladier, cotes de montage.
- 268-15 (1978) Quinzième partie: Valeurs d'adaptation recommandées pour le raccordement entre composants des systèmes électroacoustiques.
- 268-15A (1982) Premier complément.
- 574: — Equipements et systèmes audio-visuels, magnétoscopiques et de télévision.
- 574-1 (1977) Première partie: Généralités.
- 574-2 (1977) Deuxième partie: Définition des termes généraux.
- 574-3 (1983) Troisième partie: Connecteurs pour l'interconnexion des éléments de systèmes audio-visuels.
- 574-4 (1982) Quatrième partie: Valeurs d'adaptation recommandées pour l'interconnexion des équipements à l'intérieur d'un système.
- 574-5 (1980) Cinquième partie: Commande, synchronisation et codes d'adressage. Chapitre I: Pratique de montage photographique sonorisé.
- 574-5-2 (1983) Chapitre II: Systèmes de commande pour deux projecteurs de vues fixes — Pratique d'utilisation.

(Suite au verso)

* Anciennement Sous-Comité 29B: Technique acoustique, du Comité d'Etudes n° 29 de la C E I: Electroacoustique, et Sous-Comité 60C: Systèmes d'applications audio-visuelles et électroniques (pour l'information et la communication), du Comité d'Etudes n° 60 de la C E I: Enregistrement.

**I E C publications prepared
by Technical Committee No. 84 ***

- 268: — Sound system equipment.
- 268-1 (1985) Part 1: General.
- 268-2 (1971) Part 2: Explanation of general terms.
- Amendment No. 1 (1975).
- 268-3 (1969) Part 3: Sound system amplifiers.
- Amendment No. 1 (1978).
- 268-3A (1970) First supplement.
- 268-3B (1977) Second supplement.
- 268-3C (1978) Third supplement.
- 268-4 (1972) Part 4: Microphones.
- 268-5 (1972) Part 5: Loudspeakers.
- 268-5A (1980) First supplement.
- 268-6 (1971) Part 6: Auxiliary passive elements.
- 268-7 (1984) Part 7: Headphones and headsets.
- 268-8 (1973) Part 8: Automatic gain control devices.
- 268-9 (1977) Part 9: Artificial reverberation, time delay and frequency shift equipment.
- 268-10 (1976) Part 10: Programme level meters.
- 268-10A (1978) First supplement.
- 268-11 (1985) Part 11: Connectors for the interconnection of sound system components.
- 268-12 (1975) Part 12: Circular connectors for broadcast and similar use.
- 268-13 (1985) Part 13: Listening test on loudspeakers.
- 268-14 (1980) Part 14: Circular and elliptical loudspeakers; outer frame diameters and mounting dimensions.
- 268-15 (1978) Part 15: Preferred matching values for the interconnection of sound system components.
- 268-15A (1982) First supplement.
- 574: — Audio-visual, and television equipment and systems.
- 574-1 (1977) Part 1: General.
- 574-2 (1977) Part 2: Explanation of general terms.
- 574-3 (1983) Part 3: Connectors for the interconnection of equipment in audio-visual systems.
- 574-4 (1982) Part 4: Preferred matching values for the interconnection of equipment in a system.
- 574-5 (1980) Part 5: Control, synchronization and address codes. Chapter I: Synchronized tape/visual operating practice.
- 574-5-2 (1983) Chapter II: Control systems for two still projectors — Operating practice.

(Continued overleaf)

* Formerly Sub-Committee 29B: Audio Engineering, of I E C Technical Committee No. 29: Electroacoustics, and Sub-Committee 60C: Systems of Audio-visual and Electronic Technology (for Information and Communication), of I E C Technical Committee No. 60: Recording.